

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0092518\  
 Data File : P0049310.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 26 Sep 2018 00:20  
 Operator : SM/SJ  
 Sample : J4923-01  
 Misc :  
 ALS Vial : 34 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 BS-PAINT-CHIPS

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Sep 26 01:25:55 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0091918.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Sep 20 02:02:28 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1  | Resp#2  | ng/ml  | ng/ml   |
|-----------------------------|--------|-------|---------|---------|--------|---------|
| -----                       |        |       |         |         |        |         |
| System Monitoring Compounds |        |       |         |         |        |         |
| 1) SA Tetrachlo...          | 4.395  | 3.527 | 7768140 | 6721975 | 41.837 | 32.528  |
| 2) SA Decachlor...          | 10.109 | 8.458 | 9327962 | 7344845 | 33.935 | 35.879m |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0092518\  
Data File : P0049310.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 26 Sep 2018 00:20  
Operator : SM/SJ  
Sample : J4923-01  
Misc :  
ALS Vial : 34 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
BS-PAINT-CHIPS

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 26 01:25:55 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0091918.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Thu Sep 20 02:02:28 2018  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

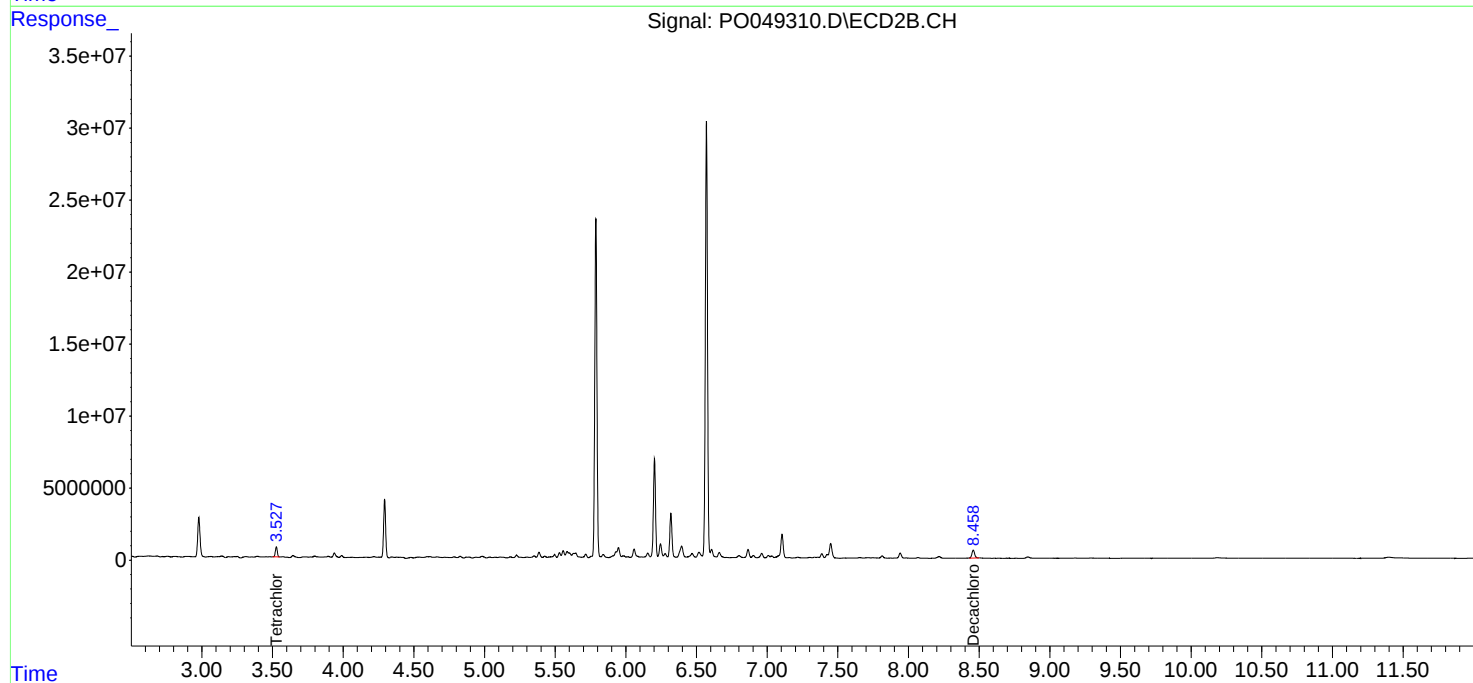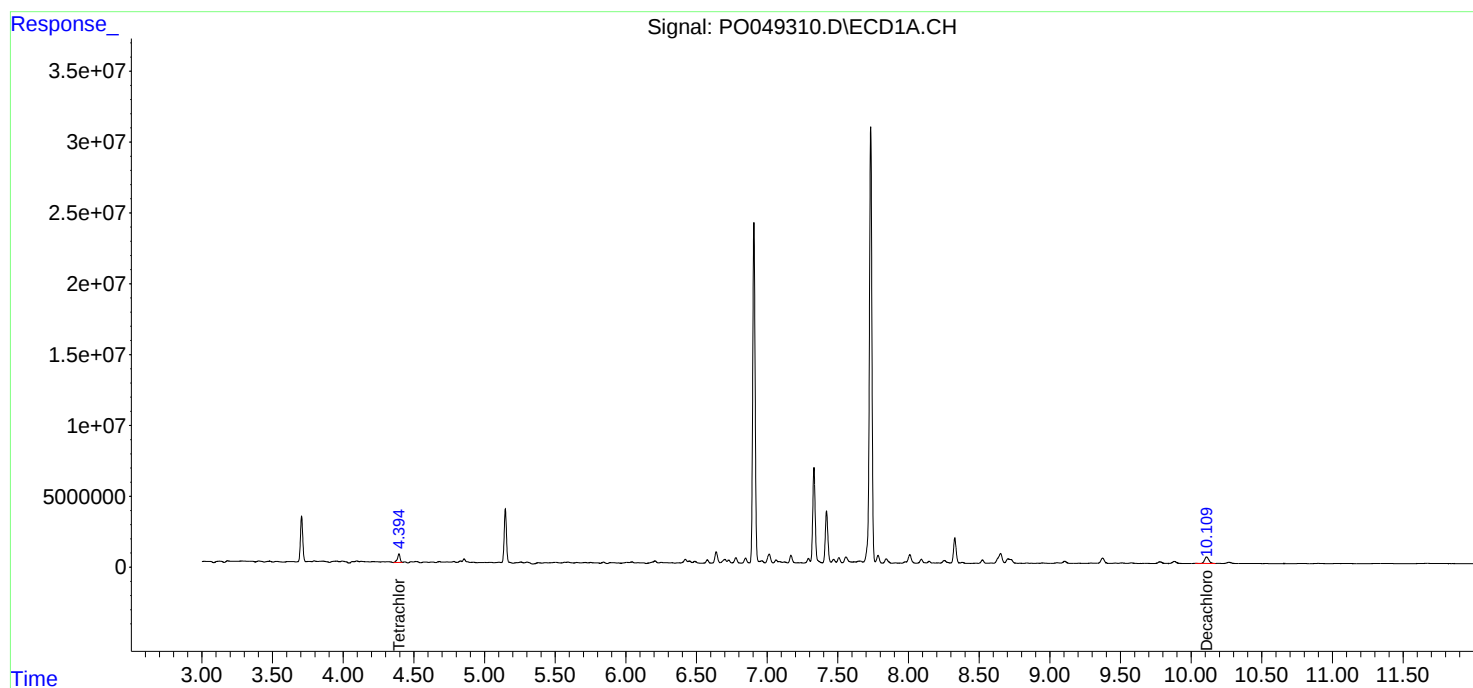


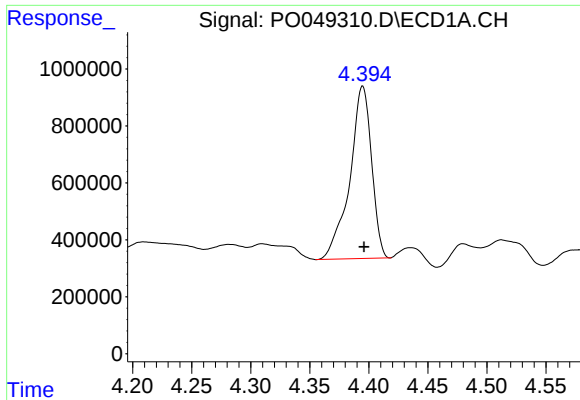

#1 Tetrachloro-m-xylene


R.T.: 4.395 min  
Delta R.T.: -0.001 min  
Response: 7768140  
Conc: 41.84 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
BS-PAINT-CHIPS

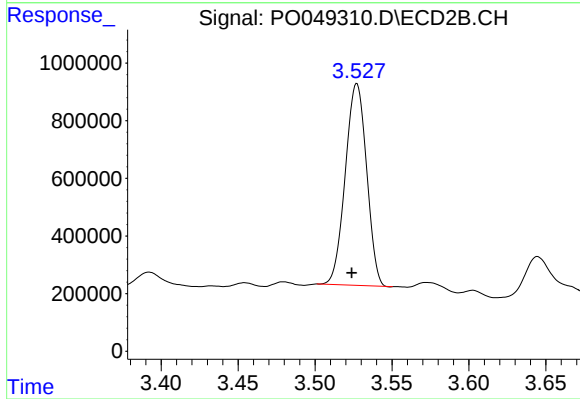


#1 Tetrachloro-m-xylene

R.T.: 3.527 min  
Delta R.T.: 0.003 min  
Response: 6721975  
Conc: 32.53 ng/ml

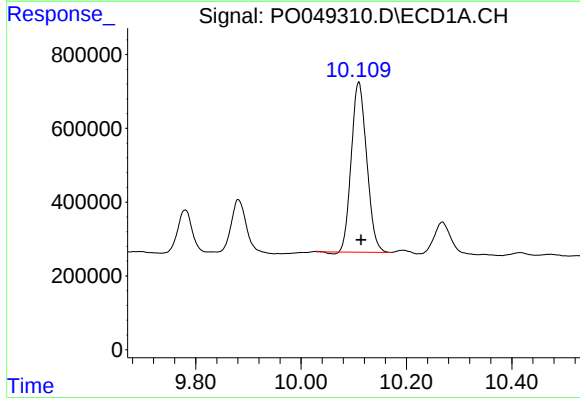

#2 Decachlorobiphenyl

R.T.: 10.109 min  
Delta R.T.: -0.004 min  
Response: 9327962  
Conc: 33.93 ng/ml

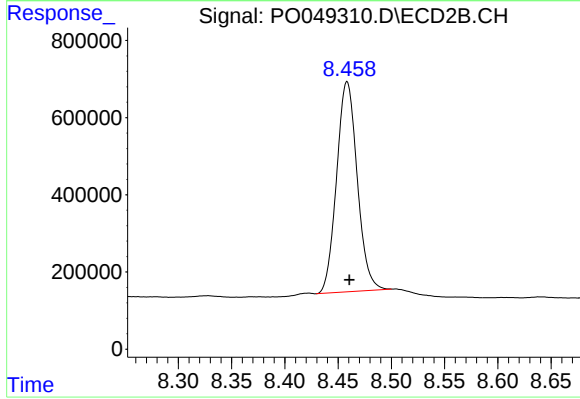

#2 Decachlorobiphenyl

R.T.: 8.458 min  
Delta R.T.: -0.002 min  
Response: 7344845  
Conc: 35.88 ng/ml m