

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092518\
 Data File : P0049313.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Sep 2018 1:56
 Operator : SM/SJ
 Sample : J5055-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PIERS

Manual Integrations
 APPROVED

Sohil
 9/26/2018 11:53:26 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 08:03:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 20 02:02:28 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.393	3.525	6711998	5623291	36.149m	27.211
2) SA Decachlor...	10.110	8.458	5794828	4127298	21.081	20.161

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092518\
Data File : PO049313.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Sep 2018 1:56
Operator : SM/SJ
Sample : J5055-01
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PIERS


Manual Integrations
APPROVED

Sohil
9/26/2018 11:53:26 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 08:03:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 20 02:02:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

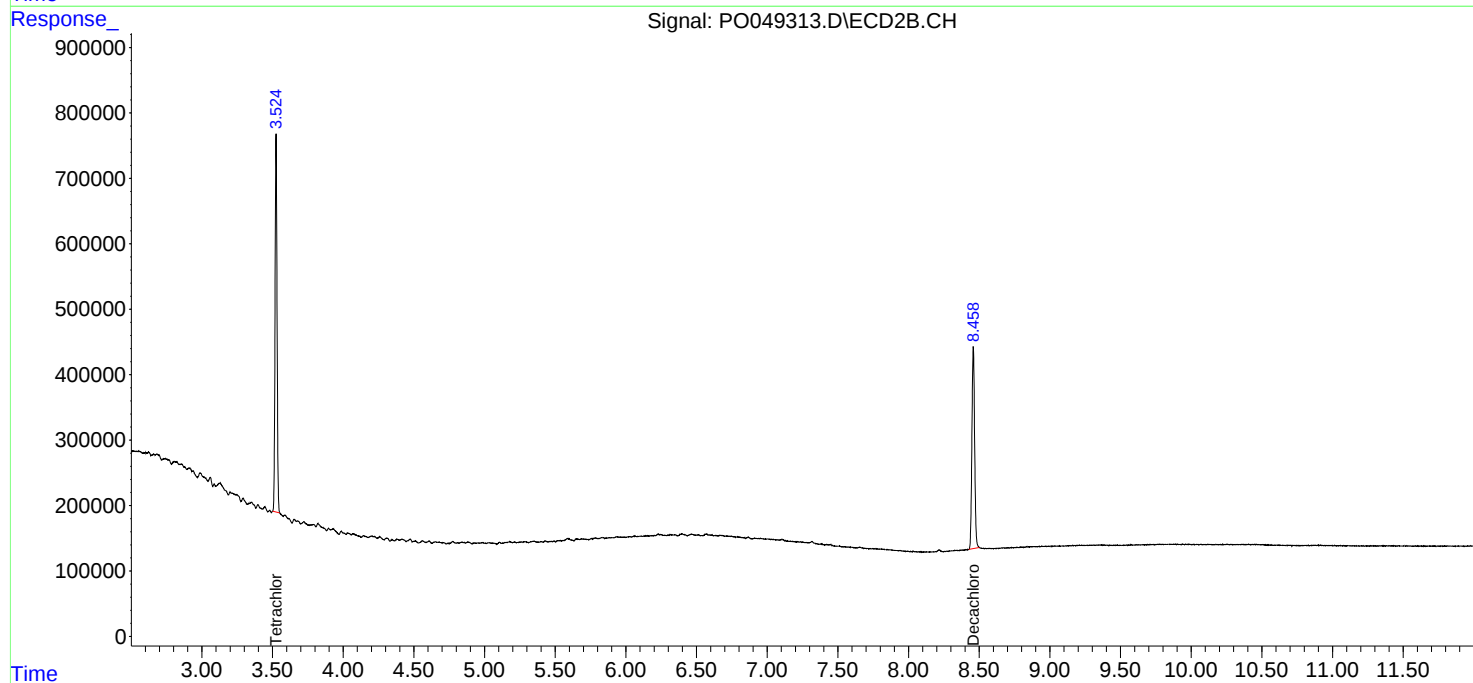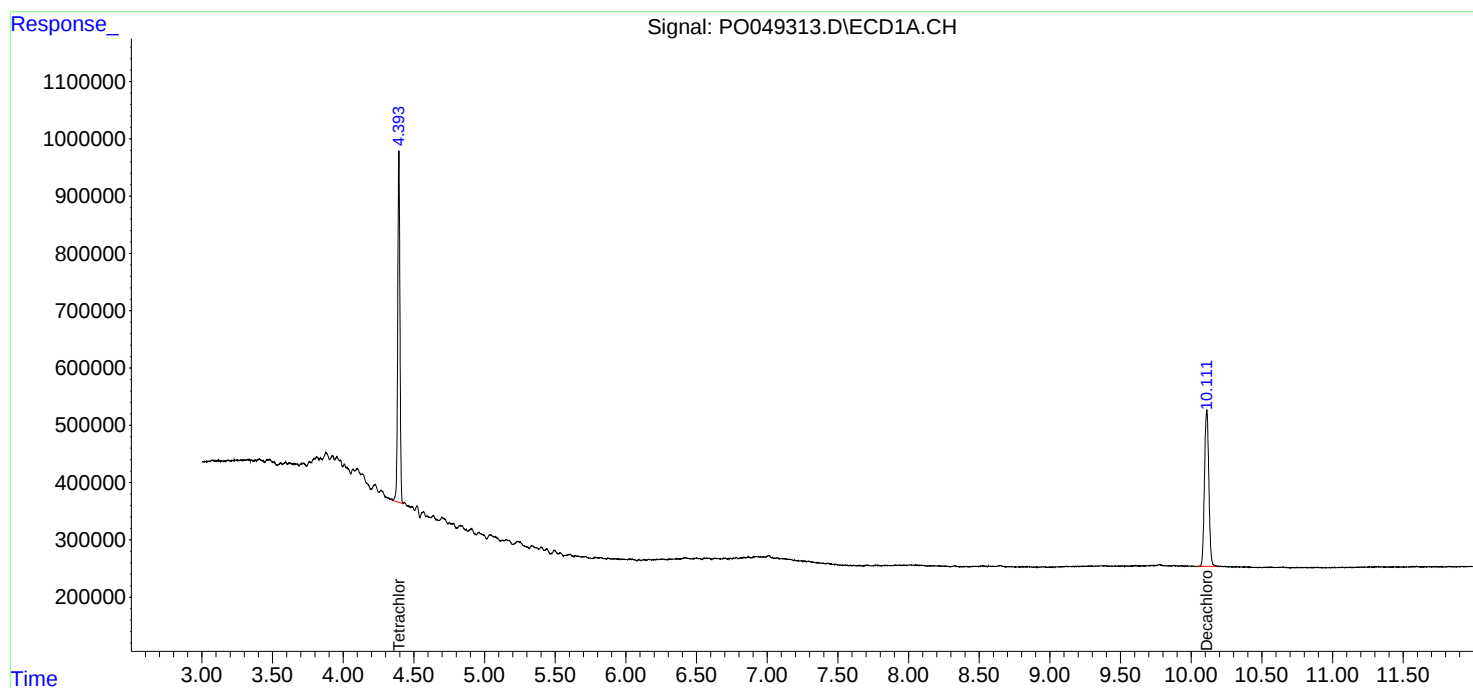

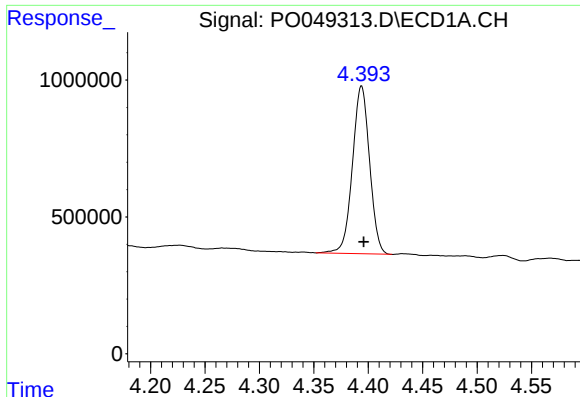


#1 Tetrachloro-m-xylene

R.T.: 4.393 min
Delta R.T.: -0.003 min
Response: 6711998
Conc: 36.15 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PIERS


Manual Integrations
APPROVED

Sohil
9/26/2018 11:53:26 AM

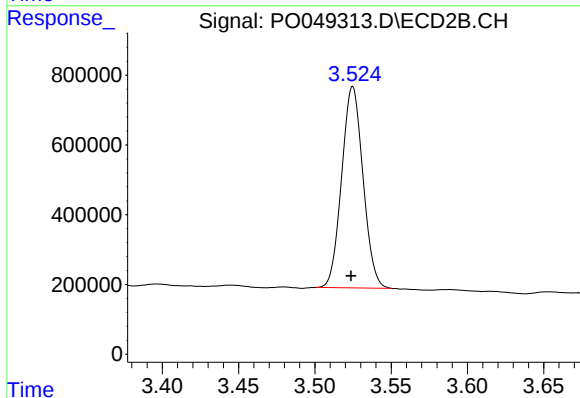


#1 Tetrachloro-m-xylene

R.T.: 3.525 min
Delta R.T.: 0.001 min
Response: 5623291
Conc: 27.21 ng/ml

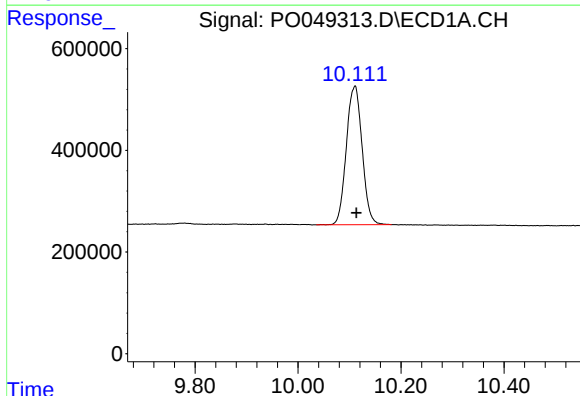

#2 Decachlorobiphenyl

R.T.: 10.110 min
Delta R.T.: -0.004 min
Response: 5794828
Conc: 21.08 ng/ml

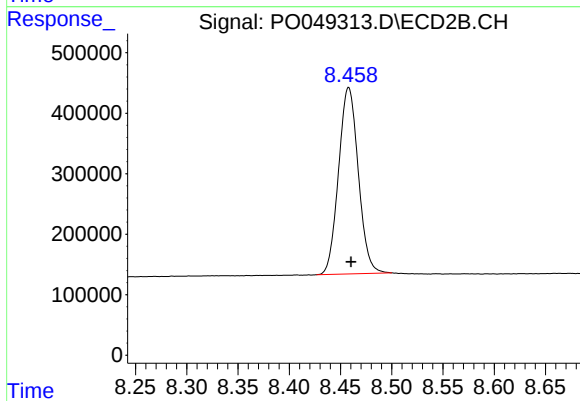

#2 Decachlorobiphenyl

R.T.: 8.458 min
Delta R.T.: -0.002 min
Response: 4127298
Conc: 20.16 ng/ml