

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092518\
 Data File : P0049317.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Sep 2018 2:59
 Operator : SM/SJ
 Sample : J5055-08
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-B

Manual Integrations
 APPROVED

Sohil
 9/26/2018 11:53:30 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 07:47:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 20 02:02:28 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.394	3.525	5194519	4475037	27.976	21.655m
2) SA Decachlor...	10.111	8.458	4054965	2894664	14.752	14.140

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092518\
Data File : PO049317.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Sep 2018 2:59
Operator : SM/SJ
Sample : J5055-08
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-B


Manual Integrations
APPROVED

Sohil
9/26/2018 11:53:30 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 07:47:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 20 02:02:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

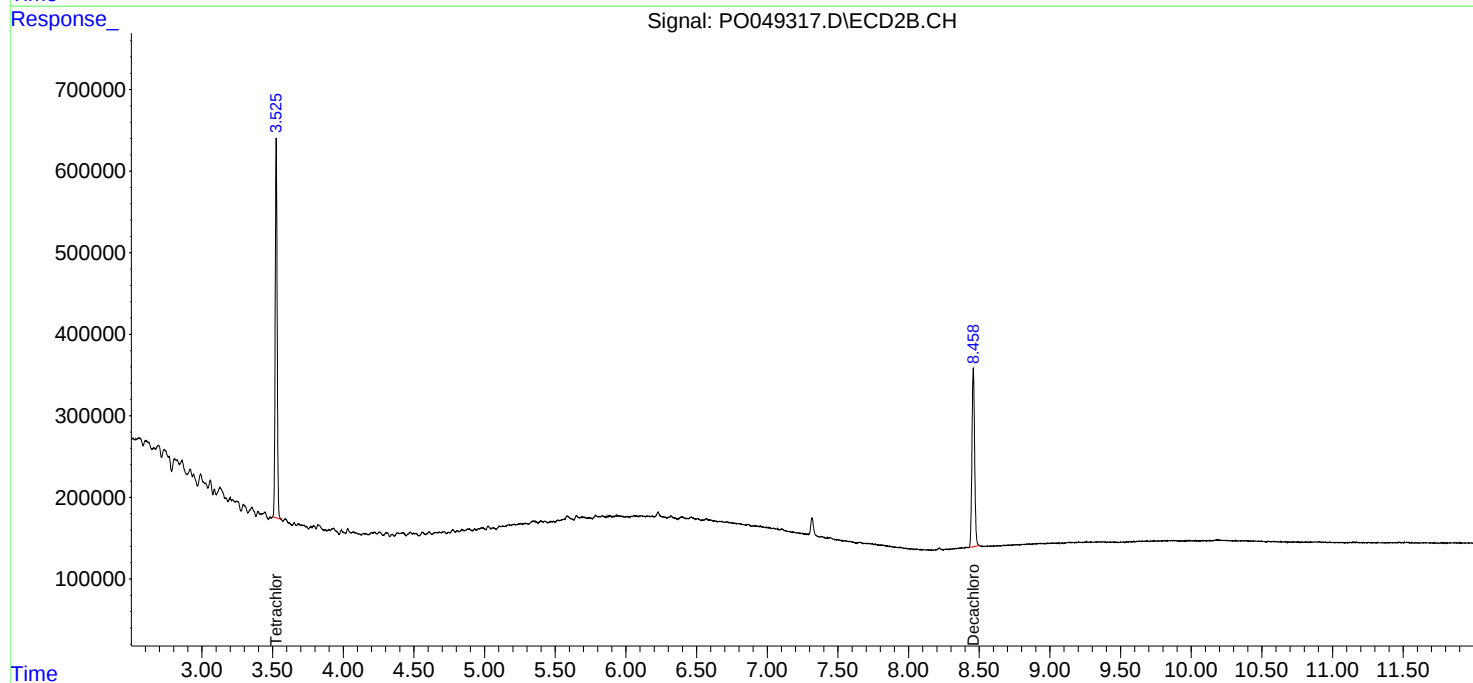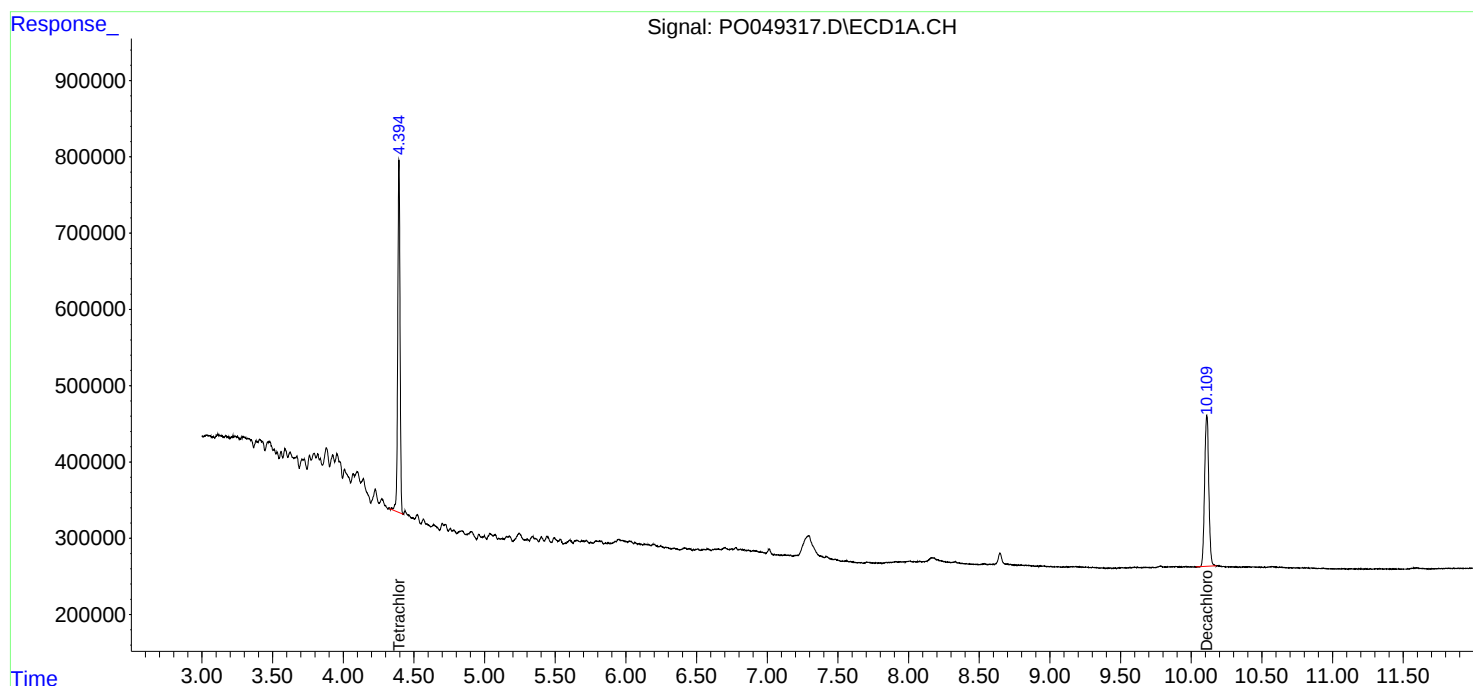

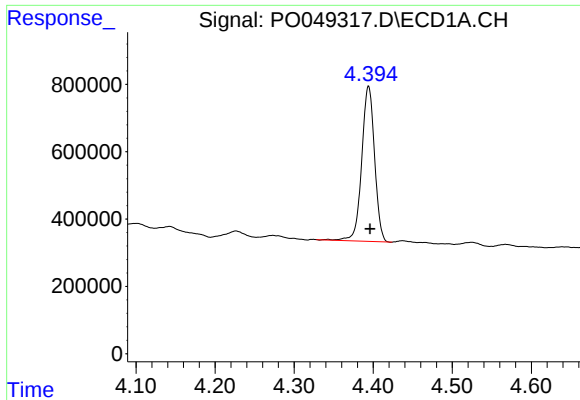


#1 Tetrachloro-m-xylene

R.T.: 4.394 min
Delta R.T.: -0.002 min
Response: 5194519
Conc: 27.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-B


Manual Integrations
APPROVED

Sohil
9/26/2018 11:53:30 AM

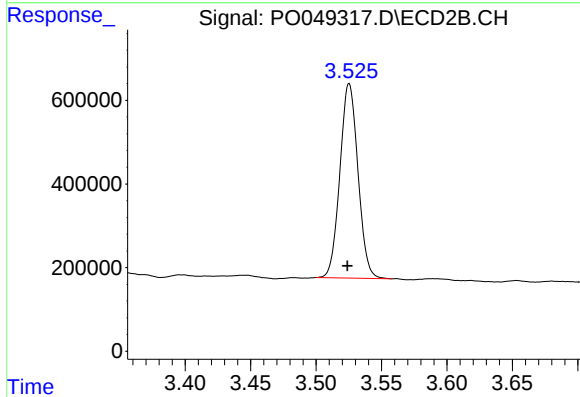


#1 Tetrachloro-m-xylene

R.T.: 3.525 min
Delta R.T.: 0.001 min
Response: 4475037
Conc: 21.65 ng/ml m

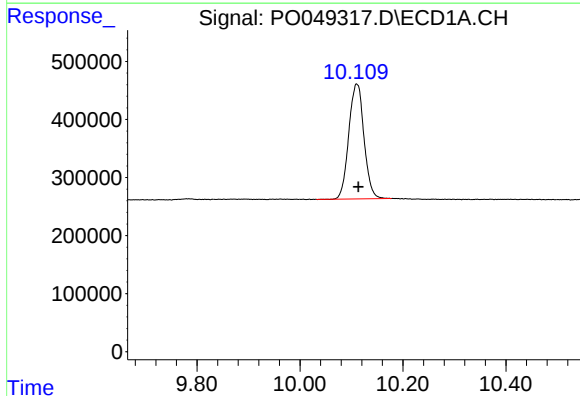

#2 Decachlorobiphenyl

R.T.: 10.111 min
Delta R.T.: -0.003 min
Response: 4054965
Conc: 14.75 ng/ml

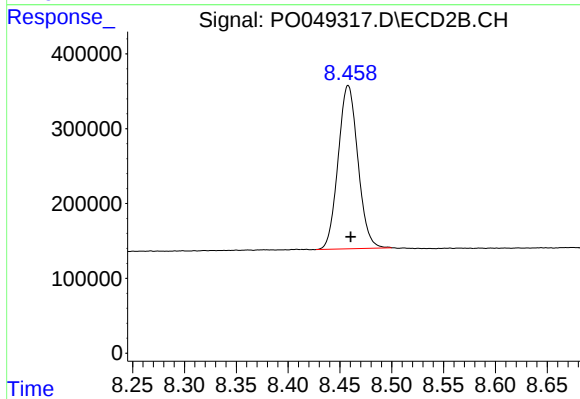

#2 Decachlorobiphenyl

R.T.: 8.458 min
Delta R.T.: -0.002 min
Response: 2894664
Conc: 14.14 ng/ml