

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092718\
 Data File : P0049399.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Sep 2018 13:11
 Operator : SM/SJ
 Sample : J5078-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 600-WILSON-AVE-NEWARK

Manual Integrations
 APPROVED

Sohil
 9/28/2018 11:02:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 16:42:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 20 02:02:28 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.390	3.520	3879343	4620306	20.893	22.358m
2) SA Decachlor...	10.102	8.453	3153493	3107606	11.472	15.180 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092718\
Data File : PO049399.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Sep 2018 13:11
Operator : SM/SJ
Sample : J5078-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
600-WILSON-AVE-NEWARK


Manual Integrations
APPROVED

Sohil
9/28/2018 11:02:17 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 16:42:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 20 02:02:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

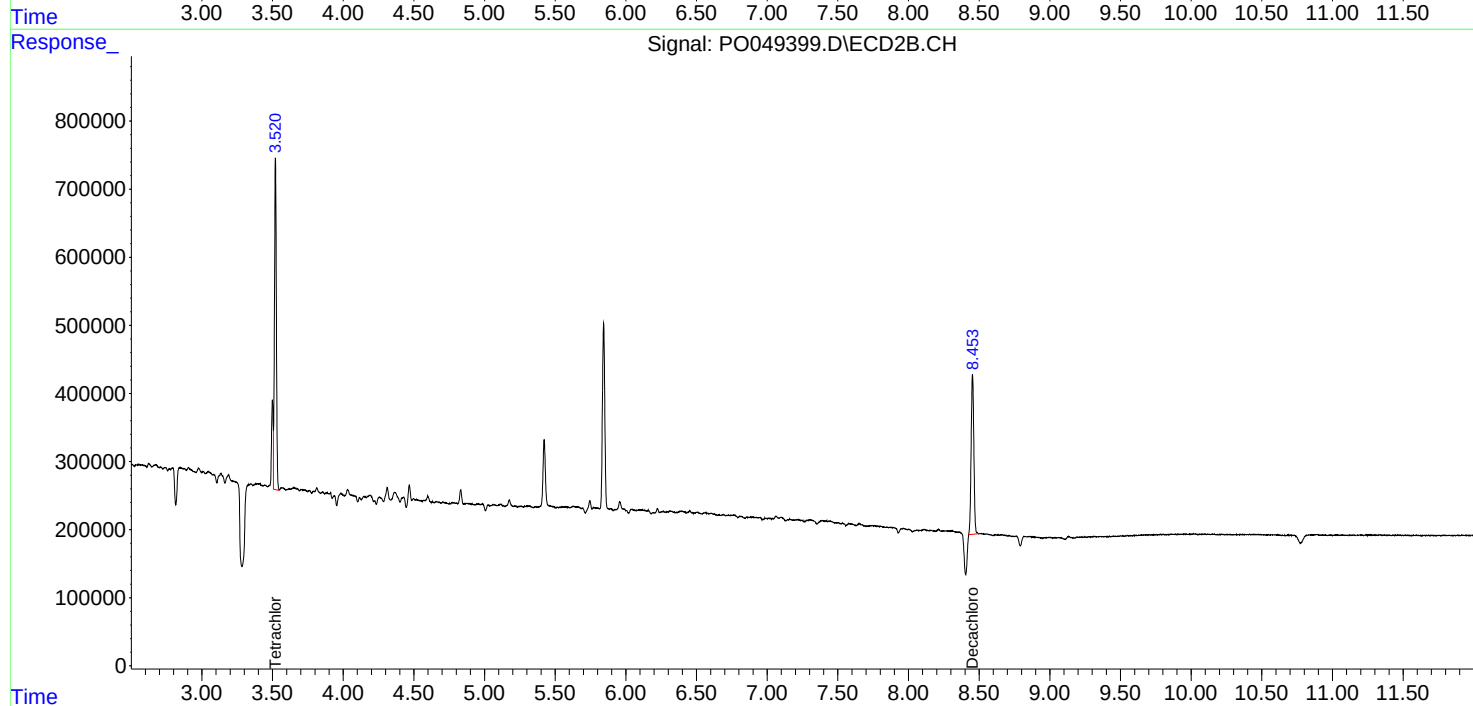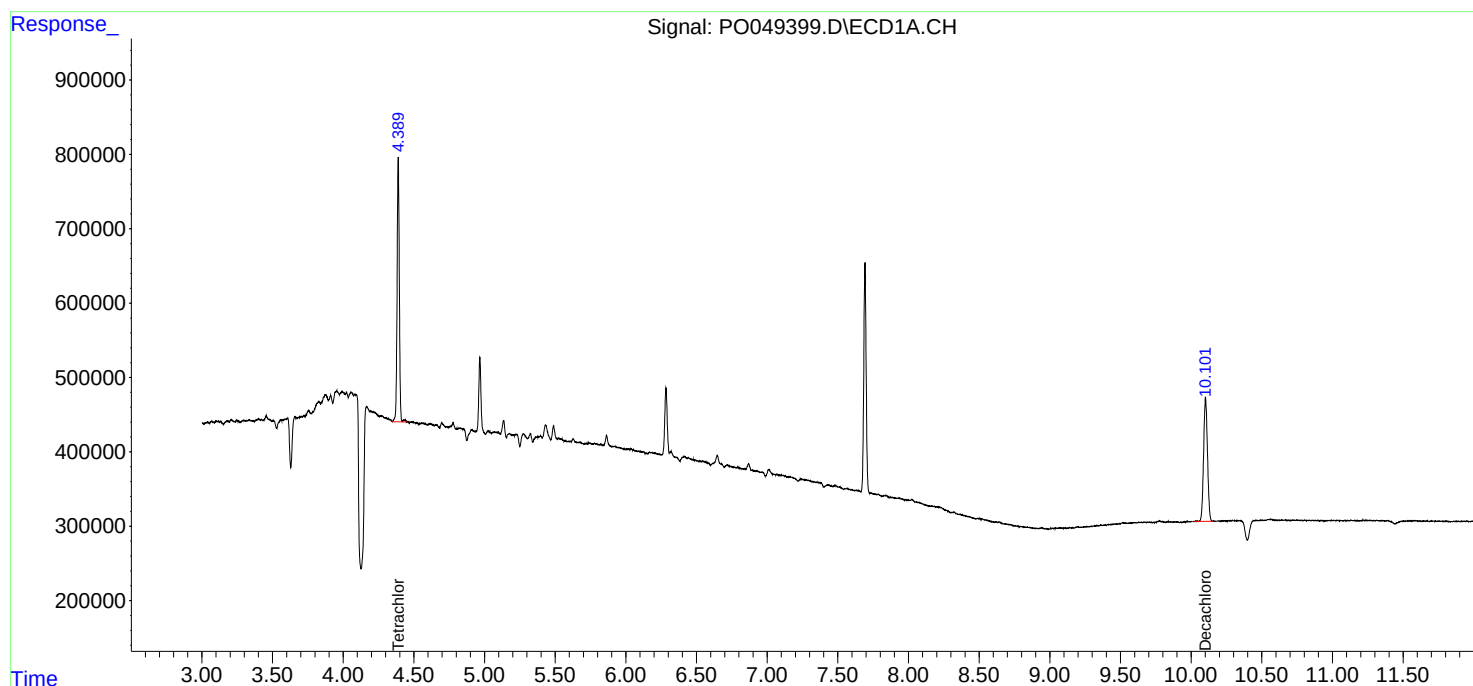

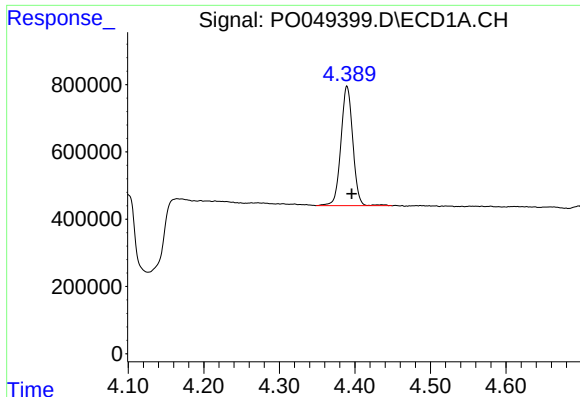


#1 Tetrachloro-m-xylene

R.T.: 4.390 min
Delta R.T.: -0.006 min
Response: 3879343
Conc: 20.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
600-WILSON-AVE-NEWARK


Manual Integrations
APPROVED

Sohil
9/28/2018 11:02:17 AM

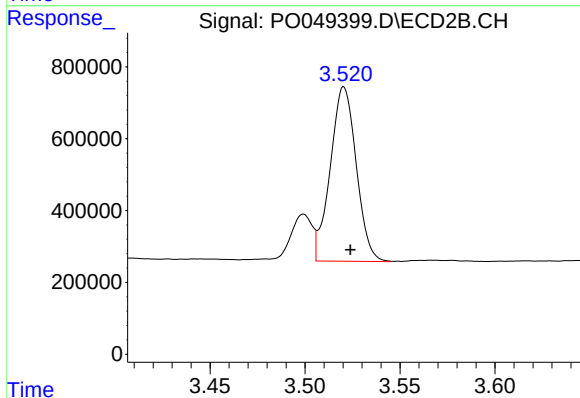


#1 Tetrachloro-m-xylene

R.T.: 3.520 min
Delta R.T.: -0.004 min
Response: 4620306
Conc: 22.36 ng/ml m

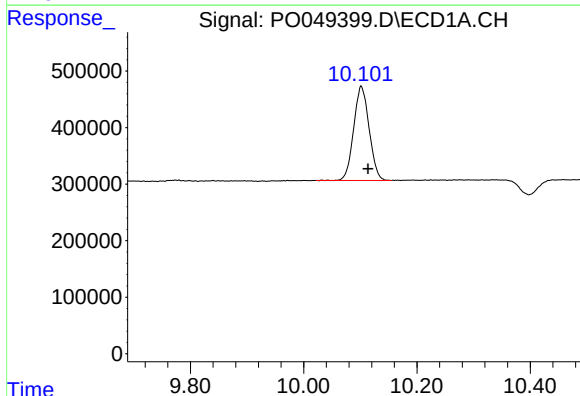

#2 Decachlorobiphenyl

R.T.: 10.102 min
Delta R.T.: -0.012 min
Response: 3153493
Conc: 11.47 ng/ml

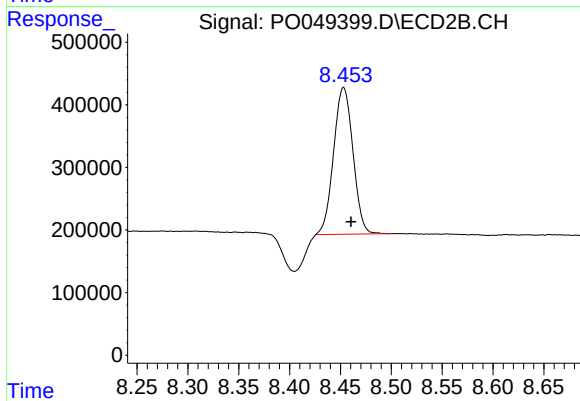

#2 Decachlorobiphenyl

R.T.: 8.453 min
Delta R.T.: -0.007 min
Response: 3107606
Conc: 15.18 ng/ml