

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0093019\
 Data File : P0061462.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Sep 2019 13:07 (#1); 30 Sep 2019 13:08 (#2)
 Operator : HP/AJ
 Sample : K5039-02DL2 200X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 30476-80DL

Manual Integrations
 APPROVED

Ankita
 10/2/2019 9:22:32 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 01:14:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

16)	L4	AR-1242-1	5.530	4.577	744992	547548	624.252	601.449m
17)	L4	AR-1242-2	5.553	4.596	1018779	708775	596.092	566.179
18)	L4	AR-1242-3	5.614	4.766	679687	431947	627.666	604.497
19)	L4	AR-1242-4	5.713	4.848	578568	363306	655.377	498.883
20)	L4	AR-1242-5	6.446	5.356	437949	395609	390.788	399.644

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO093019\
Data File : PO061462.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Sep 2019 13:07 (#1); 30 Sep 2019 13:08 (#2)
Operator : HP/AJ
Sample : K5039-02DL2 200X
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
30476-80DL


Manual Integrations
APPROVED

Ankita
10/2/2019 9:22:32 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 01:14:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

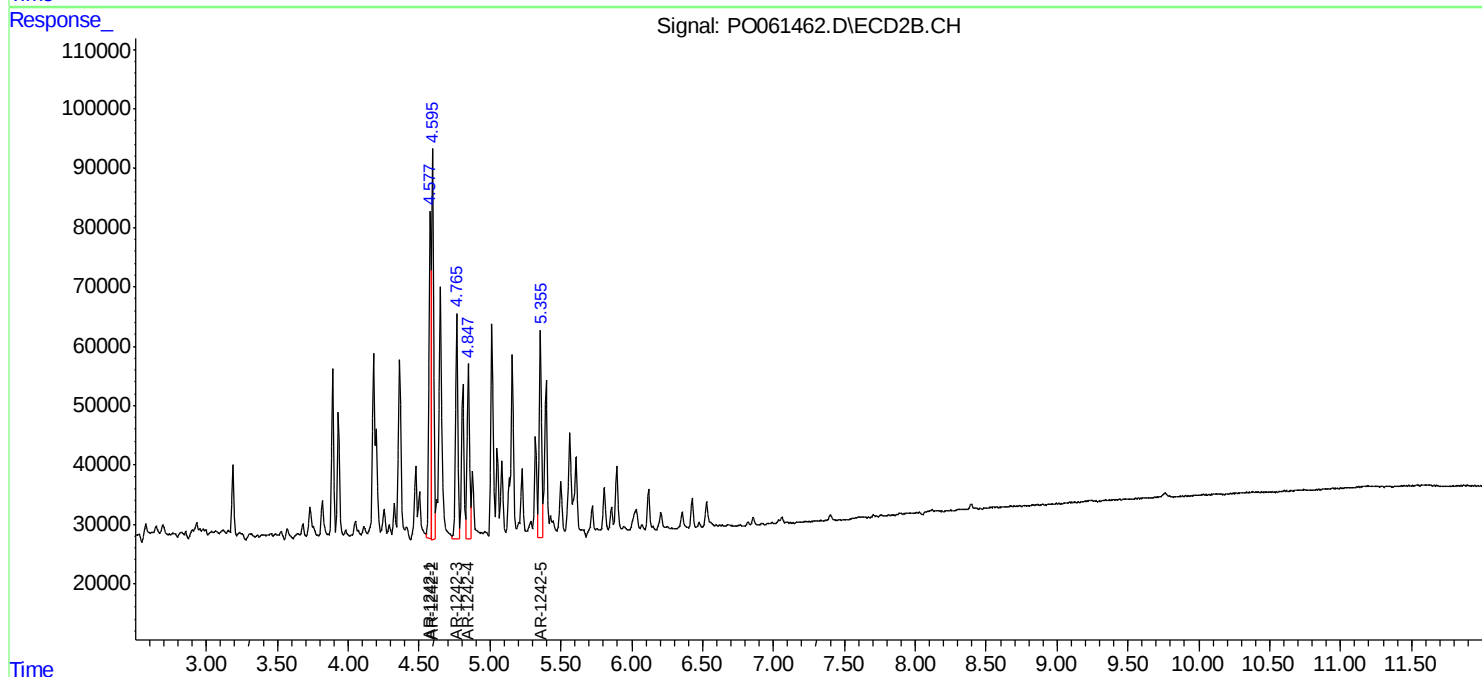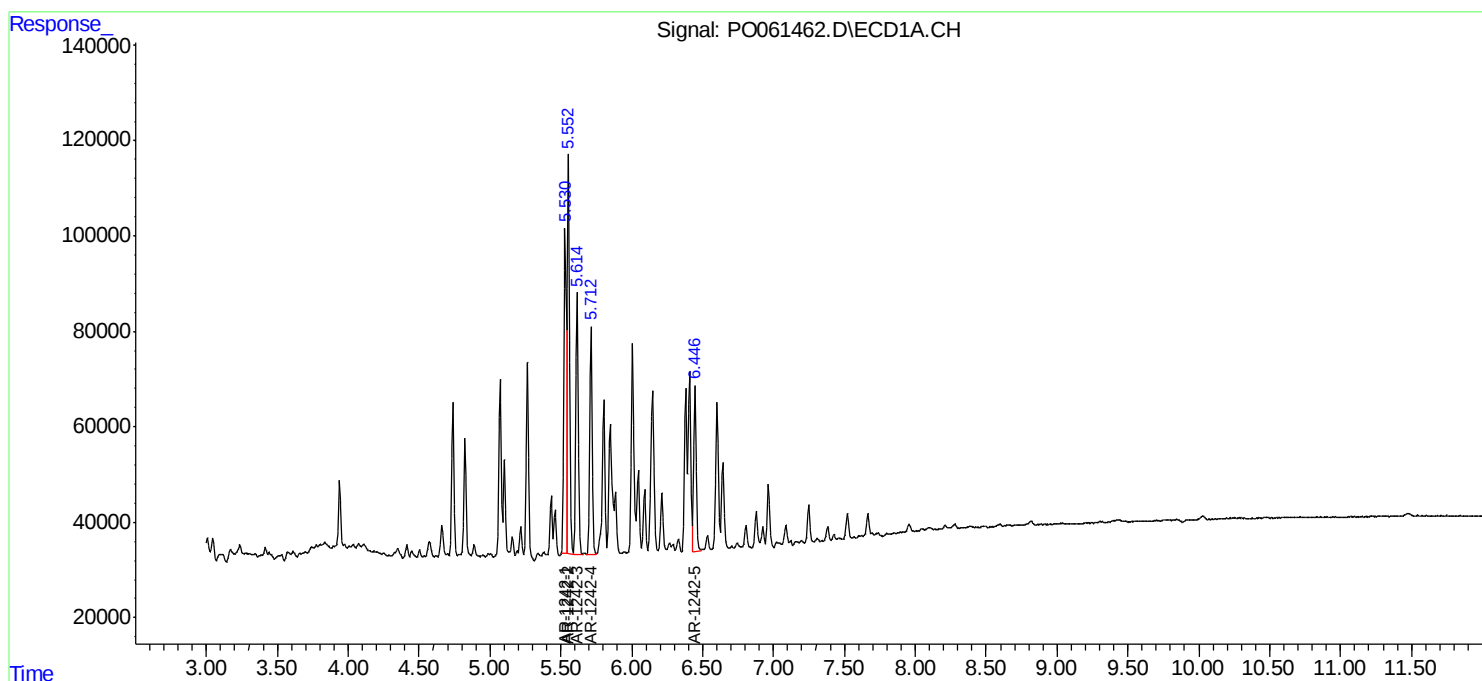

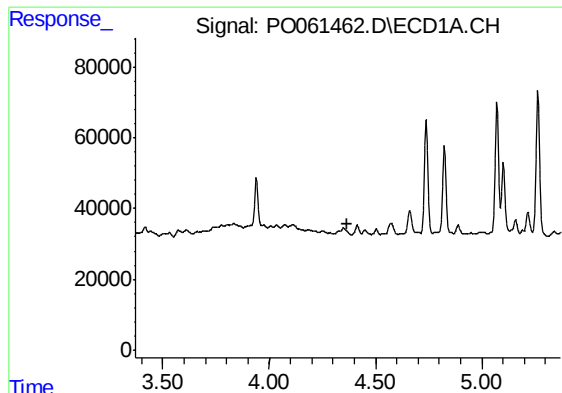


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.370 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
30476-80DL


Manual Integrations
APPROVED

Ankita
10/2/2019 9:22:32 AM

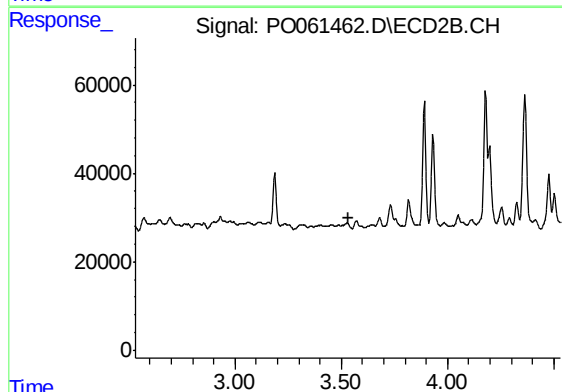


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.531 min
Response: 0
Conc: N.D.

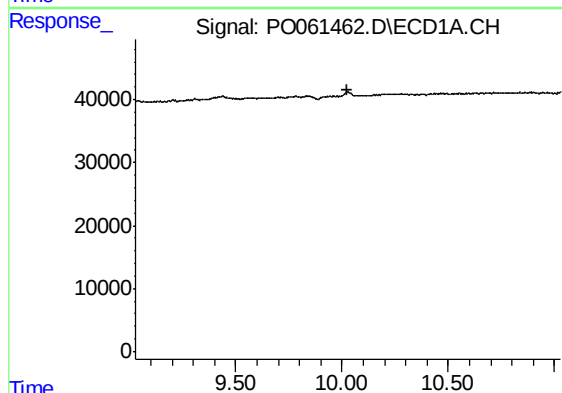


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.028 min
Response: 0
Conc: N.D.

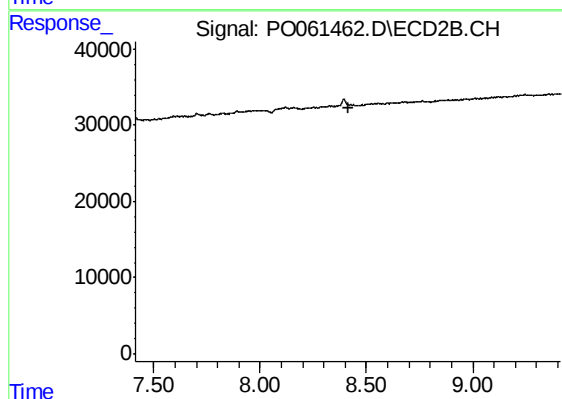

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.413 min
Response: 0
Conc: N.D.

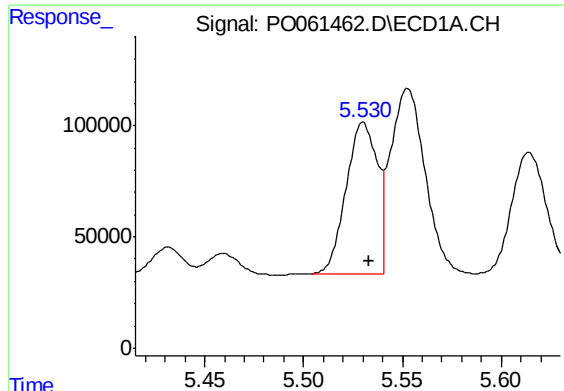


#16 AR-1242-1

R.T.: 5.530 min
Delta R.T.: -0.003 min
Response: 744992
Conc: 624.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
30476-80DL


Manual Integrations
APPROVED

Ankita
10/2/2019 9:22:32 AM

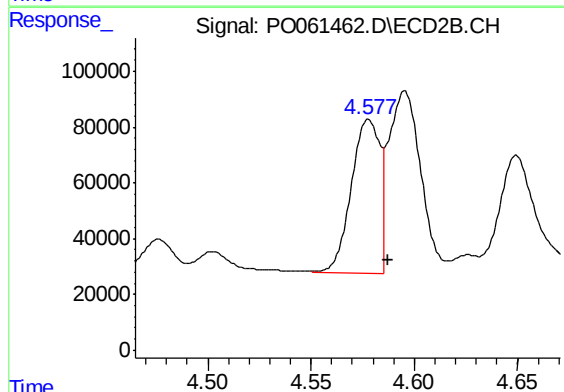


#16 AR-1242-1

R.T.: 4.577 min
Delta R.T.: -0.010 min
Response: 547548
Conc: 601.45 ng/ml m

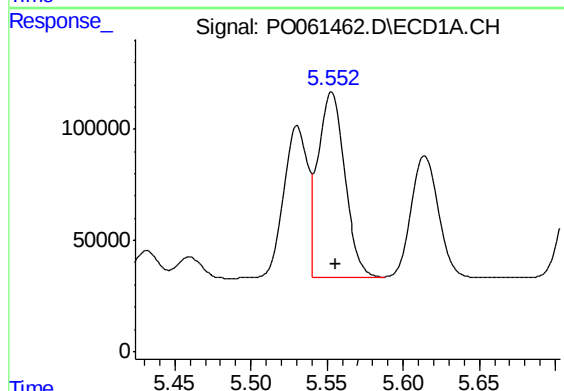


#17 AR-1242-2

R.T.: 5.553 min
Delta R.T.: -0.003 min
Response: 1018779
Conc: 596.09 ng/ml

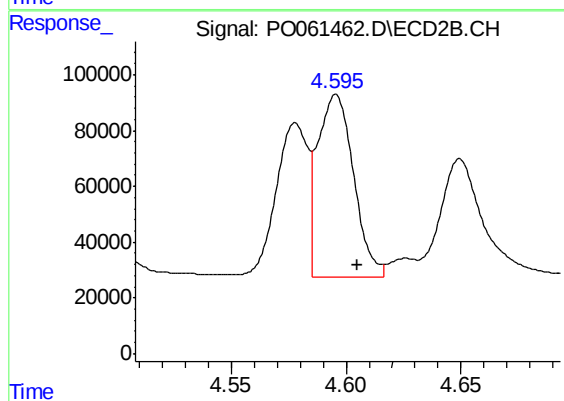

#17 AR-1242-2

R.T.: 4.596 min
Delta R.T.: -0.009 min
Response: 708775
Conc: 566.18 ng/ml

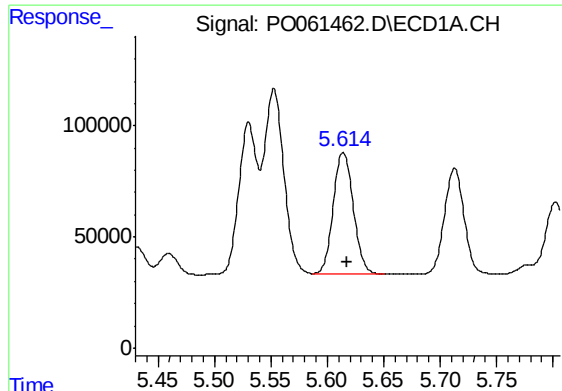


#18 AR-1242-3

R.T.: 5.614 min
Delta R.T.: -0.003 min
Response: 679687
Conc: 627.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
30476-80DL


Manual Integrations
APPROVED

Ankita
10/2/2019 9:22:32 AM

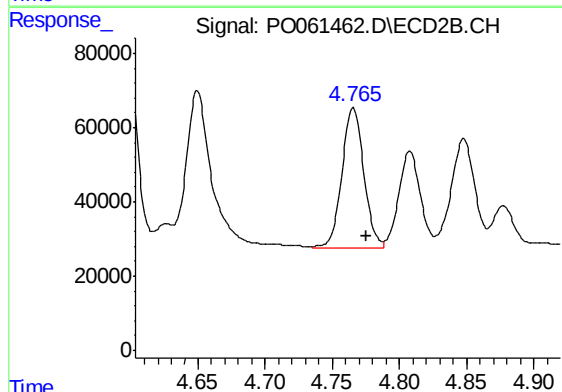


#18 AR-1242-3

R.T.: 4.766 min
Delta R.T.: -0.010 min
Response: 431947
Conc: 604.50 ng/ml

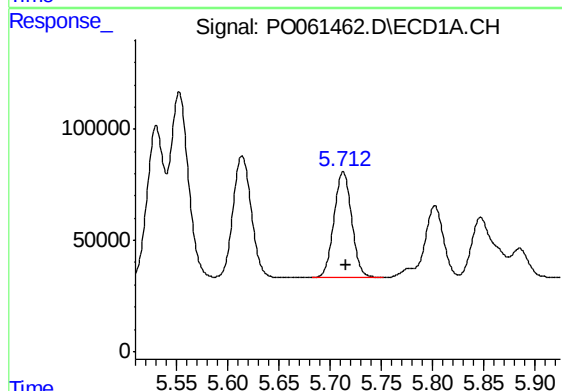


#19 AR-1242-4

R.T.: 5.713 min
Delta R.T.: -0.003 min
Response: 578568
Conc: 655.38 ng/ml

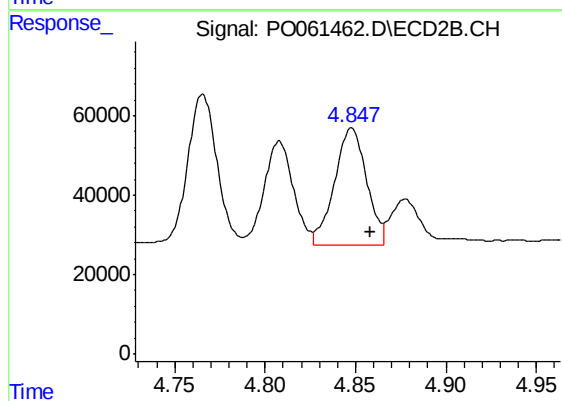

#19 AR-1242-4

R.T.: 4.848 min
Delta R.T.: -0.010 min
Response: 363306
Conc: 498.88 ng/ml

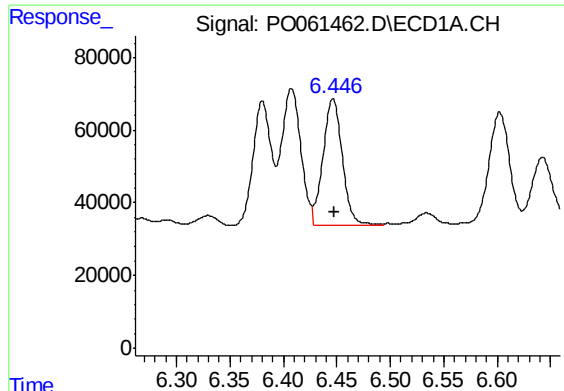


#20 AR-1242-5

R.T.: 6.446 min
Delta R.T.: -0.002 min
Response: 437949
Conc: 390.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
30476-80DL

Manual Integrations
APPROVED

Ankita
10/2/2019 9:22:32 AM

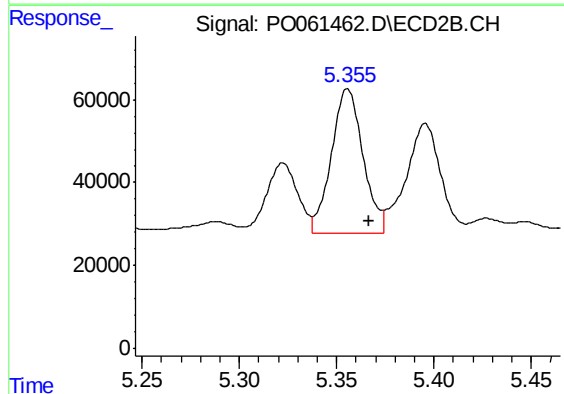

#20 AR-1242-5

R.T.: 5.356 min
Delta R.T.: -0.011 min
Response: 395609
Conc: 399.64 ng/ml