

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0093019\
 Data File : P0061469.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Sep 2019 15:52
 Operator : HP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 01:16:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.359	3.525	752995	527103	20.467	18.878
2)	SA Decachlor...	10.018	8.392	869815	653556	18.931	18.645

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO093019\
Data File : PO061469.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Sep 2019 15:52
Operator : HP/AJ
Sample : I.BLK
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 01:16:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

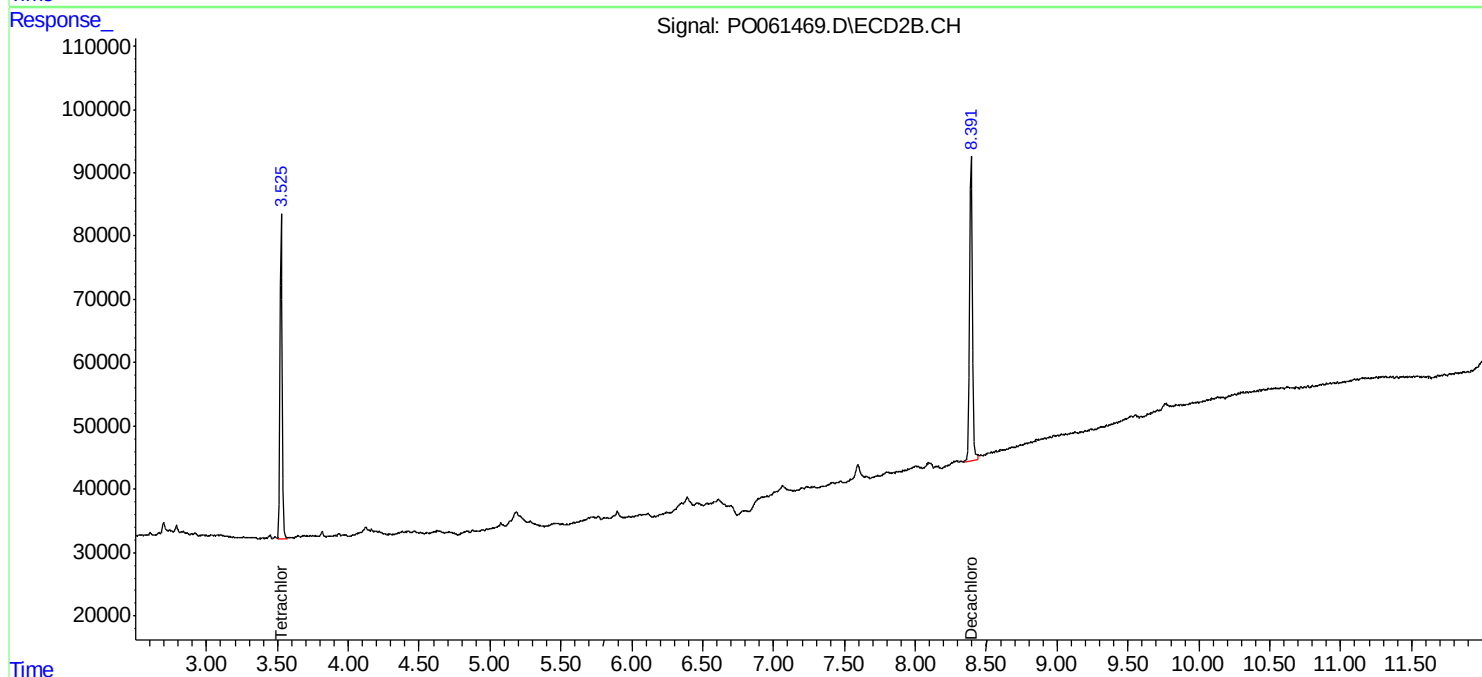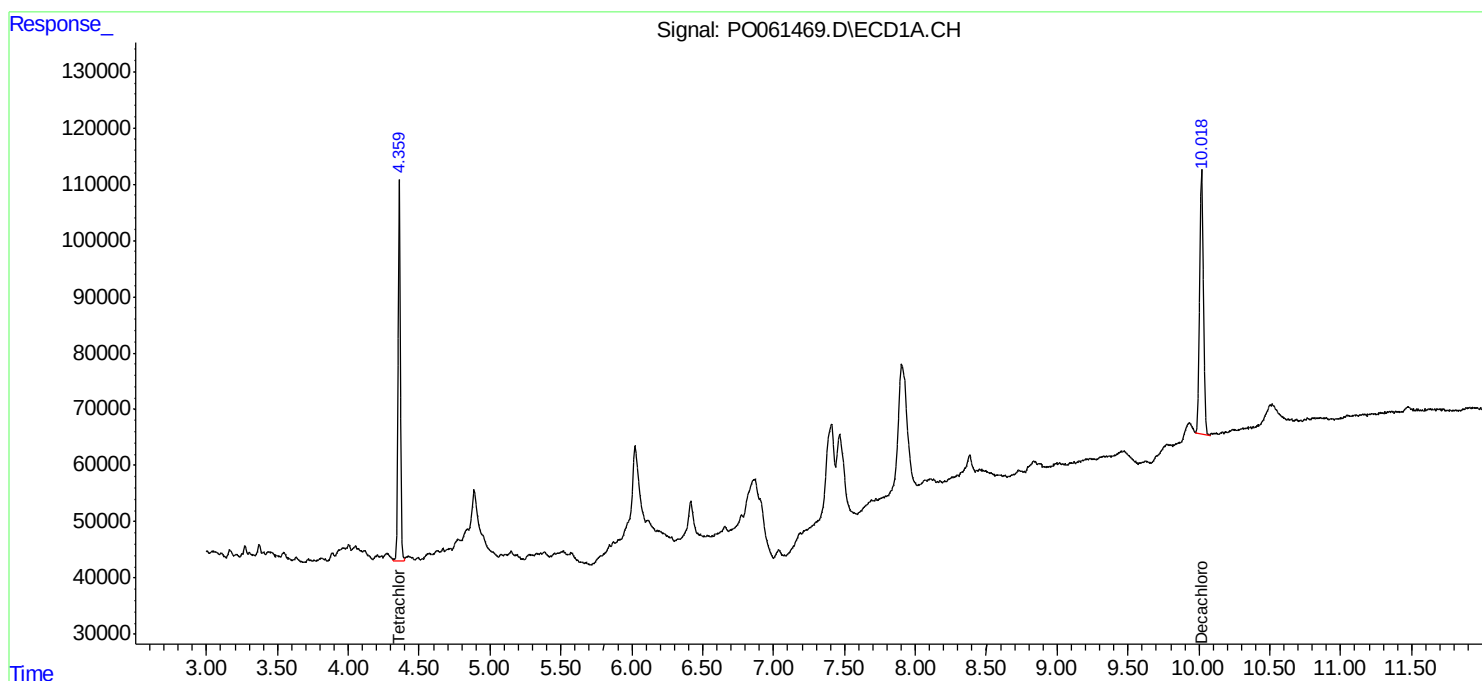


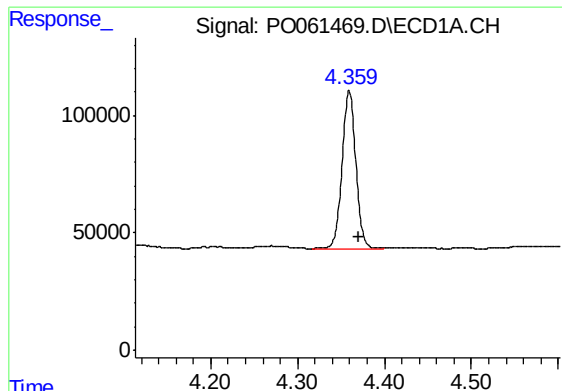

#1 Tetrachloro-m-xylene


R.T.: 4.359 min
Delta R.T.: -0.011 min
Response: 752995
Conc: 20.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

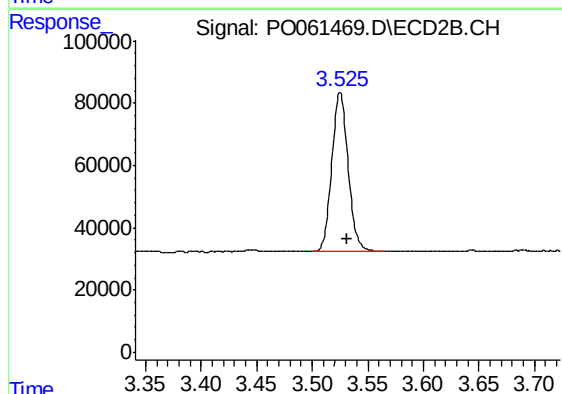


#1 Tetrachloro-m-xylene

R.T.: 3.525 min
Delta R.T.: -0.006 min
Response: 527103
Conc: 18.88 ng/ml

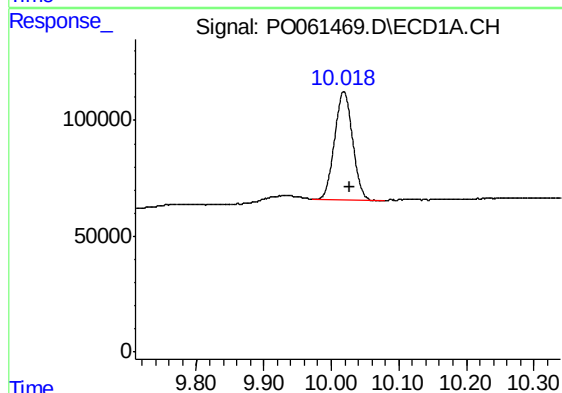

#2 Decachlorobiphenyl

R.T.: 10.018 min
Delta R.T.: -0.009 min
Response: 869815
Conc: 18.93 ng/ml

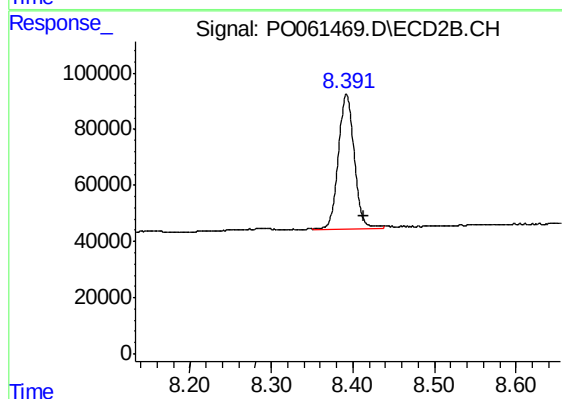

#2 Decachlorobiphenyl

R.T.: 8.392 min
Delta R.T.: -0.021 min
Response: 653556
Conc: 18.65 ng/ml