

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0093019\
 Data File : P0061478.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Sep 2019 19:13
 Operator : HP/AJ
 Sample : K5083-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20190703-RR-COMPOSITE-3

Manual Integrations
 APPROVED

Ankita
 10/2/2019 9:23:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 01:20:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.364	3.525	726236	517049	19.740	18.517
2)	SA Decachlor...	10.025	8.394	678265	474000	14.762	13.523

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO093019\
Data File : PO061478.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Sep 2019 19:13
Operator : HP/AJ
Sample : K5083-06
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
20190703-RR-COMPOSITE-3


Manual Integrations
APPROVED

Ankita
10/2/2019 9:23:17 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 01:20:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

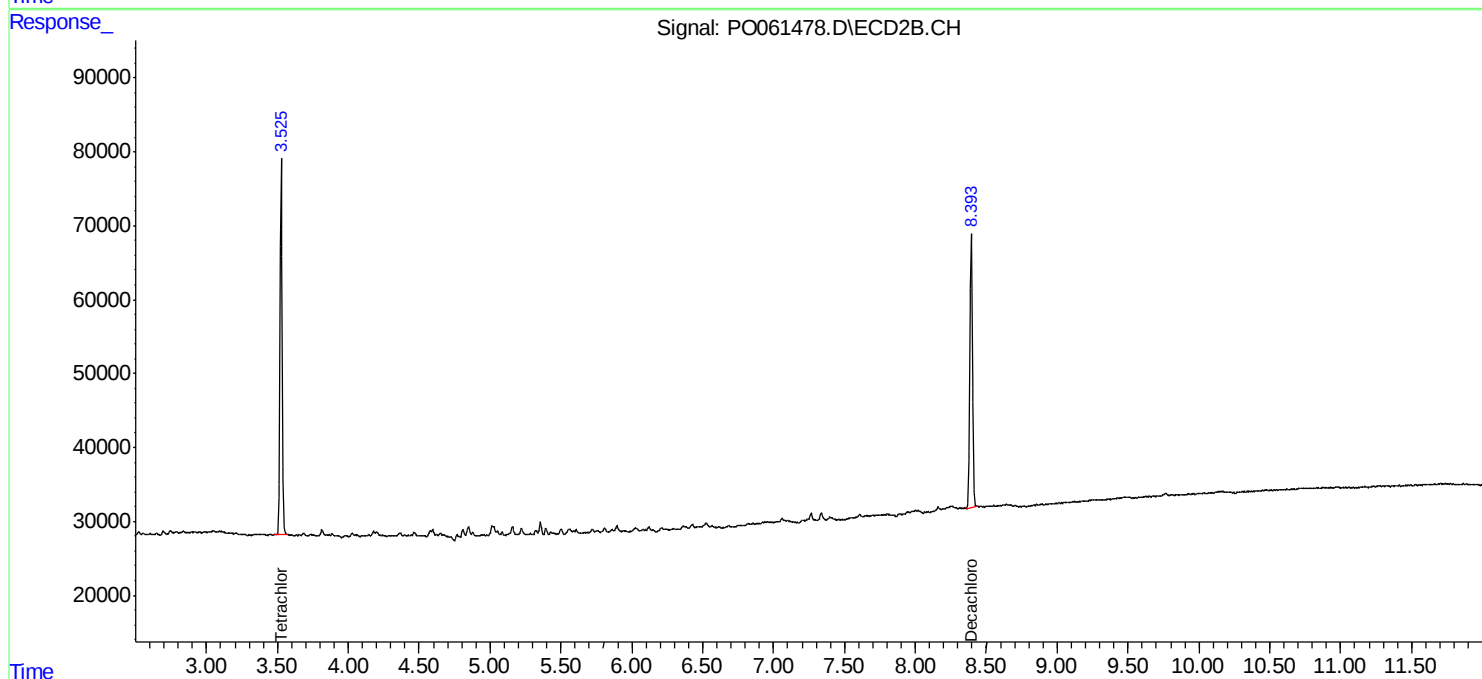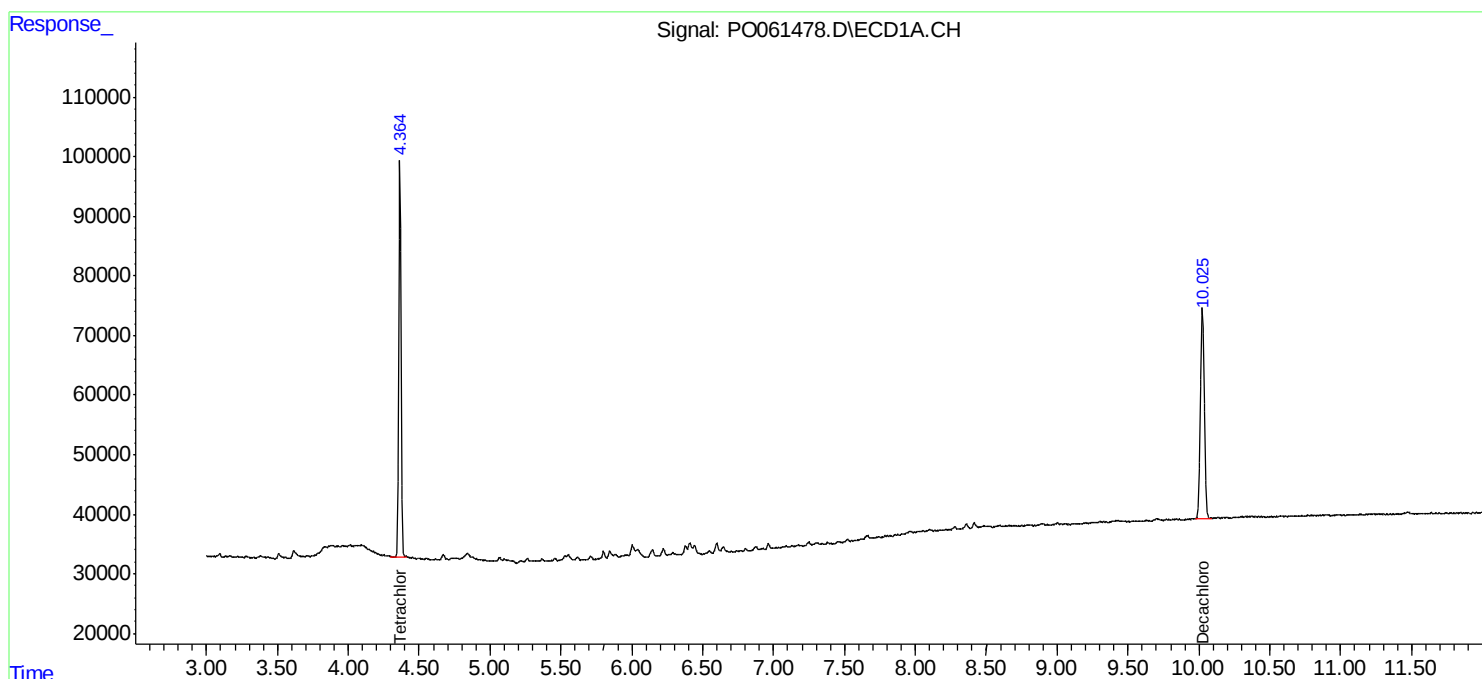

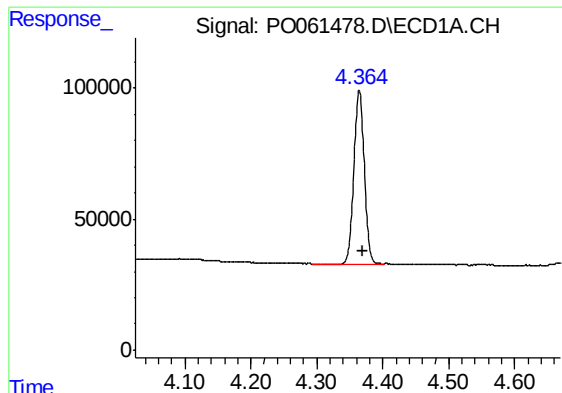


#1 Tetrachloro-m-xylene

R.T.: 4.364 min
Delta R.T.: -0.006 min
Response: 726236
Conc: 19.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
20190703-RR-COMPOSITE-3


Manual Integrations
APPROVED

Ankita
10/2/2019 9:23:17 AM

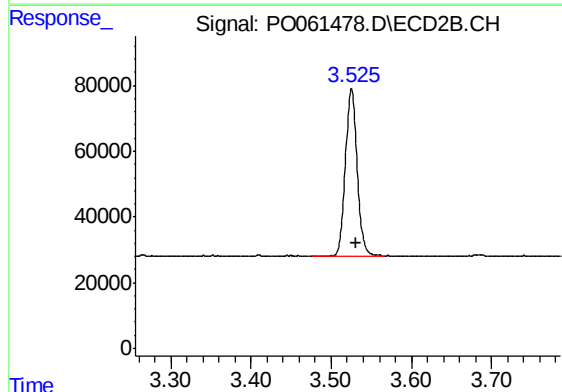


#1 Tetrachloro-m-xylene

R.T.: 3.525 min
Delta R.T.: -0.006 min
Response: 517049
Conc: 18.52 ng/ml

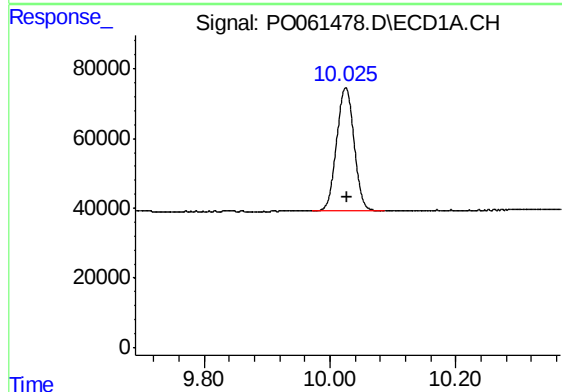

#2 Decachlorobiphenyl

R.T.: 10.025 min
Delta R.T.: -0.003 min
Response: 678265
Conc: 14.76 ng/ml

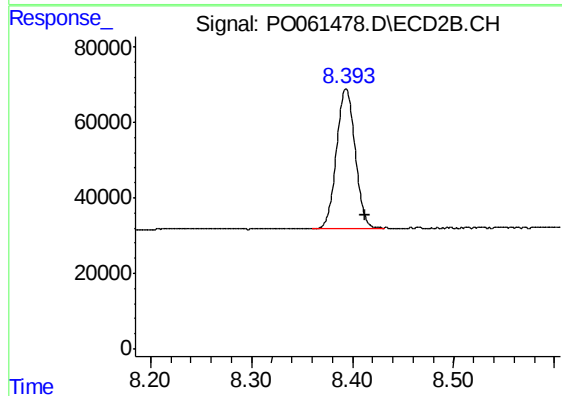

#2 Decachlorobiphenyl

R.T.: 8.394 min
Delta R.T.: -0.019 min
Response: 474000
Conc: 13.52 ng/ml