

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0093019\
 Data File : P0061480.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Sep 2019 19:45
 Operator : HP/AJ
 Sample : K5054-01RE
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PAT-091019-BRE

Manual Integrations
 APPROVED

Ankita
 10/2/2019 9:22:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 01:20:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.368	3.529	1534244	1043399	41.702	37.368m
2)	SA Decachlor...	10.024	8.394	1275713	867519	27.765m	24.750m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO093019\
Data File : PO061480.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Sep 2019 19:45
Operator : HP/AJ
Sample : K5054-01RE
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PAT-091019-BRE


Manual Integrations
APPROVED

Ankita
10/2/2019 9:22:56 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 01:20:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

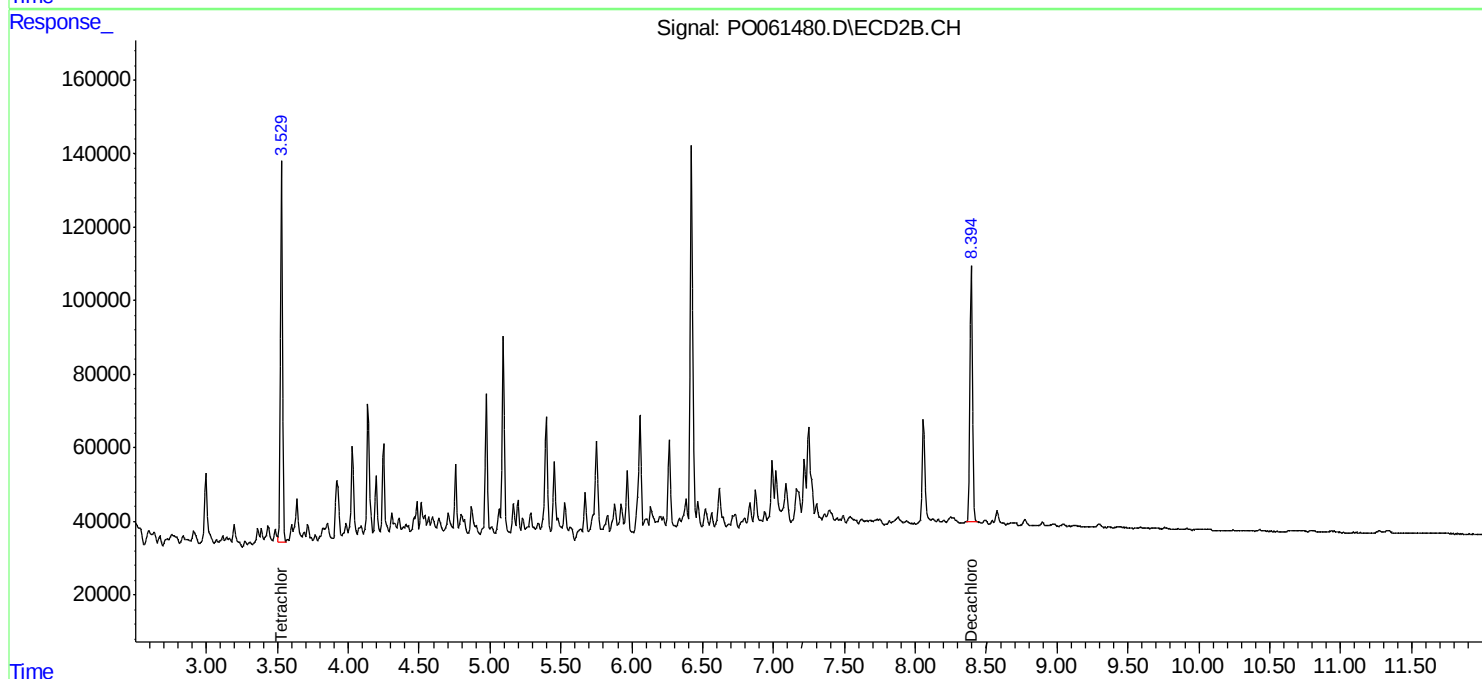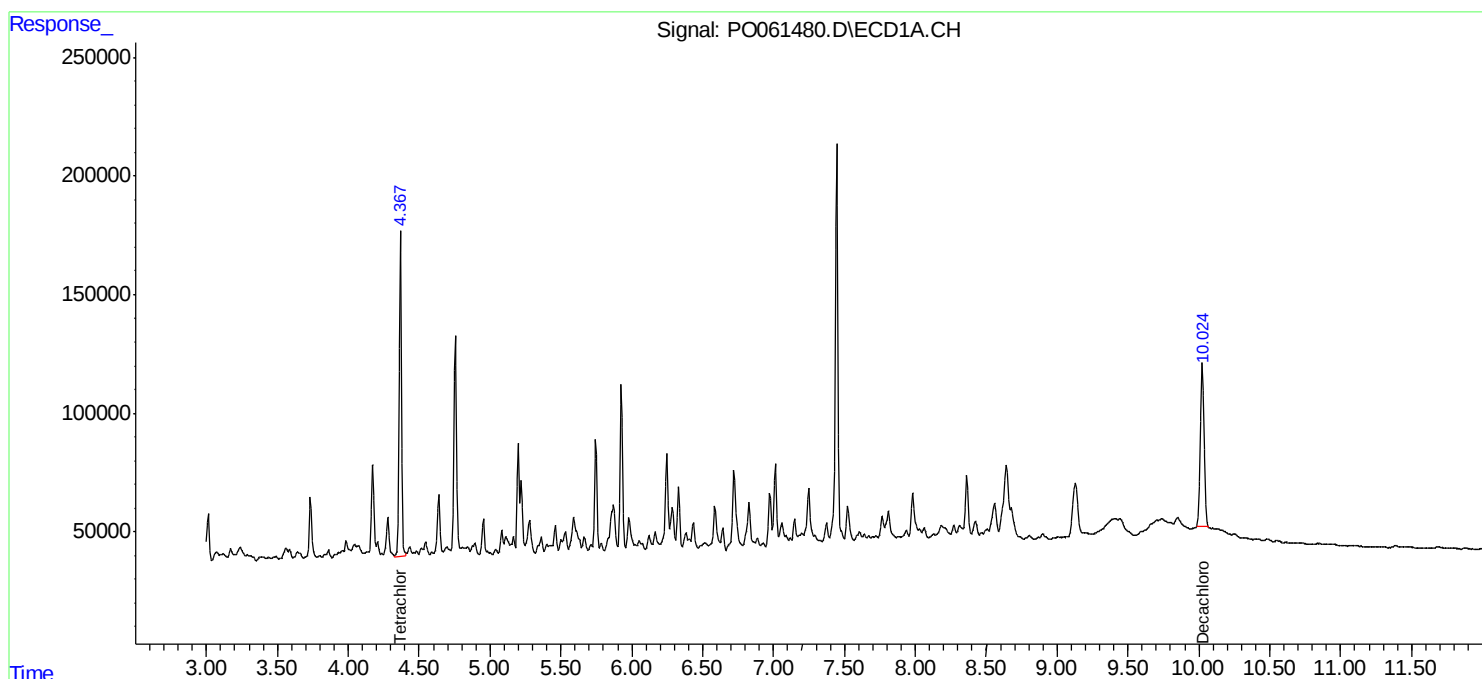

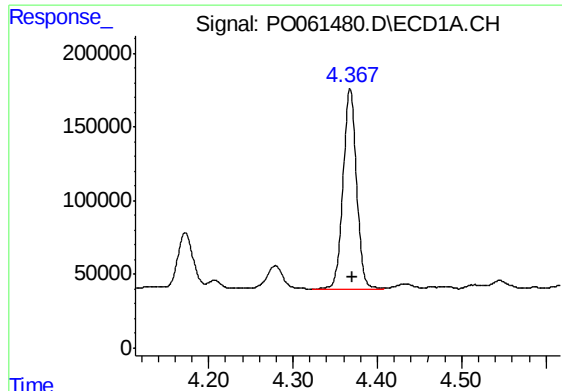


#1 Tetrachloro-m-xylene

R.T.: 4.368 min
Delta R.T.: -0.002 min
Response: 1534244
Conc: 41.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
PAT-091019-BRE


Manual Integrations
APPROVED

Ankita
10/2/2019 9:22:56 AM

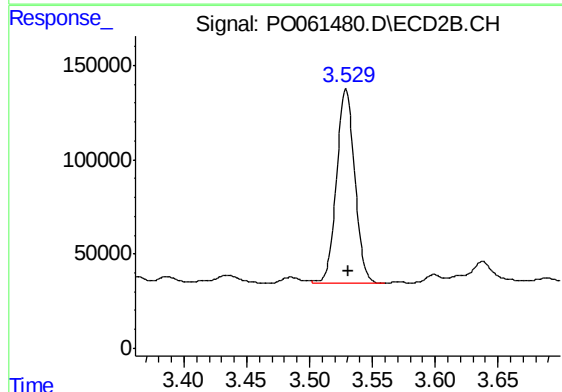


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: -0.003 min
Response: 1043399
Conc: 37.37 ng/ml m

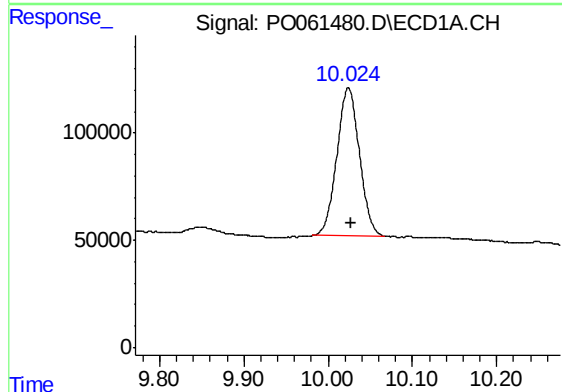

#2 Decachlorobiphenyl

R.T.: 10.024 min
Delta R.T.: -0.004 min
Response: 1275713
Conc: 27.77 ng/ml m

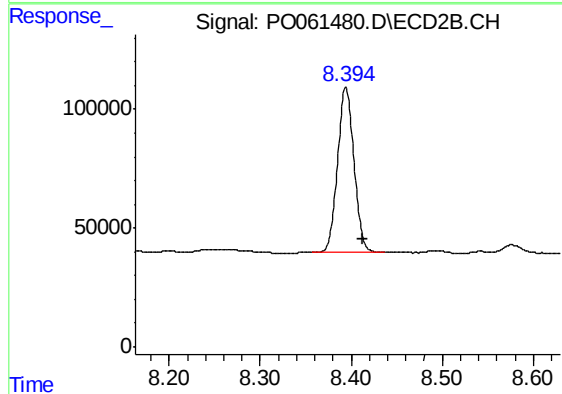

#2 Decachlorobiphenyl

R.T.: 8.394 min
Delta R.T.: -0.019 min
Response: 867519
Conc: 24.75 ng/ml m