

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0093019\
Data File : P0061495.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Oct 2019 3:37
Operator : HP/AJ
Sample : K5093-02
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-01-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 08:10:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.365	3.526	1185638	915438	32.226	32.785
2)	SA Decachlor...	10.026	8.395	1043405	732638	22.709	20.902

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO093019\
Data File : PO061495.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Oct 2019 3:37
Operator : HP/AJ
Sample : K5093-02
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-01-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 08:10:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

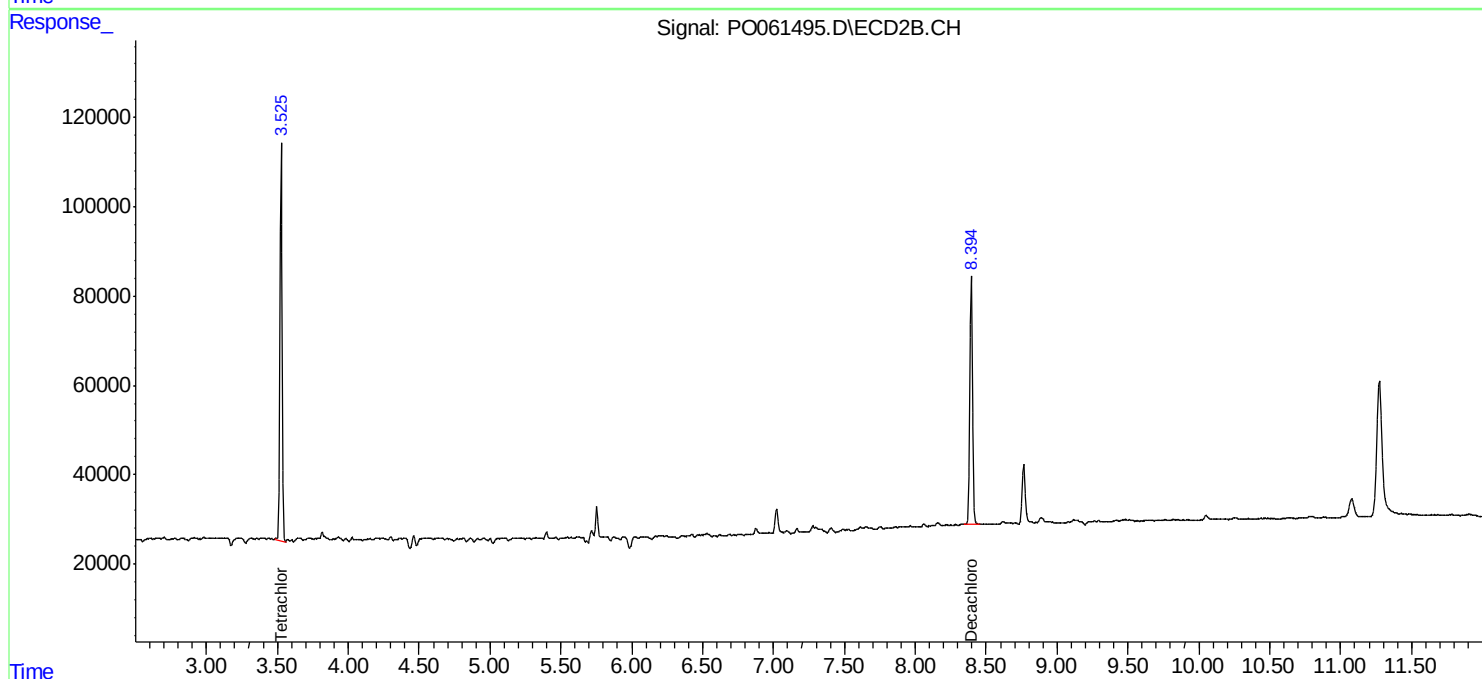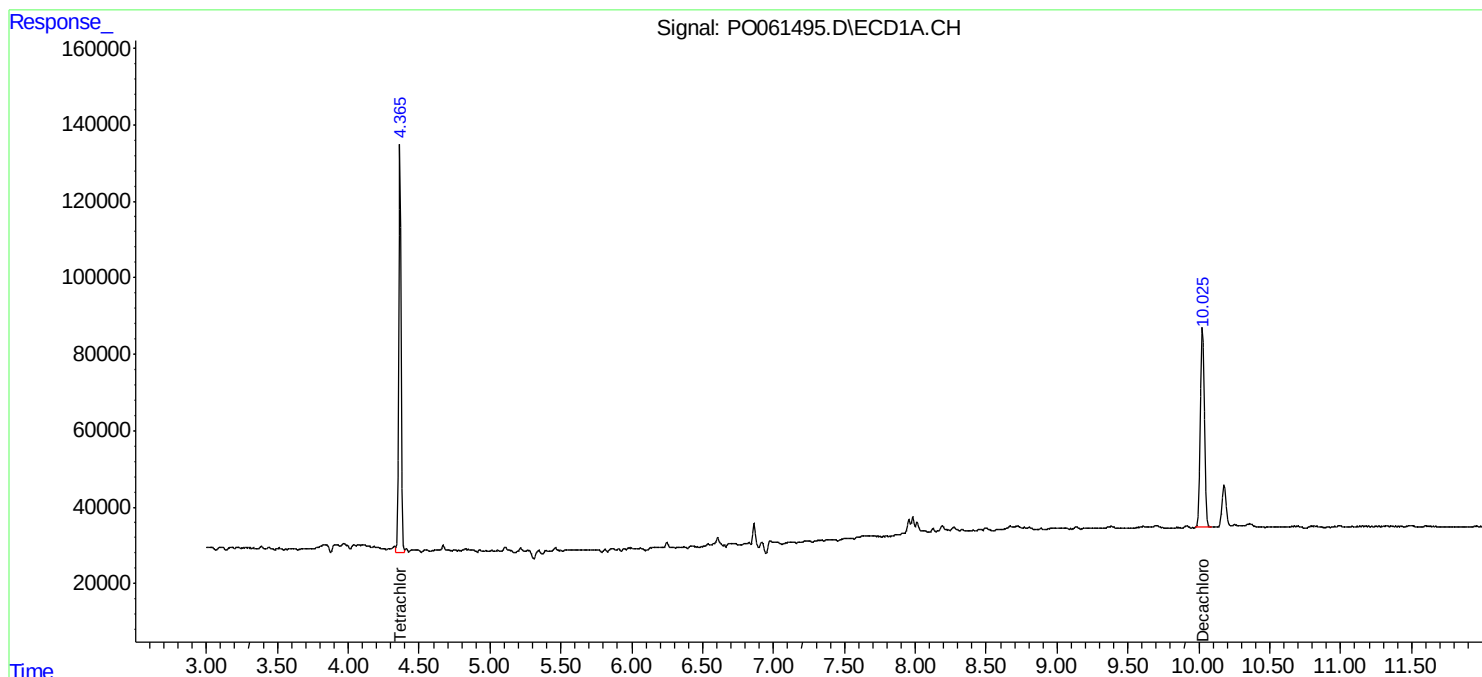


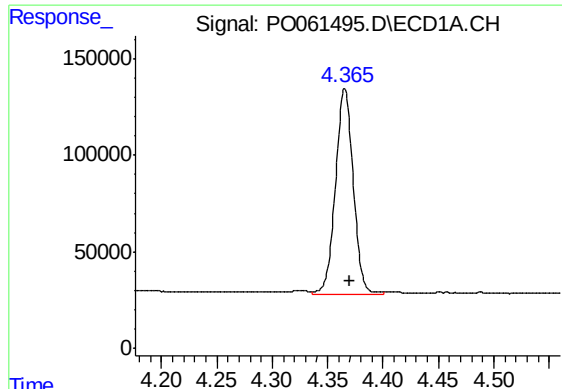

#1 Tetrachloro-m-xylene


R.T.: 4.365 min
Delta R.T.: -0.005 min
Response: 1185638
Conc: 32.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-01-COMP

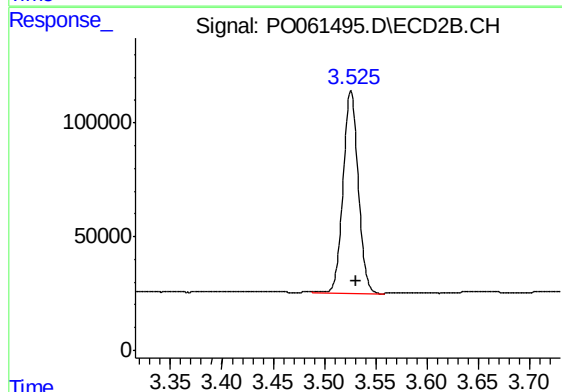


#1 Tetrachloro-m-xylene

R.T.: 3.526 min
Delta R.T.: -0.005 min
Response: 915438
Conc: 32.79 ng/ml

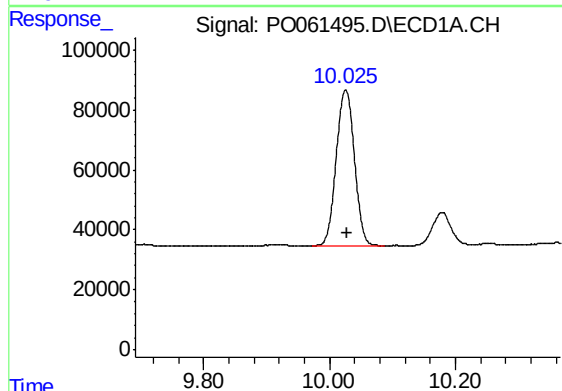

#2 Decachlorobiphenyl

R.T.: 10.026 min
Delta R.T.: -0.002 min
Response: 1043405
Conc: 22.71 ng/ml

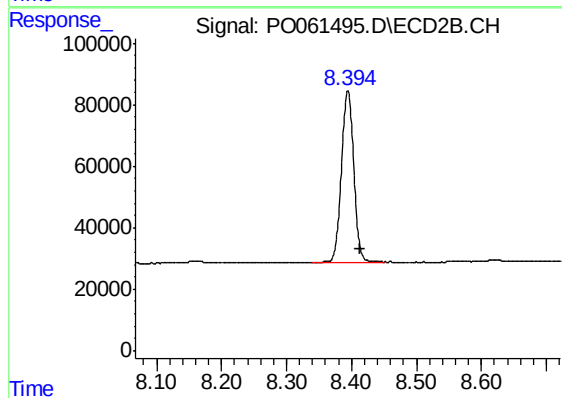

#2 Decachlorobiphenyl

R.T.: 8.395 min
Delta R.T.: -0.019 min
Response: 732638
Conc: 20.90 ng/ml