

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100118\
Data File : P0049502.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Oct 2018 9:14
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 05:16:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 01 14:47:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.382	3.516	4986501	4952694	14.121	14.562
2)	SA Decachlor...	10.088	8.443	6854315	4701271	14.465	15.387

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100118\
Data File : P0049502.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Oct 2018 9:14
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 05:16:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 01 14:47:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

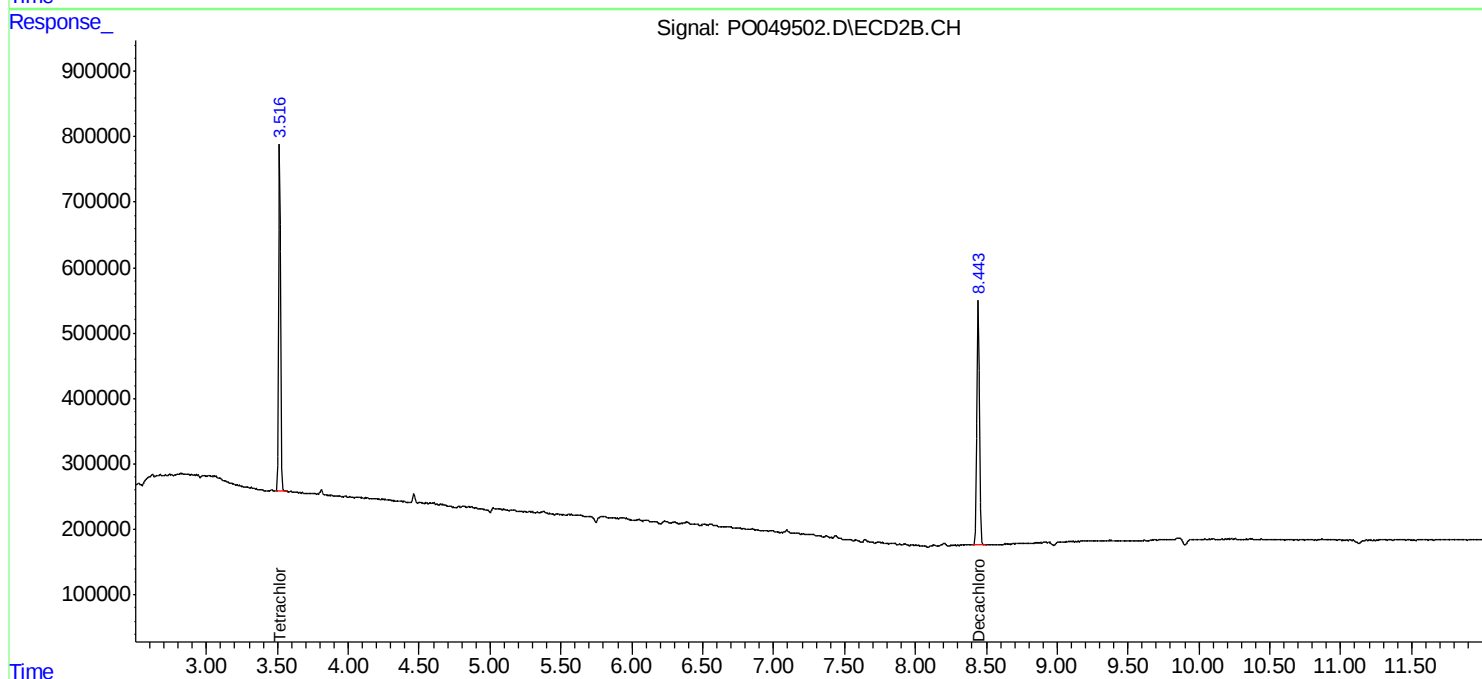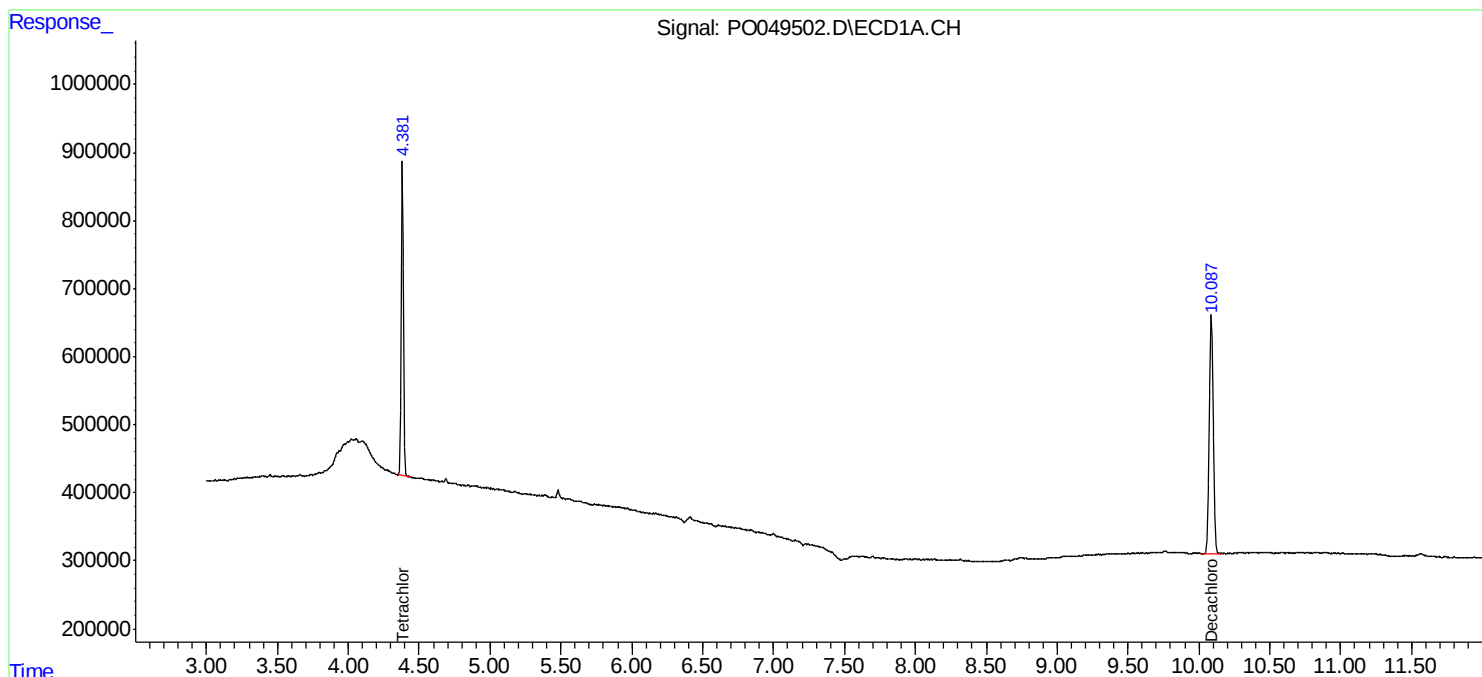


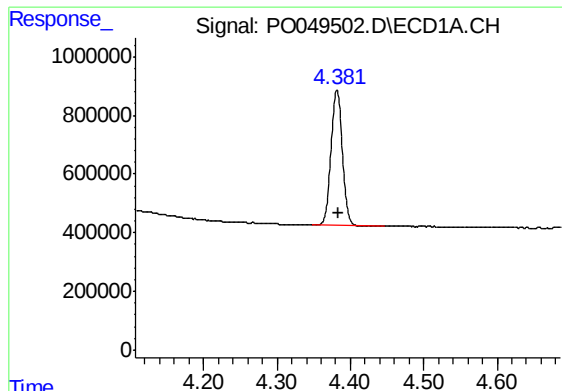

#1 Tetrachloro-m-xylene


R.T.: 4.382 min
Delta R.T.: -0.001 min
Response: 4986501
Conc: 14.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

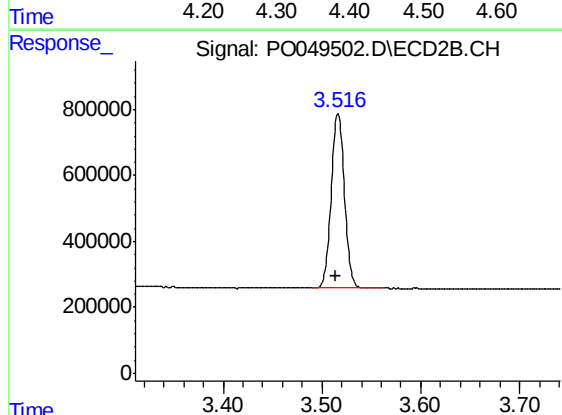


#1 Tetrachloro-m-xylene

R.T.: 3.516 min
Delta R.T.: 0.002 min
Response: 4952694
Conc: 14.56 ng/ml

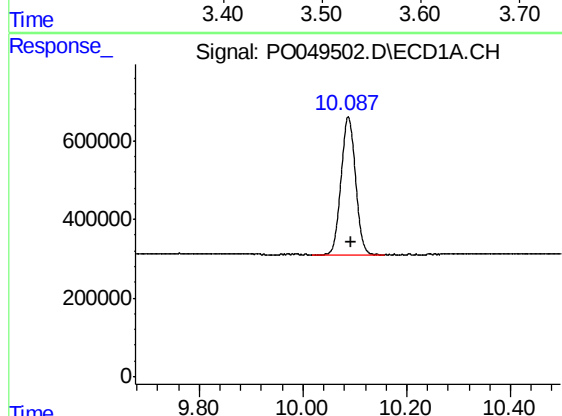

#2 Decachlorobiphenyl

R.T.: 10.088 min
Delta R.T.: -0.006 min
Response: 6854315
Conc: 14.46 ng/ml

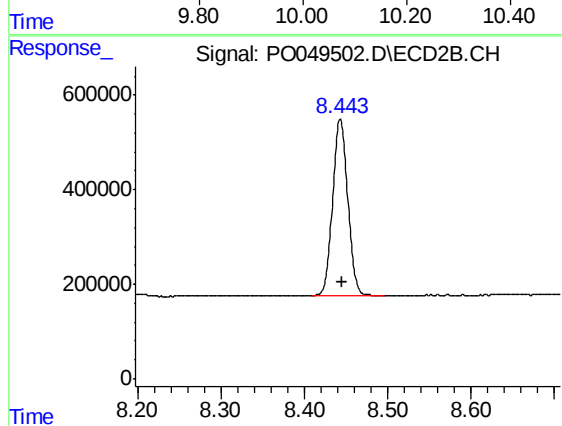

#2 Decachlorobiphenyl

R.T.: 8.443 min
Delta R.T.: -0.002 min
Response: 4701271
Conc: 15.39 ng/ml