

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100119\
 Data File : P0061531.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Oct 2019 18:36
 Operator : HP/AJ
 Sample : K5093-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-03-COMP

Manual Integrations
 APPROVED

Ankita
 10/2/2019 1:21:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 01:35:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.366	3.525	962023	749372	23.456	23.172
2)	SA Decachlor...	10.028	8.394	944262	758747	20.276m	23.436
Target Compounds							
31)	L7 AR-1260-1	7.125	6.022	269313	214556	103.164	105.185
32)	L7 AR-1260-2	7.379	6.208	613984	257702	192.592	107.298 #
33)	L7 AR-1260-3	7.739	6.357	258295	195029	107.539	86.560
34)	L7 AR-1260-4	7.963	6.821	383424	162155	143.495	87.831 #
35)	L7 AR-1260-5	8.278	7.060	502390	333984	101.531	85.777

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100119\
Data File : PO061531.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Oct 2019 18:36
Operator : HP/AJ
Sample : K5093-06
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SB-03-COMP


Manual Integrations
APPROVED

Ankita
10/2/2019 1:21:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 01:35:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

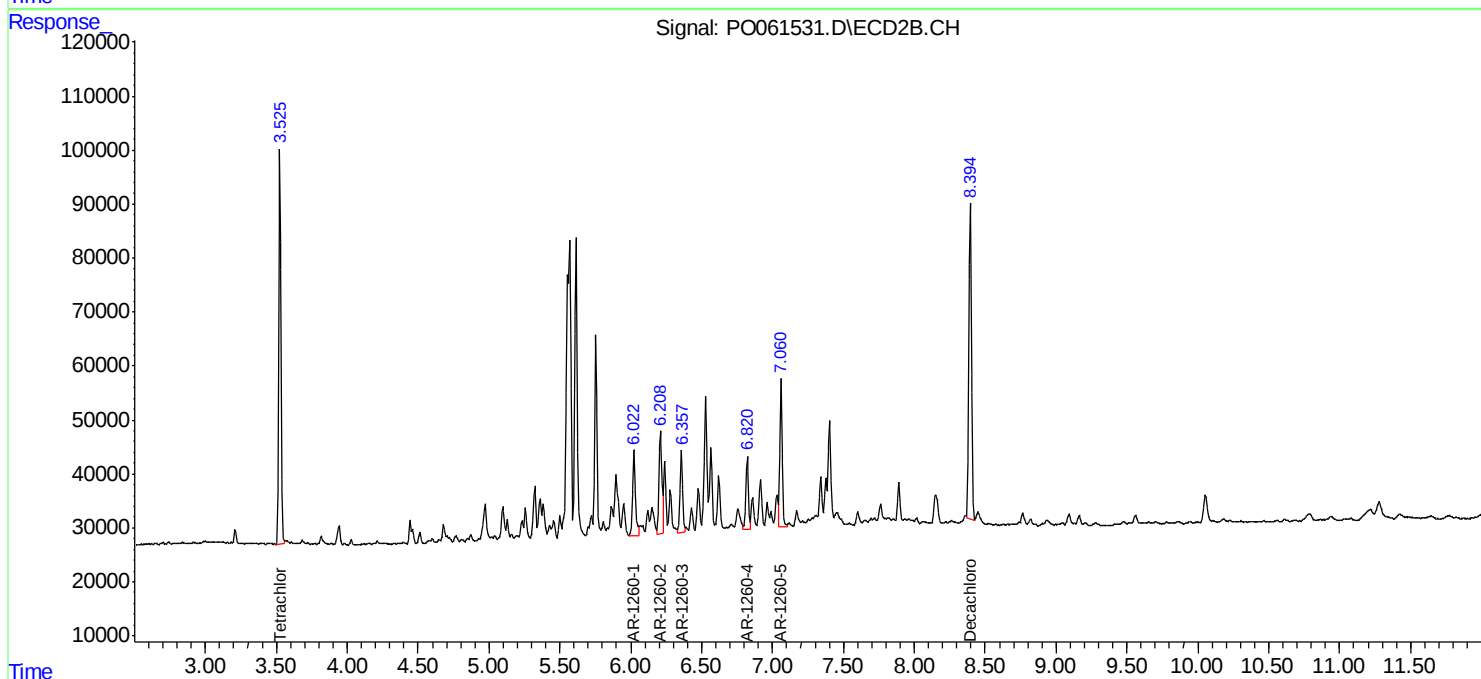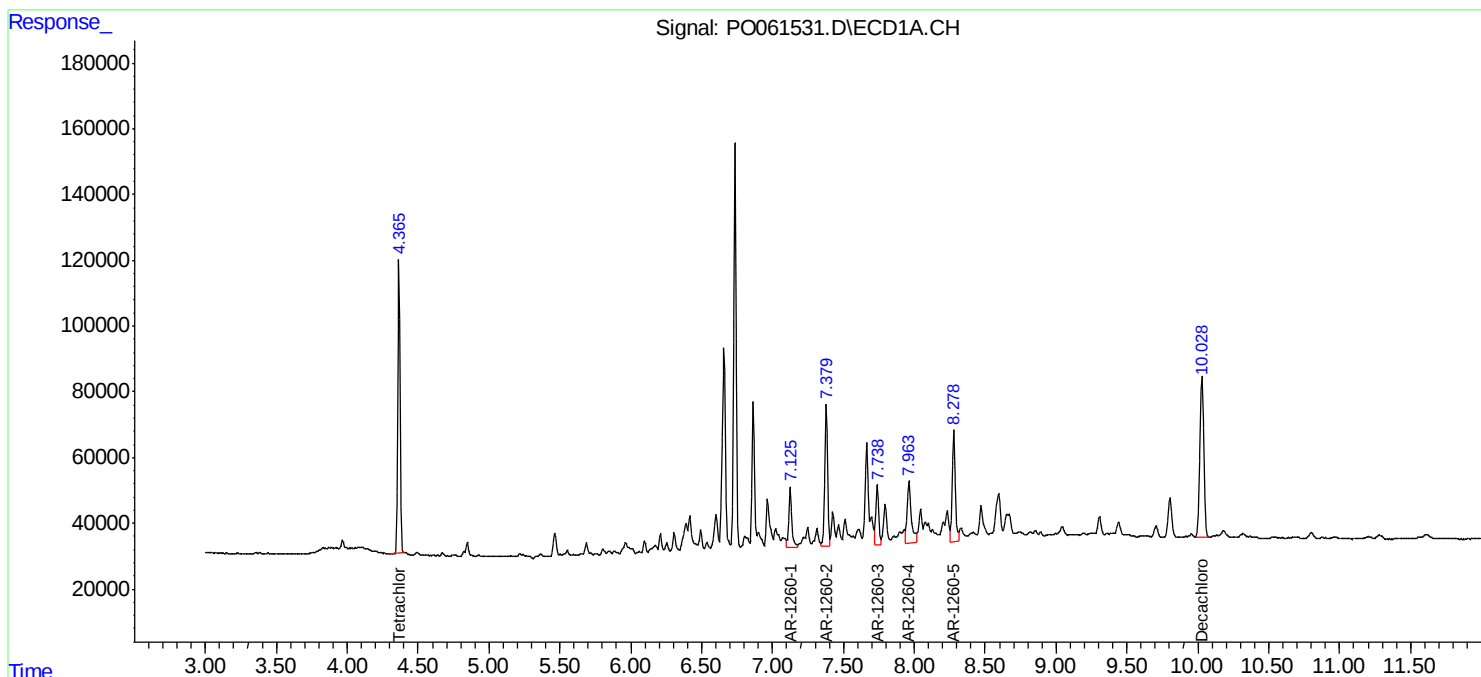

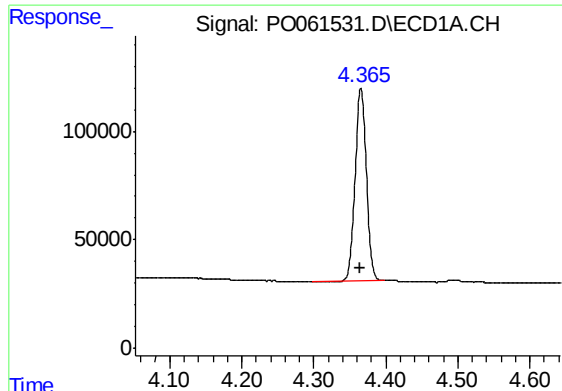


#1 Tetrachloro-m-xylene

R.T.: 4.366 min
Delta R.T.: 0.000 min
Response: 962023
Conc: 23.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-03-COMP


Manual Integrations
APPROVED

Ankita
10/2/2019 1:21:12 PM

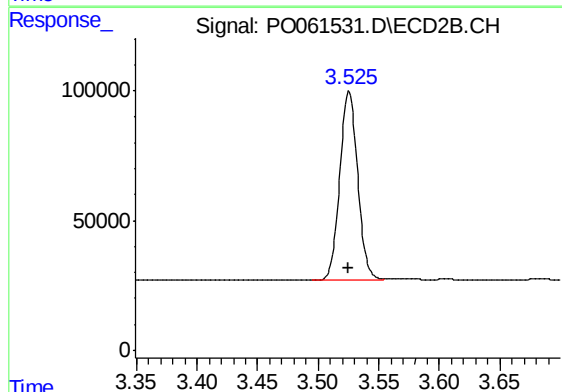


#1 Tetrachloro-m-xylene

R.T.: 3.525 min
Delta R.T.: 0.000 min
Response: 749372
Conc: 23.17 ng/ml

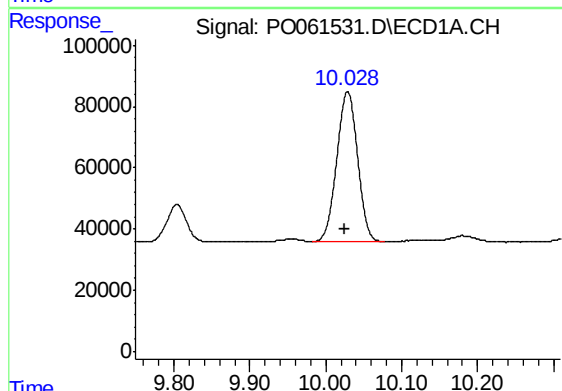


#2 Decachlorobiphenyl

R.T.: 10.028 min
Delta R.T.: 0.003 min
Response: 944262
Conc: 20.28 ng/ml m

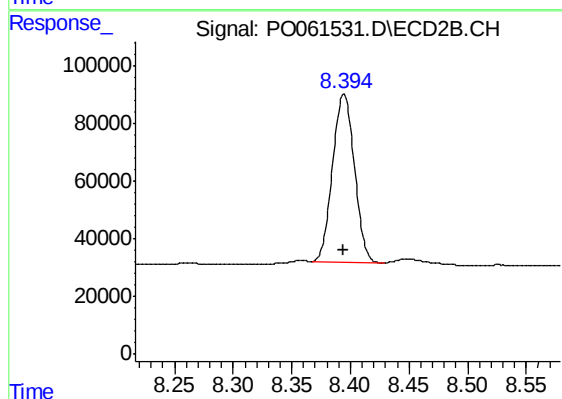

#2 Decachlorobiphenyl

R.T.: 8.394 min
Delta R.T.: 0.000 min
Response: 758747
Conc: 23.44 ng/ml

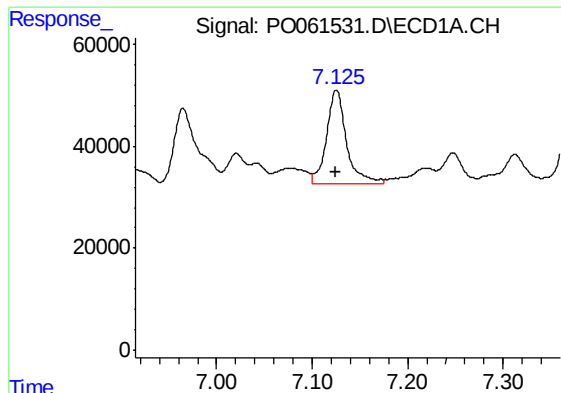


#31 AR-1260-1

R.T.: 7.125 min
Delta R.T.: 0.000 min
Response: 269313
Conc: 103.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-03-COMP


Manual Integrations
APPROVED

Ankita
10/2/2019 1:21:12 PM

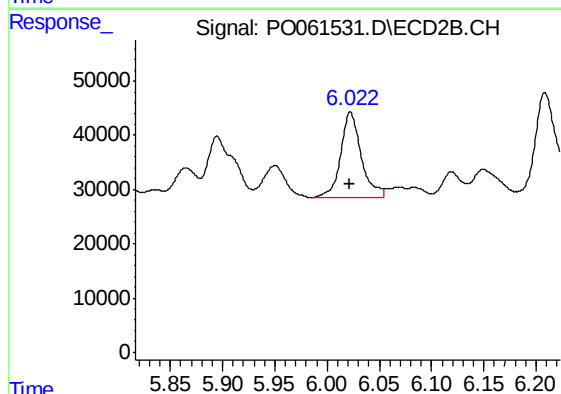


#31 AR-1260-1

R.T.: 6.022 min
Delta R.T.: 0.001 min
Response: 214556
Conc: 105.19 ng/ml

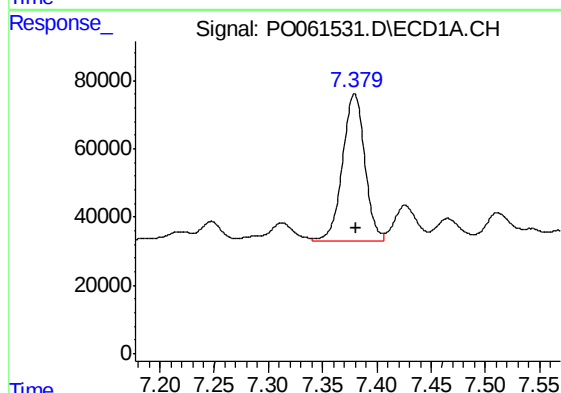


#32 AR-1260-2

R.T.: 7.379 min
Delta R.T.: -0.002 min
Response: 613984
Conc: 192.59 ng/ml

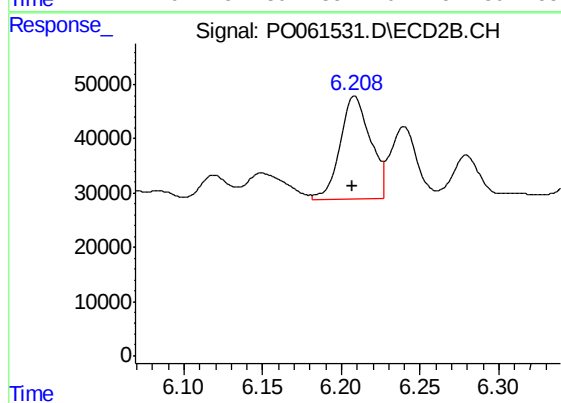

#32 AR-1260-2

R.T.: 6.208 min
Delta R.T.: 0.002 min
Response: 257702
Conc: 107.30 ng/ml

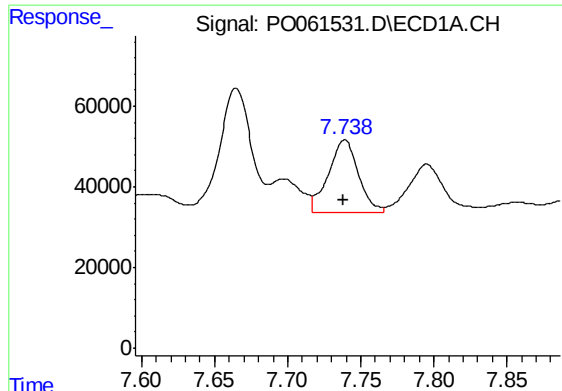


#33 AR-1260-3

R.T.: 7.739 min
Delta R.T.: 0.000 min
Response: 258295
Conc: 107.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-03-COMP


Manual Integrations
APPROVED

Ankita
10/2/2019 1:21:12 PM

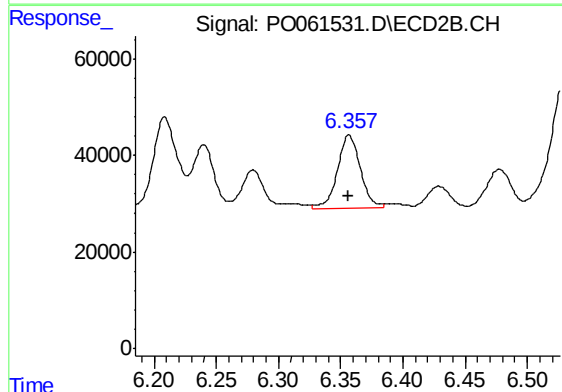


#33 AR-1260-3

R.T.: 6.357 min
Delta R.T.: 0.000 min
Response: 195029
Conc: 86.56 ng/ml

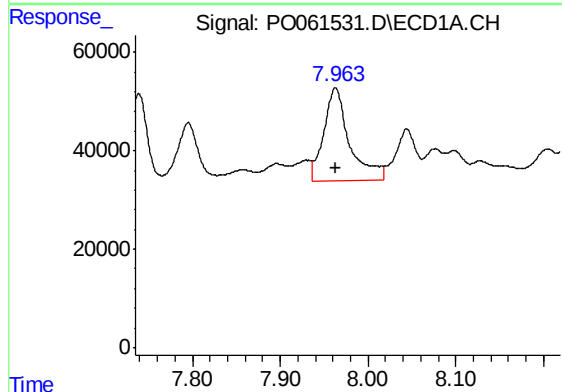


#34 AR-1260-4

R.T.: 7.963 min
Delta R.T.: 0.000 min
Response: 383424
Conc: 143.49 ng/ml

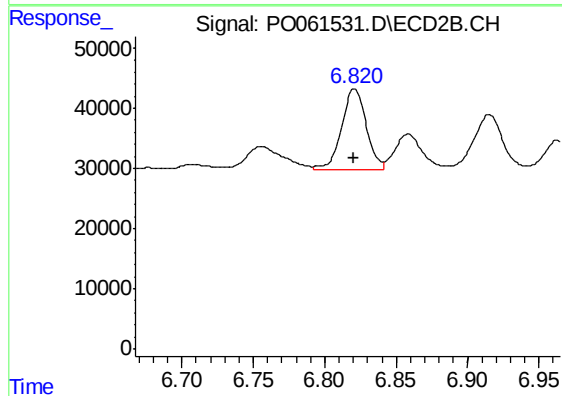

#34 AR-1260-4

R.T.: 6.821 min
Delta R.T.: 0.000 min
Response: 162155
Conc: 87.83 ng/ml

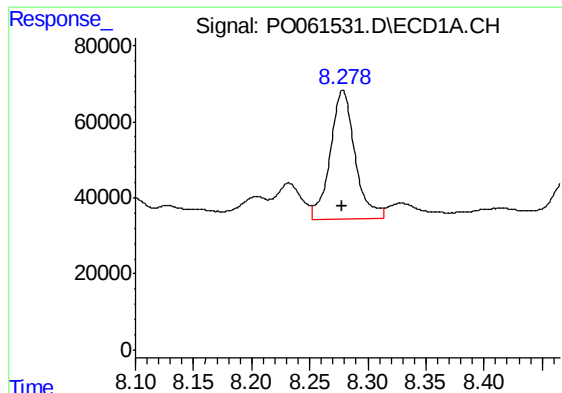


#35 AR-1260-5

R.T.: 8.278 min
Delta R.T.: 0.001 min
Response: 502390
Conc: 101.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-03-COMP

Manual Integrations
APPROVED

Ankita
10/2/2019 1:21:12 PM

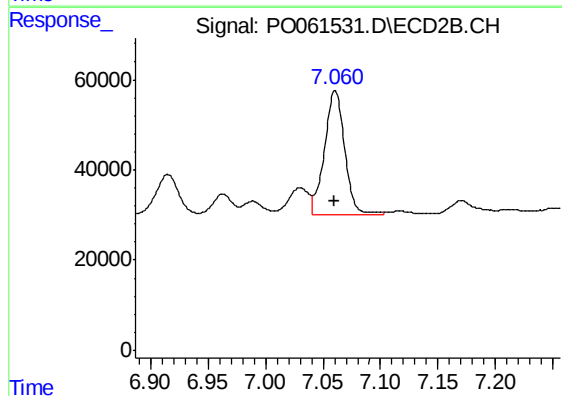

#35 AR-1260-5

R.T.: 7.060 min
Delta R.T.: 0.000 min
Response: 333984
Conc: 85.78 ng/ml