

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100119\
 Data File : P0061533.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Oct 2019 19:08
 Operator : HP/AJ
 Sample : K5076-06RE
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SIMW-04-20190926RE

Manual Integrations
 APPROVED

Ankita
 10/2/2019 1:21:14 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 01:36:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.368	3.529	1247608	957396	30.419	29.605
2)	SA Decachlor...	10.026	8.395	1126684	781863	24.193	24.150m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100119\
Data File : PO061533.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Oct 2019 19:08
Operator : HP/AJ
Sample : K5076-06RE
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SIMW-04-20190926RE


Manual Integrations
APPROVED

Ankita
10/2/2019 1:21:14 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 01:36:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

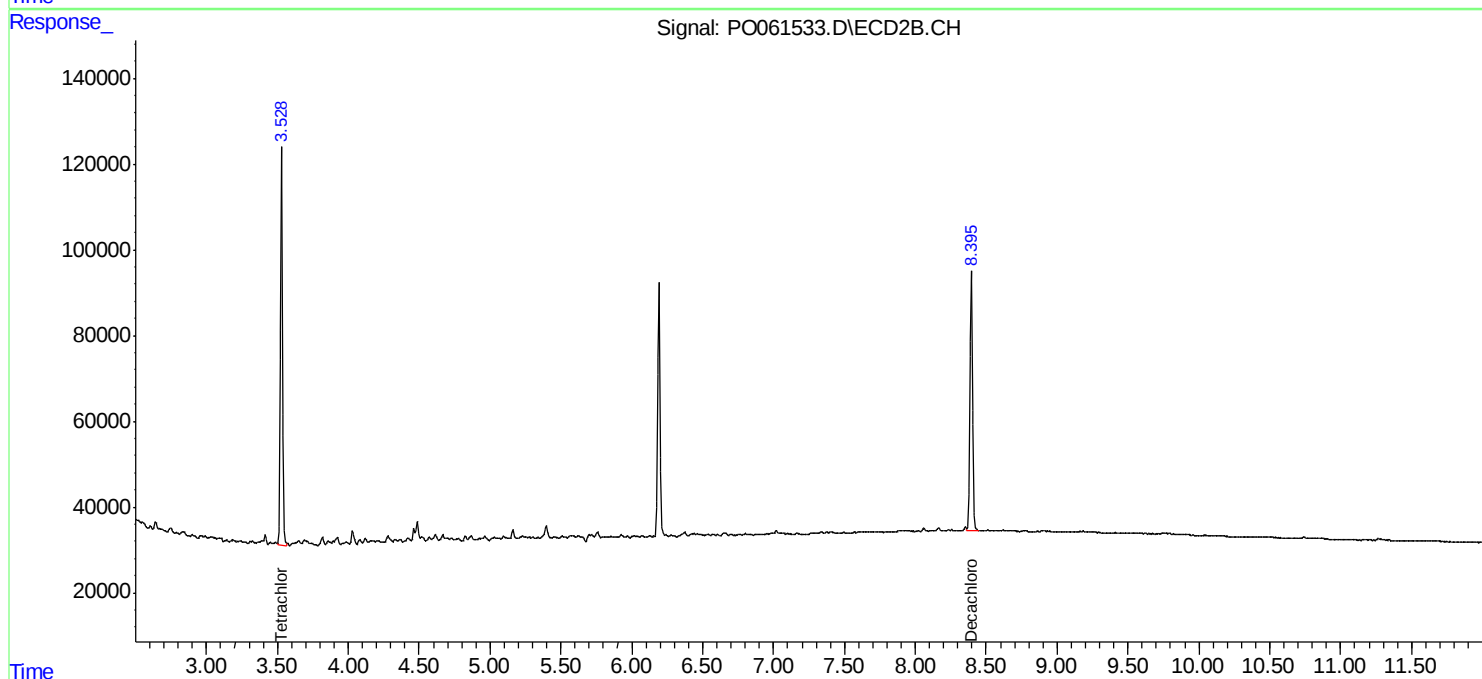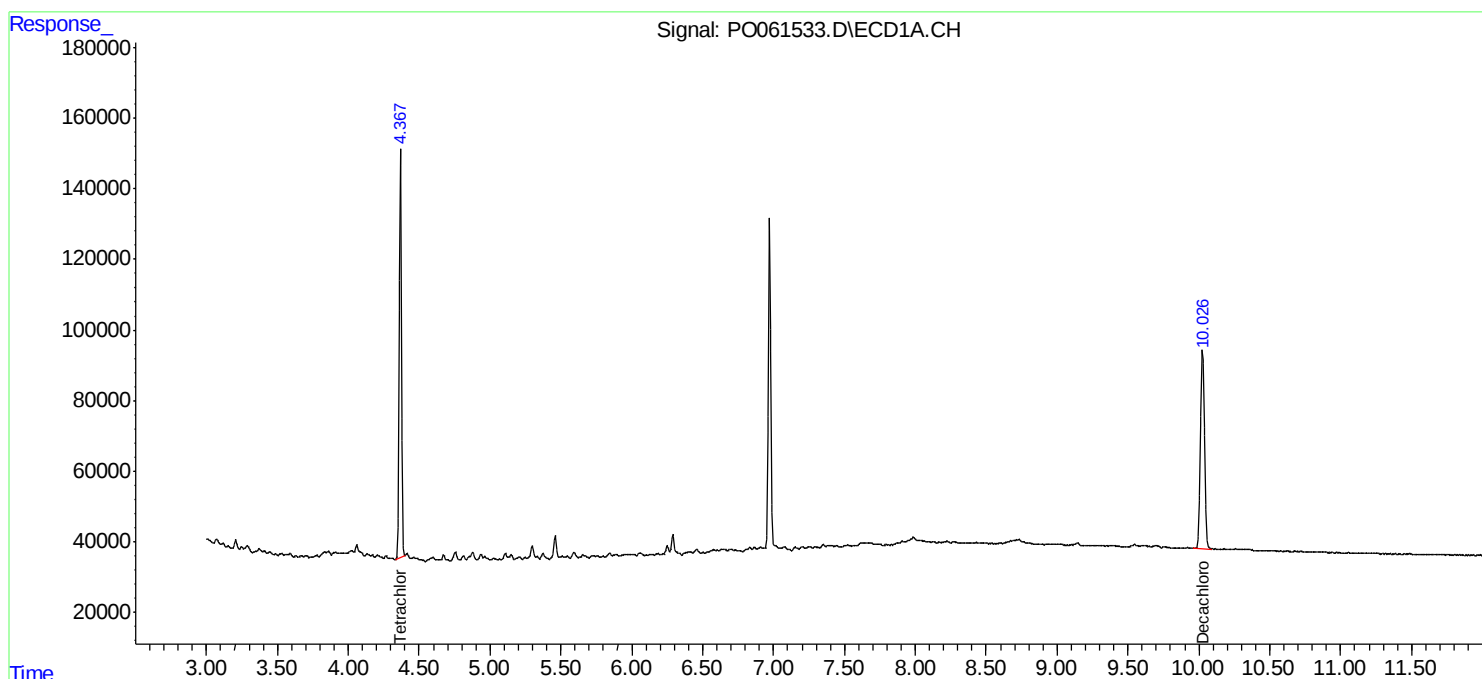

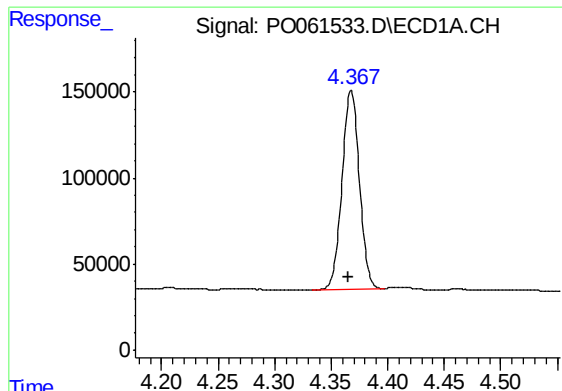


#1 Tetrachloro-m-xylene

R.T.: 4.368 min
Delta R.T.: 0.003 min
Response: 1247608
Conc: 30.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
SIMW-04-20190926RE


Manual Integrations
APPROVED

Ankita
10/2/2019 1:21:14 PM

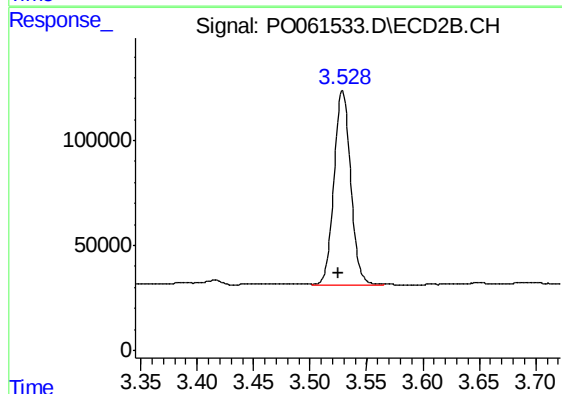


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: 0.003 min
Response: 957396
Conc: 29.60 ng/ml

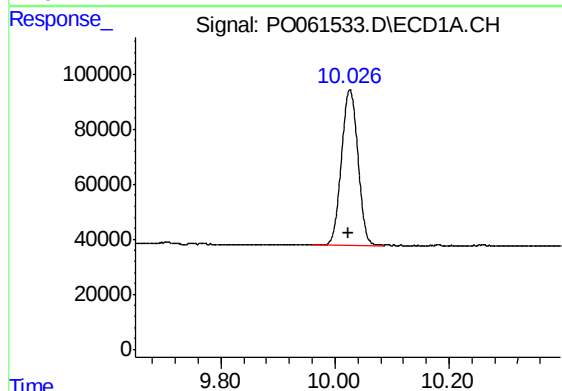

#2 Decachlorobiphenyl

R.T.: 10.026 min
Delta R.T.: 0.001 min
Response: 1126684
Conc: 24.19 ng/ml

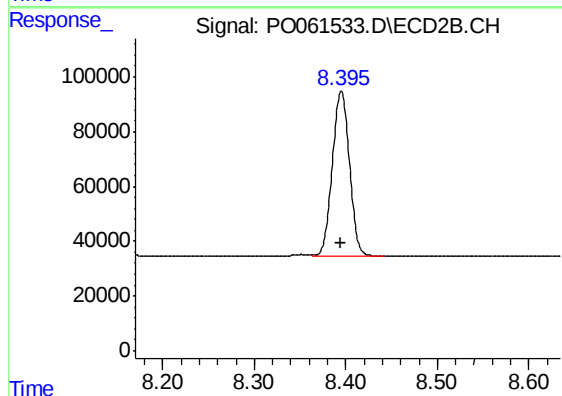

#2 Decachlorobiphenyl

R.T.: 8.395 min
Delta R.T.: 0.000 min
Response: 781863
Conc: 24.15 ng/ml m