

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100119\
 Data File : P0061557.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Oct 2019 3:00
 Operator : HP/AJ
 Sample : K5079-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-1-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 05:25:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.365	3.525	941946	724740	22.966	22.410
2)	SA Decachlor...	10.029	8.394	996474	698539	21.397	21.576

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100119\
Data File : PO061557.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Oct 2019 3:00
Operator : HP/AJ
Sample : K5079-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-1-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 05:25:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

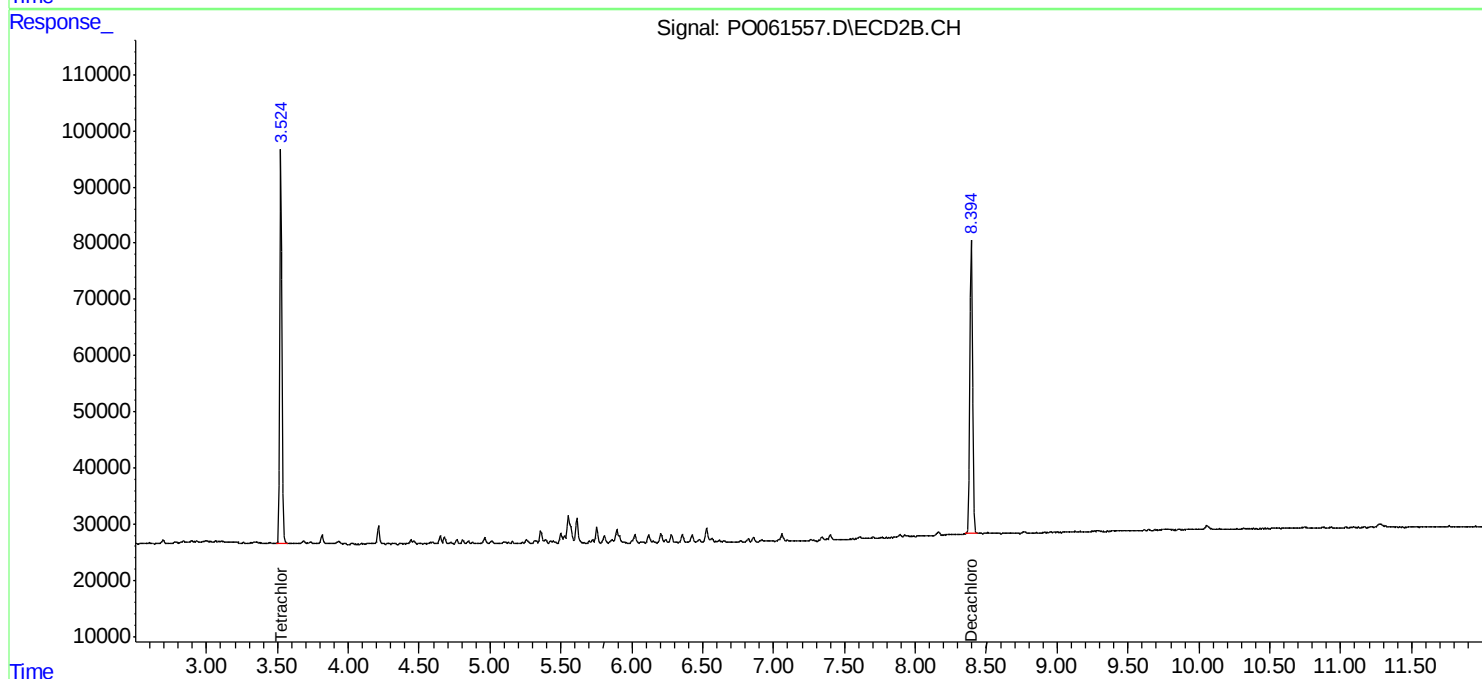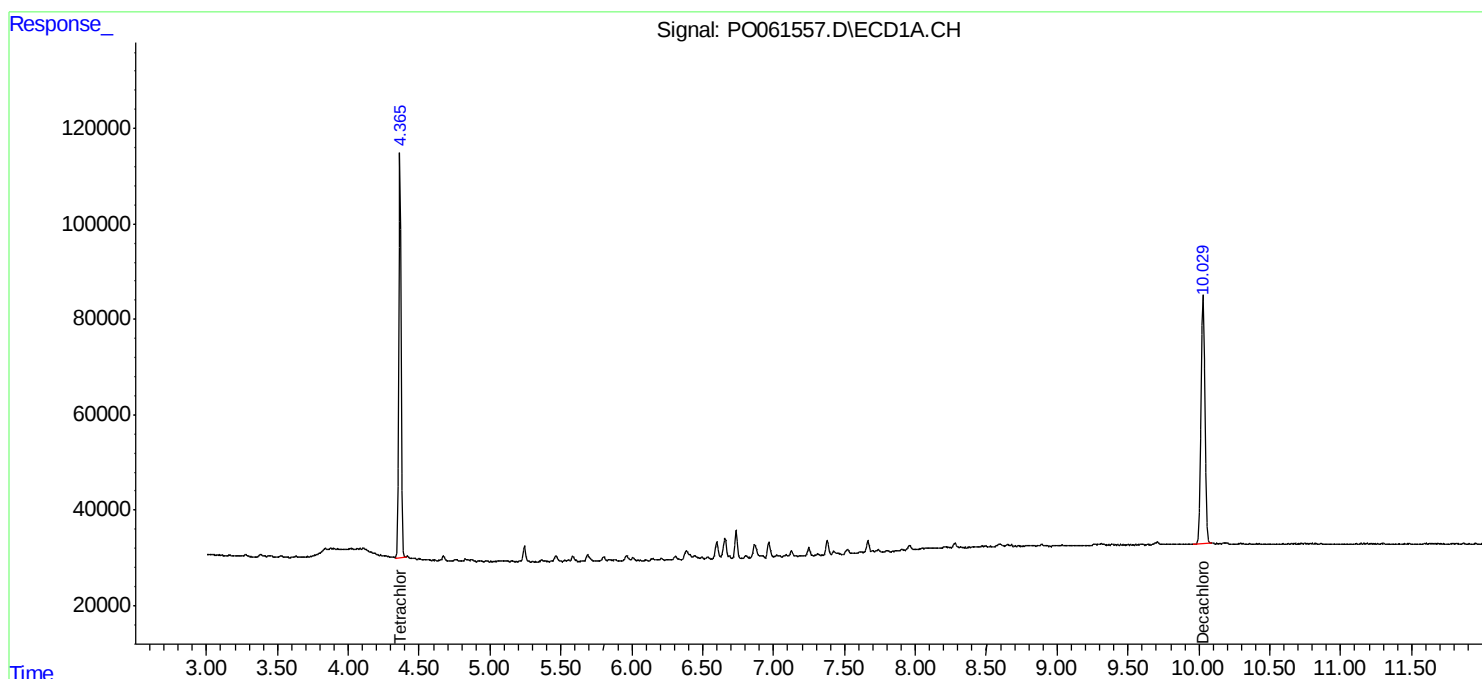


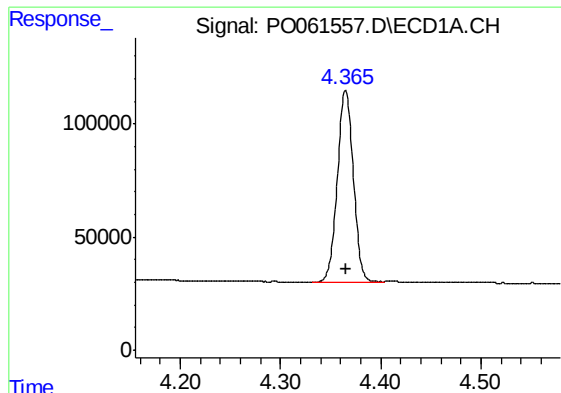

#1 Tetrachloro-m-xylene


R.T.: 4.365 min
Delta R.T.: 0.000 min
Response: 941946
Conc: 22.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1-COMP

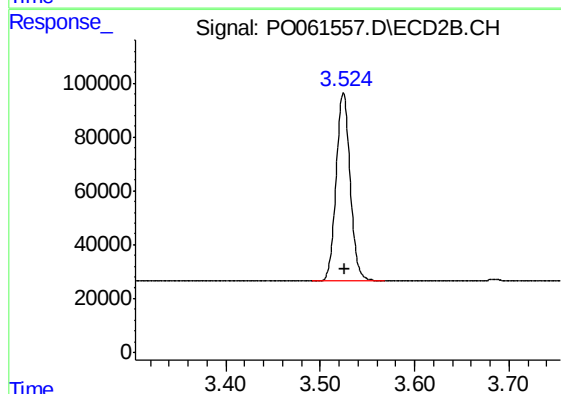


#1 Tetrachloro-m-xylene

R.T.: 3.525 min
Delta R.T.: 0.000 min
Response: 724740
Conc: 22.41 ng/ml

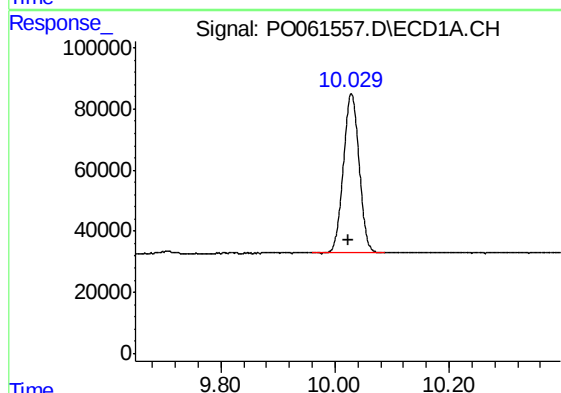

#2 Decachlorobiphenyl

R.T.: 10.029 min
Delta R.T.: 0.004 min
Response: 996474
Conc: 21.40 ng/ml

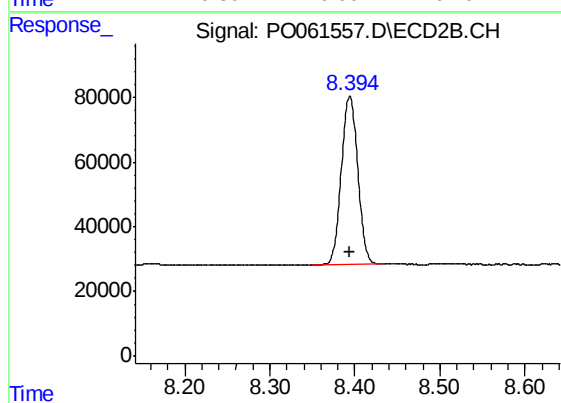

#2 Decachlorobiphenyl

R.T.: 8.394 min
Delta R.T.: 0.000 min
Response: 698539
Conc: 21.58 ng/ml