

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100119\
 Data File : P0061563.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Oct 2019 4:38
 Operator : HP/AJ
 Sample : K4853-04
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AOC14-02-B4-(24-30)

Manual Integrations
 APPROVED

Ankita
 10/2/2019 1:21:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 07:05:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.366	3.525	832700	648127	20.303	20.041m
2)	SA Decachlor...	10.031	8.395	625503	427189	13.431	13.195
Target Compounds							
26)	L6 AR-1254-1	6.380	5.356	164403	143238	72.063	65.308m
27)	L6 AR-1254-2	6.598	5.500	271073	128863	75.026	65.730m
28)	L6 AR-1254-3	6.963	5.894	285643	235243	73.104	73.889
29)	L6 AR-1254-4	7.249	6.119	199406	130498	65.840	64.321
30)	L6 AR-1254-5	7.666	6.529	230499	210848	73.398	74.545

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100119\
Data File : PO061563.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Oct 2019 4:38
Operator : HP/AJ
Sample : K4853-04
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AOC14-02-B4-(24-30)


Manual Integrations
APPROVED

Ankita
10/2/2019 1:21:28 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 07:05:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

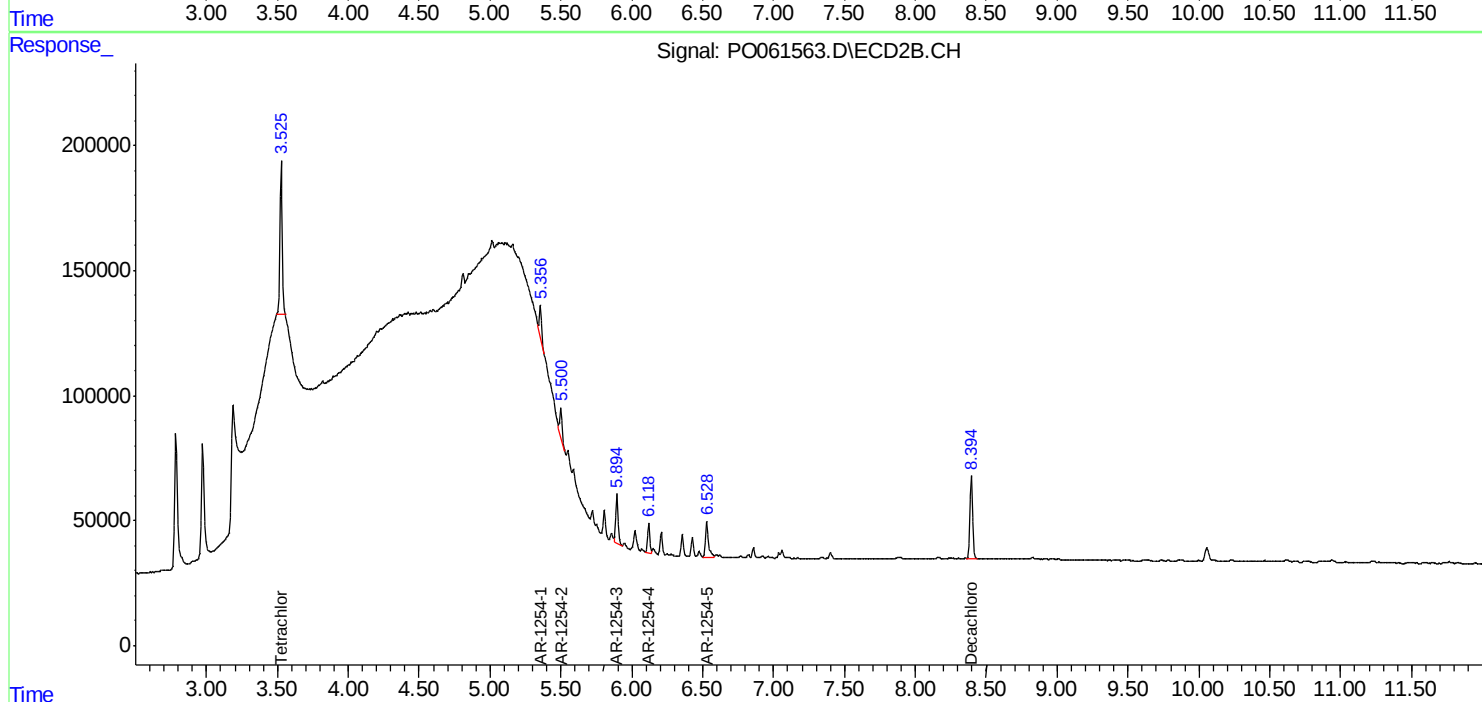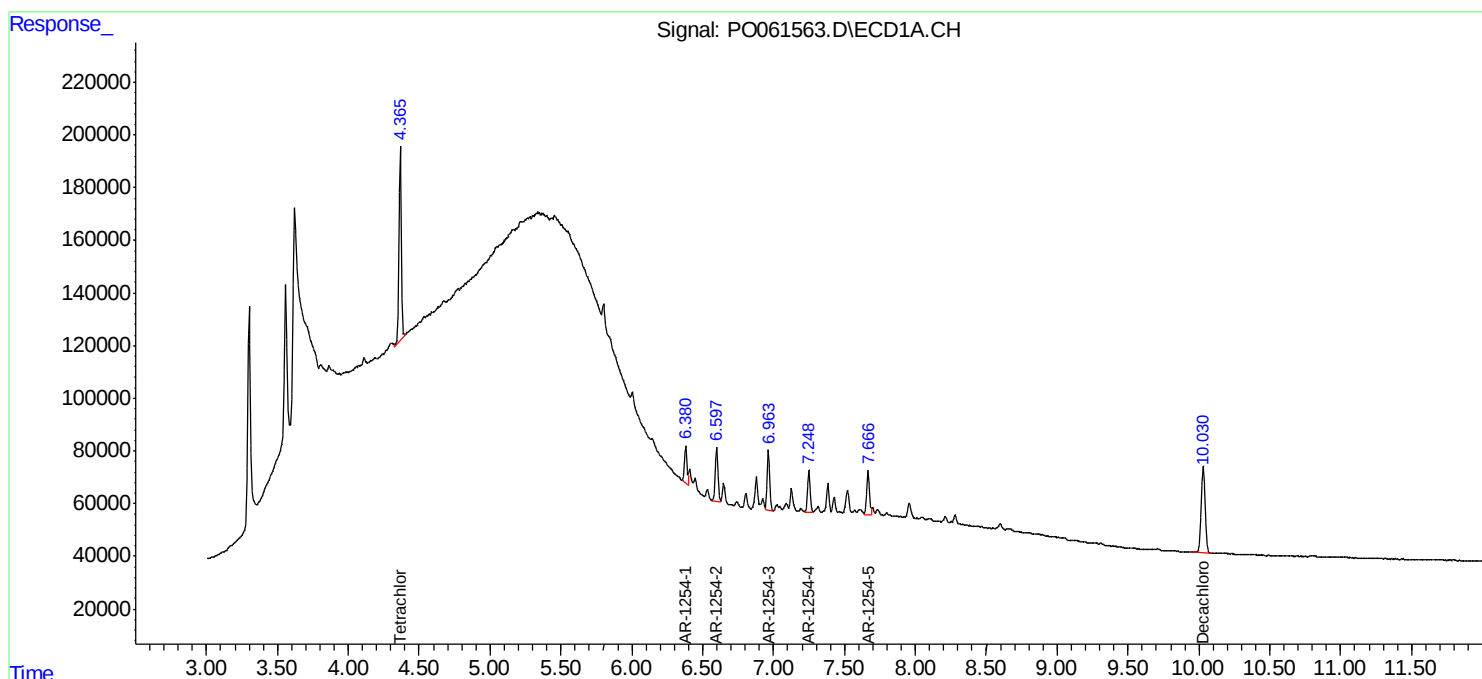

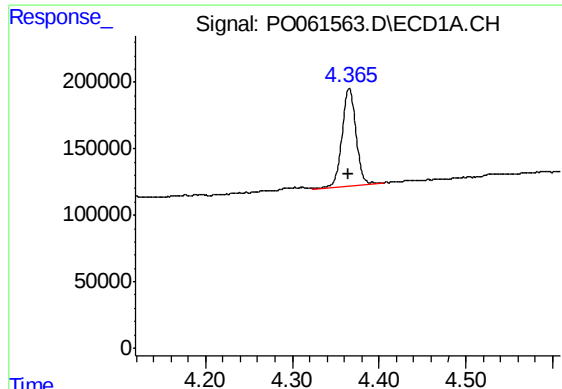


#1 Tetrachloro-m-xylene

R.T.: 4.366 min
Delta R.T.: 0.000 min
Response: 832700
Conc: 20.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
AOC14-02-B4-(24-30)


Manual Integrations
APPROVED

Ankita
10/2/2019 1:21:28 PM

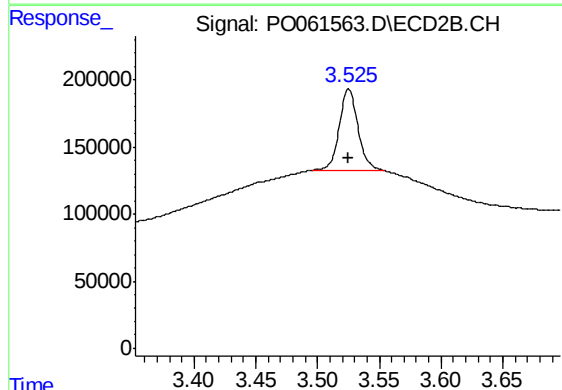


#1 Tetrachloro-m-xylene

R.T.: 3.525 min
Delta R.T.: 0.000 min
Response: 648127
Conc: 20.04 ng/ml m

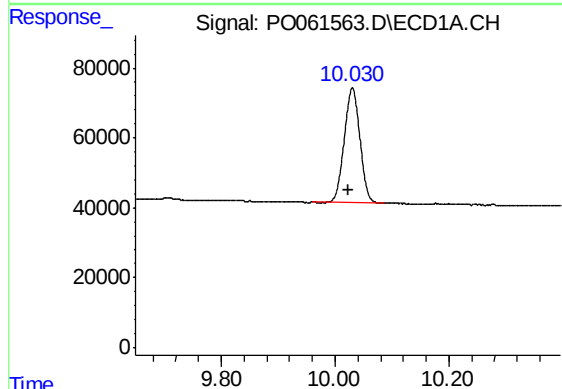


#2 Decachlorobiphenyl

R.T.: 10.031 min
Delta R.T.: 0.006 min
Response: 625503
Conc: 13.43 ng/ml

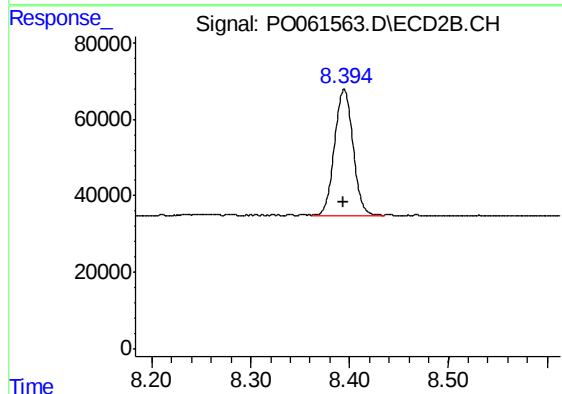

#2 Decachlorobiphenyl

R.T.: 8.395 min
Delta R.T.: 0.000 min
Response: 427189
Conc: 13.19 ng/ml

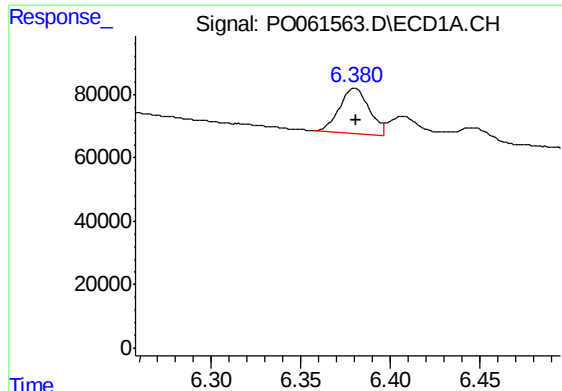


#26 AR-1254-1

R.T.: 6.380 min
Delta R.T.: -0.001 min
Response: 164403
Conc: 72.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
AOC14-02-B4-(24-30)


Manual Integrations
APPROVED

Ankita
10/2/2019 1:21:28 PM

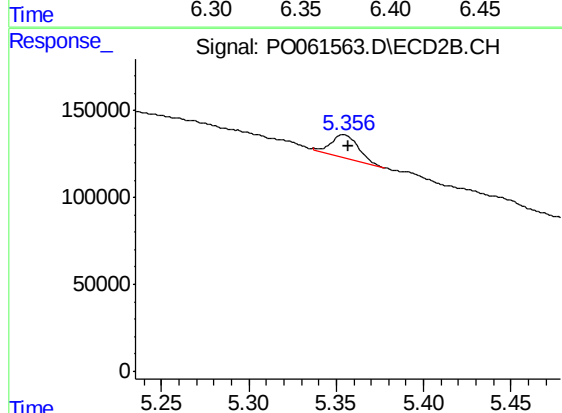


#26 AR-1254-1

R.T.: 5.356 min
Delta R.T.: 0.000 min
Response: 143238
Conc: 65.31 ng/ml m

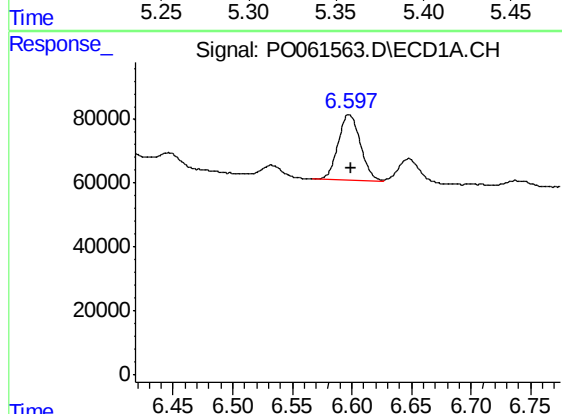


#27 AR-1254-2

R.T.: 6.598 min
Delta R.T.: -0.002 min
Response: 271073
Conc: 75.03 ng/ml

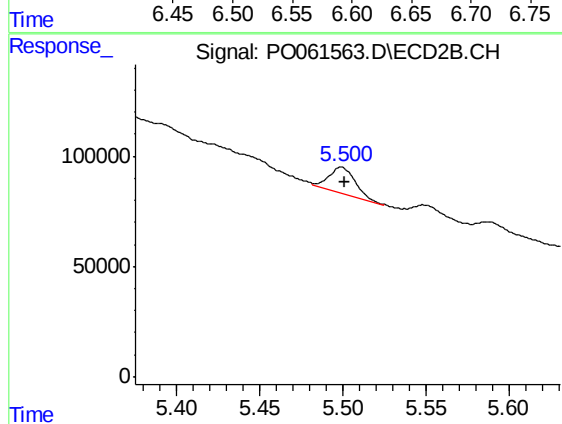

#27 AR-1254-2

R.T.: 5.500 min
Delta R.T.: -0.001 min
Response: 128863
Conc: 65.73 ng/ml m

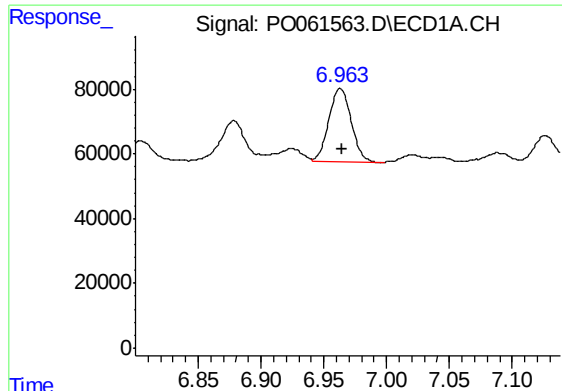


#28 AR-1254-3

R.T.: 6.963 min
Delta R.T.: -0.001 min
Response: 285643
Conc: 73.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
AOC14-02-B4-(24-30)


Manual Integrations
APPROVED

Ankita
10/2/2019 1:21:28 PM

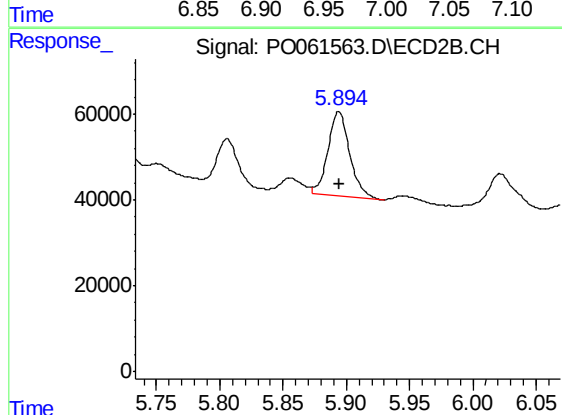


#28 AR-1254-3

R.T.: 5.894 min
Delta R.T.: -0.001 min
Response: 235243
Conc: 73.89 ng/ml

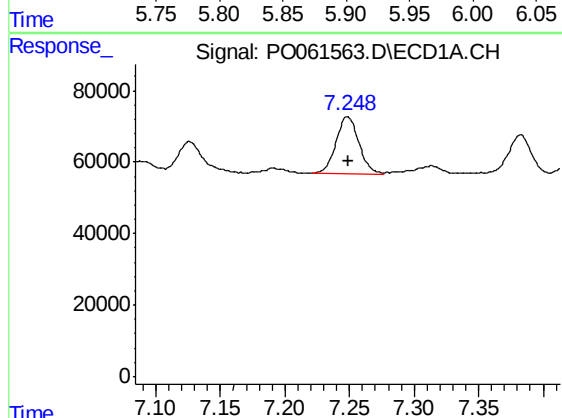


#29 AR-1254-4

R.T.: 7.249 min
Delta R.T.: -0.001 min
Response: 199406
Conc: 65.84 ng/ml

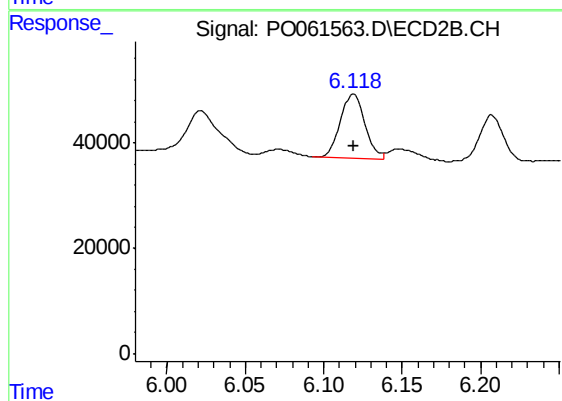

#29 AR-1254-4

R.T.: 6.119 min
Delta R.T.: 0.000 min
Response: 130498
Conc: 64.32 ng/ml

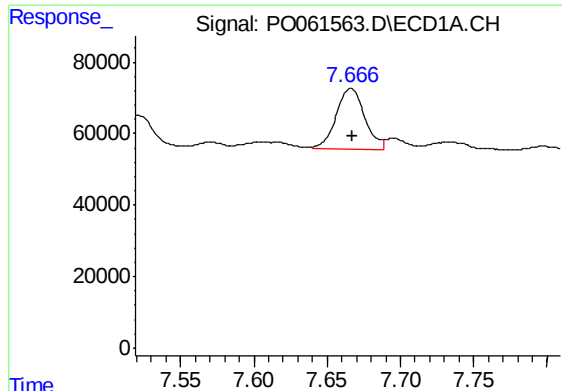


#30 AR-1254-5

R.T.: 7.666 min
Delta R.T.: 0.000 min
Response: 230499
Conc: 73.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
AOC14-02-B4-(24-30)

Manual Integrations
APPROVED

Ankita
10/2/2019 1:21:28 PM

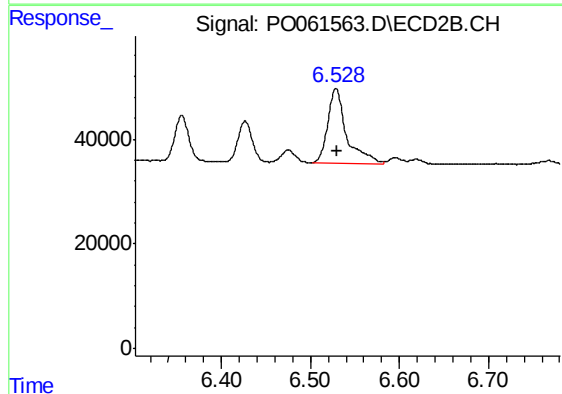

#30 AR-1254-5

R.T.: 6.529 min
Delta R.T.: -0.001 min
Response: 210848
Conc: 74.54 ng/ml