

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100219\
 Data File : P0061576.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Oct 2019 12:16
 Operator : HP/AJ
 Sample : IDOC-WATER-01
 Misc : HIRAL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IDOC-WATER-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 14:11:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	3.528	0	658588	N.D.	20.365 #
2)	SA Decachlor...	0.000	8.401	0	653302	N.D.	20.179 #
Target Compounds							
3)	L1 AR-1016-1	0.000	4.581	0	271845	N.D.	202.166 #
4)	L1 AR-1016-2	0.000	4.599	0	368322	N.D.	198.732 #
5)	L1 AR-1016-3	0.000	4.769	0	205601	N.D.	205.248 #
6)	L1 AR-1016-4	0.000	4.811	0	174517	N.D.	201.389 #
7)	L1 AR-1016-5	0.000	5.018	0	225166	N.D.	197.265 #
8)	L2 AR-1221-1	0.000	3.736	0	26170	N.D.	66.091 #
9)	L2 AR-1221-2	0.000	3.819	0	36946	N.D.	119.802 #
10)	L2 AR-1221-3	0.000	3.893	0	135668	N.D.	148.737 #
11)	L3 AR-1232-1	0.000	3.893	0	135668	N.D.	120.831 #
12)	L3 AR-1232-2	0.000	4.599	0	368322	N.D.	301.734 #
13)	L3 AR-1232-3	0.000	4.769	0	205601	N.D.	311.397 #
14)	L3 AR-1232-4	0.000	4.851	0	213612	N.D.	338.877 #
15)	L3 AR-1232-5	0.000	5.018	0	225166	N.D.	328.158 #
16)	L4 AR-1242-1	0.000	4.581	0	271845	N.D.	265.344 #
17)	L4 AR-1242-2	0.000	4.599	0	368322	N.D.	261.180 #
18)	L4 AR-1242-3	0.000	4.769	0	205601	N.D.	263.293 #
19)	L4 AR-1242-4	0.000	4.851	0	213612	N.D.	260.312 #
20)	L4 AR-1242-5	0.000	5.360	0	169500	N.D.	158.227 #
21)	L5 AR-1248-1	0.000	4.581	0	271845	N.D.	303.800 #
22)	L5 AR-1248-2	0.000	4.811	0	174517	N.D.	148.113 #
23)	L5 AR-1248-3	0.000	4.851	0	213612	N.D.	172.090 #
24)	L5 AR-1248-4	0.000	5.018	0	225166	N.D.	149.781 #
25)	L5 AR-1248-5	0.000	5.399	0	31515	N.D.	20.542 #
26)	L6 AR-1254-1	0.000	5.360	0	169500	N.D.	77.281 #
27)	L6 AR-1254-2	0.000	5.505	0	158058	N.D.	80.621 #
28)	L6 AR-1254-3	0.000	5.880	0	70716	N.D.	22.212 #
29)	L6 AR-1254-4	0.000	6.123	0	47223	N.D.	23.276 #
30)	L6 AR-1254-5	0.000	6.534	0	503437	N.D.	177.989 #
31)	L7 AR-1260-1	0.000	6.027	0	403659	N.D.	197.892 #
32)	L7 AR-1260-2	0.000	6.212	0	473725	N.D.	197.243 #
33)	L7 AR-1260-3	0.000	6.362	0	442634	N.D.	196.454 #
34)	L7 AR-1260-4	0.000	6.826	0	346934	N.D.	187.917 #
35)	L7 AR-1260-5	0.000	7.066	0	722810	N.D.	185.639 #
36)	L8 AR-1262-1	0.000	6.624	0	193556	N.D.	158.569 #
37)	L8 AR-1262-2	0.000	7.066	0	722810	N.D.	157.200 #
38)	L8 AR-1262-3	0.000	7.345	0	172925	N.D.	91.795 #
39)	L8 AR-1262-4	0.000	7.407	0	531855	N.D.	158.255 #
40)	L8 AR-1262-5	0.000	7.897	0	203852	N.D.	134.470 #
41)	L9 AR-1268-1	0.000	7.345	0	172925	N.D.	35.809 #
42)	L9 AR-1268-2	0.000	7.407	0	531855	N.D.	123.405 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100219\
 Data File : P0061576.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Oct 2019 12:16
 Operator : HP/AJ
 Sample : IDOC-WATER-01
 Misc : HIRAL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IDOC-WATER-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 14:11:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	0.000	7.612	0	16697	N.D.	4.658 #
44) L9	AR-1268-4	0.000	7.897	0	203852	N.D.	126.664 #
45) L9	AR-1268-5	0.000	8.167	0	61035	N.D.	6.070 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100219\
Data File : PO061576.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Oct 2019 12:16
Operator : HP/AJ
Sample : IDOC-WATER-01
Misc : HIRAL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 14:11:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

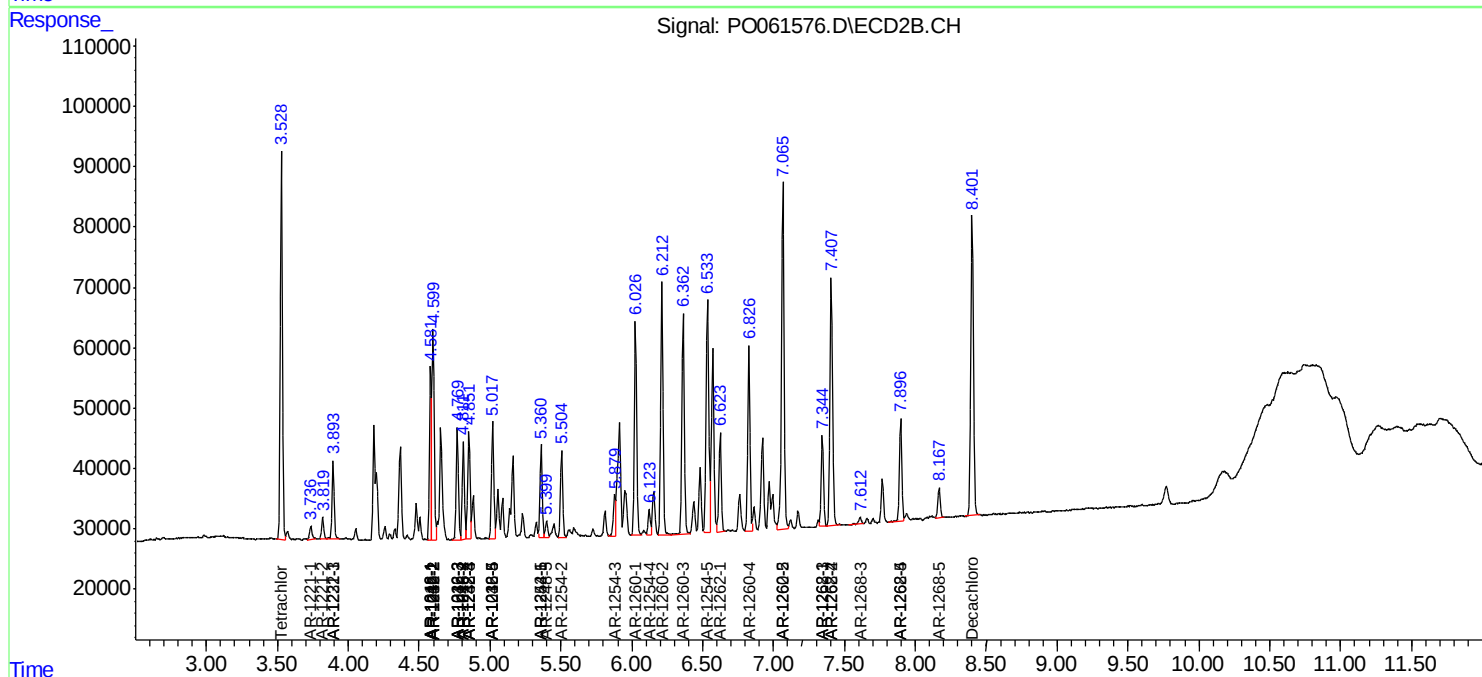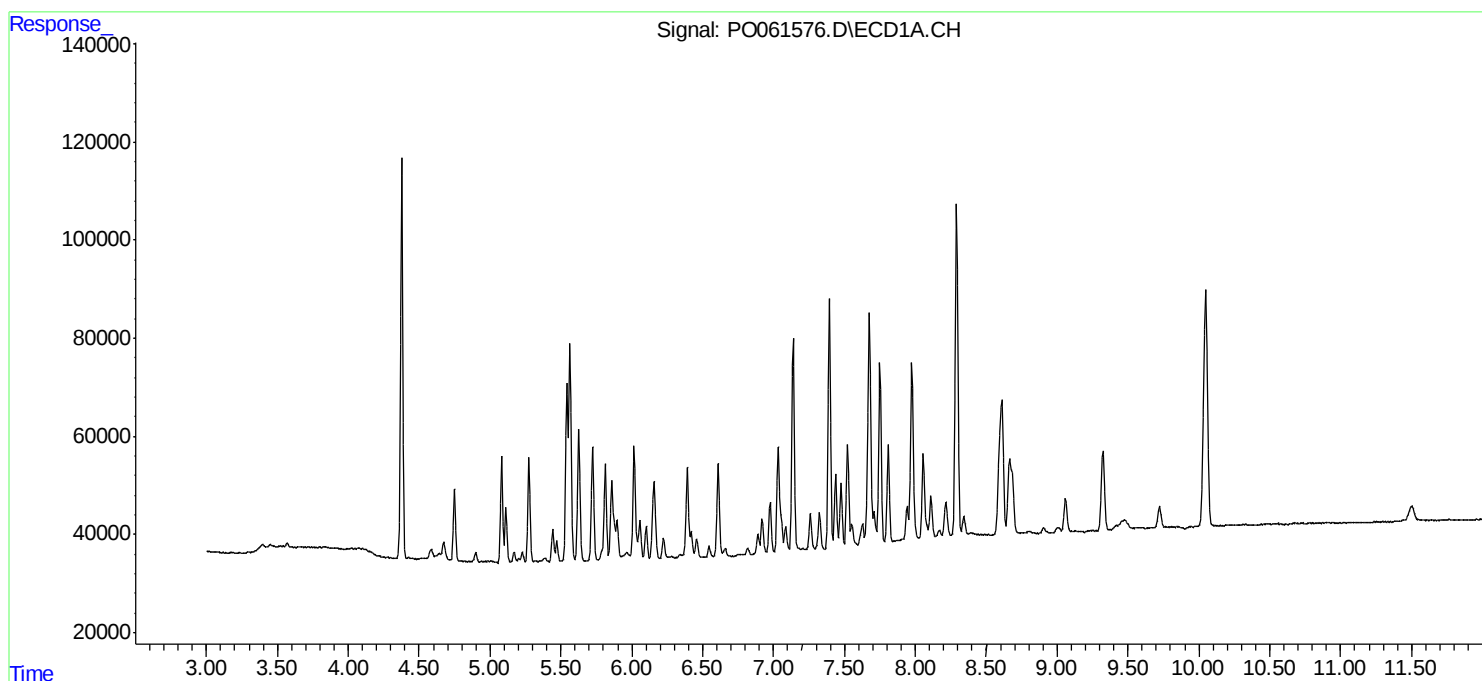


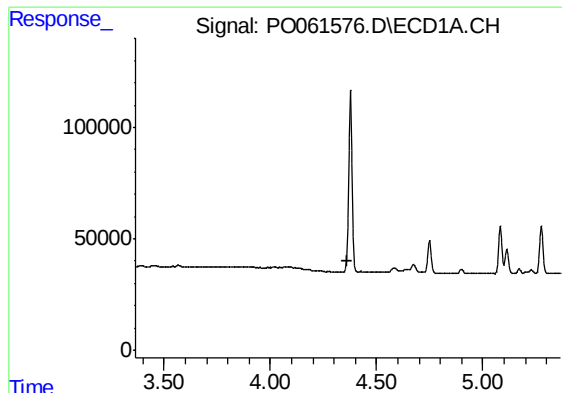

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.365 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01

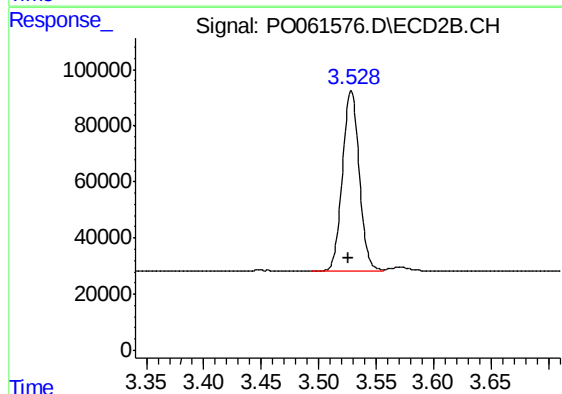


#1 Tetrachloro-m-xylene

R.T.: 3.528 min
Delta R.T.: 0.003 min
Response: 658588
Conc: 20.36 ng/ml

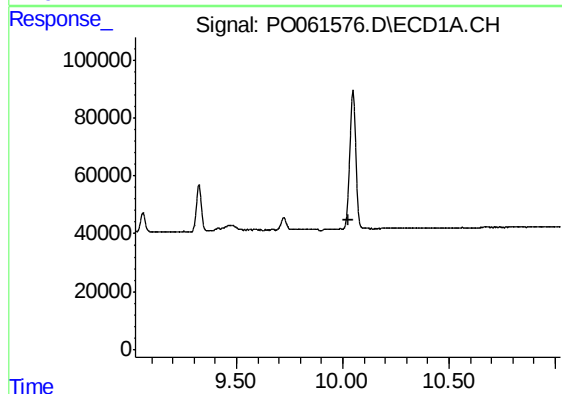


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.025 min
Response: 0
Conc: N.D.

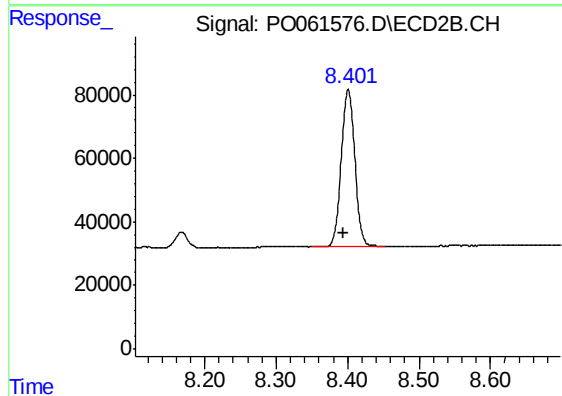

#2 Decachlorobiphenyl


R.T.: 8.401 min
Delta R.T.: 0.007 min
Response: 653302
Conc: 20.18 ng/ml

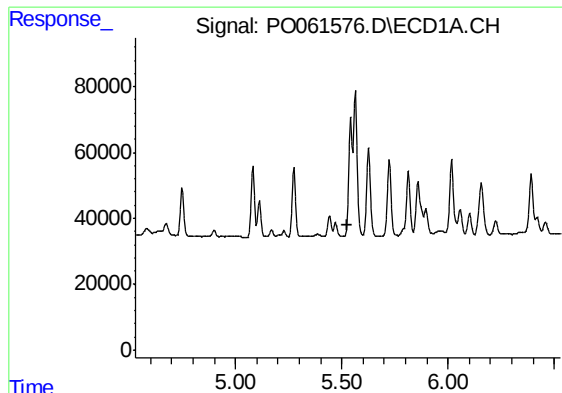

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.529 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01

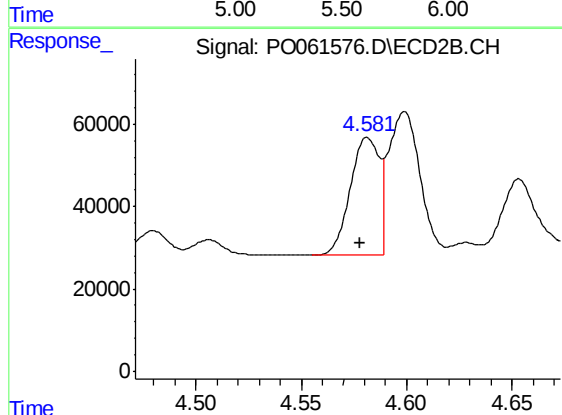


#3 AR-1016-1

R.T.: 4.581 min
Delta R.T.: 0.004 min
Response: 271845
Conc: 202.17 ng/ml

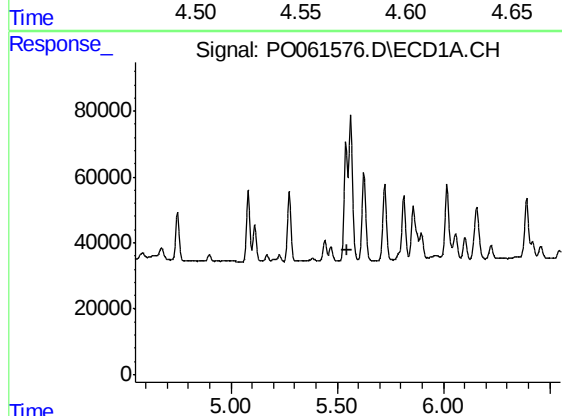


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.551 min
Response: 0
Conc: N.D.

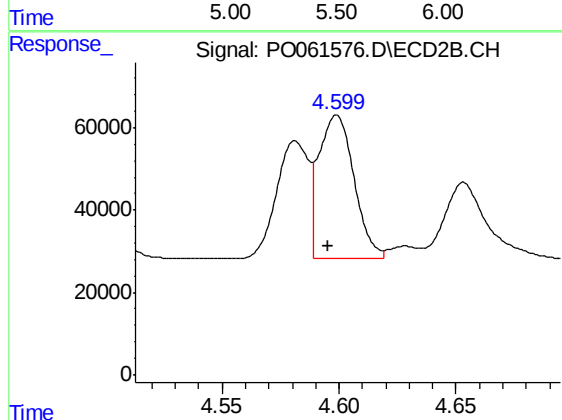

#4 AR-1016-2


R.T.: 4.599 min
Delta R.T.: 0.004 min
Response: 368322
Conc: 198.73 ng/ml

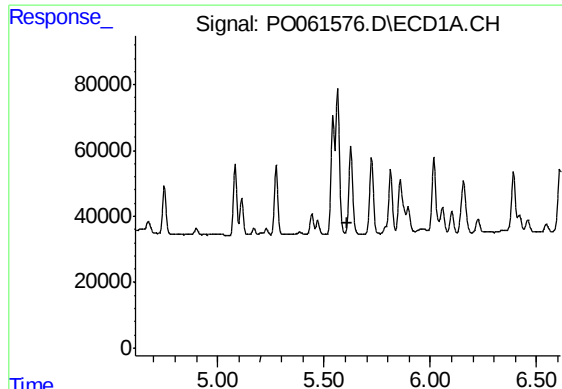

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T. : 5.612 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01




#5 AR-1016-3

R.T.: 4.769 min
Delta R.T.: 0.004 min
Response: 205601
Conc: 205.25 ng/ml




#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 5.711 min
Response: 0
Conc: N.D.

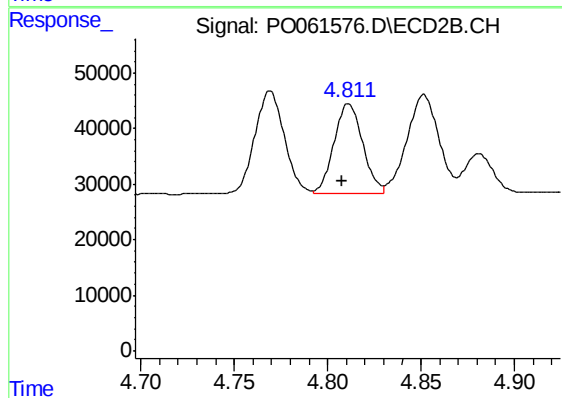

#6 AR-1016-4


R.T.: 4.811 min
Delta R.T.: 0.004 min
Response: 174517
Conc: 201.39 ng/ml



#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 6.003 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01

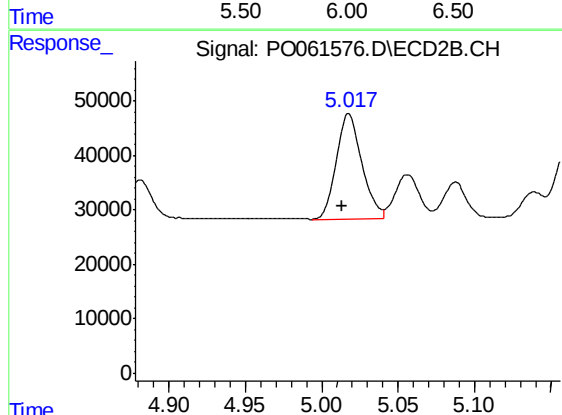


#7 AR-1016-5

R.T.: 5.018 min
Delta R.T.: 0.004 min
Response: 225166
Conc: 197.27 ng/ml

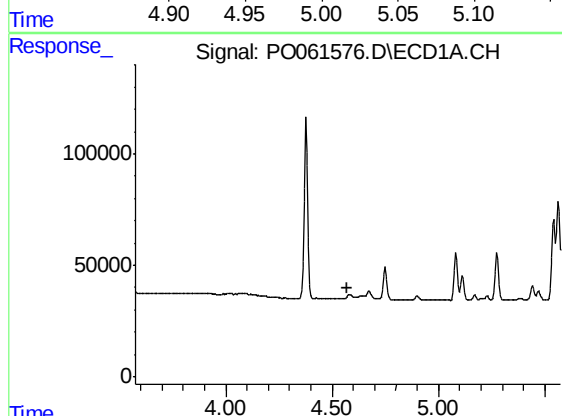


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.574 min
Response: 0
Conc: N.D.

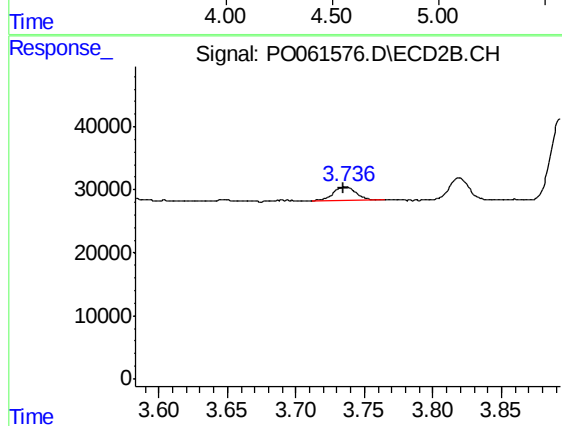

#8 AR-1221-1


R.T.: 3.736 min
Delta R.T.: 0.002 min
Response: 26170
Conc: 66.09 ng/ml

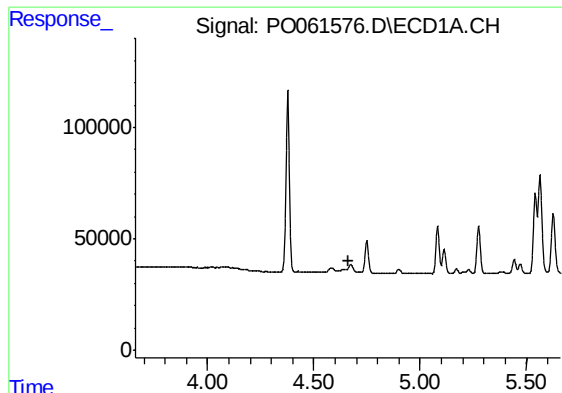

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.660 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01

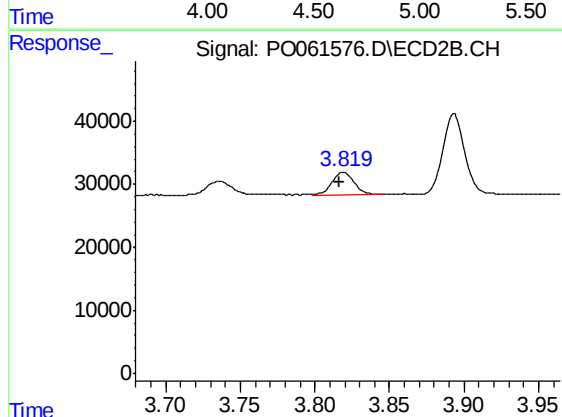


#9 AR-1221-2

R.T.: 3.819 min
Delta R.T.: 0.003 min
Response: 36946
Conc: 119.80 ng/ml

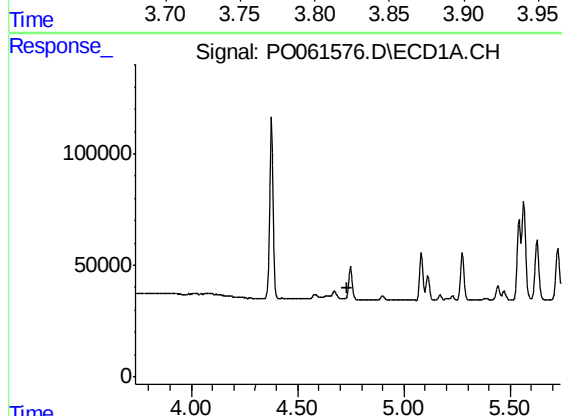


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.736 min
Response: 0
Conc: N.D.

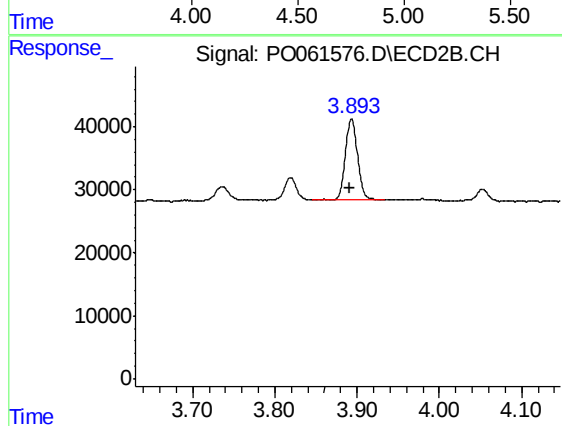

#10 AR-1221-3


R.T.: 3.893 min
Delta R.T.: 0.003 min
Response: 135668
Conc: 148.74 ng/ml



#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.735 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01




#11 AR-1232-1

R.T.: 3.893 min
Delta R.T.: 0.003 min
Response: 135668
Conc: 120.83 ng/ml




#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.261 min
Response: 0
Conc: N.D.

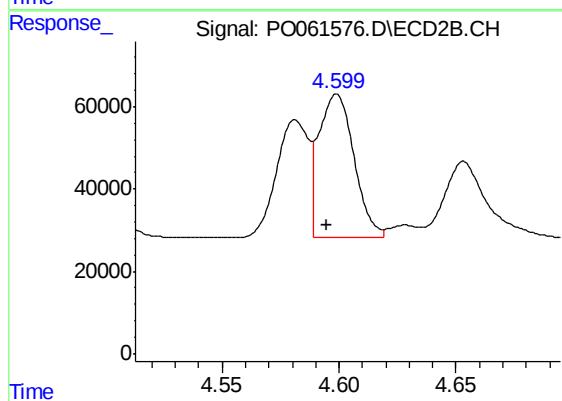

#12 AR-1232-2


R.T.: 4.599 min
Delta R.T.: 0.004 min
Response: 368322
Conc: 301.73 ng/ml



#13 AR-1232-3


R.T.: 0.000 min
Exp R.T. : 5.550 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01




#13 AR-1232-3

R.T.: 4.769 min
Delta R.T.: 0.004 min
Response: 205601
Conc: 311.40 ng/ml




#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 5.710 min
Response: 0
Conc: N.D.

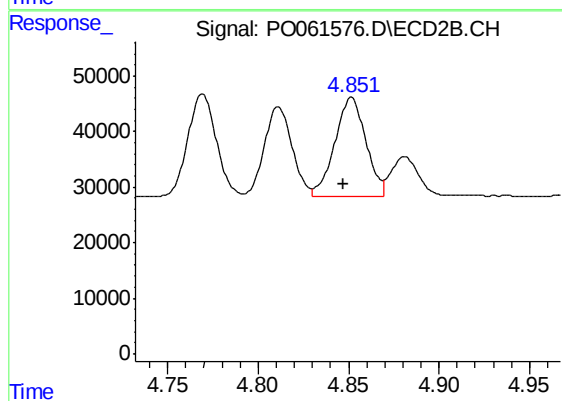

#14 AR-1232-4


R.T.: 4.851 min
Delta R.T.: 0.004 min
Response: 213612
Conc: 338.88 ng/ml



#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.799 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01




#15 AR-1232-5

R.T.: 5.018 min
Delta R.T.: 0.005 min
Response: 225166
Conc: 328.16 ng/ml




#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 5.528 min
Response: 0
Conc: N.D.

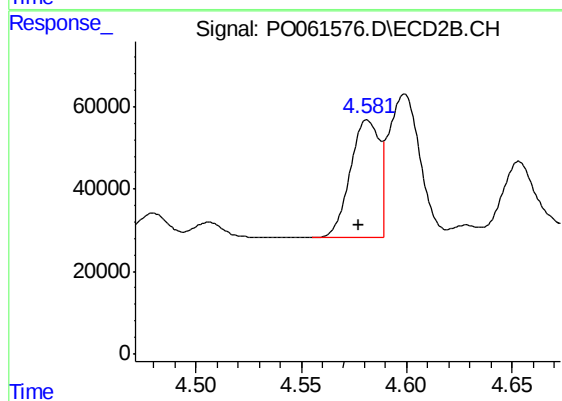

#16 AR-1242-1


R.T.: 4.581 min
Delta R.T.: 0.004 min
Response: 271845
Conc: 265.34 ng/ml



#17 AR-1242-2


R.T.: 0.000 min
Exp R.T. : 5.550 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01

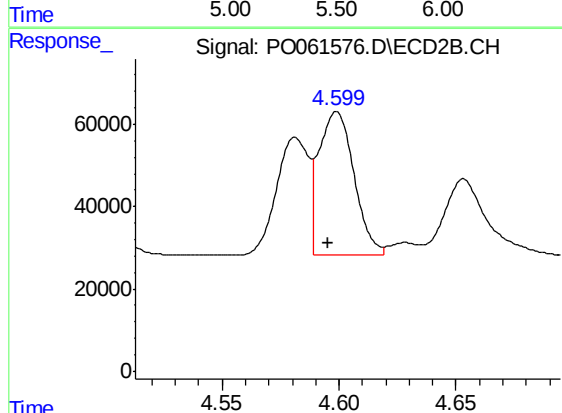


#17 AR-1242-2

R.T.: 4.599 min
Delta R.T.: 0.004 min
Response: 368322
Conc: 261.18 ng/ml

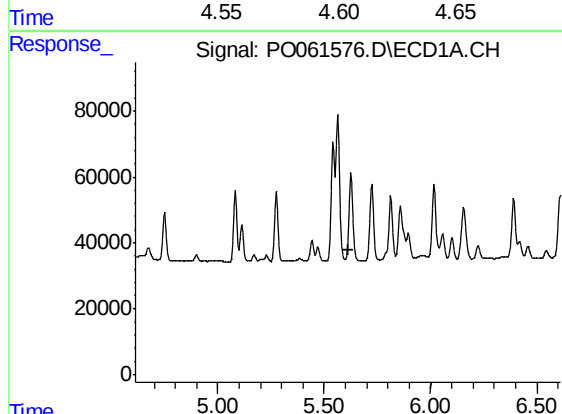


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T. : 5.612 min
Response: 0
Conc: N.D.

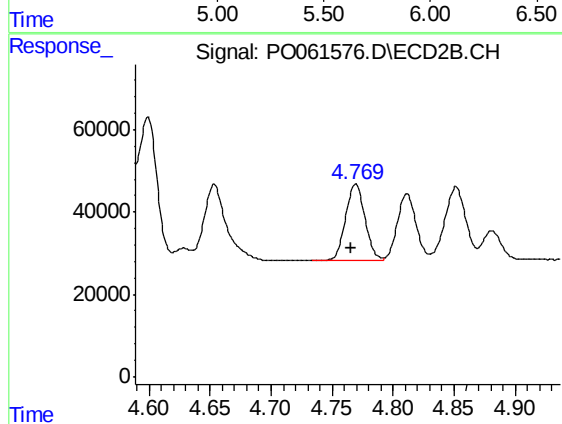

#18 AR-1242-3


R.T.: 4.769 min
Delta R.T.: 0.004 min
Response: 205601
Conc: 263.29 ng/ml

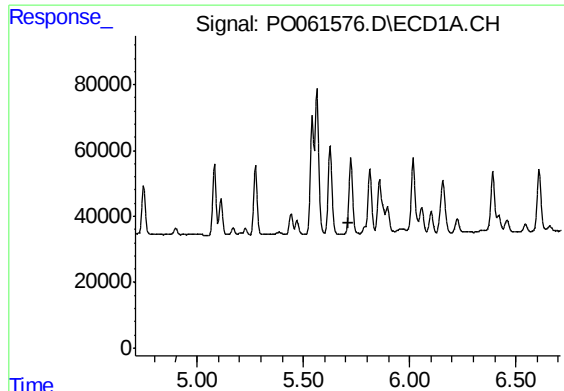

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T. : 5.710 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01

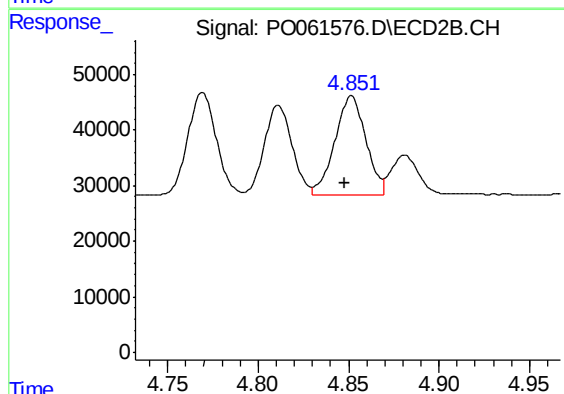


#19 AR-1242-4

R.T.: 4.851 min
Delta R.T.: 0.004 min
Response: 213612
Conc: 260.31 ng/ml

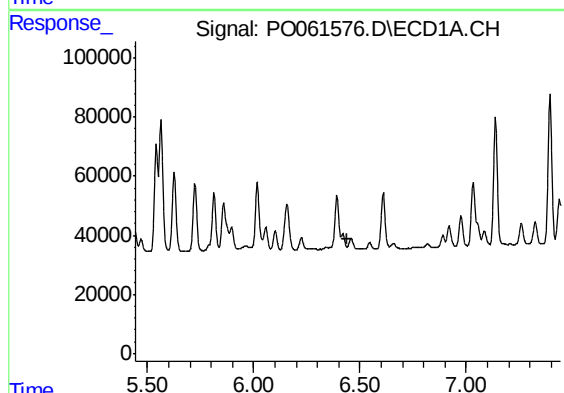


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

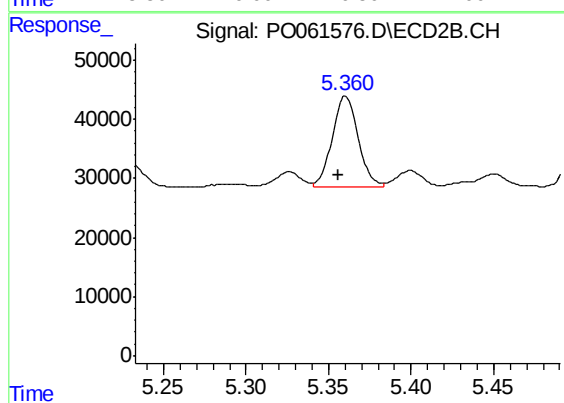

#20 AR-1242-5


R.T.: 5.360 min
Delta R.T.: 0.005 min
Response: 169500
Conc: 158.23 ng/ml



#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.528 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01

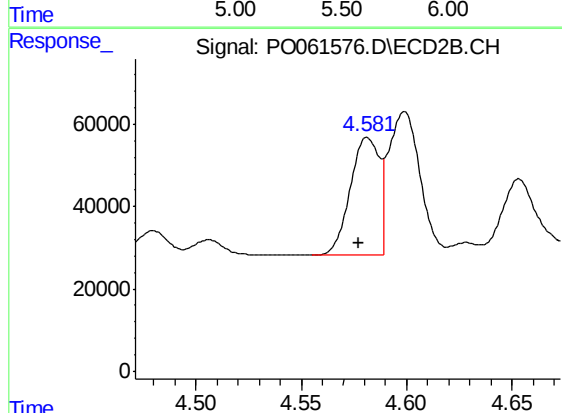


#21 AR-1248-1

R.T.: 4.581 min
Delta R.T.: 0.004 min
Response: 271845
Conc: 303.80 ng/ml

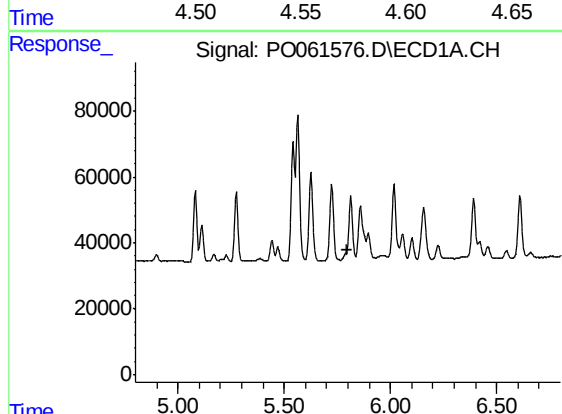


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 5.800 min
Response: 0
Conc: N.D.

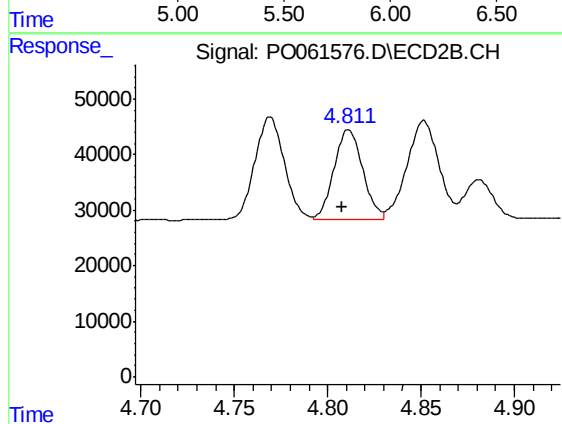

#22 AR-1248-2


R.T.: 4.811 min
Delta R.T.: 0.004 min
Response: 174517
Conc: 148.11 ng/ml

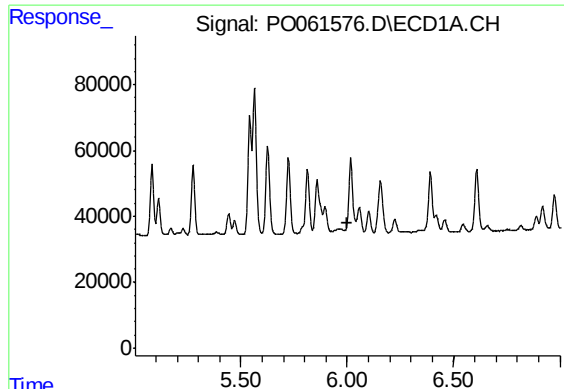

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 6.003 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01

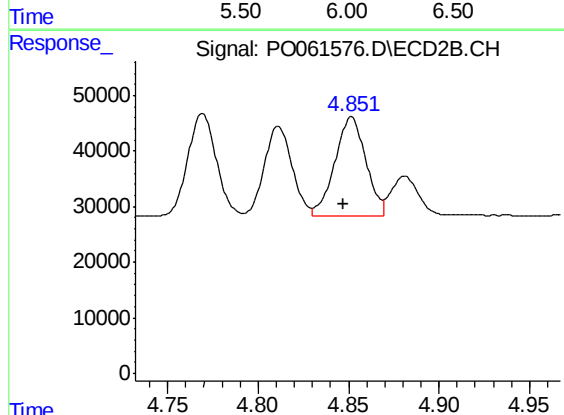


#23 AR-1248-3

R.T.: 4.851 min
Delta R.T.: 0.004 min
Response: 213612
Conc: 172.09 ng/ml

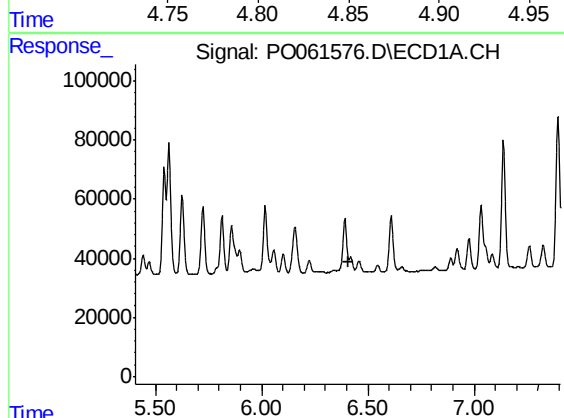


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 6.406 min
Response: 0
Conc: N.D.

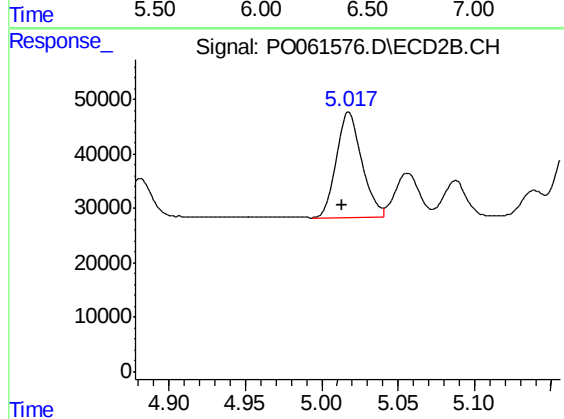

#24 AR-1248-4


R.T.: 5.018 min
Delta R.T.: 0.005 min
Response: 225166
Conc: 149.78 ng/ml



#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.444 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01

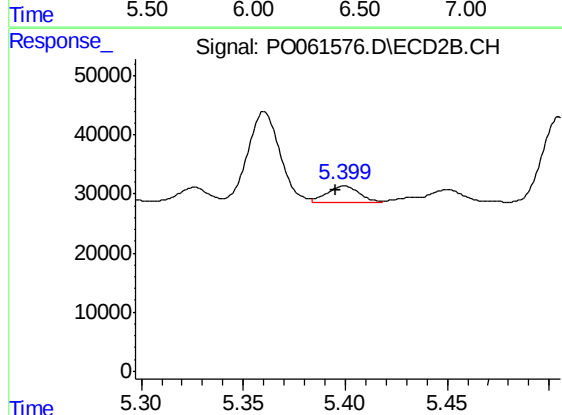


#25 AR-1248-5

R.T.: 5.399 min
Delta R.T.: 0.004 min
Response: 31515
Conc: 20.54 ng/ml

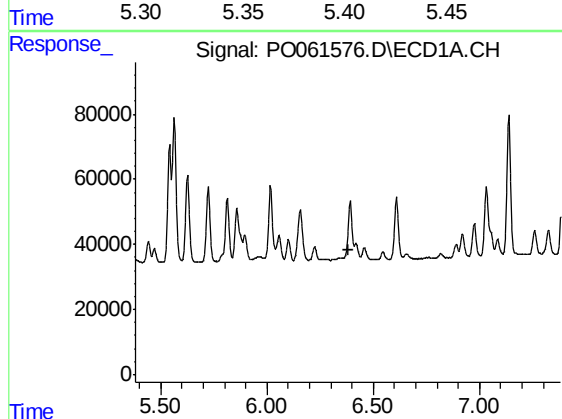


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.381 min
Response: 0
Conc: N.D.

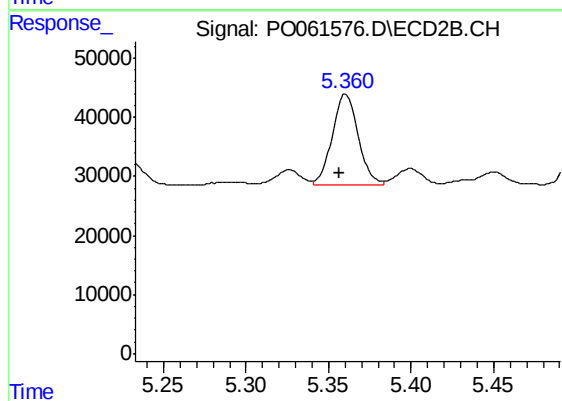

#26 AR-1254-1


R.T.: 5.360 min
Delta R.T.: 0.003 min
Response: 169500
Conc: 77.28 ng/ml

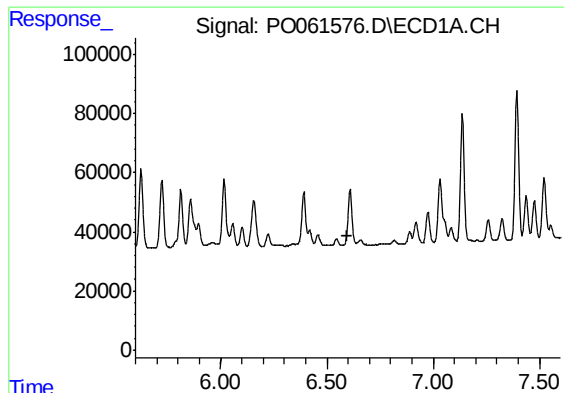

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 6.599 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01

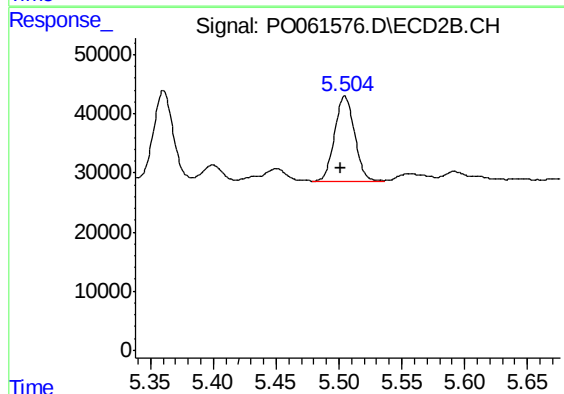


#27 AR-1254-2

R.T.: 5.505 min
Delta R.T.: 0.004 min
Response: 158058
Conc: 80.62 ng/ml

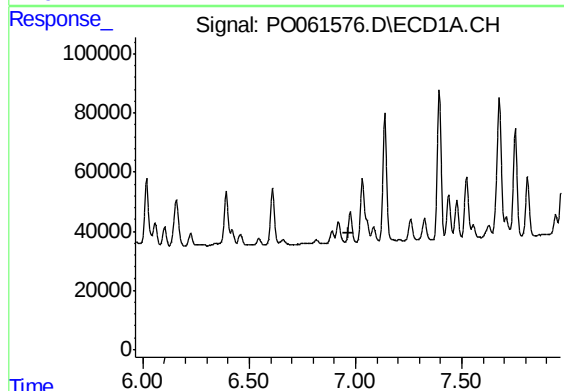


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.964 min
Response: 0
Conc: N.D.

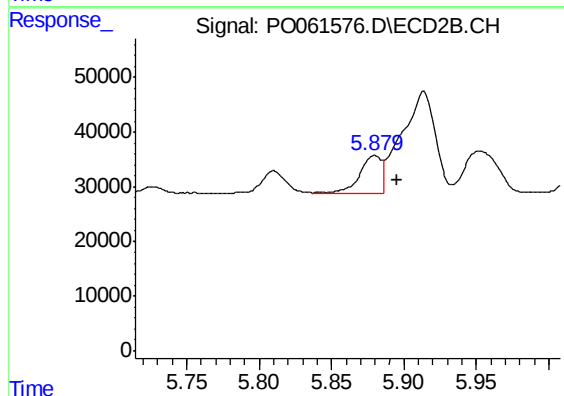

#28 AR-1254-3


R.T.: 5.880 min
Delta R.T.: -0.015 min
Response: 70716
Conc: 22.21 ng/ml

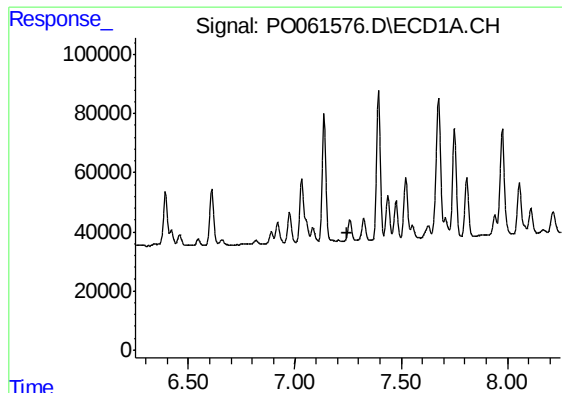

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.250 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01

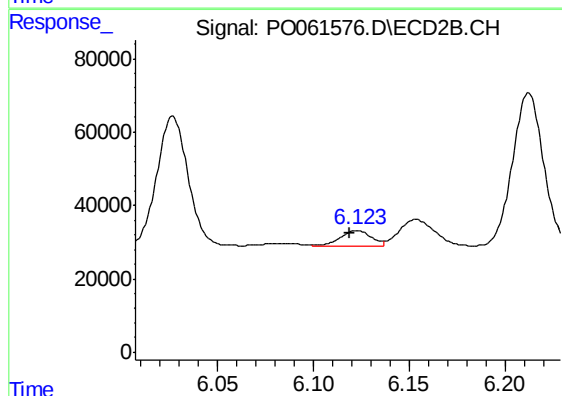


#29 AR-1254-4

R.T.: 6.123 min
Delta R.T.: 0.004 min
Response: 47223
Conc: 23.28 ng/ml

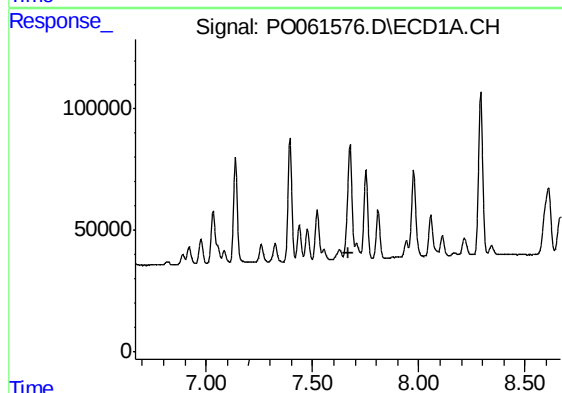


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 7.667 min
Response: 0
Conc: N.D.

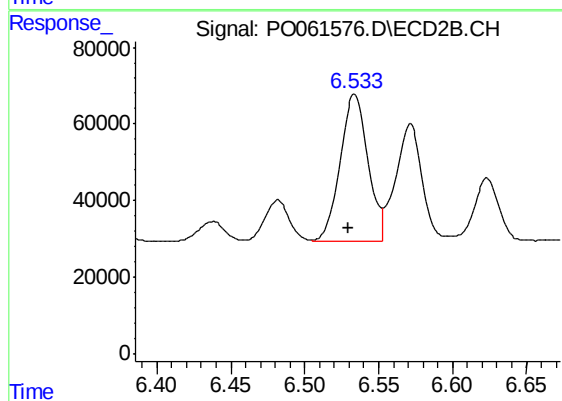

#30 AR-1254-5


R.T.: 6.534 min
Delta R.T.: 0.004 min
Response: 503437
Conc: 177.99 ng/ml



#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01




#31 AR-1260-1

R.T.: 6.027 min
Delta R.T.: 0.005 min
Response: 403659
Conc: 197.89 ng/ml




#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.381 min
Response: 0
Conc: N.D.

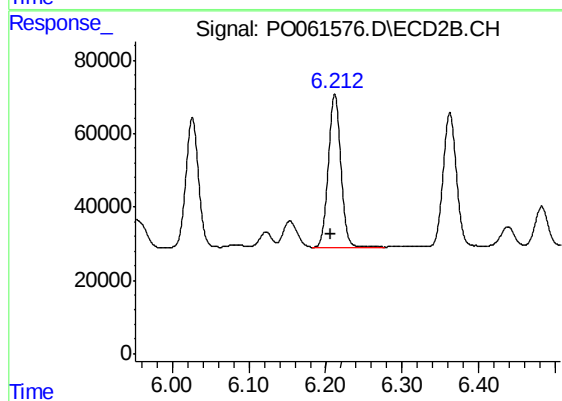

#32 AR-1260-2


R.T.: 6.212 min
Delta R.T.: 0.005 min
Response: 473725
Conc: 197.24 ng/ml

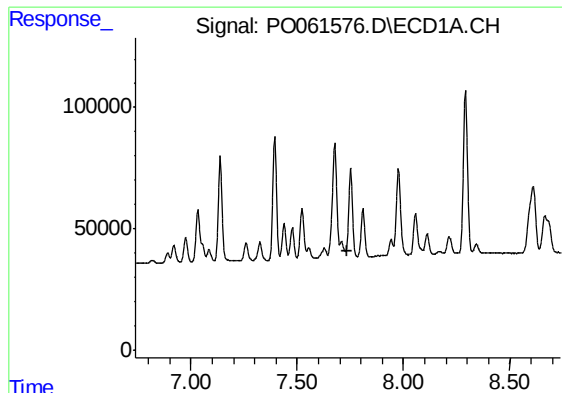

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.738 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01

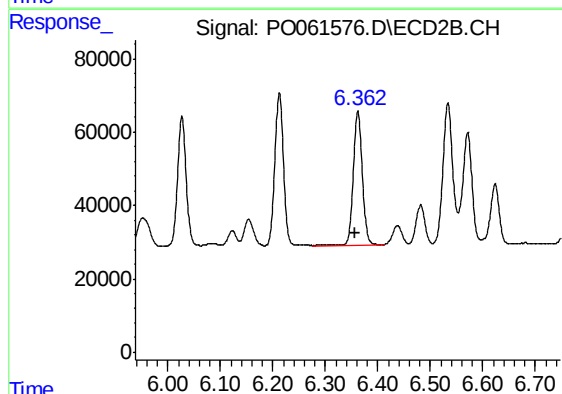


#33 AR-1260-3

R.T.: 6.362 min
Delta R.T.: 0.006 min
Response: 442634
Conc: 196.45 ng/ml

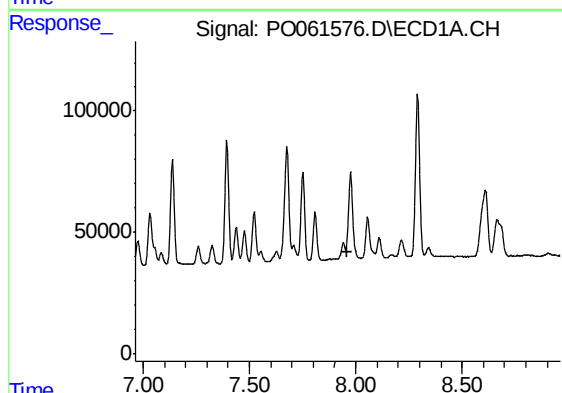


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.963 min
Response: 0
Conc: N.D.

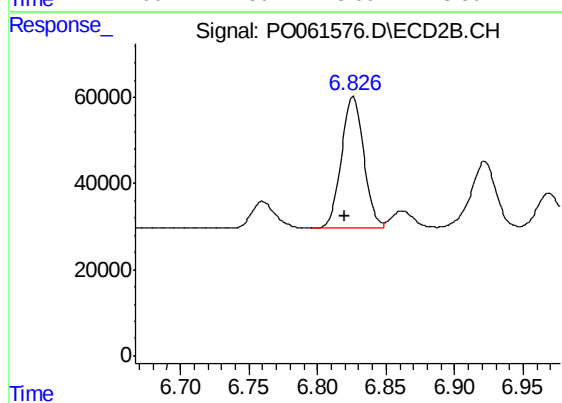

#34 AR-1260-4


R.T.: 6.826 min
Delta R.T.: 0.006 min
Response: 346934
Conc: 187.92 ng/ml



#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.277 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01




#35 AR-1260-5

R.T.: 7.066 min
Delta R.T.: 0.006 min
Response: 722810
Conc: 185.64 ng/ml




#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.740 min
Response: 0
Conc: N.D.

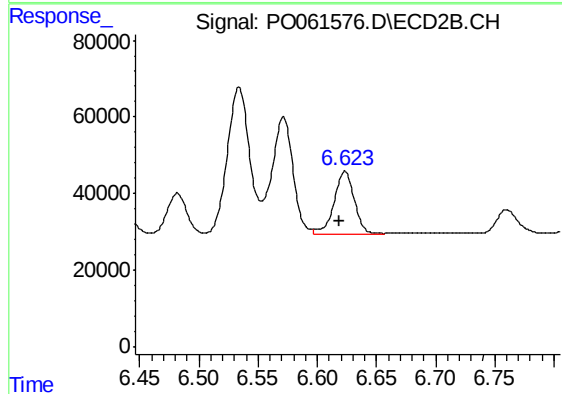

#36 AR-1262-1


R.T.: 6.624 min
Delta R.T.: 0.004 min
Response: 193556
Conc: 158.57 ng/ml



#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 8.279 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01




#37 AR-1262-2

R.T.: 7.066 min
Delta R.T.: 0.005 min
Response: 722810
Conc: 157.20 ng/ml




#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.581 min
Response: 0
Conc: N.D.

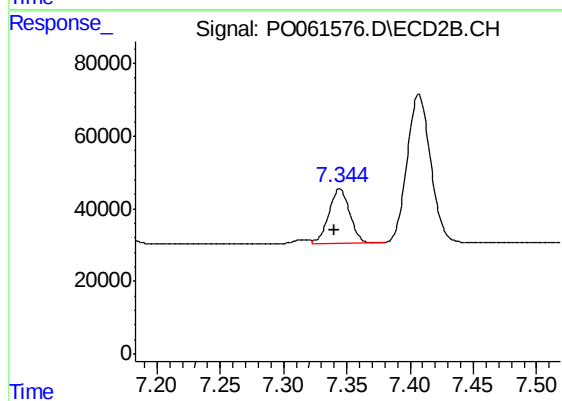

#38 AR-1262-3


R.T.: 7.345 min
Delta R.T.: 0.005 min
Response: 172925
Conc: 91.79 ng/ml



#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.669 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01




#39 AR-1262-4

R.T.: 7.407 min
Delta R.T.: 0.004 min
Response: 531855
Conc: 158.26 ng/ml




#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.307 min
Response: 0
Conc: N.D.

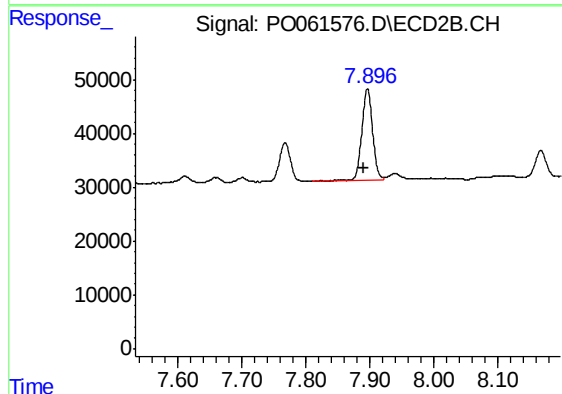

#40 AR-1262-5


R.T.: 7.897 min
Delta R.T.: 0.005 min
Response: 203852
Conc: 134.47 ng/ml



#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 8.581 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01

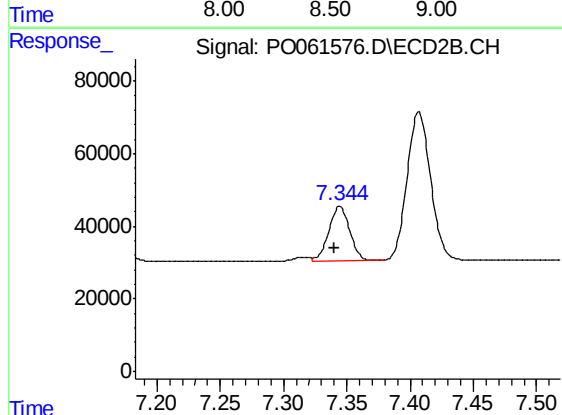


#41 AR-1268-1

R.T.: 7.345 min
Delta R.T.: 0.004 min
Response: 172925
Conc: 35.81 ng/ml

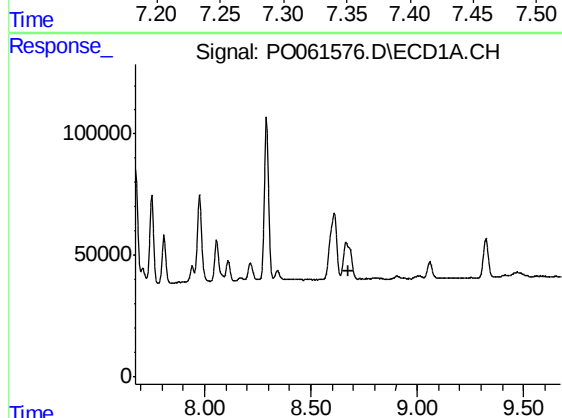


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.674 min
Response: 0
Conc: N.D.

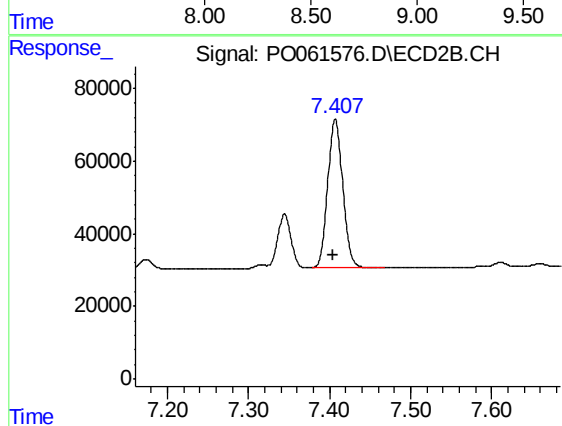

#42 AR-1268-2


R.T.: 7.407 min
Delta R.T.: 0.003 min
Response: 531855
Conc: 123.41 ng/ml



#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 8.894 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01




#43 AR-1268-3

R.T.: 7.612 min
Delta R.T.: 0.004 min
Response: 16697
Conc: 4.66 ng/ml




#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.309 min
Response: 0
Conc: N.D.

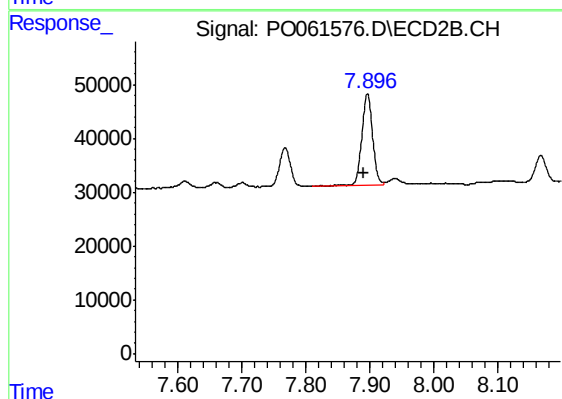

#44 AR-1268-4


R.T.: 7.897 min
Delta R.T.: 0.005 min
Response: 203852
Conc: 126.66 ng/ml

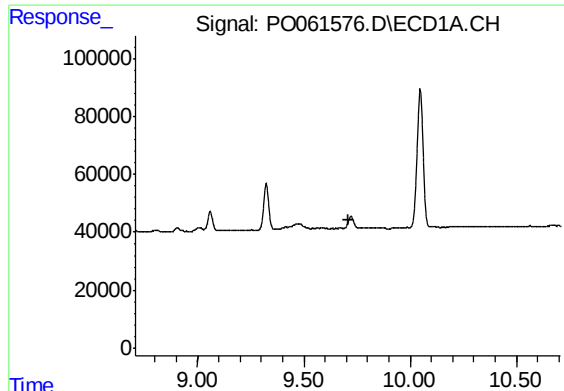

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.708 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-01

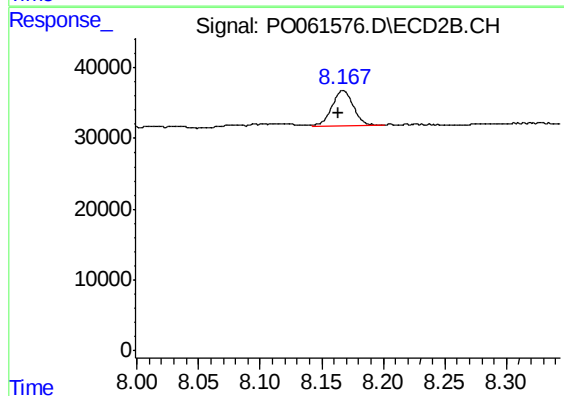

#45 AR-1268-5

R.T.: 8.167 min
Delta R.T.: 0.004 min
Response: 61035
Conc: 6.07 ng/ml