

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100219\
 Data File : P0061577.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Oct 2019 12:32
 Operator : HP/AJ
 Sample : IDOC-WATER-02
 Misc : HIRAL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IDOC-WATER-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 14:12:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	3.527	0	661011	N.D.	20.440 #
2)	SA Decachlor...	0.000	8.397	0	631781	N.D.	19.514 #
Target Compounds							
3)	L1 AR-1016-1	0.000	4.579	0	273230	N.D.	203.196 #
4)	L1 AR-1016-2	0.000	4.597	0	374703	N.D.	202.175 #
5)	L1 AR-1016-3	0.000	4.767	0	198845	N.D.	198.503 #
6)	L1 AR-1016-4	0.000	4.809	0	178304	N.D.	205.759 #
7)	L1 AR-1016-5	0.000	5.015	0	237061	N.D.	207.687 #
8)	L2 AR-1221-1	0.000	3.733	0	25278	N.D.	63.838 #
9)	L2 AR-1221-2	0.000	3.817	0	37135	N.D.	120.415 #
10)	L2 AR-1221-3	0.000	3.891	0	132795	N.D.	145.586 #
11)	L3 AR-1232-1	0.000	3.891	0	132795	N.D.	118.272 #
12)	L3 AR-1232-2	0.000	4.597	0	374703	N.D.	306.961 #
13)	L3 AR-1232-3	0.000	4.767	0	198845	N.D.	301.164 #
14)	L3 AR-1232-4	0.000	4.849	0	216434	N.D.	343.353 #
15)	L3 AR-1232-5	0.000	5.015	0	237061	N.D.	345.495 #
16)	L4 AR-1242-1	0.000	4.579	0	273230	N.D.	266.695 #
17)	L4 AR-1242-2	0.000	4.597	0	374703	N.D.	265.705 #
18)	L4 AR-1242-3	0.000	4.767	0	198845	N.D.	254.641 #
19)	L4 AR-1242-4	0.000	4.849	0	216434	N.D.	263.751 #
20)	L4 AR-1242-5	0.000	5.357	0	183427	N.D.	171.228 #
21)	L5 AR-1248-1	0.000	4.579	0	273230	N.D.	305.348 #
22)	L5 AR-1248-2	0.000	4.809	0	178304	N.D.	151.327 #
23)	L5 AR-1248-3	0.000	4.849	0	216434	N.D.	174.363 #
24)	L5 AR-1248-4	0.000	5.015	0	237061	N.D.	157.694 #
25)	L5 AR-1248-5	0.000	5.396	0	48893	N.D.	31.869 #
26)	L6 AR-1254-1	0.000	5.357	0	183427	N.D.	83.631 #
27)	L6 AR-1254-2	0.000	5.502	0	167541	N.D.	85.458 #
28)	L6 AR-1254-3	0.000	5.910	0	324539	N.D.	101.936 #
29)	L6 AR-1254-4	0.000	6.120	0	70185	N.D.	34.594 #
30)	L6 AR-1254-5	0.000	6.530	0	573897	N.D.	202.901 #
31)	L7 AR-1260-1	0.000	6.024	0	453082	N.D.	222.121 #
32)	L7 AR-1260-2	0.000	6.209	0	546960	N.D.	227.735 #
33)	L7 AR-1260-3	0.000	6.359	0	547778	N.D.	243.121 #
34)	L7 AR-1260-4	0.000	6.822	0	434417	N.D.	235.302 #
35)	L7 AR-1260-5	0.000	7.062	0	971257	N.D.	249.448 #
36)	L8 AR-1262-1	0.000	6.620	0	204471	N.D.	167.512 #
37)	L8 AR-1262-2	0.000	7.062	0	971257	N.D.	211.233 #
38)	L8 AR-1262-3	0.000	7.340	0	243508	N.D.	129.263 #
39)	L8 AR-1262-4	0.000	7.403	0	655919	N.D.	195.171 #
40)	L8 AR-1262-5	0.000	7.892	0	215863	N.D.	142.393 #
41)	L9 AR-1268-1	0.000	7.340	0	243508	N.D.	50.425 #
42)	L9 AR-1268-2	0.000	7.403	0	655919	N.D.	152.191 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100219\
 Data File : P0061577.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Oct 2019 12:32
 Operator : HP/AJ
 Sample : IDOC-WATER-02
 Misc : HIRAL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IDOC-WATER-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 14:12:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	0.000	7.609	0	97312	N.D.	27.150 #
44) L9	AR-1268-4	0.000	7.892	0	215863	N.D.	134.127 #
45) L9	AR-1268-5	0.000	8.164	0	79183	N.D.	7.874 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100219\
Data File : PO061577.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Oct 2019 12:32
Operator : HP/AJ
Sample : IDOC-WATER-02
Misc : HIRAL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 14:12:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

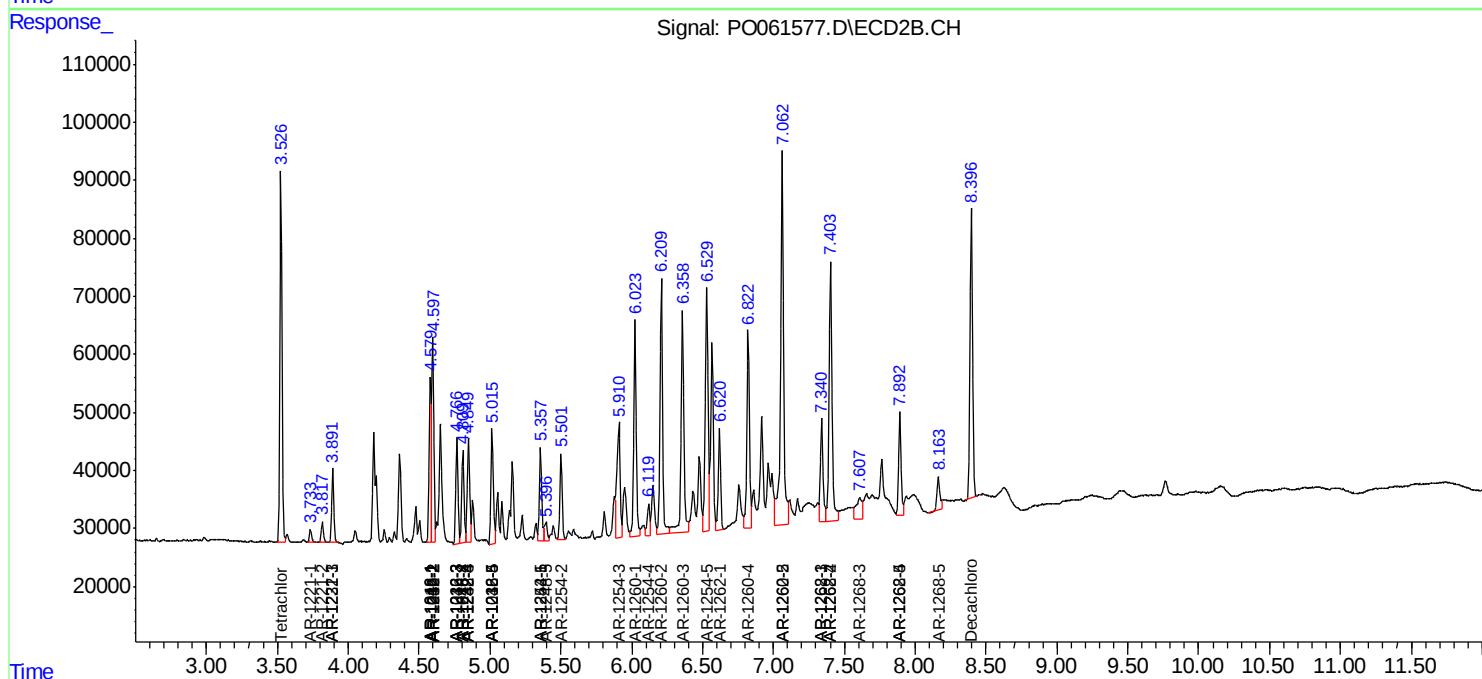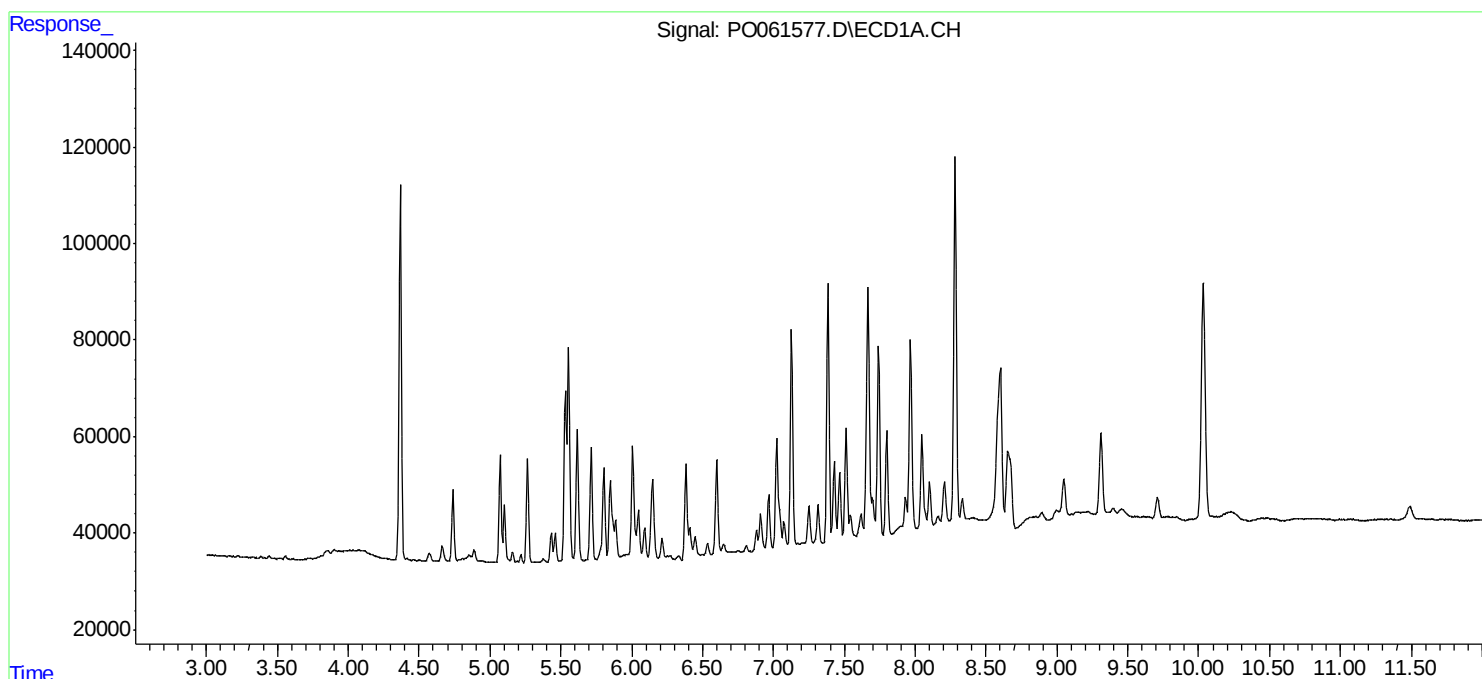


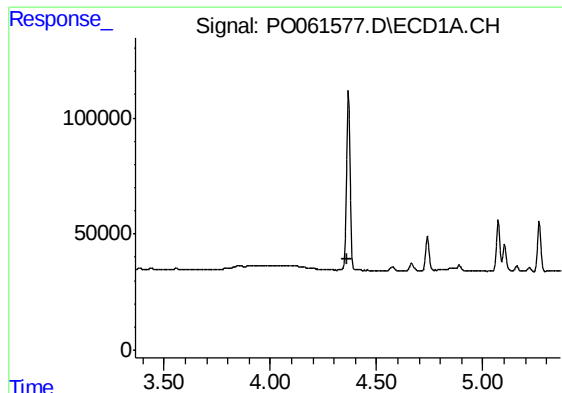

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.365 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

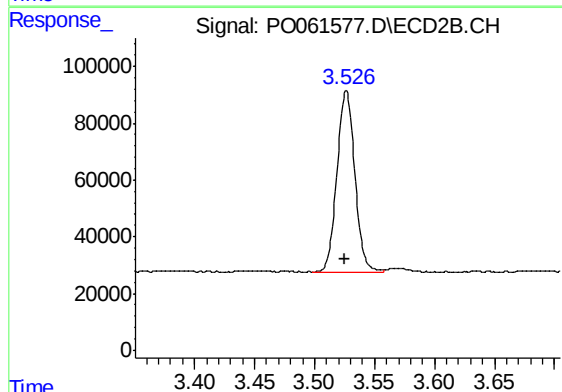


#1 Tetrachloro-m-xylene

R.T.: 3.527 min
Delta R.T.: 0.001 min
Response: 661011
Conc: 20.44 ng/ml

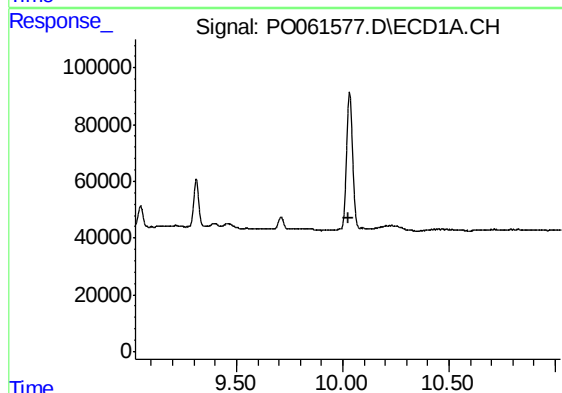


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.025 min
Response: 0
Conc: N.D.

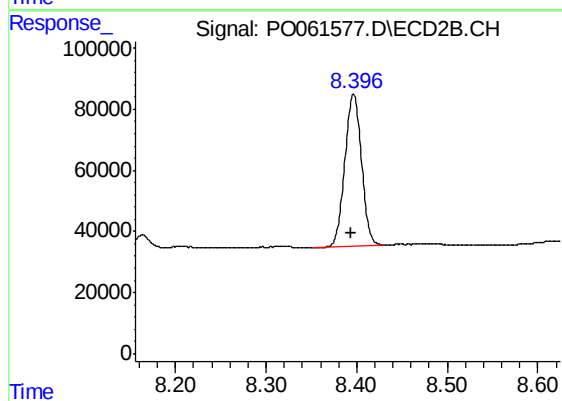

#2 Decachlorobiphenyl


R.T.: 8.397 min
Delta R.T.: 0.003 min
Response: 631781
Conc: 19.51 ng/ml

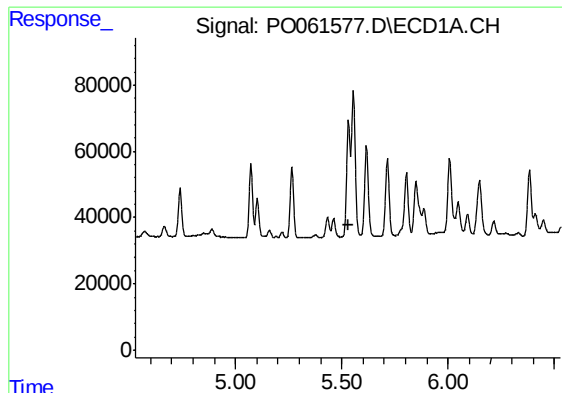

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.529 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

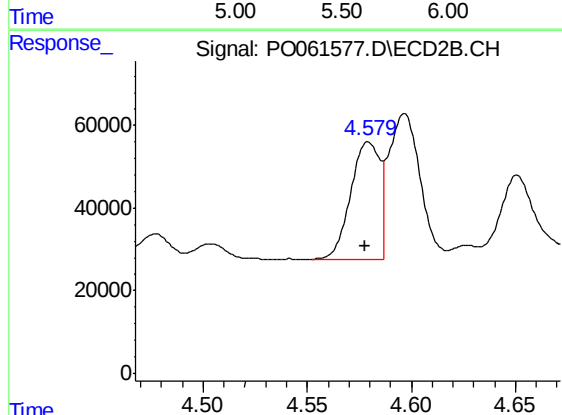


#3 AR-1016-1

R.T.: 4.579 min
Delta R.T.: 0.002 min
Response: 273230
Conc: 203.20 ng/ml

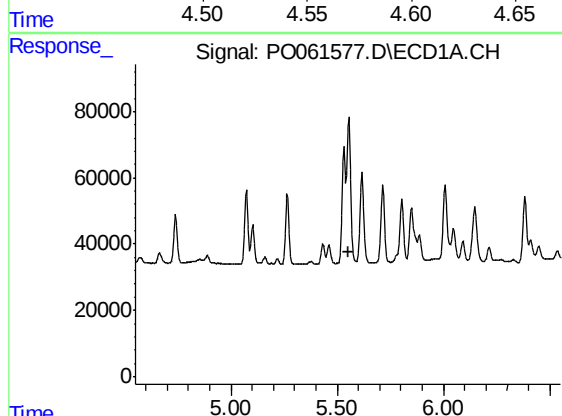


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.551 min
Response: 0
Conc: N.D.

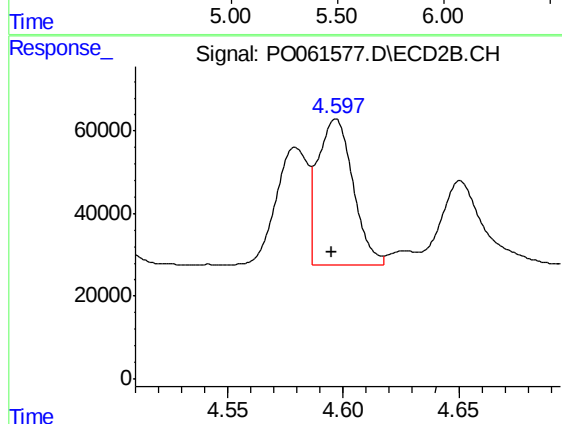

#4 AR-1016-2


R.T.: 4.597 min
Delta R.T.: 0.002 min
Response: 374703
Conc: 202.18 ng/ml

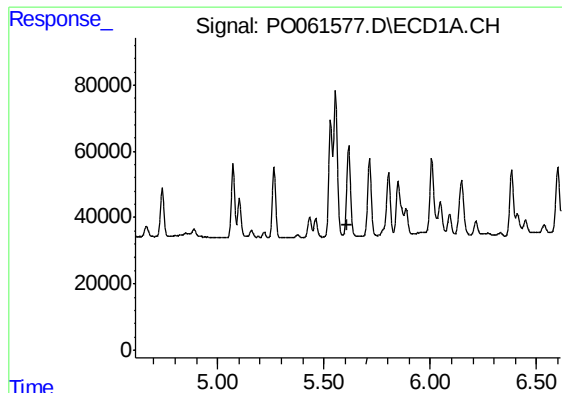

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T. : 5.612 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

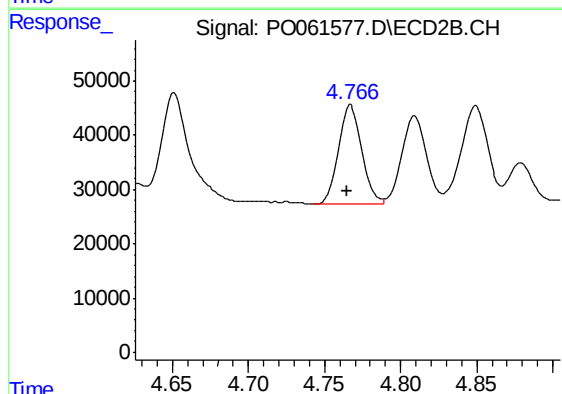


#5 AR-1016-3

R.T.: 4.767 min
Delta R.T.: 0.002 min
Response: 198845
Conc: 198.50 ng/ml

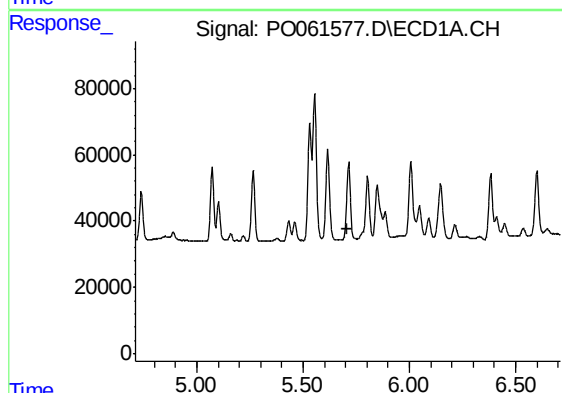


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 5.711 min
Response: 0
Conc: N.D.

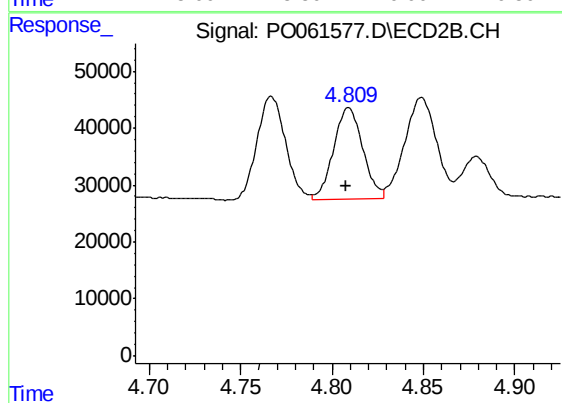

#6 AR-1016-4


R.T.: 4.809 min
Delta R.T.: 0.002 min
Response: 178304
Conc: 205.76 ng/ml

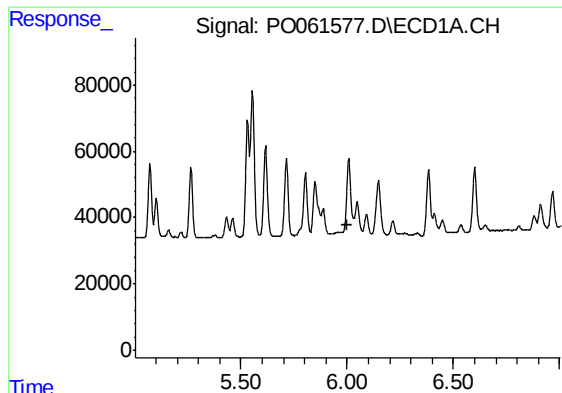

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 6.003 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

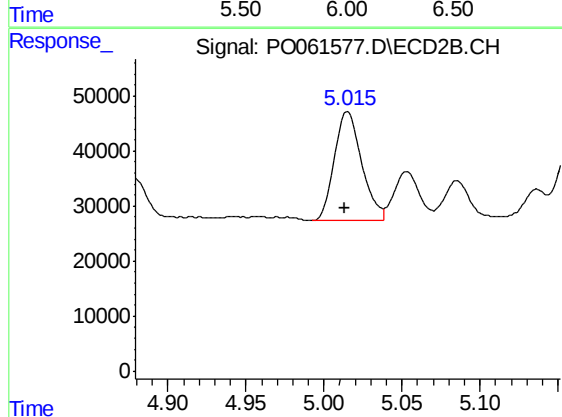


#7 AR-1016-5

R.T.: 5.015 min
Delta R.T.: 0.002 min
Response: 237061
Conc: 207.69 ng/ml

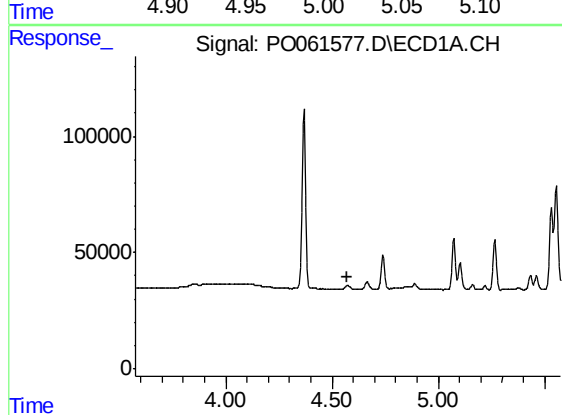


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.574 min
Response: 0
Conc: N.D.

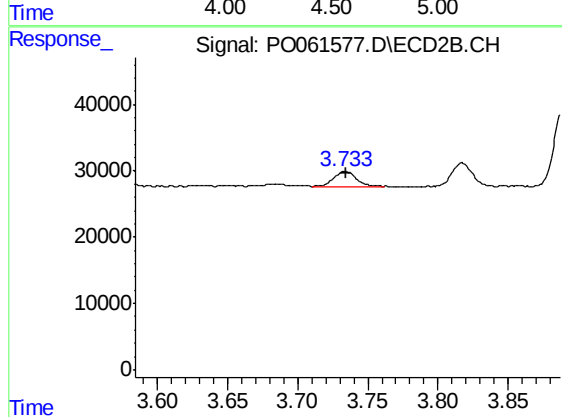

#8 AR-1221-1


R.T.: 3.733 min
Delta R.T.: -0.001 min
Response: 25278
Conc: 63.84 ng/ml

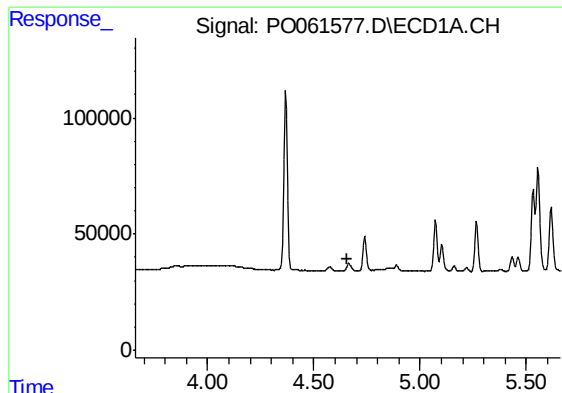

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.660 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

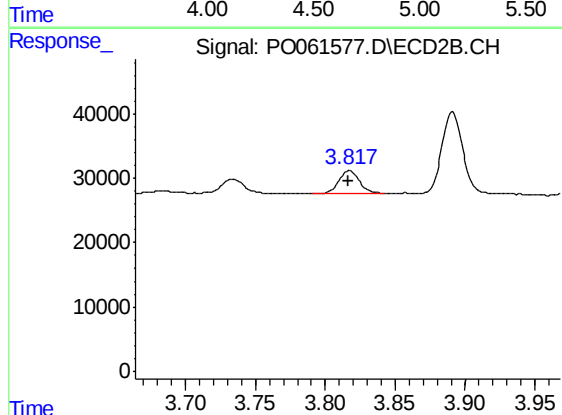


#9 AR-1221-2

R.T.: 3.817 min
Delta R.T.: 0.000 min
Response: 37135
Conc: 120.42 ng/ml

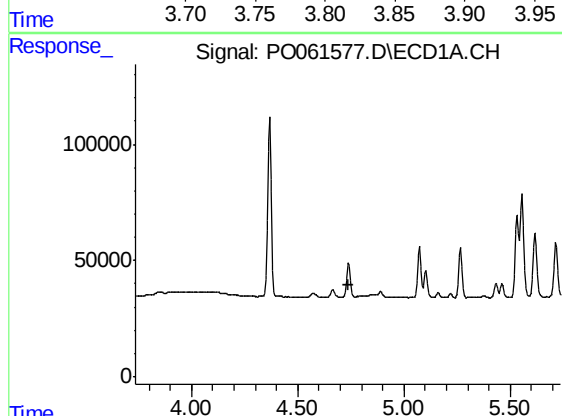


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.736 min
Response: 0
Conc: N.D.

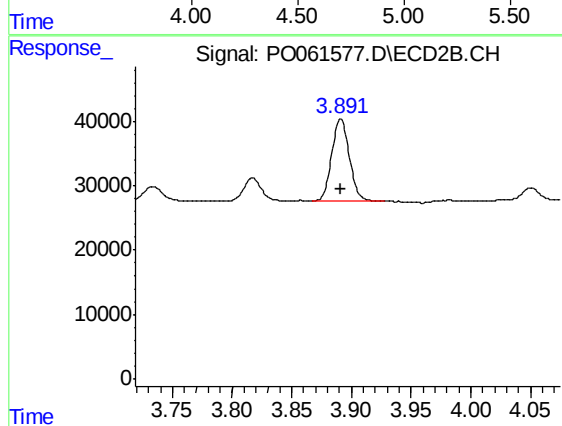

#10 AR-1221-3


R.T.: 3.891 min
Delta R.T.: 0.000 min
Response: 132795
Conc: 145.59 ng/ml



#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.735 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

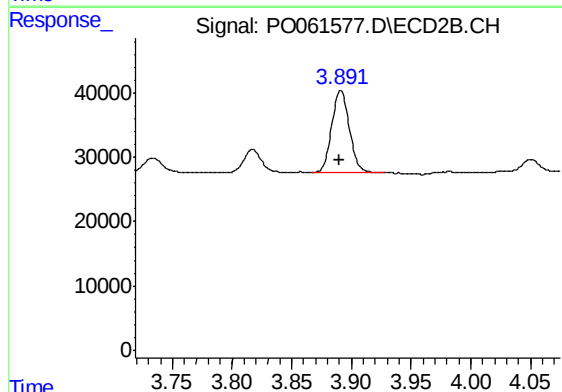


#11 AR-1232-1

R.T.: 3.891 min
Delta R.T.: 0.000 min
Response: 132795
Conc: 118.27 ng/ml




#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.261 min
Response: 0
Conc: N.D.

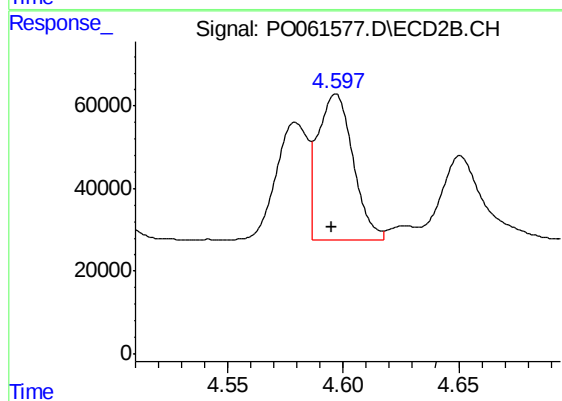

#12 AR-1232-2


R.T.: 4.597 min
Delta R.T.: 0.002 min
Response: 374703
Conc: 306.96 ng/ml

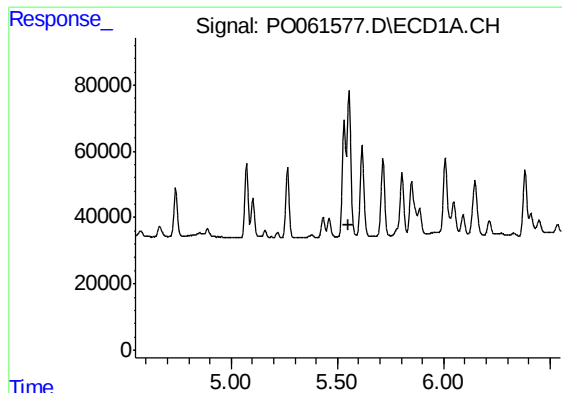

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T. : 5.550 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

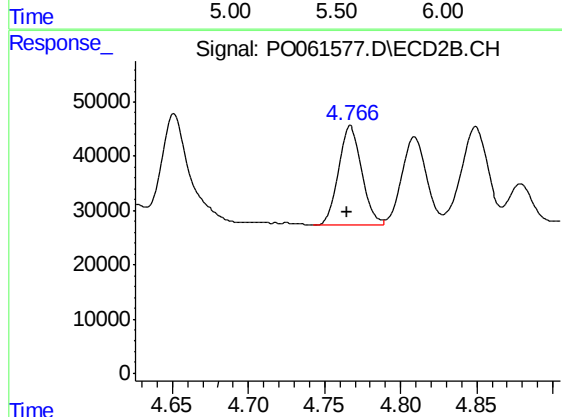


#13 AR-1232-3

R.T.: 4.767 min
Delta R.T.: 0.002 min
Response: 198845
Conc: 301.16 ng/ml

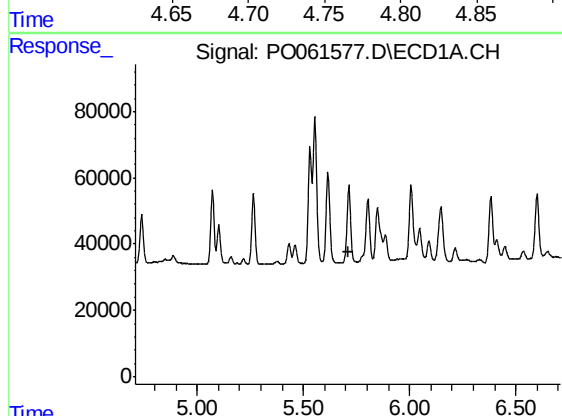


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 5.710 min
Response: 0
Conc: N.D.

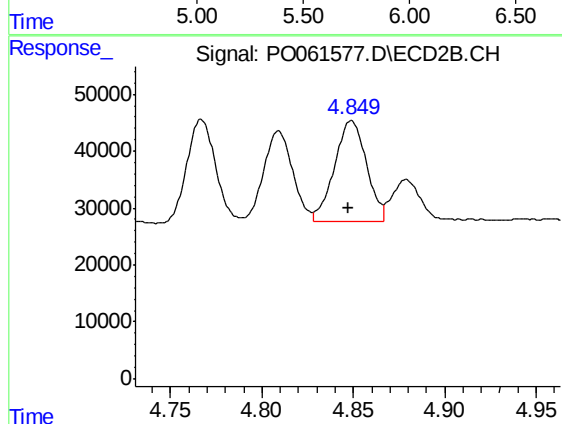

#14 AR-1232-4


R.T.: 4.849 min
Delta R.T.: 0.002 min
Response: 216434
Conc: 343.35 ng/ml



#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.799 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

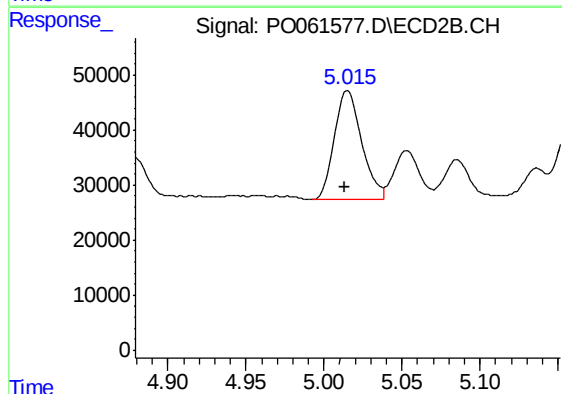


#15 AR-1232-5

R.T.: 5.015 min
Delta R.T.: 0.002 min
Response: 237061
Conc: 345.49 ng/ml




#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 5.528 min
Response: 0
Conc: N.D.

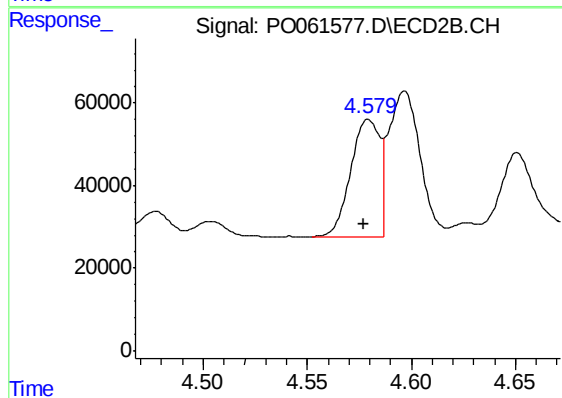

#16 AR-1242-1


R.T.: 4.579 min
Delta R.T.: 0.002 min
Response: 273230
Conc: 266.70 ng/ml



#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.550 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

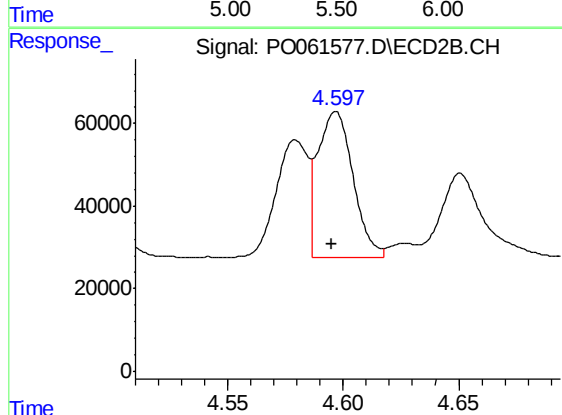


#17 AR-1242-2

R.T.: 4.597 min
Delta R.T.: 0.002 min
Response: 374703
Conc: 265.70 ng/ml

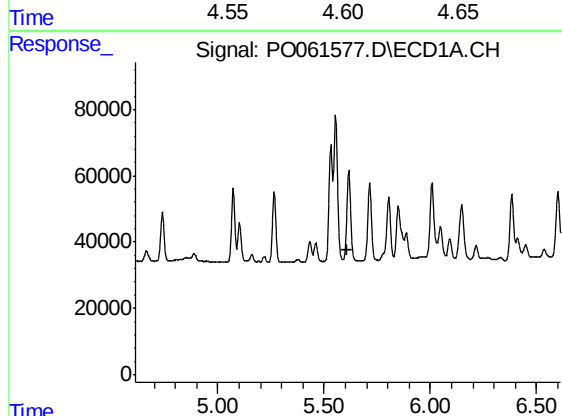


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.612 min
Response: 0
Conc: N.D.

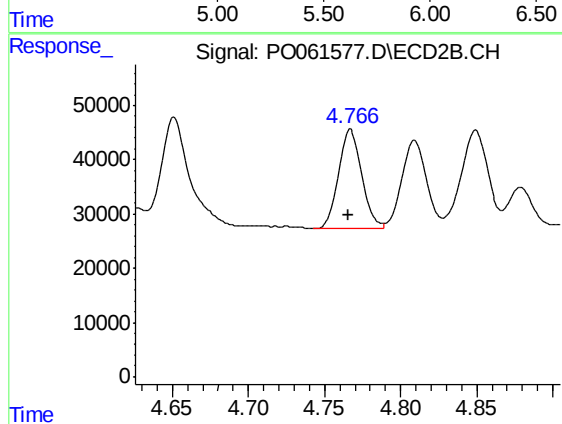

#18 AR-1242-3


R.T.: 4.767 min
Delta R.T.: 0.001 min
Response: 198845
Conc: 254.64 ng/ml

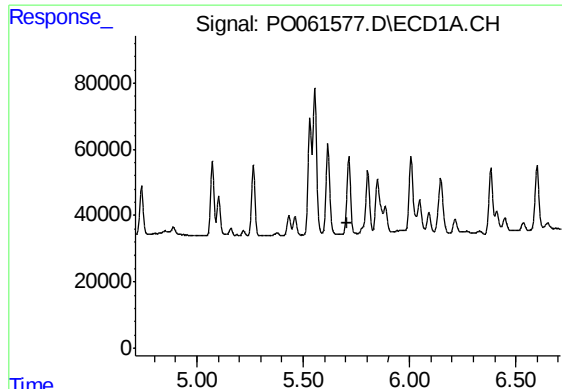

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T. : 5.710 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

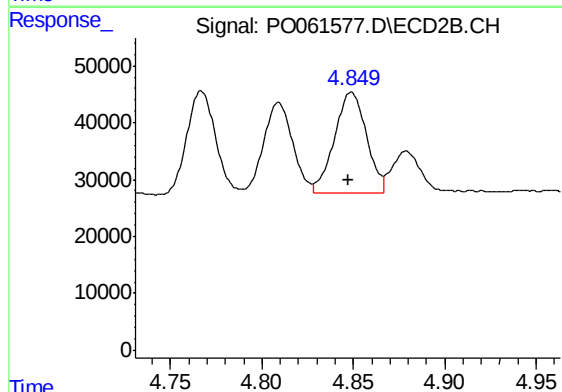


#19 AR-1242-4

R.T.: 4.849 min
Delta R.T.: 0.001 min
Response: 216434
Conc: 263.75 ng/ml




#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

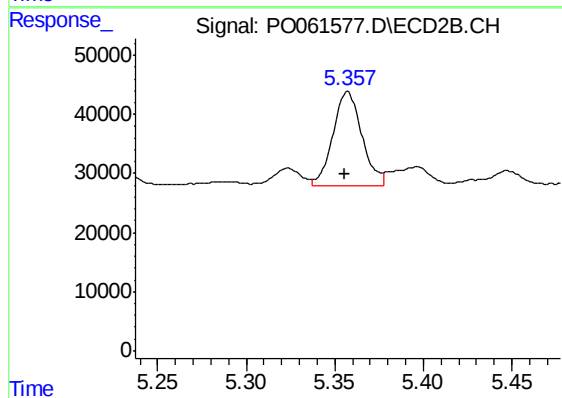

#20 AR-1242-5


R.T.: 5.357 min
Delta R.T.: 0.002 min
Response: 183427
Conc: 171.23 ng/ml



#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.528 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

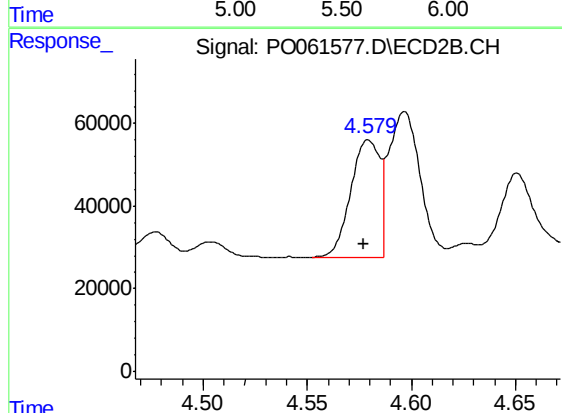


#21 AR-1248-1

R.T.: 4.579 min
Delta R.T.: 0.002 min
Response: 273230
Conc: 305.35 ng/ml

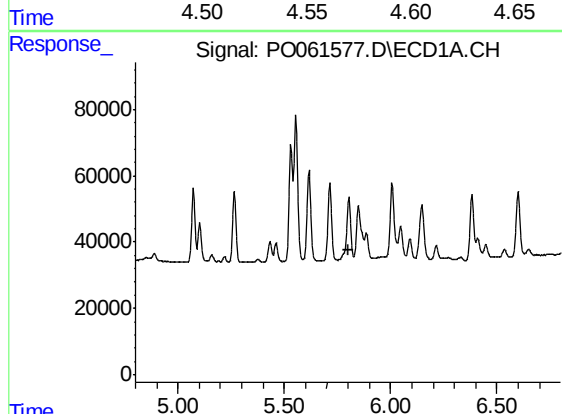


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 5.800 min
Response: 0
Conc: N.D.

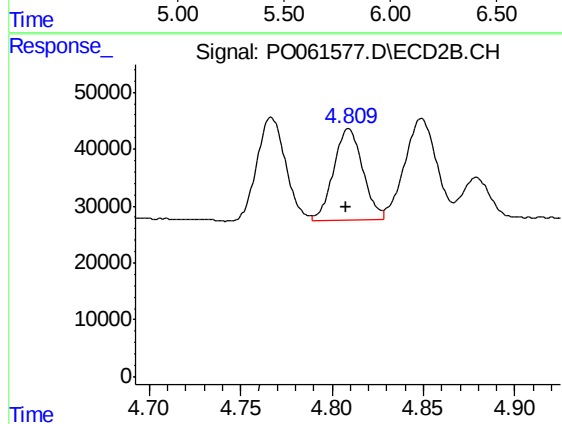

#22 AR-1248-2


R.T.: 4.809 min
Delta R.T.: 0.002 min
Response: 178304
Conc: 151.33 ng/ml

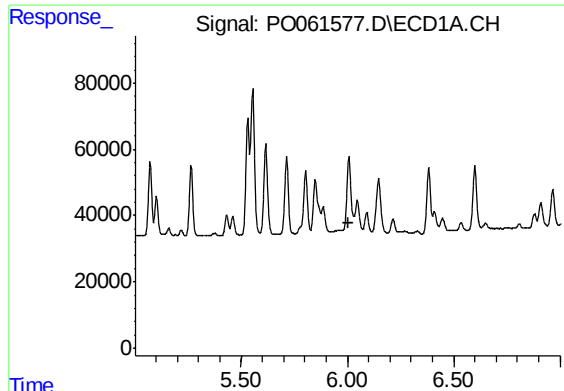

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 6.003 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

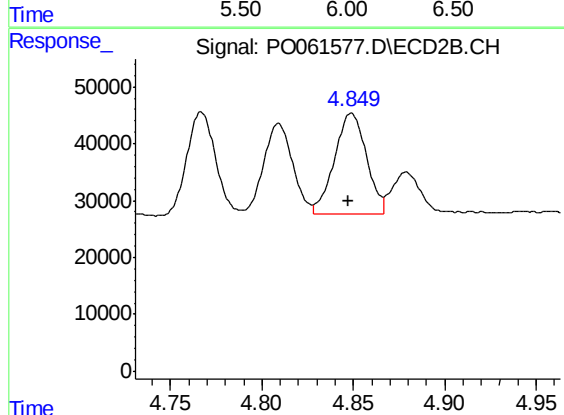


#23 AR-1248-3

R.T.: 4.849 min
Delta R.T.: 0.002 min
Response: 216434
Conc: 174.36 ng/ml

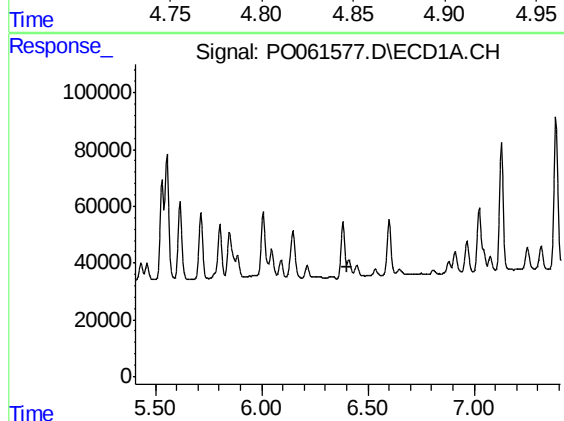


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 6.406 min
Response: 0
Conc: N.D.

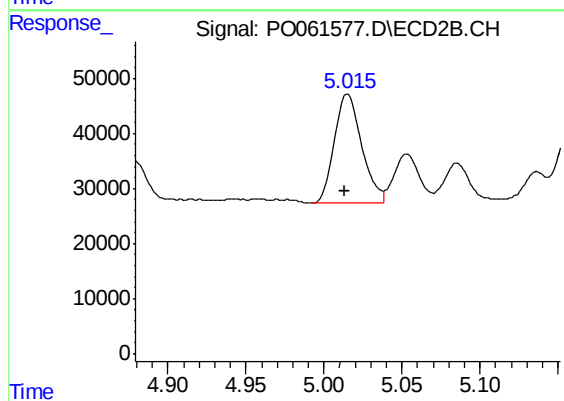

#24 AR-1248-4


R.T.: 5.015 min
Delta R.T.: 0.002 min
Response: 237061
Conc: 157.69 ng/ml



#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.444 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

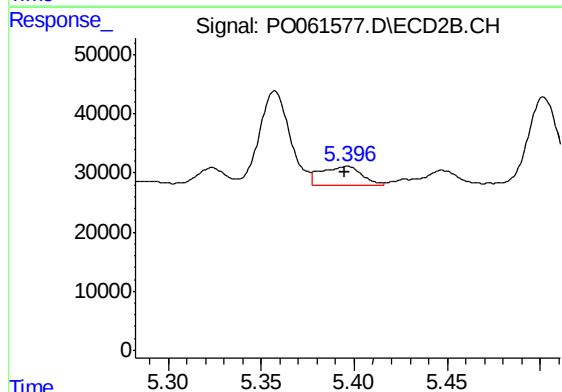


#25 AR-1248-5

R.T.: 5.396 min
Delta R.T.: 0.001 min
Response: 48893
Conc: 31.87 ng/ml




#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.381 min
Response: 0
Conc: N.D.

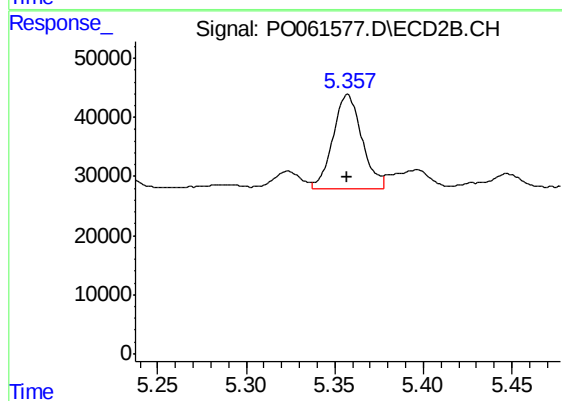

#26 AR-1254-1


R.T.: 5.357 min
Delta R.T.: 0.000 min
Response: 183427
Conc: 83.63 ng/ml

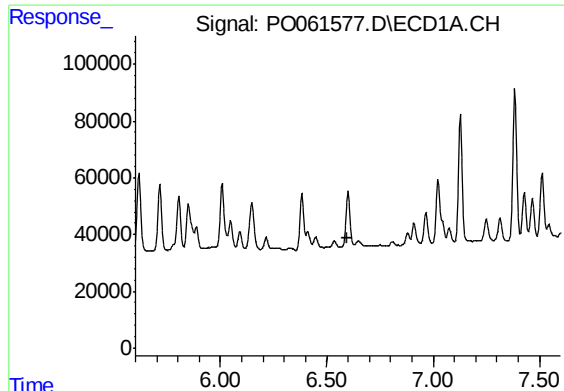

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 6.599 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

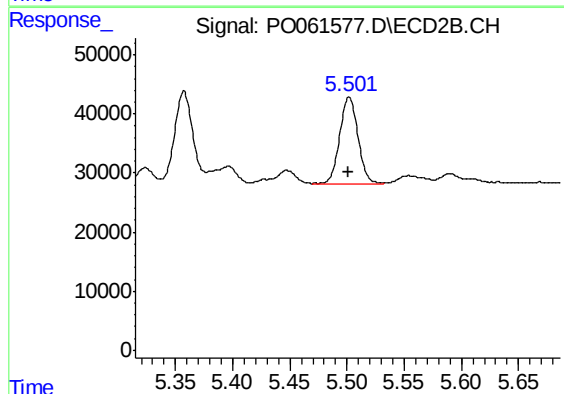


#27 AR-1254-2

R.T.: 5.502 min
Delta R.T.: 0.000 min
Response: 167541
Conc: 85.46 ng/ml

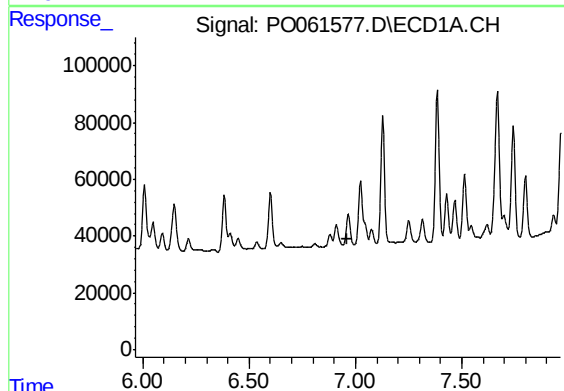


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.964 min
Response: 0
Conc: N.D.

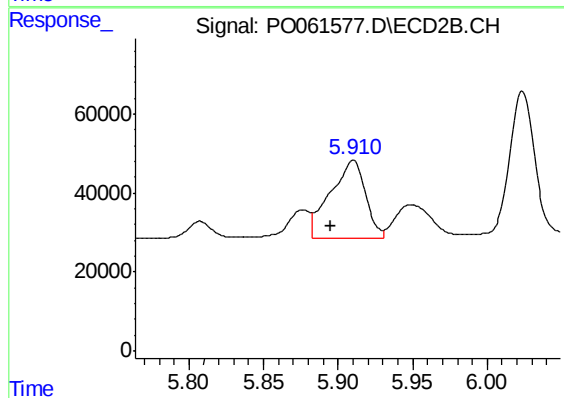

#28 AR-1254-3


R.T.: 5.910 min
Delta R.T.: 0.015 min
Response: 324539
Conc: 101.94 ng/ml



#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.250 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

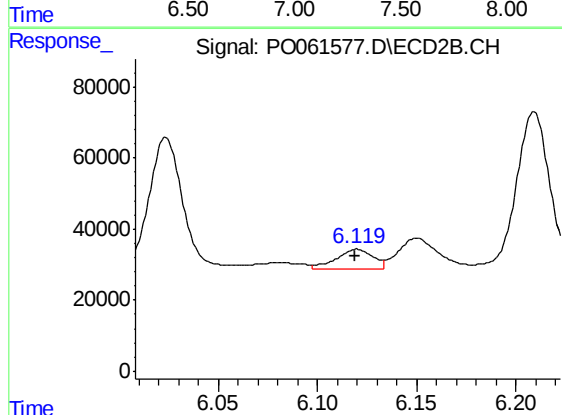


#29 AR-1254-4

R.T.: 6.120 min
Delta R.T.: 0.000 min
Response: 70185
Conc: 34.59 ng/ml

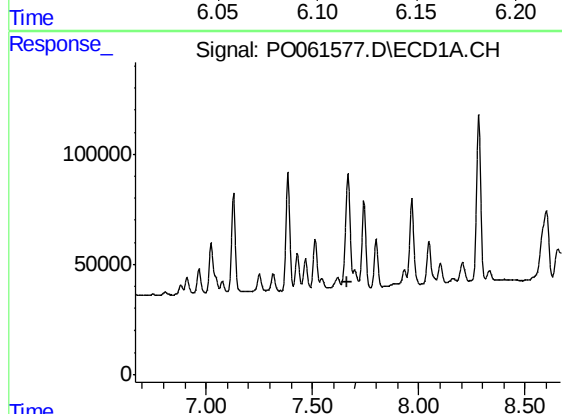


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 7.667 min
Response: 0
Conc: N.D.

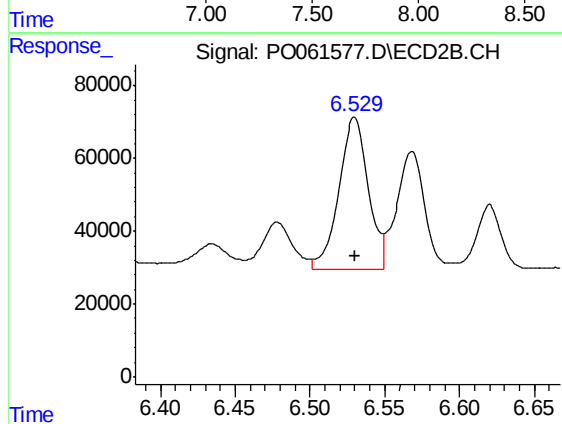

#30 AR-1254-5


R.T.: 6.530 min
Delta R.T.: 0.000 min
Response: 573897
Conc: 202.90 ng/ml

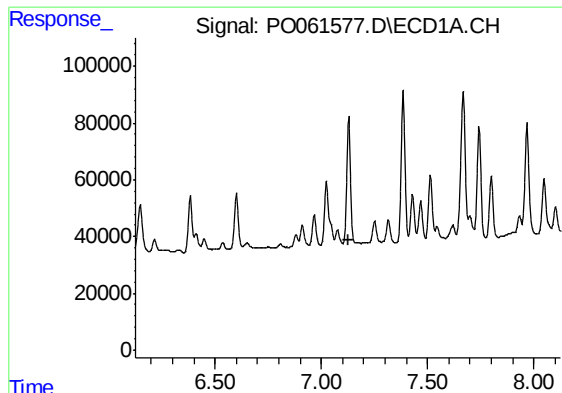

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 7.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

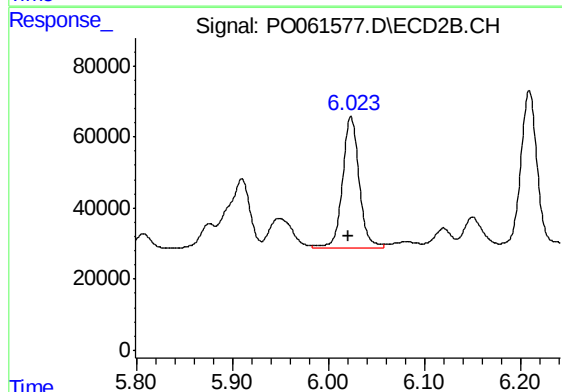


#31 AR-1260-1

R.T.: 6.024 min
Delta R.T.: 0.002 min
Response: 453082
Conc: 222.12 ng/ml




#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.381 min
Response: 0
Conc: N.D.

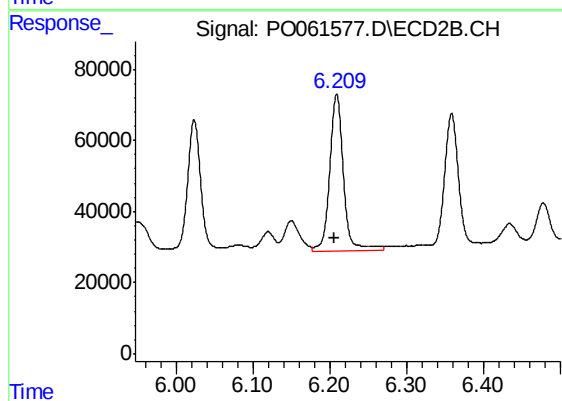

#32 AR-1260-2


R.T.: 6.209 min
Delta R.T.: 0.002 min
Response: 546960
Conc: 227.74 ng/ml

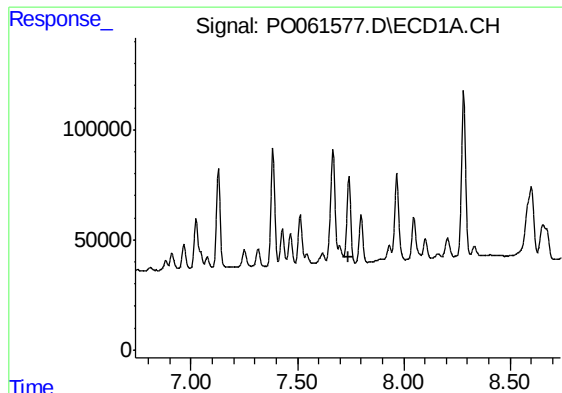

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.738 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

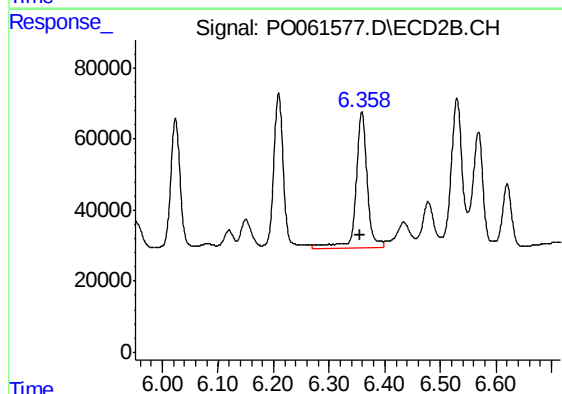


#33 AR-1260-3

R.T.: 6.359 min
Delta R.T.: 0.002 min
Response: 547778
Conc: 243.12 ng/ml

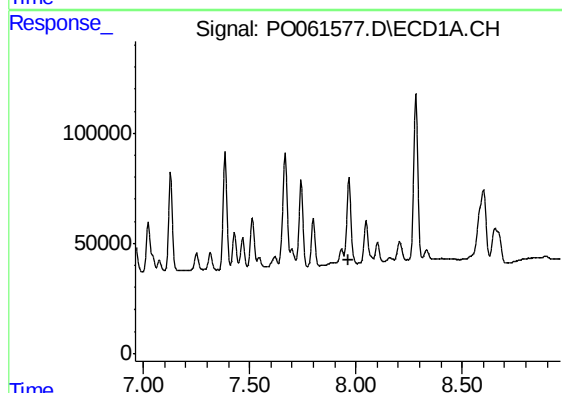


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.963 min
Response: 0
Conc: N.D.

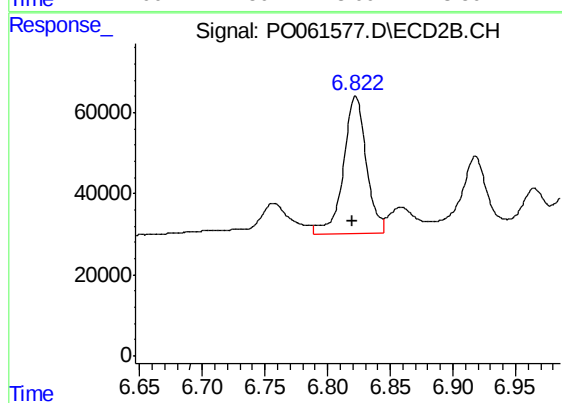

#34 AR-1260-4


R.T.: 6.822 min
Delta R.T.: 0.002 min
Response: 434417
Conc: 235.30 ng/ml



#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.277 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

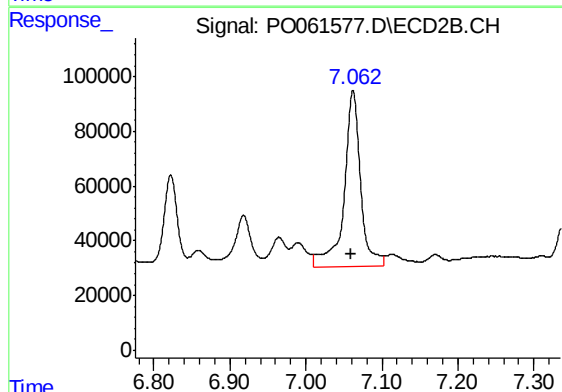


#35 AR-1260-5

R.T.: 7.062 min
Delta R.T.: 0.002 min
Response: 971257
Conc: 249.45 ng/ml

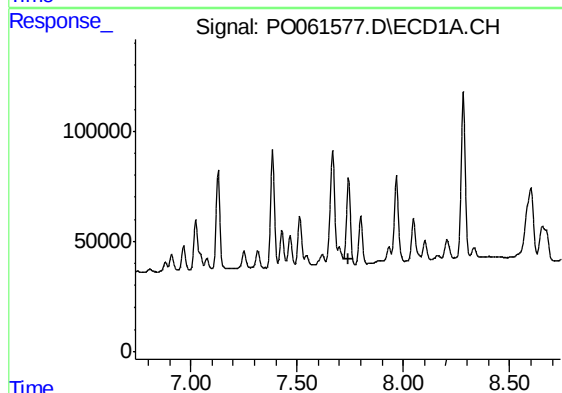


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.740 min
Response: 0
Conc: N.D.

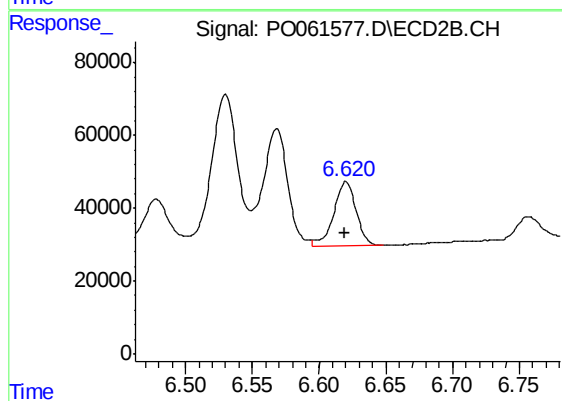

#36 AR-1262-1


R.T.: 6.620 min
Delta R.T.: 0.001 min
Response: 204471
Conc: 167.51 ng/ml



#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.279 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

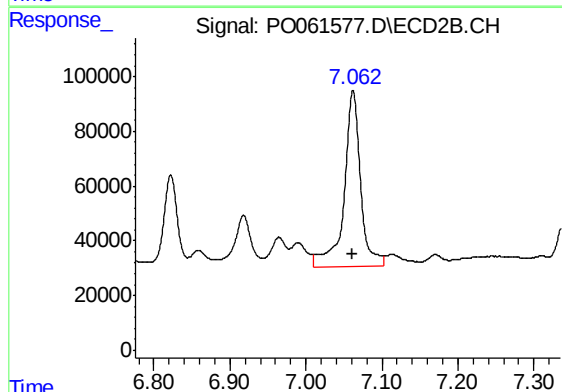


#37 AR-1262-2

R.T.: 7.062 min
Delta R.T.: 0.001 min
Response: 971257
Conc: 211.23 ng/ml




#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.581 min
Response: 0
Conc: N.D.

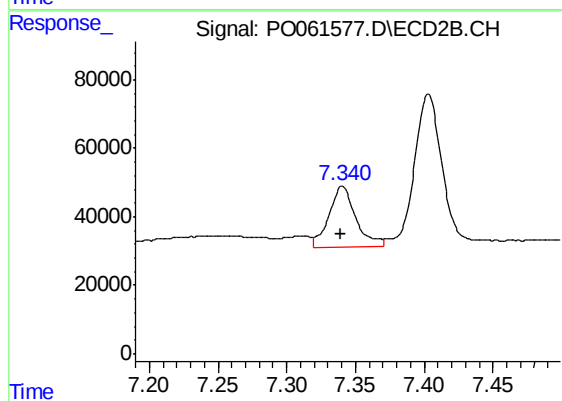

#38 AR-1262-3


R.T.: 7.340 min
Delta R.T.: 0.000 min
Response: 243508
Conc: 129.26 ng/ml

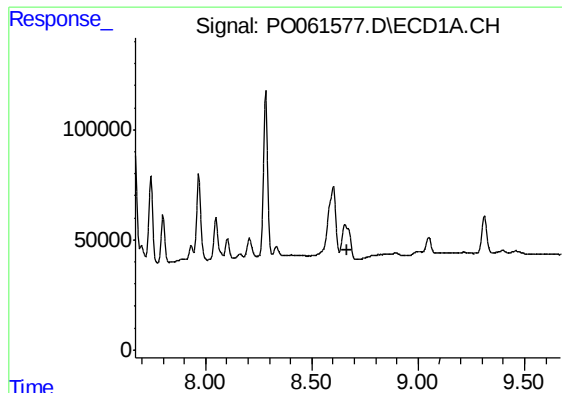

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.669 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

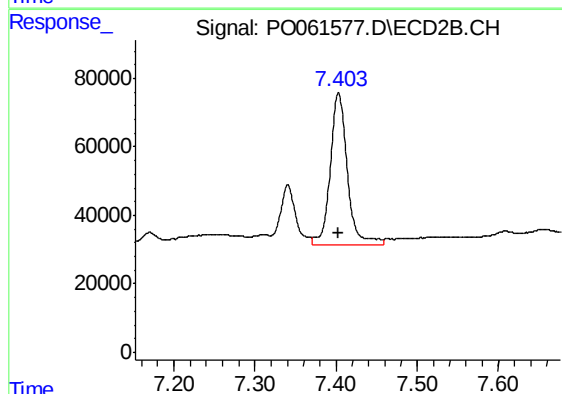


#39 AR-1262-4

R.T.: 7.403 min
Delta R.T.: 0.000 min
Response: 655919
Conc: 195.17 ng/ml

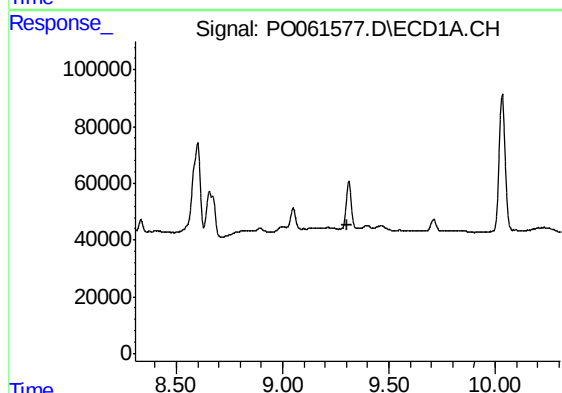


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.307 min
Response: 0
Conc: N.D.

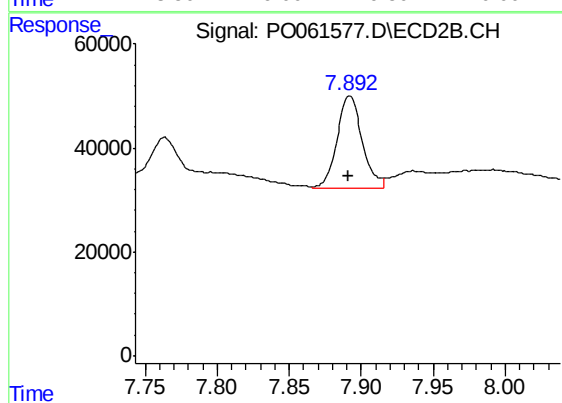

#40 AR-1262-5


R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 215863
Conc: 142.39 ng/ml



#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 8.581 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

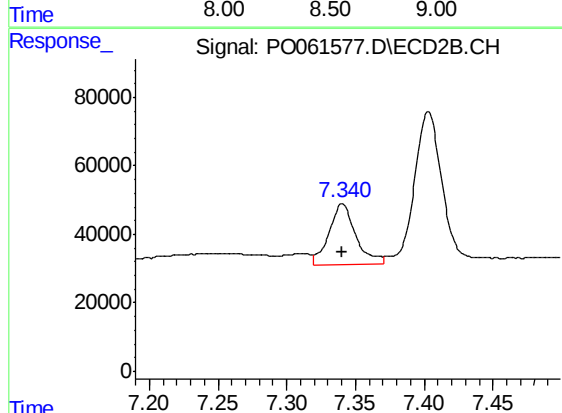


#41 AR-1268-1

R.T.: 7.340 min
Delta R.T.: 0.000 min
Response: 243508
Conc: 50.42 ng/ml

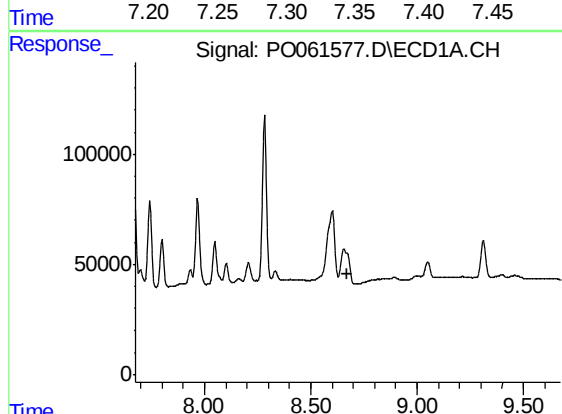


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.674 min
Response: 0
Conc: N.D.

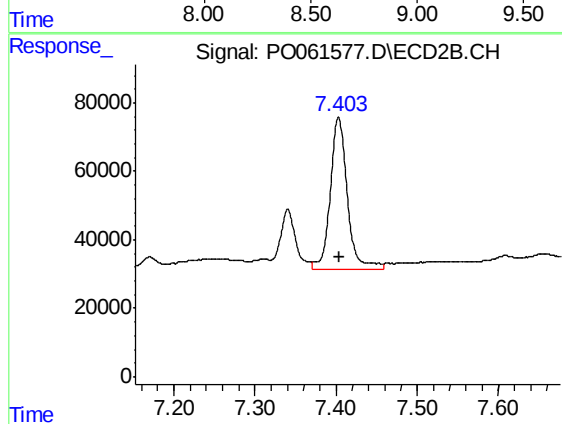

#42 AR-1268-2


R.T.: 7.403 min
Delta R.T.: -0.001 min
Response: 655919
Conc: 152.19 ng/ml



#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 8.894 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

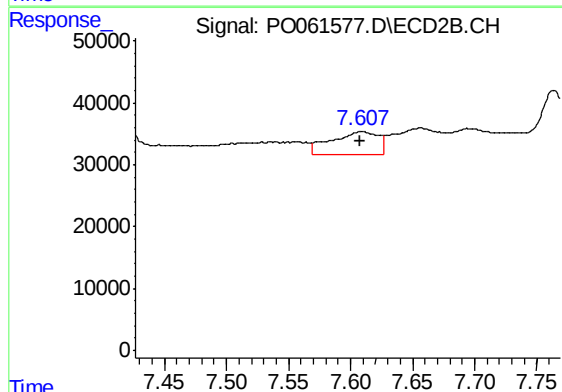


#43 AR-1268-3

R.T.: 7.609 min
Delta R.T.: 0.001 min
Response: 97312
Conc: 27.15 ng/ml




#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.309 min
Response: 0
Conc: N.D.

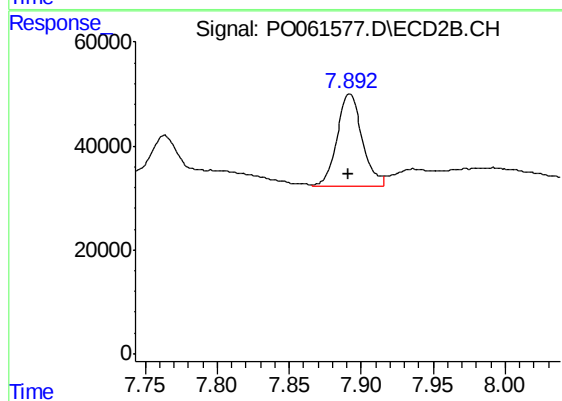

#44 AR-1268-4


R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 215863
Conc: 134.13 ng/ml

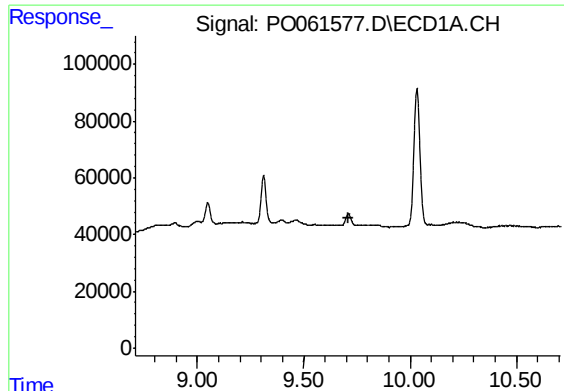

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.708 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-02

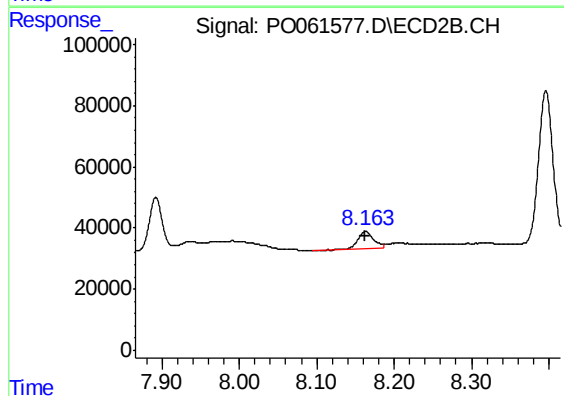

#45 AR-1268-5

R.T.: 8.164 min
Delta R.T.: 0.000 min
Response: 79183
Conc: 7.87 ng/ml