

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100219\
 Data File : P0061578.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Oct 2019 12:49
 Operator : HP/AJ
 Sample : IDOC-WATER-03
 Misc : HIRAL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IDOC-WATER-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 14:13:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	0.000	3.527	0	672921	N.D.	20.808 #
2) SA Decachlor...	0.000	8.397	0	629770	N.D.	19.452 #
Target Compounds						
3) L1 AR-1016-1	0.000	4.580	0	287498	N.D.	213.807 #
4) L1 AR-1016-2	0.000	4.598	0	384928	N.D.	207.692 #
5) L1 AR-1016-3	0.000	4.768	0	214793	N.D.	214.424 #
6) L1 AR-1016-4	0.000	4.810	0	181776	N.D.	209.767 #
7) L1 AR-1016-5	0.000	5.016	0	226995	N.D.	198.867 #
8) L2 AR-1221-1	0.000	3.734	0	25884	N.D.	65.369 #
9) L2 AR-1221-2	0.000	3.818	0	37038	N.D.	120.100 #
10) L2 AR-1221-3	0.000	3.892	0	128972	N.D.	141.395 #
11) L3 AR-1232-1	0.000	3.892	0	128972	N.D.	114.867 #
12) L3 AR-1232-2	0.000	4.598	0	384928	N.D.	315.338 #
13) L3 AR-1232-3	0.000	4.768	0	214793	N.D.	325.318 #
14) L3 AR-1232-4	0.000	4.850	0	218921	N.D.	347.300 #
15) L3 AR-1232-5	0.000	5.016	0	226995	N.D.	330.824 #
16) L4 AR-1242-1	0.000	4.580	0	287498	N.D.	280.622 #
17) L4 AR-1242-2	0.000	4.598	0	384928	N.D.	272.956 #
18) L4 AR-1242-3	0.000	4.768	0	214793	N.D.	275.064 #
19) L4 AR-1242-4	0.000	4.850	0	218921	N.D.	266.782 #
20) L4 AR-1242-5	0.000	5.358	0	172617	N.D.	161.137 #
21) L5 AR-1248-1	0.000	4.580	0	287498	N.D.	321.293 #
22) L5 AR-1248-2	0.000	4.810	0	181776	N.D.	154.275 #
23) L5 AR-1248-3	0.000	4.850	0	218921	N.D.	176.368 #
24) L5 AR-1248-4	0.000	5.016	0	226995	N.D.	150.998 #
25) L5 AR-1248-5	0.000	5.397	0	33283	N.D.	21.695 #
26) L6 AR-1254-1	0.000	5.358	0	172617	N.D.	78.702 #
27) L6 AR-1254-2	0.000	5.503	0	158414	N.D.	80.803 #
28) L6 AR-1254-3	0.000	5.911	0	303939	N.D.	95.466 #
29) L6 AR-1254-4	0.000	6.121	0	52726	N.D.	25.988 #
30) L6 AR-1254-5	0.000	6.531	0	534745	N.D.	189.058 #
31) L7 AR-1260-1	0.000	6.025	0	414696	N.D.	203.302 #
32) L7 AR-1260-2	0.000	6.210	0	491848	N.D.	204.789 #
33) L7 AR-1260-3	0.000	6.360	0	472749	N.D.	209.820 #
34) L7 AR-1260-4	0.000	6.823	0	380219	N.D.	205.946 #
35) L7 AR-1260-5	0.000	7.063	0	826452	N.D.	212.258 #
36) L8 AR-1262-1	0.000	6.621	0	199874	N.D.	163.746 #
37) L8 AR-1262-2	0.000	7.063	0	826452	N.D.	179.741 #
38) L8 AR-1262-3	0.000	7.342	0	201977	N.D.	107.217 #
39) L8 AR-1262-4	0.000	7.404	0	584303	N.D.	173.862 #
40) L8 AR-1262-5	0.000	7.893	0	207441	N.D.	136.837 #
41) L9 AR-1268-1	0.000	7.342	0	201977	N.D.	41.825 #
42) L9 AR-1268-2	0.000	7.404	0	584303	N.D.	135.575 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100219\
 Data File : P0061578.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Oct 2019 12:49
 Operator : HP/AJ
 Sample : IDOC-WATER-03
 Misc : HIRAL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IDOC-WATER-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 14:13:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	0.000	7.609	0	77805	N.D.	21.708 #
44) L9	AR-1268-4	0.000	7.893	0	207441	N.D.	128.894 #
45) L9	AR-1268-5	0.000	8.165	0	85220	N.D.	8.474 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100219\
Data File : PO061578.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Oct 2019 12:49
Operator : HP/AJ
Sample : IDOC-WATER-03
Misc : HIRAL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 14:13:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

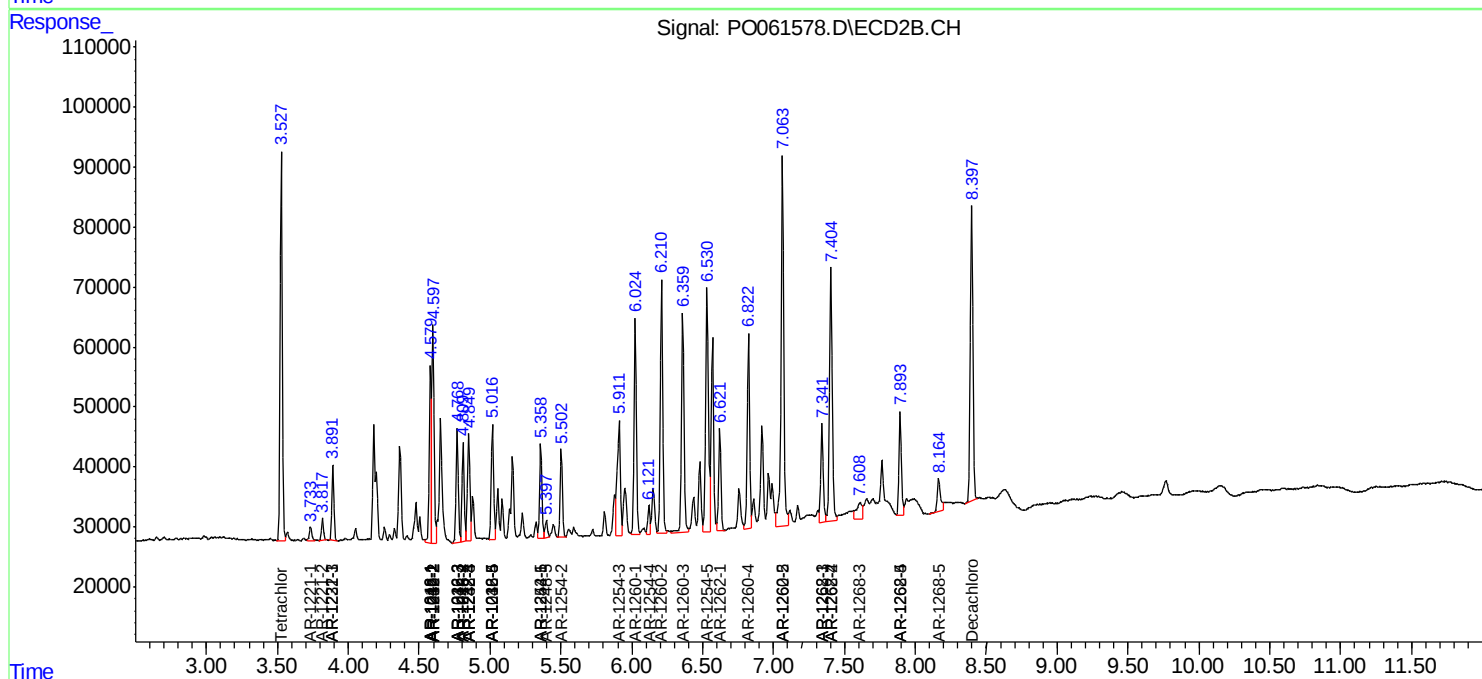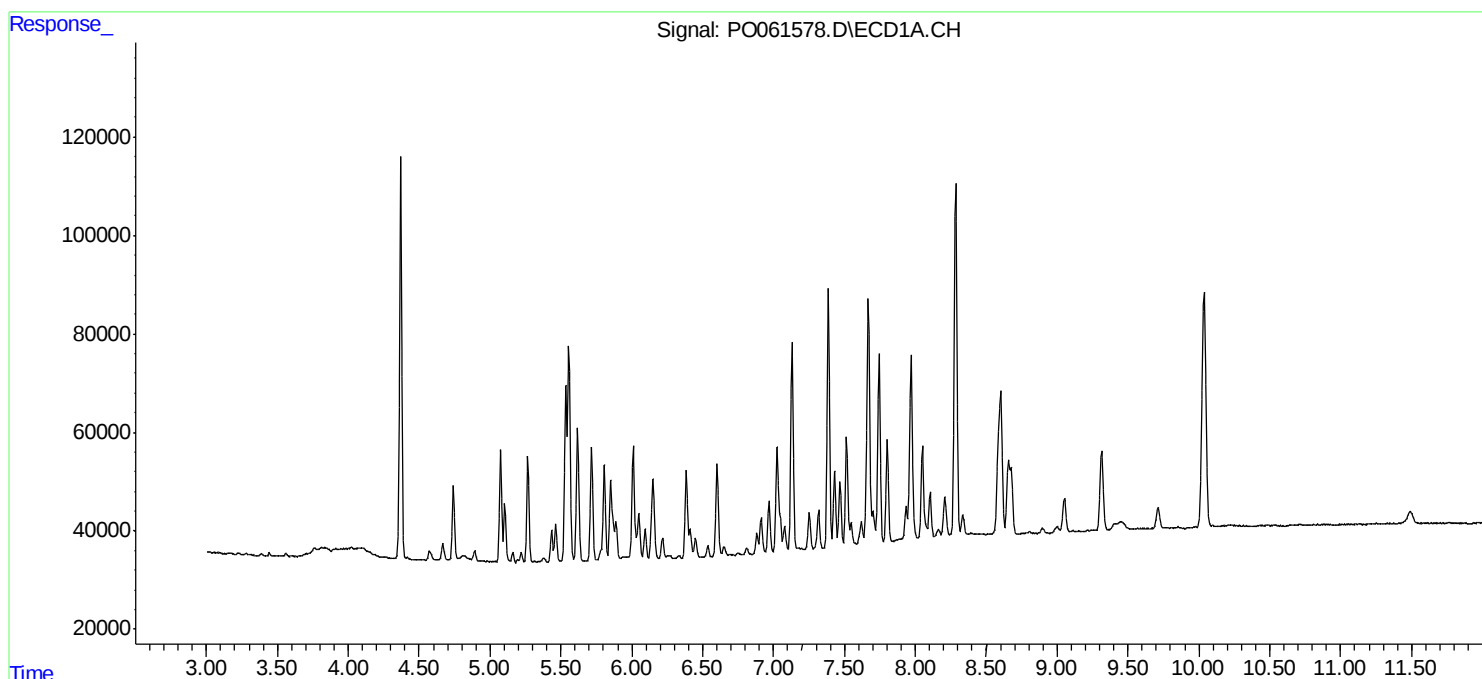


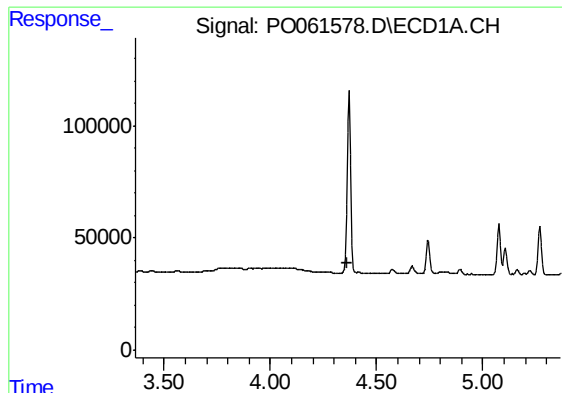

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.365 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

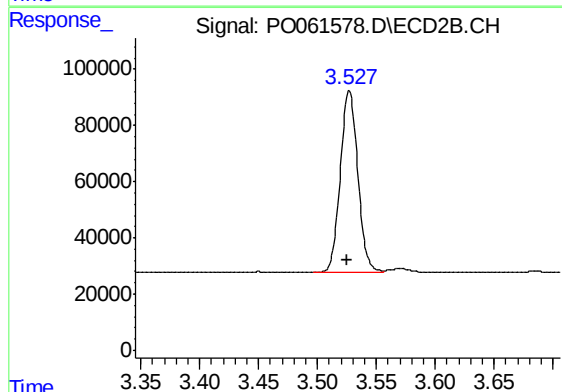


#1 Tetrachloro-m-xylene

R.T.: 3.527 min
Delta R.T.: 0.002 min
Response: 672921
Conc: 20.81 ng/ml




#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.025 min
Response: 0
Conc: N.D.

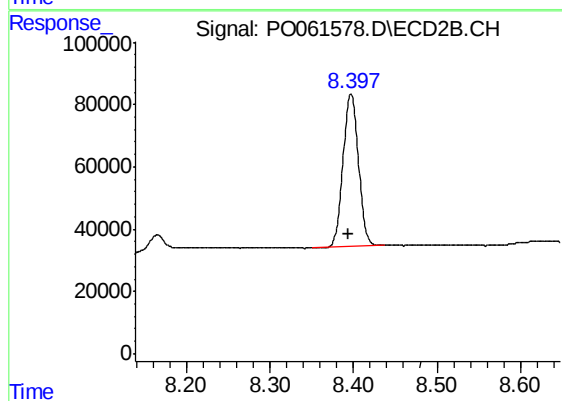

#2 Decachlorobiphenyl


R.T.: 8.397 min
Delta R.T.: 0.003 min
Response: 629770
Conc: 19.45 ng/ml

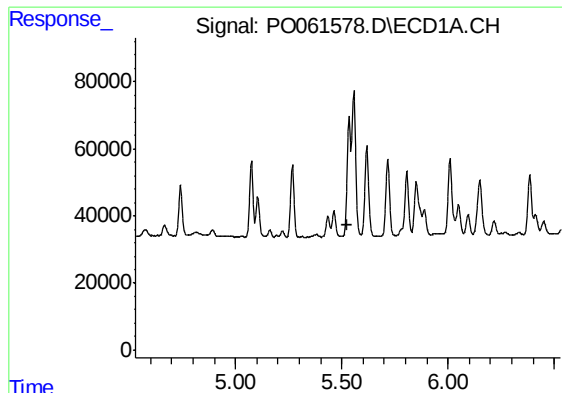

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T. : 5.529 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

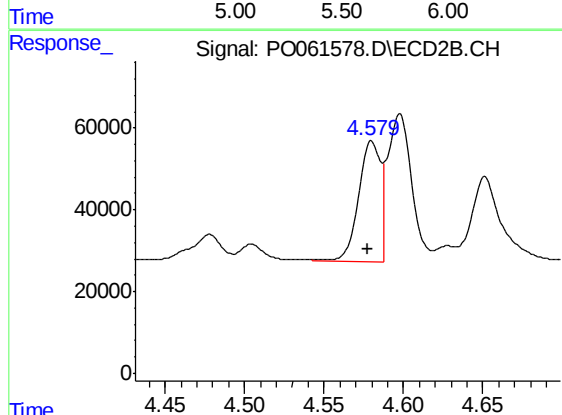


#3 AR-1016-1

R.T.: 4.580 min
Delta R.T.: 0.002 min
Response: 287498
Conc: 213.81 ng/ml

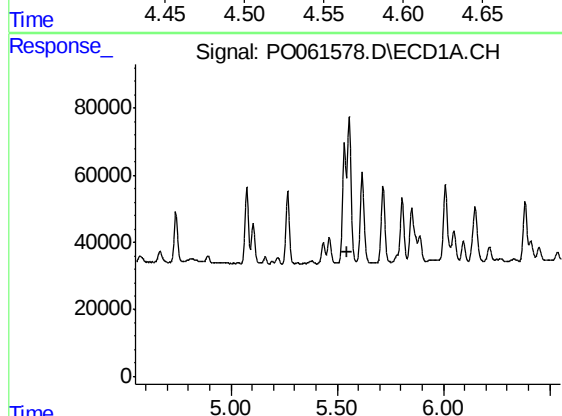


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T. : 5.551 min
Response: 0
Conc: N.D.

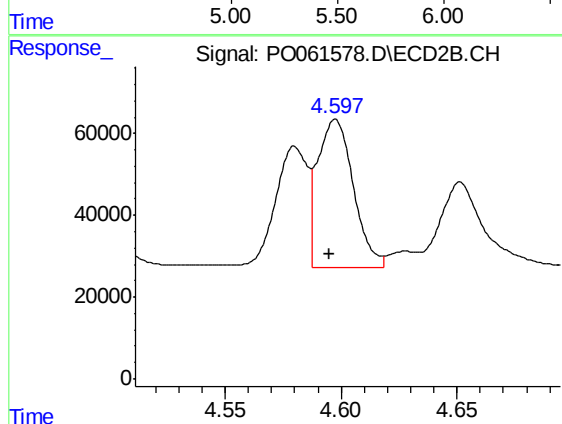

#4 AR-1016-2


R.T.: 4.598 min
Delta R.T.: 0.003 min
Response: 384928
Conc: 207.69 ng/ml



#5 AR-1016-3


R.T.: 0.000 min
Exp R.T. : 5.612 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

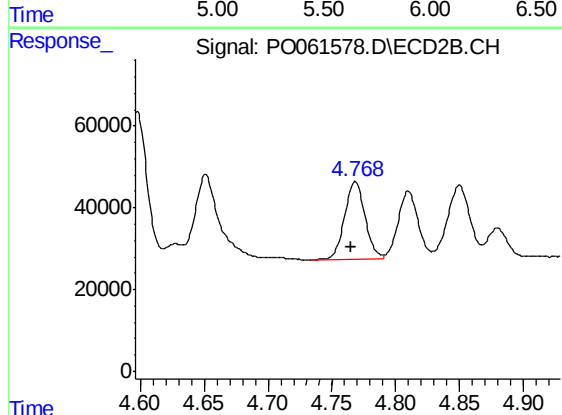


#5 AR-1016-3

R.T.: 4.768 min
Delta R.T.: 0.003 min
Response: 214793
Conc: 214.42 ng/ml

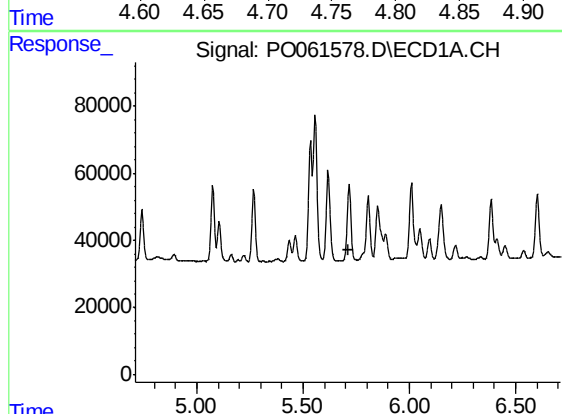


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 5.711 min
Response: 0
Conc: N.D.

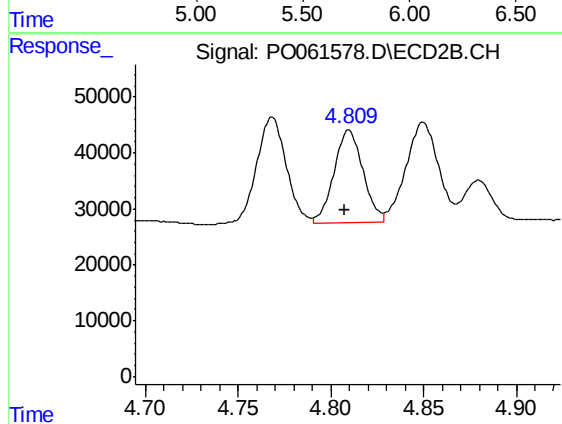

#6 AR-1016-4


R.T.: 4.810 min
Delta R.T.: 0.002 min
Response: 181776
Conc: 209.77 ng/ml

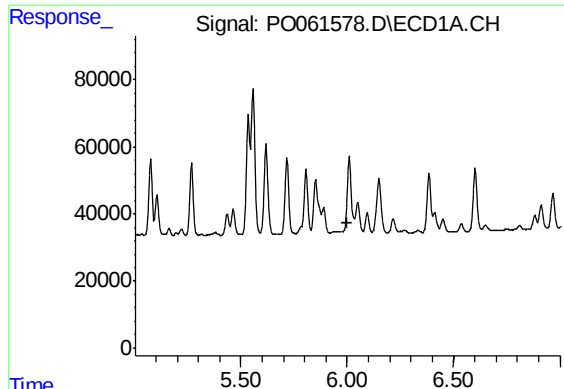

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 6.003 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

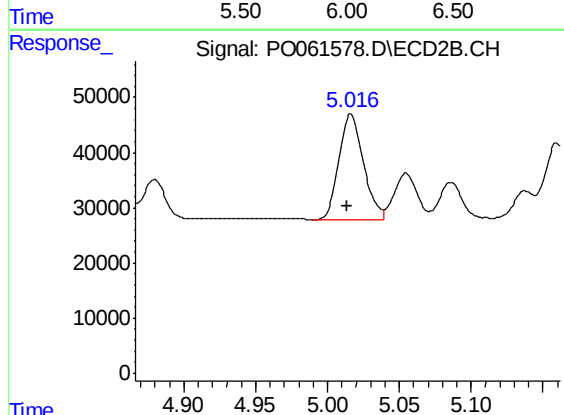


#7 AR-1016-5

R.T.: 5.016 min
Delta R.T.: 0.003 min
Response: 226995
Conc: 198.87 ng/ml

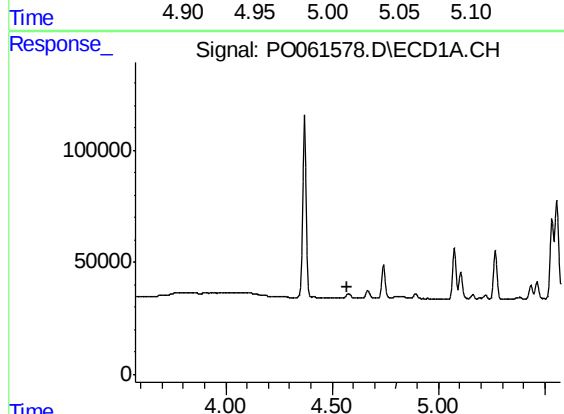


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.574 min
Response: 0
Conc: N.D.

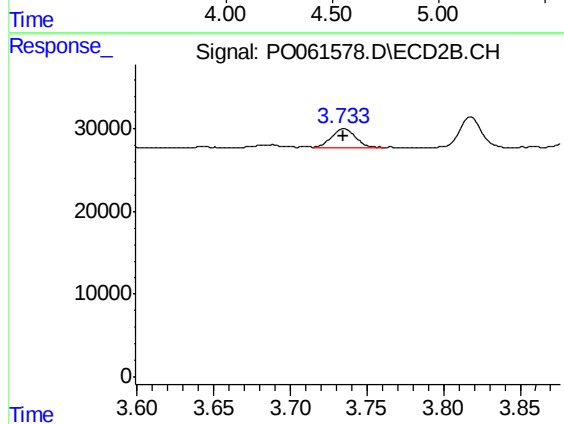

#8 AR-1221-1


R.T.: 3.734 min
Delta R.T.: 0.000 min
Response: 25884
Conc: 65.37 ng/ml

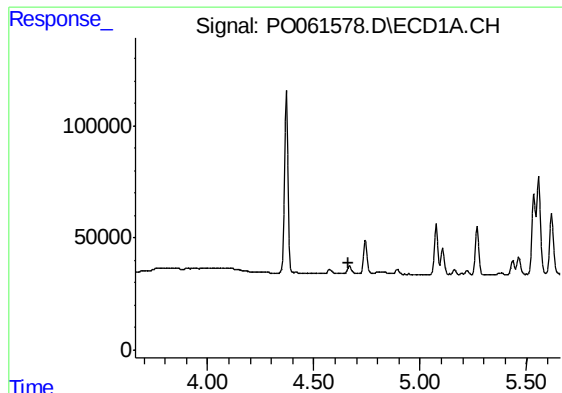

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.660 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

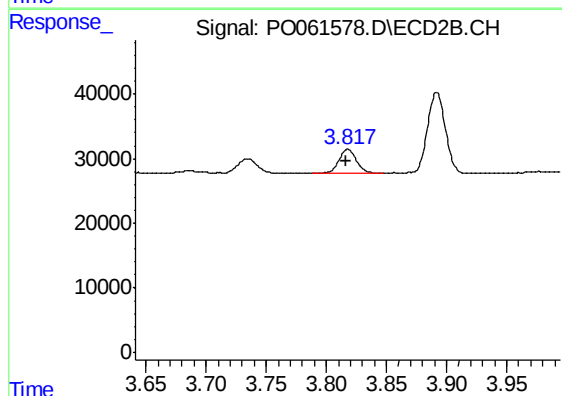


#9 AR-1221-2

R.T.: 3.818 min
Delta R.T.: 0.001 min
Response: 37038
Conc: 120.10 ng/ml

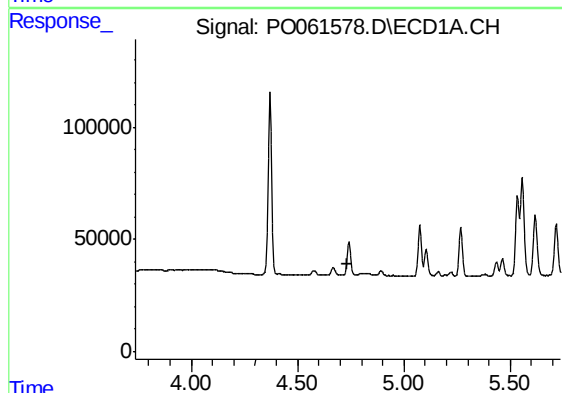


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.736 min
Response: 0
Conc: N.D.

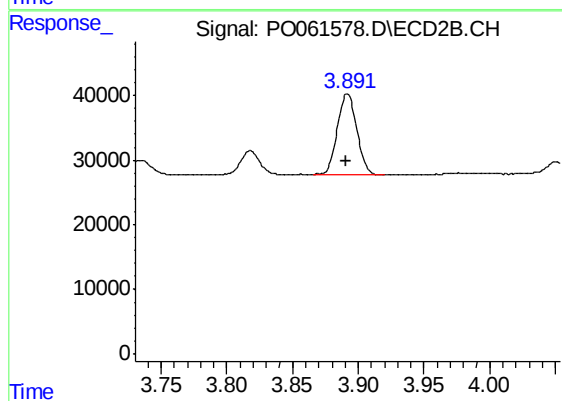

#10 AR-1221-3


R.T.: 3.892 min
Delta R.T.: 0.001 min
Response: 128972
Conc: 141.40 ng/ml

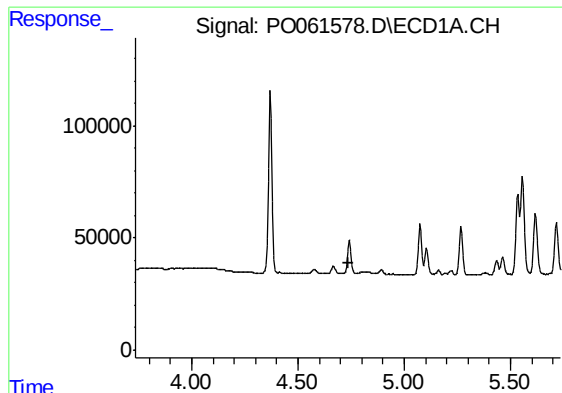

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.735 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

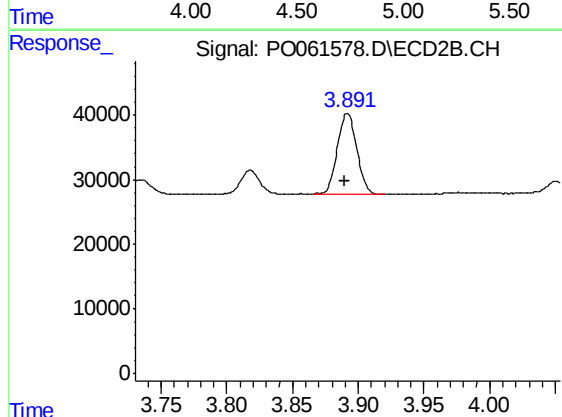


#11 AR-1232-1

R.T.: 3.892 min
Delta R.T.: 0.002 min
Response: 128972
Conc: 114.87 ng/ml

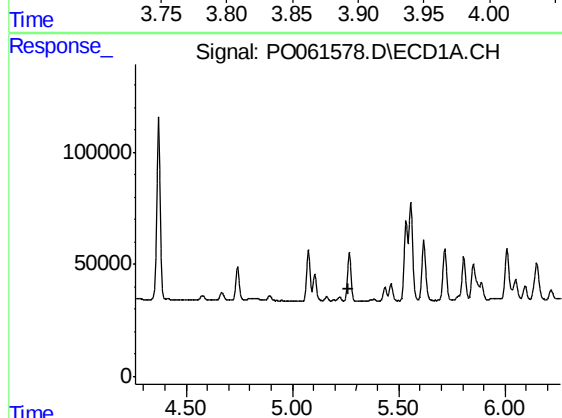


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.261 min
Response: 0
Conc: N.D.

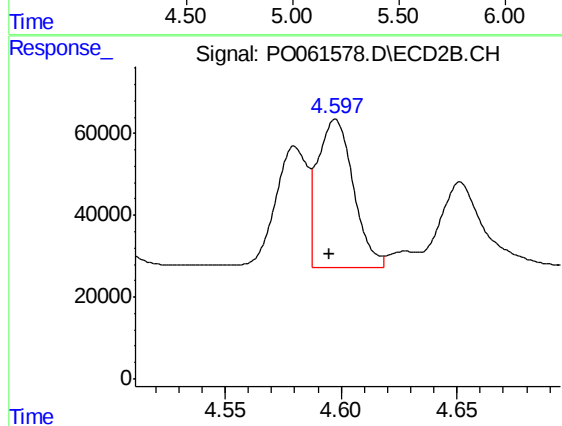

#12 AR-1232-2


R.T.: 4.598 min
Delta R.T.: 0.003 min
Response: 384928
Conc: 315.34 ng/ml



#13 AR-1232-3


R.T.: 0.000 min
Exp R.T. : 5.550 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

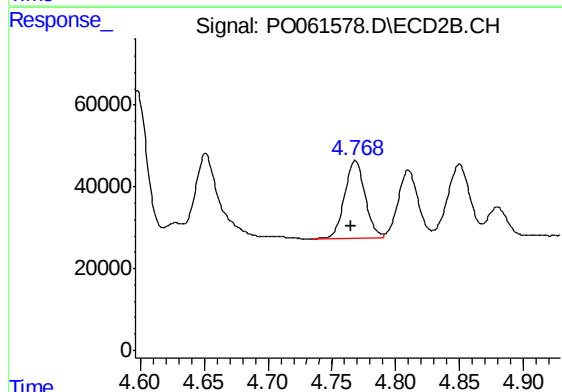


#13 AR-1232-3

R.T.: 4.768 min
Delta R.T.: 0.003 min
Response: 214793
Conc: 325.32 ng/ml




#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 5.710 min
Response: 0
Conc: N.D.

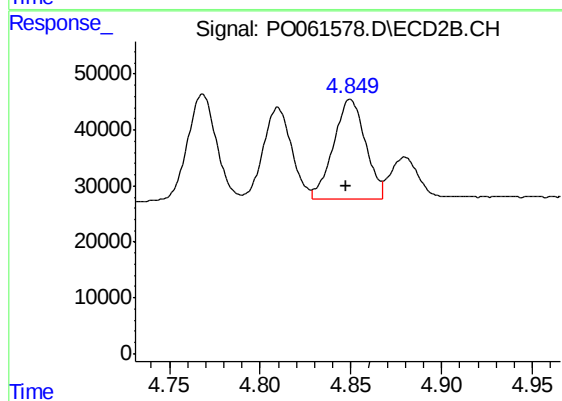

#14 AR-1232-4


R.T.: 4.850 min
Delta R.T.: 0.003 min
Response: 218921
Conc: 347.30 ng/ml



#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.799 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

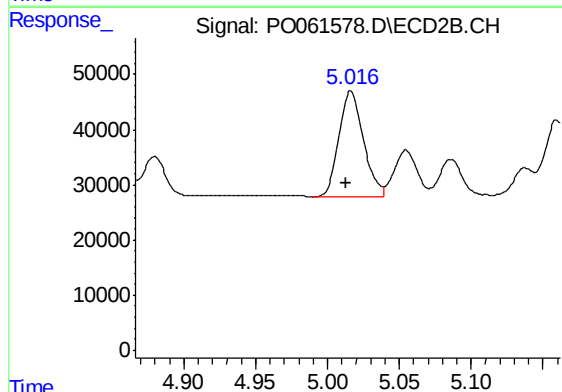


#15 AR-1232-5

R.T.: 5.016 min
Delta R.T.: 0.003 min
Response: 226995
Conc: 330.82 ng/ml




#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 5.528 min
Response: 0
Conc: N.D.

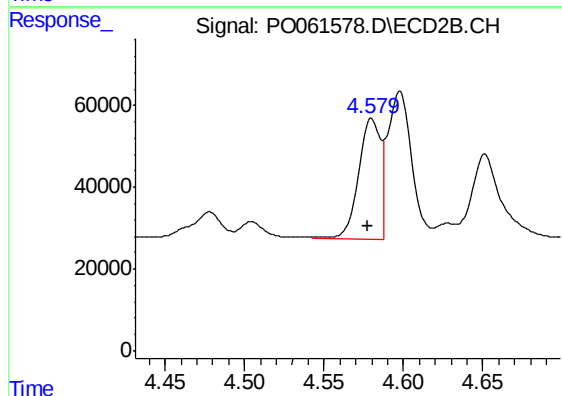

#16 AR-1242-1


R.T.: 4.580 min
Delta R.T.: 0.002 min
Response: 287498
Conc: 280.62 ng/ml



#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.550 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

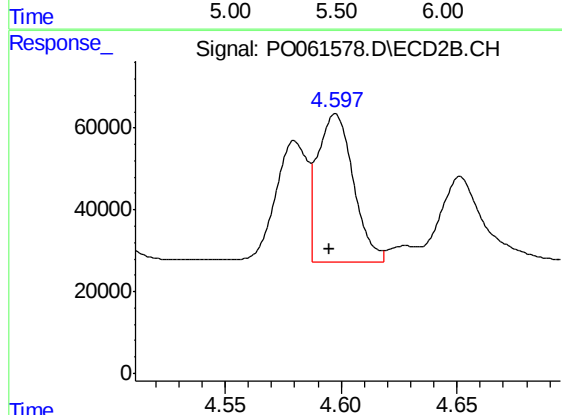


#17 AR-1242-2

R.T.: 4.598 min
Delta R.T.: 0.003 min
Response: 384928
Conc: 272.96 ng/ml

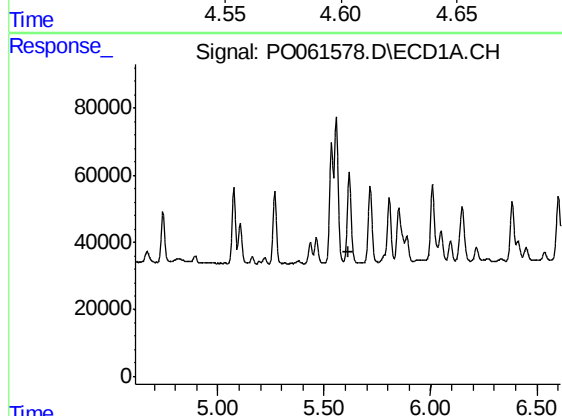


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.612 min
Response: 0
Conc: N.D.

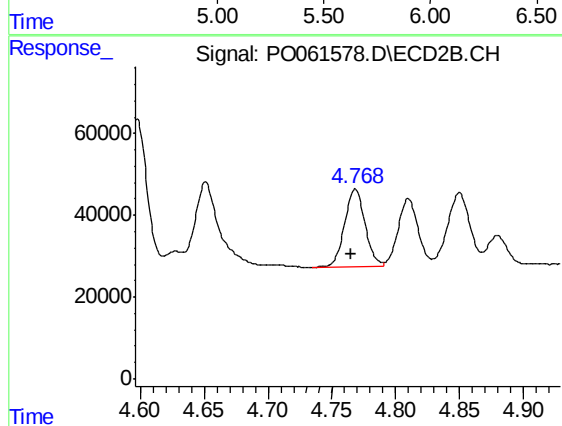

#18 AR-1242-3


R.T.: 4.768 min
Delta R.T.: 0.003 min
Response: 214793
Conc: 275.06 ng/ml

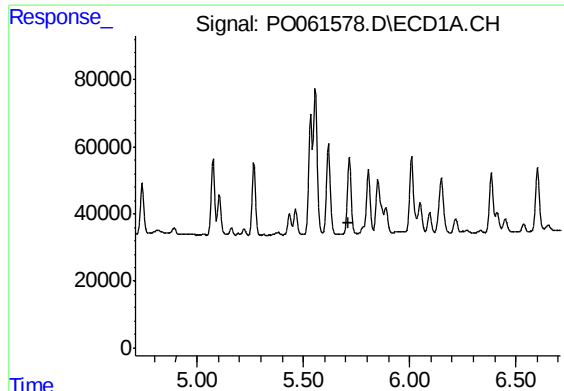

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T. : 5.710 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

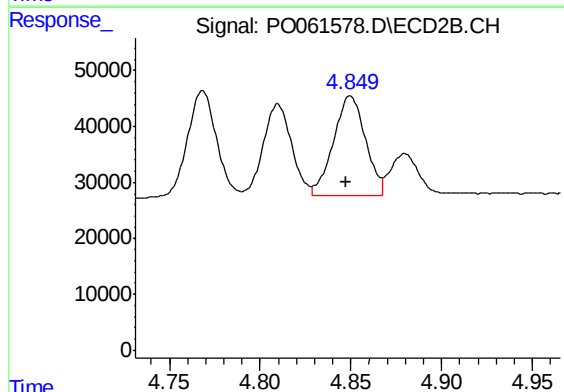


#19 AR-1242-4

R.T.: 4.850 min
Delta R.T.: 0.002 min
Response: 218921
Conc: 266.78 ng/ml

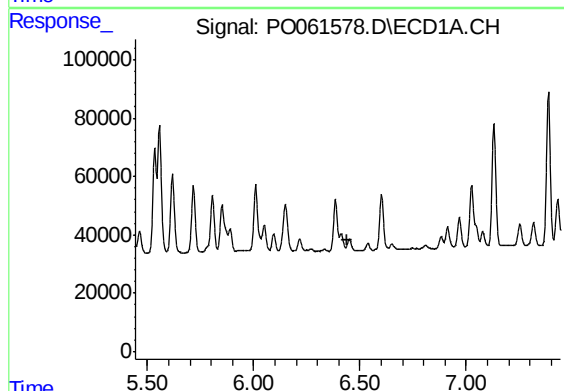


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

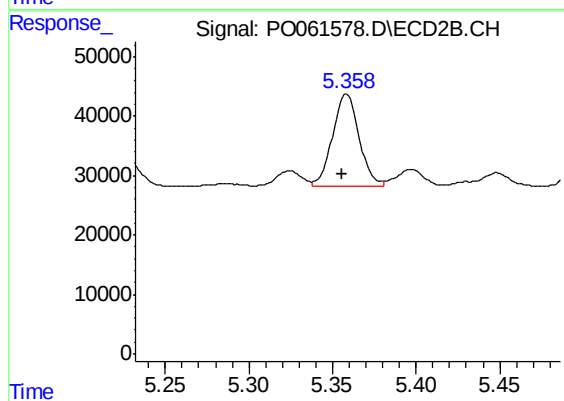

#20 AR-1242-5


R.T.: 5.358 min
Delta R.T.: 0.003 min
Response: 172617
Conc: 161.14 ng/ml



#21 AR-1248-1


R.T.: 0.000 min
Exp R.T. : 5.528 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

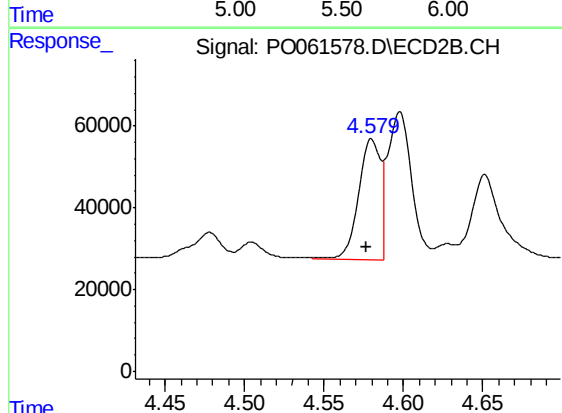


#21 AR-1248-1

R.T.: 4.580 min
Delta R.T.: 0.003 min
Response: 287498
Conc: 321.29 ng/ml

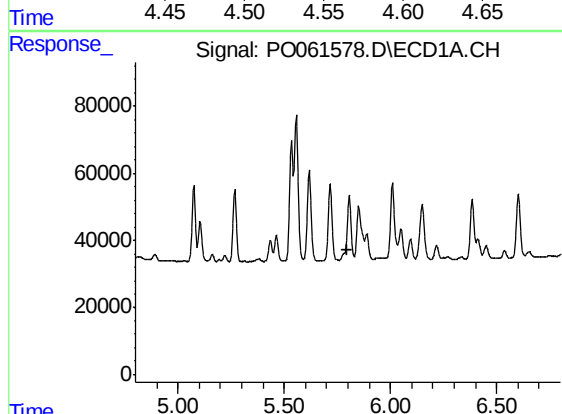


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 5.800 min
Response: 0
Conc: N.D.

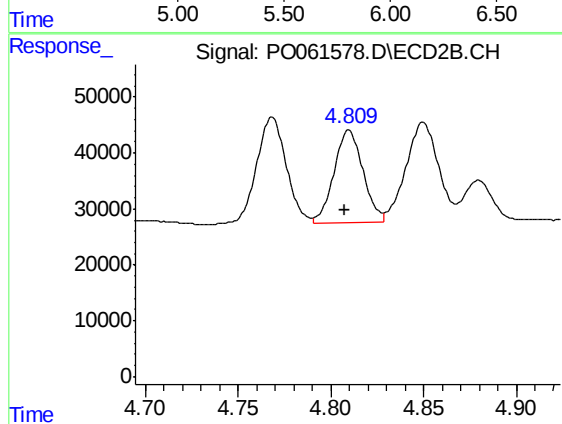

#22 AR-1248-2


R.T.: 4.810 min
Delta R.T.: 0.002 min
Response: 181776
Conc: 154.27 ng/ml

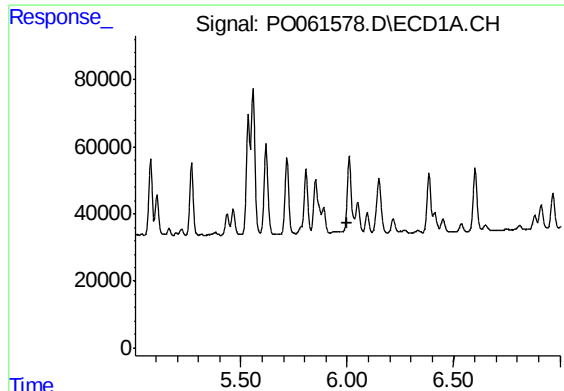

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 6.003 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

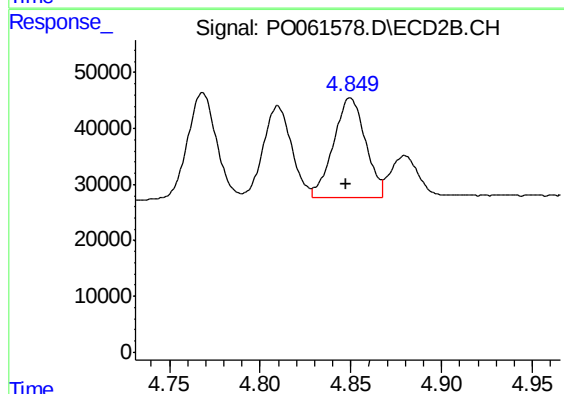


#23 AR-1248-3

R.T.: 4.850 min
Delta R.T.: 0.003 min
Response: 218921
Conc: 176.37 ng/ml

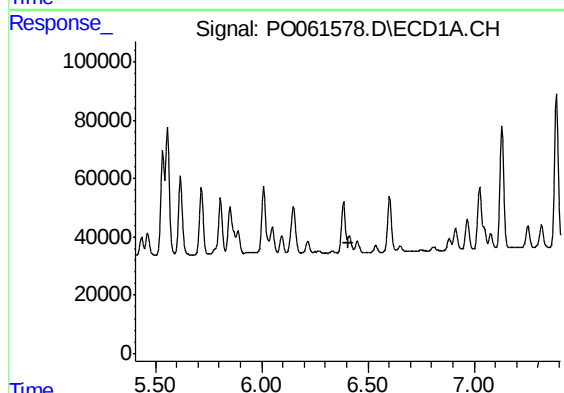


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 6.406 min
Response: 0
Conc: N.D.

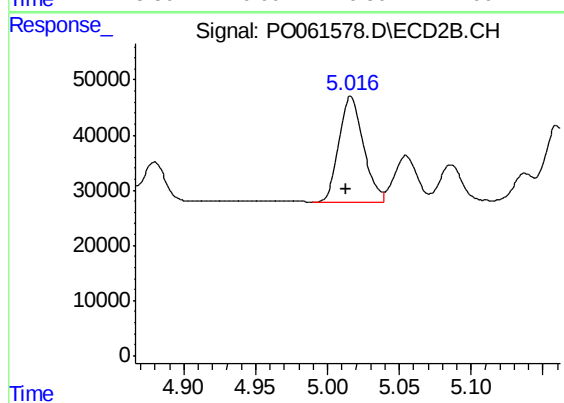

#24 AR-1248-4


R.T.: 5.016 min
Delta R.T.: 0.003 min
Response: 226995
Conc: 151.00 ng/ml



#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 6.444 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

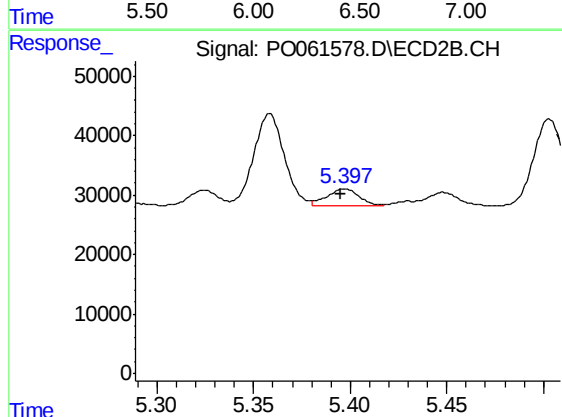


#25 AR-1248-5

R.T.: 5.397 min
Delta R.T.: 0.002 min
Response: 33283
Conc: 21.69 ng/ml

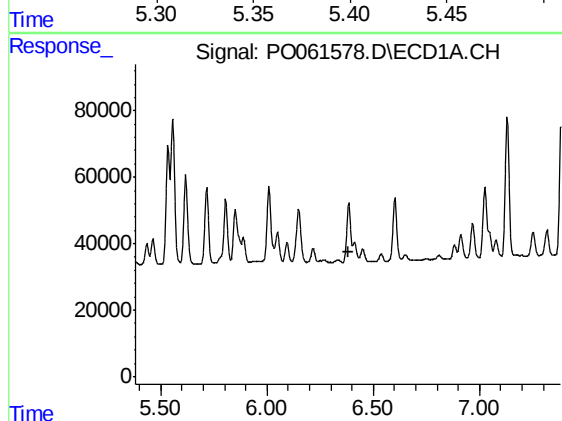


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.381 min
Response: 0
Conc: N.D.

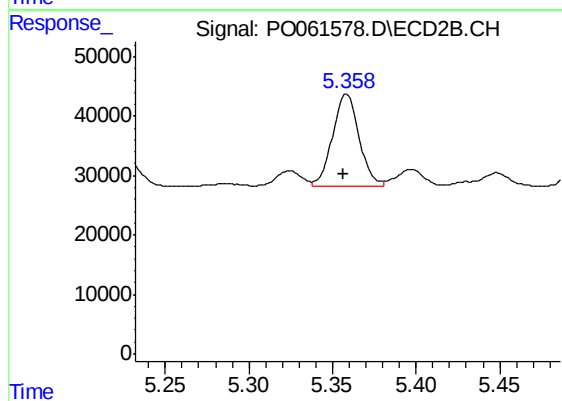

#26 AR-1254-1


R.T.: 5.358 min
Delta R.T.: 0.002 min
Response: 172617
Conc: 78.70 ng/ml

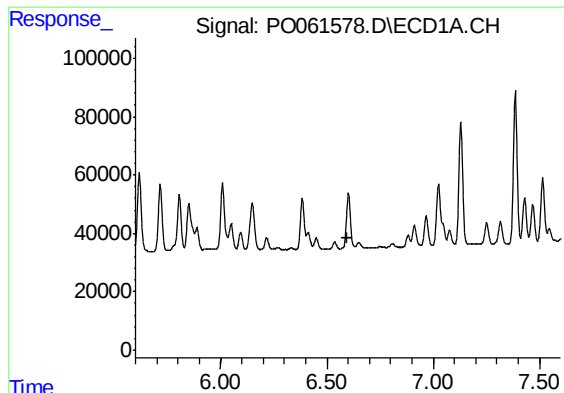

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 6.599 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

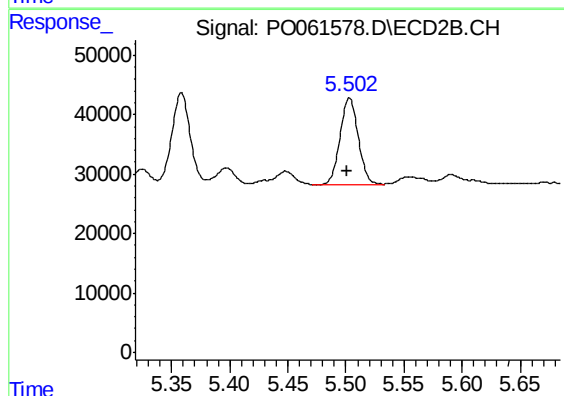


#27 AR-1254-2

R.T.: 5.503 min
Delta R.T.: 0.002 min
Response: 158414
Conc: 80.80 ng/ml

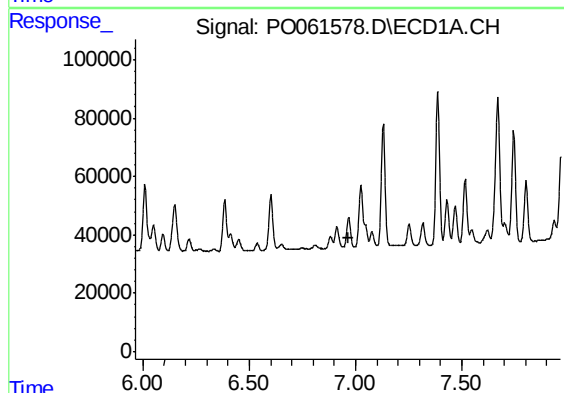


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T.: 6.964 min
Response: 0
Conc: N.D.

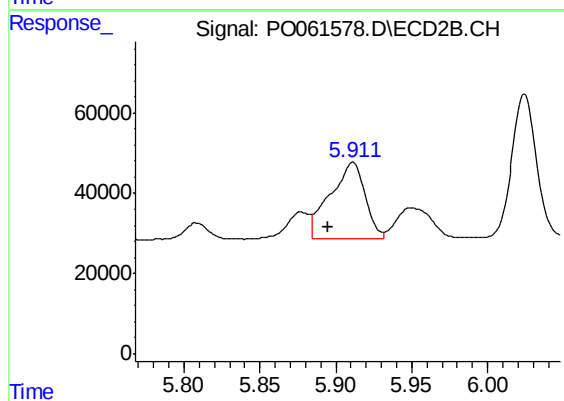

#28 AR-1254-3


R.T.: 5.911 min
Delta R.T.: 0.016 min
Response: 303939
Conc: 95.47 ng/ml

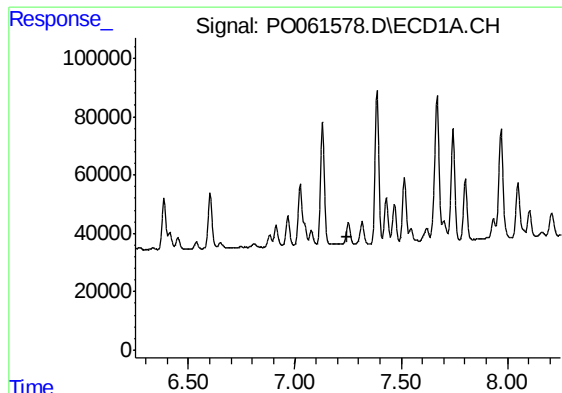

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 7.250 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

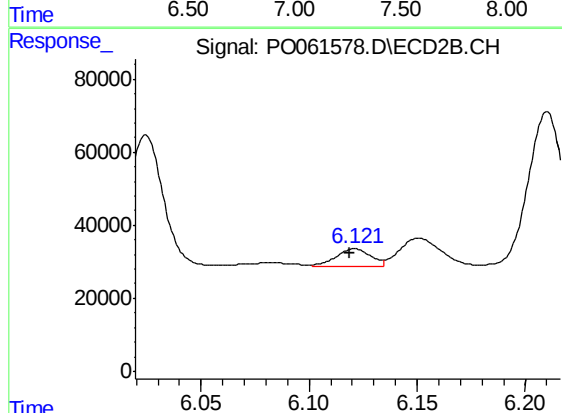


#29 AR-1254-4

R.T.: 6.121 min
Delta R.T.: 0.002 min
Response: 52726
Conc: 25.99 ng/ml

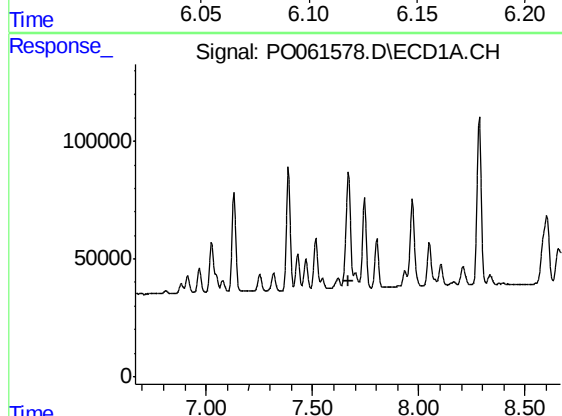


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.667 min
Response: 0
Conc: N.D.

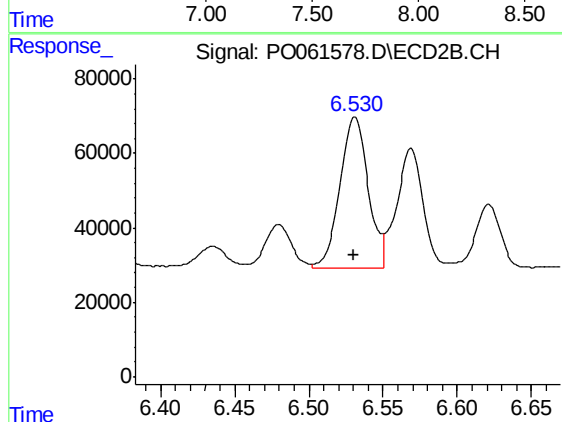

#30 AR-1254-5


R.T.: 6.531 min
Delta R.T.: 0.000 min
Response: 534745
Conc: 189.06 ng/ml



#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

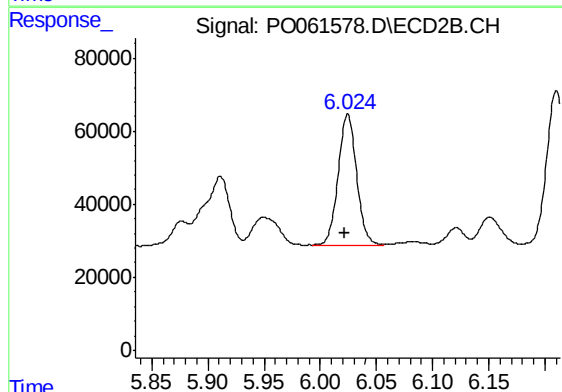


#31 AR-1260-1

R.T.: 6.025 min
Delta R.T.: 0.003 min
Response: 414696
Conc: 203.30 ng/ml

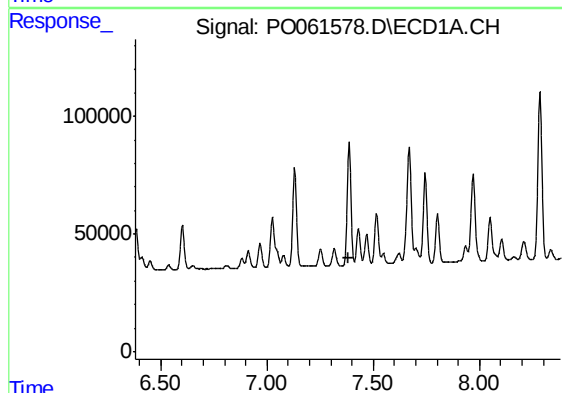


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.381 min
Response: 0
Conc: N.D.

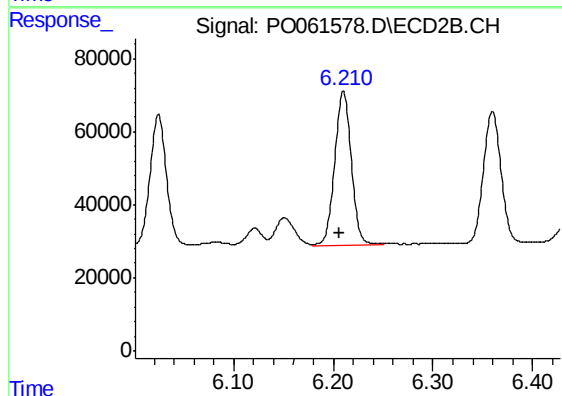

#32 AR-1260-2


R.T.: 6.210 min
Delta R.T.: 0.003 min
Response: 491848
Conc: 204.79 ng/ml

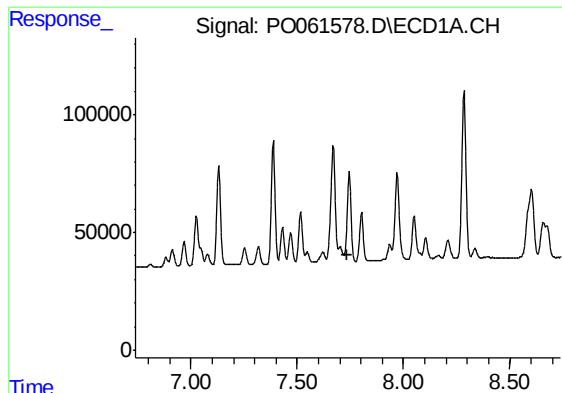

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.738 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

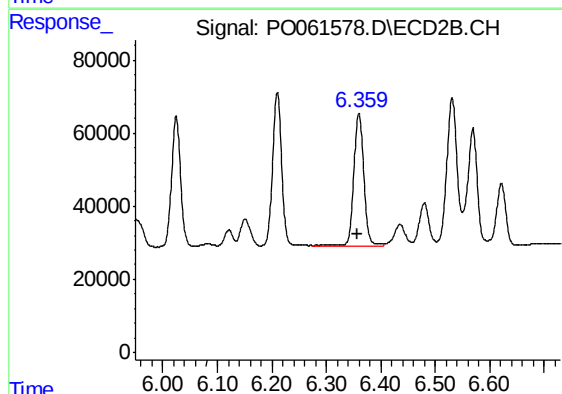


#33 AR-1260-3

R.T.: 6.360 min
Delta R.T.: 0.003 min
Response: 472749
Conc: 209.82 ng/ml

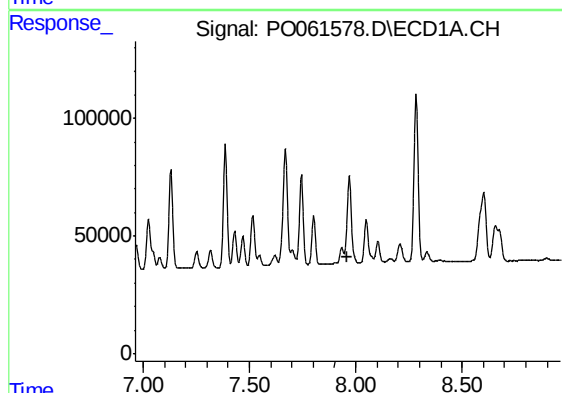


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.963 min
Response: 0
Conc: N.D.

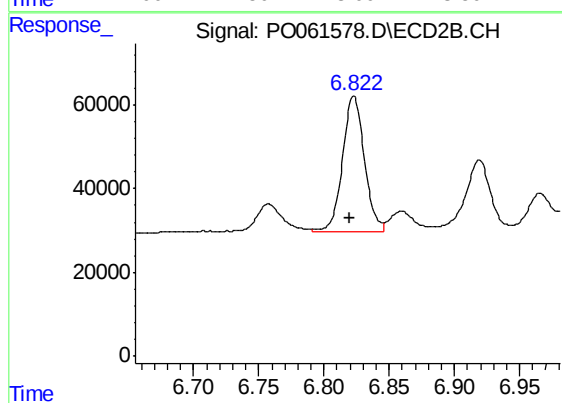

#34 AR-1260-4


R.T.: 6.823 min
Delta R.T.: 0.003 min
Response: 380219
Conc: 205.95 ng/ml



#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.277 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

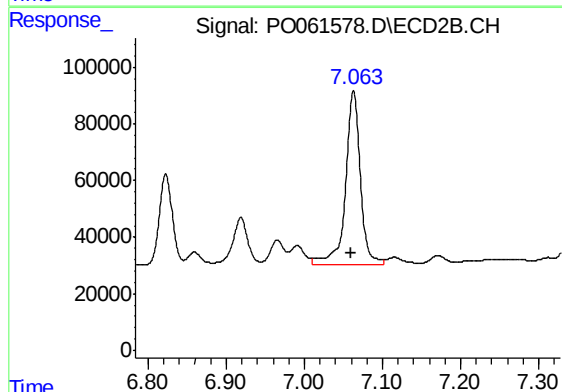


#35 AR-1260-5

R.T.: 7.063 min
Delta R.T.: 0.004 min
Response: 826452
Conc: 212.26 ng/ml




#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.740 min
Response: 0
Conc: N.D.

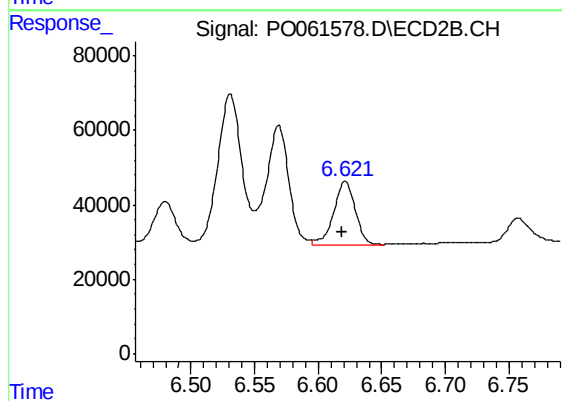

#36 AR-1262-1


R.T.: 6.621 min
Delta R.T.: 0.002 min
Response: 199874
Conc: 163.75 ng/ml



#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 8.279 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

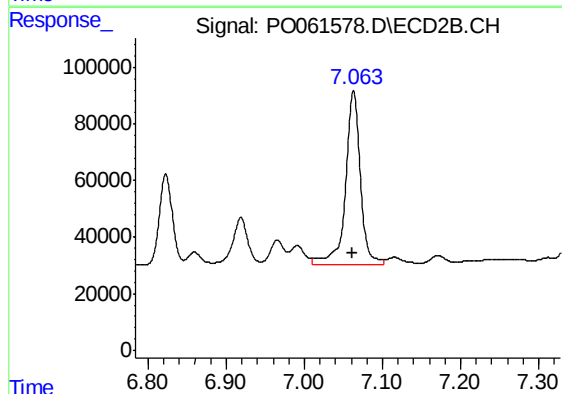


#37 AR-1262-2

R.T.: 7.063 min
Delta R.T.: 0.002 min
Response: 826452
Conc: 179.74 ng/ml




#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.581 min
Response: 0
Conc: N.D.

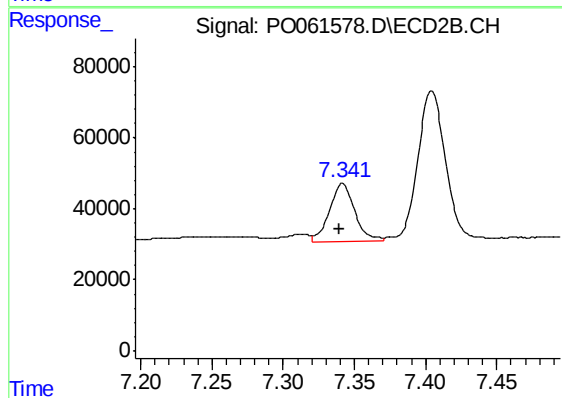

#38 AR-1262-3


R.T.: 7.342 min
Delta R.T.: 0.002 min
Response: 201977
Conc: 107.22 ng/ml



#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.669 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

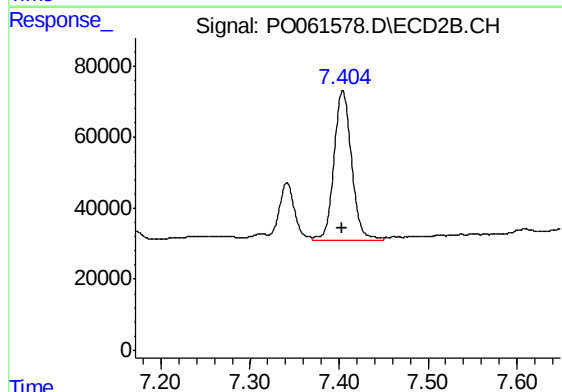


#39 AR-1262-4

R.T.: 7.404 min
Delta R.T.: 0.000 min
Response: 584303
Conc: 173.86 ng/ml




#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.307 min
Response: 0
Conc: N.D.

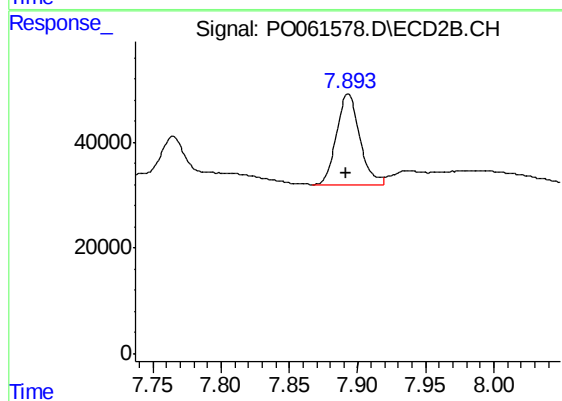

#40 AR-1262-5


R.T.: 7.893 min
Delta R.T.: 0.002 min
Response: 207441
Conc: 136.84 ng/ml



#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 8.581 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

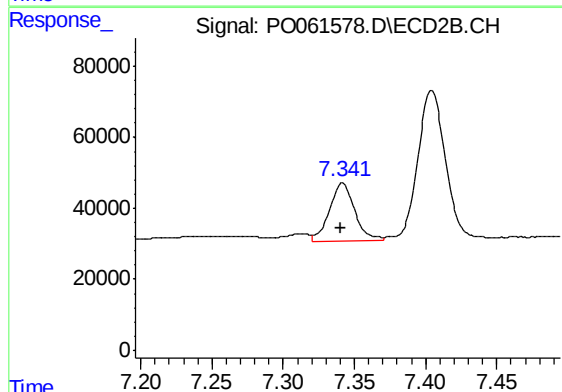


#41 AR-1268-1

R.T.: 7.342 min
Delta R.T.: 0.001 min
Response: 201977
Conc: 41.82 ng/ml




#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.674 min
Response: 0
Conc: N.D.

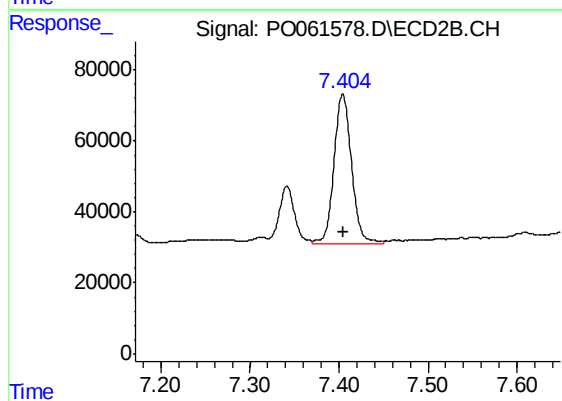

#42 AR-1268-2


R.T.: 7.404 min
Delta R.T.: 0.000 min
Response: 584303
Conc: 135.57 ng/ml



#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 8.894 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

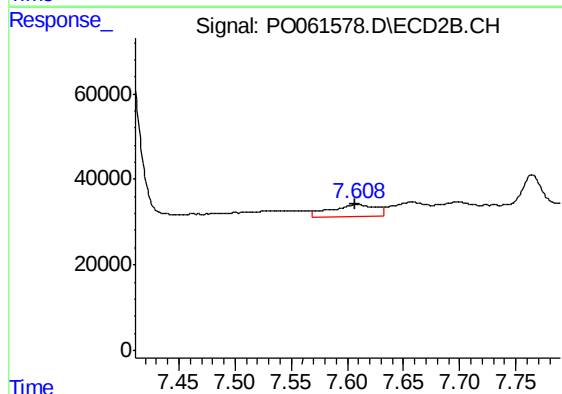


#43 AR-1268-3

R.T.: 7.609 min
Delta R.T.: 0.002 min
Response: 77805
Conc: 21.71 ng/ml




#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.309 min
Response: 0
Conc: N.D.

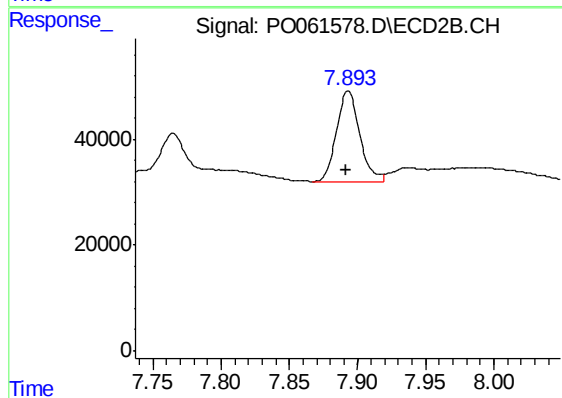

#44 AR-1268-4


R.T.: 7.893 min
Delta R.T.: 0.002 min
Response: 207441
Conc: 128.89 ng/ml

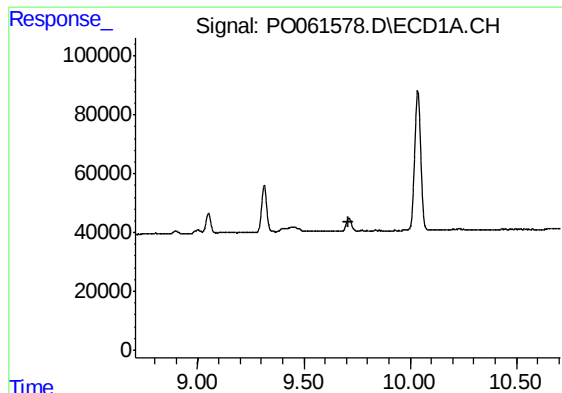

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.708 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDOC-WATER-03

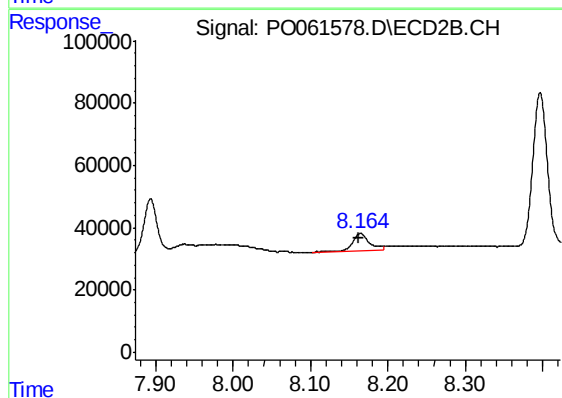

#45 AR-1268-5

R.T.: 8.165 min
Delta R.T.: 0.002 min
Response: 85220
Conc: 8.47 ng/ml