

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100219\
 Data File : P0061589.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Oct 2019 16:17
 Operator : HP/AJ
 Sample : PB123553BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB123553BL

Manual Integrations
 APPROVED

Ankita
 10/3/2019 12:04:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 01:01:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.380	3.529	1182057	875455	28.821	27.071
2)	SA Decachlor...	10.051	8.403	1144204	770868	24.569m	23.810

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100219\
Data File : PO061589.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Oct 2019 16:17
Operator : HP/AJ
Sample : PB123553BL
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB123553BL


Manual Integrations
APPROVED

Ankita
10/3/2019 12:04:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 01:01:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

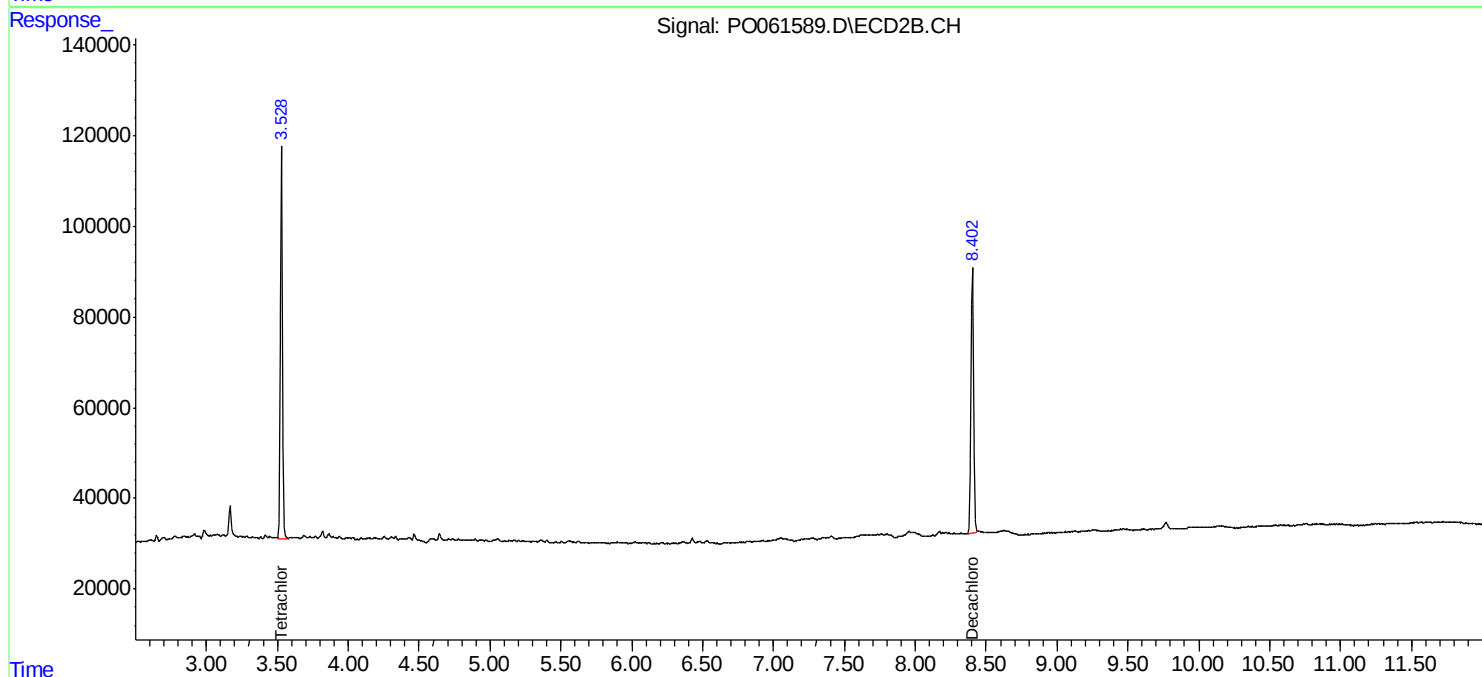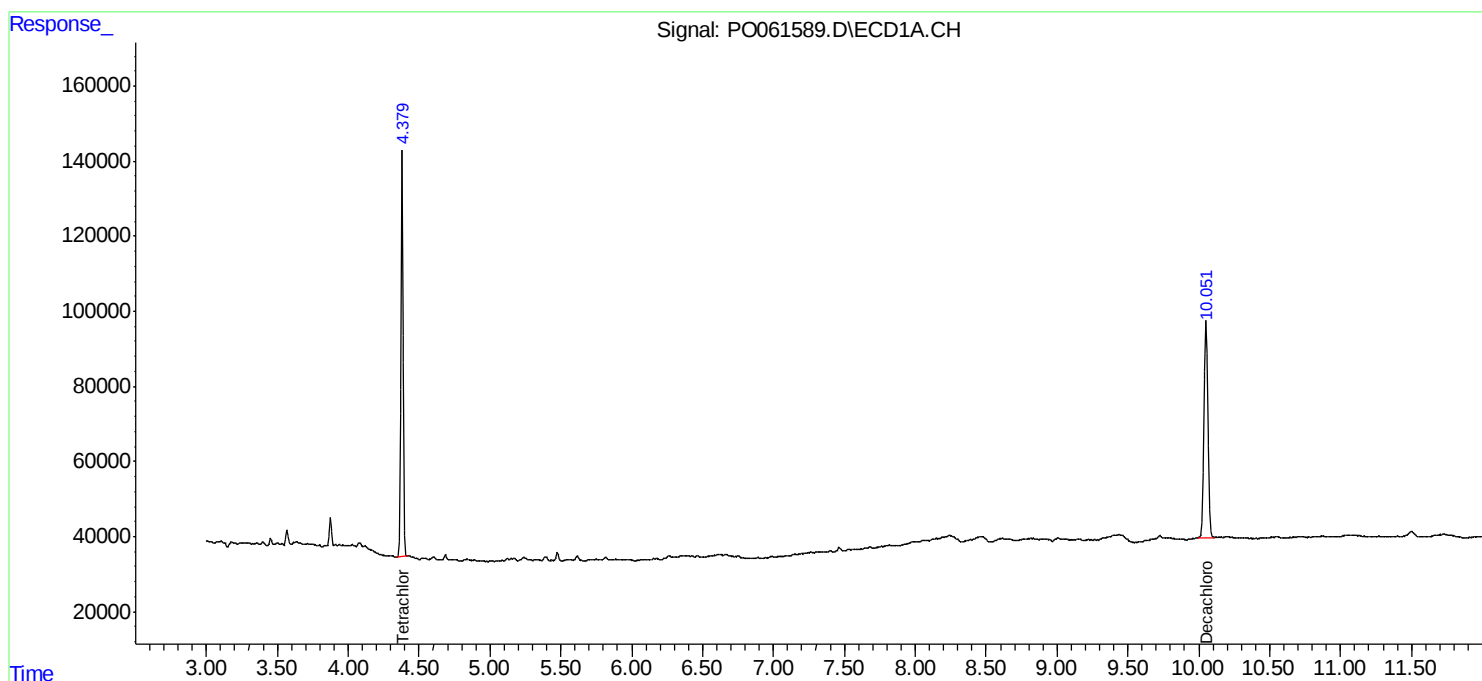

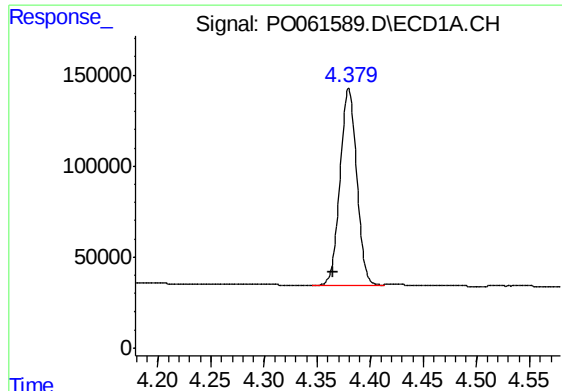


#1 Tetrachloro-m-xylene

R.T.: 4.380 min
Delta R.T.: 0.015 min
Response: 1182057
Conc: 28.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB123553BL


Manual Integrations
APPROVED

Ankita
10/3/2019 12:04:48 PM

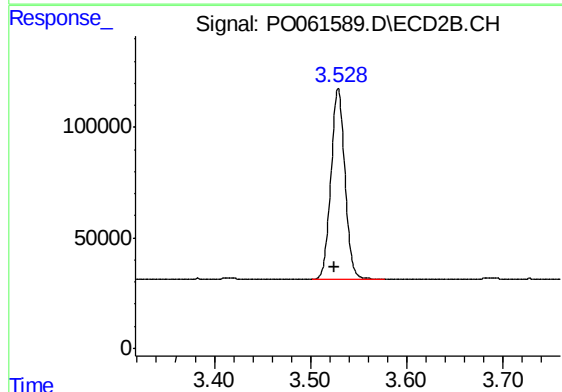


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: 0.003 min
Response: 875455
Conc: 27.07 ng/ml

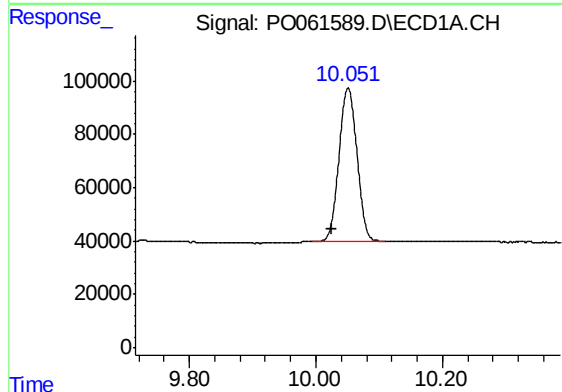

#2 Decachlorobiphenyl

R.T.: 10.051 min
Delta R.T.: 0.026 min
Response: 1144204
Conc: 24.57 ng/ml m

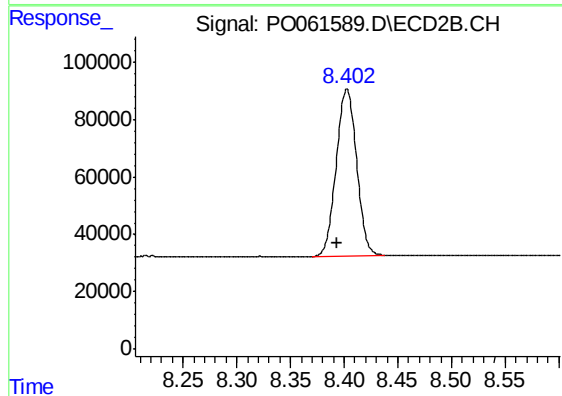

#2 Decachlorobiphenyl

R.T.: 8.403 min
Delta R.T.: 0.009 min
Response: 770868
Conc: 23.81 ng/ml