

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100219\
Data File : P0061613.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Oct 2019 00:26
Operator : HP/AJ
Sample : K5137-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-047-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 01:12:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.368	3.528	1175010	859730	28.649	26.585
2)	SA Decachlor...	10.032	8.395	869496	581237	18.670	17.953

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100219\
Data File : PO061613.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Oct 2019 00:26
Operator : HP/AJ
Sample : K5137-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-047-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 01:12:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

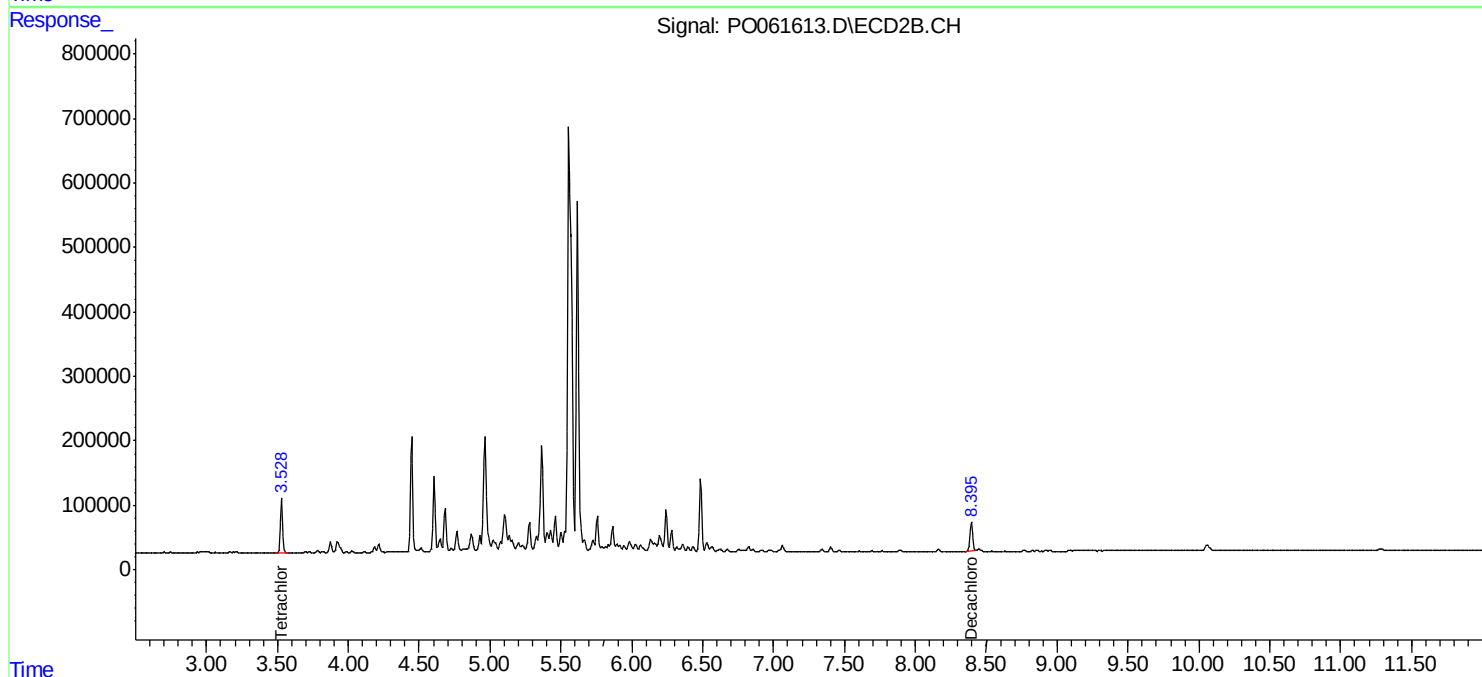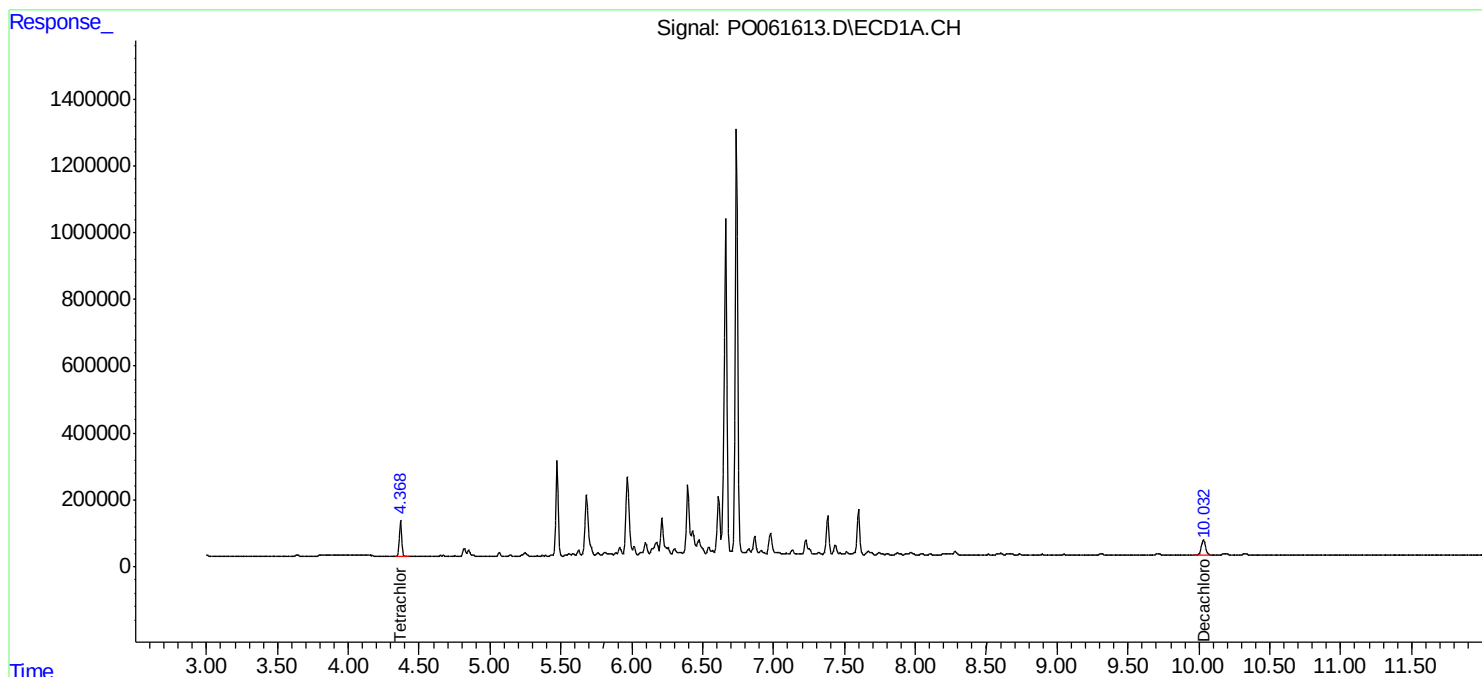

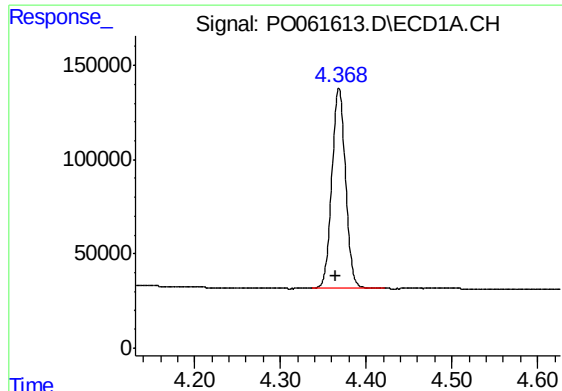

#1 Tetrachloro-m-xylene

R.T.: 4.368 min
Delta R.T.: 0.003 min
Response: 1175010
Conc: 28.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-047-A

#1 Tetrachloro-m-xylene

R.T.: 3.528 min
Delta R.T.: 0.003 min
Response: 859730
Conc: 26.58 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.032 min
Delta R.T.: 0.007 min
Response: 869496
Conc: 18.67 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.395 min
Delta R.T.: 0.000 min
Response: 581237
Conc: 17.95 ng/ml