

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100219\
 Data File : P0061614.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Oct 2019 00:42
 Operator : HP/AJ
 Sample : K5137-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-GF-02-047-B

Manual Integrations
 APPROVED

Ankita
 10/3/2019 12:05:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 04:29:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.367	3.527	1044700	778340	25.472	24.068
2)	SA Decachlor...	10.030	8.394	730217	502375	15.680	15.517m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100219\
Data File : PO061614.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Oct 2019 00:42
Operator : HP/AJ
Sample : K5137-03
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-GF-02-047-B


Manual Integrations
APPROVED

Ankita
10/3/2019 12:05:28 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 04:29:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

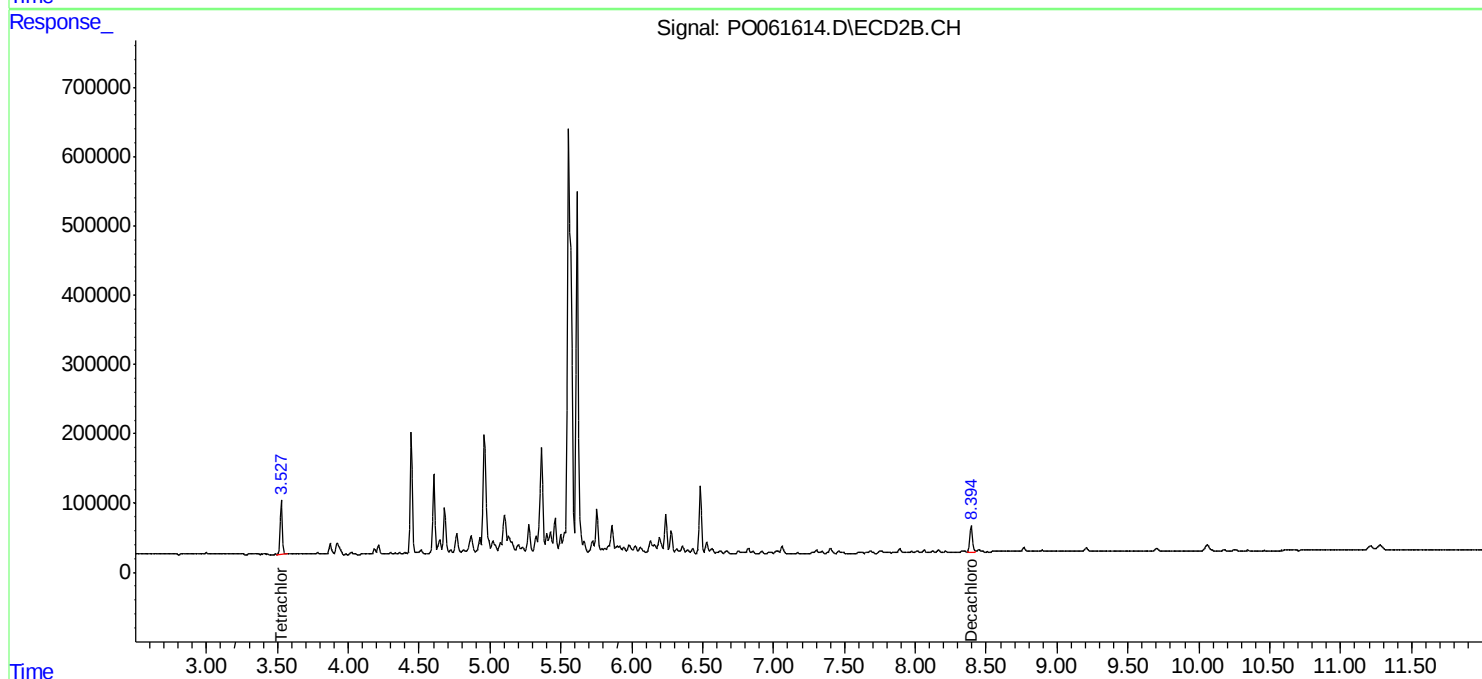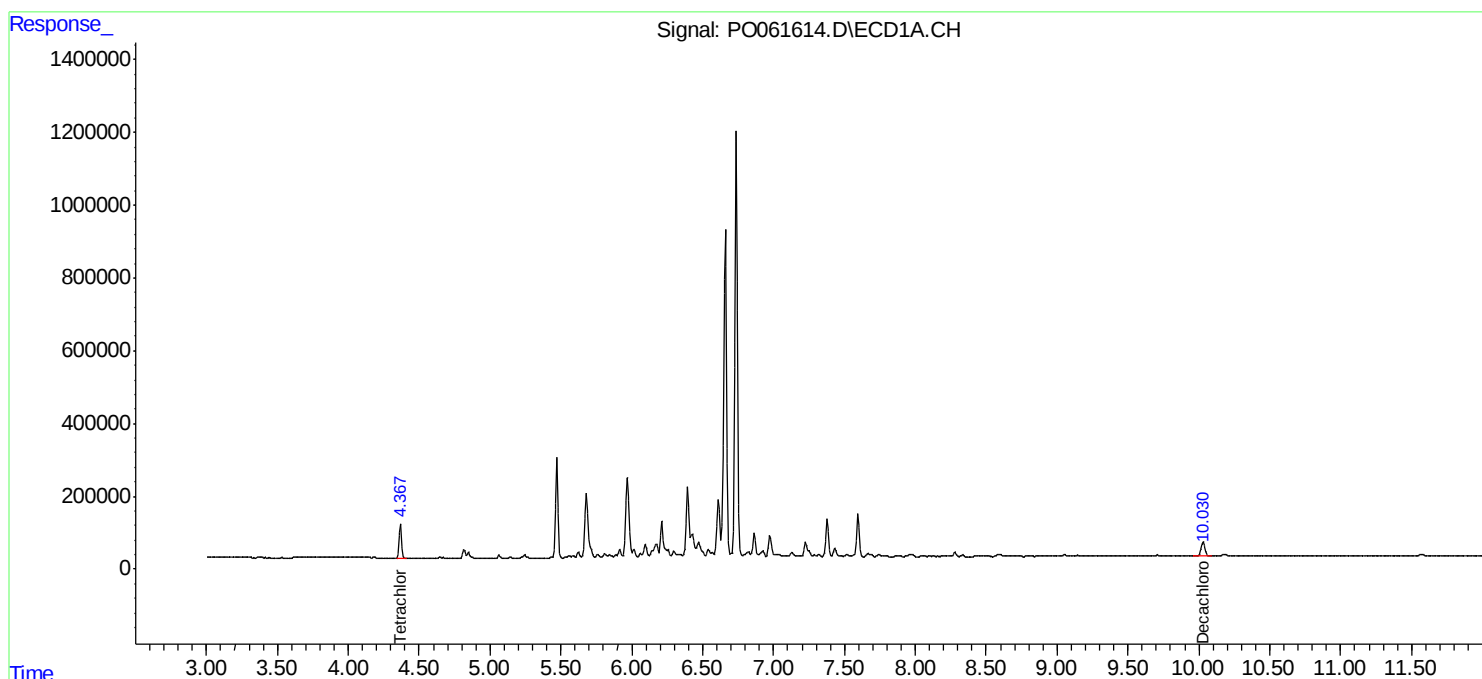

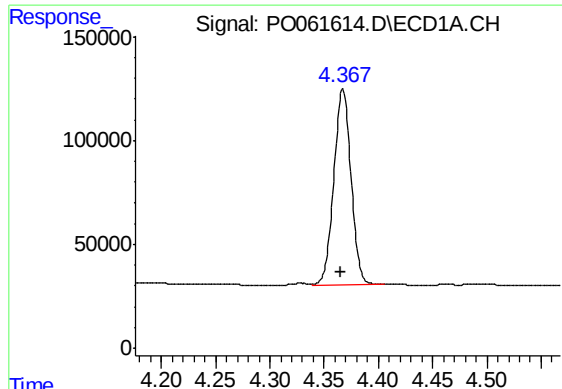


#1 Tetrachloro-m-xylene

R.T.: 4.367 min
Delta R.T.: 0.002 min
Response: 1044700
Conc: 25.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-047-B


Manual Integrations
APPROVED

Ankita
10/3/2019 12:05:28 PM

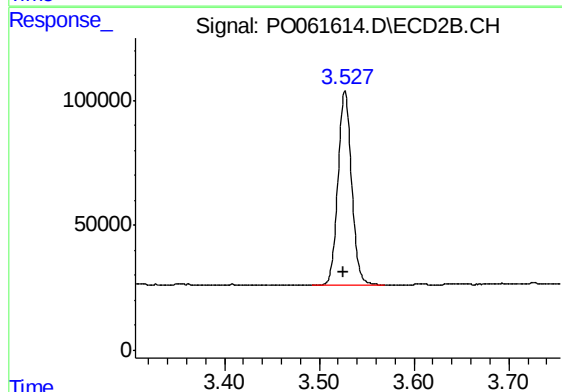


#1 Tetrachloro-m-xylene

R.T.: 3.527 min
Delta R.T.: 0.002 min
Response: 778340
Conc: 24.07 ng/ml

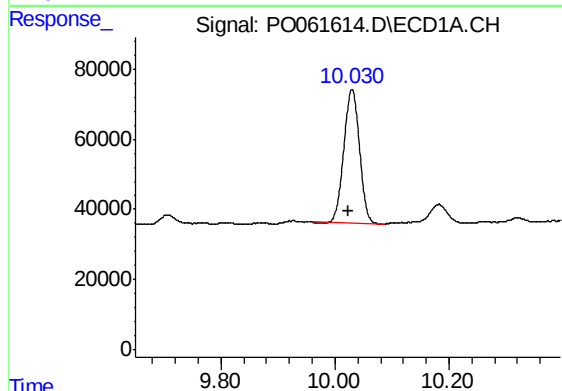

#2 Decachlorobiphenyl

R.T.: 10.030 min
Delta R.T.: 0.005 min
Response: 730217
Conc: 15.68 ng/ml

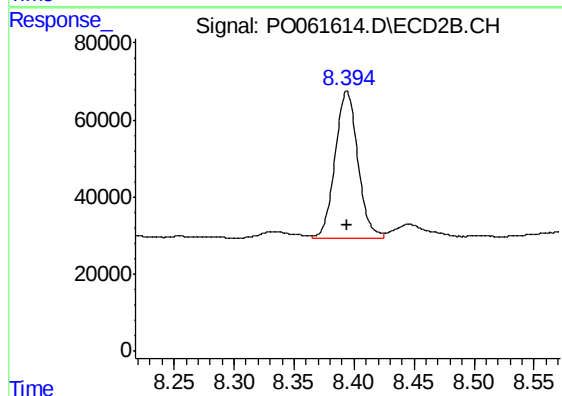

#2 Decachlorobiphenyl

R.T.: 8.394 min
Delta R.T.: 0.000 min
Response: 502375
Conc: 15.52 ng/ml m