

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100319\
 Data File : P0061640.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Oct 2019 13:43
 Operator : HP/AJ
 Sample : K5176-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 40166

Manual Integrations
 APPROVED

Ankita
 10/4/2019 5:10:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 14:31:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.358	3.518	616629	462061	15.035	14.288
2) SA Decachlor...	10.012	8.384	574825	547653	12.343m	16.916 #
Target Compounds						
21) L5 AR-1248-1	5.521	4.569	180337	148638	153.502	166.110
22) L5 AR-1248-2	5.793	4.800	220566	160759	130.732	136.437
23) L5 AR-1248-3	5.996	4.839	340723	175859	182.318m	141.676
24) L5 AR-1248-4	6.397	5.006	430679	192118	182.272m	127.798 #
25) L5 AR-1248-5	6.436	5.388	427983	183540	188.752m	119.635m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100319\
Data File : PO061640.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Oct 2019 13:43
Operator : HP/AJ
Sample : K5176-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
40166


Manual Integrations
APPROVED

Ankita
10/4/2019 5:10:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 14:31:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

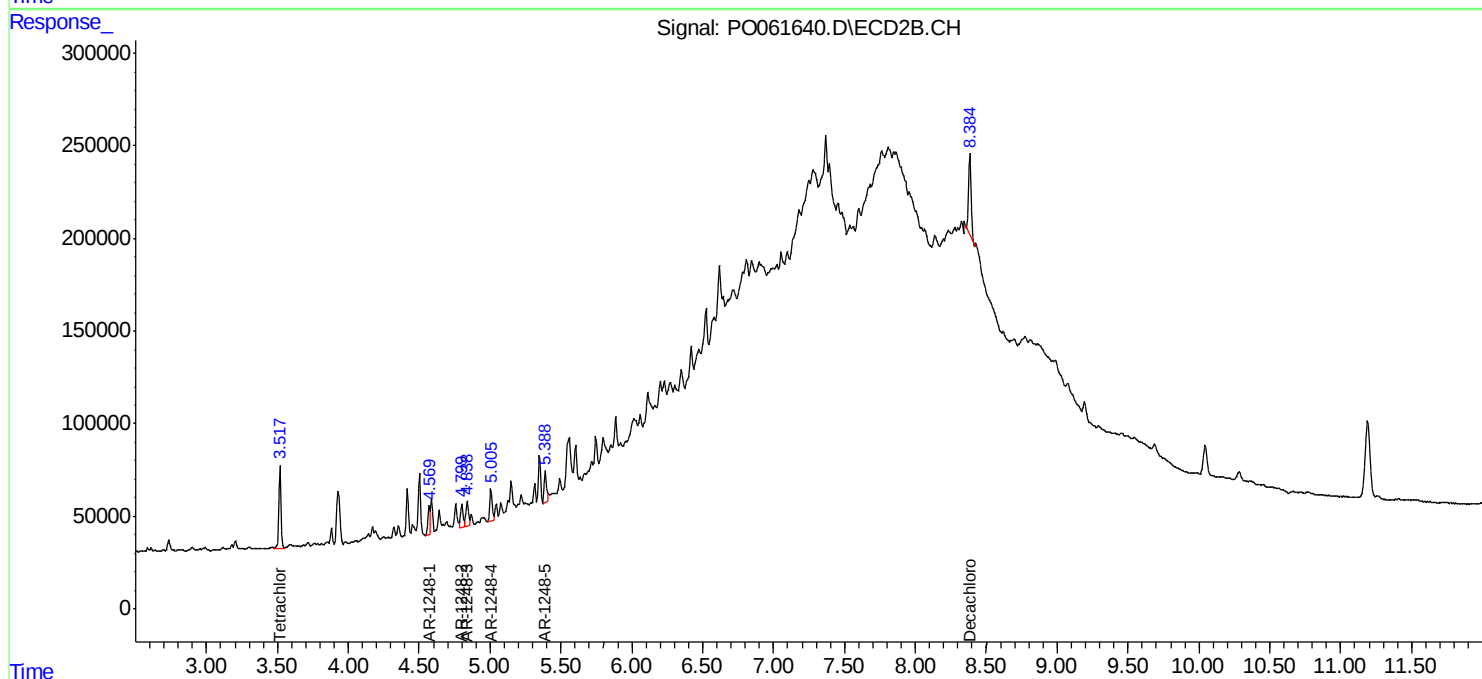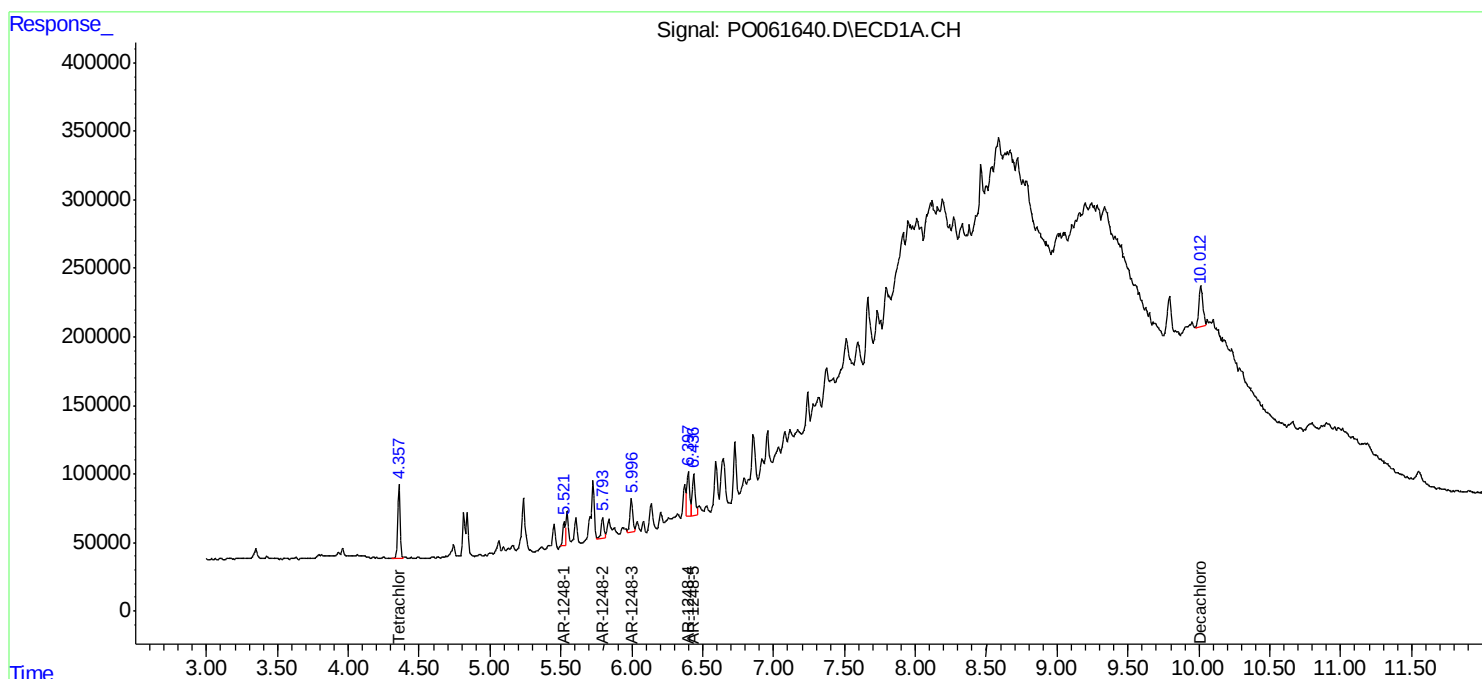

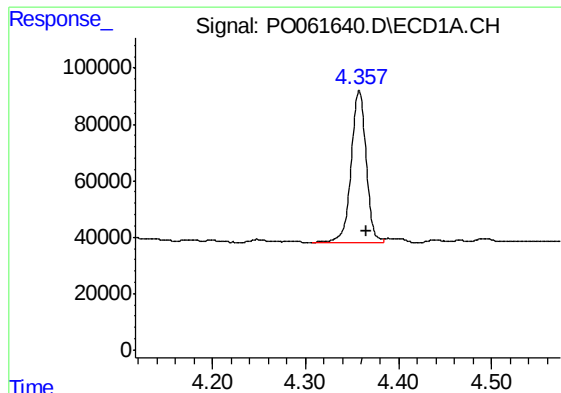


#1 Tetrachloro-m-xylene

R.T.: 4.358 min
Delta R.T.: -0.007 min
Response: 616629
Conc: 15.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
40166


Manual Integrations
APPROVED

Ankita
10/4/2019 5:10:53 PM

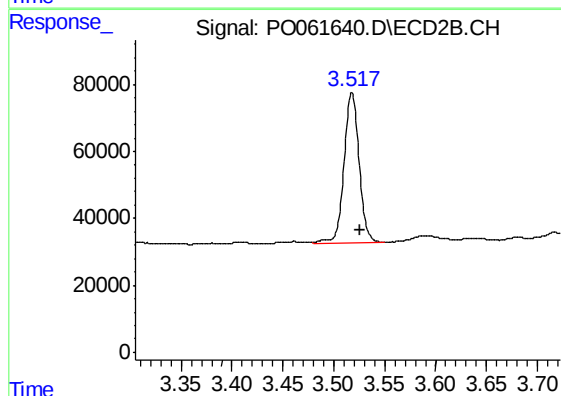


#1 Tetrachloro-m-xylene

R.T.: 3.518 min
Delta R.T.: -0.008 min
Response: 462061
Conc: 14.29 ng/ml

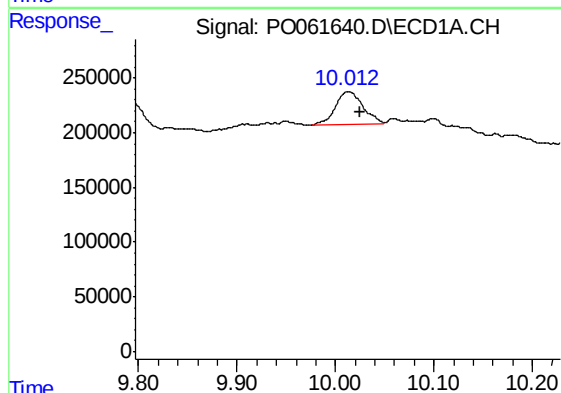


#2 Decachlorobiphenyl

R.T.: 10.012 min
Delta R.T.: -0.013 min
Response: 574825
Conc: 12.34 ng/ml m

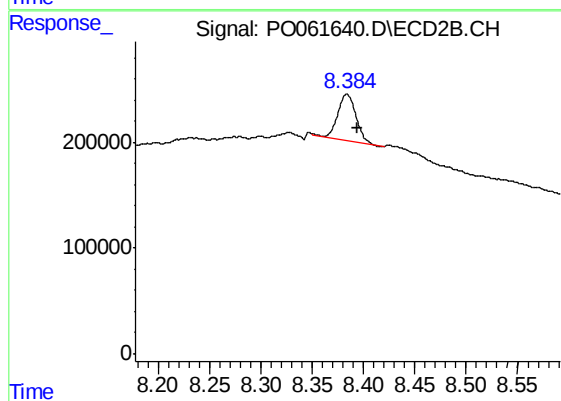

#2 Decachlorobiphenyl

R.T.: 8.384 min
Delta R.T.: -0.010 min
Response: 547653
Conc: 16.92 ng/ml

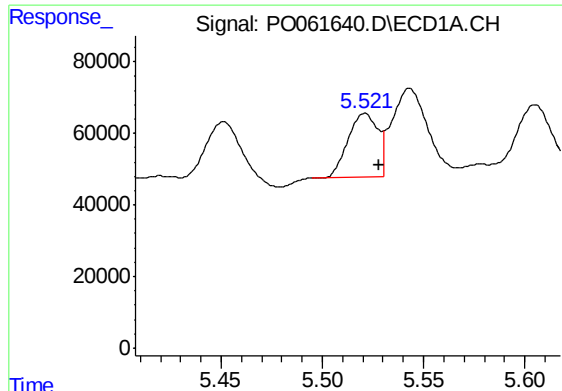


#21 AR-1248-1

R.T.: 5.521 min
Delta R.T.: -0.007 min
Response: 180337
Conc: 153.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
40166


Manual Integrations
APPROVED

Ankita
10/4/2019 5:10:53 PM

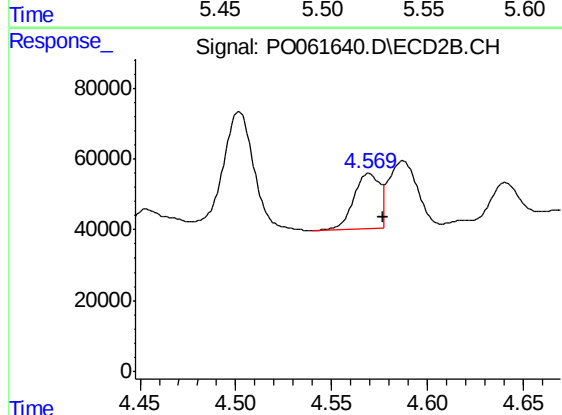


#21 AR-1248-1

R.T.: 4.569 min
Delta R.T.: -0.008 min
Response: 148638
Conc: 166.11 ng/ml

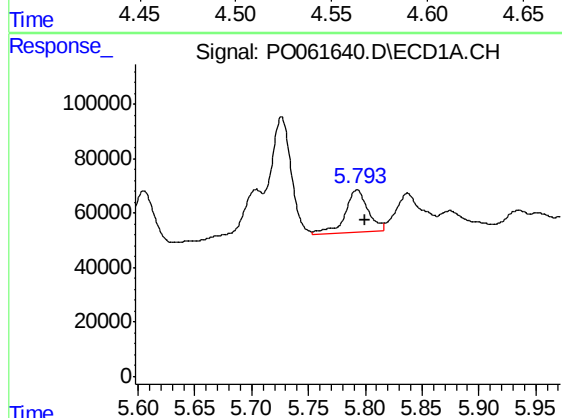


#22 AR-1248-2

R.T.: 5.793 min
Delta R.T.: -0.007 min
Response: 220566
Conc: 130.73 ng/ml

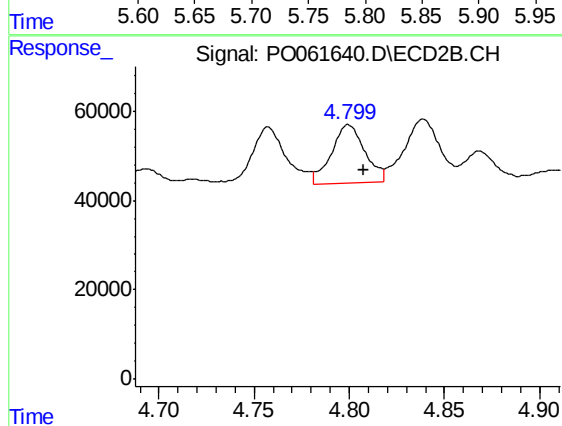

#22 AR-1248-2

R.T.: 4.800 min
Delta R.T.: -0.008 min
Response: 160759
Conc: 136.44 ng/ml

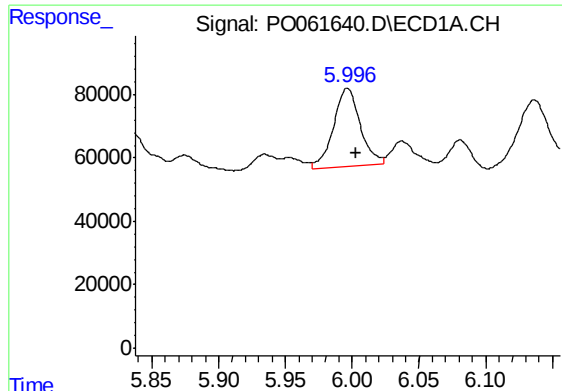


#23 AR-1248-3

R.T.: 5.996 min
Delta R.T.: -0.007 min
Response: 340723
Conc: 182.32 ng/ml m

Instrument :
ECD_O
ClientSampleId :
40166


Manual Integrations
APPROVED

Ankita
10/4/2019 5:10:53 PM

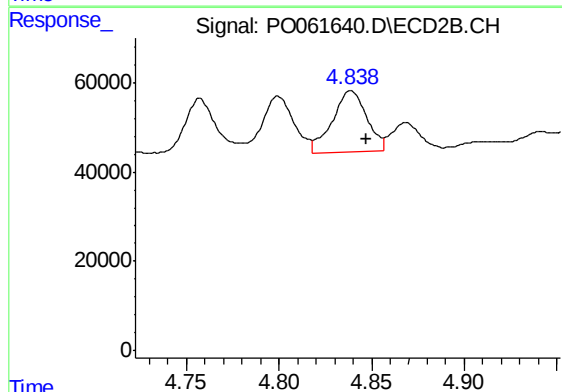


#23 AR-1248-3

R.T.: 4.839 min
Delta R.T.: -0.008 min
Response: 175859
Conc: 141.68 ng/ml

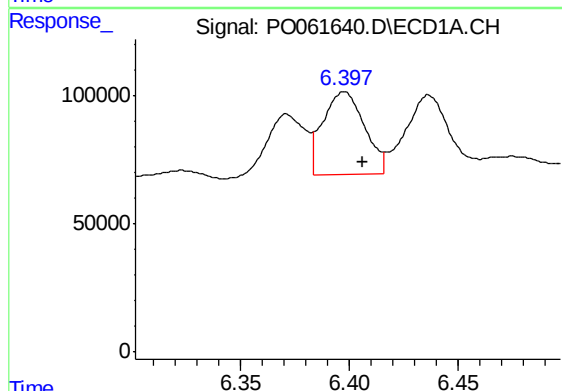


#24 AR-1248-4

R.T.: 6.397 min
Delta R.T.: -0.009 min
Response: 430679
Conc: 182.27 ng/ml m

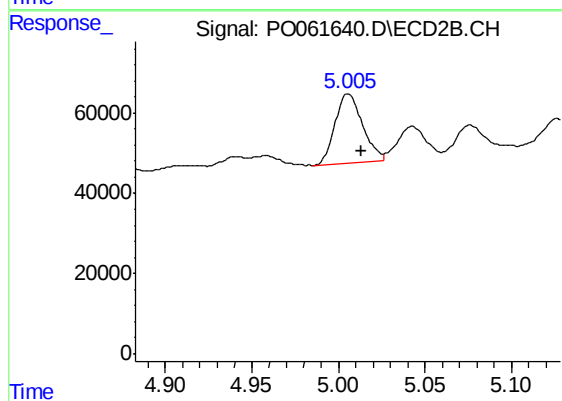

#24 AR-1248-4

R.T.: 5.006 min
Delta R.T.: -0.008 min
Response: 192118
Conc: 127.80 ng/ml

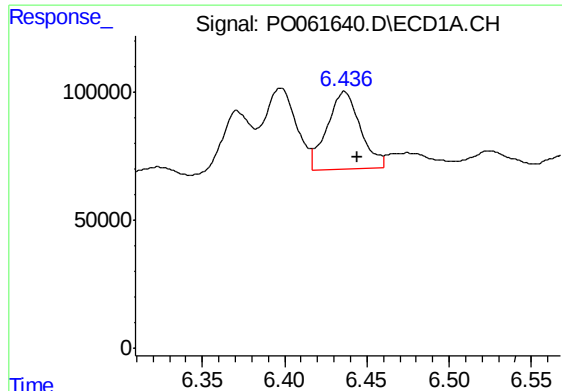


#25 AR-1248-5

R.T.: 6.436 min
Delta R.T.: -0.008 min
Response: 427983
Conc: 188.75 ng/ml m

Instrument :
ECD_O
ClientSampleId :
40166

Manual Integrations
APPROVED

Ankita
10/4/2019 5:10:53 PM

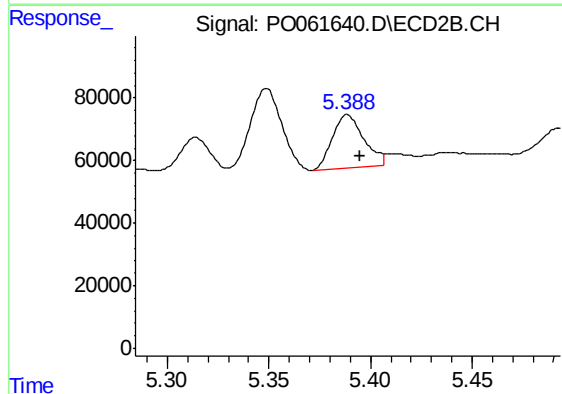

#25 AR-1248-5

R.T.: 5.388 min
Delta R.T.: -0.007 min
Response: 183540
Conc: 119.64 ng/ml m