

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100319\
 Data File : P0061657.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Oct 2019 20:11
 Operator : HP/AJ
 Sample : K5143-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NB-08-100219

Manual Integrations
 APPROVED

Ankita
 10/4/2019 5:11:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 01:34:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.381	3.540	913756	727724	22.279	22.503
2)	SA Decachlor...	10.049	8.406	640284	433987	13.749m	13.405

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100319\
Data File : PO061657.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Oct 2019 20:11
Operator : HP/AJ
Sample : K5143-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NB-08-100219


Manual Integrations
APPROVED

Ankita
10/4/2019 5:11:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 01:34:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

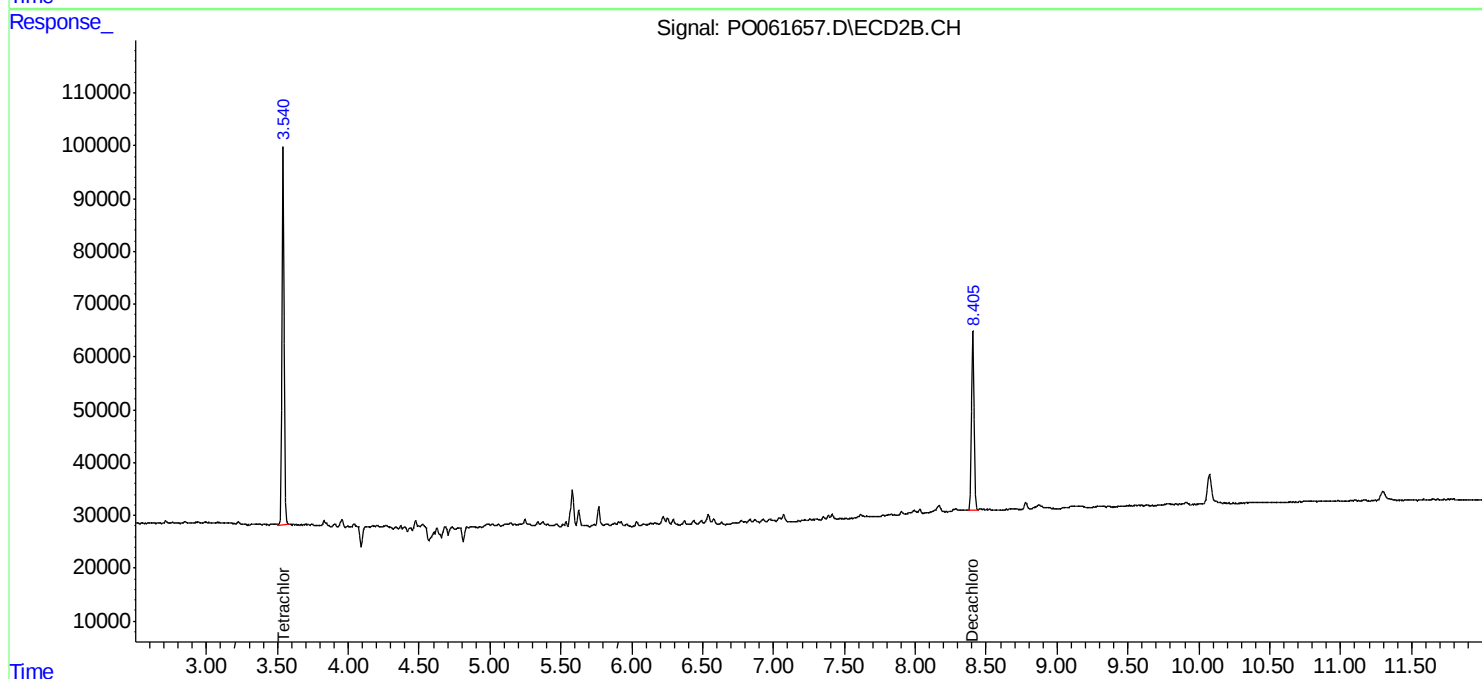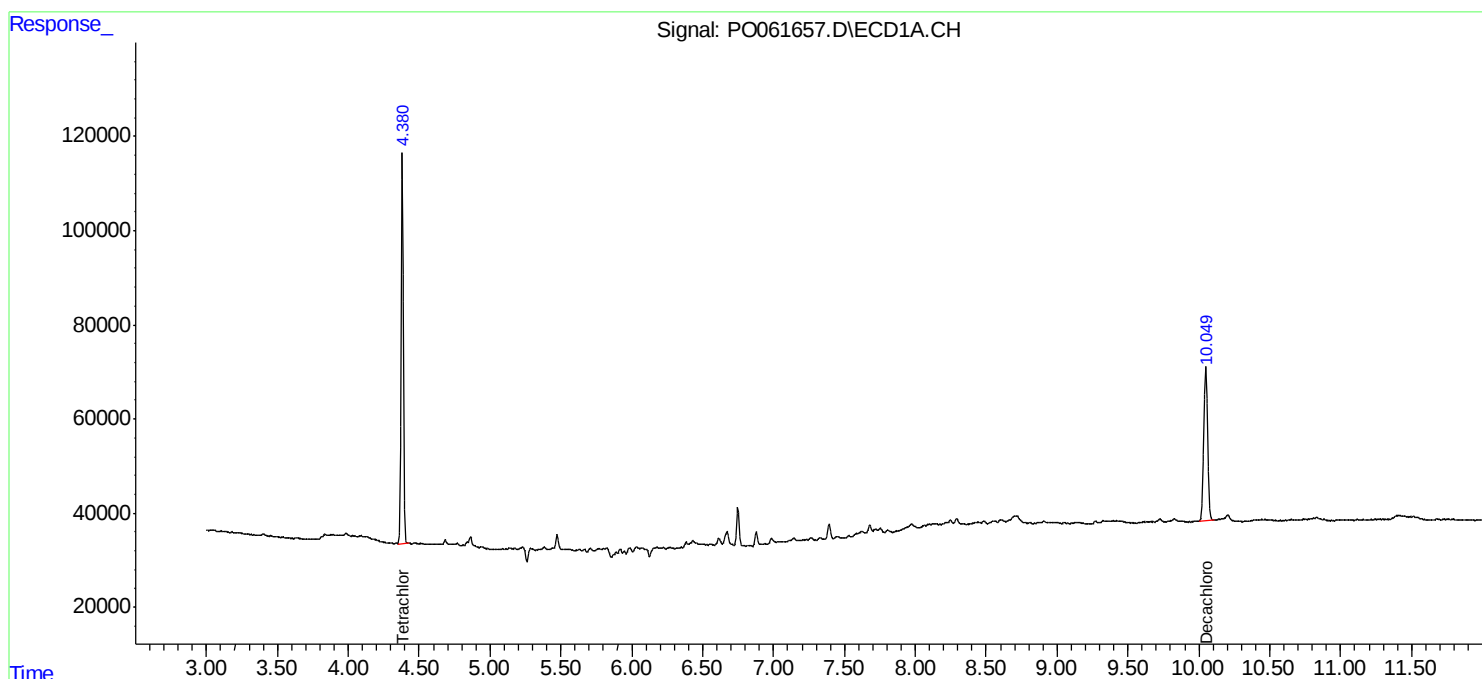

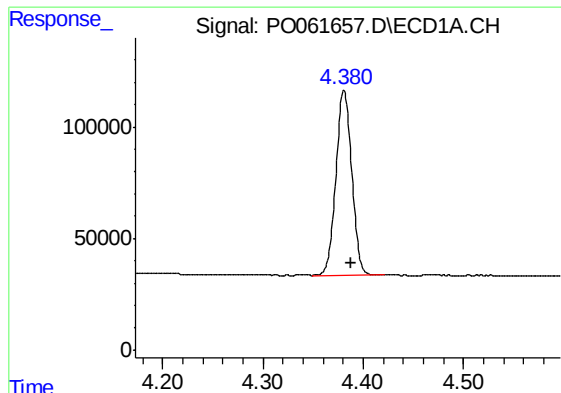


#1 Tetrachloro-m-xylene

R.T.: 4.381 min
Delta R.T.: -0.007 min
Response: 913756
Conc: 22.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
NB-08-100219


Manual Integrations
APPROVED

Ankita
10/4/2019 5:11:40 PM

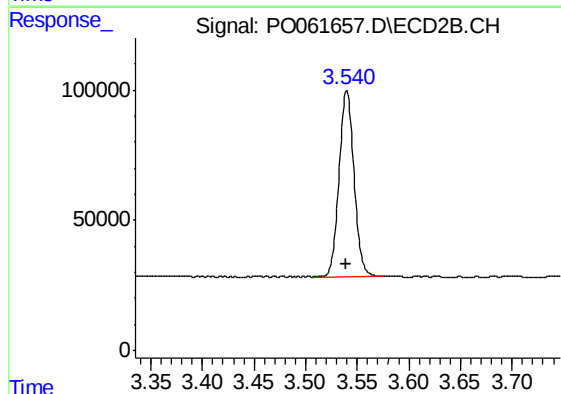


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 727724
Conc: 22.50 ng/ml

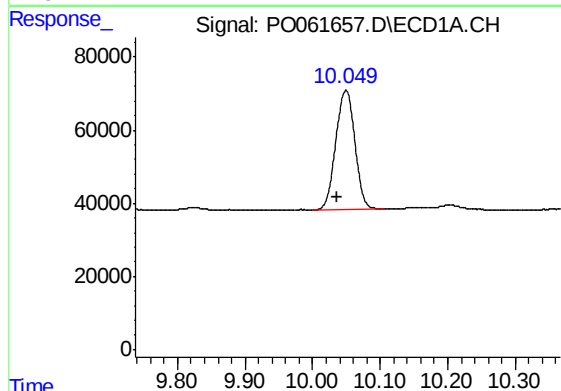

#2 Decachlorobiphenyl

R.T.: 10.049 min
Delta R.T.: 0.013 min
Response: 640284
Conc: 13.75 ng/ml m

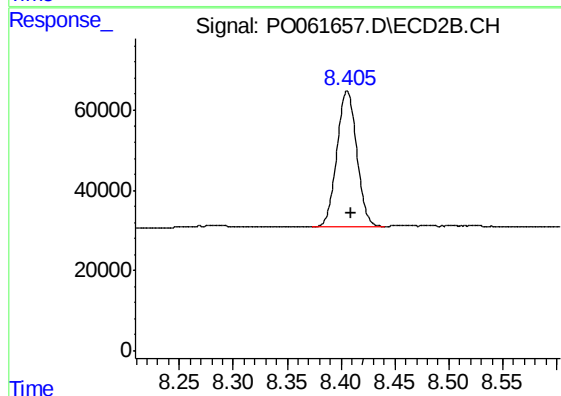

#2 Decachlorobiphenyl

R.T.: 8.406 min
Delta R.T.: -0.003 min
Response: 433987
Conc: 13.40 ng/ml