

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100319\
 Data File : P0061673.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Oct 2019 00:48
 Operator : HP/AJ
 Sample : K4660-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-1-GROUNDWATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 05:22:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.380	3.539	795732	611436	19.401	18.907
2)	SA Decachlor...	10.047	8.403	600020	426296	12.884	13.167

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100319\
Data File : PO061673.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Oct 2019 00:48
Operator : HP/AJ
Sample : K4660-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-1-GROUNDWATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 05:22:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

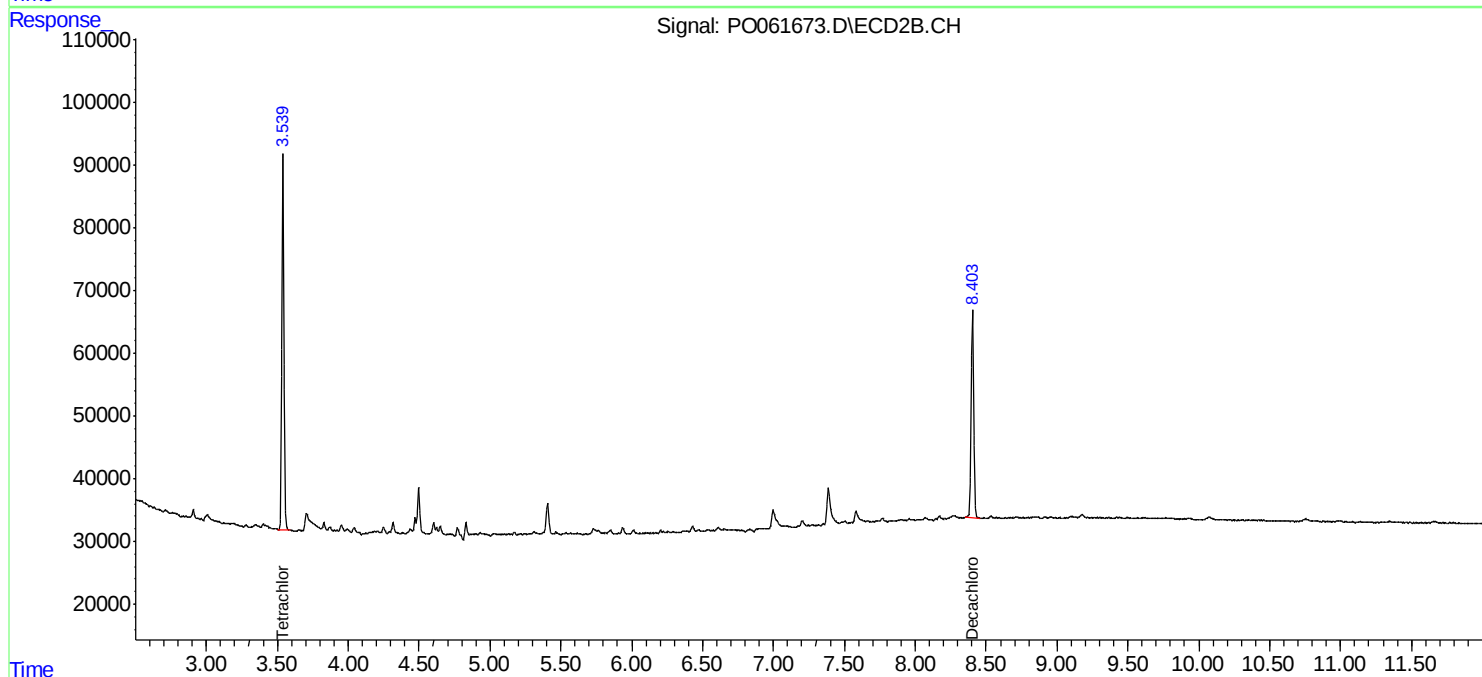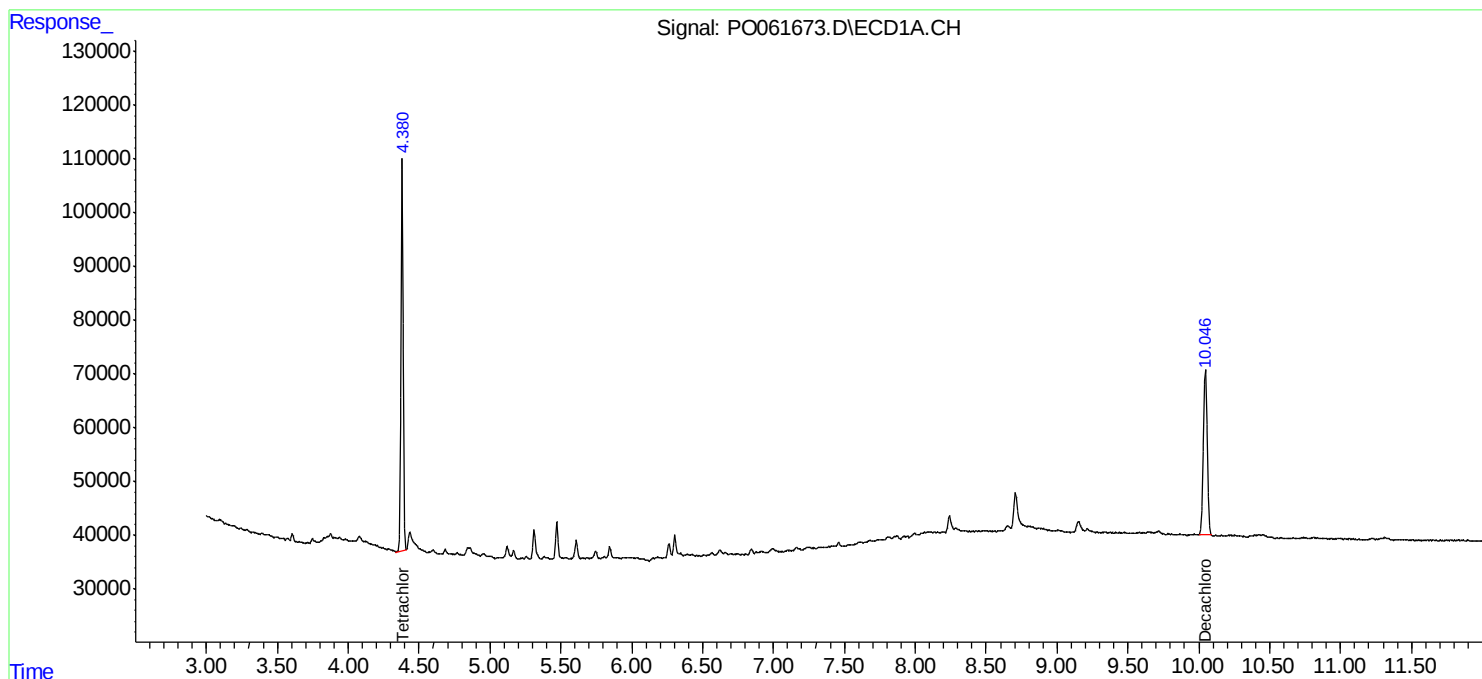


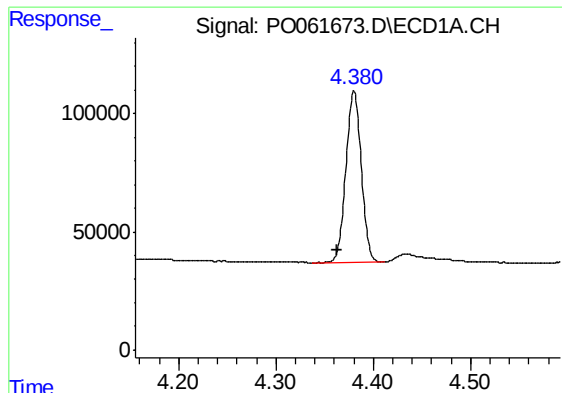

#1 Tetrachloro-m-xylene


R.T.: 4.380 min
Delta R.T.: 0.017 min
Response: 795732
Conc: 19.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1-GROUNDWATER

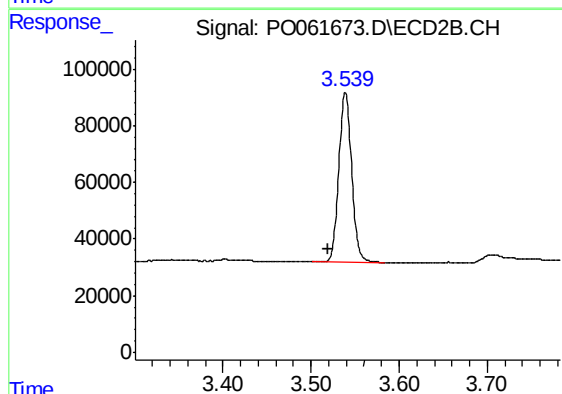


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: 0.020 min
Response: 611436
Conc: 18.91 ng/ml

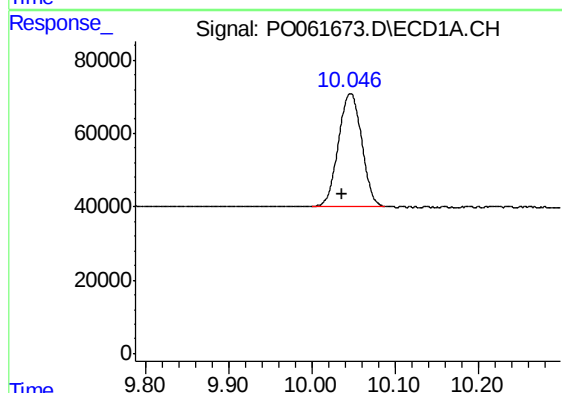

#2 Decachlorobiphenyl

R.T.: 10.047 min
Delta R.T.: 0.011 min
Response: 600020
Conc: 12.88 ng/ml

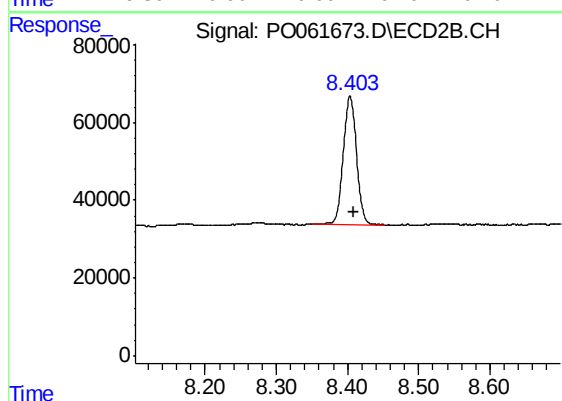

#2 Decachlorobiphenyl

R.T.: 8.403 min
Delta R.T.: -0.006 min
Response: 426296
Conc: 13.17 ng/ml