

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100319\
 Data File : P0061680.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Oct 2019 2:43
 Operator : HP/AJ
 Sample : K5176-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 30440-3077

Manual Integrations
 APPROVED

Ankita
 10/4/2019 5:12:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 05:25:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.362	3.527	1306281	535948	31.849	16.573m#
2)	SA Decachlor...	10.054	8.411	709718	396835	15.239	12.257

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100319\
Data File : PO061680.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Oct 2019 2:43
Operator : HP/AJ
Sample : K5176-02
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
30440-3077


Manual Integrations
APPROVED

Ankita
10/4/2019 5:12:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 05:25:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

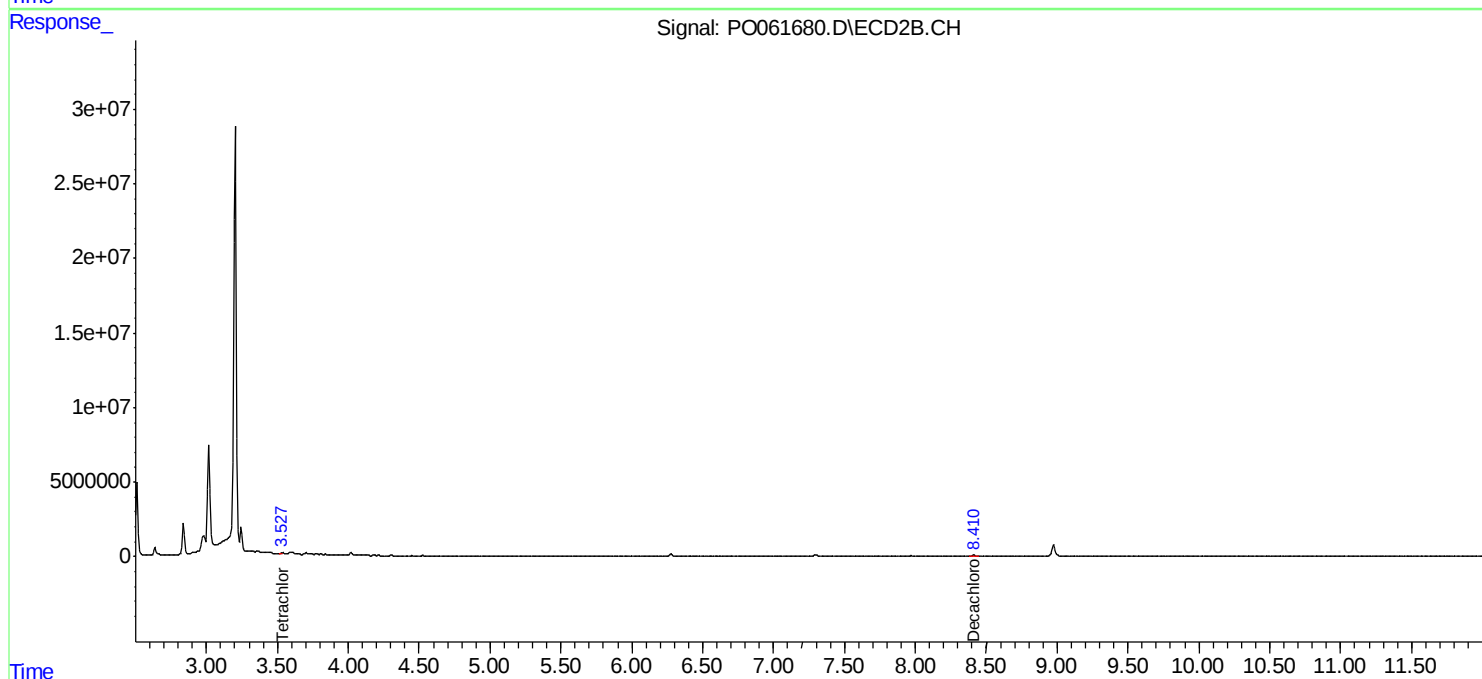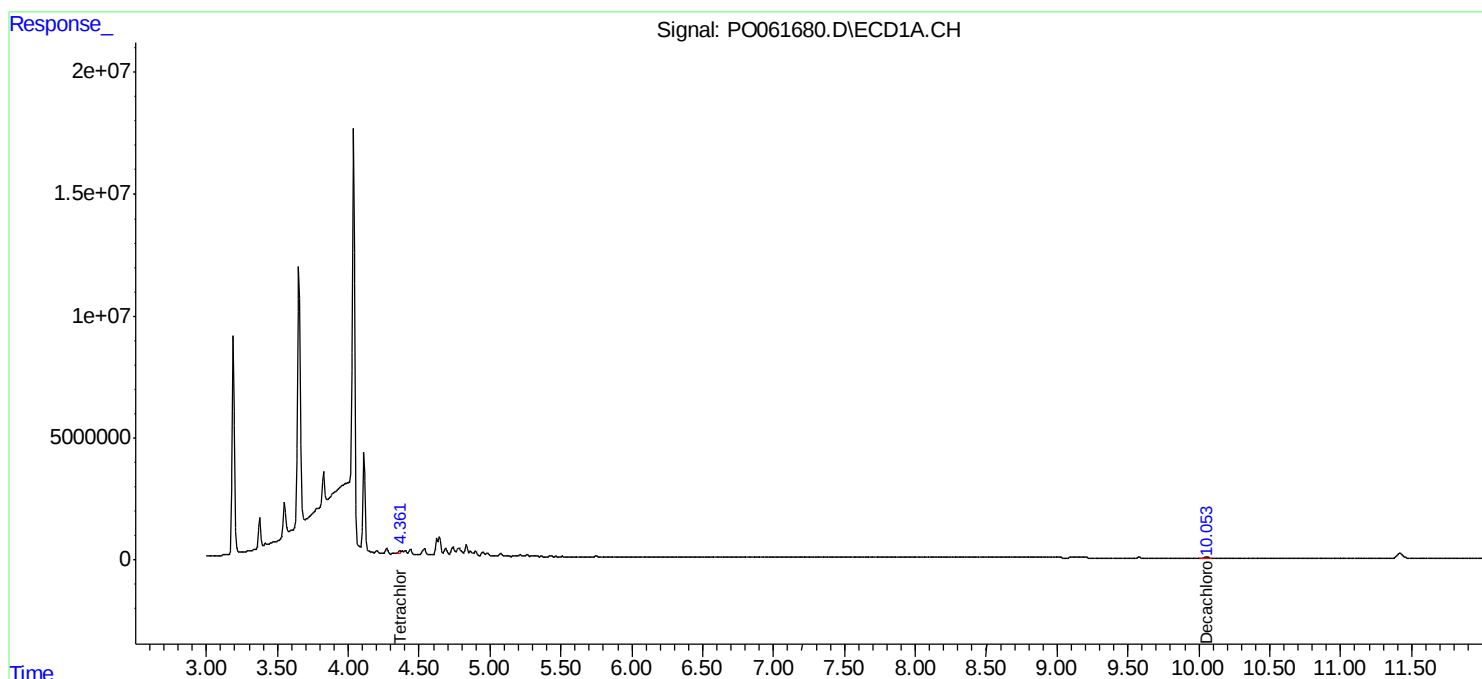

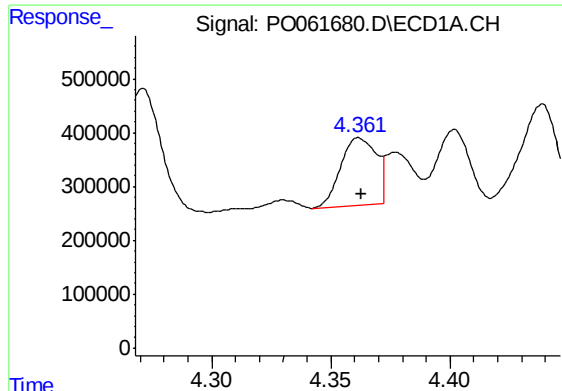


#1 Tetrachloro-m-xylene

R.T.: 4.362 min
Delta R.T.: -0.001 min
Response: 1306281
Conc: 31.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
30440-3077


Manual Integrations
APPROVED

Ankita
10/4/2019 5:12:30 PM

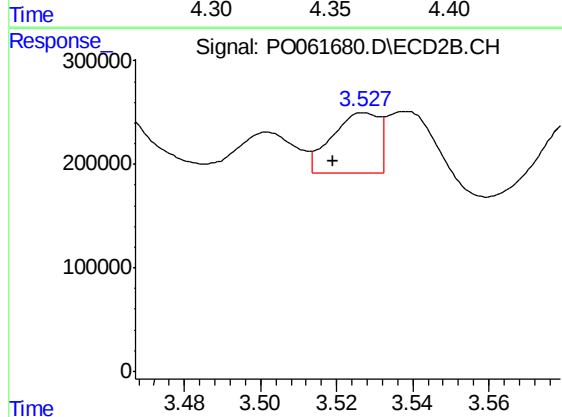


#1 Tetrachloro-m-xylene

R.T.: 3.527 min
Delta R.T.: 0.008 min
Response: 535948
Conc: 16.57 ng/ml m

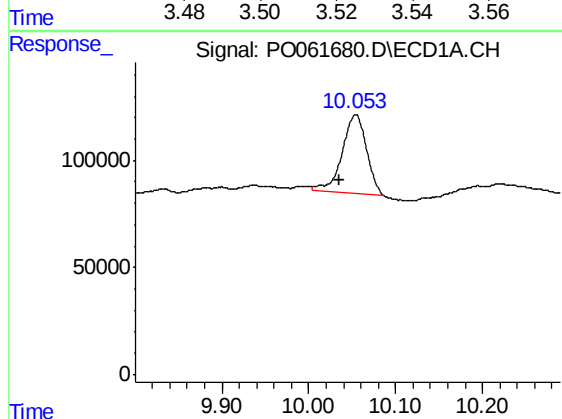

#2 Decachlorobiphenyl

R.T.: 10.054 min
Delta R.T.: 0.018 min
Response: 709718
Conc: 15.24 ng/ml

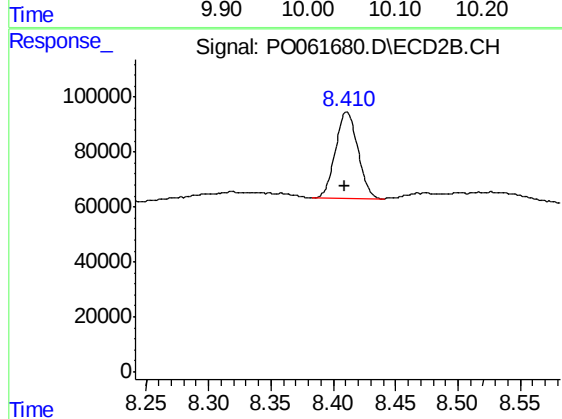

#2 Decachlorobiphenyl

R.T.: 8.411 min
Delta R.T.: 0.002 min
Response: 396835
Conc: 12.26 ng/ml