

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100419\
 Data File : PO061691.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Oct 2019 11:23
 Operator : HP/AJ
 Sample : K5134-01RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-061RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 14:01:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.357	3.517	753160	586927	18.363	18.149
2)	SA Decachlor...	10.016	8.382	517013	364165	11.102	11.248
Target Compounds							
3)	L1 AR-1016-1	5.541	0.000	3012	0	1.642	N.D. #
4)	L1 AR-1016-2	5.586	4.669	2659	24988	1.029	13.482 #
5)	L1 AR-1016-3	5.639	4.761	456	7293	0.284	7.280 #
6)	L1 AR-1016-4	5.747	4.803	2897	5587	2.167	6.447 #
7)	L1 AR-1016-5	6.045	4.989	2763	2390	2.014	2.094
8)	L2 AR-1221-1	4.553	0.000	571	0	1.234	N.D. #
9)	L2 AR-1221-2	4.661	3.822	12885	5309	35.888	17.215 #
10)	L2 AR-1221-3	4.743	3.880	32950	29223	28.941	32.038
11)	L3 AR-1232-1	4.743	3.880	32950	29223	23.563	26.027
12)	L3 AR-1232-2	5.259	0.000	2980	0	3.798	N.D. #
13)	L3 AR-1232-3	5.541	4.761	3012	7293	1.763	11.046 #
14)	L3 AR-1232-4	5.677	4.861	27483	8489	31.062	13.466 #
15)	L3 AR-1232-5	5.798	4.989	5371	2390	7.746	3.483 #
16)	L4 AR-1242-1	5.520	0.000	1721	0	1.212	N.D. #
17)	L4 AR-1242-2	5.541	0.000	3012	0	1.499	N.D. #
18)	L4 AR-1242-3	5.586	4.761	2659	7293	2.107	9.339 #
19)	L4 AR-1242-4	5.677	4.861	27483	8489	26.155	10.344 #
20)	L4 AR-1242-5	6.459	5.353	8359	45709	6.250	42.669 #
21)	L5 AR-1248-1	5.541	0.000	3012	0	2.564	N.D. #
22)	L5 AR-1248-2	5.798	4.803	5371	5587	3.183	4.742 #
23)	L5 AR-1248-3	6.045	4.861	2763	8489	1.478	6.839 #
24)	L5 AR-1248-4	6.406	4.989	69780	2390	29.532	1.590 #
25)	L5 AR-1248-5	6.459	5.419	8359	6638	3.686	4.327
26)	L6 AR-1254-1	6.380	5.353	52083	45709	22.829	20.841
27)	L6 AR-1254-2	6.598	5.490	102357	6628	28.330	3.381 #
28)	L6 AR-1254-3	6.963	5.883	36021	4715	9.219	1.481 #
29)	L6 AR-1254-4	7.238	6.112	16076	5329	5.308	2.627 #
30)	L6 AR-1254-5	7.655	6.518	44971	10448	14.320	3.694 #
31)	L7 AR-1260-1	7.157	5.972	8781	1641	3.364	0.804 #
32)	L7 AR-1260-2	7.423	6.230	32680	46841	10.251	19.503 #
33)	L7 AR-1260-3	7.788	6.415	31163	10845	12.975	4.814 #
34)	L7 AR-1260-4	7.945	0.000	109595	0	41.015	N.D. #
35)	L7 AR-1260-5	8.314	0.000	25114	0	5.075	N.D. #
36)	L8 AR-1262-1	7.727	6.552	30767	7645	8.030	6.263
37)	L8 AR-1262-2	8.270	0.000	44906	0	7.234	N.D. #
38)	L8 AR-1262-3	8.581	7.333	31193	4364	7.505	2.316 #
39)	L8 AR-1262-4	8.653	7.364	78598	5650	24.898	1.681 #
40)	L8 AR-1262-5	9.294	7.879	4673	11912	2.298	7.858 #
41)	L9 AR-1268-1	8.581	7.333	31193	4364	4.639	0.904 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100419\
 Data File : PO061691.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Oct 2019 11:23
 Operator : HP/AJ
 Sample : K5134-01RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-061RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 14:01:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.653	7.364	78598	5650	12.693	1.311 #
43) L9	AR-1268-3	8.892	7.547	24642	21098	4.820	5.886
44) L9	AR-1268-4	9.294	7.879	4673	11912	2.137	7.402 #
45) L9	AR-1268-5	9.694	8.149	6000	11291	0.399	1.123 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100419\
Data File : P0061691.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Oct 2019 11:23
Operator : HP/AJ
Sample : K5134-01RE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 14:01:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

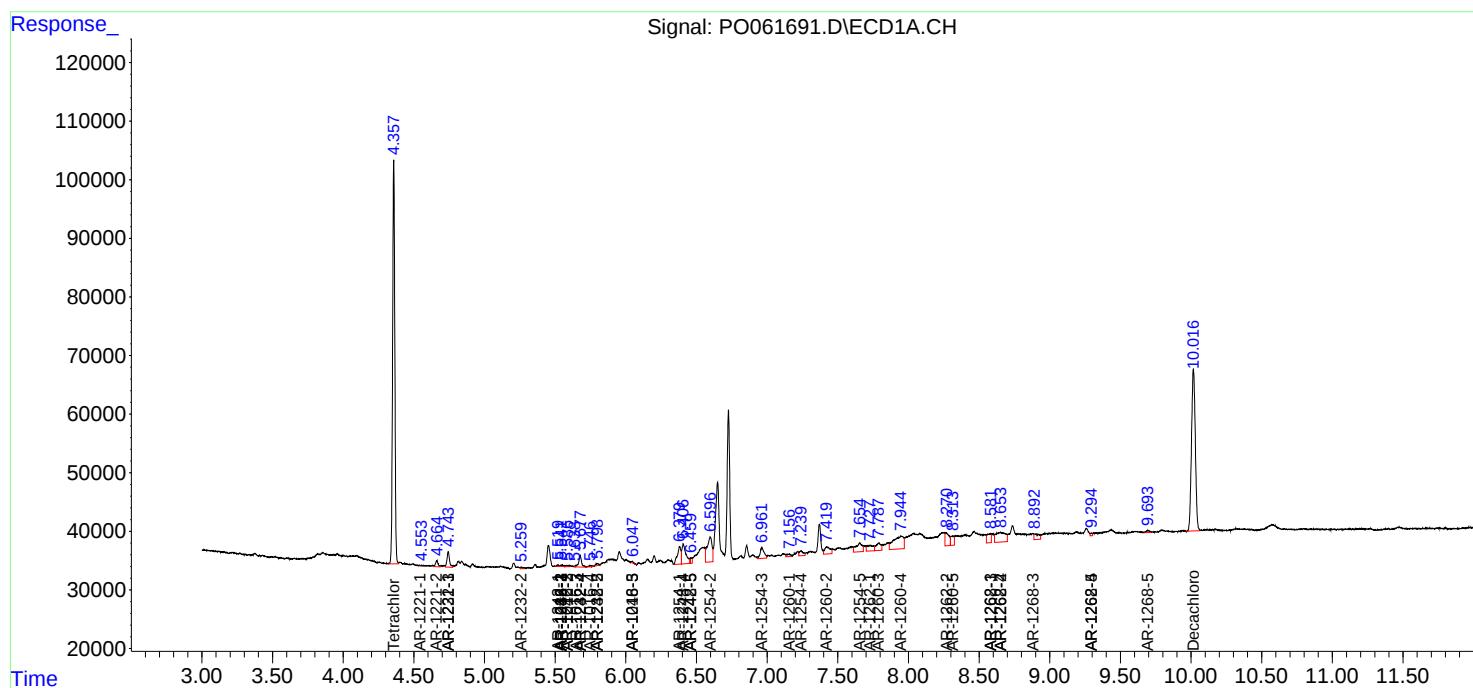


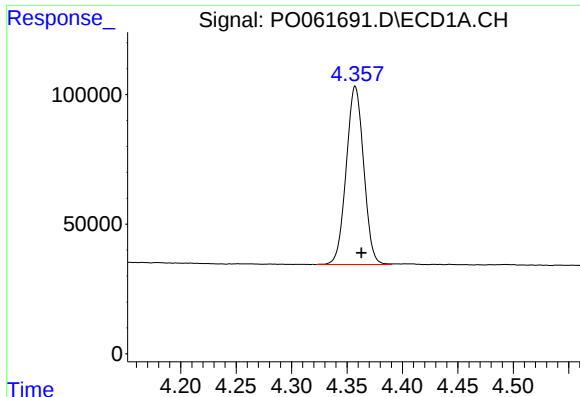

#1 Tetrachloro-m-xylene


R.T.: 4.357 min
Delta R.T.: -0.006 min
Response: 753160
Conc: 18.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

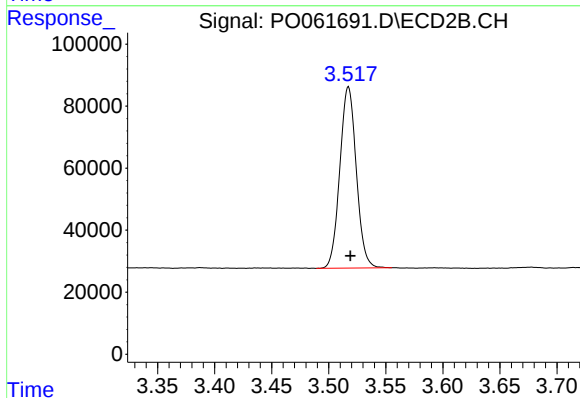


#1 Tetrachloro-m-xylene

R.T.: 3.517 min
Delta R.T.: -0.002 min
Response: 586927
Conc: 18.15 ng/ml

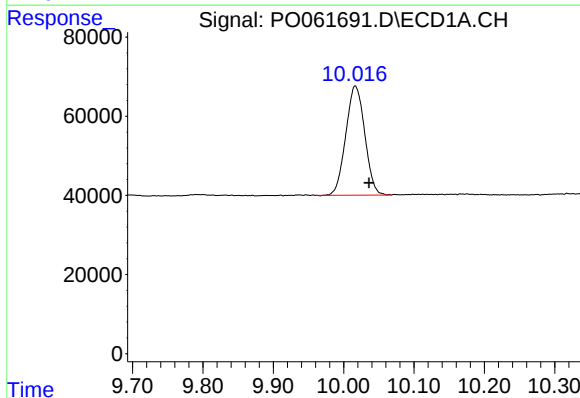


#2 Decachlorobiphenyl

R.T.: 10.016 min
Delta R.T.: -0.020 min
Response: 517013
Conc: 11.10 ng/ml

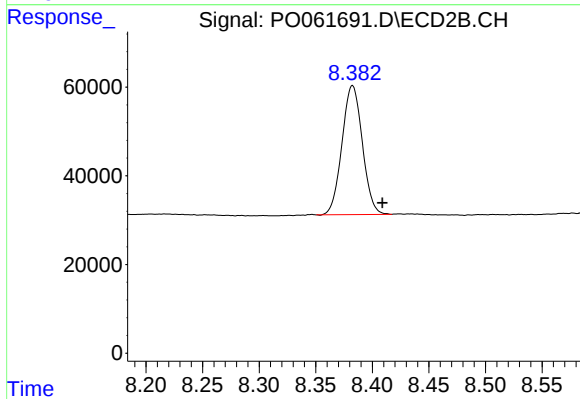

#2 Decachlorobiphenyl


R.T.: 8.382 min
Delta R.T.: -0.027 min
Response: 364165
Conc: 11.25 ng/ml

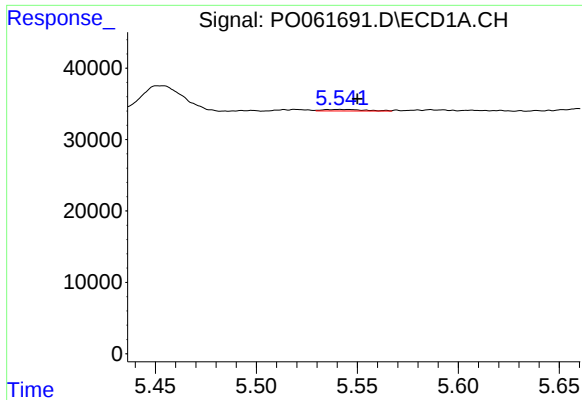

#3 AR-1016-1


R.T.: 5.541 min
Delta R.T.: -0.009 min
Response: 3012
Conc: 1.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

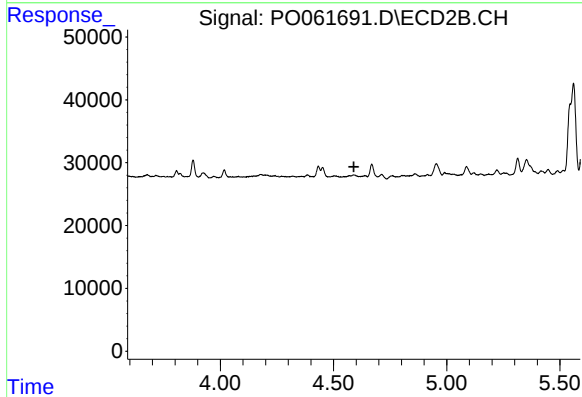


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.590 min
Response: 0
Conc: N.D.

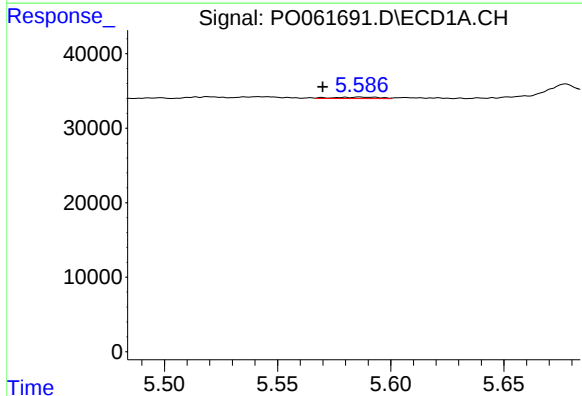


#4 AR-1016-2

R.T.: 5.586 min
Delta R.T.: 0.016 min
Response: 2659
Conc: 1.03 ng/ml

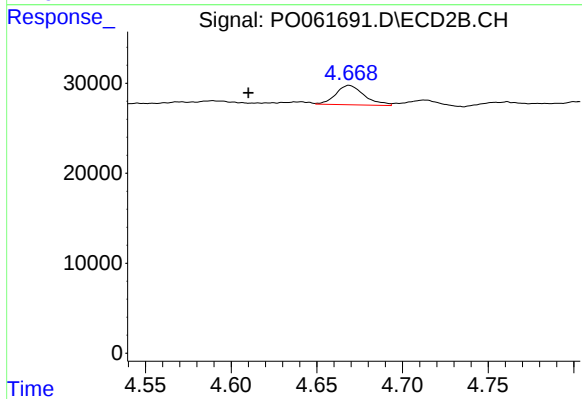

#4 AR-1016-2


R.T.: 4.669 min
Delta R.T.: 0.059 min
Response: 24988
Conc: 13.48 ng/ml

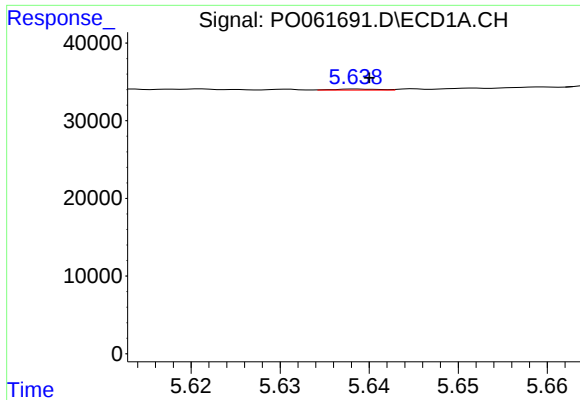

#5 AR-1016-3


R.T.: 5.639 min
Delta R.T.: -0.001 min
Response: 456
Conc: 0.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

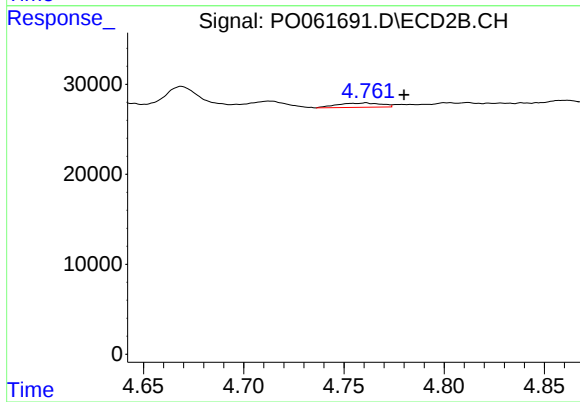


#5 AR-1016-3

R.T.: 4.761 min
Delta R.T.: -0.019 min
Response: 7293
Conc: 7.28 ng/ml

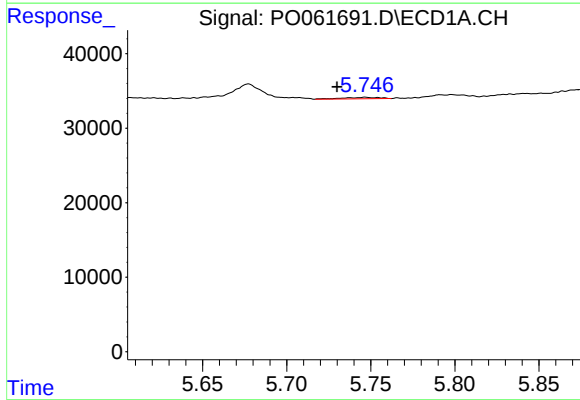


#6 AR-1016-4

R.T.: 5.747 min
Delta R.T.: 0.017 min
Response: 2897
Conc: 2.17 ng/ml

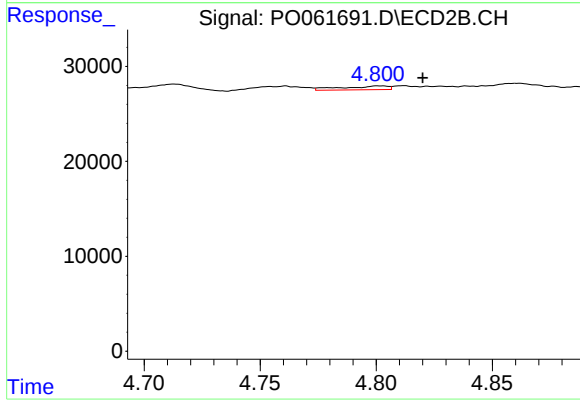

#6 AR-1016-4


R.T.: 4.803 min
Delta R.T.: -0.017 min
Response: 5587
Conc: 6.45 ng/ml

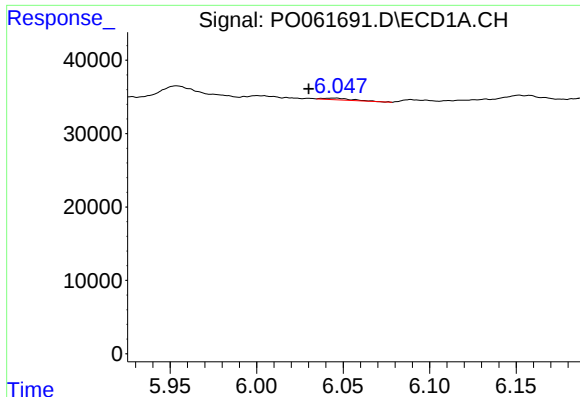

#7 AR-1016-5


R.T.: 6.045 min
Delta R.T.: 0.015 min
Response: 2763
Conc: 2.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

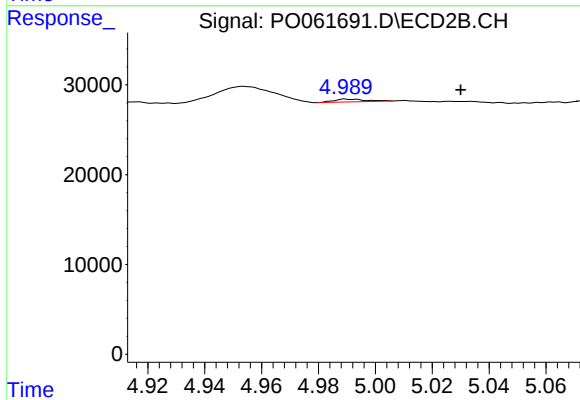


#7 AR-1016-5

R.T.: 4.989 min
Delta R.T.: -0.041 min
Response: 2390
Conc: 2.09 ng/ml

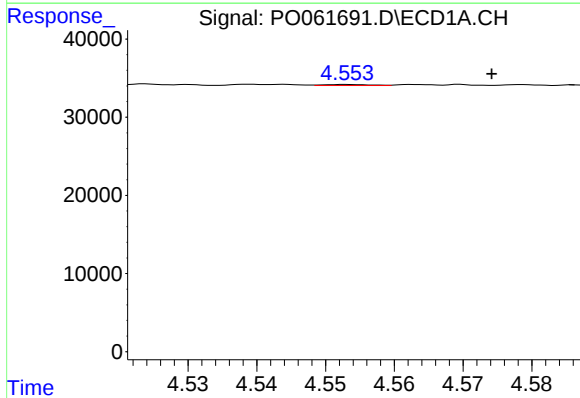


#8 AR-1221-1

R.T.: 4.553 min
Delta R.T.: -0.021 min
Response: 571
Conc: 1.23 ng/ml

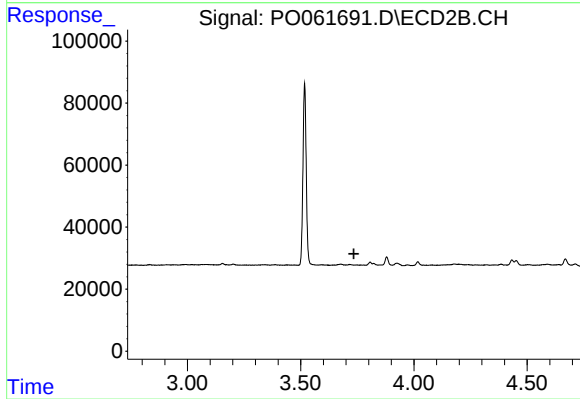

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 3.735 min
Response: 0
Conc: N.D.

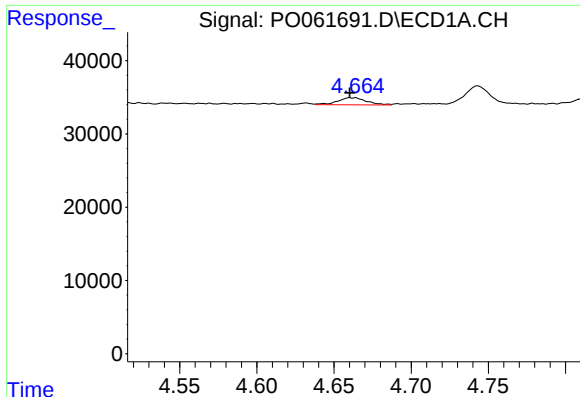

#9 AR-1221-2


R.T.: 4.661 min
Delta R.T.: 0.000 min
Response: 12885
Conc: 35.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

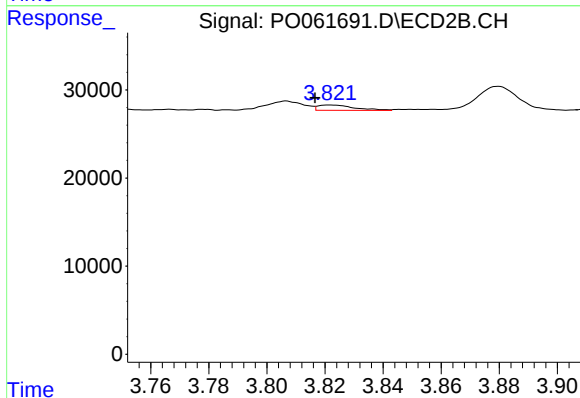


#9 AR-1221-2

R.T.: 3.822 min
Delta R.T.: 0.005 min
Response: 5309
Conc: 17.22 ng/ml

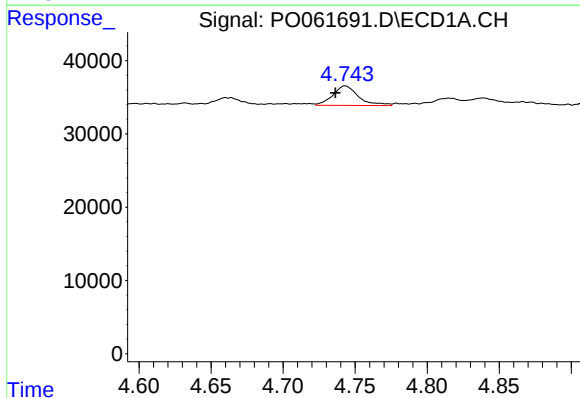


#10 AR-1221-3

R.T.: 4.743 min
Delta R.T.: 0.007 min
Response: 32950
Conc: 28.94 ng/ml

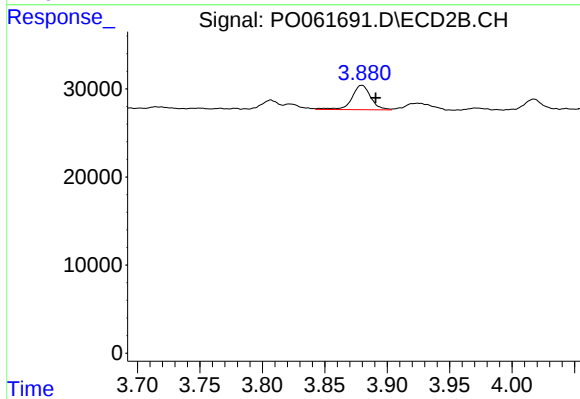

#10 AR-1221-3


R.T.: 3.880 min
Delta R.T.: -0.011 min
Response: 29223
Conc: 32.04 ng/ml

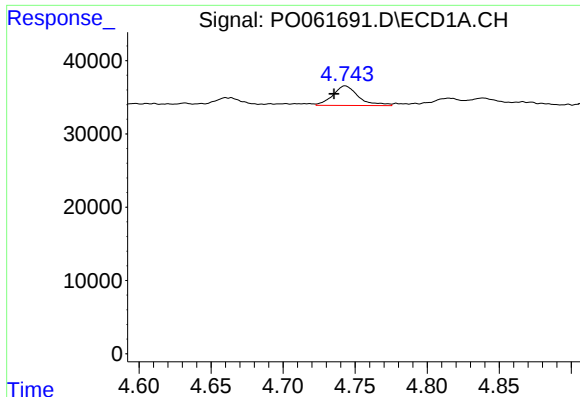

#11 AR-1232-1


R.T.: 4.743 min
Delta R.T.: 0.008 min
Response: 32950
Conc: 23.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

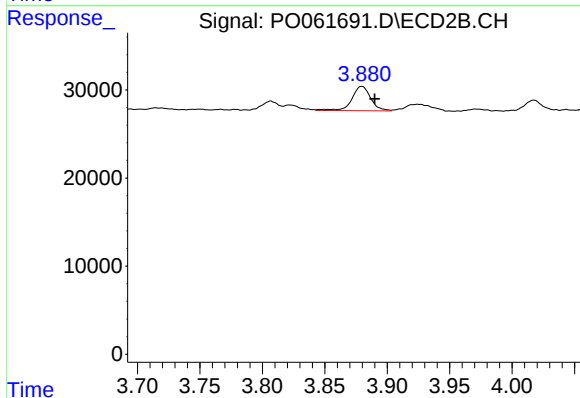


#11 AR-1232-1

R.T.: 3.880 min
Delta R.T.: -0.010 min
Response: 29223
Conc: 26.03 ng/ml

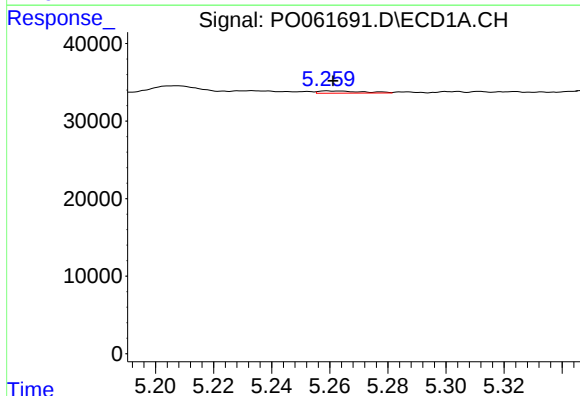


#12 AR-1232-2

R.T.: 5.259 min
Delta R.T.: -0.002 min
Response: 2980
Conc: 3.80 ng/ml

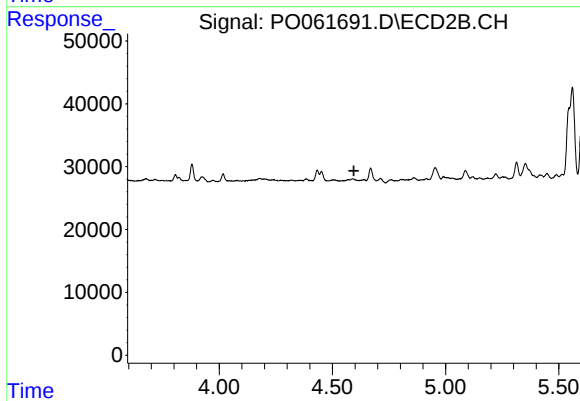

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 4.595 min
Response: 0
Conc: N.D.

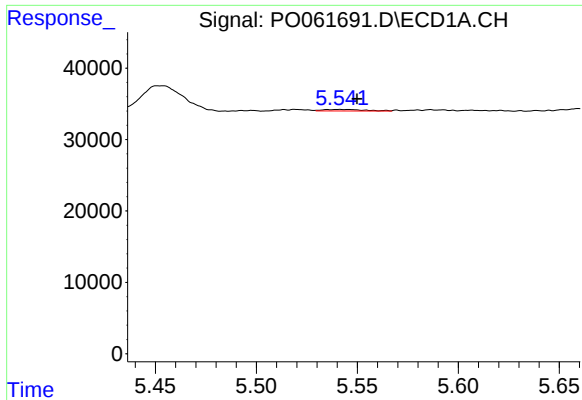

#13 AR-1232-3


R.T.: 5.541 min
Delta R.T.: -0.008 min
Response: 3012
Conc: 1.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

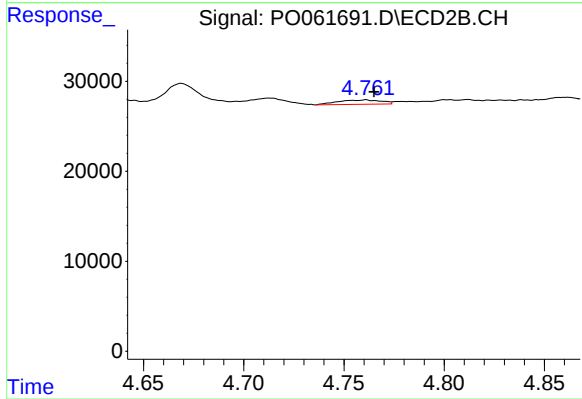


#13 AR-1232-3

R.T.: 4.761 min
Delta R.T.: -0.004 min
Response: 7293
Conc: 11.05 ng/ml

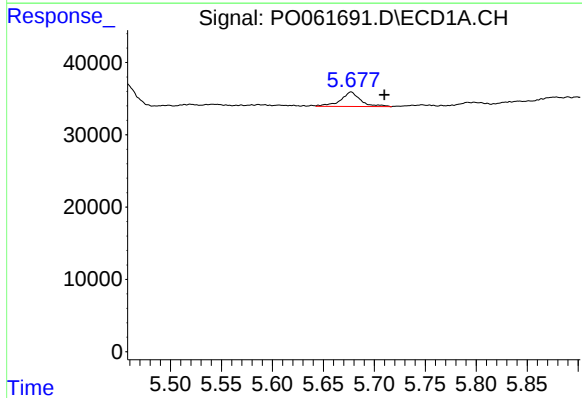


#14 AR-1232-4

R.T.: 5.677 min
Delta R.T.: -0.033 min
Response: 27483
Conc: 31.06 ng/ml

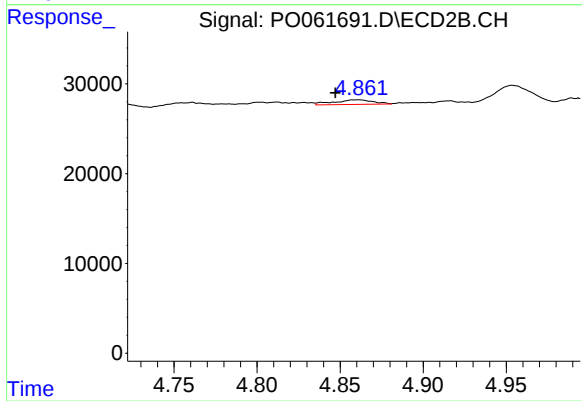

#14 AR-1232-4


R.T.: 4.861 min
Delta R.T.: 0.014 min
Response: 8489
Conc: 13.47 ng/ml

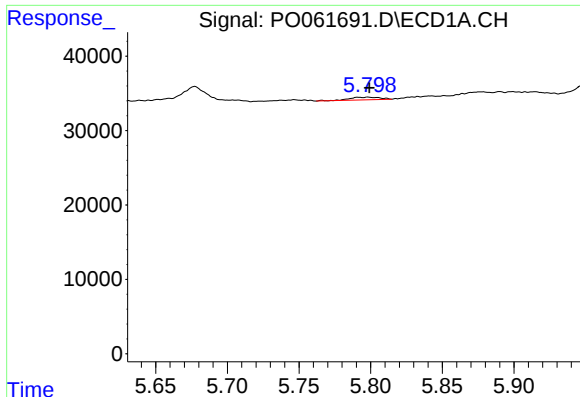

#15 AR-1232-5


R.T.: 5.798 min
Delta R.T.: 0.000 min
Response: 5371
Conc: 7.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

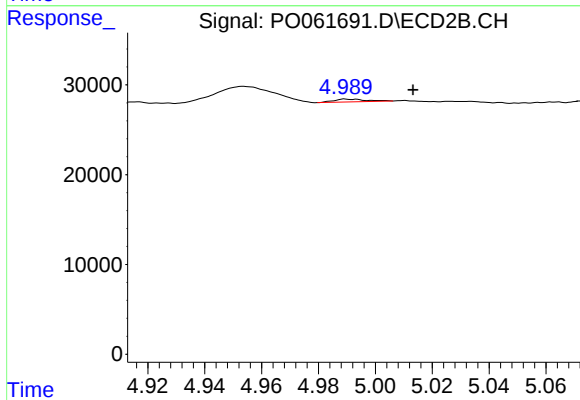


#15 AR-1232-5

R.T.: 4.989 min
Delta R.T.: -0.024 min
Response: 2390
Conc: 3.48 ng/ml

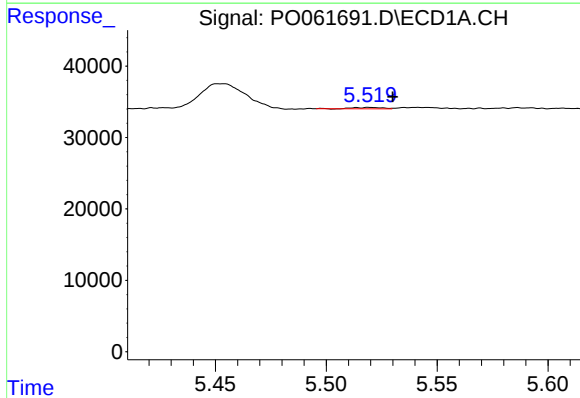


#16 AR-1242-1

R.T.: 5.520 min
Delta R.T.: -0.010 min
Response: 1721
Conc: 1.21 ng/ml

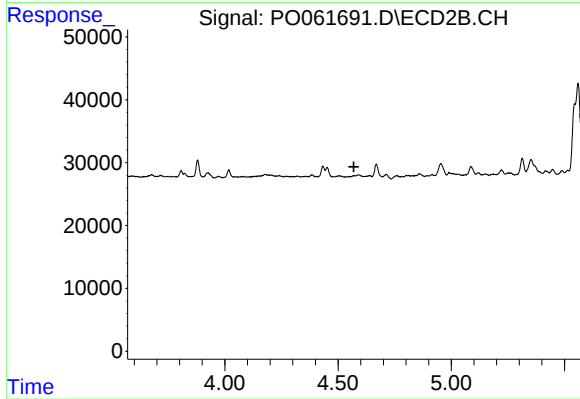

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T.: 4.570 min
Response: 0
Conc: N.D.

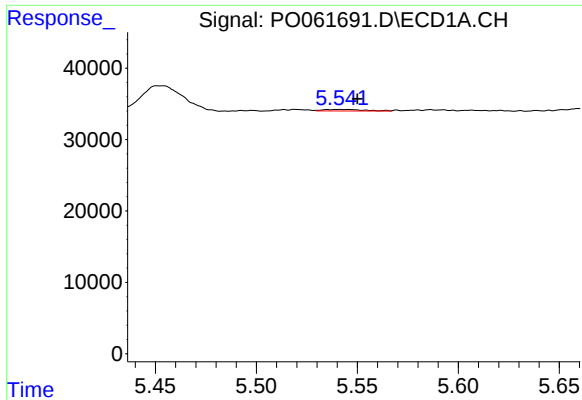

#17 AR-1242-2


R.T.: 5.541 min
Delta R.T.: -0.009 min
Response: 3012
Conc: 1.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

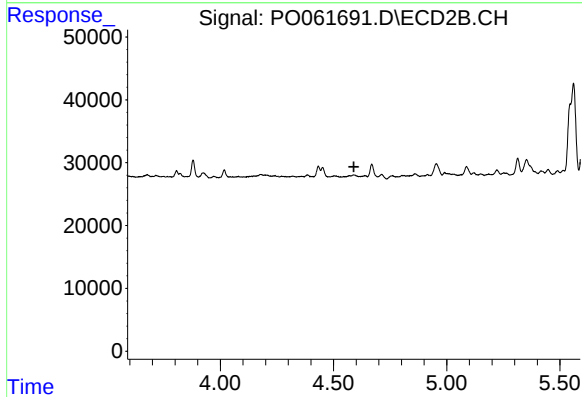


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 4.590 min
Response: 0
Conc: N.D.

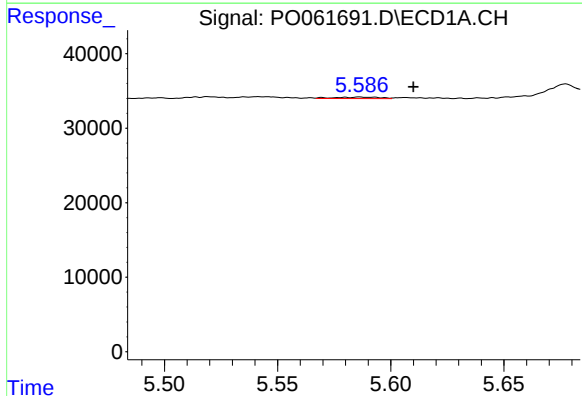


#18 AR-1242-3

R.T.: 5.586 min
Delta R.T.: -0.024 min
Response: 2659
Conc: 2.11 ng/ml

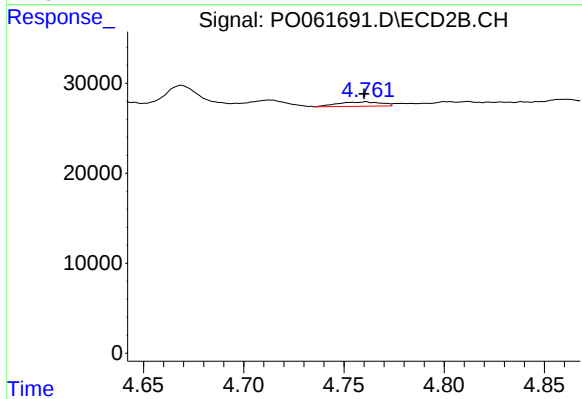

#18 AR-1242-3


R.T.: 4.761 min
Delta R.T.: 0.001 min
Response: 7293
Conc: 9.34 ng/ml

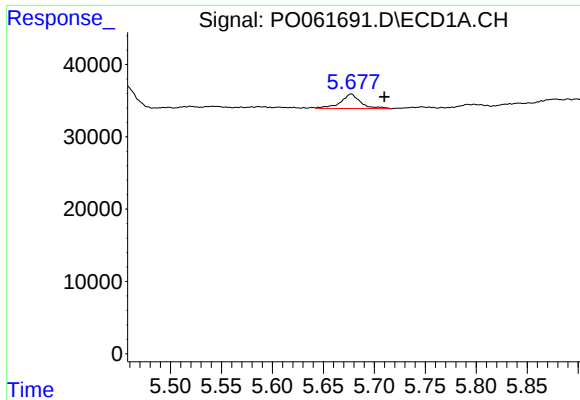

#19 AR-1242-4


R.T.: 5.677 min
Delta R.T.: -0.033 min
Response: 27483
Conc: 26.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

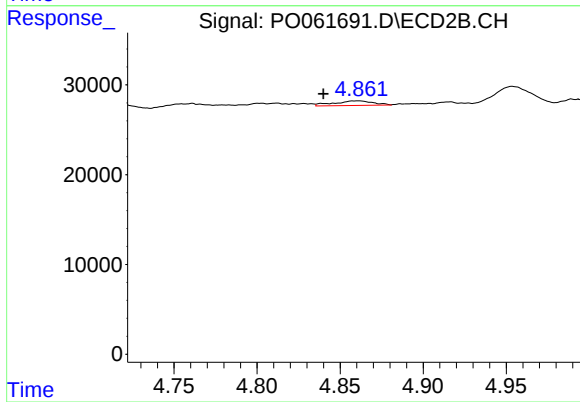


#19 AR-1242-4

R.T.: 4.861 min
Delta R.T.: 0.021 min
Response: 8489
Conc: 10.34 ng/ml

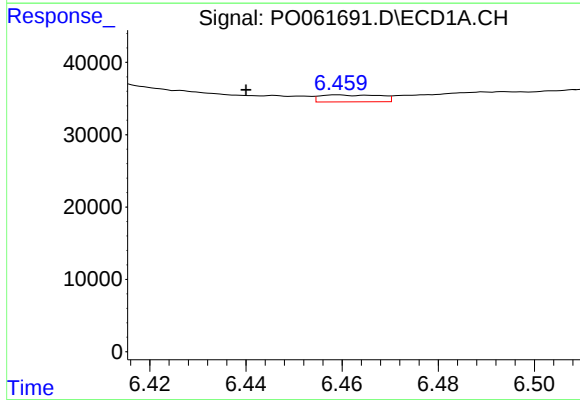


#20 AR-1242-5

R.T.: 6.459 min
Delta R.T.: 0.019 min
Response: 8359
Conc: 6.25 ng/ml

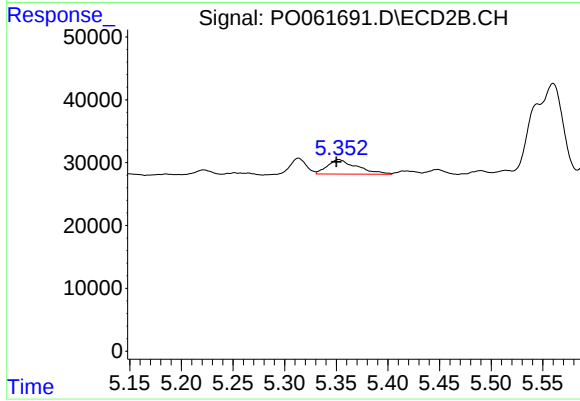

#20 AR-1242-5


R.T.: 5.353 min
Delta R.T.: 0.003 min
Response: 45709
Conc: 42.67 ng/ml

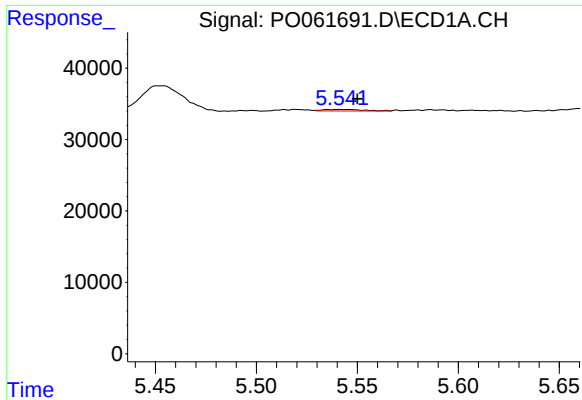

#21 AR-1248-1


R.T.: 5.541 min
Delta R.T.: -0.009 min
Response: 3012
Conc: 2.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

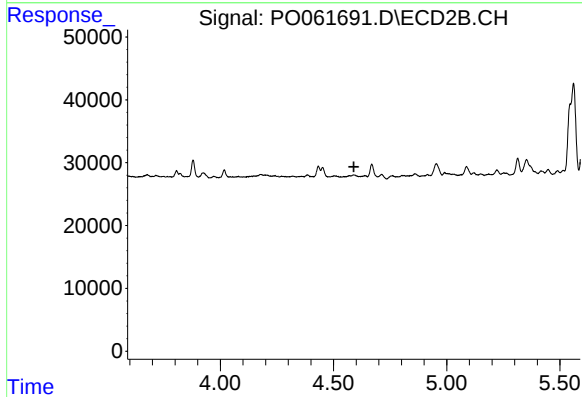


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.590 min
Response: 0
Conc: N.D.

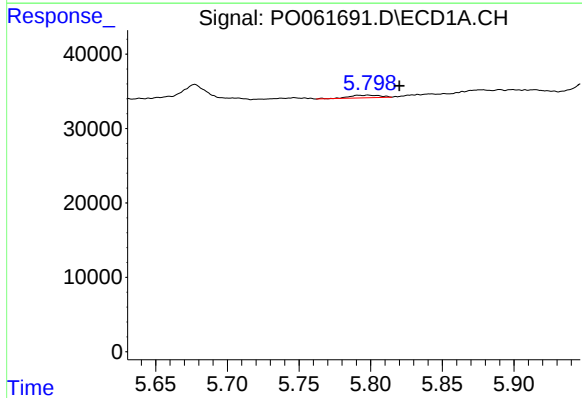


#22 AR-1248-2

R.T.: 5.798 min
Delta R.T.: -0.022 min
Response: 5371
Conc: 3.18 ng/ml

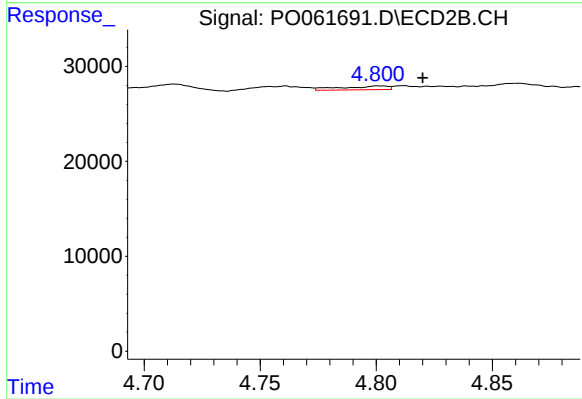

#22 AR-1248-2


R.T.: 4.803 min
Delta R.T.: -0.017 min
Response: 5587
Conc: 4.74 ng/ml

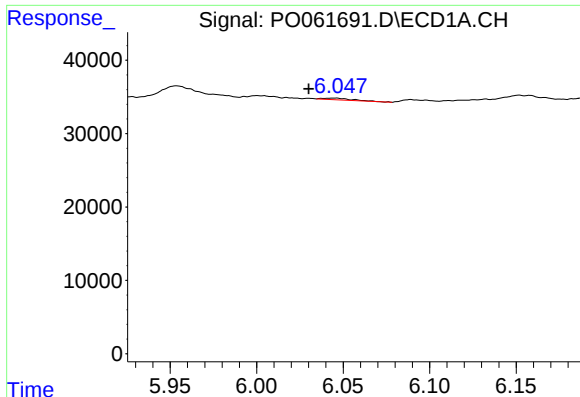

#23 AR-1248-3


R.T.: 6.045 min
Delta R.T.: 0.015 min
Response: 2763
Conc: 1.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

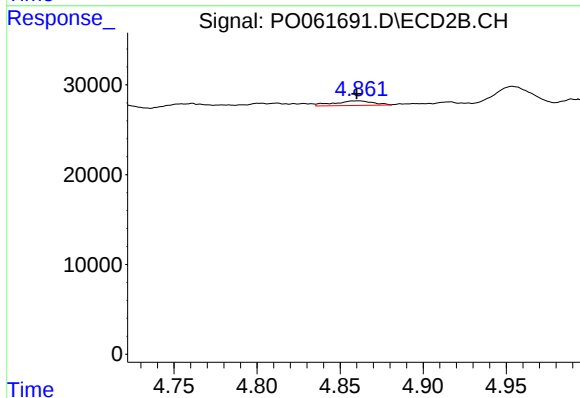


#23 AR-1248-3

R.T.: 4.861 min
Delta R.T.: 0.001 min
Response: 8489
Conc: 6.84 ng/ml

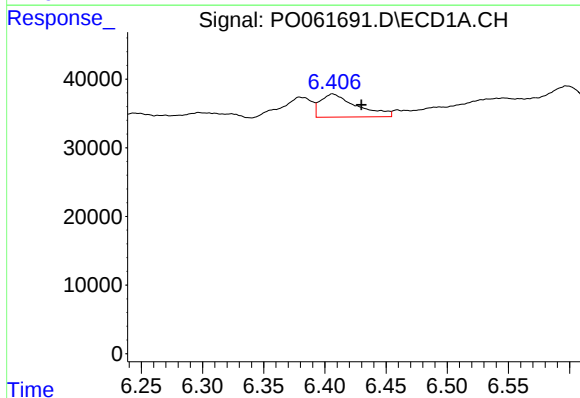


#24 AR-1248-4

R.T.: 6.406 min
Delta R.T.: -0.024 min
Response: 69780
Conc: 29.53 ng/ml

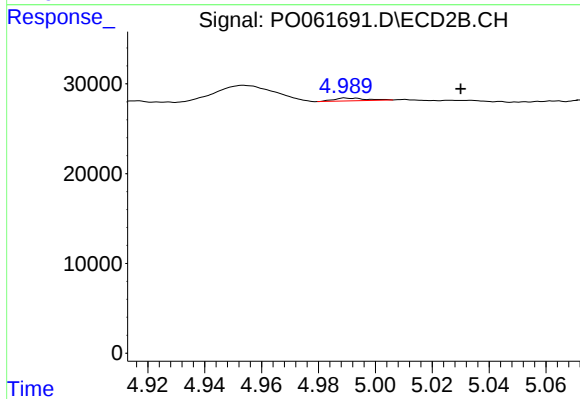

#24 AR-1248-4


R.T.: 4.989 min
Delta R.T.: -0.041 min
Response: 2390
Conc: 1.59 ng/ml

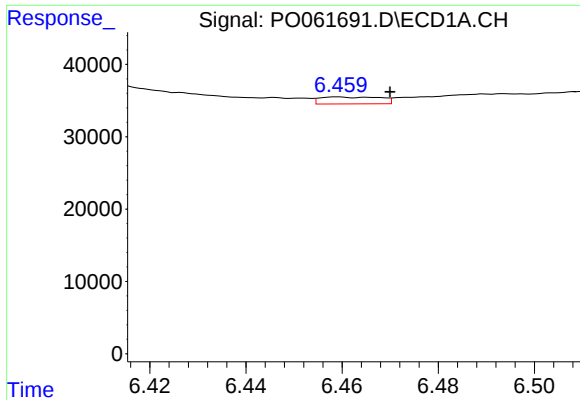

#25 AR-1248-5


R.T.: 6.459 min
Delta R.T.: -0.011 min
Response: 8359
Conc: 3.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

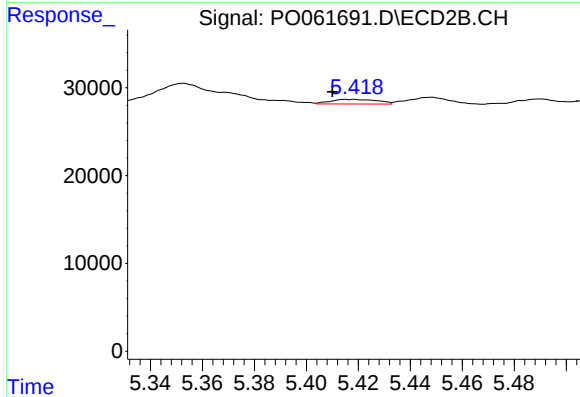


#25 AR-1248-5

R.T.: 5.419 min
Delta R.T.: 0.009 min
Response: 6638
Conc: 4.33 ng/ml

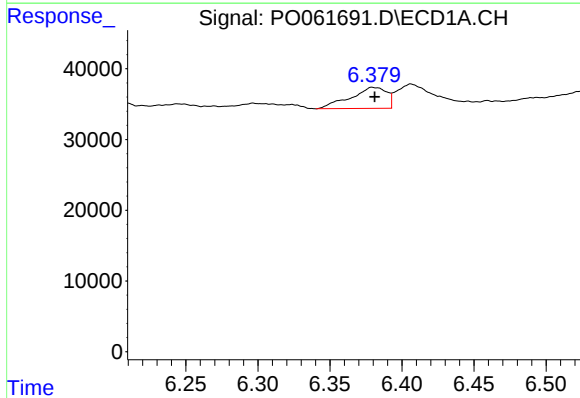


#26 AR-1254-1

R.T.: 6.380 min
Delta R.T.: -0.001 min
Response: 52083
Conc: 22.83 ng/ml

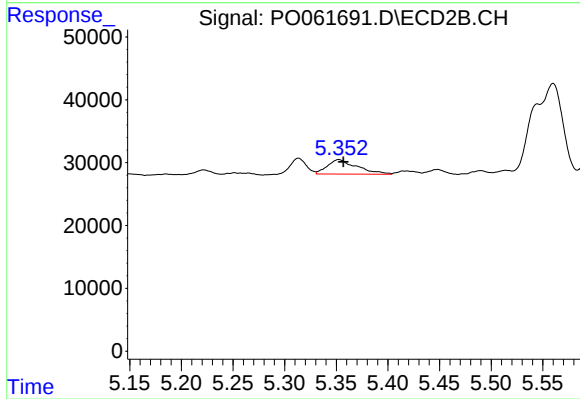

#26 AR-1254-1


R.T.: 5.353 min
Delta R.T.: -0.004 min
Response: 45709
Conc: 20.84 ng/ml

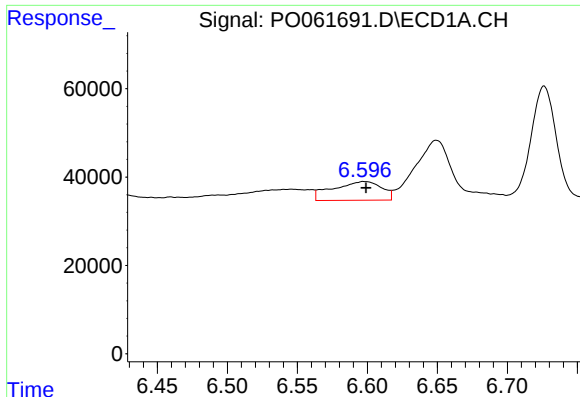

#27 AR-1254-2


R.T.: 6.598 min
Delta R.T.: -0.001 min
Response: 102357
Conc: 28.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

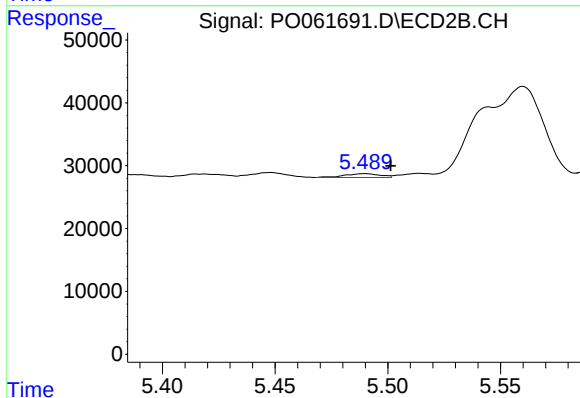


#27 AR-1254-2

R.T.: 5.490 min
Delta R.T.: -0.011 min
Response: 6628
Conc: 3.38 ng/ml

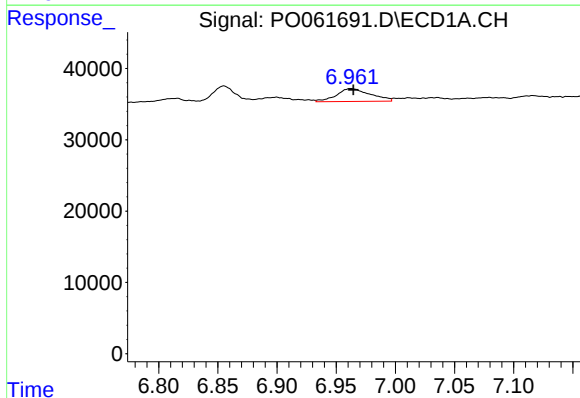


#28 AR-1254-3

R.T.: 6.963 min
Delta R.T.: -0.002 min
Response: 36021
Conc: 9.22 ng/ml

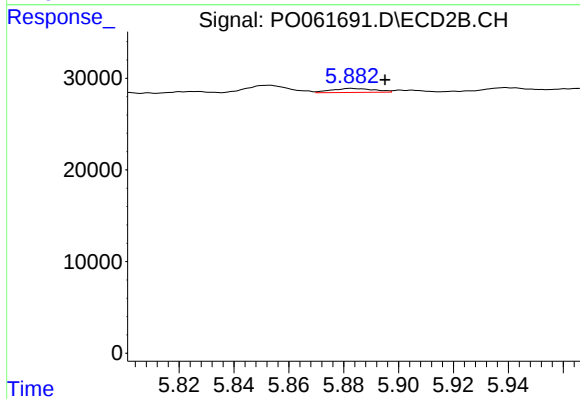

#28 AR-1254-3


R.T.: 5.883 min
Delta R.T.: -0.012 min
Response: 4715
Conc: 1.48 ng/ml

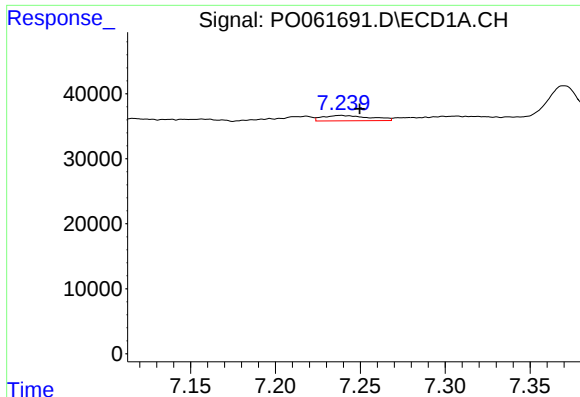

#29 AR-1254-4


R.T.: 7.238 min
Delta R.T.: -0.011 min
Response: 16076
Conc: 5.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

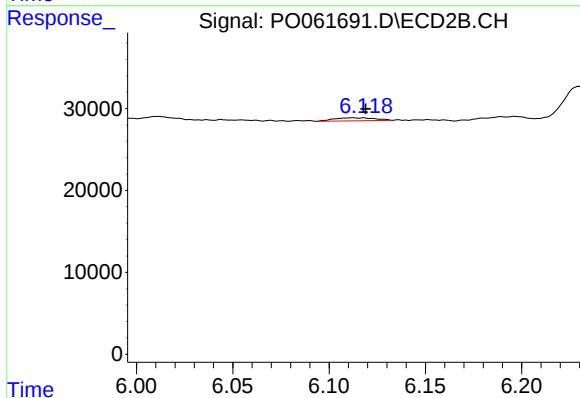


#29 AR-1254-4

R.T.: 6.112 min
Delta R.T.: -0.007 min
Response: 5329
Conc: 2.63 ng/ml

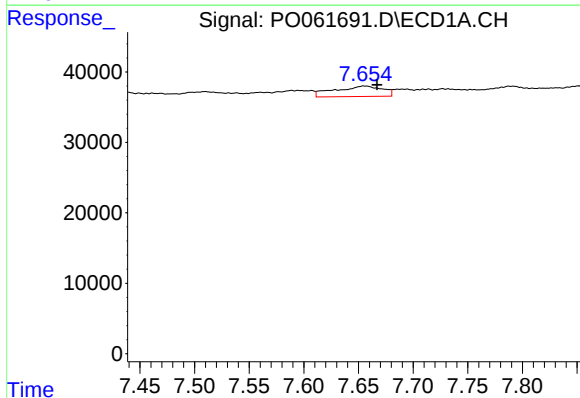


#30 AR-1254-5

R.T.: 7.655 min
Delta R.T.: -0.012 min
Response: 44971
Conc: 14.32 ng/ml

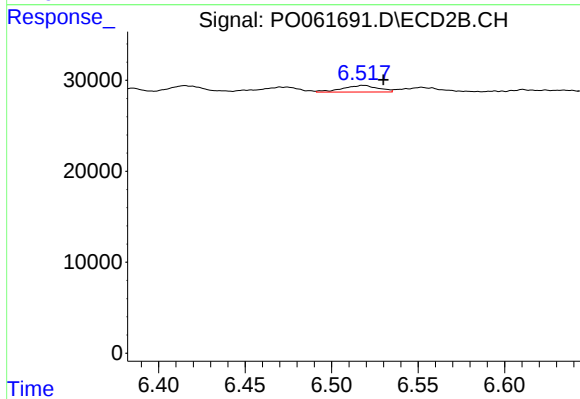

#30 AR-1254-5


R.T.: 6.518 min
Delta R.T.: -0.012 min
Response: 10448
Conc: 3.69 ng/ml

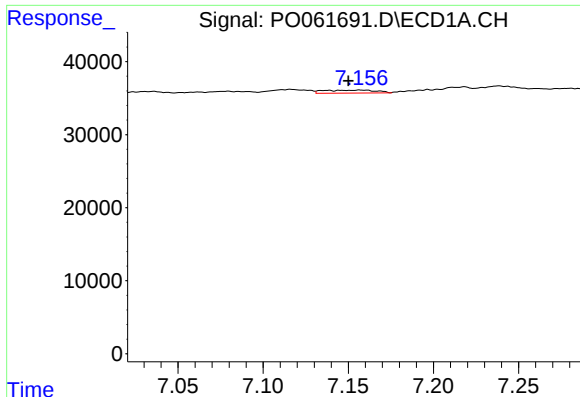

#31 AR-1260-1


R.T.: 7.157 min
Delta R.T.: 0.007 min
Response: 8781
Conc: 3.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

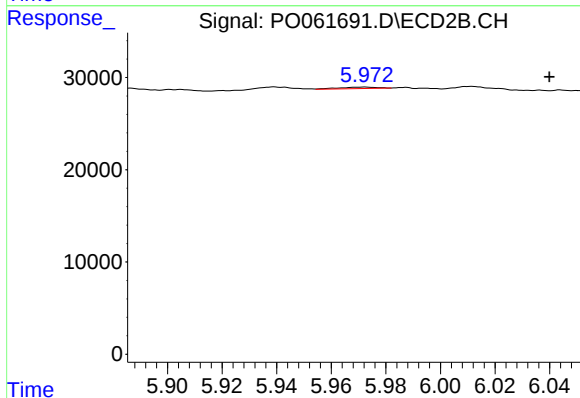


#31 AR-1260-1

R.T.: 5.972 min
Delta R.T.: -0.068 min
Response: 1641
Conc: 0.80 ng/ml

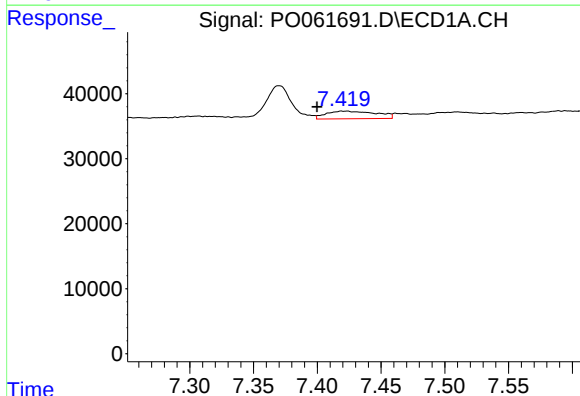


#32 AR-1260-2

R.T.: 7.423 min
Delta R.T.: 0.023 min
Response: 32680
Conc: 10.25 ng/ml

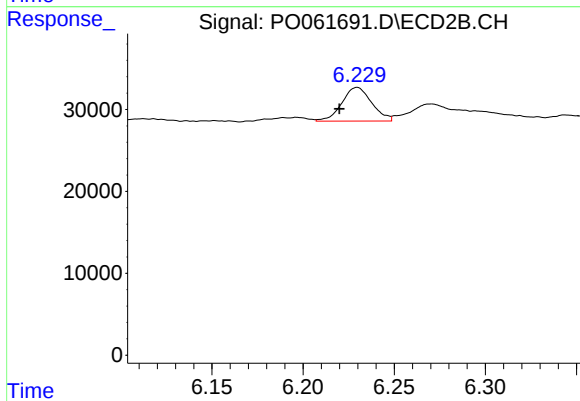

#32 AR-1260-2


R.T.: 6.230 min
Delta R.T.: 0.010 min
Response: 46841
Conc: 19.50 ng/ml

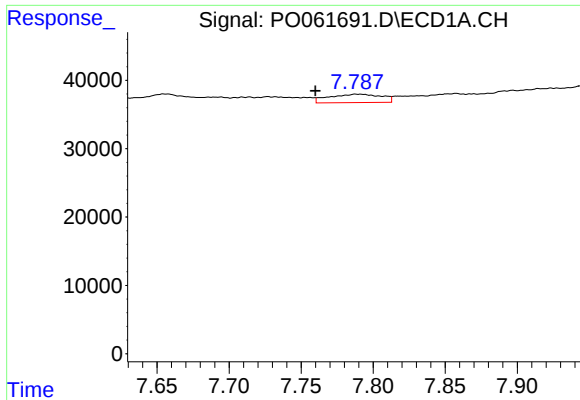

#33 AR-1260-3


R.T.: 7.788 min
Delta R.T.: 0.028 min
Response: 31163
Conc: 12.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

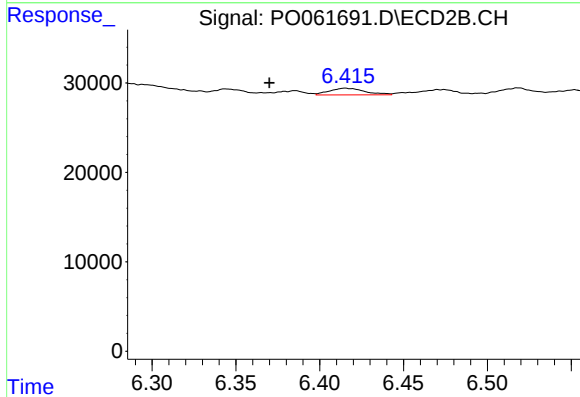


#33 AR-1260-3

R.T.: 6.415 min
Delta R.T.: 0.045 min
Response: 10845
Conc: 4.81 ng/ml

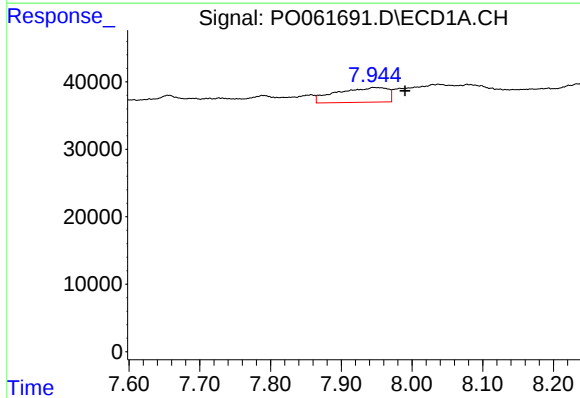


#34 AR-1260-4

R.T.: 7.945 min
Delta R.T.: -0.045 min
Response: 109595
Conc: 41.02 ng/ml

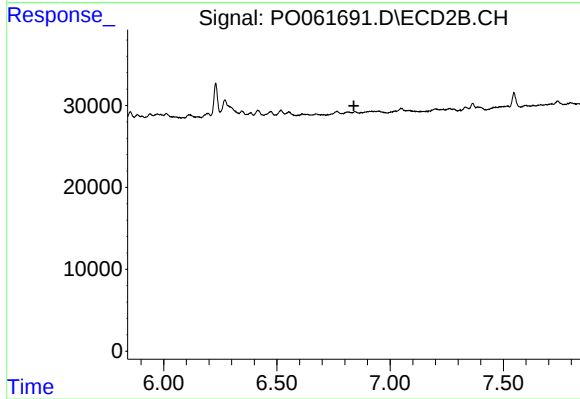

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 6.840 min
Response: 0
Conc: N.D.

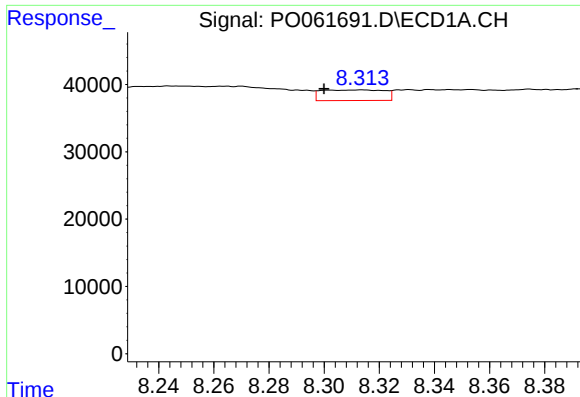

#35 AR-1260-5


R.T.: 8.314 min
Delta R.T.: 0.014 min
Response: 25114
Conc: 5.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

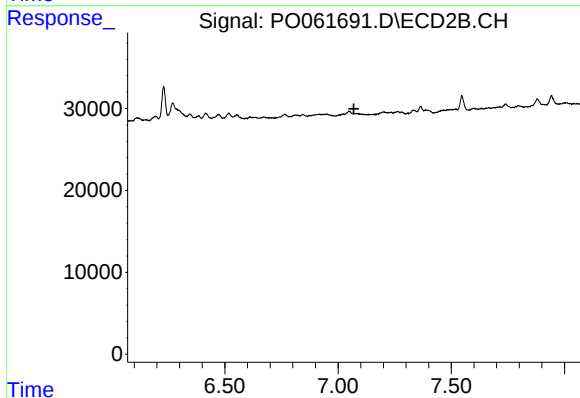


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.070 min
Response: 0
Conc: N.D.

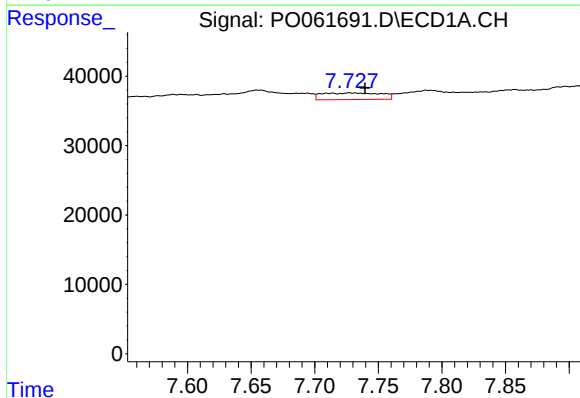


#36 AR-1262-1

R.T.: 7.727 min
Delta R.T.: -0.013 min
Response: 30767
Conc: 8.03 ng/ml

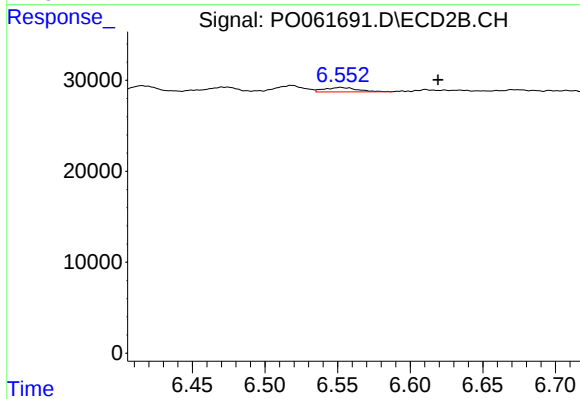

#36 AR-1262-1


R.T.: 6.552 min
Delta R.T.: -0.067 min
Response: 7645
Conc: 6.26 ng/ml

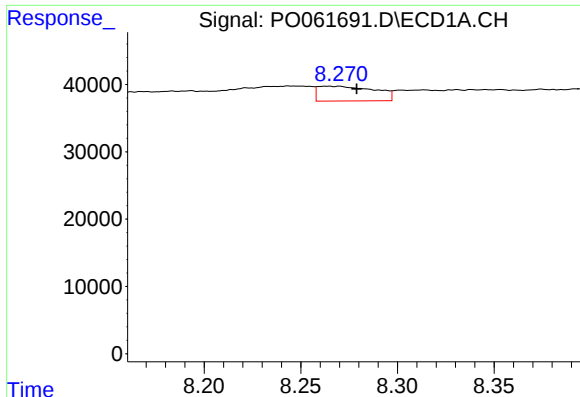

#37 AR-1262-2


R.T.: 8.270 min
Delta R.T.: -0.009 min
Response: 44906
Conc: 7.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

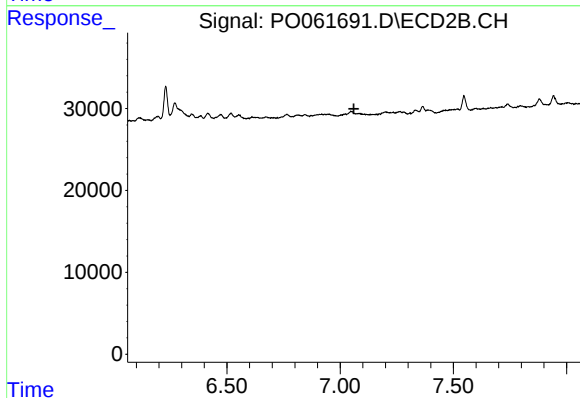


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.061 min
Response: 0
Conc: N.D.

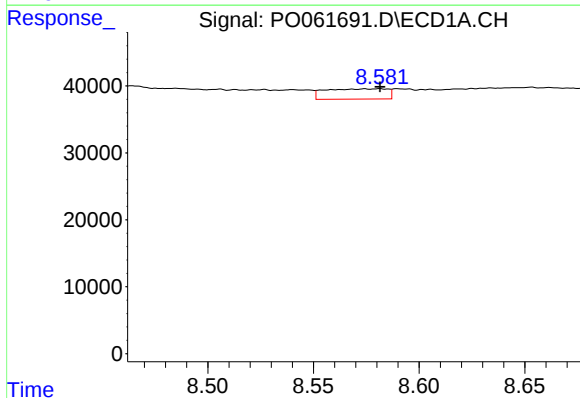


#38 AR-1262-3

R.T.: 8.581 min
Delta R.T.: 0.000 min
Response: 31193
Conc: 7.50 ng/ml

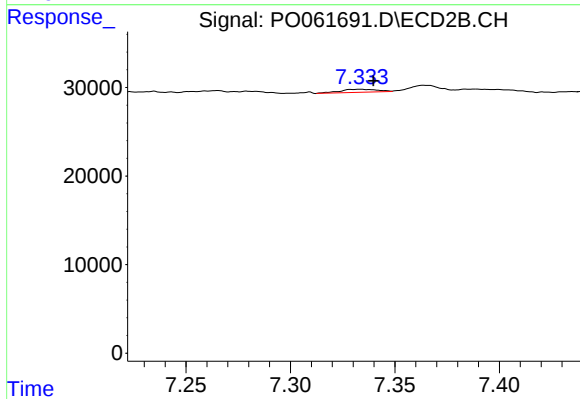

#38 AR-1262-3


R.T.: 7.333 min
Delta R.T.: -0.006 min
Response: 4364
Conc: 2.32 ng/ml

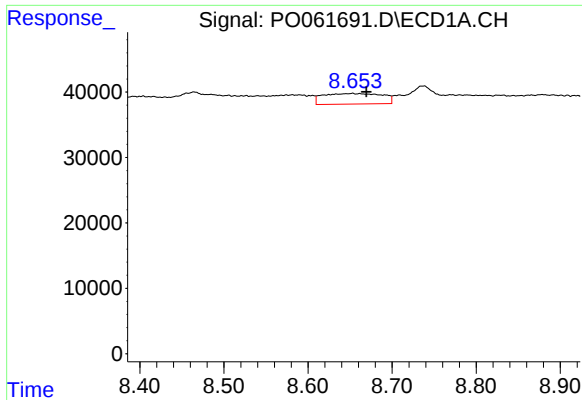

#39 AR-1262-4


R.T.: 8.653 min
Delta R.T.: -0.016 min
Response: 78598
Conc: 24.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

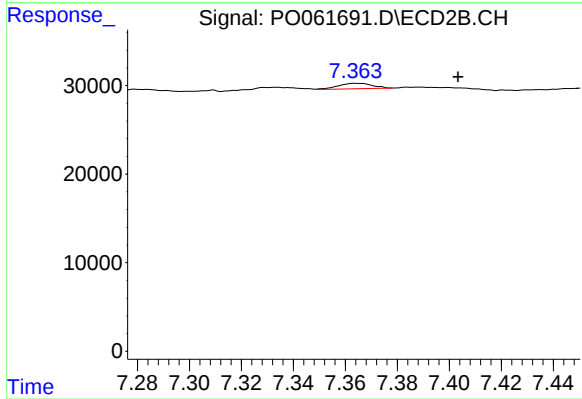


#39 AR-1262-4

R.T.: 7.364 min
Delta R.T.: -0.040 min
Response: 5650
Conc: 1.68 ng/ml

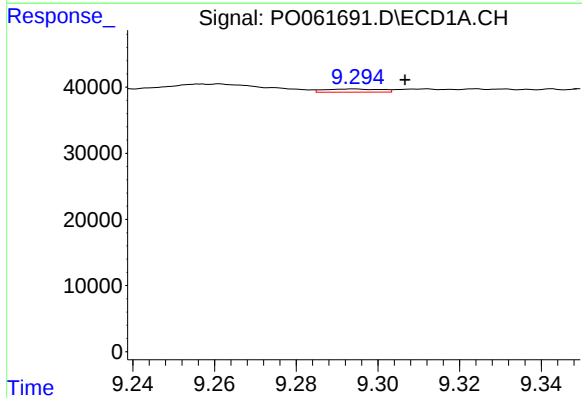


#40 AR-1262-5

R.T.: 9.294 min
Delta R.T.: -0.013 min
Response: 4673
Conc: 2.30 ng/ml

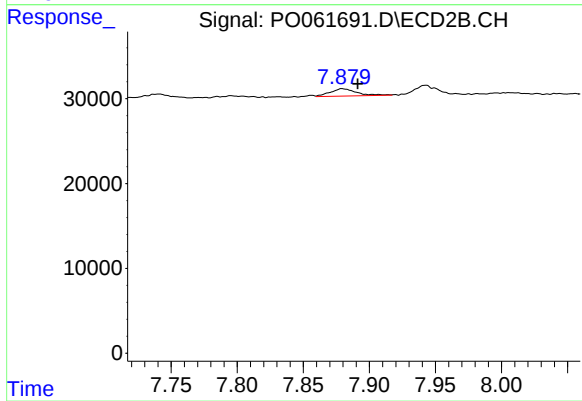

#40 AR-1262-5


R.T.: 7.879 min
Delta R.T.: -0.012 min
Response: 11912
Conc: 7.86 ng/ml

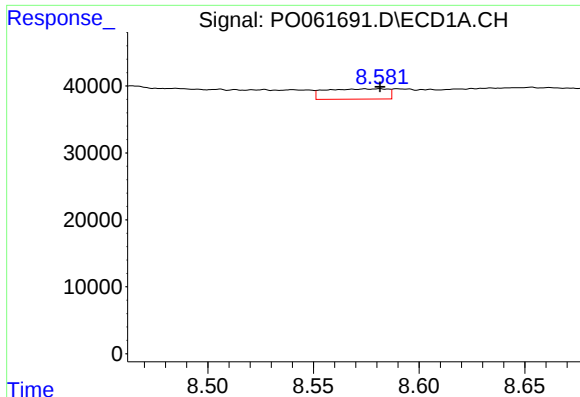

#41 AR-1268-1


R.T.: 8.581 min
Delta R.T.: 0.000 min
Response: 31193
Conc: 4.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

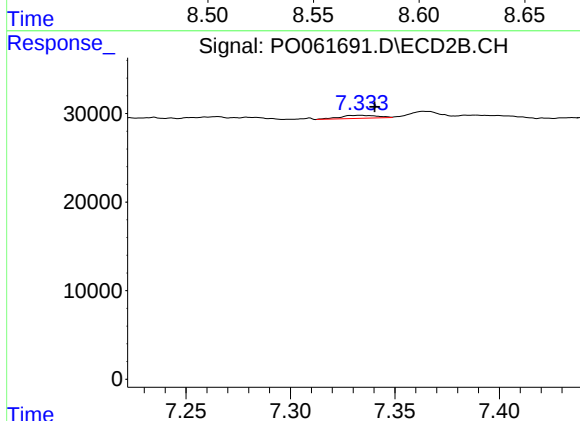


#41 AR-1268-1

R.T.: 7.333 min
Delta R.T.: -0.007 min
Response: 4364
Conc: 0.90 ng/ml

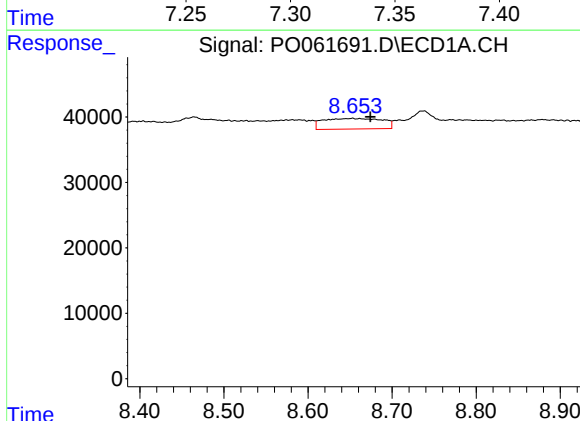


#42 AR-1268-2

R.T.: 8.653 min
Delta R.T.: -0.022 min
Response: 78598
Conc: 12.69 ng/ml

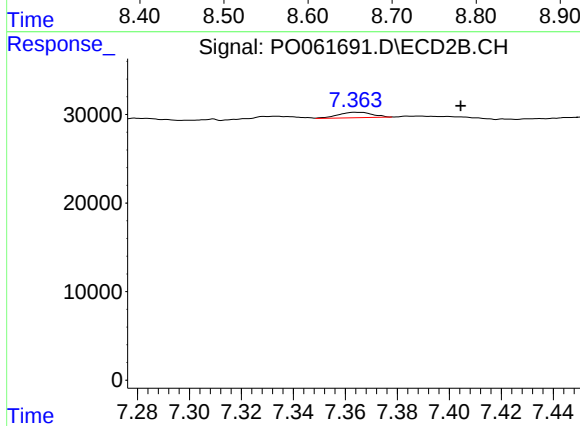

#42 AR-1268-2


R.T.: 7.364 min
Delta R.T.: -0.040 min
Response: 5650
Conc: 1.31 ng/ml

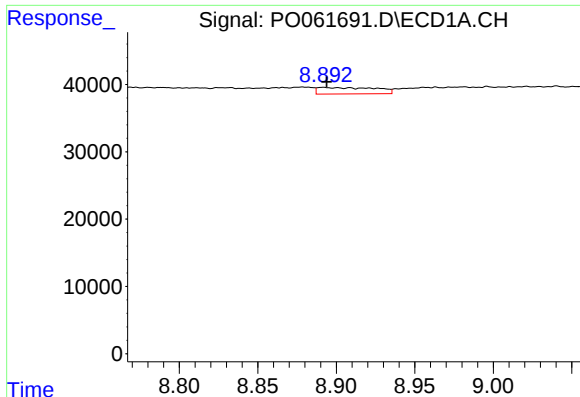

#43 AR-1268-3


R.T.: 8.892 min
Delta R.T.: -0.002 min
Response: 24642
Conc: 4.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

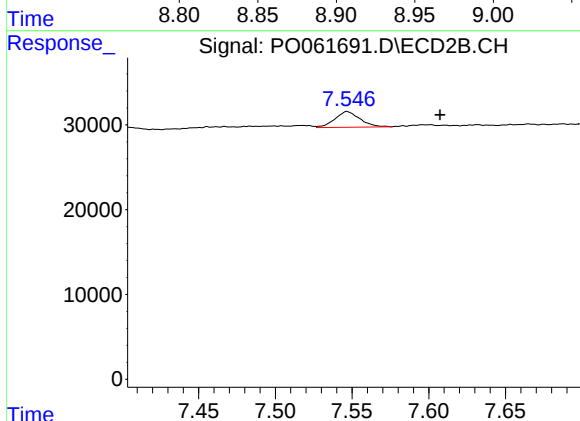


#43 AR-1268-3

R.T.: 7.547 min
Delta R.T.: -0.061 min
Response: 21098
Conc: 5.89 ng/ml

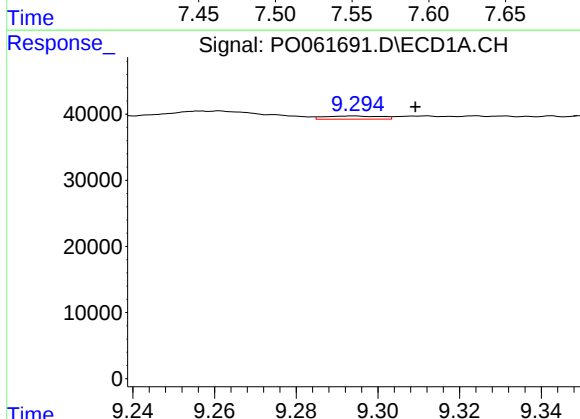


#44 AR-1268-4

R.T.: 9.294 min
Delta R.T.: -0.015 min
Response: 4673
Conc: 2.14 ng/ml

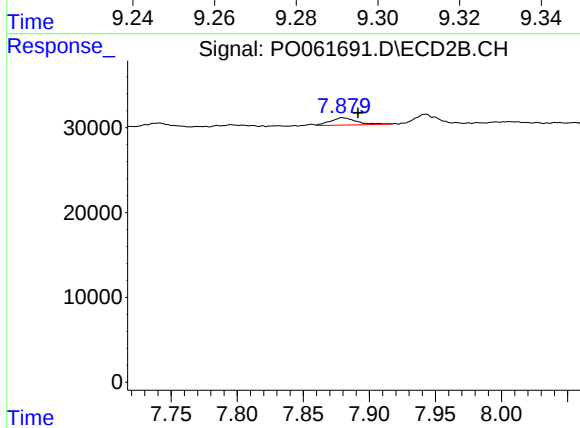

#44 AR-1268-4


R.T.: 7.879 min
Delta R.T.: -0.012 min
Response: 11912
Conc: 7.40 ng/ml

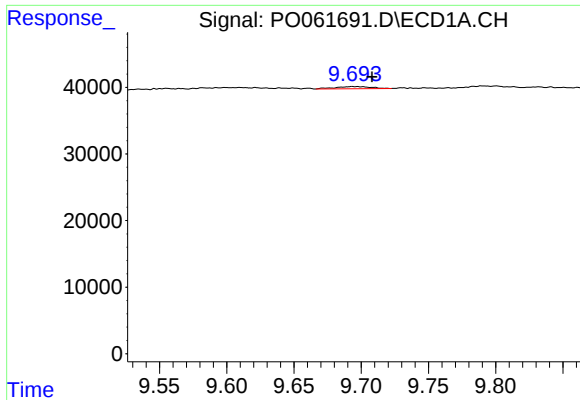

#45 AR-1268-5

R.T.: 9.694 min
Delta R.T.: -0.014 min
Response: 6000
Conc: 0.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-061RE

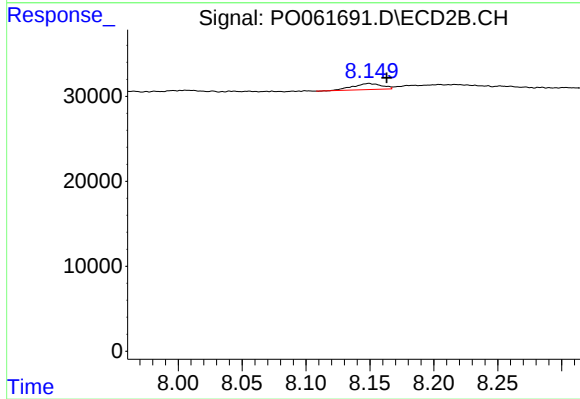

#45 AR-1268-5

R.T.: 8.149 min
Delta R.T.: -0.014 min
Response: 11291
Conc: 1.12 ng/ml