

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100419\
 Data File : P0061690.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Oct 2019 11:07
 Operator : HP/AJ
 Sample : K5156-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PSEG-GAS

Manual Integrations
 APPROVED

Ankita
 10/7/2019 10:34:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 14:00:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.358	3.517	710258	582860	17.317	18.023m
2) SA Decachlor...	10.017	8.382	569755	383182	12.234	11.835

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100419\
Data File : P0061690.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Oct 2019 11:07
Operator : HP/AJ
Sample : K5156-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PSEG-GAS


Manual Integrations
APPROVED

Ankita
10/7/2019 10:34:08 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 14:00:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

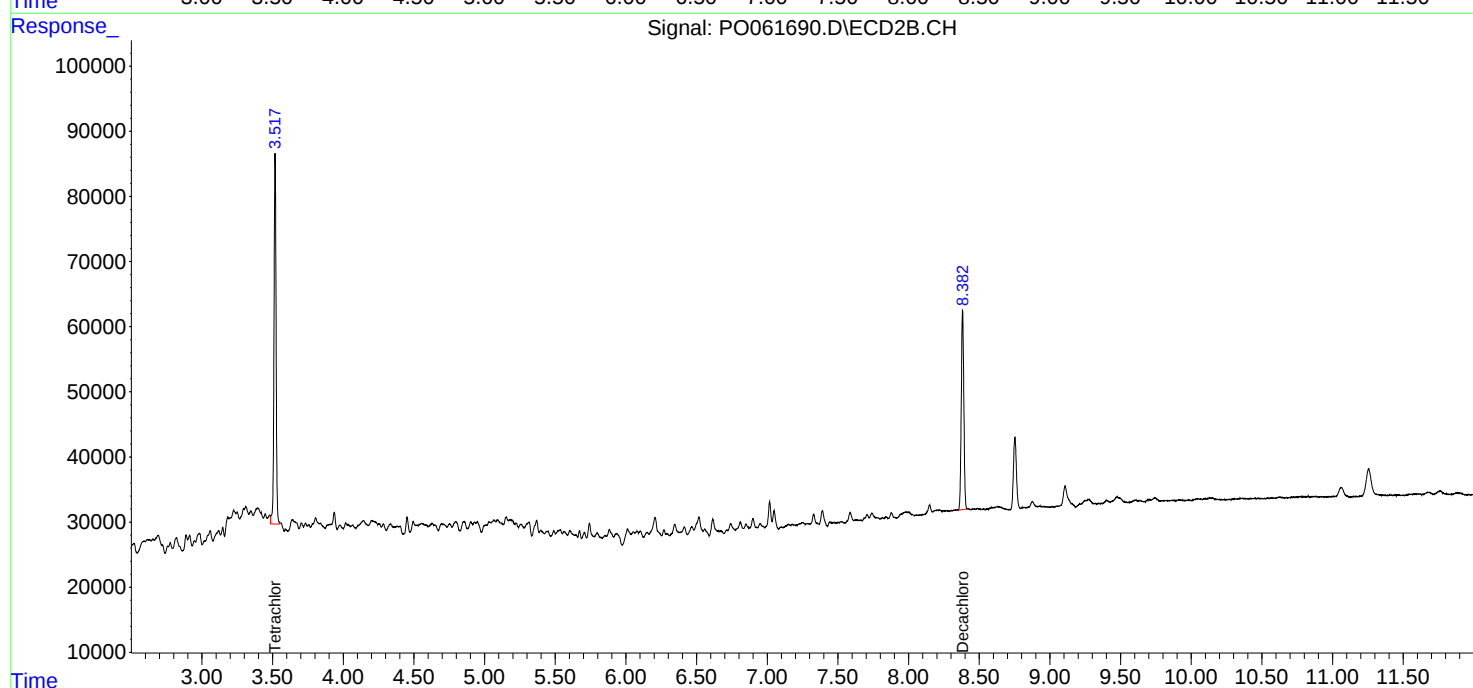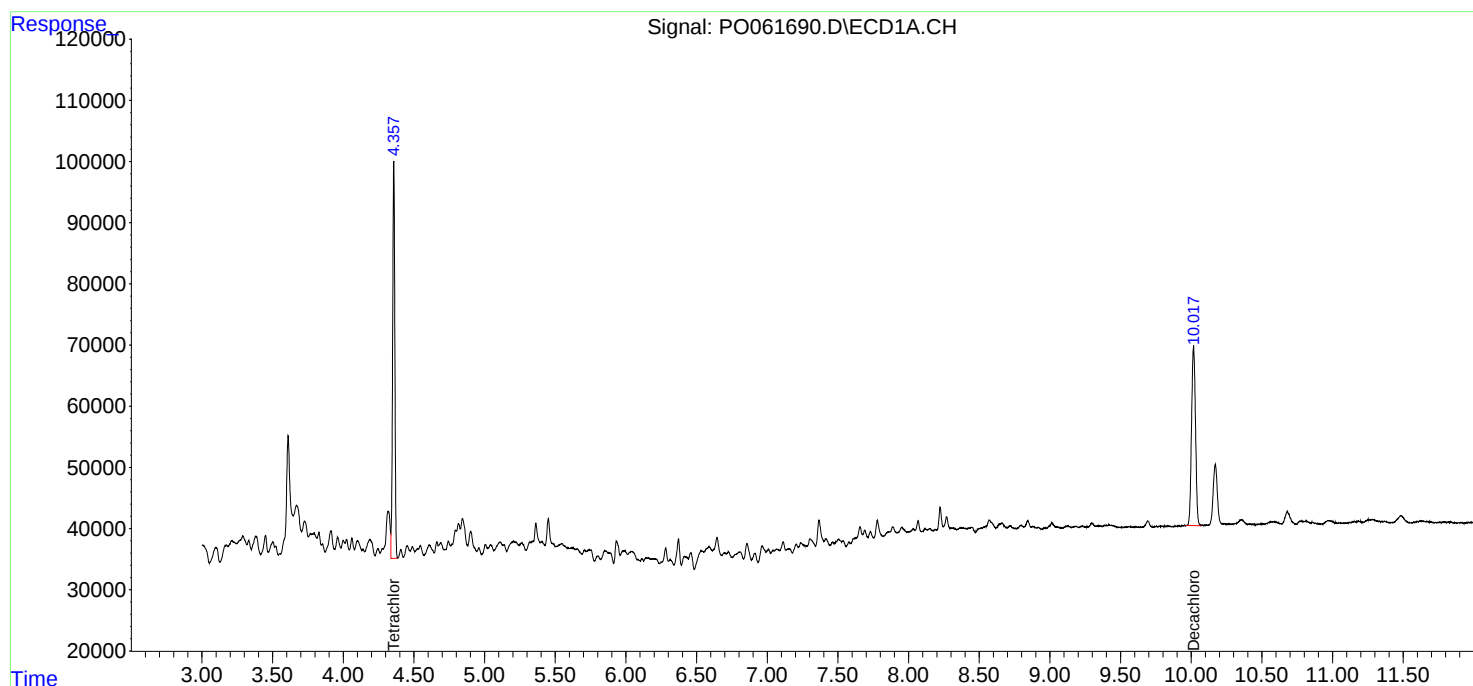

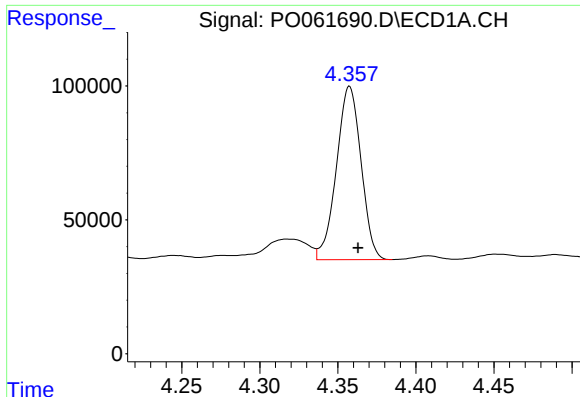


#1 Tetrachloro-m-xylene

R.T.: 4.358 min
Delta R.T.: -0.005 min
Response: 710258
Conc: 17.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
PSEG-GAS


Manual Integrations
APPROVED

Ankita
10/7/2019 10:34:08 AM

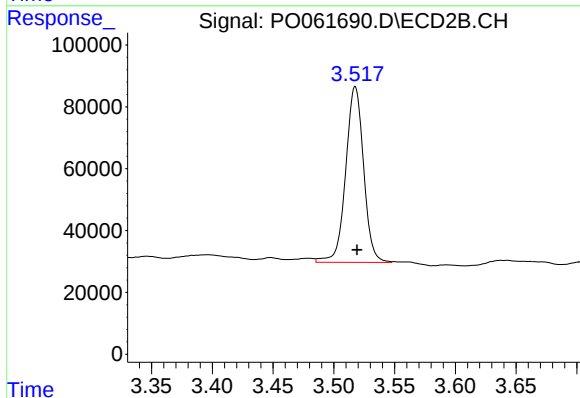


#1 Tetrachloro-m-xylene

R.T.: 3.517 min
Delta R.T.: -0.002 min
Response: 582860
Conc: 18.02 ng/ml m

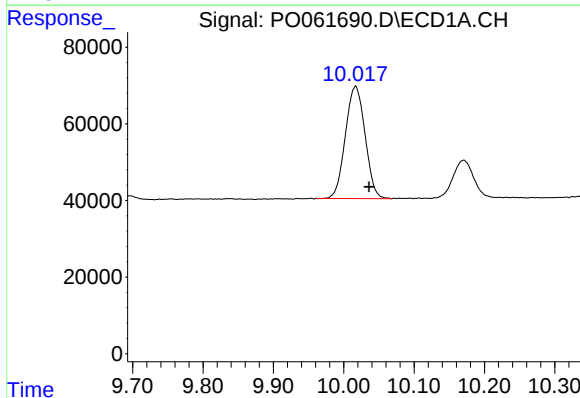

#2 Decachlorobiphenyl

R.T.: 10.017 min
Delta R.T.: -0.019 min
Response: 569755
Conc: 12.23 ng/ml

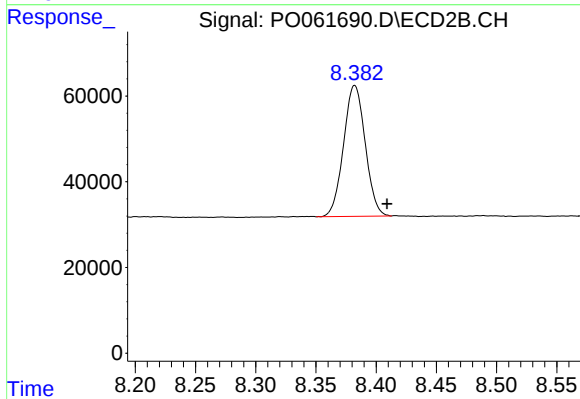

#2 Decachlorobiphenyl

R.T.: 8.382 min
Delta R.T.: -0.027 min
Response: 383182
Conc: 11.84 ng/ml