

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100419\
 Data File : PO061715.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Oct 2019 19:20
 Operator : HP/AJ
 Sample : K5193-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20190879-COMPOSITE-K

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 23:35:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.359	3.519	584435	491851	14.250	15.209
2) SA Decachlor...	10.019	8.382	588358	395221	12.634	12.207

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100419\
Data File : P0061715.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Oct 2019 19:20
Operator : HP/AJ
Sample : K5193-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20190879-COMPOSITE-K

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 23:35:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

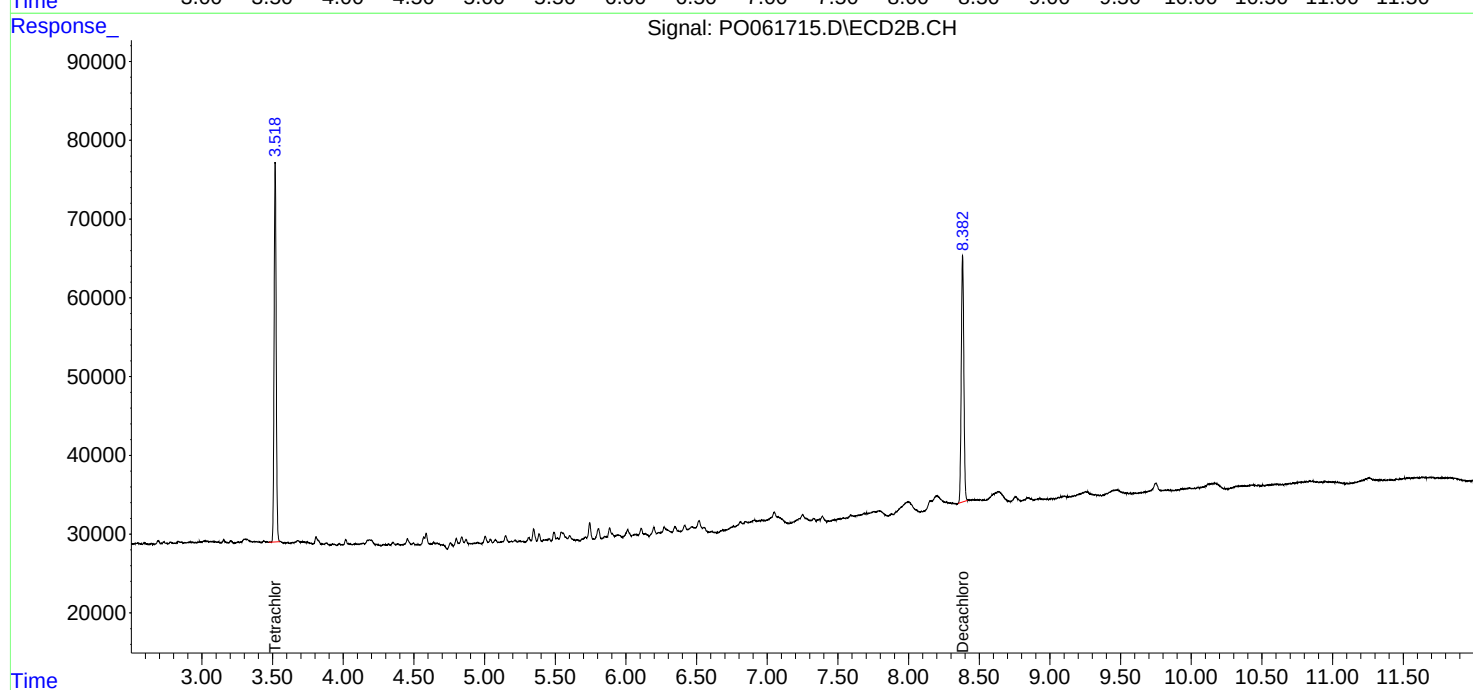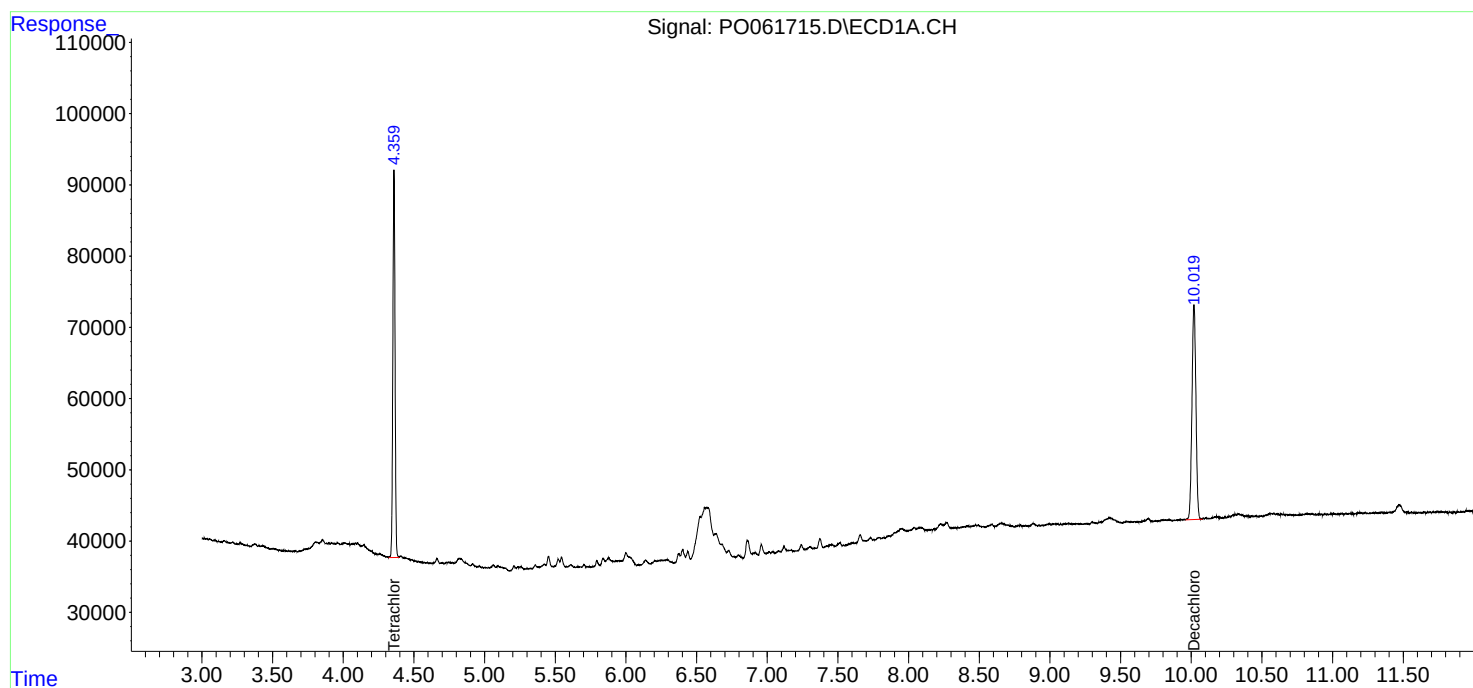


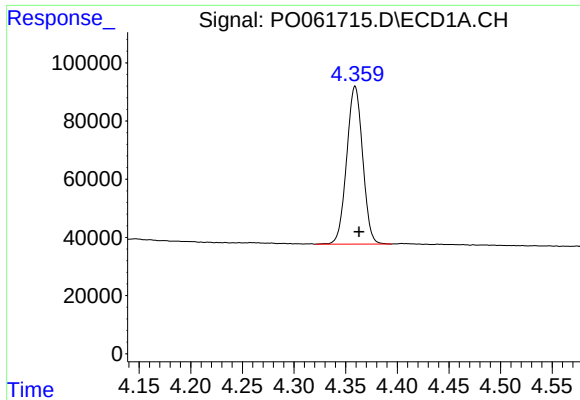

#1 Tetrachloro-m-xylene


R.T.: 4.359 min
Delta R.T.: -0.004 min
Response: 584435
Conc: 14.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
20190879-COMPOSITE-K

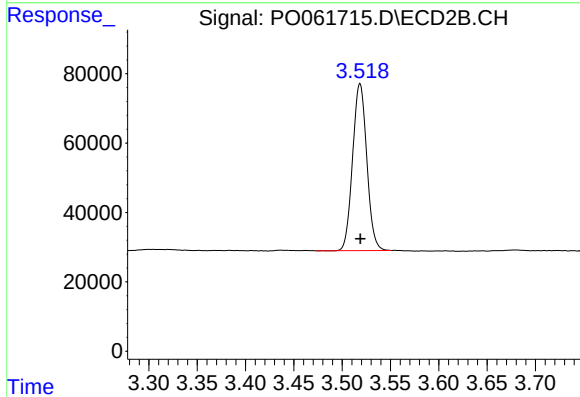


#1 Tetrachloro-m-xylene

R.T.: 3.519 min
Delta R.T.: 0.000 min
Response: 491851
Conc: 15.21 ng/ml

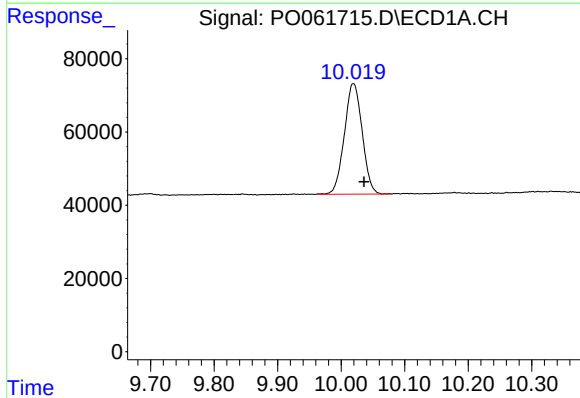

#2 Decachlorobiphenyl

R.T.: 10.019 min
Delta R.T.: -0.017 min
Response: 588358
Conc: 12.63 ng/ml

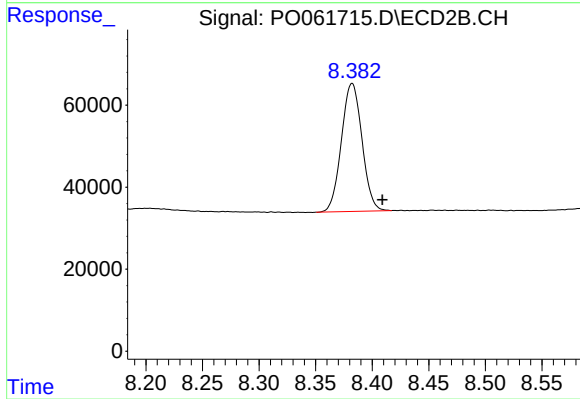

#2 Decachlorobiphenyl

R.T.: 8.382 min
Delta R.T.: -0.027 min
Response: 395221
Conc: 12.21 ng/ml