

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100419\
 Data File : P0061721.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Oct 2019 20:58
 Operator : HP/AJ
 Sample : K5204-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RBR-200055-RT-1868

Manual Integrations
 APPROVED

Ankita
 10/7/2019 10:35:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 23:38:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.358	3.519	947896	727835	23.111	22.506
2) SA Decachlor...	10.016	8.381	805687	488155	17.300	15.078m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100419\
Data File : P0061721.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Oct 2019 20:58
Operator : HP/AJ
Sample : K5204-01
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RBR-200055-RT-1868


Manual Integrations
APPROVED

Ankita
10/7/2019 10:35:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 23:38:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

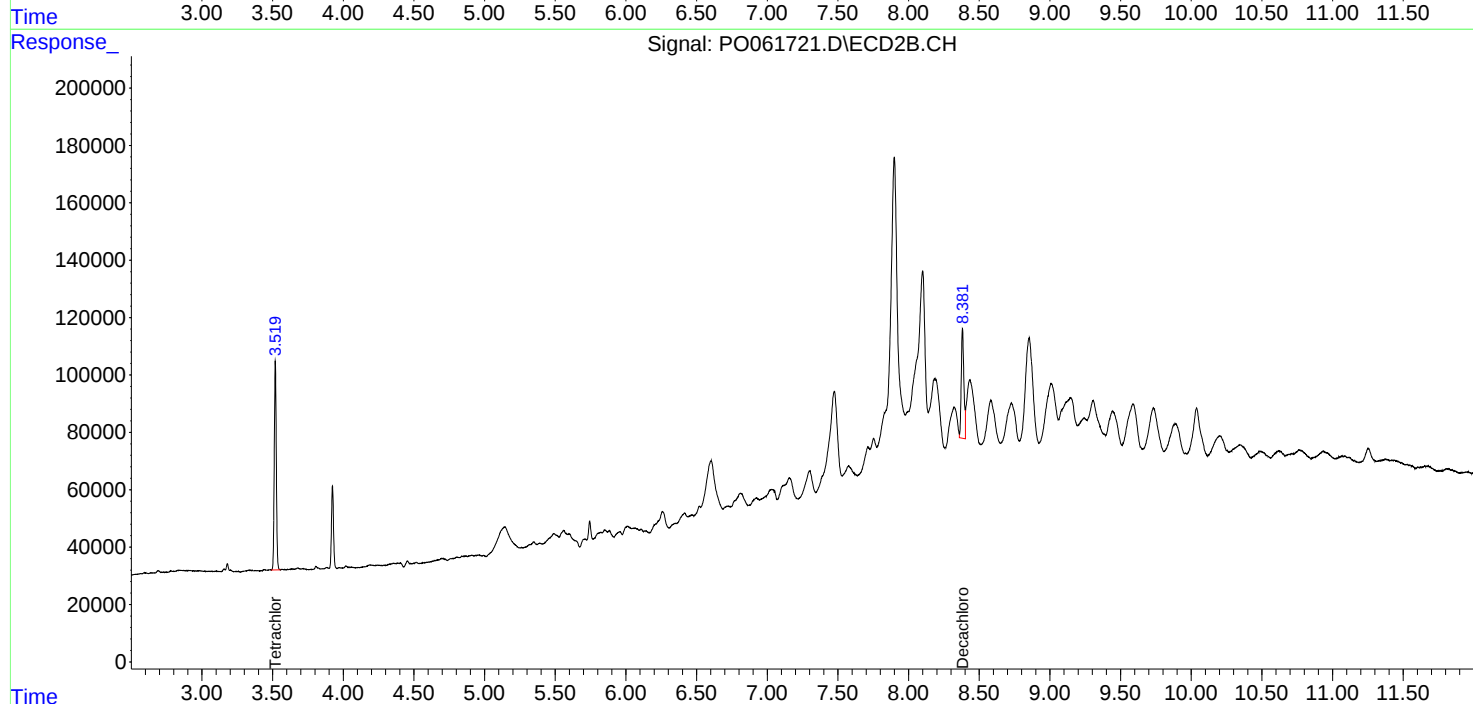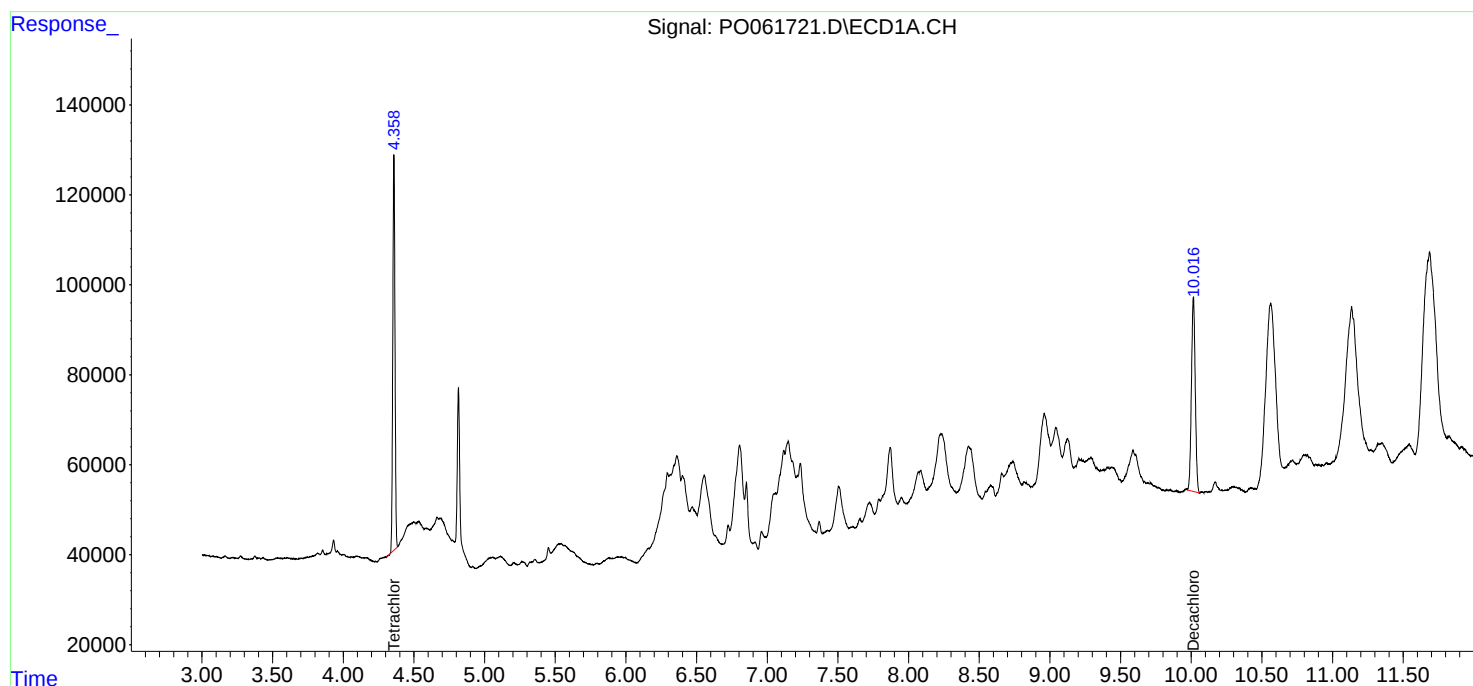

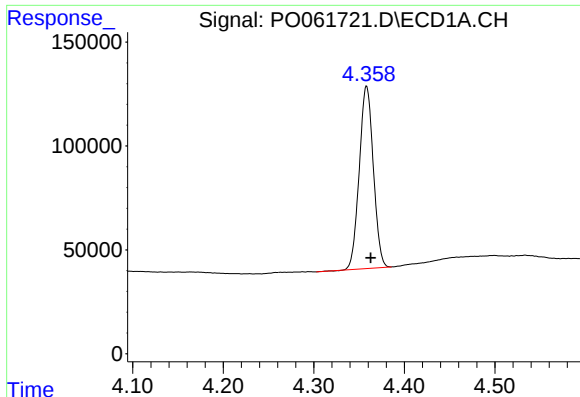


#1 Tetrachloro-m-xylene

R.T.: 4.358 min
Delta R.T.: -0.005 min
Response: 947896
Conc: 23.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
RBR-200055-RT-1868


Manual Integrations
APPROVED

Ankita
10/7/2019 10:35:03 AM

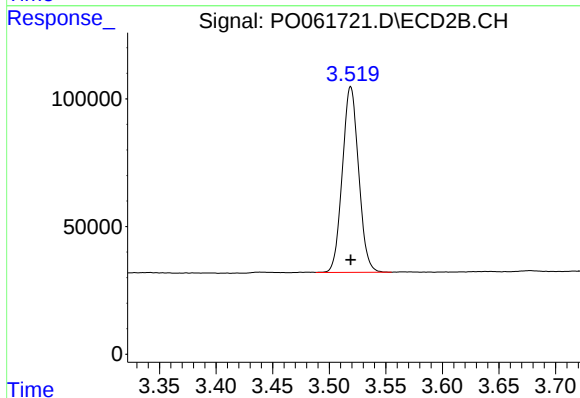


#1 Tetrachloro-m-xylene

R.T.: 3.519 min
Delta R.T.: 0.000 min
Response: 727835
Conc: 22.51 ng/ml

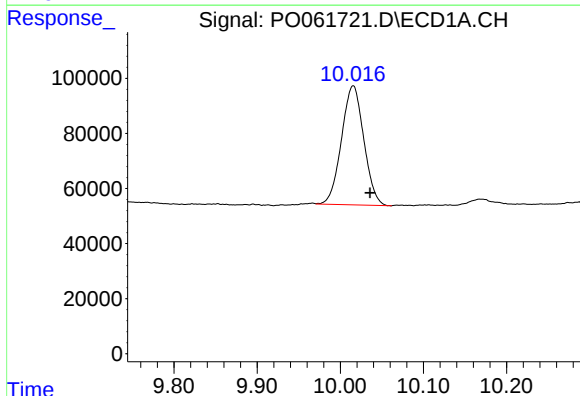

#2 Decachlorobiphenyl

R.T.: 10.016 min
Delta R.T.: -0.020 min
Response: 805687
Conc: 17.30 ng/ml

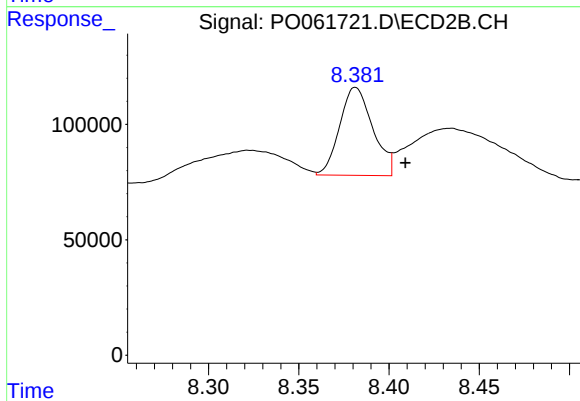

#2 Decachlorobiphenyl

R.T.: 8.381 min
Delta R.T.: -0.028 min
Response: 488155
Conc: 15.08 ng/ml m