

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100620\
Data File : P0072064.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Oct 2020 22:00
Operator : DD\AJ
Sample : L4272-40
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SC-7-(6.5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 02:36:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.327	3.511	1901983	888816	26.480	23.729
2)	SA Decachlor...	9.934	8.685	2249072	1134901	20.426	19.953

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100620\
Data File : PO072064.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Oct 2020 22:00
Operator : DD\AJ
Sample : L4272-40
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SC-7-(6.5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 02:36:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

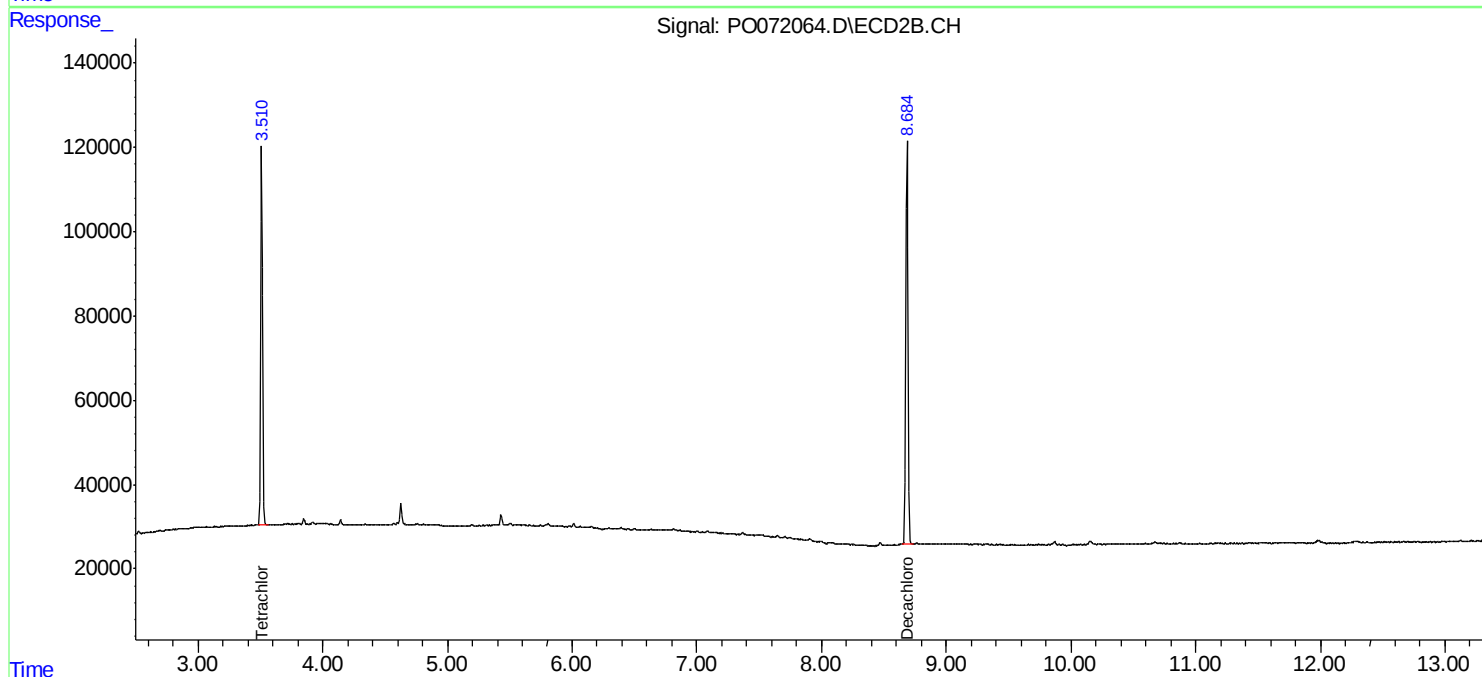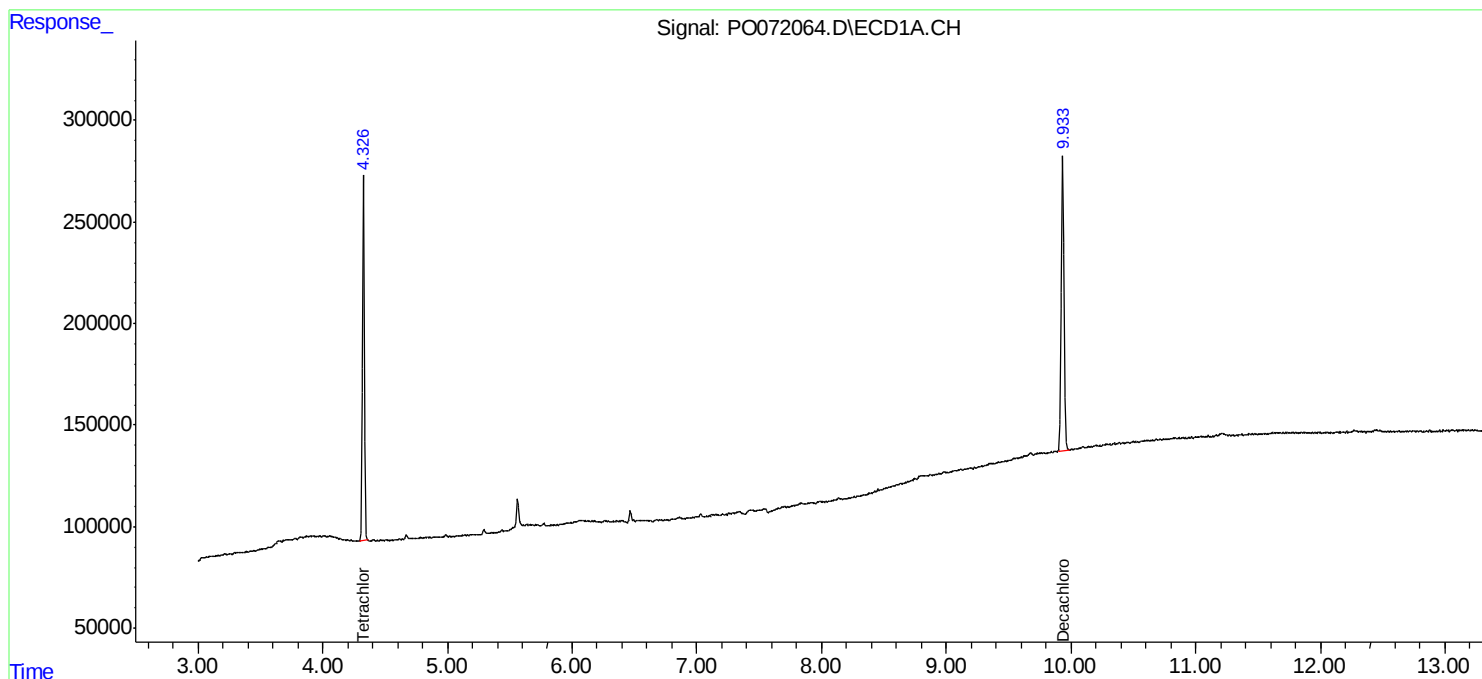


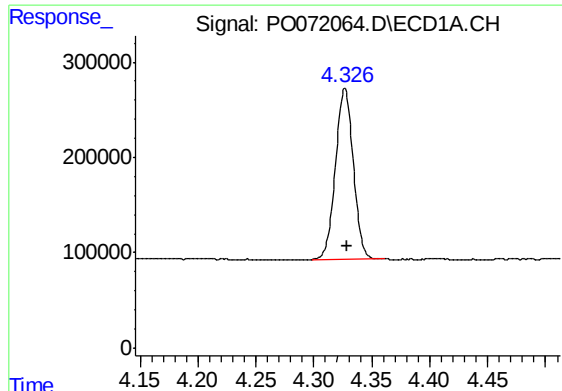

#1 Tetrachloro-m-xylene


R.T.: 4.327 min
Delta R.T.: -0.002 min
Response: 1901983
Conc: 26.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
SC-7-(6.5)

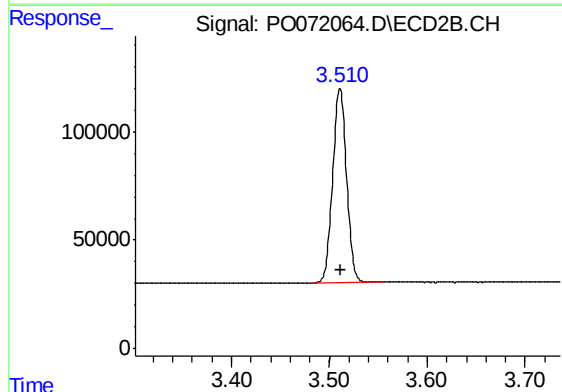


#1 Tetrachloro-m-xylene

R.T.: 3.511 min
Delta R.T.: -0.002 min
Response: 888816
Conc: 23.73 ng/ml

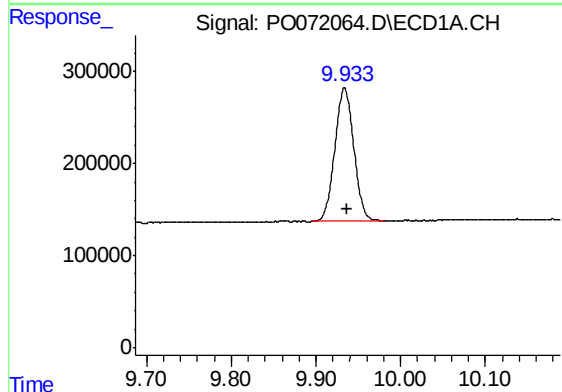

#2 Decachlorobiphenyl

R.T.: 9.934 min
Delta R.T.: -0.003 min
Response: 2249072
Conc: 20.43 ng/ml

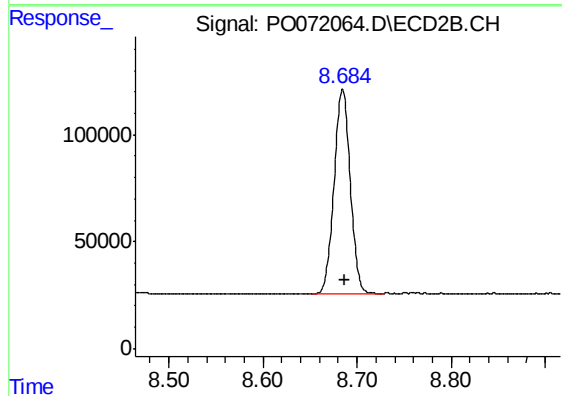

#2 Decachlorobiphenyl

R.T.: 8.685 min
Delta R.T.: -0.002 min
Response: 1134901
Conc: 19.95 ng/ml