

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100620\
 Data File : P0072075.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Oct 2020 1:08
 Operator : DD\AJ
 Sample : L4270-01
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TOTE-COMP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 02:40:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.326	3.511	1696685	819700	23.622	21.884
2)	SA Decachlor...	9.933	8.683	1587503	830820	14.418	14.607

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100620\
Data File : PO072075.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Oct 2020 1:08
Operator : DD\AJ
Sample : L4270-01
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TOTE-COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 02:40:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

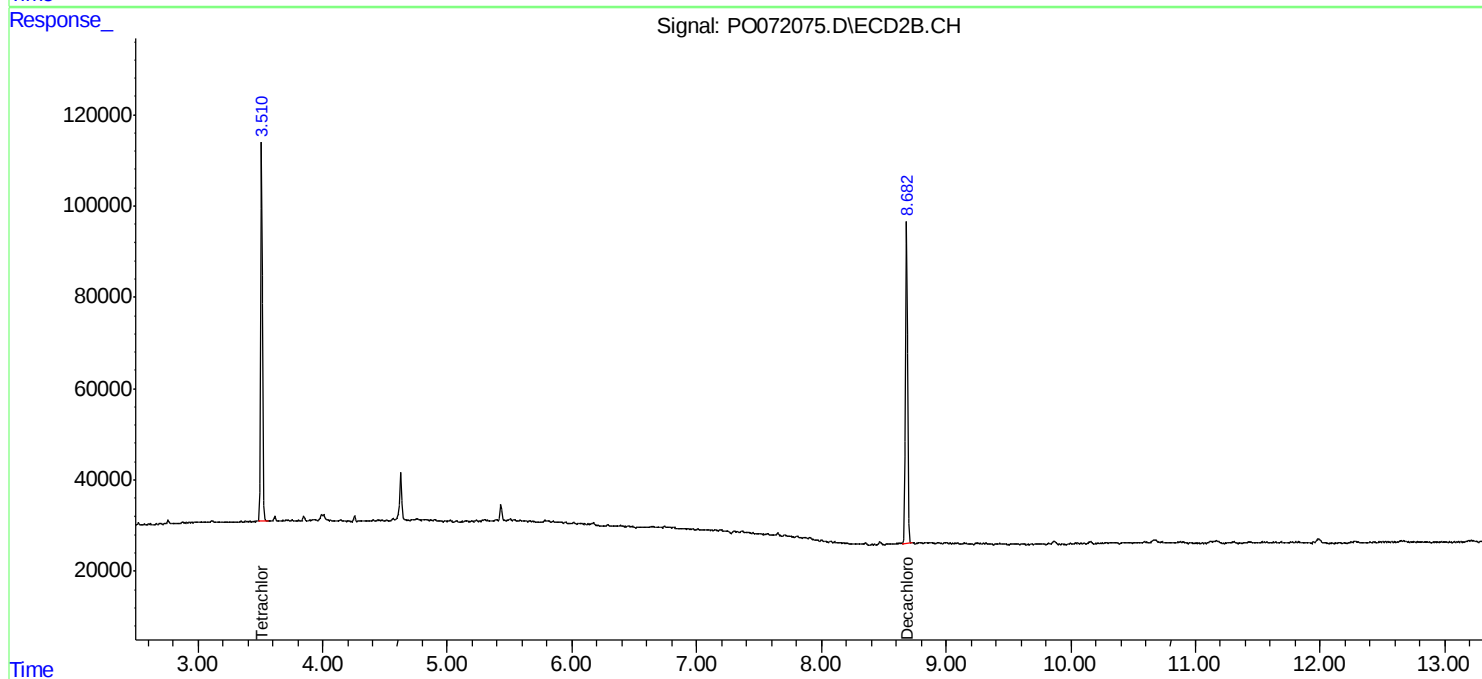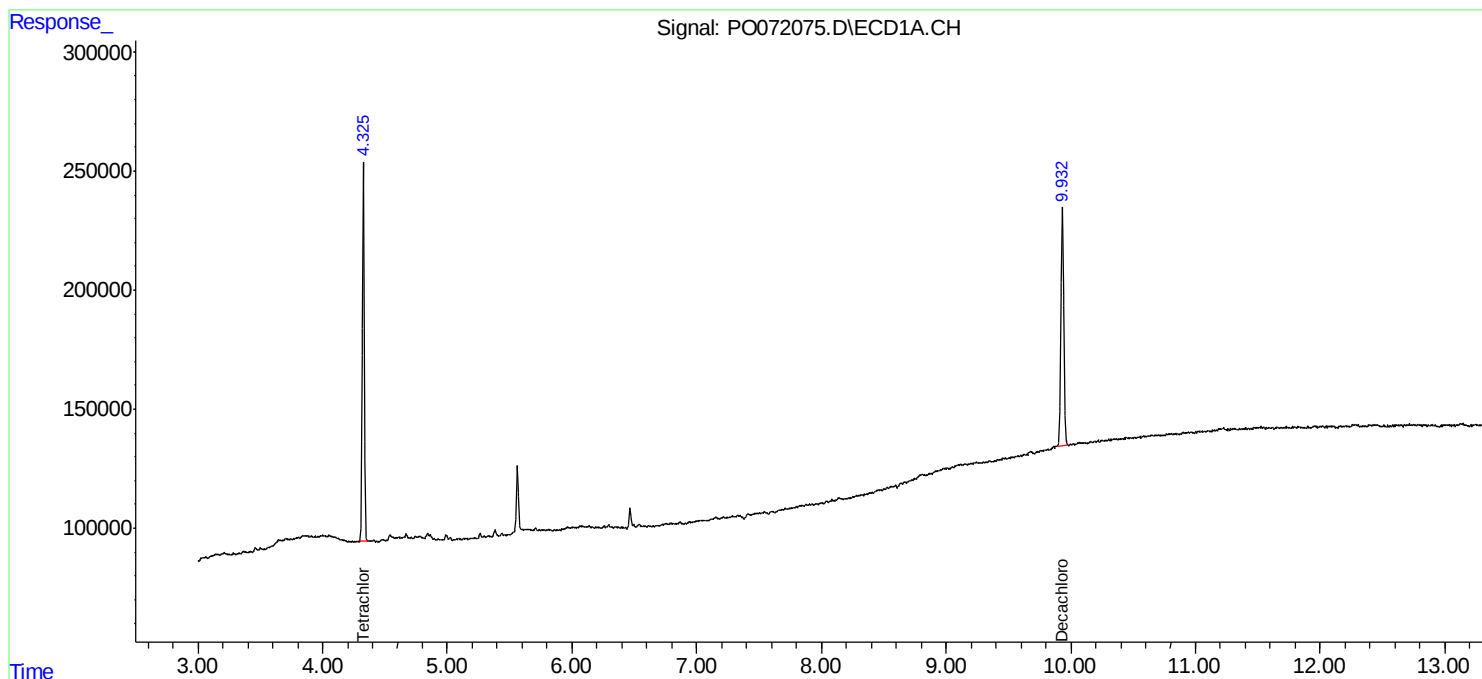


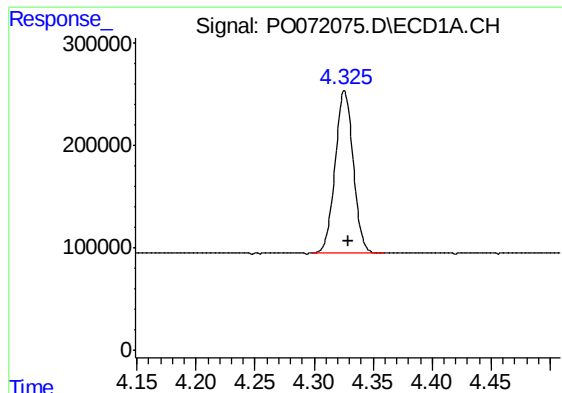

#1 Tetrachloro-m-xylene


R.T.: 4.326 min
Delta R.T.: -0.003 min
Response: 1696685
Conc: 23.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
TOTE-COMP-1

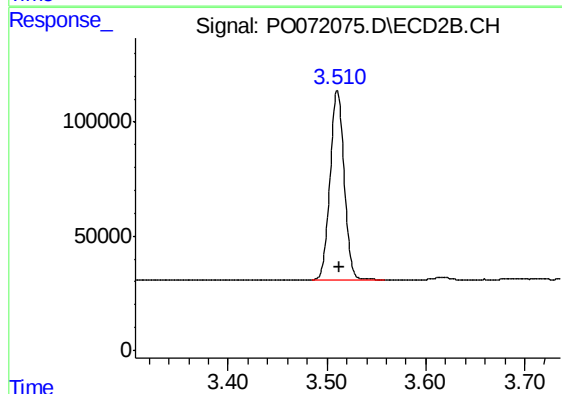


#1 Tetrachloro-m-xylene

R.T.: 3.511 min
Delta R.T.: -0.002 min
Response: 819700
Conc: 21.88 ng/ml

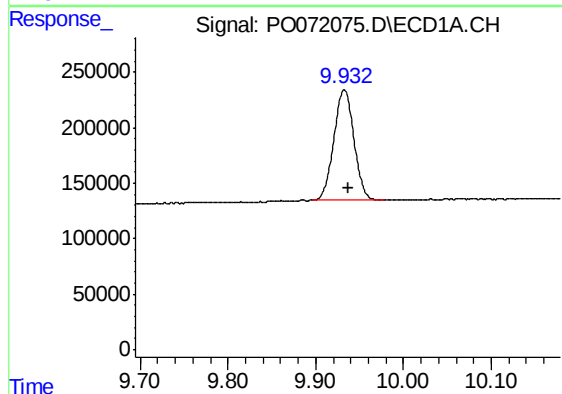

#2 Decachlorobiphenyl

R.T.: 9.933 min
Delta R.T.: -0.004 min
Response: 1587503
Conc: 14.42 ng/ml

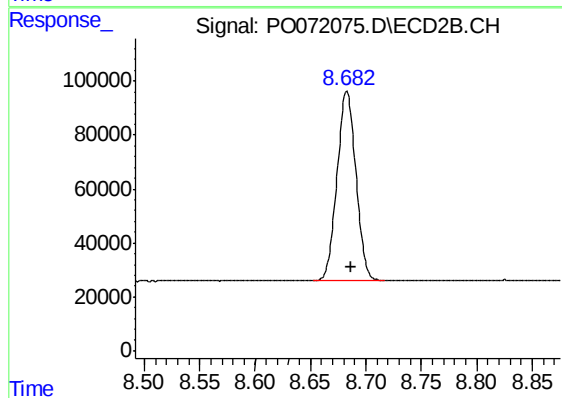

#2 Decachlorobiphenyl

R.T.: 8.683 min
Delta R.T.: -0.004 min
Response: 830820
Conc: 14.61 ng/ml