

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100620\
 Data File : P0072076.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Oct 2020 1:25
 Operator : DD\AJ
 Sample : L4270-03
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TOTE-COMP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 02:40:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.326	3.510	1816990	875387	25.297	23.371
2) SA Decachlor...	9.932	8.683	1900048	981616	17.256	17.258
Target Compounds						
8) L2 AR-1221-1	4.559f	0.000	874	0	1.185	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100620\
Data File : PO072076.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Oct 2020 1:25
Operator : DD\AJ
Sample : L4270-03
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TOTE-COMP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 02:40:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

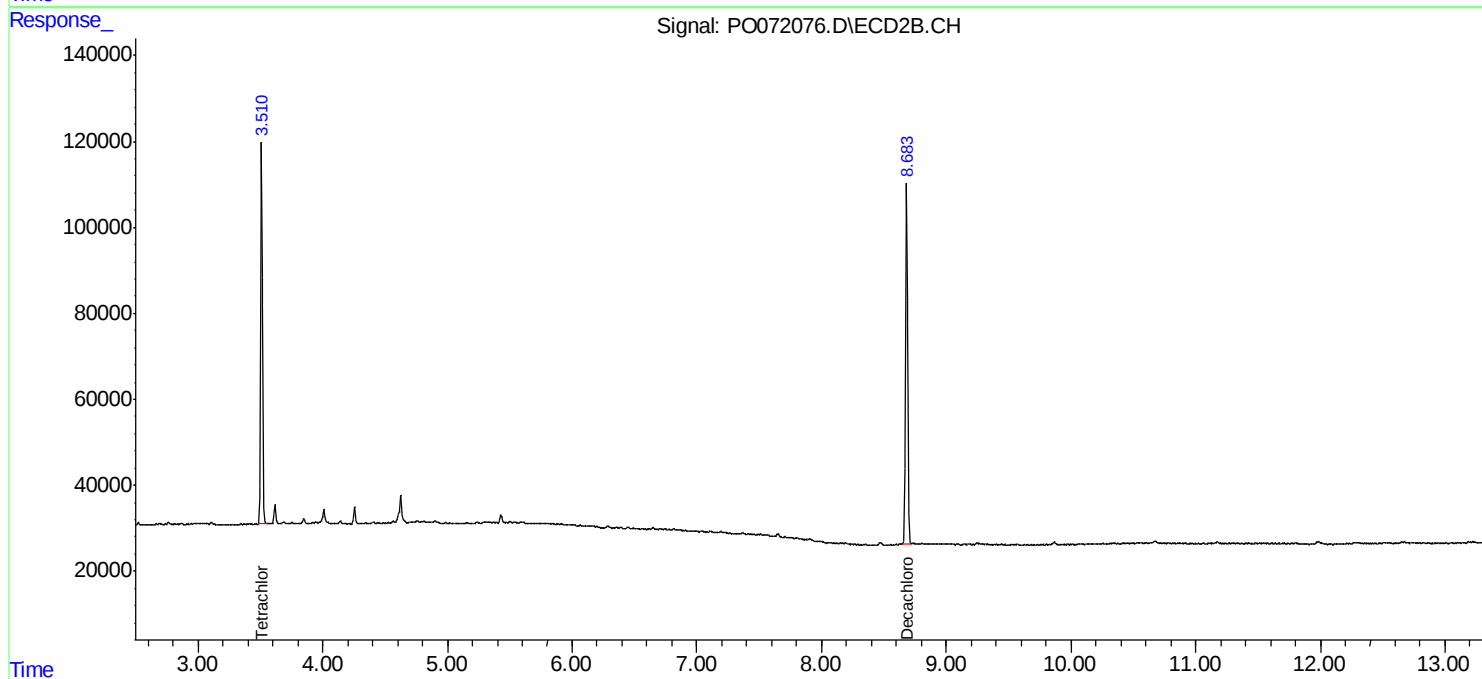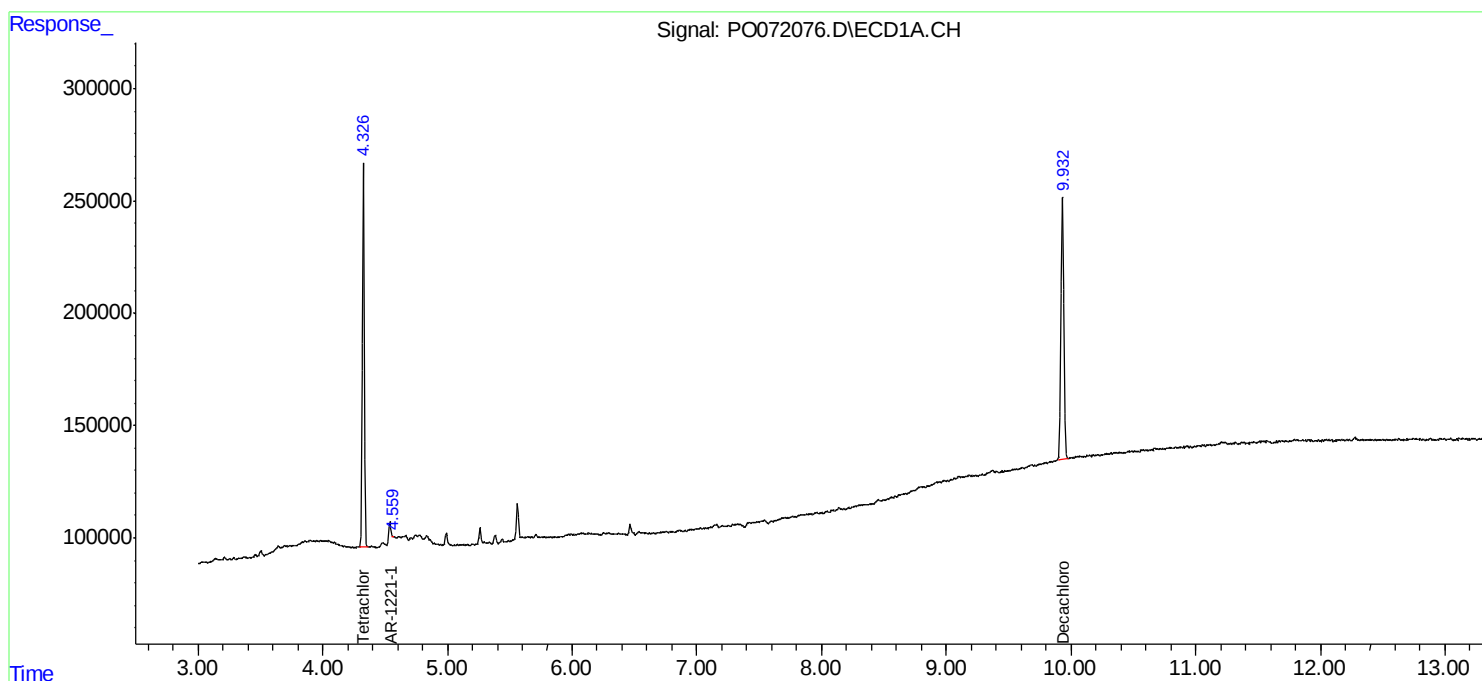


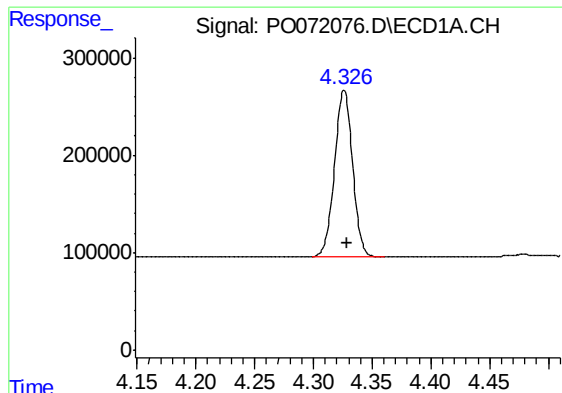

#1 Tetrachloro-m-xylene


R.T.: 4.326 min
Delta R.T.: -0.003 min
Response: 1816990
Conc: 25.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
TOTE-COMP-2

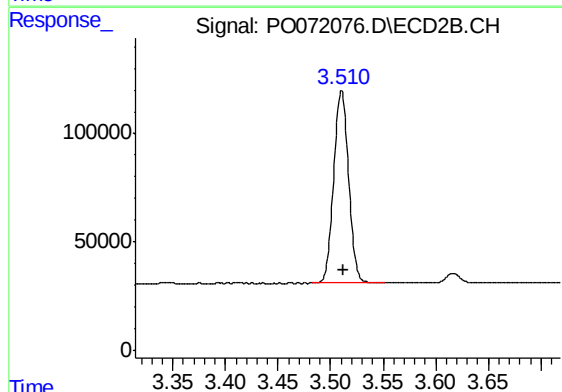


#1 Tetrachloro-m-xylene

R.T.: 3.510 min
Delta R.T.: -0.002 min
Response: 875387
Conc: 23.37 ng/ml

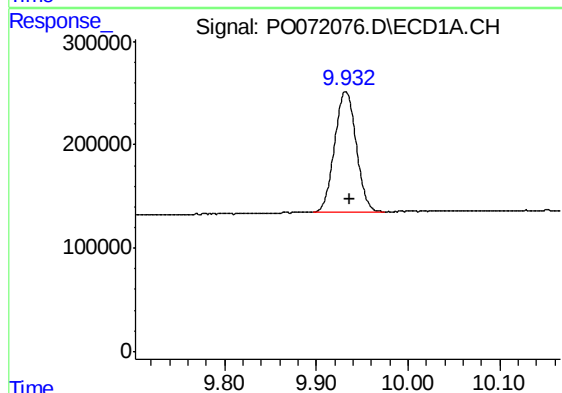


#2 Decachlorobiphenyl

R.T.: 9.932 min
Delta R.T.: -0.005 min
Response: 1900048
Conc: 17.26 ng/ml

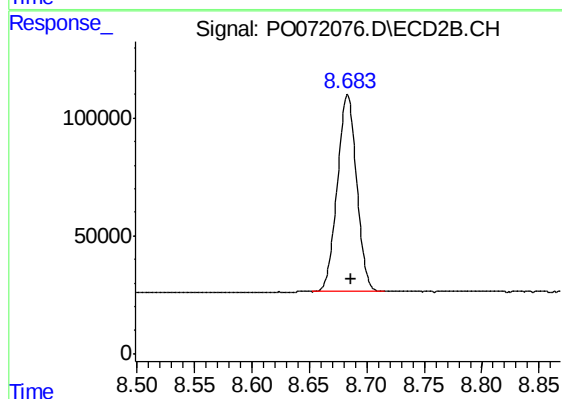

#2 Decachlorobiphenyl


R.T.: 8.683 min
Delta R.T.: -0.003 min
Response: 981616
Conc: 17.26 ng/ml

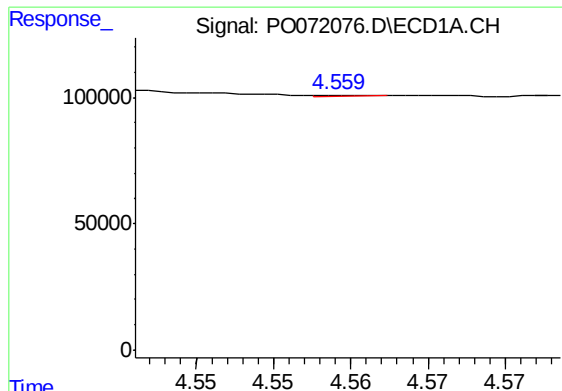

#8 AR-1221-1

R.T.: 4.559 min
Delta R.T.: -0.026 min
Response: 874
Conc: 1.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
TOTE-COMP-2

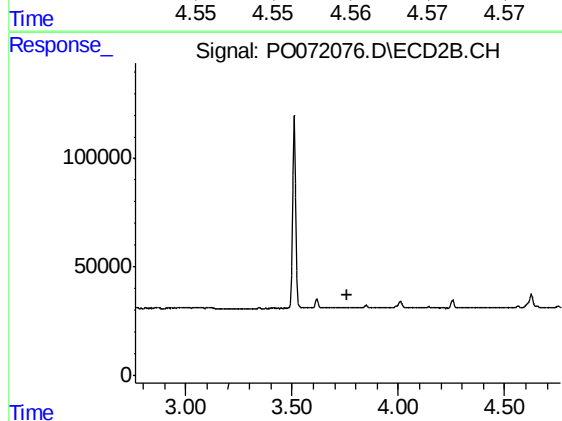

#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 3.763 min
Response: 0
Conc: N.D.