

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100620\
 Data File : P0072077.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Oct 2020 1:43
 Operator : DD\AJ
 Sample : L4270-05
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TOTE-COMP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 02:40:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.326	3.510	1847969	884677	25.728	23.619
2)	SA Decachlor...	9.933	8.682	1808814	940170	16.428	16.529

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100620\
Data File : PO072077.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Oct 2020 1:43
Operator : DD\AJ
Sample : L4270-05
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TOTE-COMP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 02:40:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

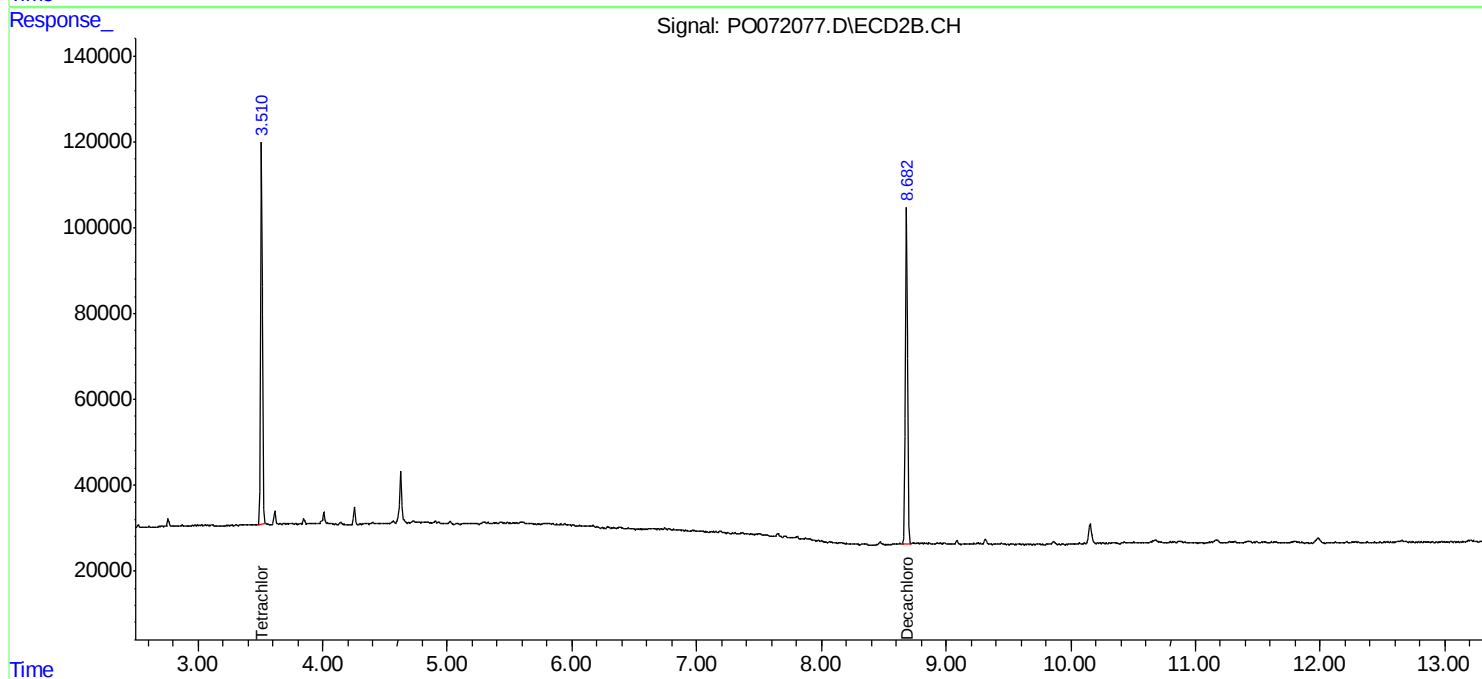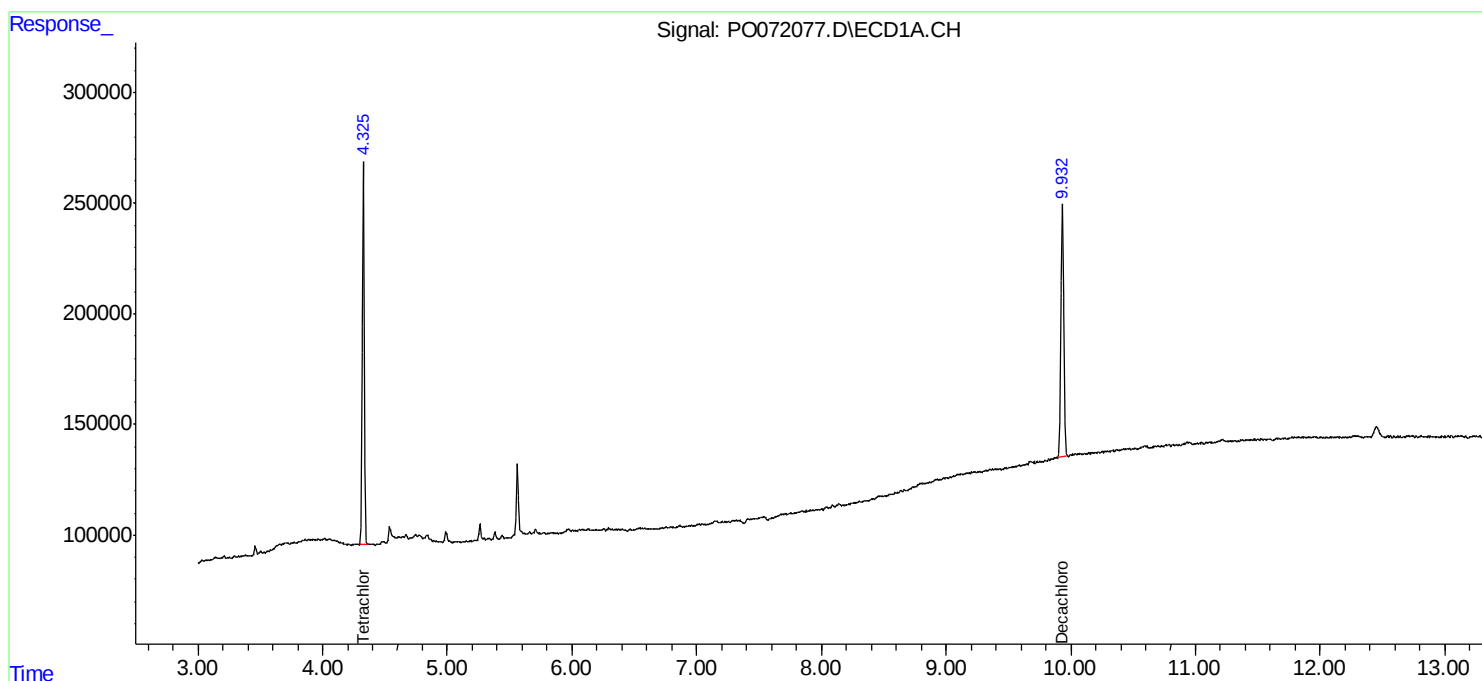


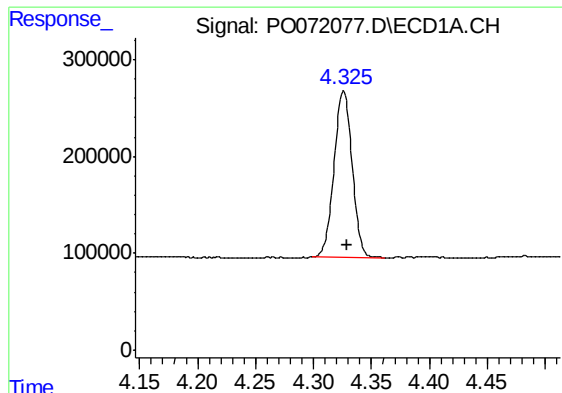

#1 Tetrachloro-m-xylene


R.T.: 4.326 min
Delta R.T.: -0.003 min
Response: 1847969
Conc: 25.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
TOTE-COMP-3

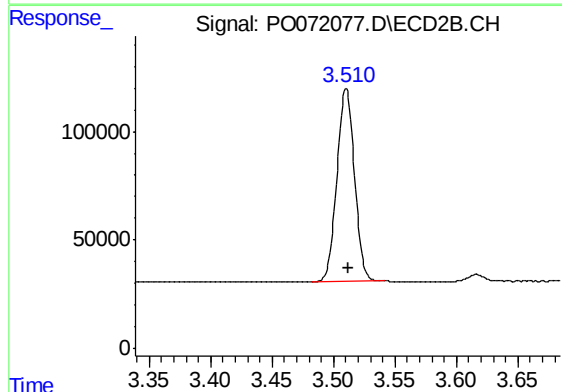


#1 Tetrachloro-m-xylene

R.T.: 3.510 min
Delta R.T.: -0.002 min
Response: 884677
Conc: 23.62 ng/ml

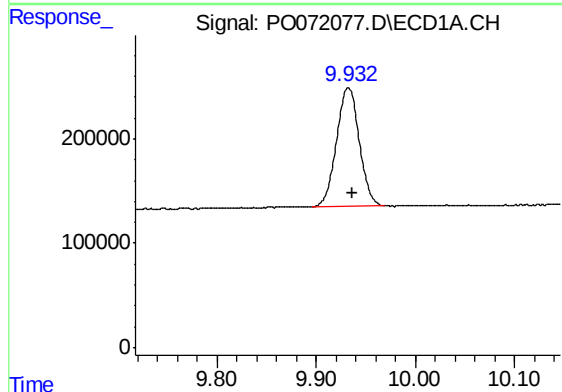

#2 Decachlorobiphenyl

R.T.: 9.933 min
Delta R.T.: -0.004 min
Response: 1808814
Conc: 16.43 ng/ml

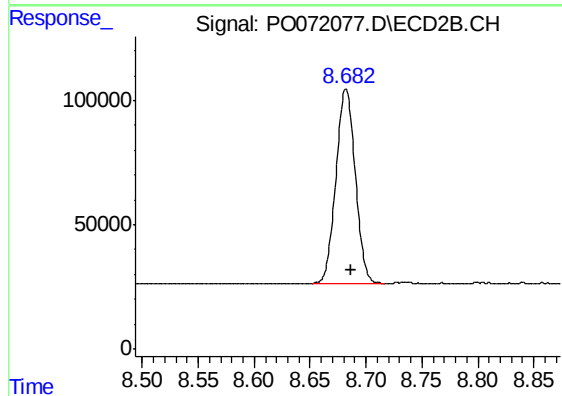

#2 Decachlorobiphenyl

R.T.: 8.682 min
Delta R.T.: -0.004 min
Response: 940170
Conc: 16.53 ng/ml