

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100620\
 Data File : PO072039.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Oct 2020 14:16
 Operator : DD\AJ
 Sample : L4260-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PAV-B21-100220-10-18.5

Manual Integrations
 APPROVED

Ankita
 10/7/2020 3:32:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 17:02:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.325	3.509	1784101	850563	24.839m	22.708
2) SA Decachlor...	9.932	8.682	1841955	924843	16.729	16.260

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100620\
Data File : PO072039.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Oct 2020 14:16
Operator : DD\AJ
Sample : L4260-05
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PAV-B21-100220-10-18.5


Manual Integrations
APPROVED

Ankita
10/7/2020 3:32:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 17:02:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

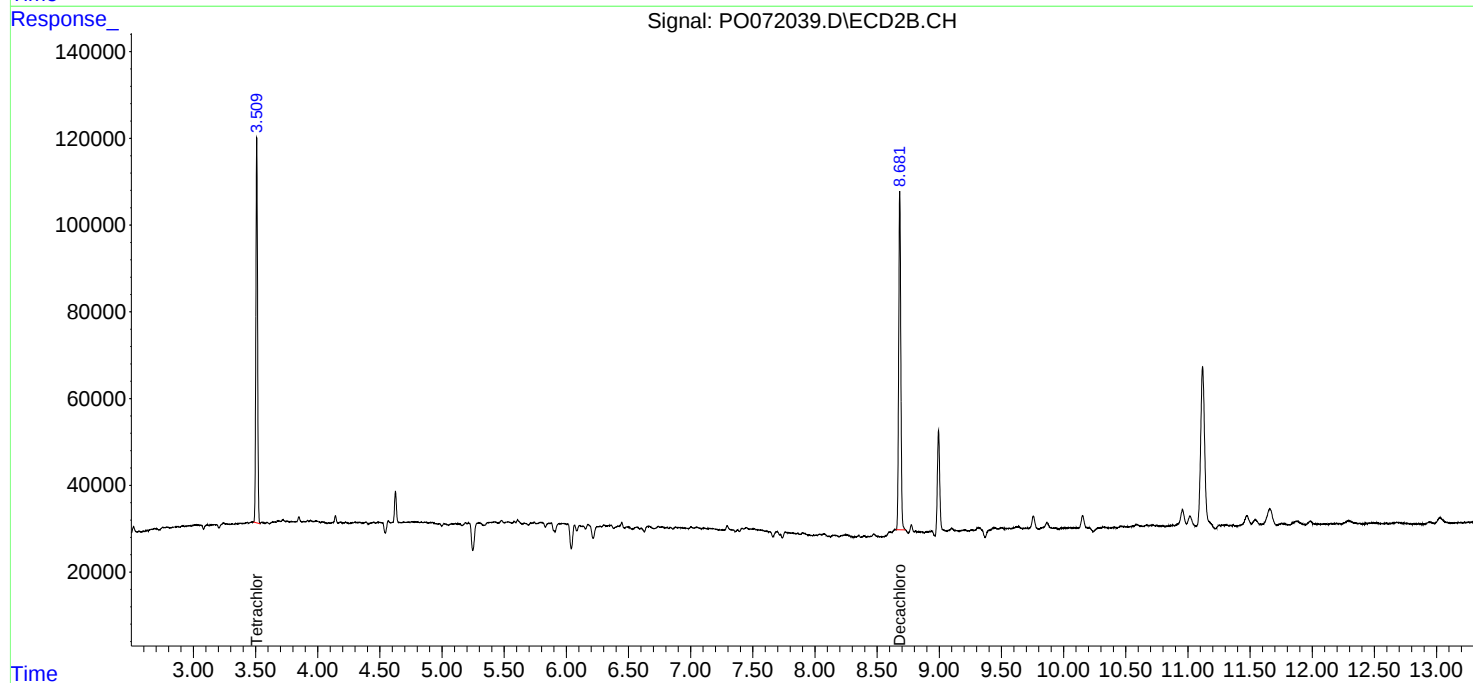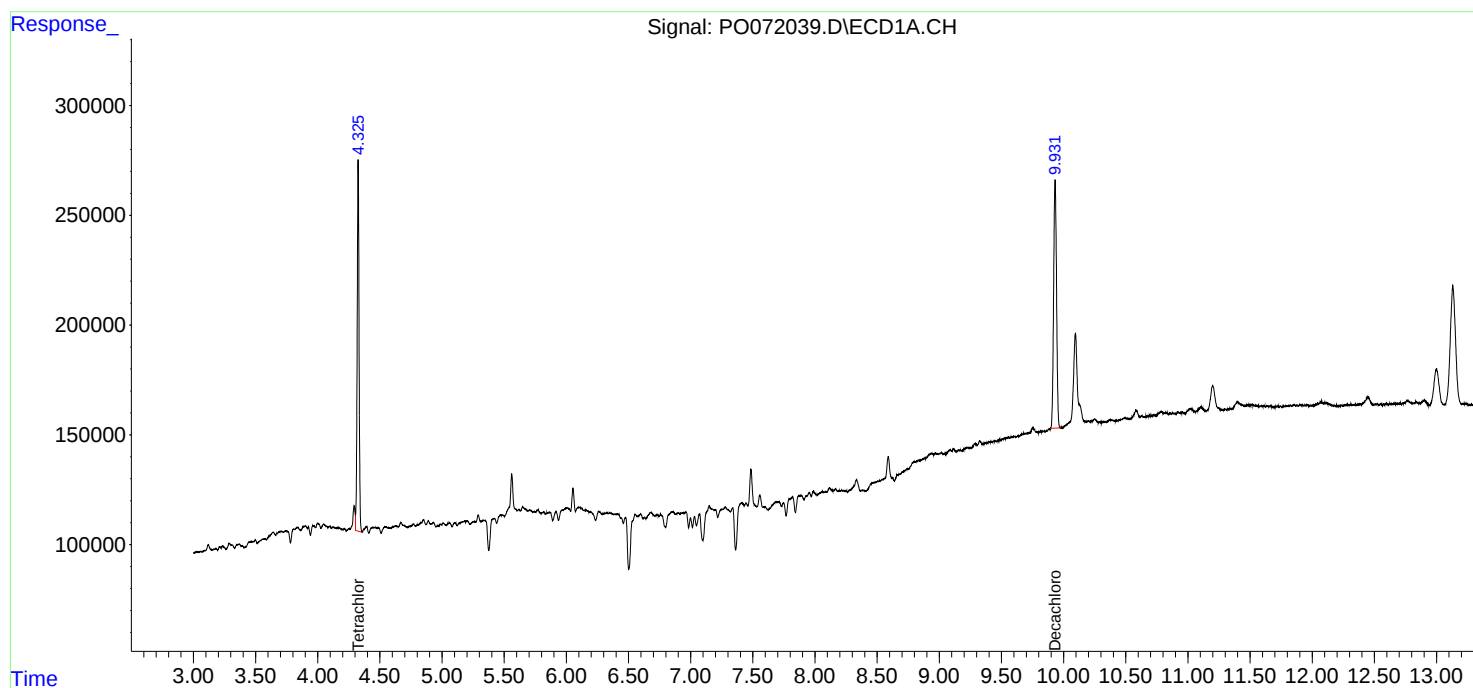

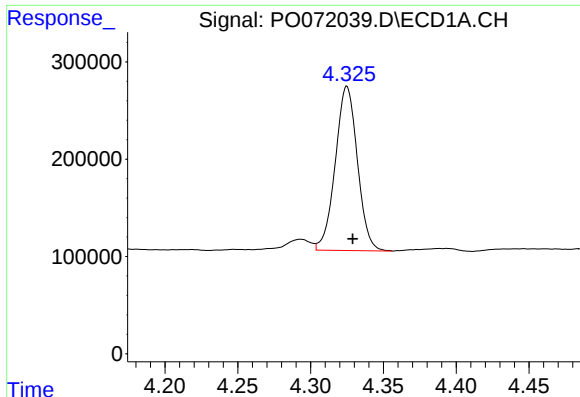


#1 Tetrachloro-m-xylene

R.T.: 4.325 min
Delta R.T.: -0.004 min
Response: 1784101
Conc: 24.84 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PAV-B21-100220-10-18.5


Manual Integrations
APPROVED

Ankita
10/7/2020 3:32:57 PM

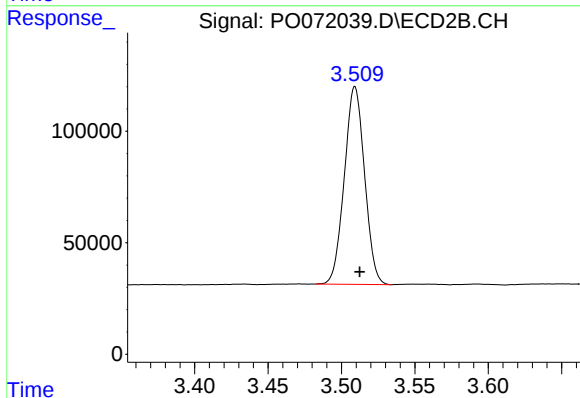


#1 Tetrachloro-m-xylene

R.T.: 3.509 min
Delta R.T.: -0.003 min
Response: 850563
Conc: 22.71 ng/ml

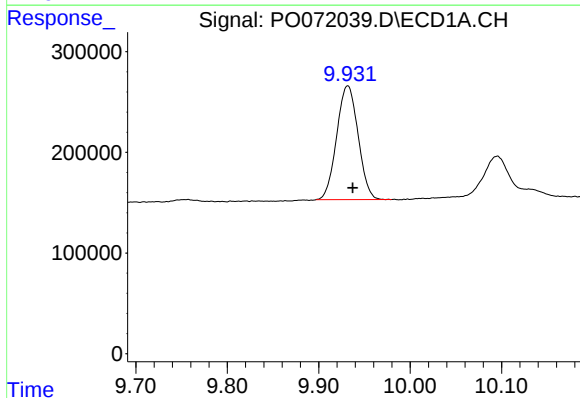

#2 Decachlorobiphenyl

R.T.: 9.932 min
Delta R.T.: -0.005 min
Response: 1841955
Conc: 16.73 ng/ml

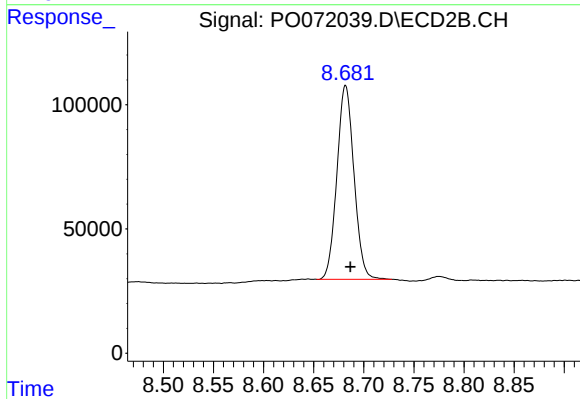

#2 Decachlorobiphenyl

R.T.: 8.682 min
Delta R.T.: -0.005 min
Response: 924843
Conc: 16.26 ng/ml