

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100620\
 Data File : PO072041.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Oct 2020 14:50
 Operator : DD\AJ
 Sample : L4247-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 B-19(4-5)

Manual Integrations
 APPROVED

Ankita
 10/7/2020 3:33:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 17:03:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.325	3.510	1654184	783355	23.030m	20.914
2)	SA Decachlor...	9.932	8.683	4141544	1929631	37.614	33.925
Target Compounds							
31)	L7 AR-1260-1	7.285	6.289	287481	162309	59.983	63.392m
32)	L7 AR-1260-2	7.559	6.490	798133	209400	106.558	65.456 #
33)	L7 AR-1260-3	7.909	6.633	330369	127354	51.820	43.153
34)	L7 AR-1260-4	8.136	7.111	331300	132546	55.193	50.096
35)	L7 AR-1260-5	8.451	7.364	597942	274176	43.151	41.267

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100620\
Data File : PO072041.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Oct 2020 14:50
Operator : DD\AJ
Sample : L4247-13
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
B-19(4-5)


Manual Integrations
APPROVED

Ankita
10/7/2020 3:33:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 17:03:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

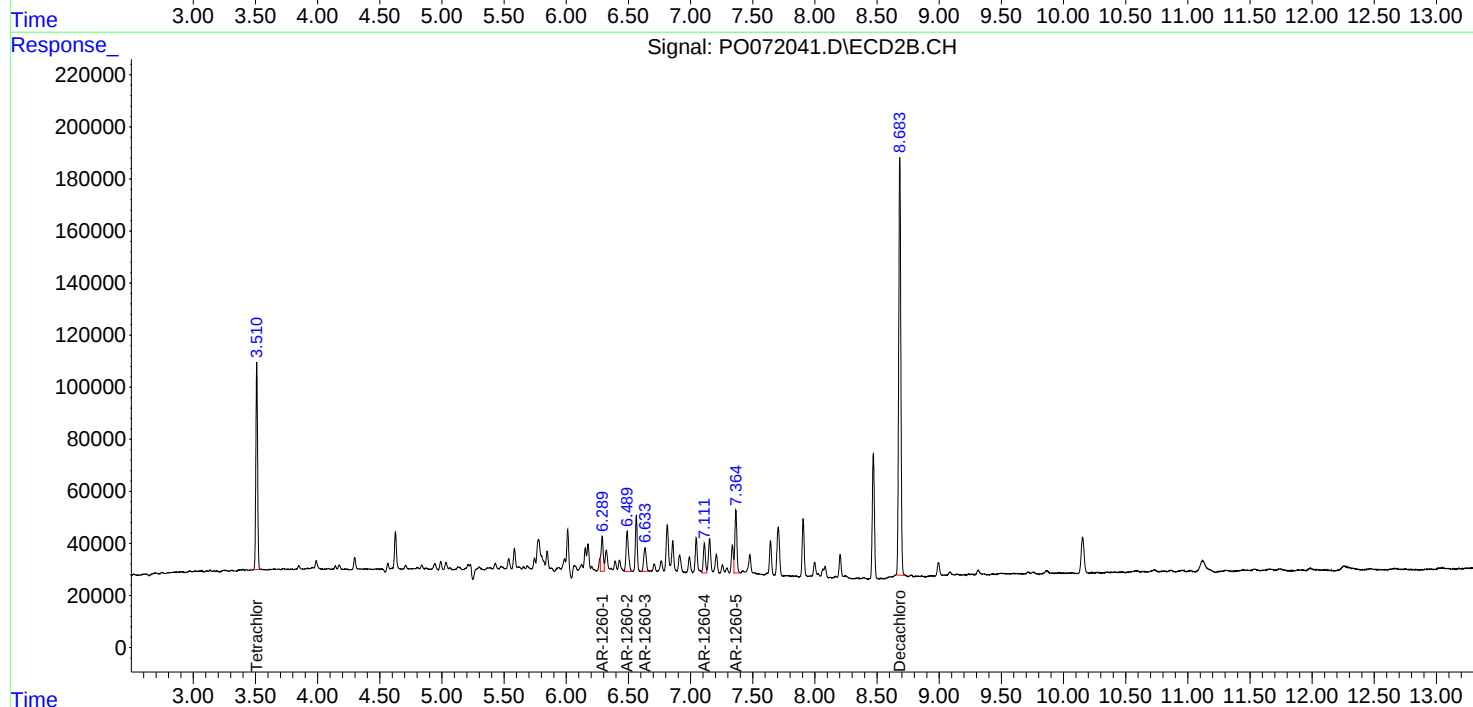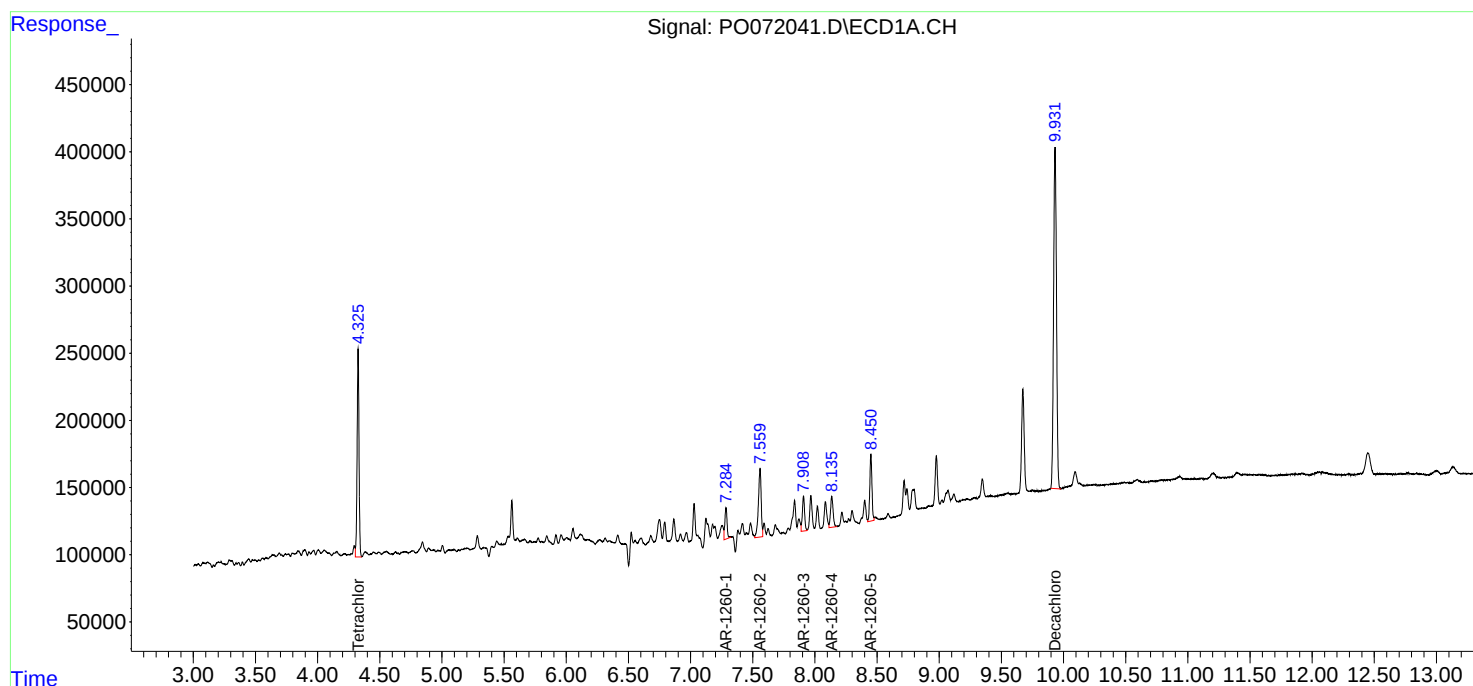

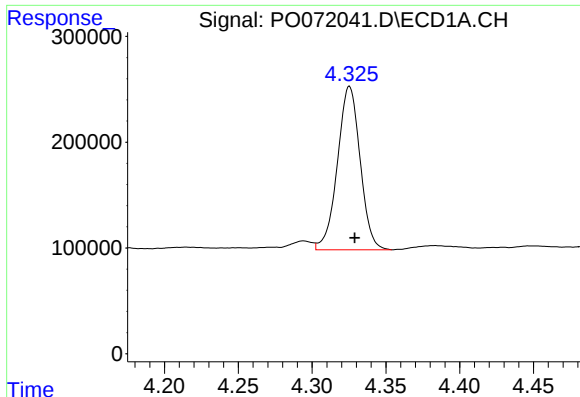


#1 Tetrachloro-m-xylene

R.T.: 4.325 min
Delta R.T.: -0.004 min
Response: 1654184
Conc: 23.03 ng/ml m

Instrument :
ECD_O
ClientSampleId :
B-19(4-5)


Manual Integrations
APPROVED

Ankita
10/7/2020 3:33:01 PM

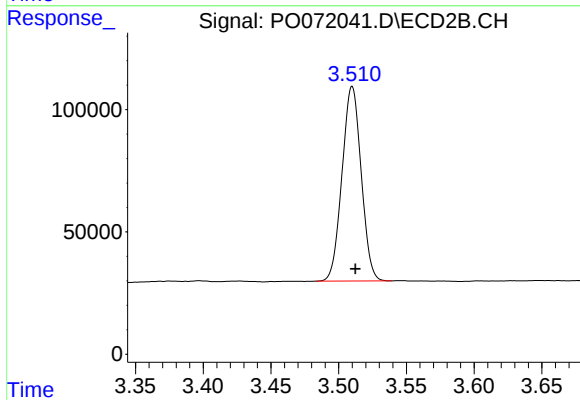


#1 Tetrachloro-m-xylene

R.T.: 3.510 min
Delta R.T.: -0.002 min
Response: 783355
Conc: 20.91 ng/ml

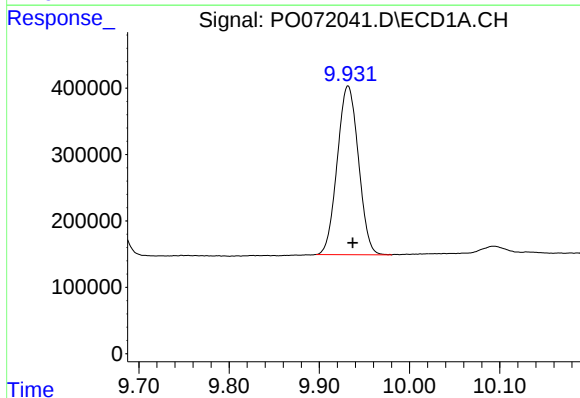


#2 Decachlorobiphenyl

R.T.: 9.932 min
Delta R.T.: -0.005 min
Response: 4141544
Conc: 37.61 ng/ml

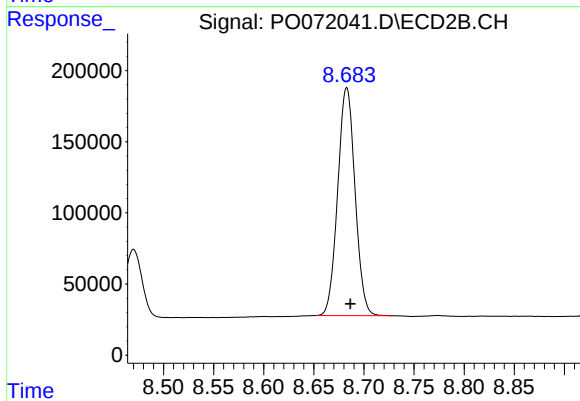

#2 Decachlorobiphenyl

R.T.: 8.683 min
Delta R.T.: -0.004 min
Response: 1929631
Conc: 33.93 ng/ml

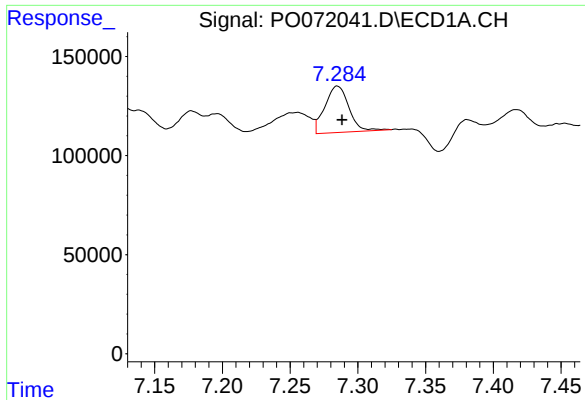


#31 AR-1260-1

R.T.: 7.285 min
Delta R.T.: -0.003 min
Response: 287481
Conc: 59.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
B-19(4-5)


Manual Integrations
APPROVED

Ankita
10/7/2020 3:33:01 PM

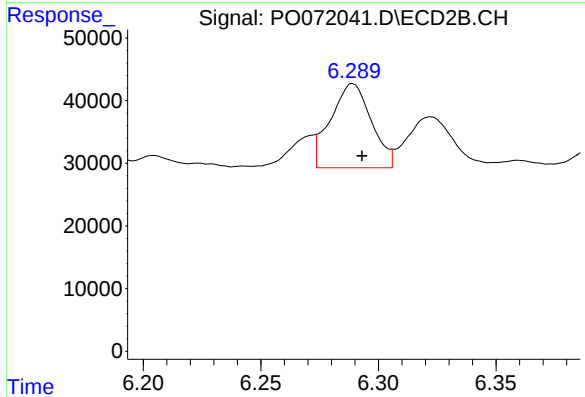


#31 AR-1260-1

R.T.: 6.289 min
Delta R.T.: -0.005 min
Response: 162309
Conc: 63.39 ng/ml m

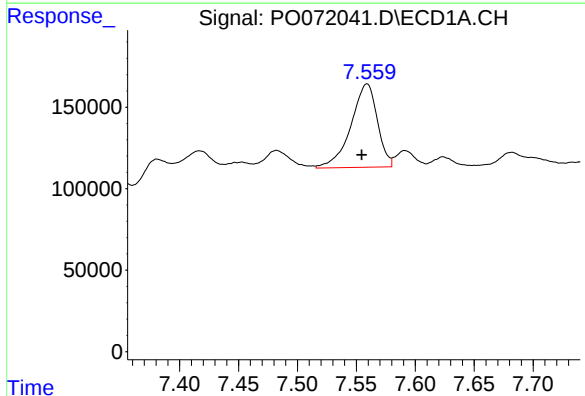


#32 AR-1260-2

R.T.: 7.559 min
Delta R.T.: 0.004 min
Response: 798133
Conc: 106.56 ng/ml

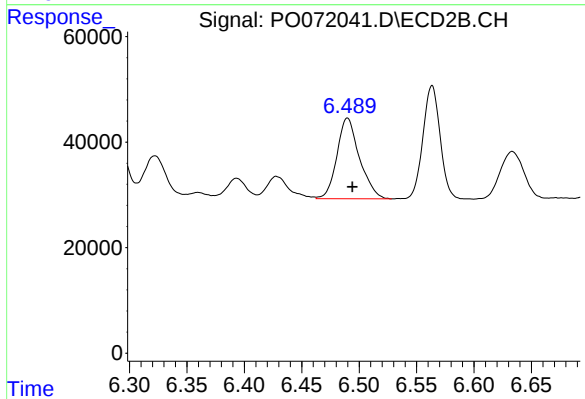

#32 AR-1260-2

R.T.: 6.490 min
Delta R.T.: -0.004 min
Response: 209400
Conc: 65.46 ng/ml

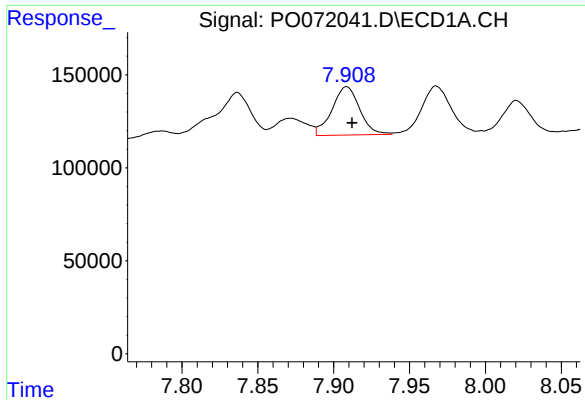


#33 AR-1260-3

R.T.: 7.909 min
Delta R.T.: -0.003 min
Response: 330369
Conc: 51.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
B-19(4-5)


Manual Integrations
APPROVED

Ankita
10/7/2020 3:33:01 PM

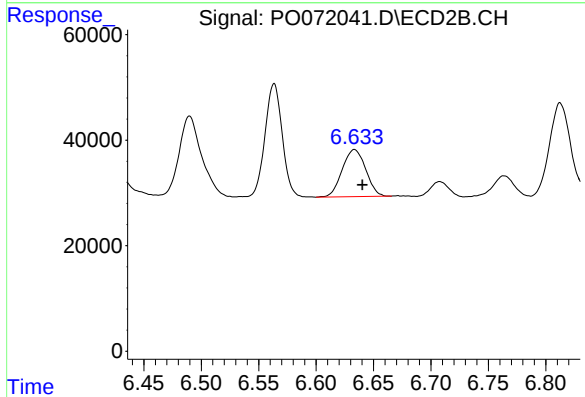


#33 AR-1260-3

R.T.: 6.633 min
Delta R.T.: -0.007 min
Response: 127354
Conc: 43.15 ng/ml

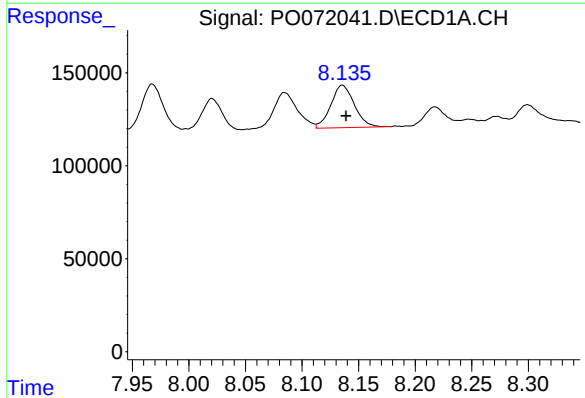


#34 AR-1260-4

R.T.: 8.136 min
Delta R.T.: -0.003 min
Response: 331300
Conc: 55.19 ng/ml

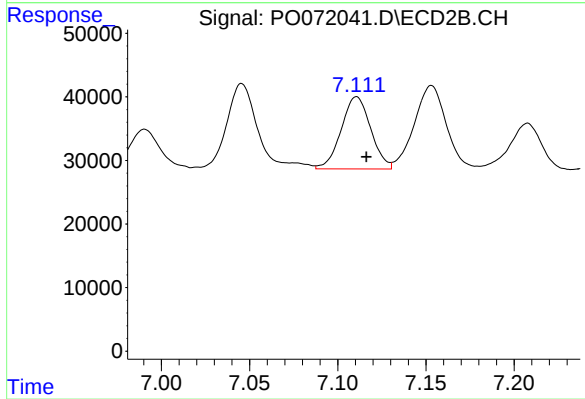

#34 AR-1260-4

R.T.: 7.111 min
Delta R.T.: -0.005 min
Response: 132546
Conc: 50.10 ng/ml

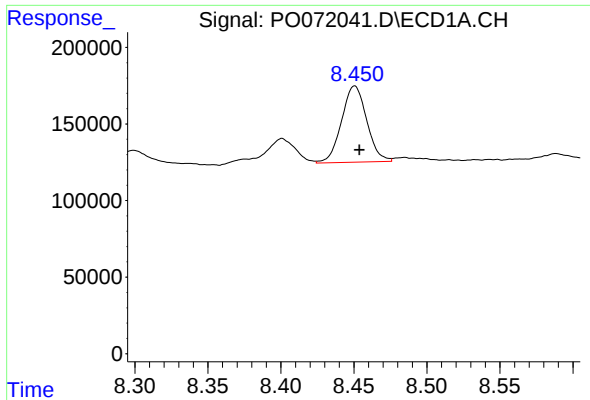


#35 AR-1260-5

R.T.: 8.451 min
Delta R.T.: -0.003 min
Response: 597942
Conc: 43.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
B-19(4-5)

Manual Integrations
APPROVED

Ankita
10/7/2020 3:33:01 PM

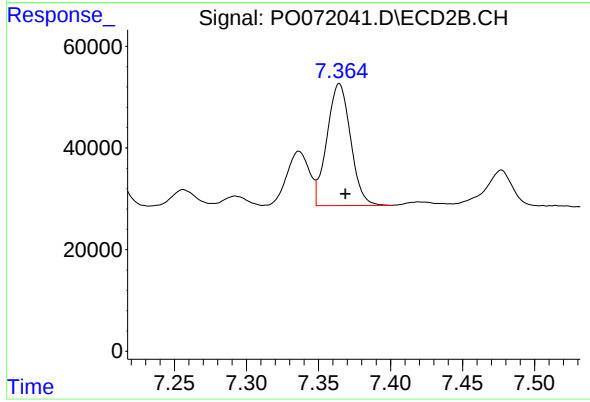

#35 AR-1260-5

R.T.: 7.364 min
Delta R.T.: -0.004 min
Response: 274176
Conc: 41.27 ng/ml