

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO100620\  
 Data File : PO072066.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 06 Oct 2020 22:34  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 07 02:36:33 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO100320.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Mon Oct 05 11:48:20 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1  | RT#2  | Resp#1  | Resp#2  | ng/ml  | ng/ml  |
|-----------------------------|-------|-------|---------|---------|--------|--------|
| -----                       |       |       |         |         |        |        |
| System Monitoring Compounds |       |       |         |         |        |        |
| 1) SA Tetrachlo...          | 4.326 | 3.510 | 1755995 | 819202  | 24.448 | 21.871 |
| 2) SA Decachlor...          | 9.932 | 8.682 | 2179023 | 1095479 | 19.790 | 19.260 |

Target Compounds

-----



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO100620\  
Data File : PO072066.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 06 Oct 2020 22:34  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 07 02:36:33 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO100320.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Mon Oct 05 11:48:20 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

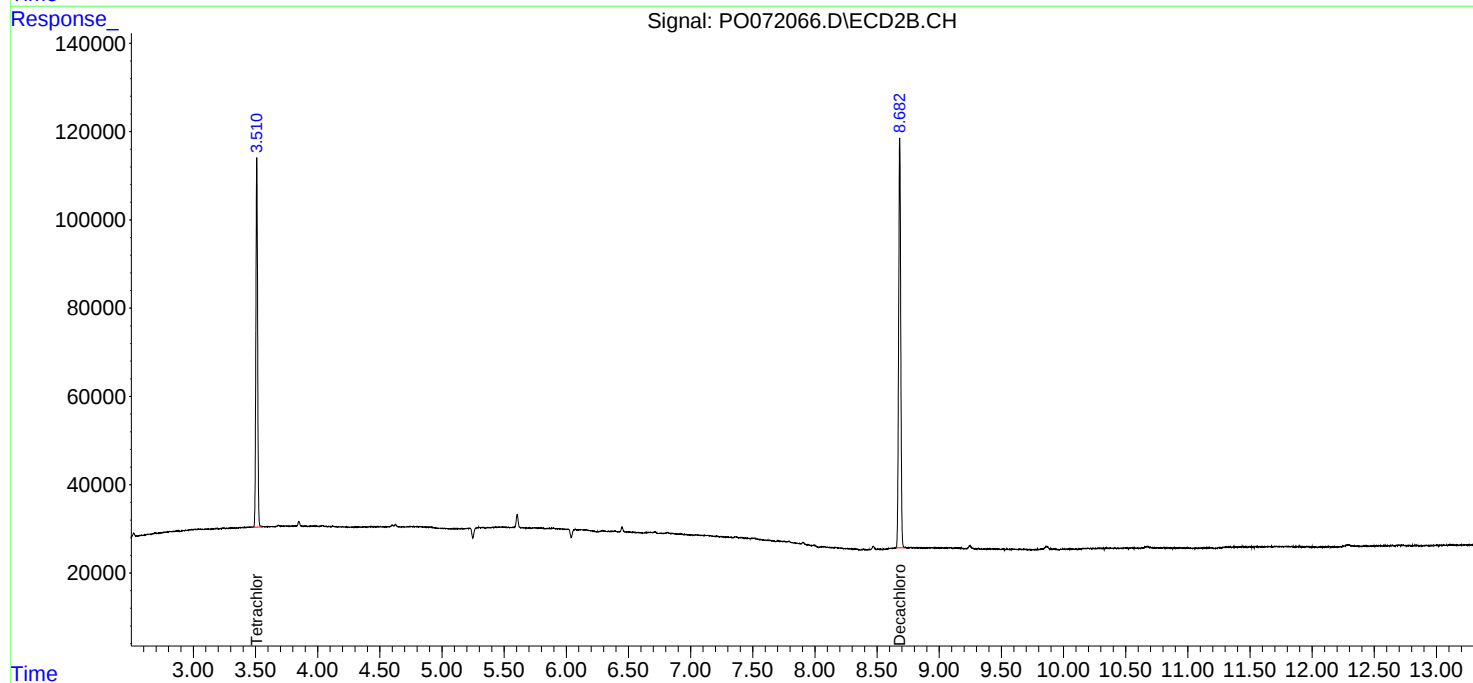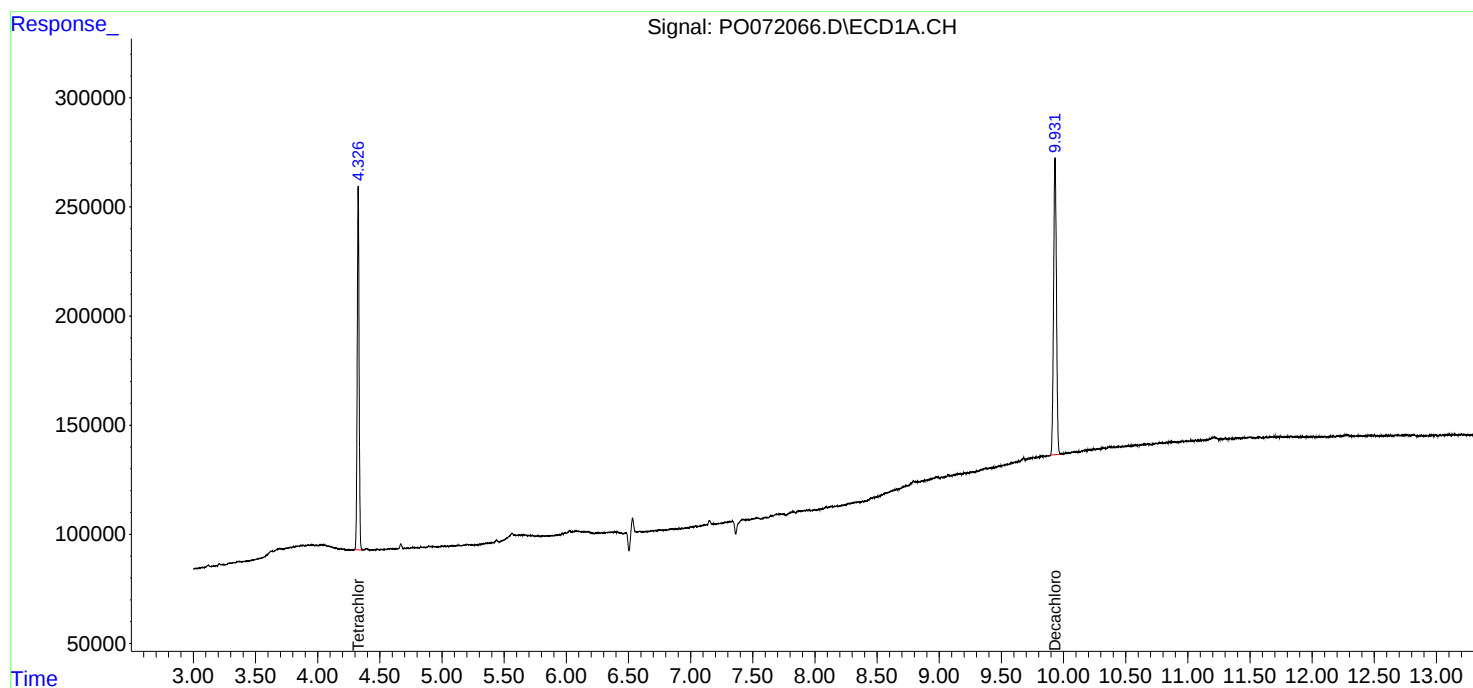


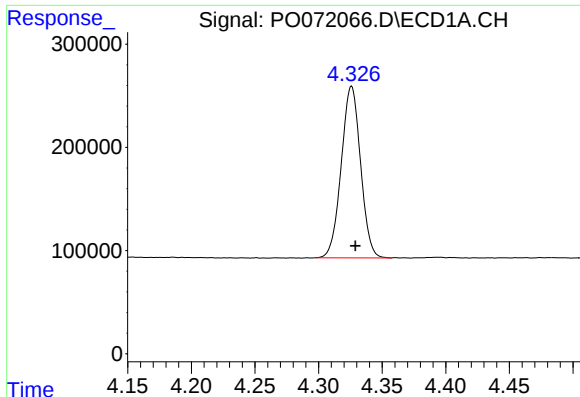

#1 Tetrachloro-m-xylene


R.T.: 4.326 min  
Delta R.T.: -0.003 min  
Response: 1755995  
Conc: 24.45 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
I.BLK

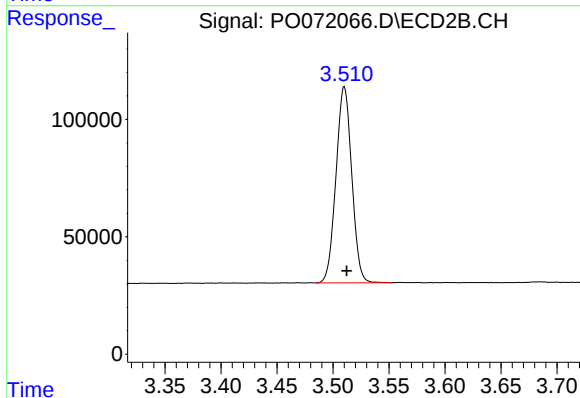


#1 Tetrachloro-m-xylene

R.T.: 3.510 min  
Delta R.T.: -0.002 min  
Response: 819202  
Conc: 21.87 ng/ml

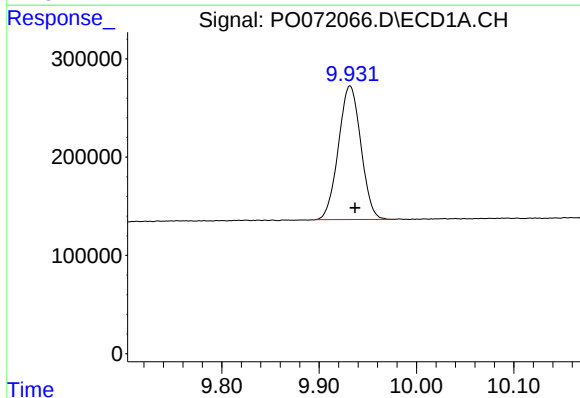

#2 Decachlorobiphenyl

R.T.: 9.932 min  
Delta R.T.: -0.005 min  
Response: 2179023  
Conc: 19.79 ng/ml

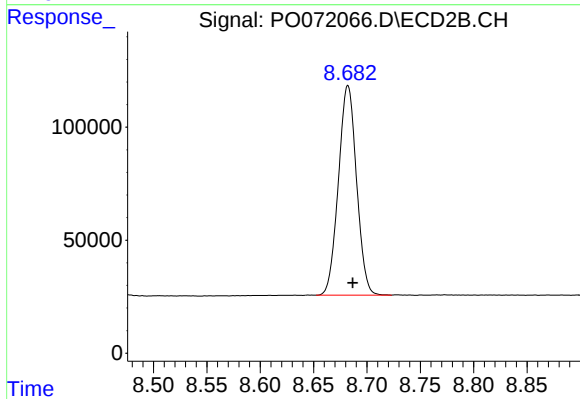

#2 Decachlorobiphenyl

R.T.: 8.682 min  
Delta R.T.: -0.004 min  
Response: 1095479  
Conc: 19.26 ng/ml