

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100818\
 Data File : PO049775.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2018 21:02
 Operator : SM/SJ
 Sample : J5299-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 100518-SIDI-F-D-S

Manual Integrations
 APPROVED

Sohil
 10/9/2018 3:35:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 05:23:17 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 08 15:27:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.383	3.513	5133515	4960264	22.709	20.566
2) SA Decachlor...	10.088	8.436	5937479	4591669	17.820m	17.555

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100818\
Data File : P0049775.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2018 21:02
Operator : SM/SJ
Sample : J5299-07
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
100518-SIDI-F-D-S


Manual Integrations
APPROVED

Sohil
10/9/2018 3:35:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 05:23:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100818.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 08 15:27:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

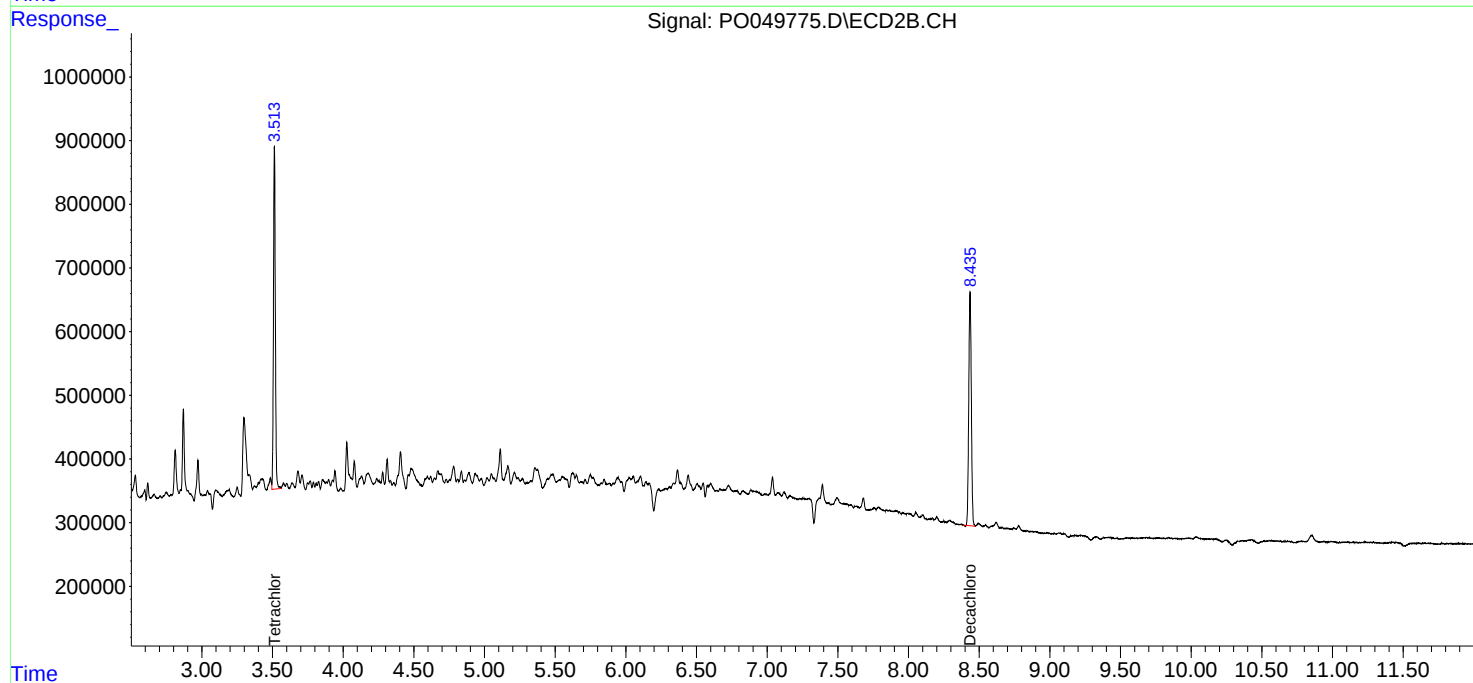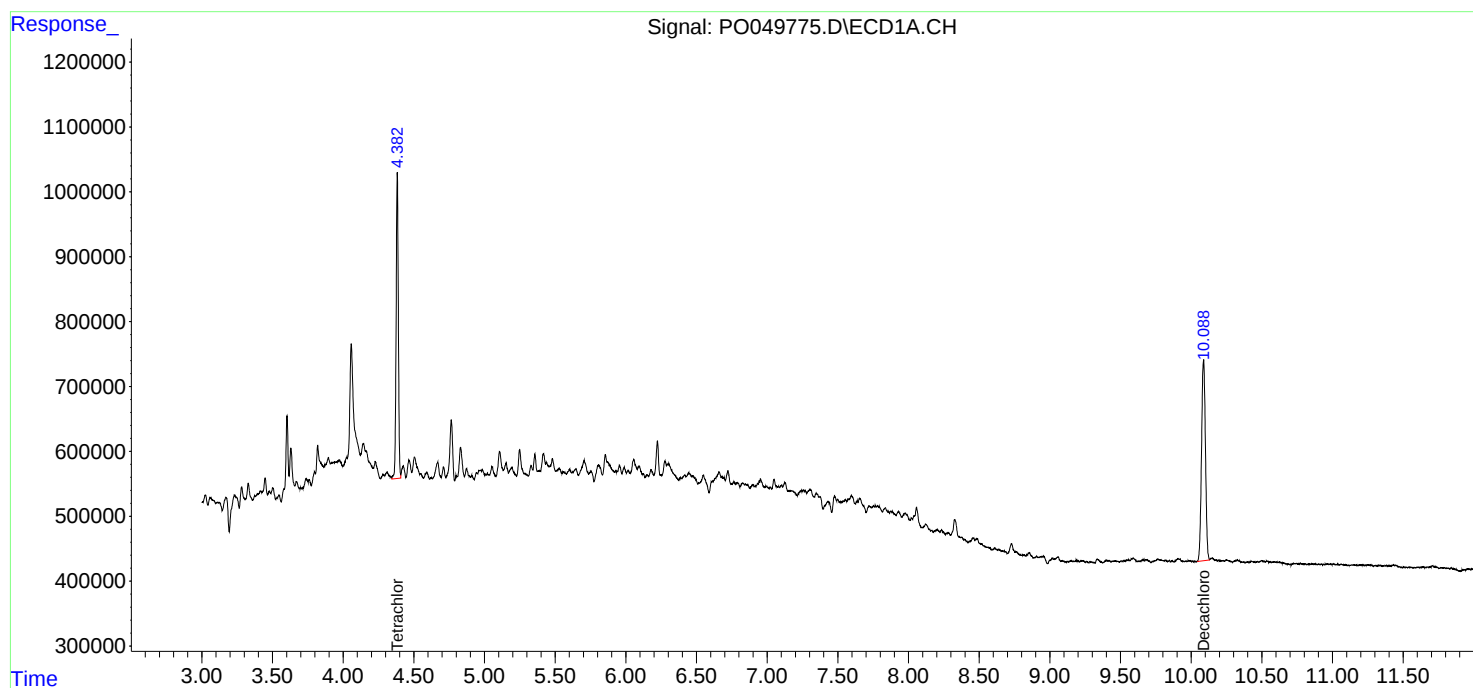

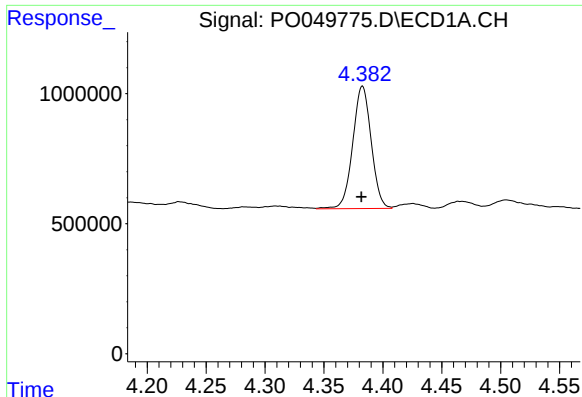


#1 Tetrachloro-m-xylene

R.T.: 4.383 min
Delta R.T.: 0.000 min
Response: 5133515
Conc: 22.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
100518-SIDI-F-D-S


Manual Integrations
APPROVED

Sohil
10/9/2018 3:35:32 PM

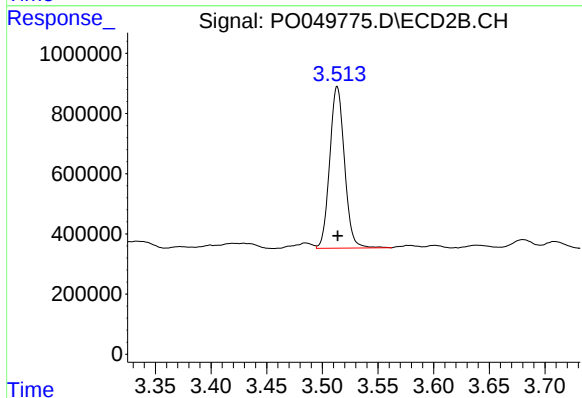


#1 Tetrachloro-m-xylene

R.T.: 3.513 min
Delta R.T.: 0.000 min
Response: 4960264
Conc: 20.57 ng/ml

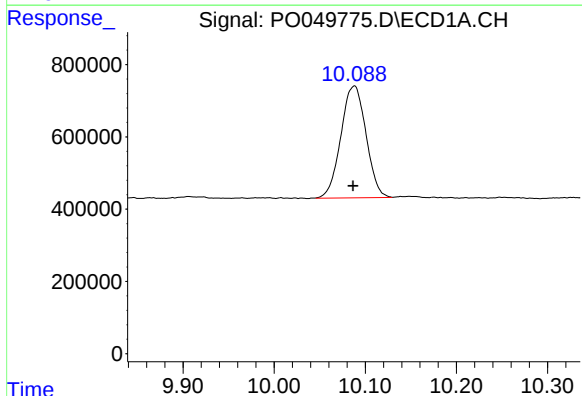

#2 Decachlorobiphenyl

R.T.: 10.088 min
Delta R.T.: 0.001 min
Response: 5937479
Conc: 17.82 ng/ml m

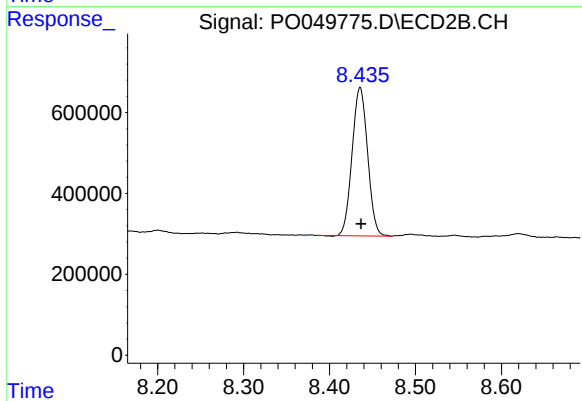

#2 Decachlorobiphenyl

R.T.: 8.436 min
Delta R.T.: -0.001 min
Response: 4591669
Conc: 17.55 ng/ml