

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100818\
 Data File : PO049776.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2018 21:18
 Operator : SM/SJ
 Sample : J5299-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 100518-SIDI-F-U-B

Manual Integrations
 APPROVED

Sohil
 10/9/2018 3:35:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 05:23:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 08 15:27:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.383	3.513	4871097	4922465	21.548	20.409
2) SA Decachlor...	10.087	8.435	5061312	4079720	15.190	15.597m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100818\
Data File : PO049776.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2018 21:18
Operator : SM/SJ
Sample : J5299-08
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
100518-SIDI-F-U-B


Manual Integrations
APPROVED

Sohil
10/9/2018 3:35:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 05:23:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100818.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 08 15:27:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

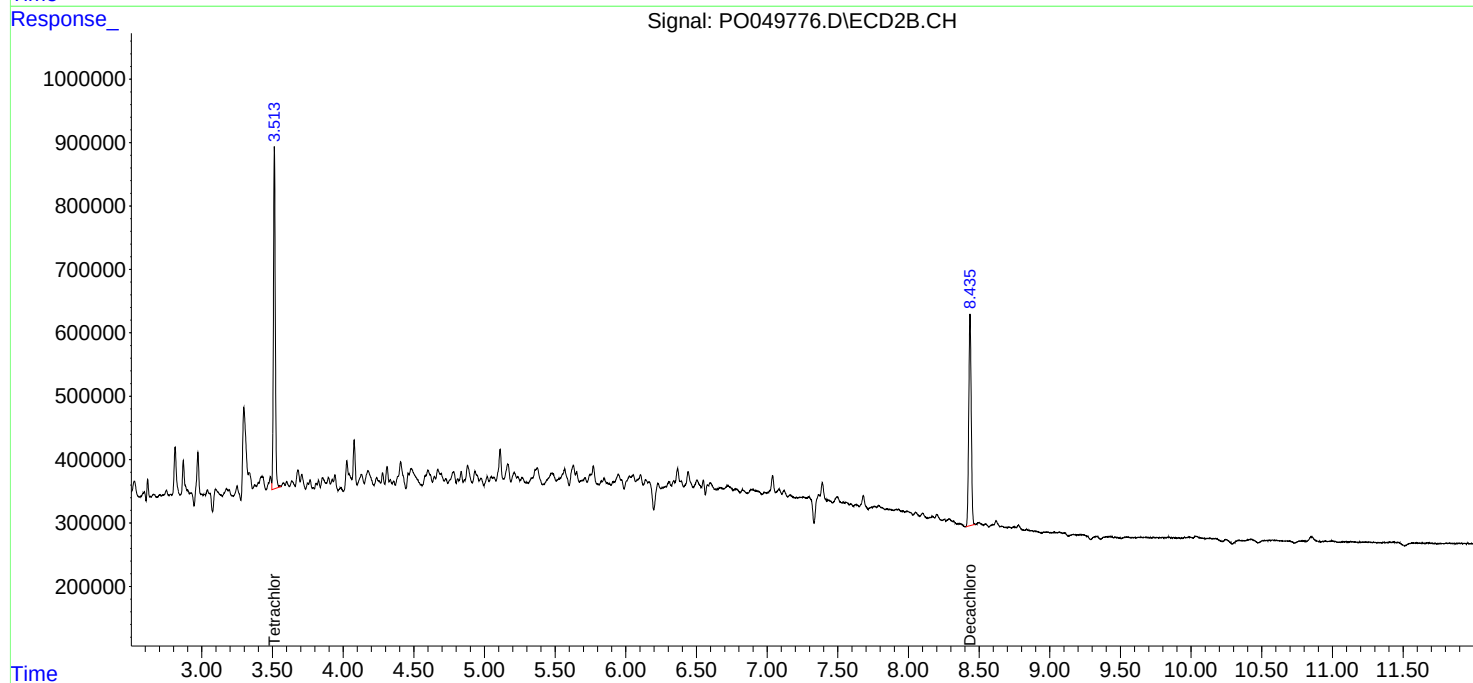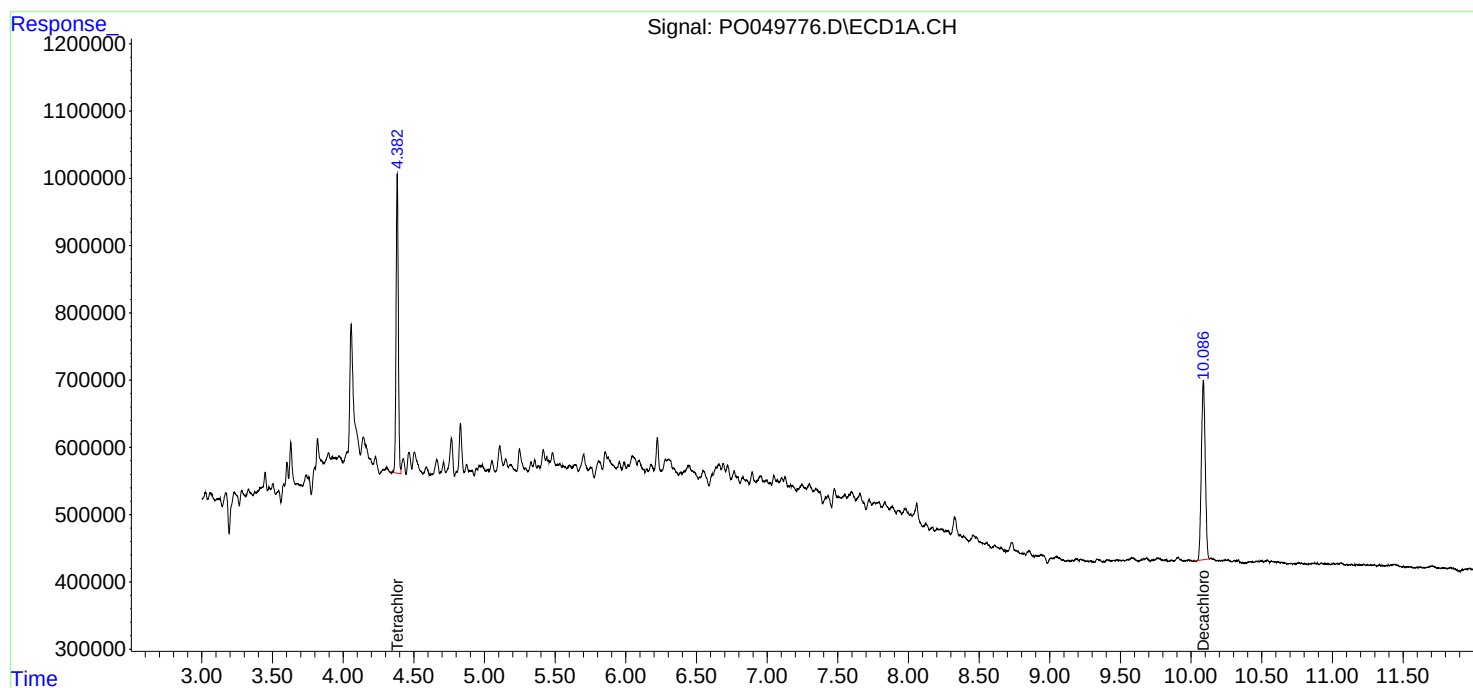

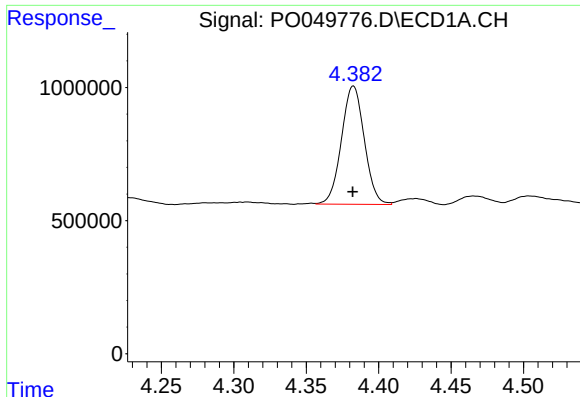


#1 Tetrachloro-m-xylene

R.T.: 4.383 min
Delta R.T.: 0.000 min
Response: 4871097
Conc: 21.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
100518-SIDI-F-U-B


Manual Integrations
APPROVED

Sohil
10/9/2018 3:35:32 PM

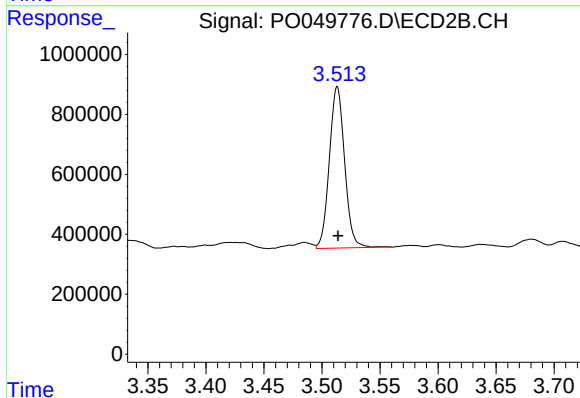


#1 Tetrachloro-m-xylene

R.T.: 3.513 min
Delta R.T.: 0.000 min
Response: 4922465
Conc: 20.41 ng/ml

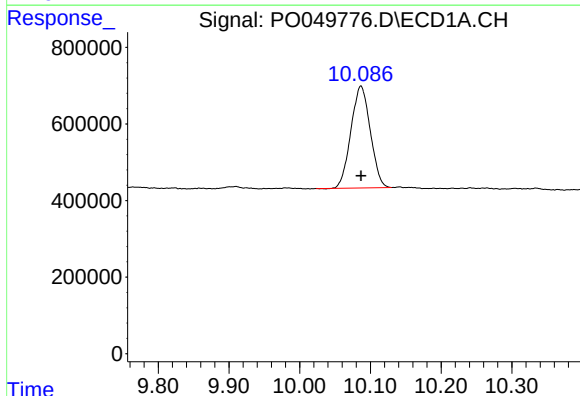

#2 Decachlorobiphenyl

R.T.: 10.087 min
Delta R.T.: 0.000 min
Response: 5061312
Conc: 15.19 ng/ml

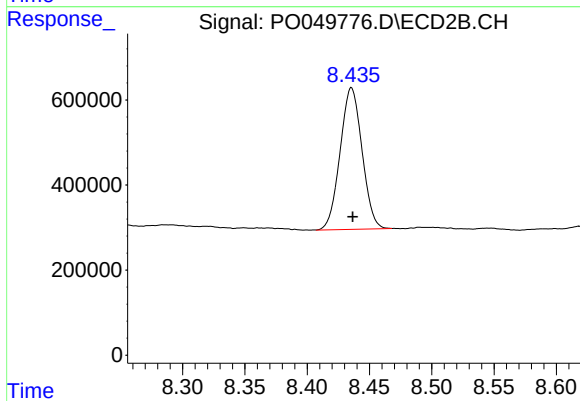

#2 Decachlorobiphenyl

R.T.: 8.435 min
Delta R.T.: -0.002 min
Response: 4079720
Conc: 15.60 ng/ml m