

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100819\
 Data File : P0061790.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2019 17:26
 Operator : HP/AJ
 Sample : PB123723BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB123723BL

Manual Integrations
 APPROVED

Ankita
 10/9/2019 12:14:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 01:17:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.360	3.519	830207	616794	20.242	19.072
2)	SA Decachlor...	10.020	8.381	1049155	732511	22.528	22.625m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100819\
Data File : PO061790.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2019 17:26
Operator : HP/AJ
Sample : PB123723BL
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB123723BL


Manual Integrations
APPROVED

Ankita
10/9/2019 12:14:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 01:17:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

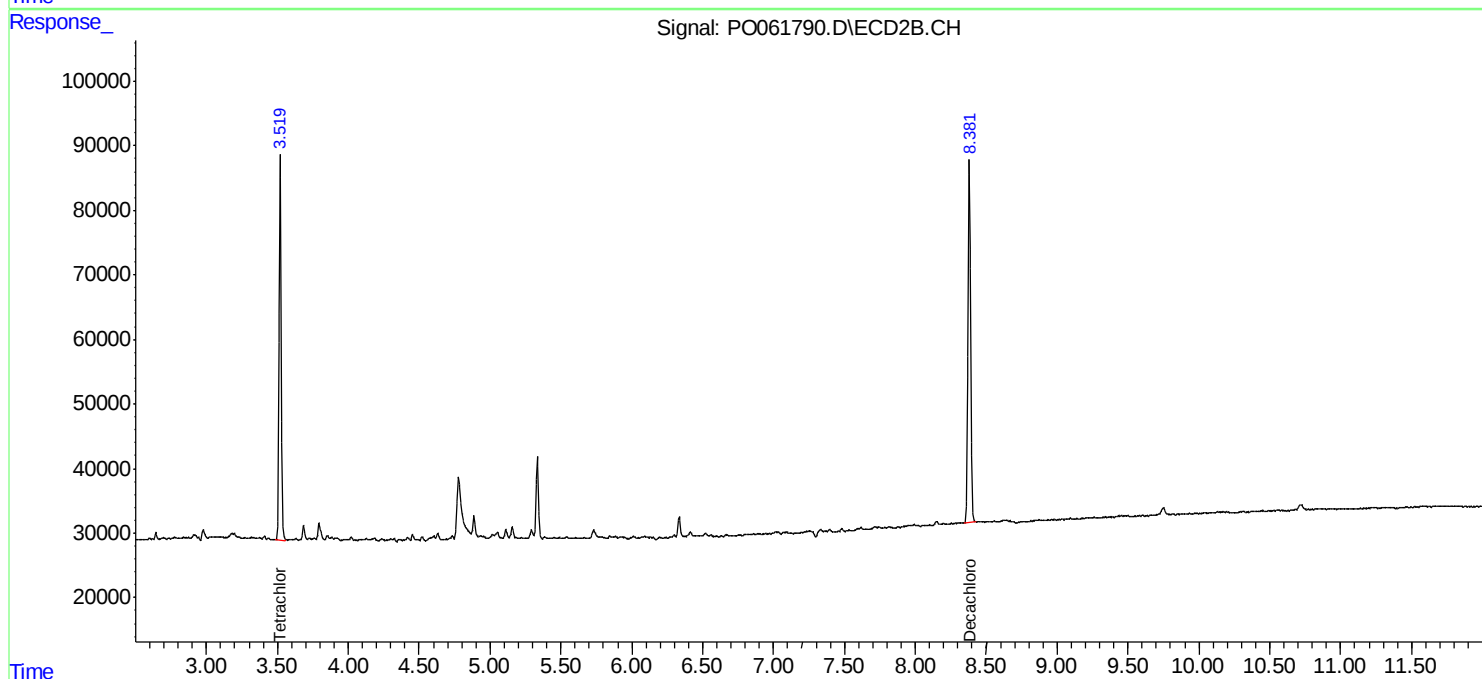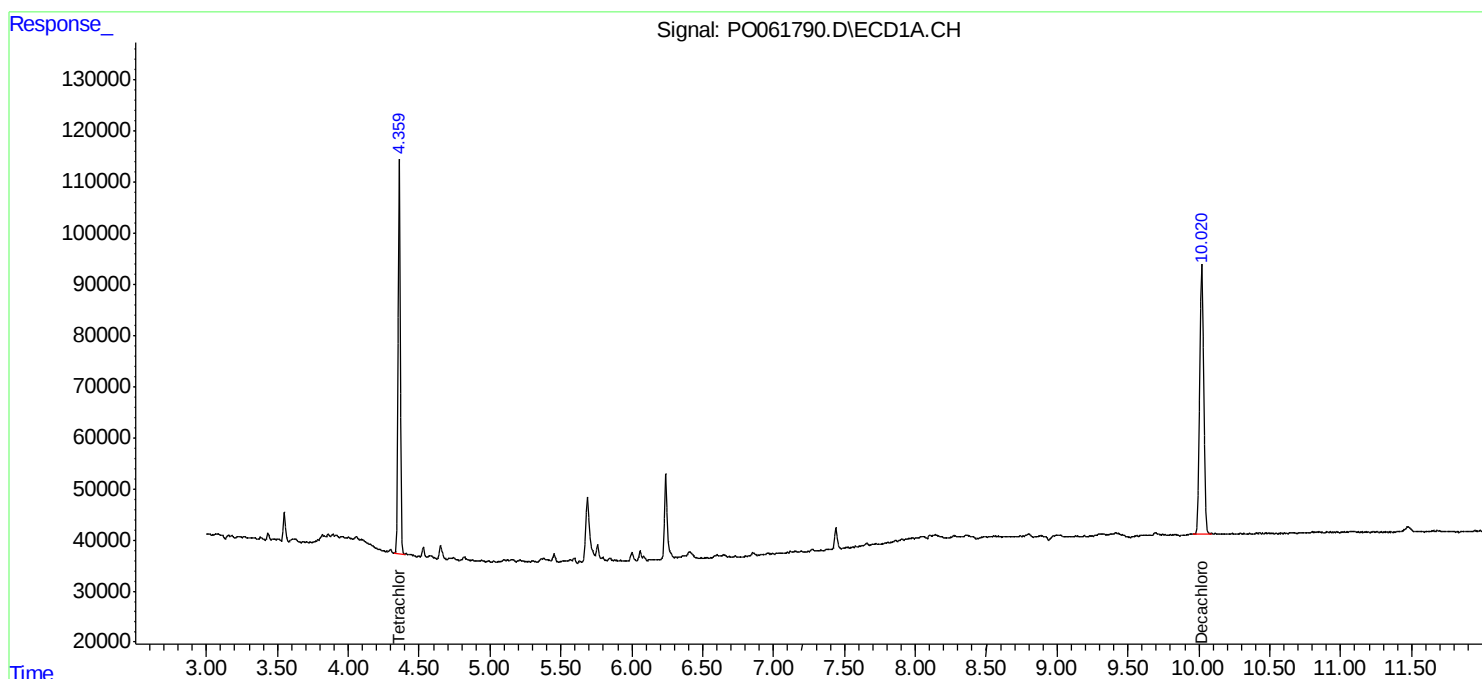

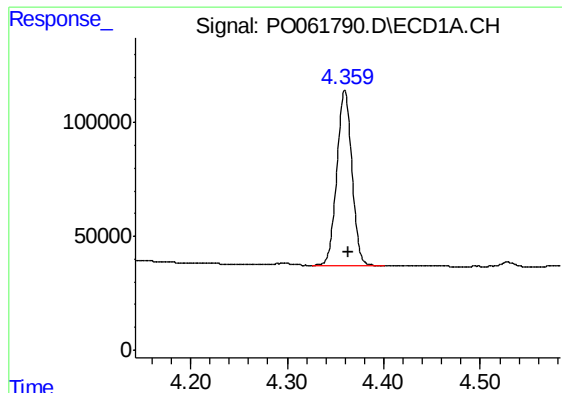


#1 Tetrachloro-m-xylene

R.T.: 4.360 min
Delta R.T.: -0.003 min
Response: 830207
Conc: 20.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB123723BL


Manual Integrations
APPROVED

Ankita
10/9/2019 12:14:27 PM

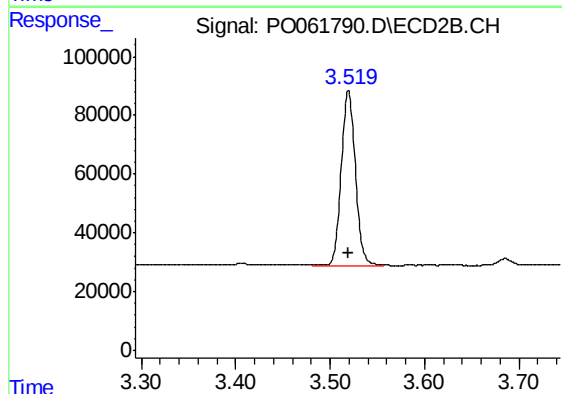


#1 Tetrachloro-m-xylene

R.T.: 3.519 min
Delta R.T.: 0.000 min
Response: 616794
Conc: 19.07 ng/ml

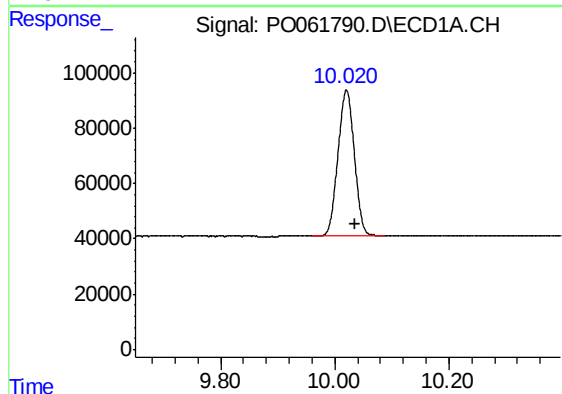

#2 Decachlorobiphenyl

R.T.: 10.020 min
Delta R.T.: -0.016 min
Response: 1049155
Conc: 22.53 ng/ml

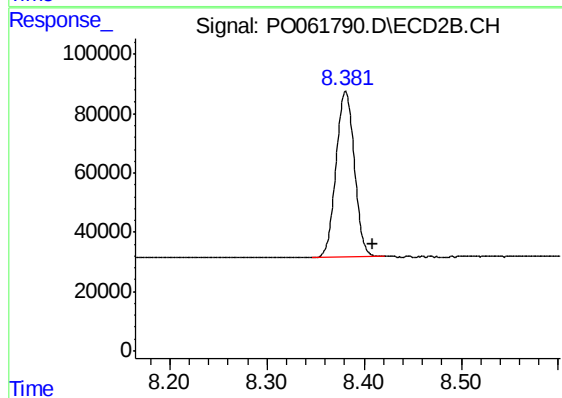

#2 Decachlorobiphenyl

R.T.: 8.381 min
Delta R.T.: -0.028 min
Response: 732511
Conc: 22.63 ng/ml m