

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100819\
 Data File : PO061799.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2019 19:53
 Operator : HP/AJ
 Sample : K5213-08RE
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S-4(5-10)RE

Manual Integrations
 APPROVED

Ankita
 10/9/2019 3:31:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 01:20:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.360	3.521	1038073	747730	25.310	23.121
2) SA Decachlor...	10.021	8.380	744520	508047	15.987	15.692m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100819\
Data File : P0061799.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2019 19:53
Operator : HP/AJ
Sample : K5213-08RE
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S-4(5-10)RE


Manual Integrations
APPROVED

Ankita
10/9/2019 3:31:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 01:20:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

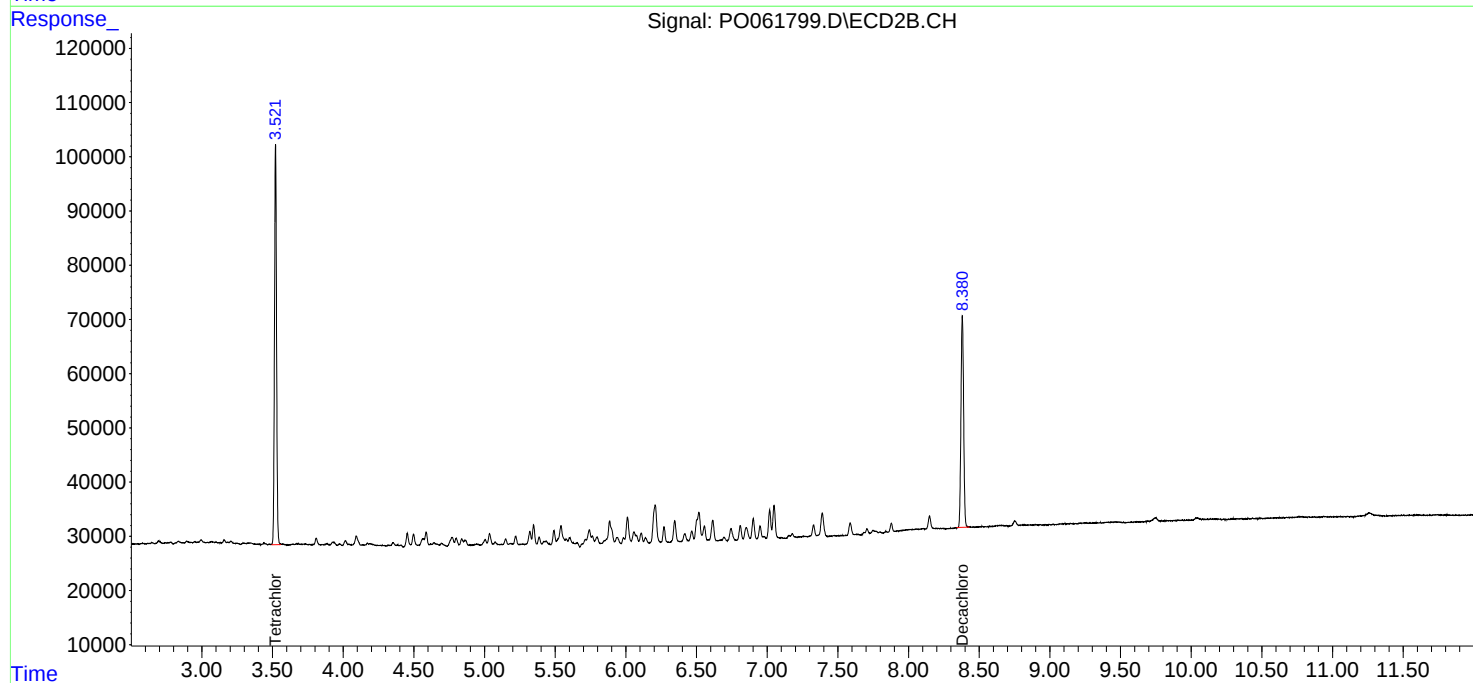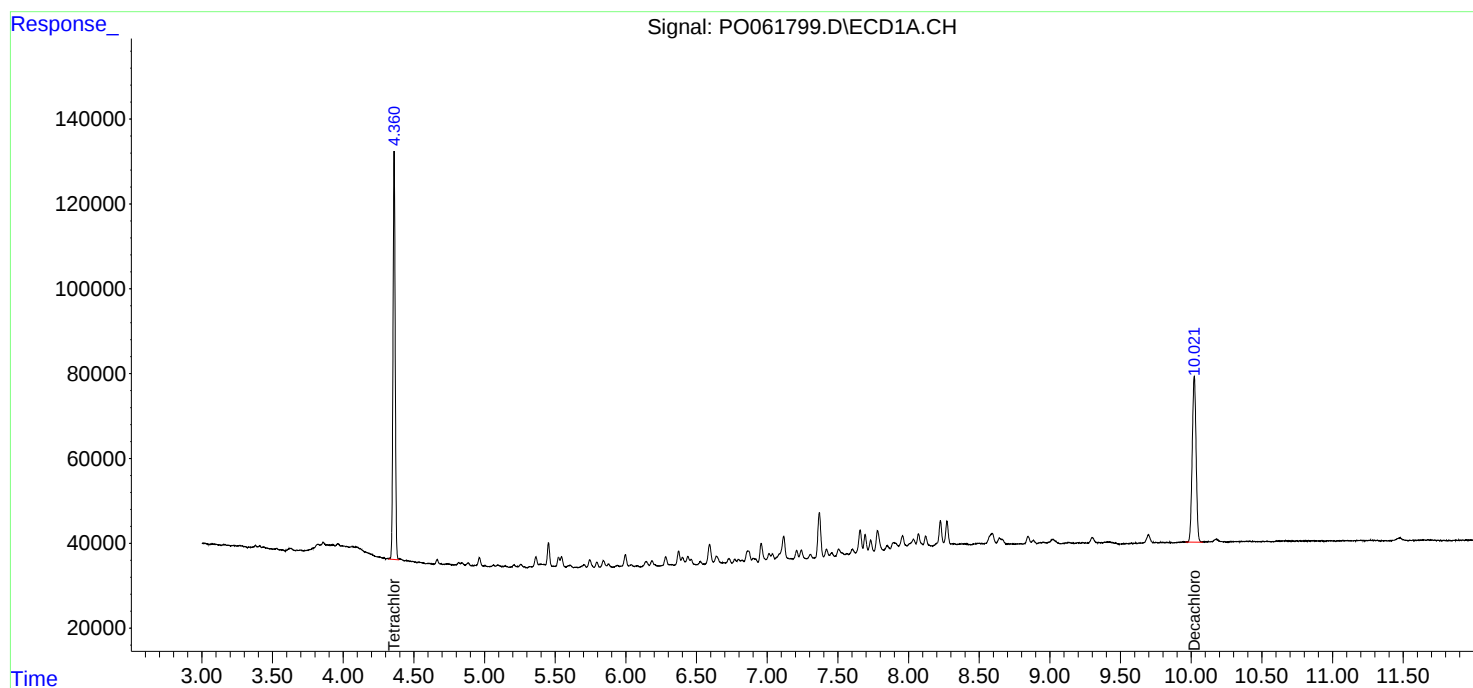

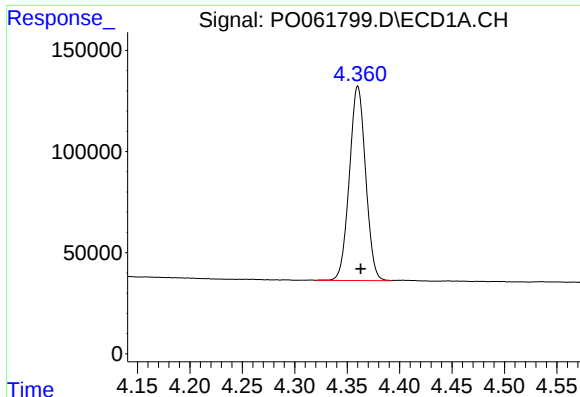


#1 Tetrachloro-m-xylene

R.T.: 4.360 min
Delta R.T.: -0.003 min
Response: 1038073
Conc: 25.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
S-4(5-10)RE


Manual Integrations
APPROVED

Ankita
10/9/2019 3:31:49 PM

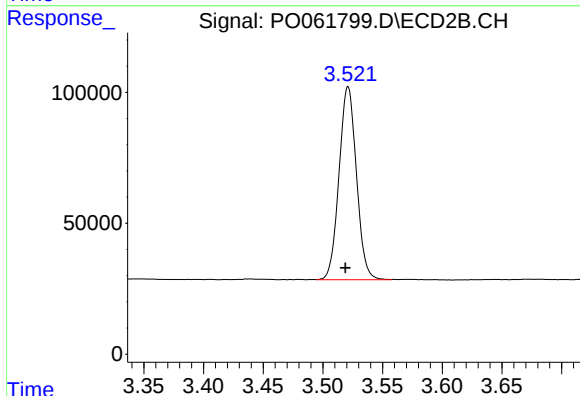


#1 Tetrachloro-m-xylene

R.T.: 3.521 min
Delta R.T.: 0.002 min
Response: 747730
Conc: 23.12 ng/ml

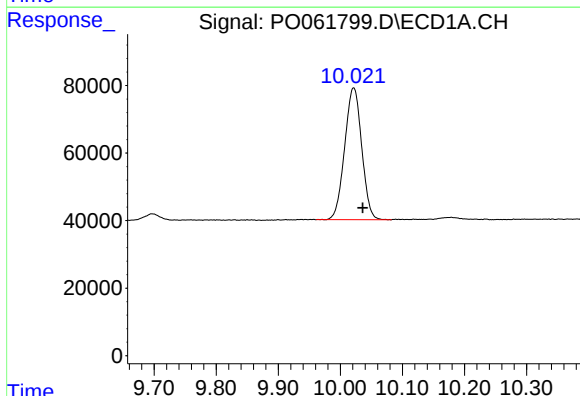

#2 Decachlorobiphenyl

R.T.: 10.021 min
Delta R.T.: -0.015 min
Response: 744520
Conc: 15.99 ng/ml

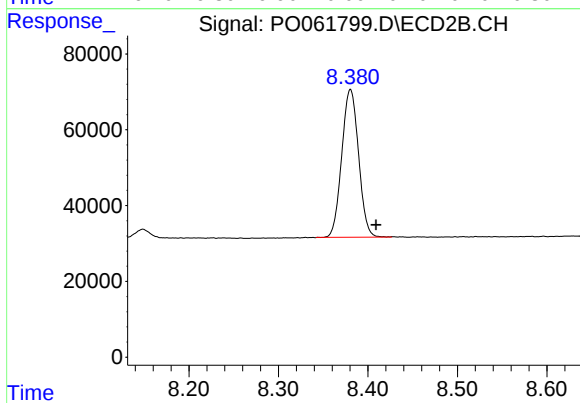

#2 Decachlorobiphenyl

R.T.: 8.380 min
Delta R.T.: -0.029 min
Response: 508047
Conc: 15.69 ng/ml m