

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100819\
 Data File : P0061804.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2019 21:15
 Operator : HP/AJ
 Sample : K5147-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-03-100719

Manual Integrations
 APPROVED

Ankita
 10/9/2019 12:14:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 01:22:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.360	3.520	1162826	922307	28.352	28.520
2)	SA Decachlor...	10.021	8.383	834337	516518	17.915	15.954
Target Compounds							
26)	L6 AR-1254-1	6.374	5.348	127215	127730	55.762	58.237
27)	L6 AR-1254-2	6.592	5.493	234860	117990	65.003	60.184
28)	L6 AR-1254-3	6.957	5.885	292201	237144	74.782	74.486
29)	L6 AR-1254-4	7.242	6.110	147972	84316	48.858	41.559
30)	L6 AR-1254-5	7.659	6.520	250275	245330	79.695m	86.736

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100819\
Data File : PO061804.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2019 21:15
Operator : HP/AJ
Sample : K5147-01
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleID :
OK-03-100719


Manual Integrations
APPROVED

Ankita
10/9/2019 12:14:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 01:22:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

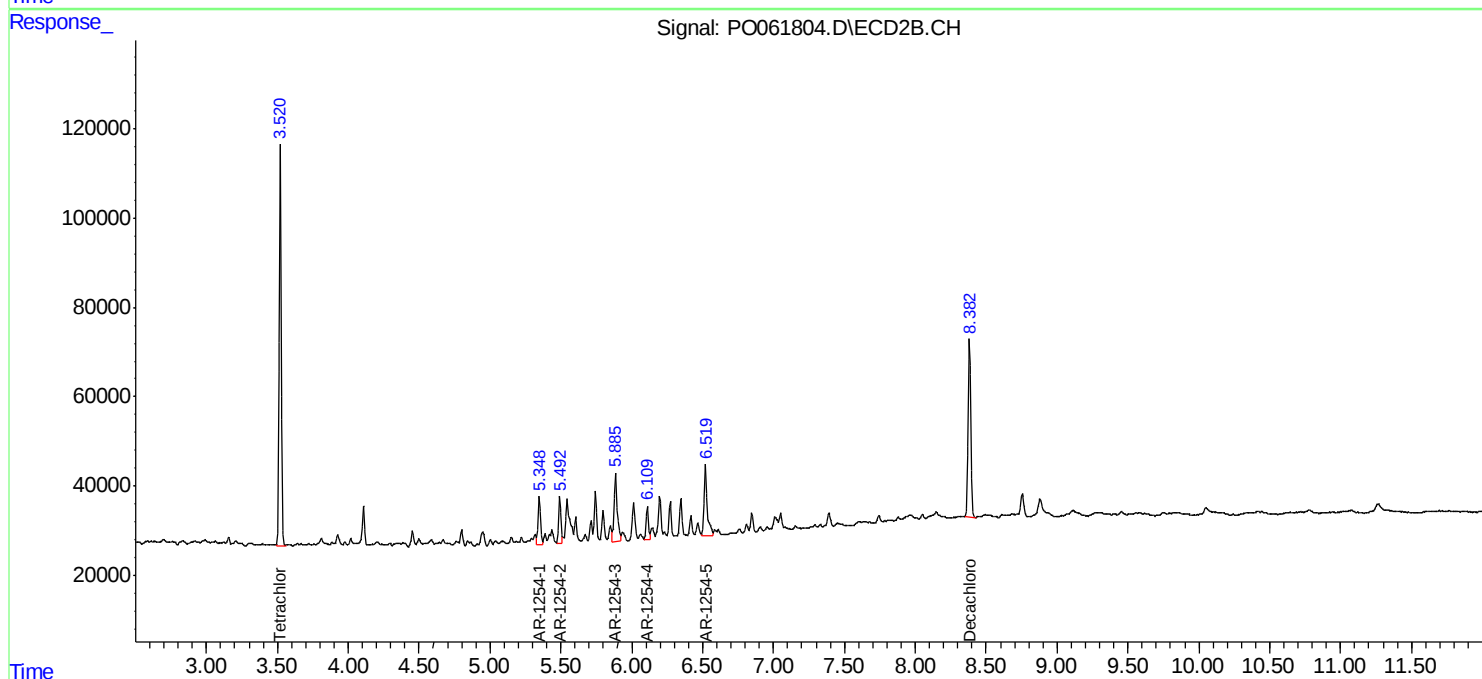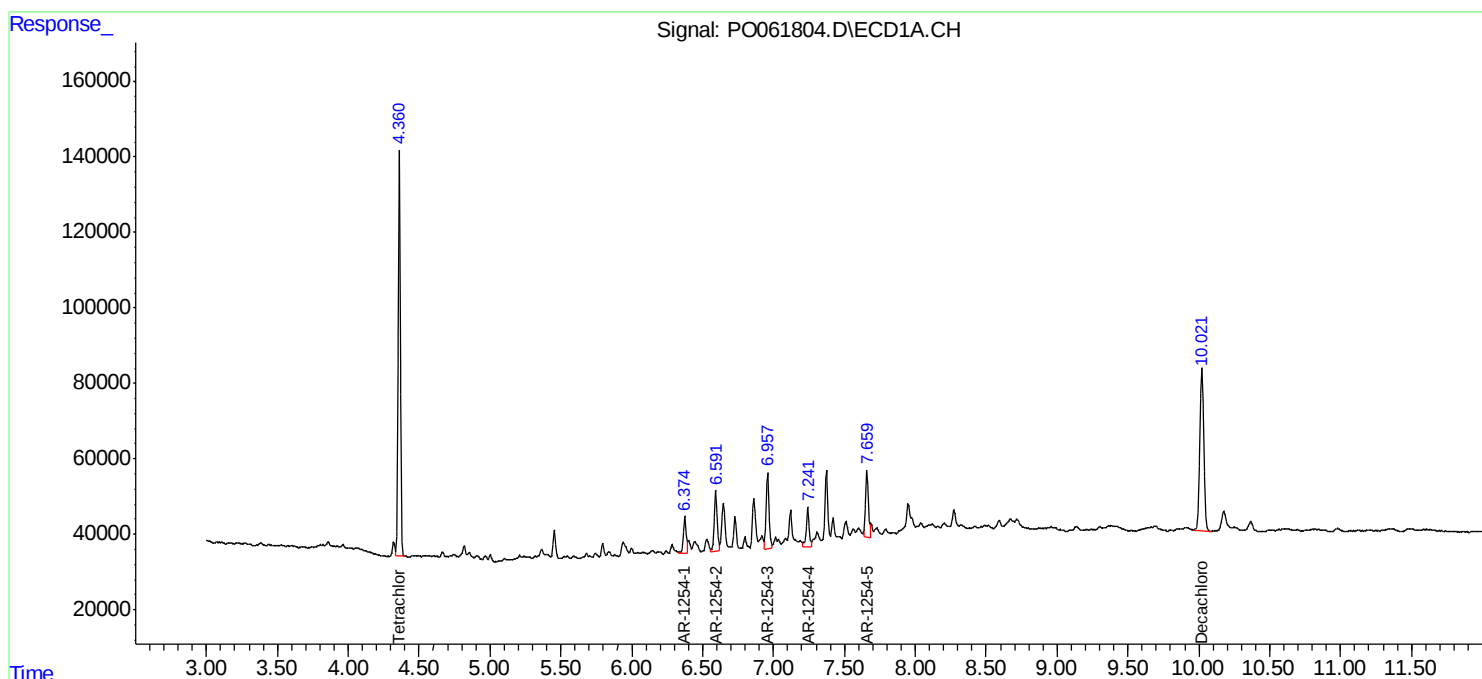

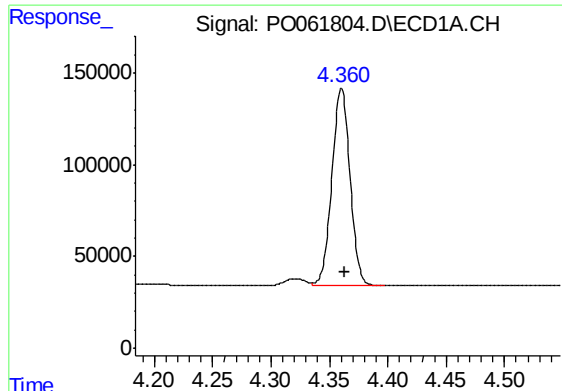


#1 Tetrachloro-m-xylene

R.T.: 4.360 min
Delta R.T.: -0.003 min
Response: 1162826
Conc: 28.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-03-100719


Manual Integrations
APPROVED

Ankita
10/9/2019 12:14:58 PM

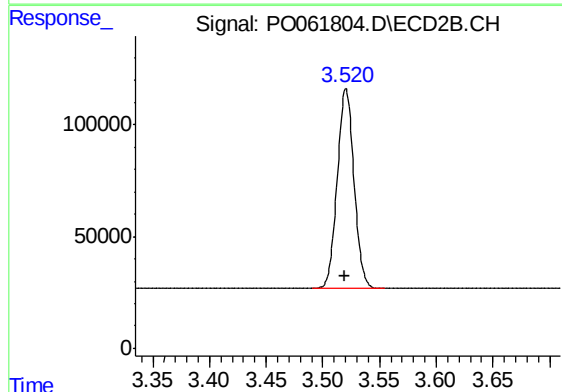


#1 Tetrachloro-m-xylene

R.T.: 3.520 min
Delta R.T.: 0.001 min
Response: 922307
Conc: 28.52 ng/ml

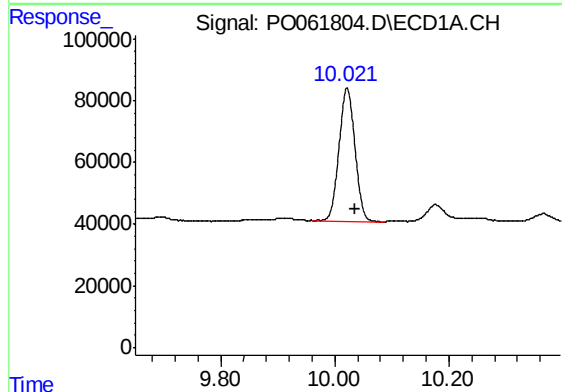


#2 Decachlorobiphenyl

R.T.: 10.021 min
Delta R.T.: -0.015 min
Response: 834337
Conc: 17.92 ng/ml

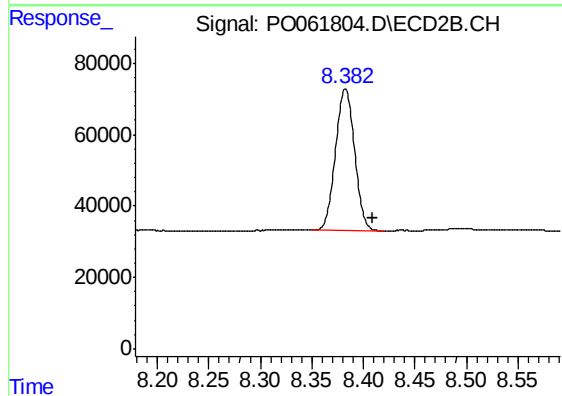

#2 Decachlorobiphenyl

R.T.: 8.383 min
Delta R.T.: -0.026 min
Response: 516518
Conc: 15.95 ng/ml

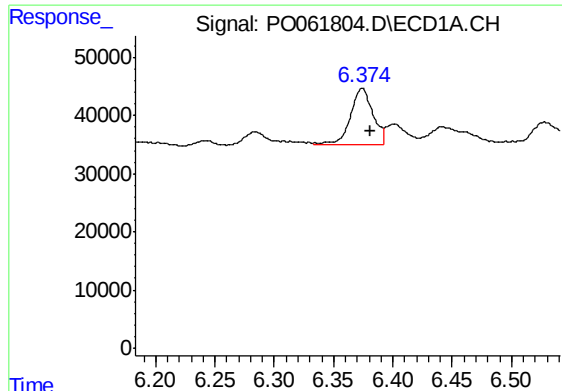


#26 AR-1254-1

R.T.: 6.374 min
Delta R.T.: -0.007 min
Response: 127215
Conc: 55.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-03-100719


Manual Integrations
APPROVED

Ankita
10/9/2019 12:14:58 PM

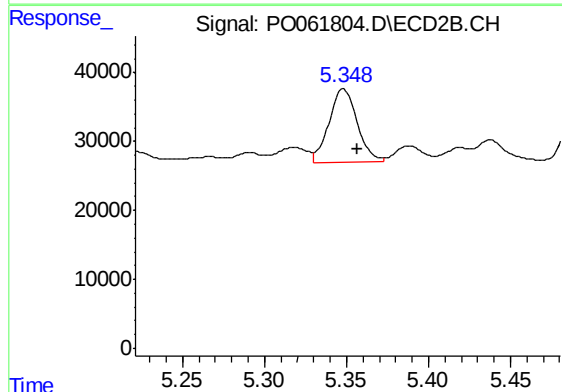


#26 AR-1254-1

R.T.: 5.348 min
Delta R.T.: -0.009 min
Response: 127730
Conc: 58.24 ng/ml

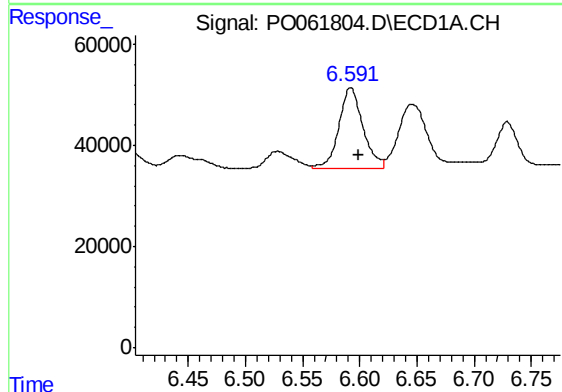


#27 AR-1254-2

R.T.: 6.592 min
Delta R.T.: -0.007 min
Response: 234860
Conc: 65.00 ng/ml

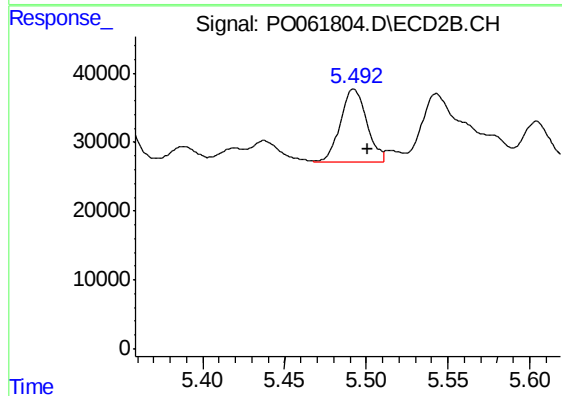

#27 AR-1254-2

R.T.: 5.493 min
Delta R.T.: -0.009 min
Response: 117990
Conc: 60.18 ng/ml

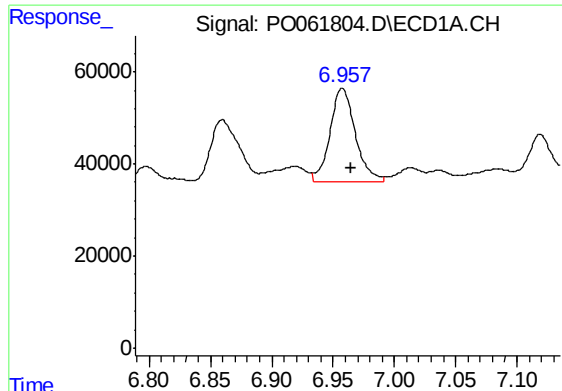


#28 AR-1254-3

R.T.: 6.957 min
Delta R.T.: -0.007 min
Response: 292201
Conc: 74.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-03-100719


Manual Integrations
APPROVED

Ankita
10/9/2019 12:14:58 PM

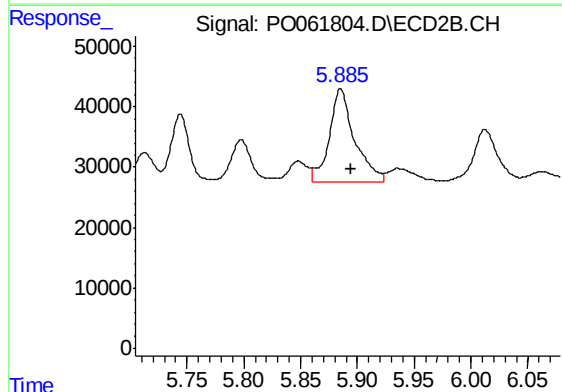


#28 AR-1254-3

R.T.: 5.885 min
Delta R.T.: -0.010 min
Response: 237144
Conc: 74.49 ng/ml

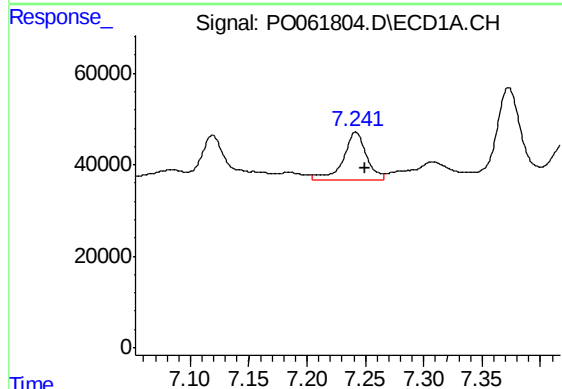


#29 AR-1254-4

R.T.: 7.242 min
Delta R.T.: -0.008 min
Response: 147972
Conc: 48.86 ng/ml

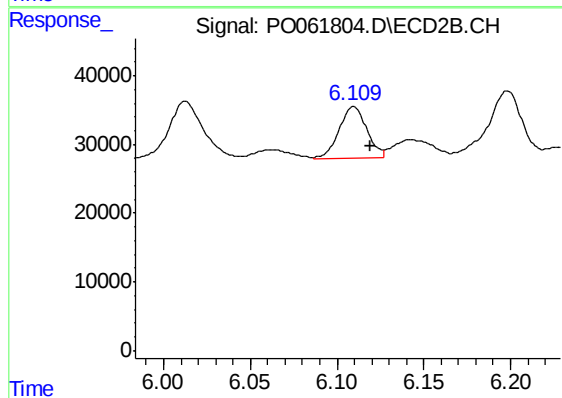

#29 AR-1254-4

R.T.: 6.110 min
Delta R.T.: -0.010 min
Response: 84316
Conc: 41.56 ng/ml

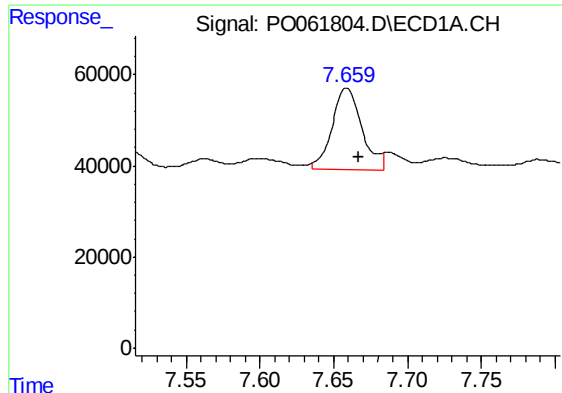


#30 AR-1254-5

R.T.: 7.659 min
Delta R.T.: -0.008 min
Response: 250275
Conc: 79.69 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OK-03-100719

Manual Integrations
APPROVED

Ankita
10/9/2019 12:14:58 PM

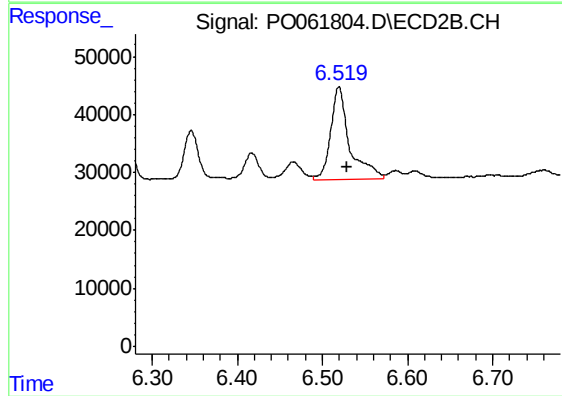

#30 AR-1254-5

R.T.: 6.520 min
Delta R.T.: -0.010 min
Response: 245330
Conc: 86.74 ng/ml