

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100819\
 Data File : P0061807.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2019 22:04
 Operator : HP/AJ
 Sample : K5152-01
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SU-02-100719

Manual Integrations
 APPROVED

Ankita
 10/9/2019 12:15:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 01:23:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.361	3.521	1108515	876828	27.028	27.113m
2) SA Decachlor...	10.023	8.384	786191	500196	16.882	15.450

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100819\
Data File : PO061807.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2019 22:04
Operator : HP/AJ
Sample : K5152-01
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SU-02-100719


Manual Integrations
APPROVED

Ankita
10/9/2019 12:15:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 01:23:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

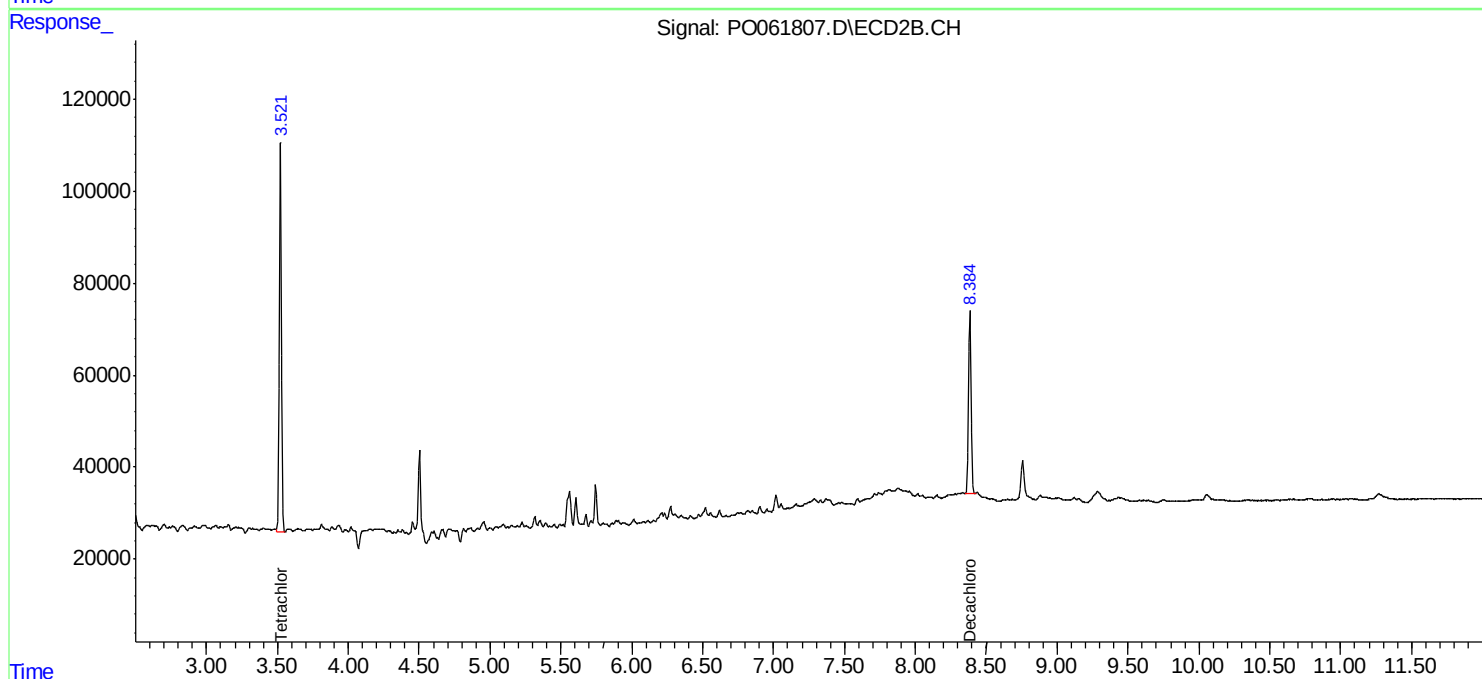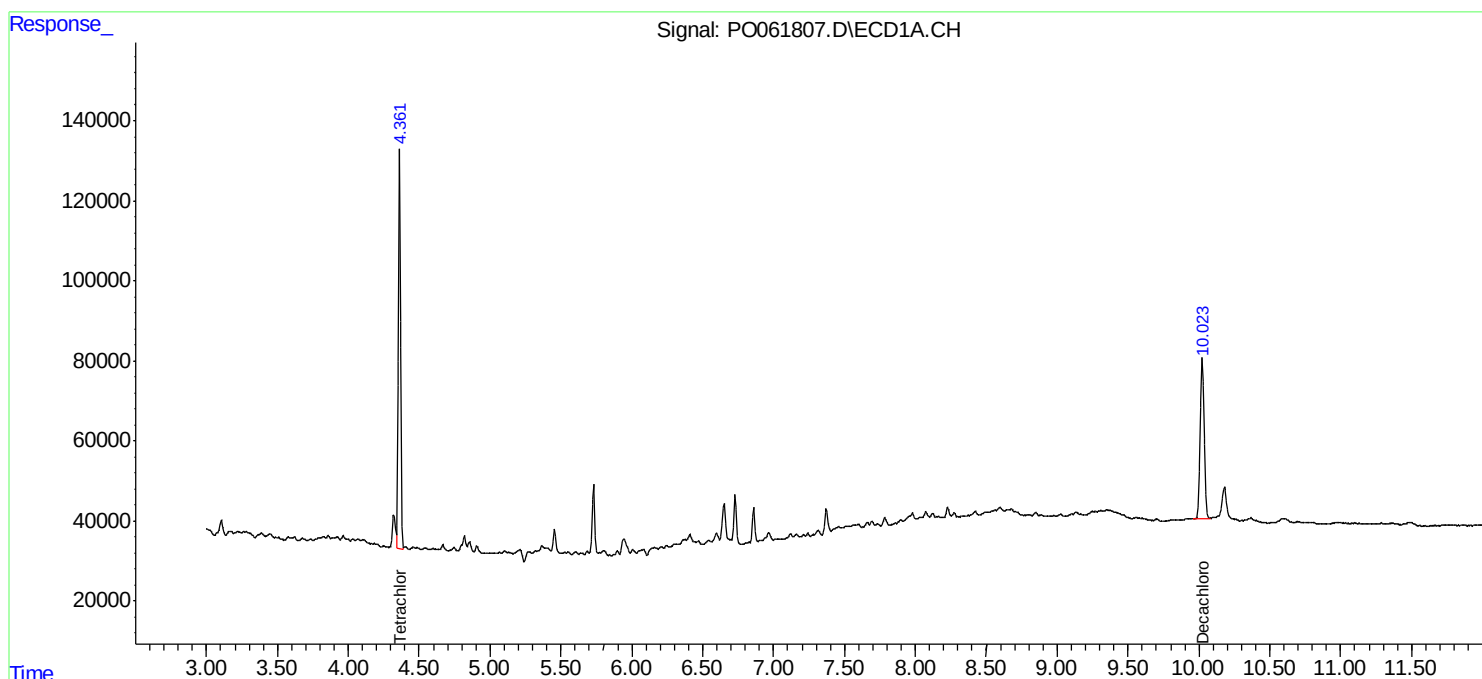

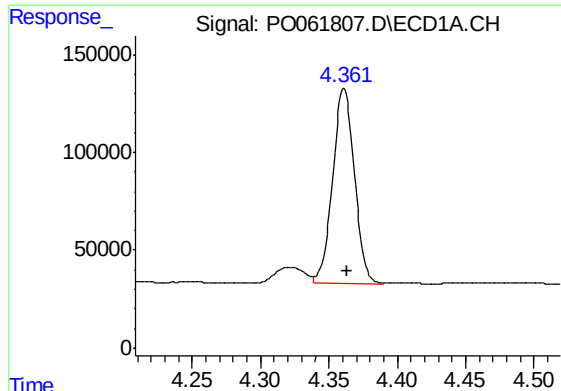


#1 Tetrachloro-m-xylene

R.T.: 4.361 min
Delta R.T.: -0.002 min
Response: 1108515
Conc: 27.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU-02-100719


Manual Integrations
APPROVED

Ankita
10/9/2019 12:15:05 PM

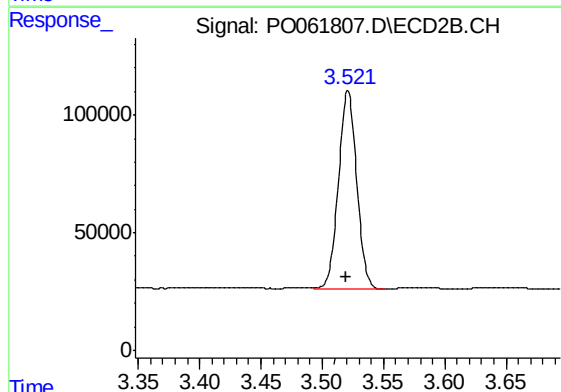


#1 Tetrachloro-m-xylene

R.T.: 3.521 min
Delta R.T.: 0.002 min
Response: 876828
Conc: 27.11 ng/ml m

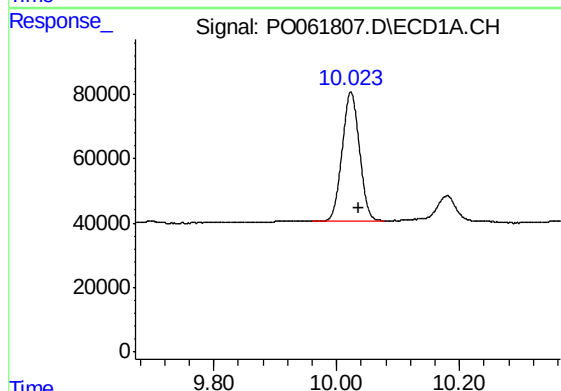

#2 Decachlorobiphenyl

R.T.: 10.023 min
Delta R.T.: -0.013 min
Response: 786191
Conc: 16.88 ng/ml

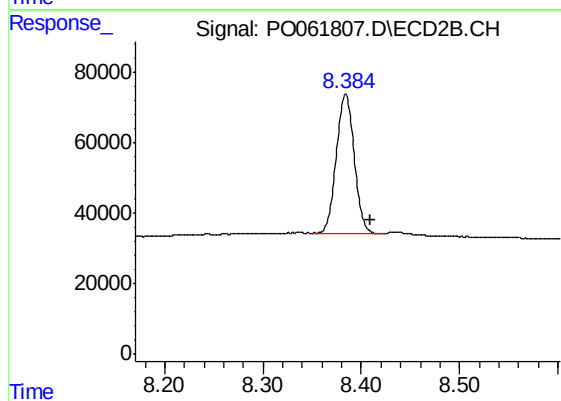

#2 Decachlorobiphenyl

R.T.: 8.384 min
Delta R.T.: -0.025 min
Response: 500196
Conc: 15.45 ng/ml