

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100918\
 Data File : PO049797.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Oct 2018 15:41
 Operator : SM/SJ
 Sample : J5223-03RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SSSI-1001-S-DH-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 00:55:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 08 15:27:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.388	3.513	4346912	3928288	19.229	16.287
2)	SA Decachlor...	10.097	8.438	4736487	3528891	14.215	13.491

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100918\
Data File : PO049797.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Oct 2018 15:41
Operator : SM/SJ
Sample : J5223-03RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SSSI-1001-S-DH-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 00:55:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100818.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 08 15:27:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

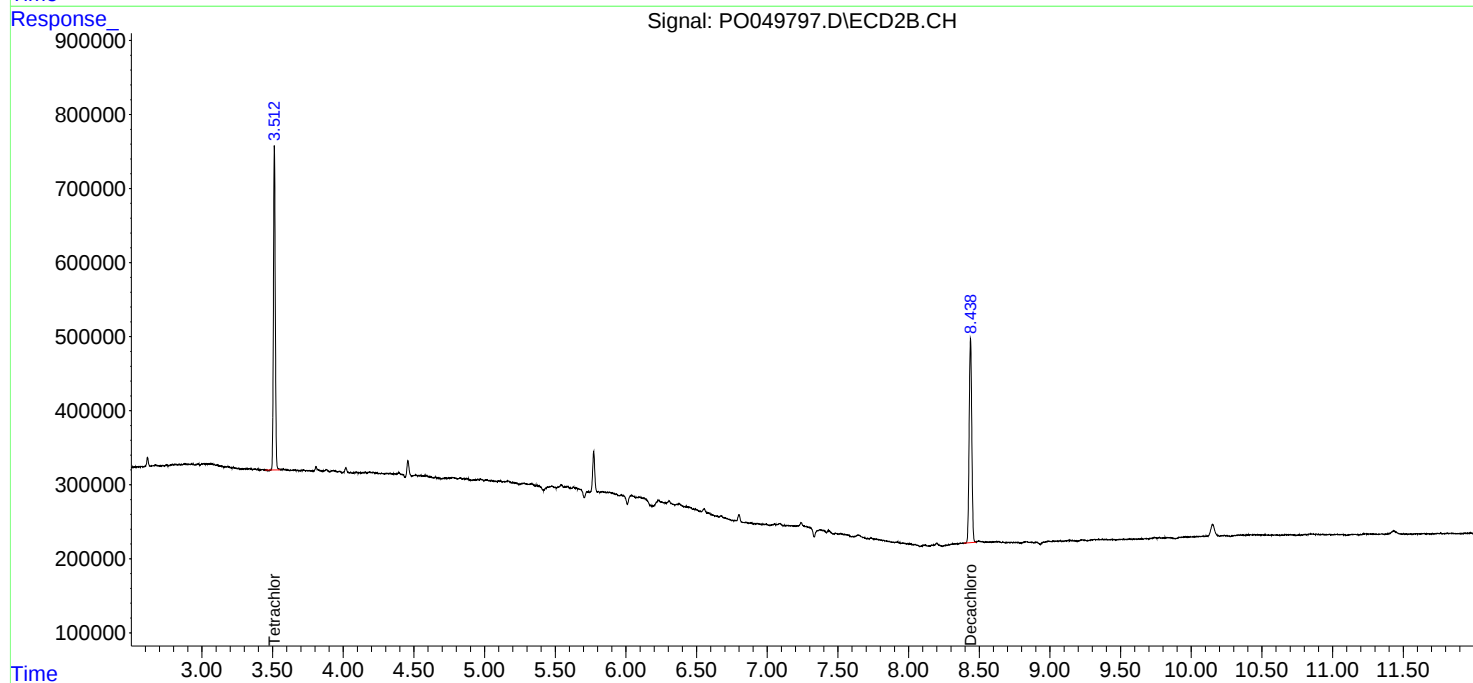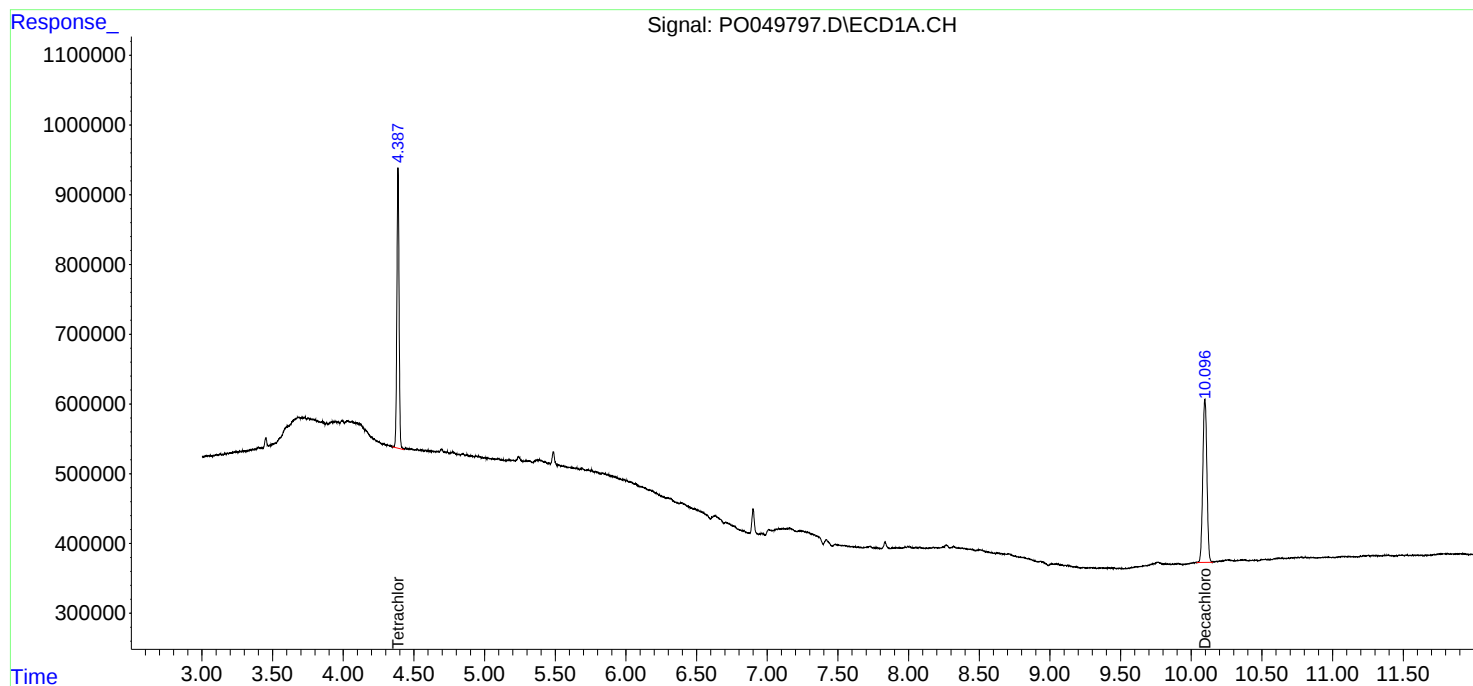


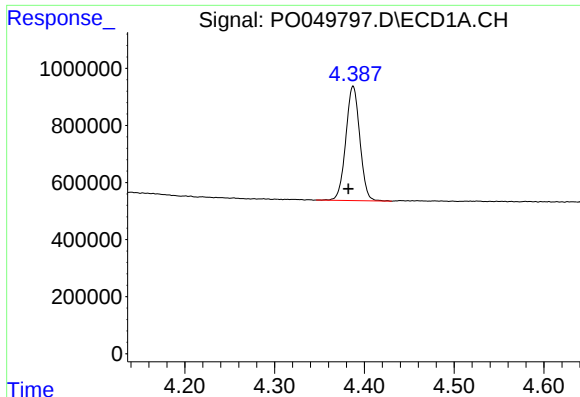

#1 Tetrachloro-m-xylene


R.T.: 4.388 min
Delta R.T.: 0.006 min
Response: 4346912
Conc: 19.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
SSSI-1001-S-DH-01

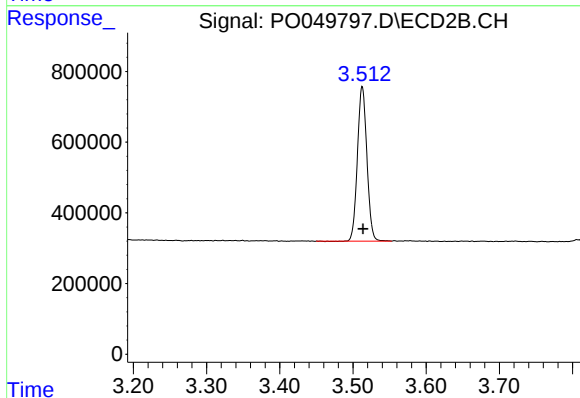


#1 Tetrachloro-m-xylene

R.T.: 3.513 min
Delta R.T.: -0.001 min
Response: 3928288
Conc: 16.29 ng/ml

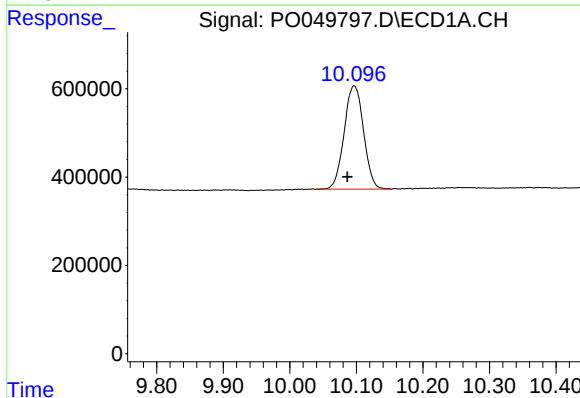

#2 Decachlorobiphenyl

R.T.: 10.097 min
Delta R.T.: 0.010 min
Response: 4736487
Conc: 14.22 ng/ml

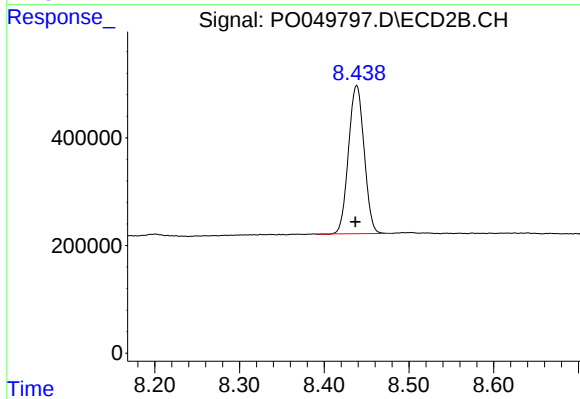

#2 Decachlorobiphenyl

R.T.: 8.438 min
Delta R.T.: 0.002 min
Response: 3528891
Conc: 13.49 ng/ml