

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100918\
 Data File : PO049842.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Oct 2018 3:44
 Operator : SM/SJ
 Sample : J5314-06
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DOCUMENTATION-23

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 05:08:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 08 15:27:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.383	3.513	5846719	5700140	25.864	23.633
2) SA Decachlor...	10.090	8.437	7312155	5446584	21.945	20.823

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100918\
Data File : PO049842.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Oct 2018 3:44
Operator : SM/SJ
Sample : J5314-06
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DOCUMENTATION-23

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 05:08:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100818.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 08 15:27:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

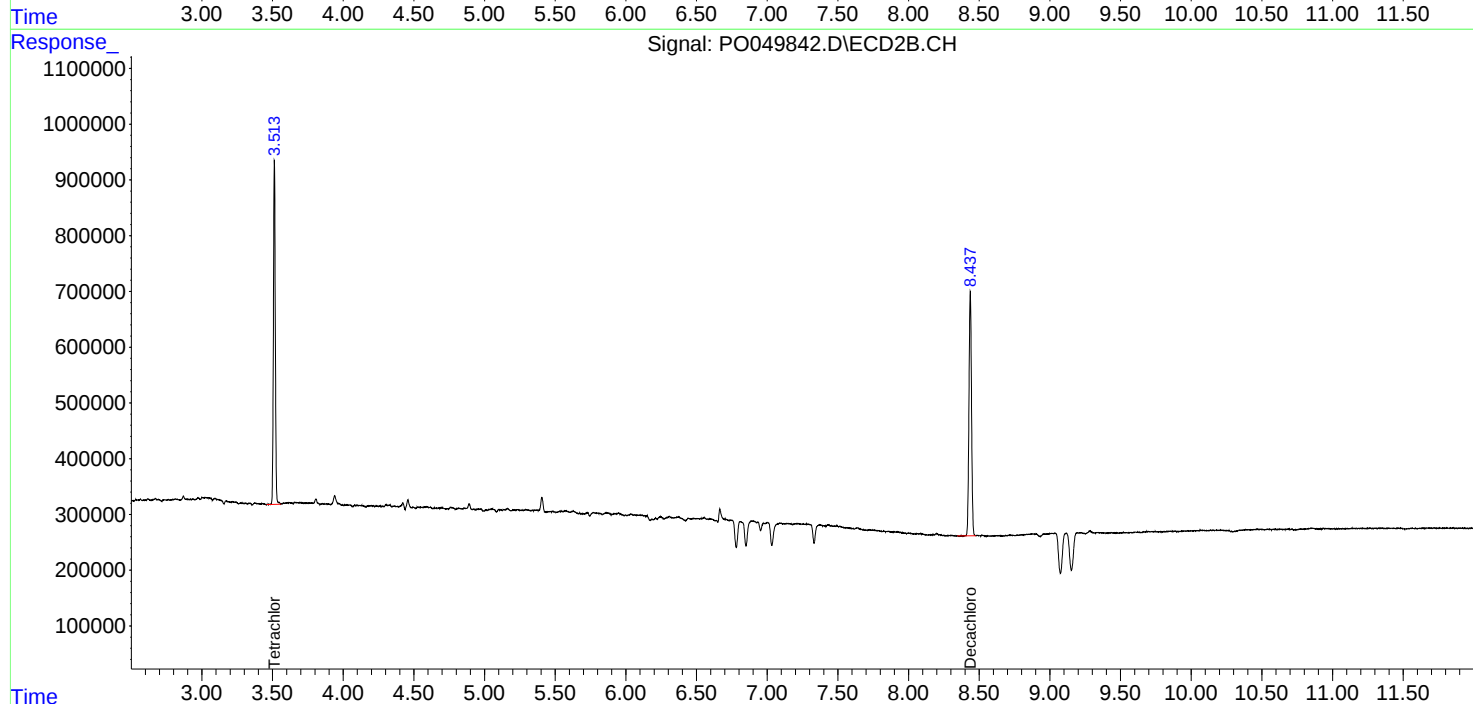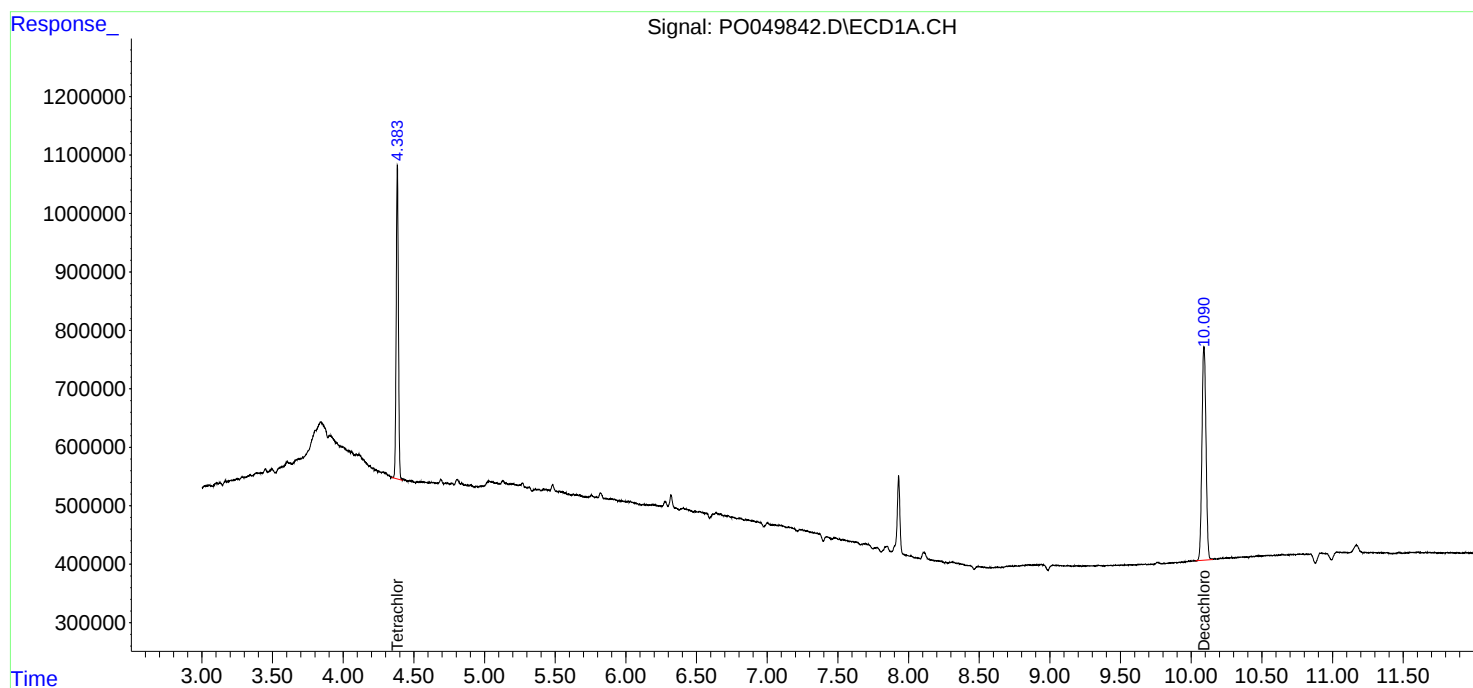


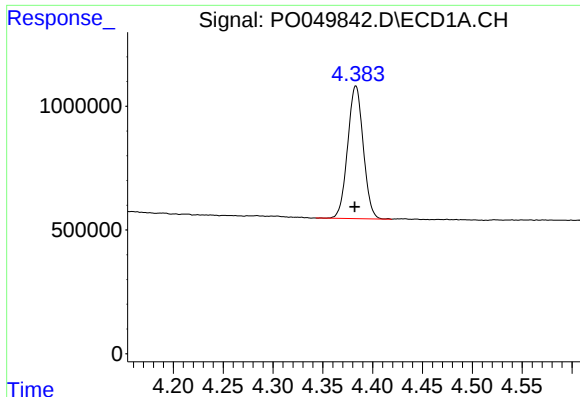

#1 Tetrachloro-m-xylene


R.T.: 4.383 min
Delta R.T.: 0.001 min
Response: 5846719
Conc: 25.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
DOCUMENTATION-23

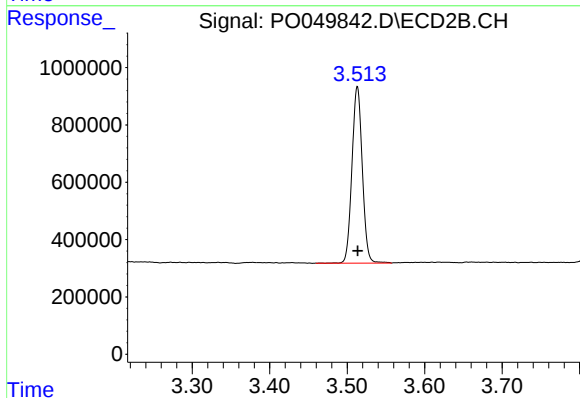


#1 Tetrachloro-m-xylene

R.T.: 3.513 min
Delta R.T.: 0.000 min
Response: 5700140
Conc: 23.63 ng/ml

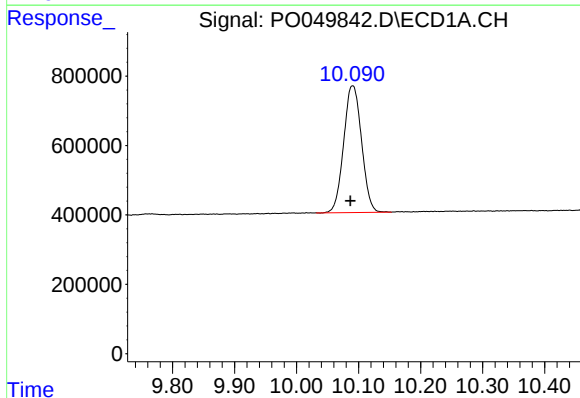

#2 Decachlorobiphenyl

R.T.: 10.090 min
Delta R.T.: 0.004 min
Response: 7312155
Conc: 21.95 ng/ml

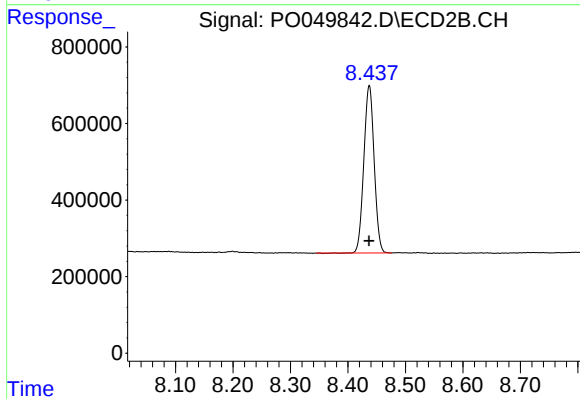

#2 Decachlorobiphenyl

R.T.: 8.437 min
Delta R.T.: 0.000 min
Response: 5446584
Conc: 20.82 ng/ml