

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100919\
 Data File : PO061827.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Oct 2019 13:47
 Operator : HP/AJ
 Sample : K5241-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONCRETE-PILE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 14:01:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.349	3.511	1206539	913767	29.418	28.255
2)	SA Decachlor...	10.004	8.369	866159	489038	18.599	15.105
Target Compounds							
3)	L1 AR-1016-1	5.579	4.572	6208	7640	3.385	5.682 #
4)	L1 AR-1016-2	5.579	4.612	6208	217	2.402	0.117 #
5)	L1 AR-1016-3	5.635	4.789	678	831	0.422	0.829 #
6)	L1 AR-1016-4	5.712	4.800	868	906	0.650	1.046 #
7)	L1 AR-1016-5	6.011	5.029	647	940	0.472	0.824 #
8)	L2 AR-1221-1	0.000	3.729	0	242	N.D.	0.612 #
9)	L2 AR-1221-2	4.653	3.798	14113	16622	39.308	53.897 #
10)	L2 AR-1221-3	4.720	3.872	4084	2458	3.587	2.695
11)	L3 AR-1232-1	4.720	3.872	4084	2458	2.920	2.189 #
12)	L3 AR-1232-2	5.248	4.612	3378	217	4.306	0.178 #
13)	L3 AR-1232-3	5.579	4.752	6208	383	3.633	0.579 #
14)	L3 AR-1232-4	5.712	4.800	868	906	0.981	1.438 #
15)	L3 AR-1232-5	5.785	5.010	4023	886	5.803	1.291 #
16)	L4 AR-1242-1	5.512	4.572	3404	7640	2.397	7.457 #
17)	L4 AR-1242-2	5.579	4.572	6208	7640	3.089	5.417 #
18)	L4 AR-1242-3	5.635	4.752	678	383	0.537	0.490
19)	L4 AR-1242-4	5.712	4.800	868	906	0.826	1.104 #
20)	L4 AR-1242-5	6.414	5.359	7083	6472	5.296	6.042
21)	L5 AR-1248-1	5.579	4.572	6208	7640	5.284	8.538 #
22)	L5 AR-1248-2	5.814	4.800	5657	906	3.353	0.769 #
23)	L5 AR-1248-3	6.011	4.800	647	906	0.346	0.730 #
24)	L5 AR-1248-4	6.414	5.029	7083	940	2.998	0.626 #
25)	L5 AR-1248-5	6.518	5.447	16511	4340	7.282	2.829 #
26)	L6 AR-1254-1	6.392	5.359	6193	6472	2.714	2.951
27)	L6 AR-1254-2	6.583	5.504	15462	7326	4.280	3.737
28)	L6 AR-1254-3	6.956	5.893	29518	4775	7.555	1.500 #
29)	L6 AR-1254-4	7.258	6.120	8108	674	2.677	0.332 #
30)	L6 AR-1254-5	7.663	6.541	76038	11962	24.213	4.229 #
31)	L7 AR-1260-1	7.165	6.045	18134	303	6.947	0.149 #
32)	L7 AR-1260-2	7.430	6.217	44483	2069	13.953	0.861 #
33)	L7 AR-1260-3	7.756	6.355	14290	1074	5.950	0.477 #
34)	L7 AR-1260-4	7.990	6.838	49065	4767	18.362	2.582 #
35)	L7 AR-1260-5	8.288	7.037	10948	1697	2.213	0.436 #
36)	L8 AR-1262-1	7.725	6.605	37967	843	9.909	0.691 #
37)	L8 AR-1262-2	8.288	7.037	10948	1697	1.764	0.369 #
38)	L8 AR-1262-3	8.581	7.328	53121	4150	12.781	2.203 #
39)	L8 AR-1262-4	8.676	7.389	28359	2211	8.983	0.658 #
40)	L8 AR-1262-5	9.290	7.885	79454	1300	39.070	0.858 #
41)	L9 AR-1268-1	8.581	7.328	53121	4150	7.900	0.859 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100919\
Data File : PO061827.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Oct 2019 13:47
Operator : HP/AJ
Sample : K5241-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 14:01:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.676	7.389	28359	2211	4.580	0.513 #
43)	L9 AR-1268-3	8.916	7.610	32886	791	6.433	0.221 #
44)	L9 AR-1268-4	9.290	7.885	79454	1300	36.337	0.808 #
45)	L9 AR-1268-5	9.681	8.154	9782	2122	0.651	0.211 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100919\
Data File : P0061827.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Oct 2019 13:47
Operator : HP/AJ
Sample : K5241-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 14:01:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

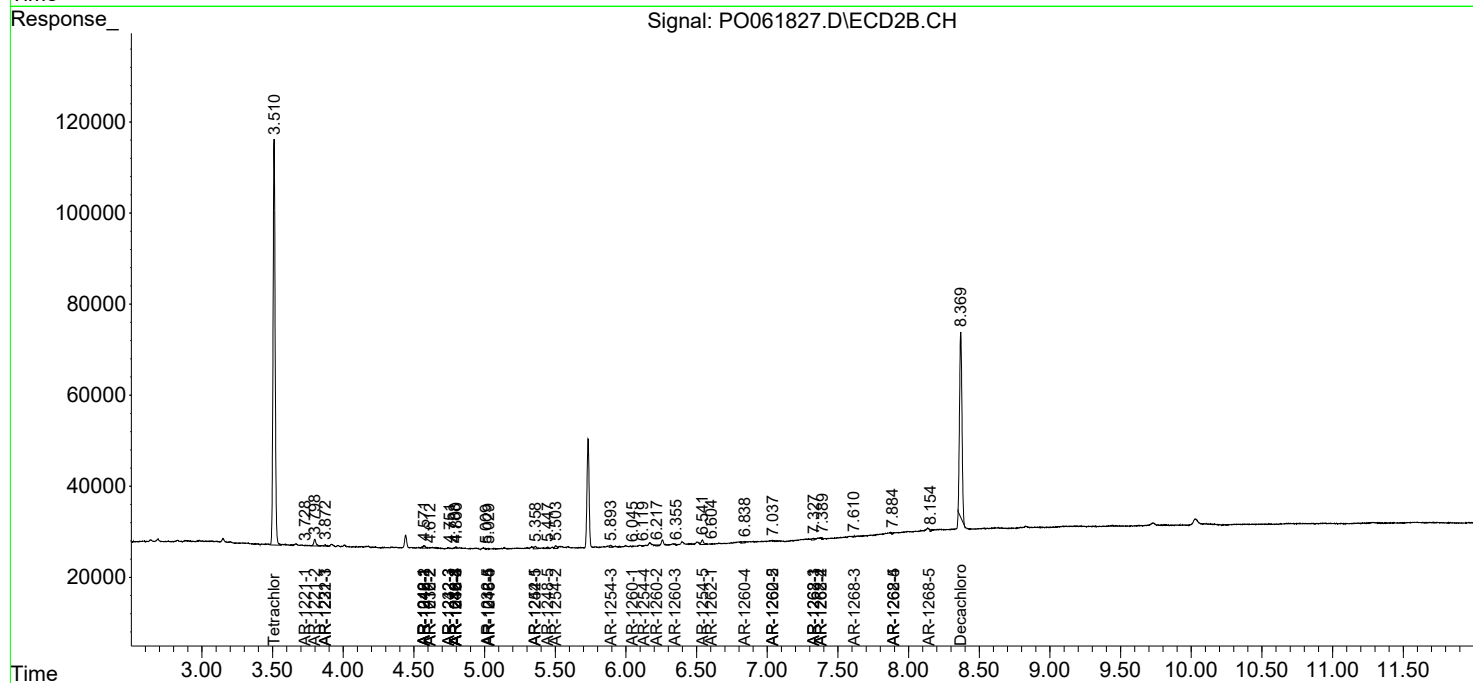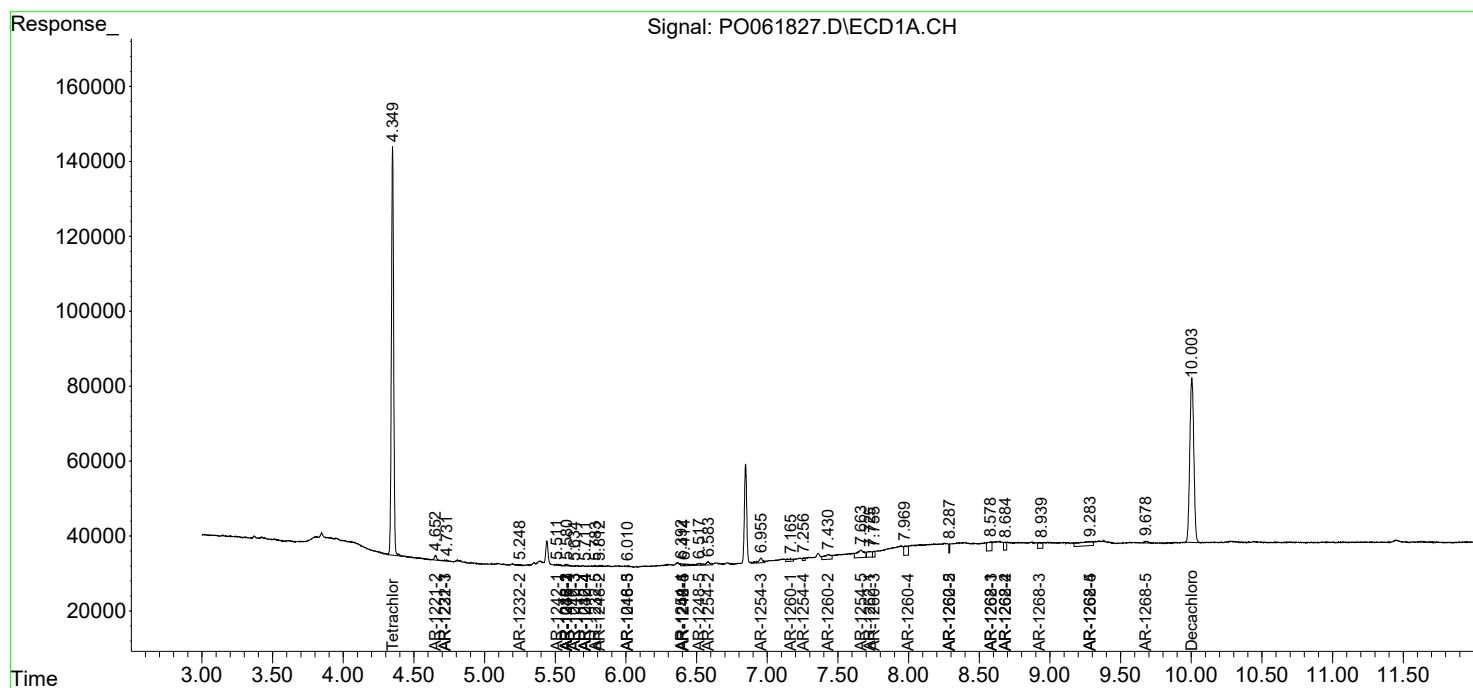


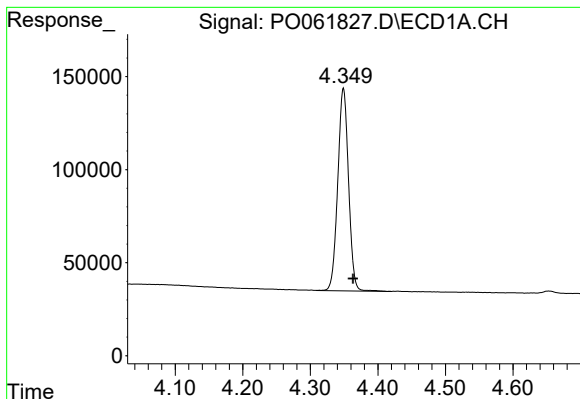

#1 Tetrachloro-m-xylene


R.T.: 4.349 min
Delta R.T.: -0.014 min
Response: 1206539
Conc: 29.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

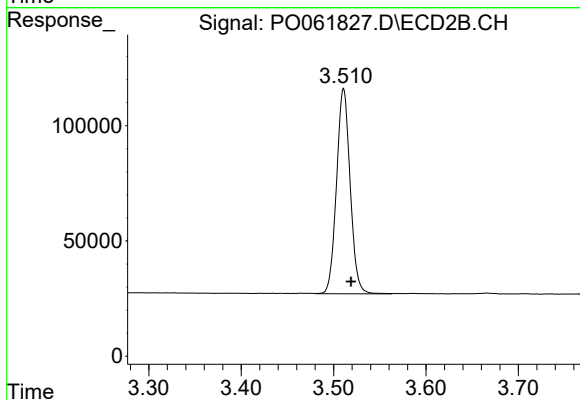


#1 Tetrachloro-m-xylene

R.T.: 3.511 min
Delta R.T.: -0.008 min
Response: 913767
Conc: 28.26 ng/ml

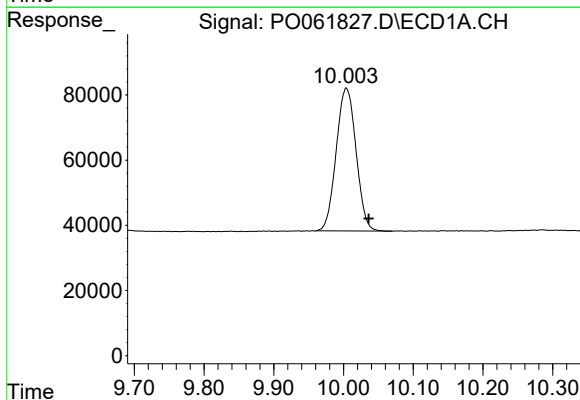


#2 Decachlorobiphenyl

R.T.: 10.004 min
Delta R.T.: -0.032 min
Response: 866159
Conc: 18.60 ng/ml

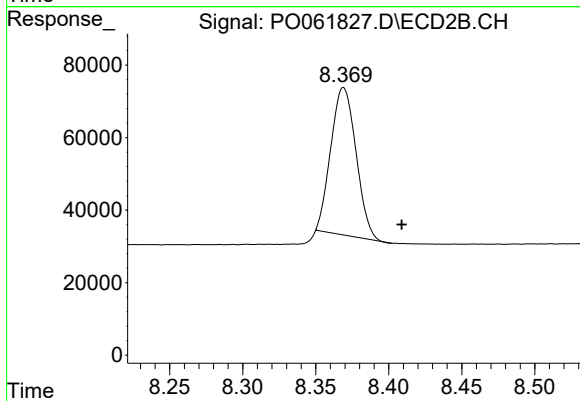

#2 Decachlorobiphenyl


R.T.: 8.369 min
Delta R.T.: -0.040 min
Response: 489038
Conc: 15.11 ng/ml

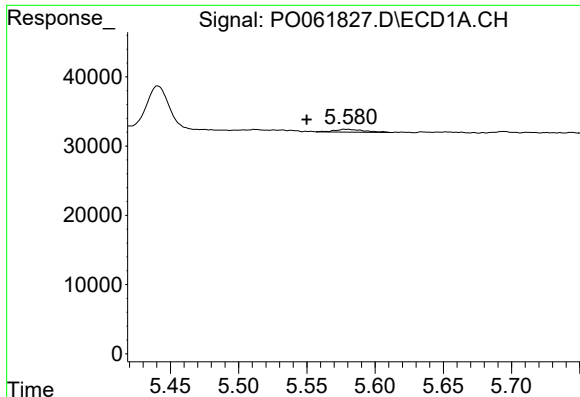

#3 AR-1016-1


R.T.: 5.579 min
Delta R.T.: 0.029 min
Response: 6208
Conc: 3.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

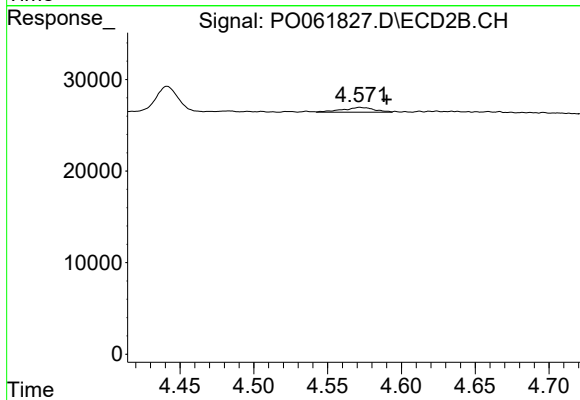


#3 AR-1016-1

R.T.: 4.572 min
Delta R.T.: -0.018 min
Response: 7640
Conc: 5.68 ng/ml

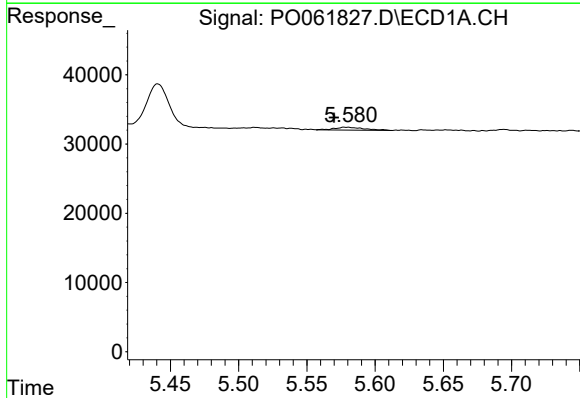


#4 AR-1016-2

R.T.: 5.579 min
Delta R.T.: 0.009 min
Response: 6208
Conc: 2.40 ng/ml

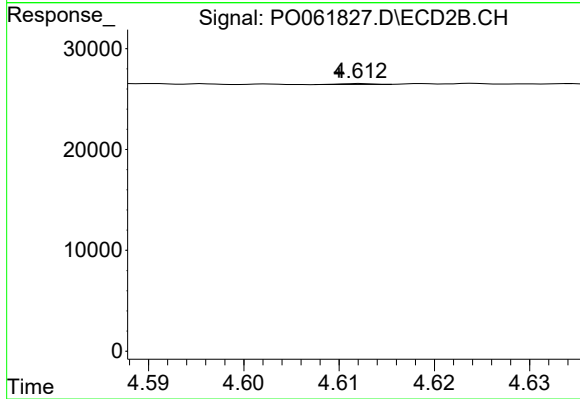

#4 AR-1016-2


R.T.: 4.612 min
Delta R.T.: 0.002 min
Response: 217
Conc: 0.12 ng/ml

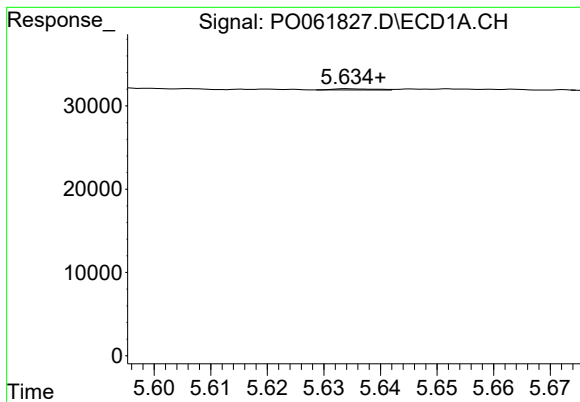

#5 AR-1016-3


R.T.: 5.635 min
Delta R.T.: -0.005 min
Response: 678
Conc: 0.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

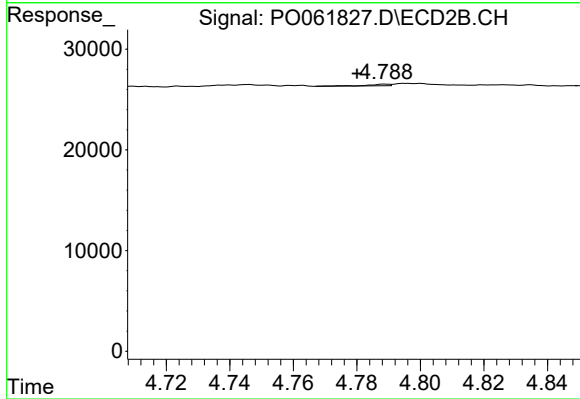


#5 AR-1016-3

R.T.: 4.789 min
Delta R.T.: 0.009 min
Response: 831
Conc: 0.83 ng/ml

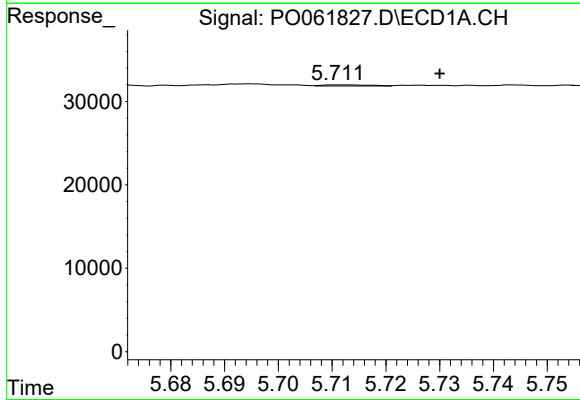


#6 AR-1016-4

R.T.: 5.712 min
Delta R.T.: -0.018 min
Response: 868
Conc: 0.65 ng/ml

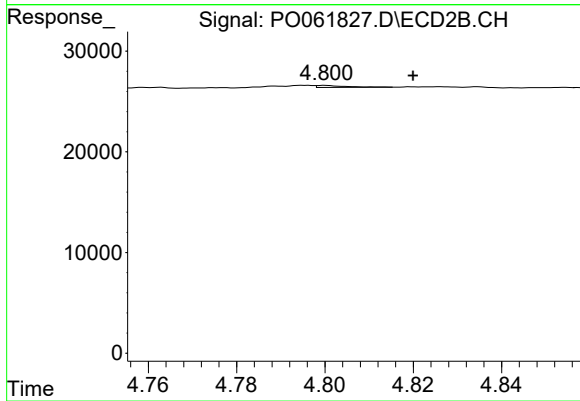

#6 AR-1016-4


R.T.: 4.800 min
Delta R.T.: -0.020 min
Response: 906
Conc: 1.05 ng/ml

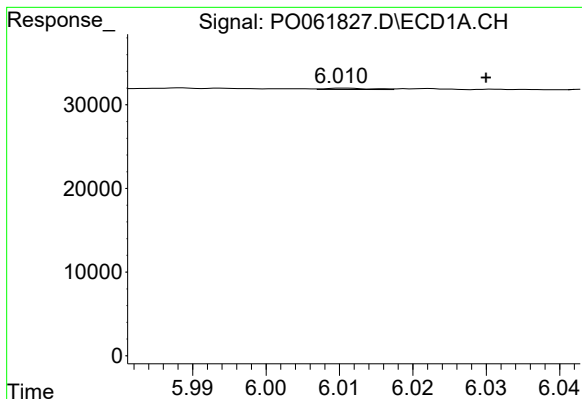

#7 AR-1016-5


R.T.: 6.011 min
Delta R.T.: -0.019 min
Response: 647
Conc: 0.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

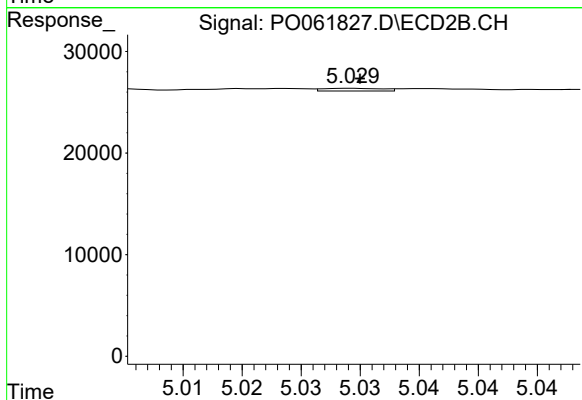


#7 AR-1016-5

R.T.: 5.029 min
Delta R.T.: 0.000 min
Response: 940
Conc: 0.82 ng/ml

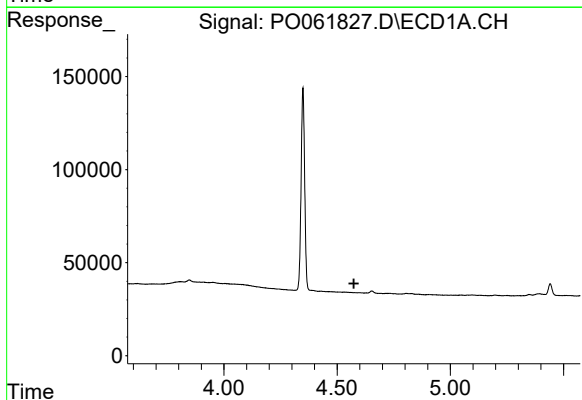


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.574 min
Response: 0
Conc: N.D.

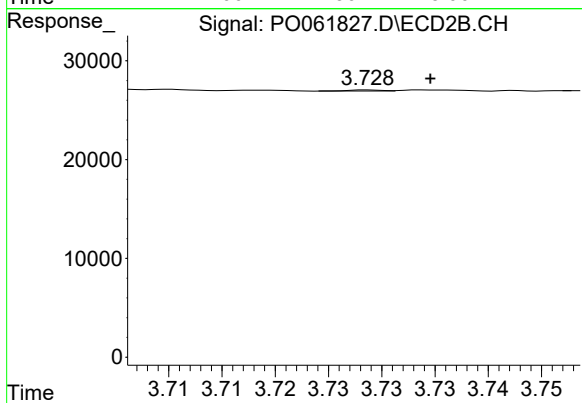

#8 AR-1221-1


R.T.: 3.729 min
Delta R.T.: -0.006 min
Response: 242
Conc: 0.61 ng/ml

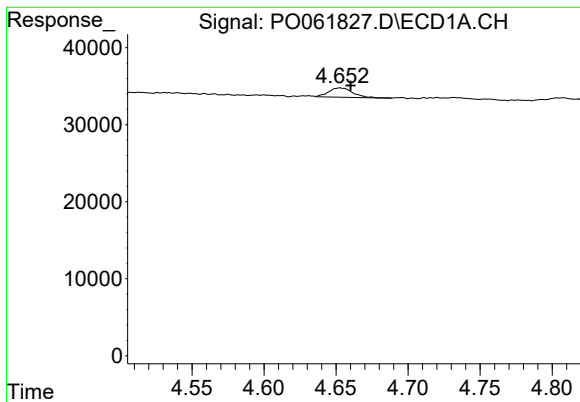

#9 AR-1221-2


R.T.: 4.653 min
Delta R.T.: -0.007 min
Response: 14113
Conc: 39.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

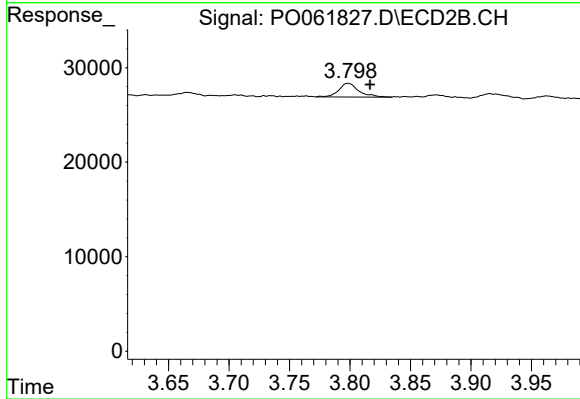


#9 AR-1221-2

R.T.: 3.798 min
Delta R.T.: -0.018 min
Response: 16622
Conc: 53.90 ng/ml

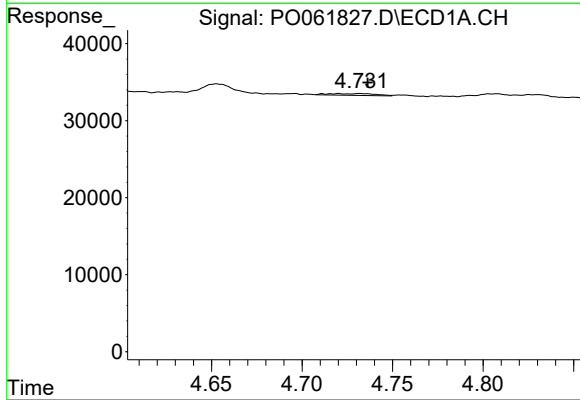


#10 AR-1221-3

R.T.: 4.720 min
Delta R.T.: -0.016 min
Response: 4084
Conc: 3.59 ng/ml

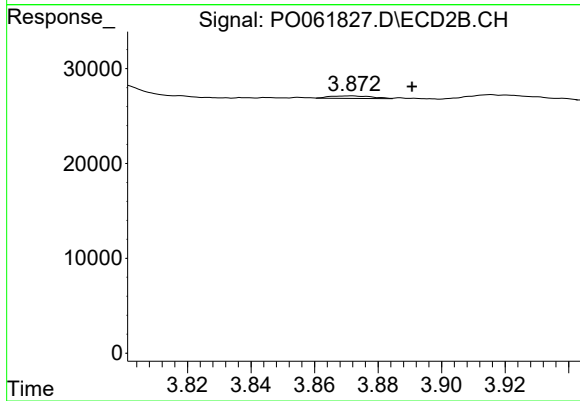

#10 AR-1221-3


R.T.: 3.872 min
Delta R.T.: -0.019 min
Response: 2458
Conc: 2.69 ng/ml

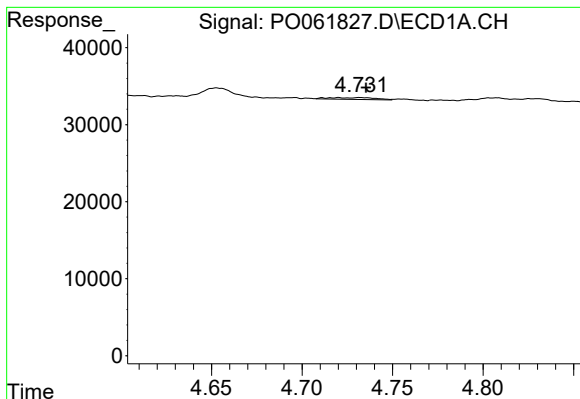

#11 AR-1232-1


R.T.: 4.720 min
Delta R.T.: -0.015 min
Response: 4084
Conc: 2.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

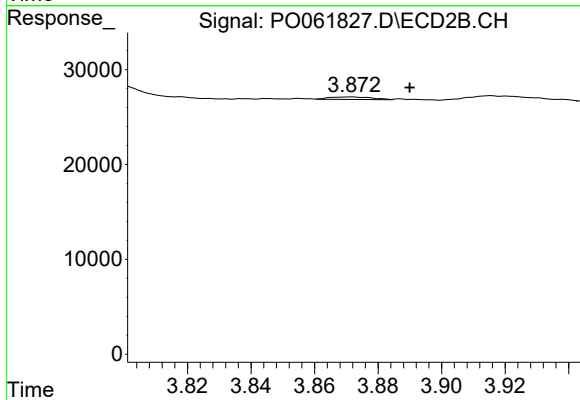


#11 AR-1232-1

R.T.: 3.872 min
Delta R.T.: -0.018 min
Response: 2458
Conc: 2.19 ng/ml

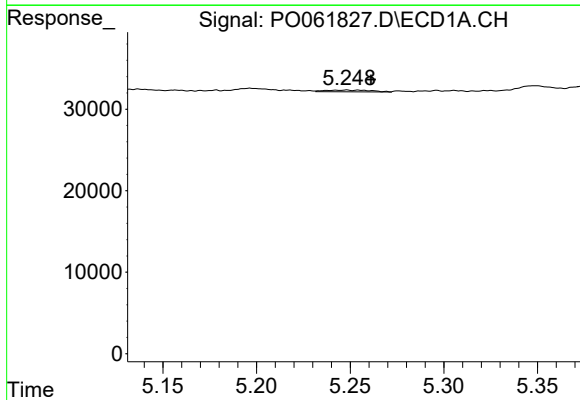


#12 AR-1232-2

R.T.: 5.248 min
Delta R.T.: -0.013 min
Response: 3378
Conc: 4.31 ng/ml

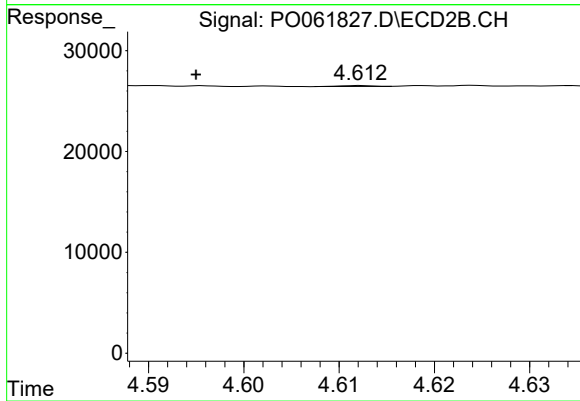

#12 AR-1232-2


R.T.: 4.612 min
Delta R.T.: 0.017 min
Response: 217
Conc: 0.18 ng/ml

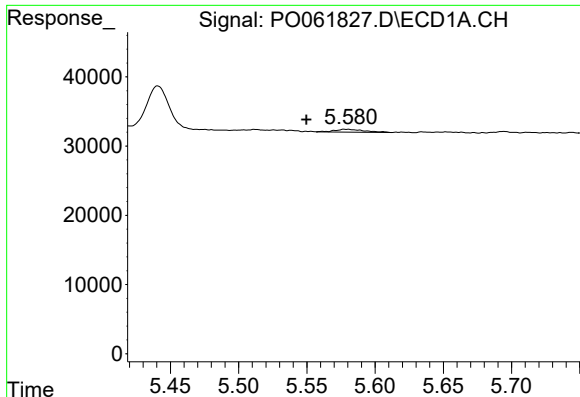

#13 AR-1232-3


R.T.: 5.579 min
Delta R.T.: 0.029 min
Response: 6208
Conc: 3.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

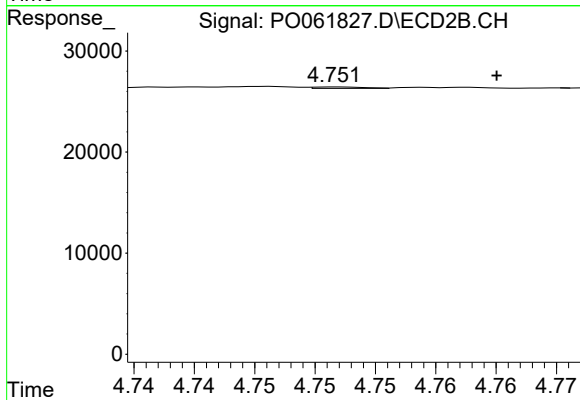


#13 AR-1232-3

R.T.: 4.752 min
Delta R.T.: -0.013 min
Response: 383
Conc: 0.58 ng/ml

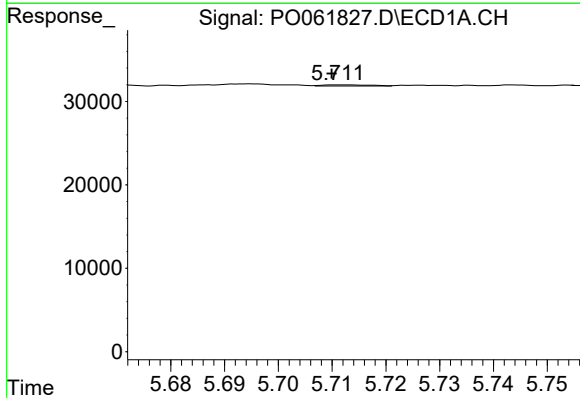


#14 AR-1232-4

R.T.: 5.712 min
Delta R.T.: 0.002 min
Response: 868
Conc: 0.98 ng/ml

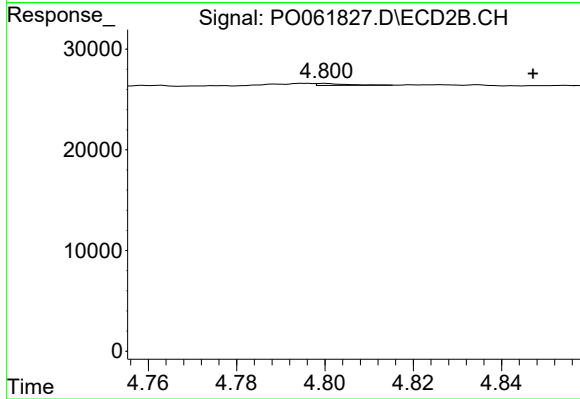

#14 AR-1232-4


R.T.: 4.800 min
Delta R.T.: -0.047 min
Response: 906
Conc: 1.44 ng/ml

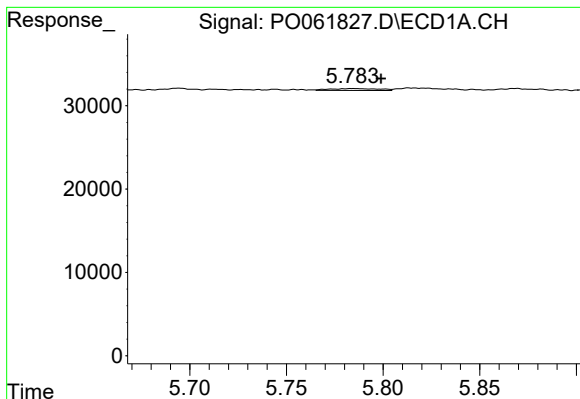

#15 AR-1232-5


R.T.: 5.785 min
Delta R.T.: -0.014 min
Response: 4023
Conc: 5.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

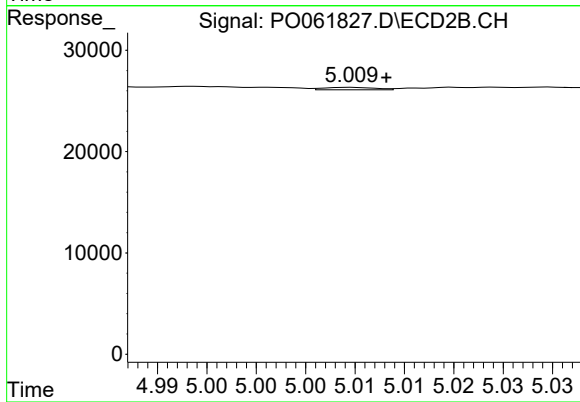


#15 AR-1232-5

R.T.: 5.010 min
Delta R.T.: -0.004 min
Response: 886
Conc: 1.29 ng/ml

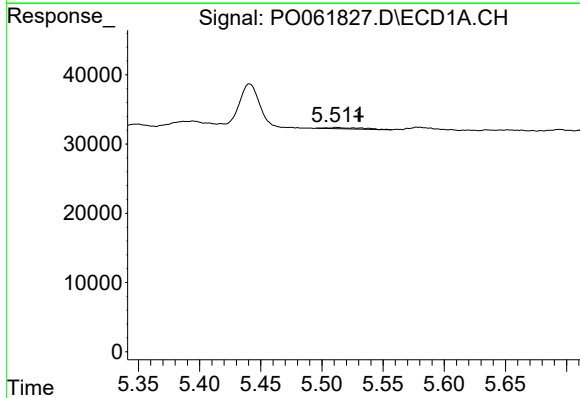


#16 AR-1242-1

R.T.: 5.512 min
Delta R.T.: -0.018 min
Response: 3404
Conc: 2.40 ng/ml

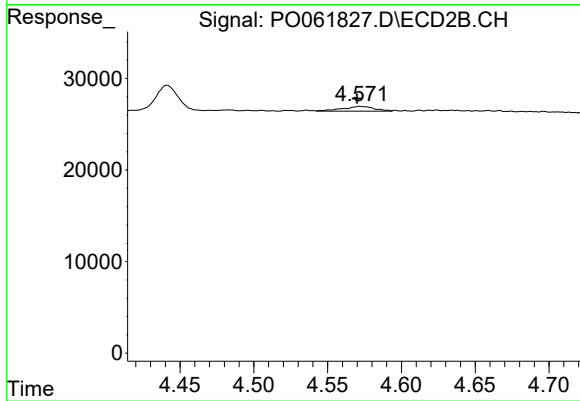

#16 AR-1242-1


R.T.: 4.572 min
Delta R.T.: 0.002 min
Response: 7640
Conc: 7.46 ng/ml

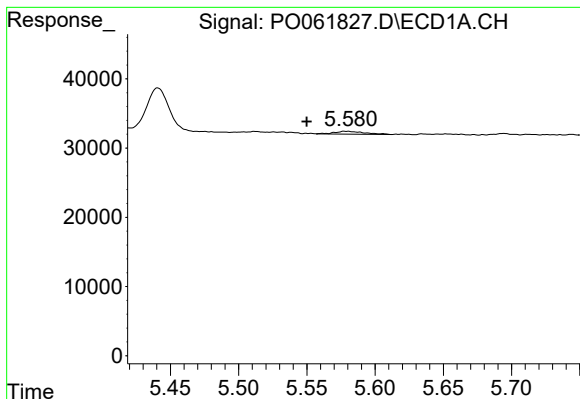

#17 AR-1242-2


R.T.: 5.579 min
Delta R.T.: 0.029 min
Response: 6208
Conc: 3.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

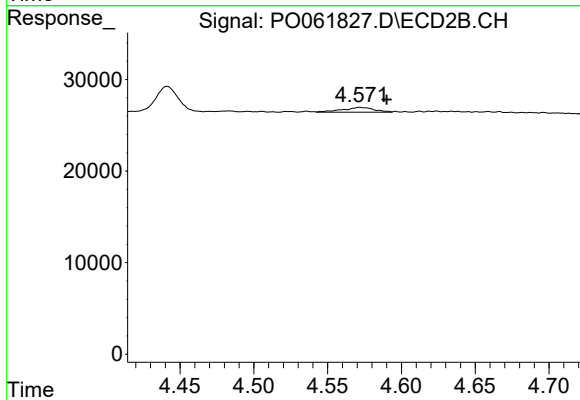


#17 AR-1242-2

R.T.: 4.572 min
Delta R.T.: -0.018 min
Response: 7640
Conc: 5.42 ng/ml

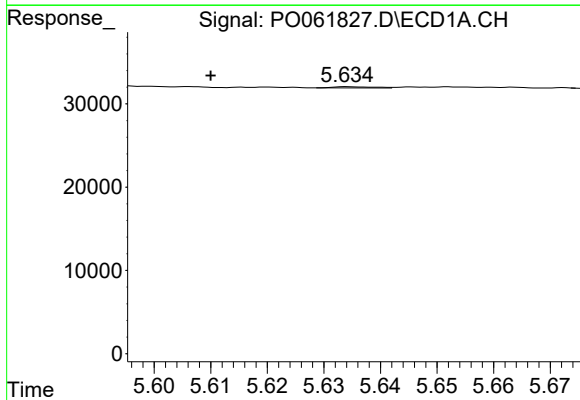


#18 AR-1242-3

R.T.: 5.635 min
Delta R.T.: 0.025 min
Response: 678
Conc: 0.54 ng/ml

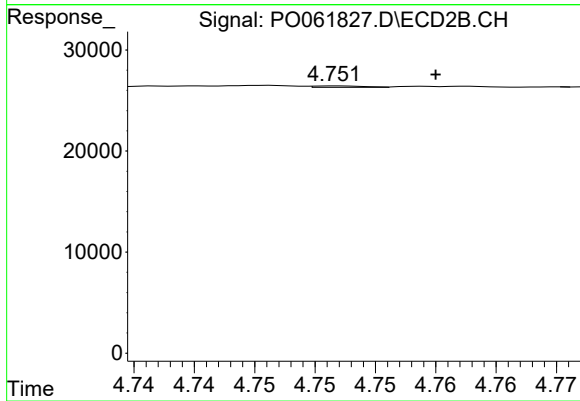

#18 AR-1242-3


R.T.: 4.752 min
Delta R.T.: -0.008 min
Response: 383
Conc: 0.49 ng/ml

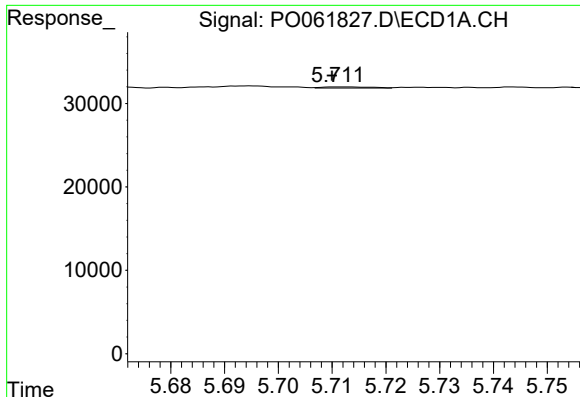

#19 AR-1242-4


R.T.: 5.712 min
Delta R.T.: 0.002 min
Response: 868
Conc: 0.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

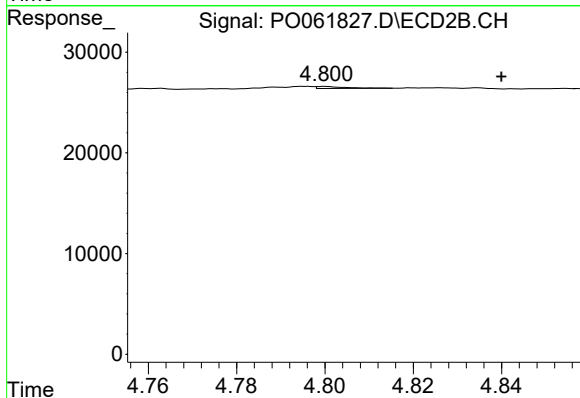


#19 AR-1242-4

R.T.: 4.800 min
Delta R.T.: -0.040 min
Response: 906
Conc: 1.10 ng/ml

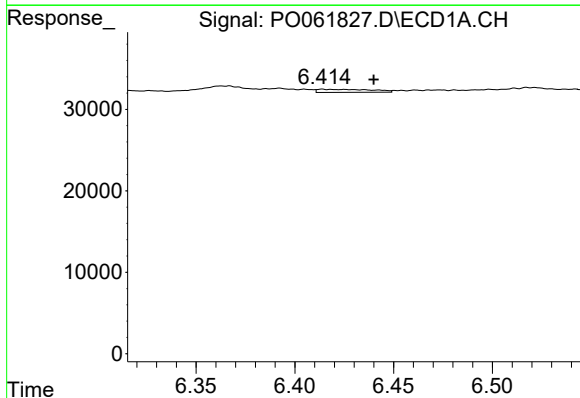


#20 AR-1242-5

R.T.: 6.414 min
Delta R.T.: -0.026 min
Response: 7083
Conc: 5.30 ng/ml

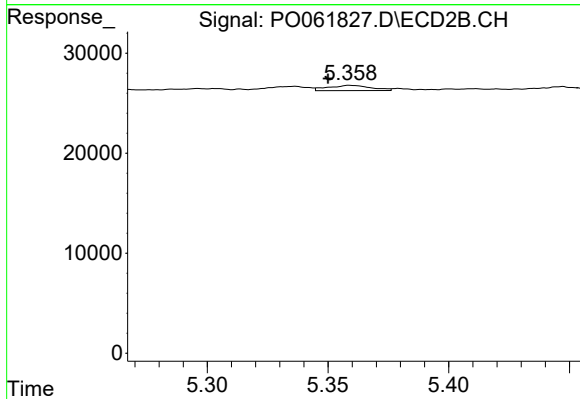

#20 AR-1242-5


R.T.: 5.359 min
Delta R.T.: 0.009 min
Response: 6472
Conc: 6.04 ng/ml

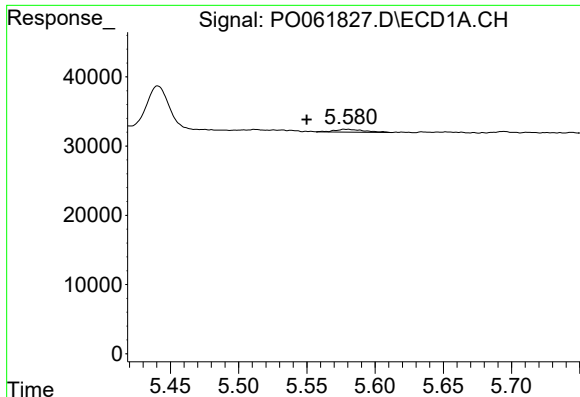

#21 AR-1248-1


R.T.: 5.579 min
Delta R.T.: 0.029 min
Response: 6208
Conc: 5.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

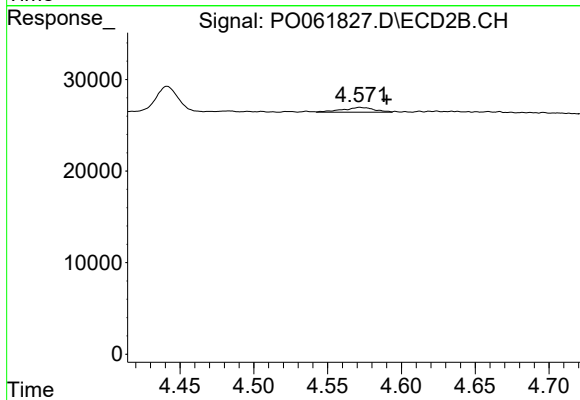


#21 AR-1248-1

R.T.: 4.572 min
Delta R.T.: -0.018 min
Response: 7640
Conc: 8.54 ng/ml

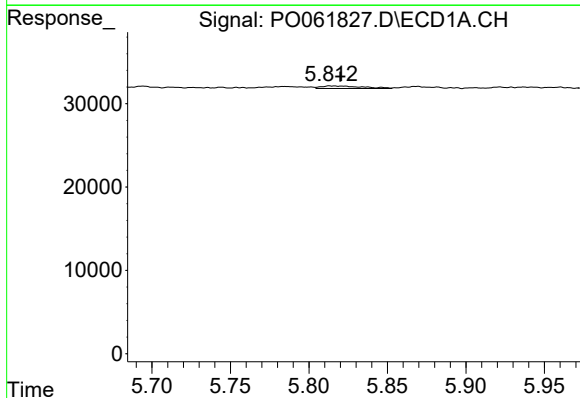


#22 AR-1248-2

R.T.: 5.814 min
Delta R.T.: -0.006 min
Response: 5657
Conc: 3.35 ng/ml

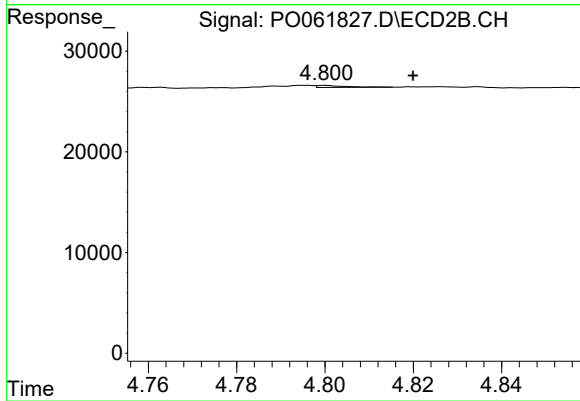

#22 AR-1248-2


R.T.: 4.800 min
Delta R.T.: -0.020 min
Response: 906
Conc: 0.77 ng/ml

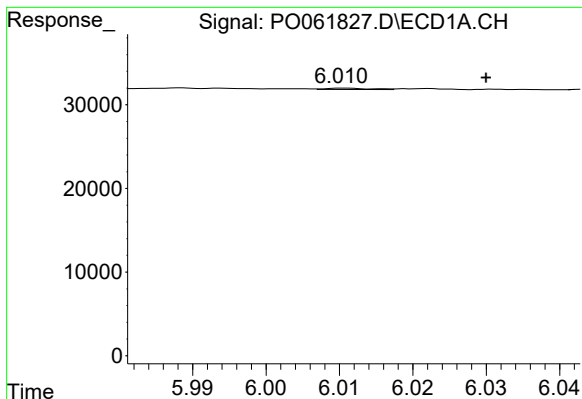

#23 AR-1248-3


R.T.: 6.011 min
Delta R.T.: -0.019 min
Response: 647
Conc: 0.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

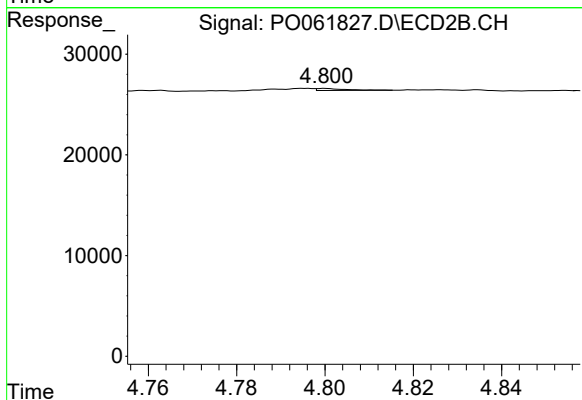


#23 AR-1248-3

R.T.: 4.800 min
Delta R.T.: -0.060 min
Response: 906
Conc: 0.73 ng/ml

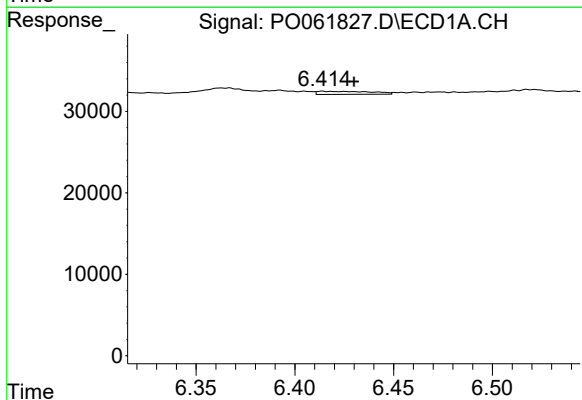


#24 AR-1248-4

R.T.: 6.414 min
Delta R.T.: -0.016 min
Response: 7083
Conc: 3.00 ng/ml

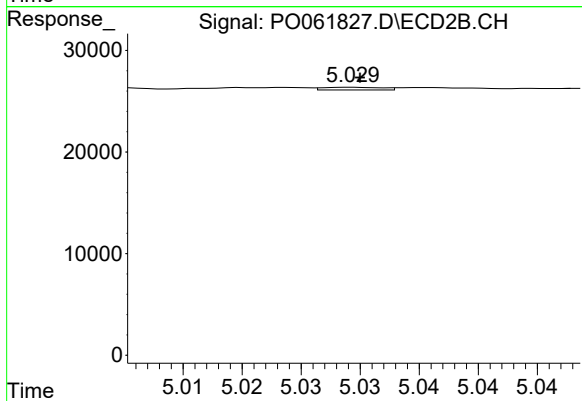

#24 AR-1248-4


R.T.: 5.029 min
Delta R.T.: 0.000 min
Response: 940
Conc: 0.63 ng/ml

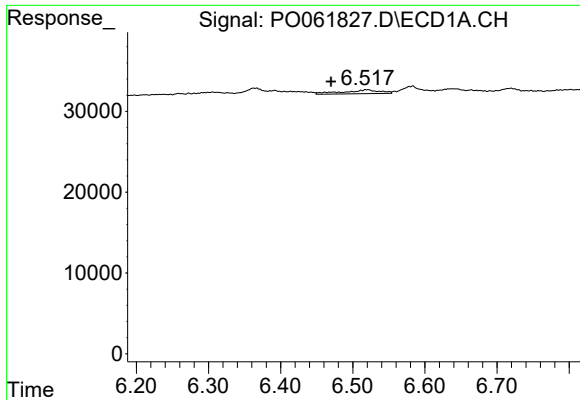

#25 AR-1248-5


R.T.: 6.518 min
Delta R.T.: 0.048 min
Response: 16511
Conc: 7.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

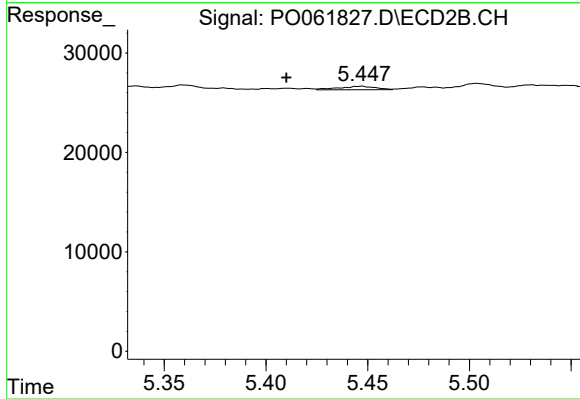


#25 AR-1248-5

R.T.: 5.447 min
Delta R.T.: 0.037 min
Response: 4340
Conc: 2.83 ng/ml

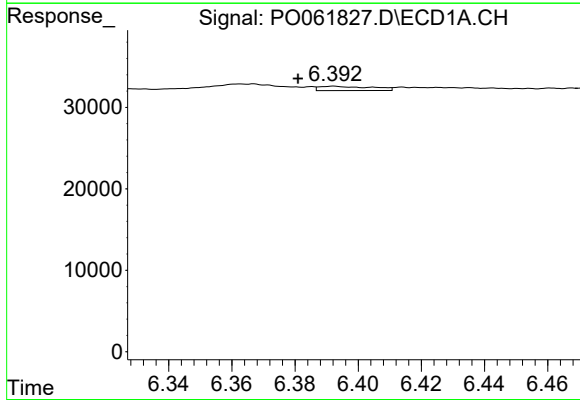


#26 AR-1254-1

R.T.: 6.392 min
Delta R.T.: 0.011 min
Response: 6193
Conc: 2.71 ng/ml

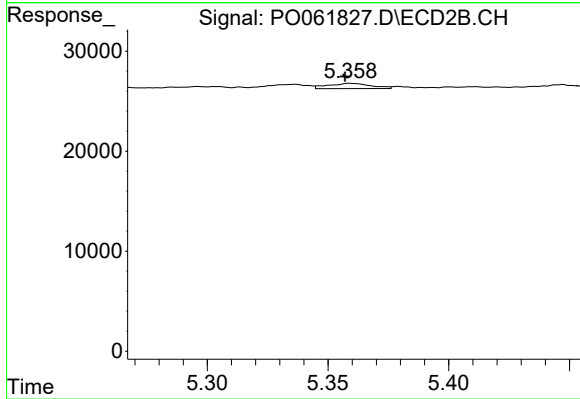

#26 AR-1254-1


R.T.: 5.359 min
Delta R.T.: 0.002 min
Response: 6472
Conc: 2.95 ng/ml

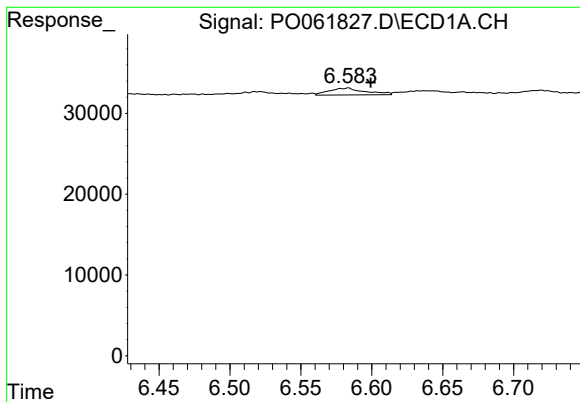

#27 AR-1254-2


R.T.: 6.583 min
Delta R.T.: -0.016 min
Response: 15462
Conc: 4.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

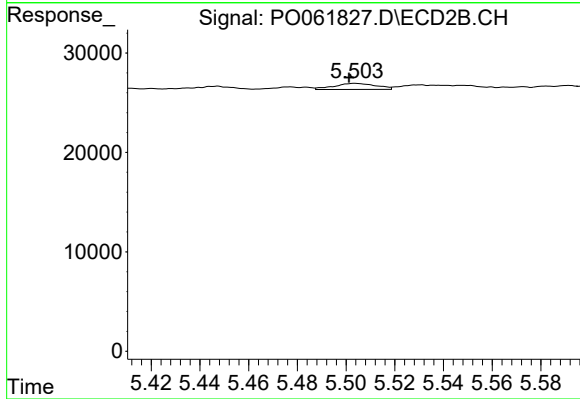


#27 AR-1254-2

R.T.: 5.504 min
Delta R.T.: 0.003 min
Response: 7326
Conc: 3.74 ng/ml

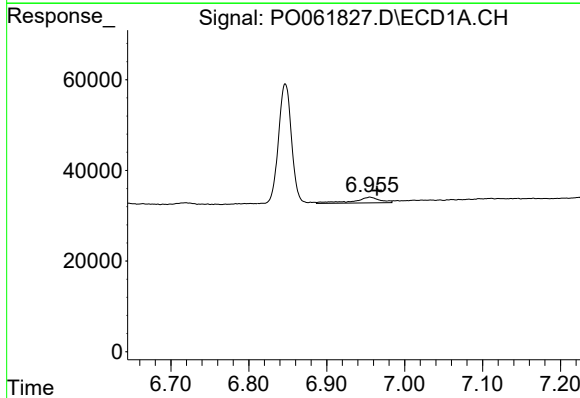


#28 AR-1254-3

R.T.: 6.956 min
Delta R.T.: -0.009 min
Response: 29518
Conc: 7.55 ng/ml

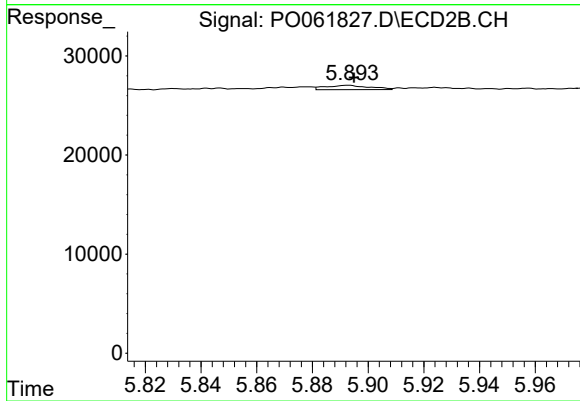

#28 AR-1254-3


R.T.: 5.893 min
Delta R.T.: -0.002 min
Response: 4775
Conc: 1.50 ng/ml

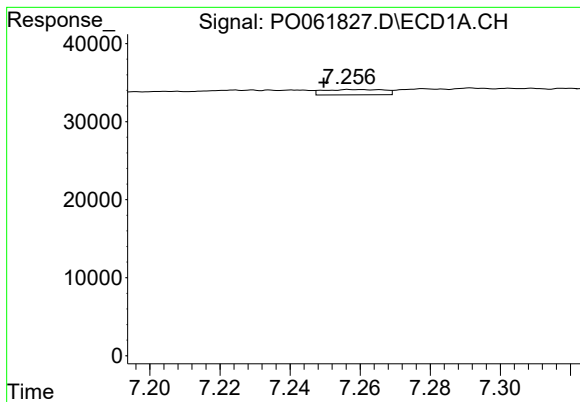

#29 AR-1254-4


R.T.: 7.258 min
Delta R.T.: 0.008 min
Response: 8108
Conc: 2.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

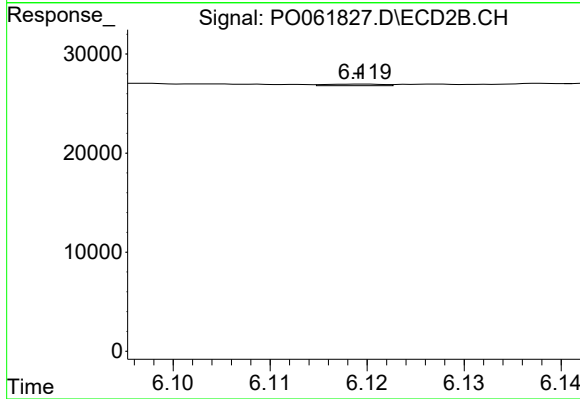


#29 AR-1254-4

R.T.: 6.120 min
Delta R.T.: 0.000 min
Response: 674
Conc: 0.33 ng/ml

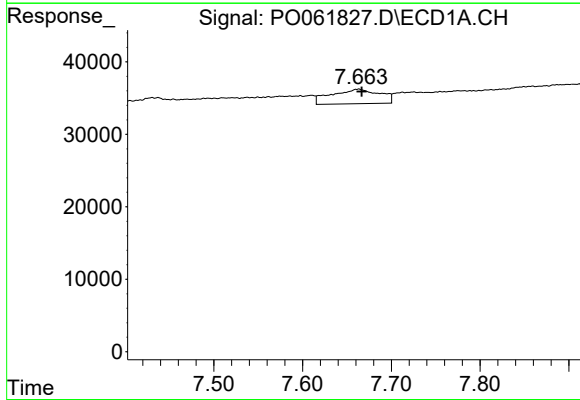


#30 AR-1254-5

R.T.: 7.663 min
Delta R.T.: -0.004 min
Response: 76038
Conc: 24.21 ng/ml

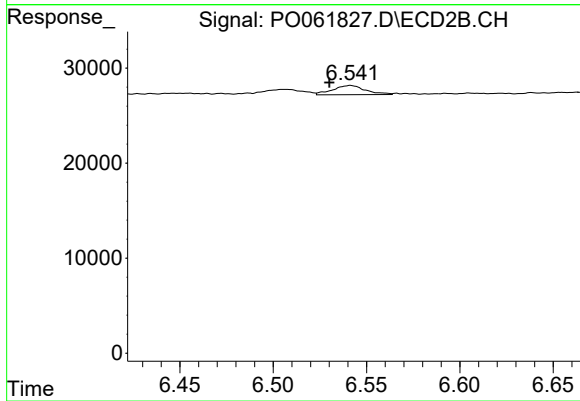

#30 AR-1254-5


R.T.: 6.541 min
Delta R.T.: 0.011 min
Response: 11962
Conc: 4.23 ng/ml

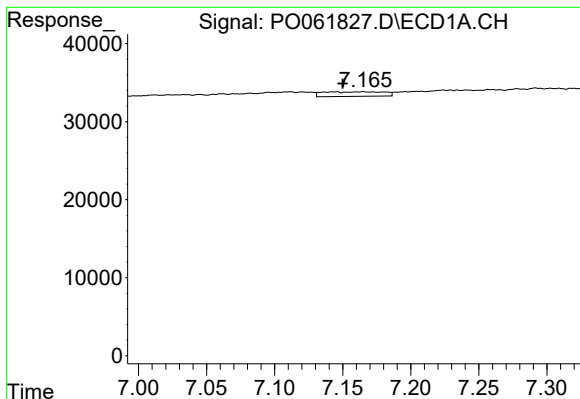

#31 AR-1260-1


R.T.: 7.165 min
Delta R.T.: 0.015 min
Response: 18134
Conc: 6.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

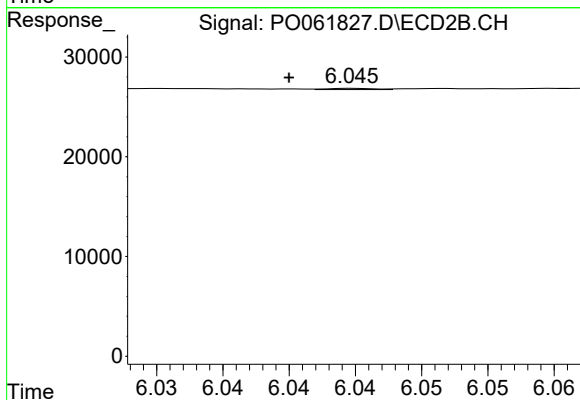


#31 AR-1260-1

R.T.: 6.045 min
Delta R.T.: 0.005 min
Response: 303
Conc: 0.15 ng/ml

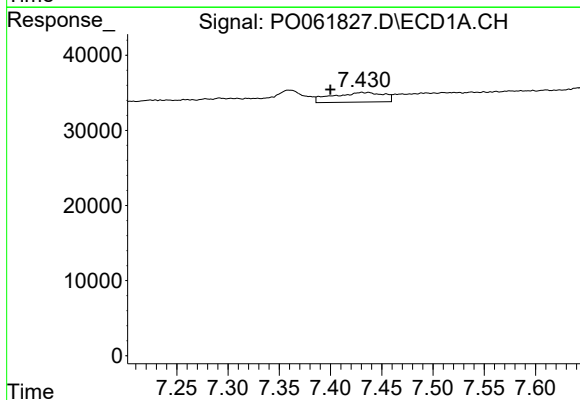


#32 AR-1260-2

R.T.: 7.430 min
Delta R.T.: 0.030 min
Response: 44483
Conc: 13.95 ng/ml

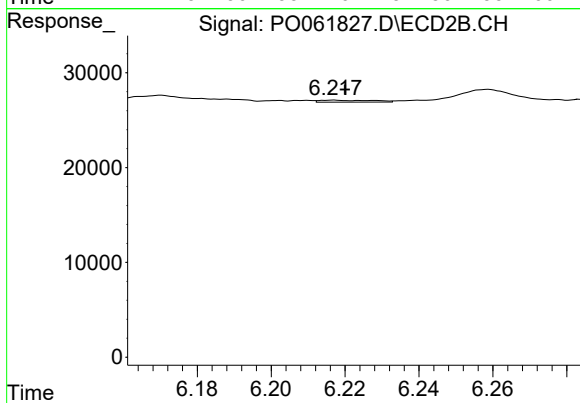

#32 AR-1260-2


R.T.: 6.217 min
Delta R.T.: -0.003 min
Response: 2069
Conc: 0.86 ng/ml

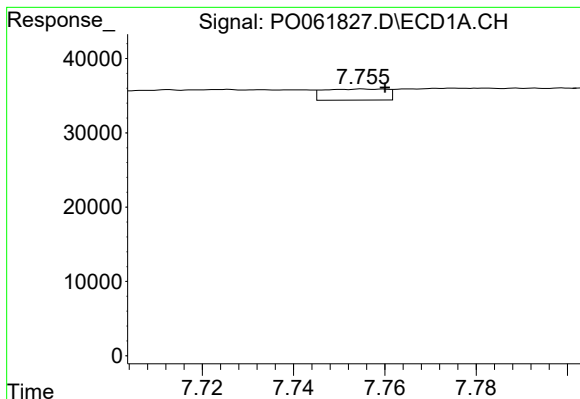

#33 AR-1260-3


R.T.: 7.756 min
Delta R.T.: -0.004 min
Response: 14290
Conc: 5.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

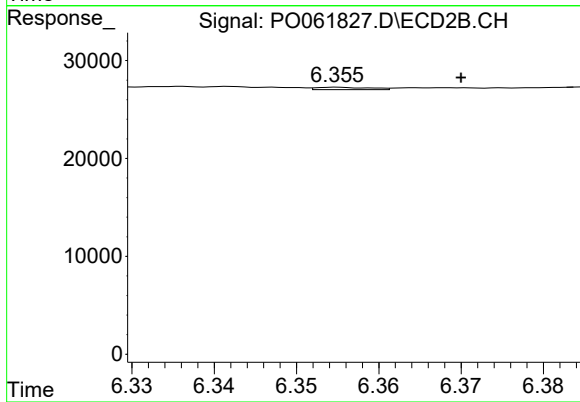


#33 AR-1260-3

R.T.: 6.355 min
Delta R.T.: -0.015 min
Response: 1074
Conc: 0.48 ng/ml

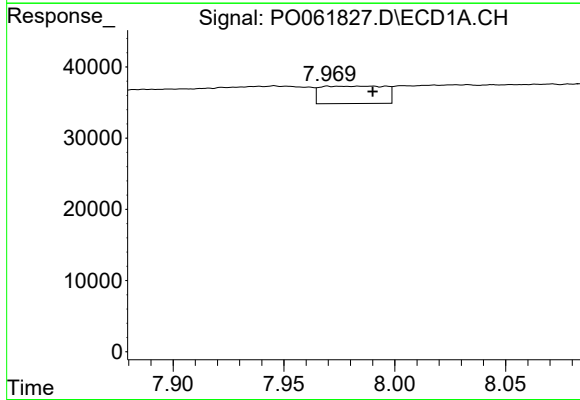


#34 AR-1260-4

R.T.: 7.990 min
Delta R.T.: 0.000 min
Response: 49065
Conc: 18.36 ng/ml

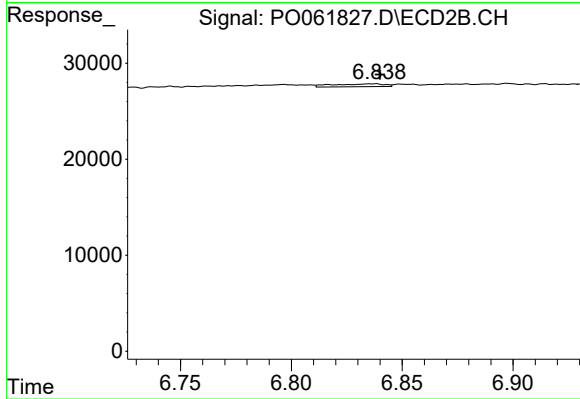

#34 AR-1260-4


R.T.: 6.838 min
Delta R.T.: -0.002 min
Response: 4767
Conc: 2.58 ng/ml

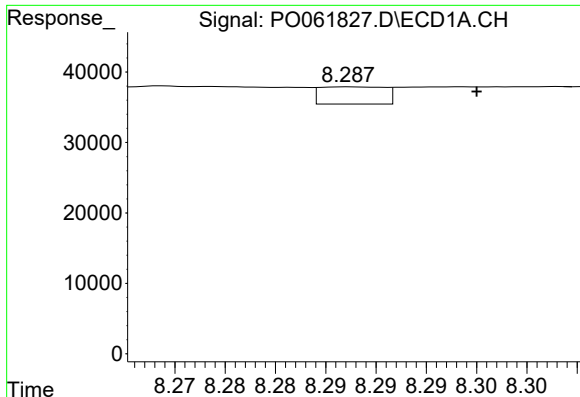

#35 AR-1260-5


R.T.: 8.288 min
Delta R.T.: -0.012 min
Response: 10948
Conc: 2.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

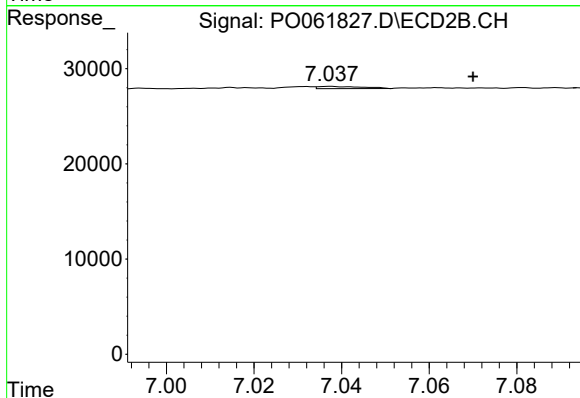


#35 AR-1260-5

R.T.: 7.037 min
Delta R.T.: -0.033 min
Response: 1697
Conc: 0.44 ng/ml

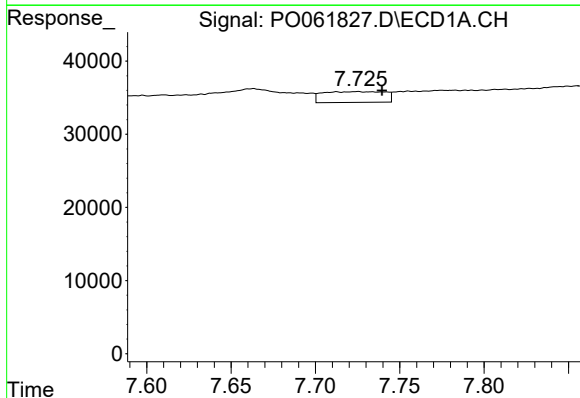


#36 AR-1262-1

R.T.: 7.725 min
Delta R.T.: -0.014 min
Response: 37967
Conc: 9.91 ng/ml

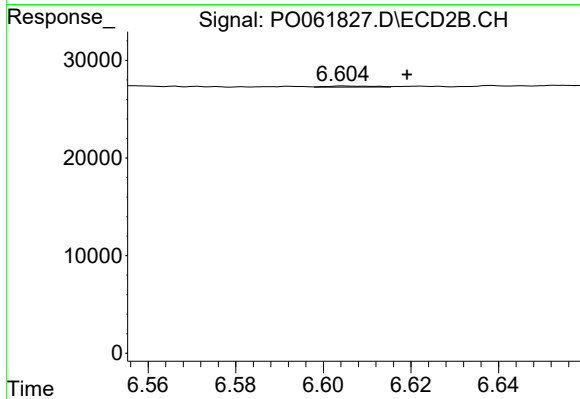

#36 AR-1262-1


R.T.: 6.605 min
Delta R.T.: -0.015 min
Response: 843
Conc: 0.69 ng/ml

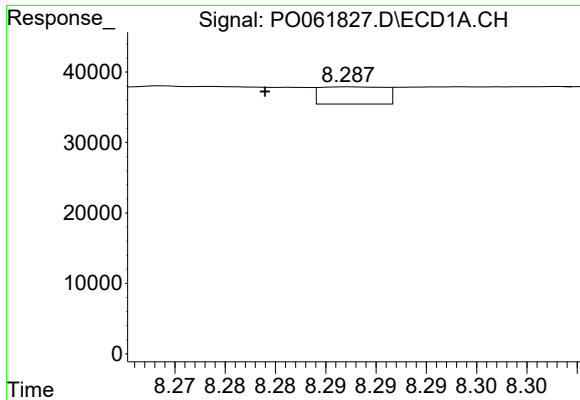

#37 AR-1262-2


R.T.: 8.288 min
Delta R.T.: 0.009 min
Response: 10948
Conc: 1.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

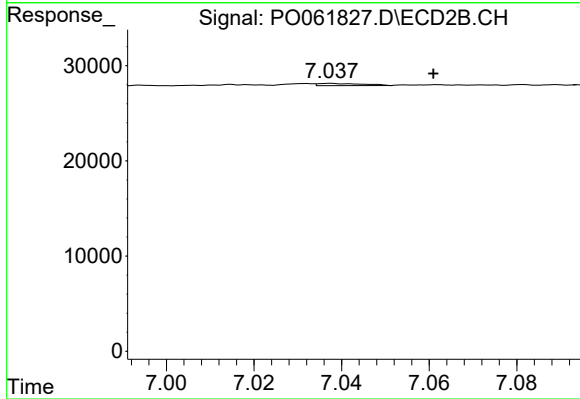


#37 AR-1262-2

R.T.: 7.037 min
Delta R.T.: -0.024 min
Response: 1697
Conc: 0.37 ng/ml

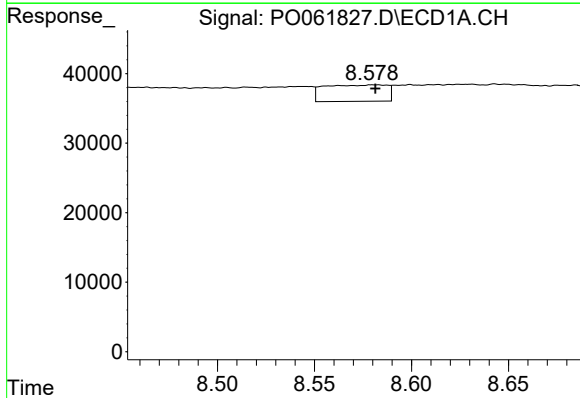


#38 AR-1262-3

R.T.: 8.581 min
Delta R.T.: 0.000 min
Response: 53121
Conc: 12.78 ng/ml

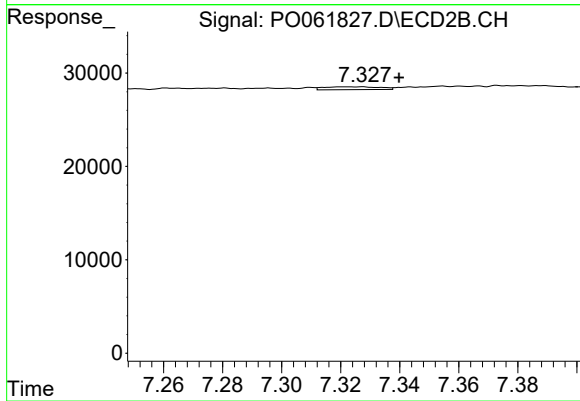

#38 AR-1262-3


R.T.: 7.328 min
Delta R.T.: -0.012 min
Response: 4150
Conc: 2.20 ng/ml

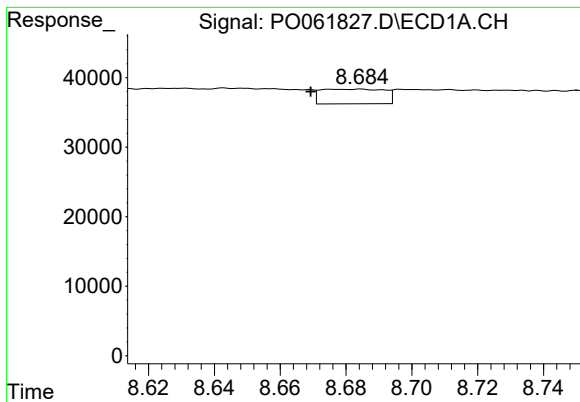

#39 AR-1262-4


R.T.: 8.676 min
Delta R.T.: 0.007 min
Response: 28359
Conc: 8.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

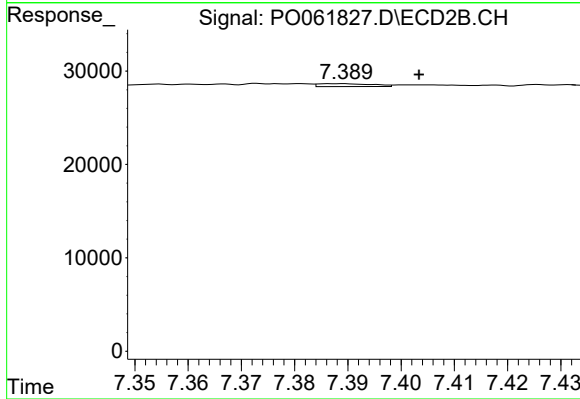


#39 AR-1262-4

R.T.: 7.389 min
Delta R.T.: -0.014 min
Response: 2211
Conc: 0.66 ng/ml

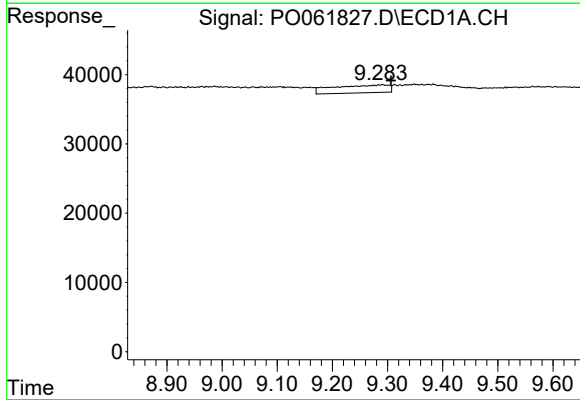


#40 AR-1262-5

R.T.: 9.290 min
Delta R.T.: -0.017 min
Response: 79454
Conc: 39.07 ng/ml

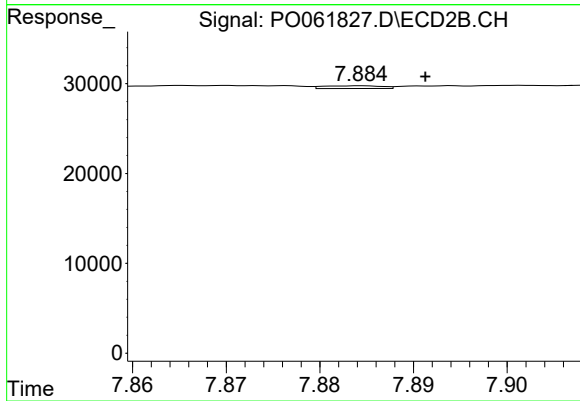

#40 AR-1262-5


R.T.: 7.885 min
Delta R.T.: -0.007 min
Response: 1300
Conc: 0.86 ng/ml

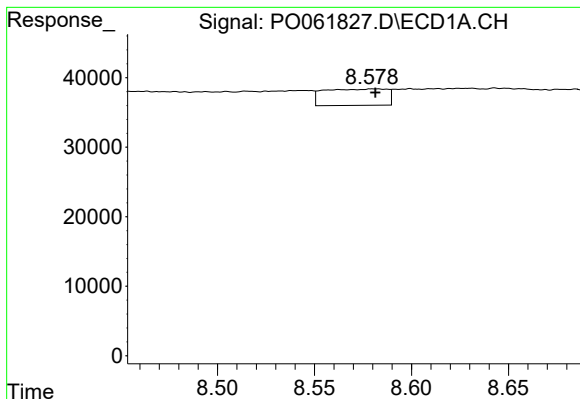

#41 AR-1268-1


R.T.: 8.581 min
Delta R.T.: 0.000 min
Response: 53121
Conc: 7.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

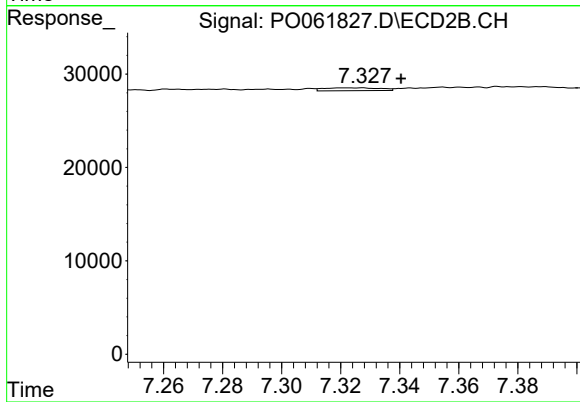


#41 AR-1268-1

R.T.: 7.328 min
Delta R.T.: -0.013 min
Response: 4150
Conc: 0.86 ng/ml

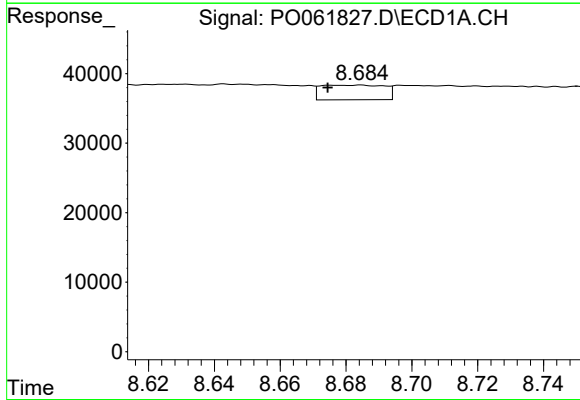


#42 AR-1268-2

R.T.: 8.676 min
Delta R.T.: 0.002 min
Response: 28359
Conc: 4.58 ng/ml

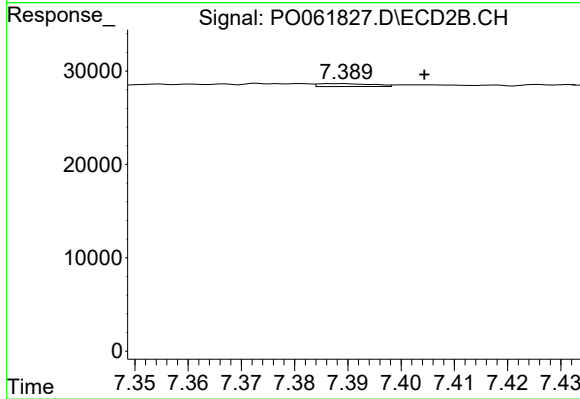

#42 AR-1268-2


R.T.: 7.389 min
Delta R.T.: -0.015 min
Response: 2211
Conc: 0.51 ng/ml

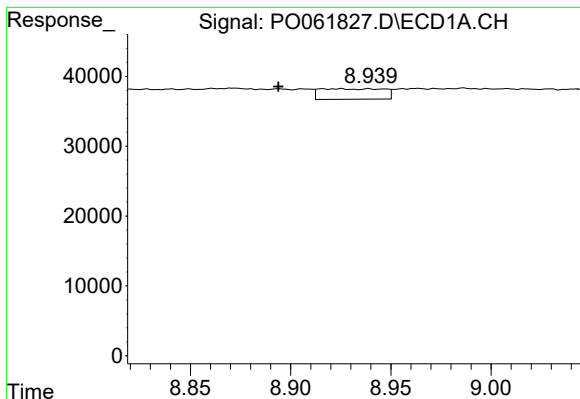

#43 AR-1268-3


R.T.: 8.916 min
Delta R.T.: 0.022 min
Response: 32886
Conc: 6.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

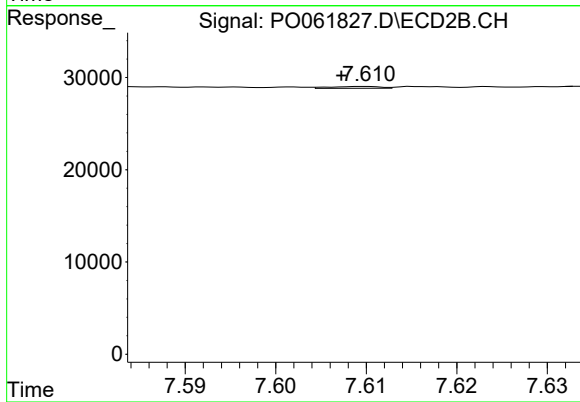


#43 AR-1268-3

R.T.: 7.610 min
Delta R.T.: 0.003 min
Response: 791
Conc: 0.22 ng/ml

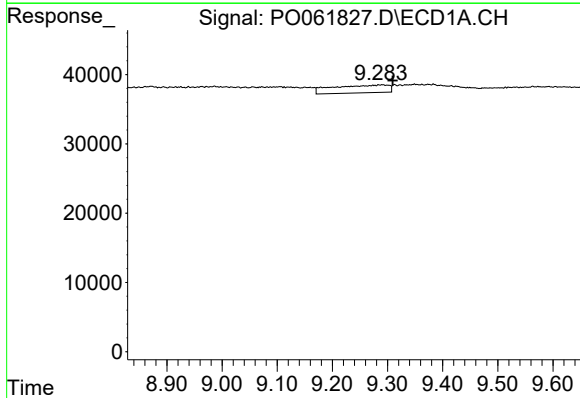


#44 AR-1268-4

R.T.: 9.290 min
Delta R.T.: -0.020 min
Response: 79454
Conc: 36.34 ng/ml

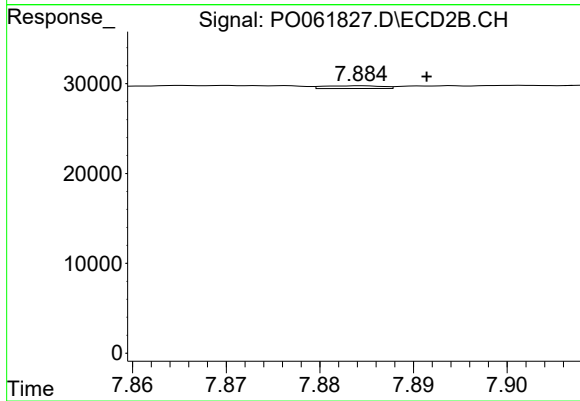

#44 AR-1268-4


R.T.: 7.885 min
Delta R.T.: -0.007 min
Response: 1300
Conc: 0.81 ng/ml

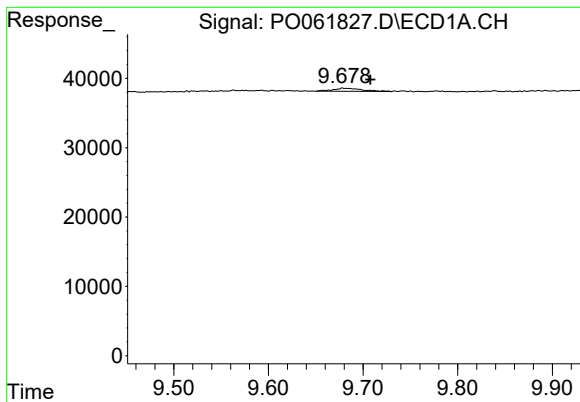

#45 AR-1268-5

R.T.: 9.681 min
Delta R.T.: -0.027 min
Response: 9782
Conc: 0.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

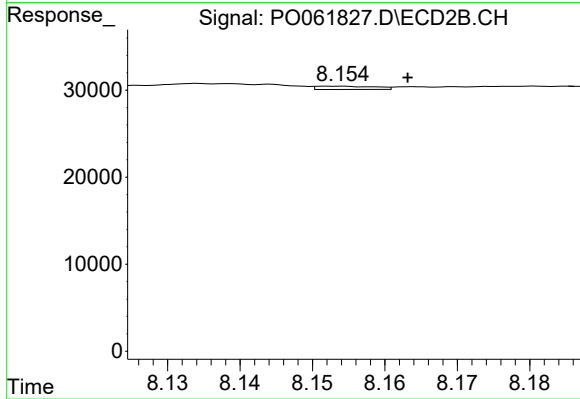

#45 AR-1268-5

R.T.: 8.154 min
Delta R.T.: -0.009 min
Response: 2122
Conc: 0.21 ng/ml