

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100919\
 Data File : PO061833.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Oct 2019 16:58
 Operator : HP/AJ
 Sample : K5281-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-062

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 01:12:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.352	3.513	766889	541989	18.698	16.759
2)	SA Decachlor...	10.009	8.425	668522	2436	14.355	0.075 #
Target Compounds							
3)	L1 AR-1016-1	5.571	4.583	1990	8316	1.085	6.185 #
4)	L1 AR-1016-2	5.571	4.629	1990	4929	0.770	2.659 #
5)	L1 AR-1016-3	5.673	4.782	31235	1616	19.444	1.614 #
6)	L1 AR-1016-4	5.735	4.814	3013	1133	2.253	1.307 #
7)	L1 AR-1016-5	5.995	5.010	27725	4318	20.217	3.783 #
8)	L2 AR-1221-1	4.587	3.729	1695	1392	3.668	3.516
9)	L2 AR-1221-2	4.655	3.818	15818	4480	44.058	14.528 #
10)	L2 AR-1221-3	4.738	3.874	93935	63992	82.506	70.156
11)	L3 AR-1232-1	4.738	3.874	93935	63992	67.173	56.994
12)	L3 AR-1232-2	5.256	4.583	1351	8316	1.722	6.813 #
13)	L3 AR-1232-3	5.571	4.752	1990	11926	1.164	18.063 #
14)	L3 AR-1232-4	5.720	4.854	475	13759	0.537	21.827 #
15)	L3 AR-1232-5	5.790	5.010	11009	4318	15.879	6.293 #
16)	L4 AR-1242-1	5.513	4.566	4231	4466	2.980	4.359 #
17)	L4 AR-1242-2	5.571	4.583	1990	8316	0.990	5.897 #
18)	L4 AR-1242-3	5.585	4.752	1568	11926	1.243	15.273 #
19)	L4 AR-1242-4	5.720	4.837	475	1767	0.452	2.153 #
20)	L4 AR-1242-5	6.454	5.345	6651	64815	4.973	60.504 #
21)	L5 AR-1248-1	5.571	4.583	1990	8316	1.694	9.294 #
22)	L5 AR-1248-2	5.822	4.814	5884	1133	3.487	0.961 #
23)	L5 AR-1248-3	5.995	4.854	27725	13759	14.836	11.084 #
24)	L5 AR-1248-4	6.454	5.010	6651	4318	2.815	2.872
25)	L5 AR-1248-5	6.481	5.410	6756	13969	2.980	9.105 #
26)	L6 AR-1254-1	6.381	5.345	39403	64815	17.272	29.551 #
27)	L6 AR-1254-2	6.593	5.504	46828	11595	12.961	5.914 #
28)	L6 AR-1254-3	6.960	5.890	35797	9192	9.161	2.887 #
29)	L6 AR-1254-4	7.237	6.108	13547	5787	4.473	2.852 #
30)	L6 AR-1254-5	7.680	6.530	11603	652	3.695	0.231 #
31)	L7 AR-1260-1	7.166	6.039	7581	5620	2.904	2.755
32)	L7 AR-1260-2	7.417	6.222	37699	71511	11.825	29.775 #
33)	L7 AR-1260-3	7.736	6.376	11370	8260	4.734	3.666
34)	L7 AR-1260-4	7.986	6.835	17814	3656	6.667	1.980 #
35)	L7 AR-1260-5	8.308	7.075	44395	1531	8.972	0.393 #
36)	L8 AR-1262-1	7.736	6.612	11370	1098	2.967	0.900 #
37)	L8 AR-1262-2	8.264	7.075	63935	1531	10.299	0.333 #
38)	L8 AR-1262-3	8.584	7.341	78319	767	18.843	0.407 #
39)	L8 AR-1262-4	8.663	7.388	18305	4505	5.799	1.340 #
40)	L8 AR-1262-5	9.316	7.888	7172	761	3.527	0.502 #
41)	L9 AR-1268-1	8.584	7.341	78319	767	11.647	0.159 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100919\
Data File : P0061833.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Oct 2019 16:58
Operator : HP/AJ
Sample : K5281-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 01:12:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.686	7.420	13422	307	2.167	0.071 #
43)	L9 AR-1268-3	8.895	7.601	10189	2015	1.993	0.562 #
44)	L9 AR-1268-4	9.316	7.888	7172	761	3.280	0.473 #
45)	L9 AR-1268-5	9.690	8.170	6796	540	0.452	0.054 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO100919\
Data File : P0061833.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Oct 2019 16:58
Operator : HP/AJ
Sample : K5281-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
FK-PS-01-062

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 01:12:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

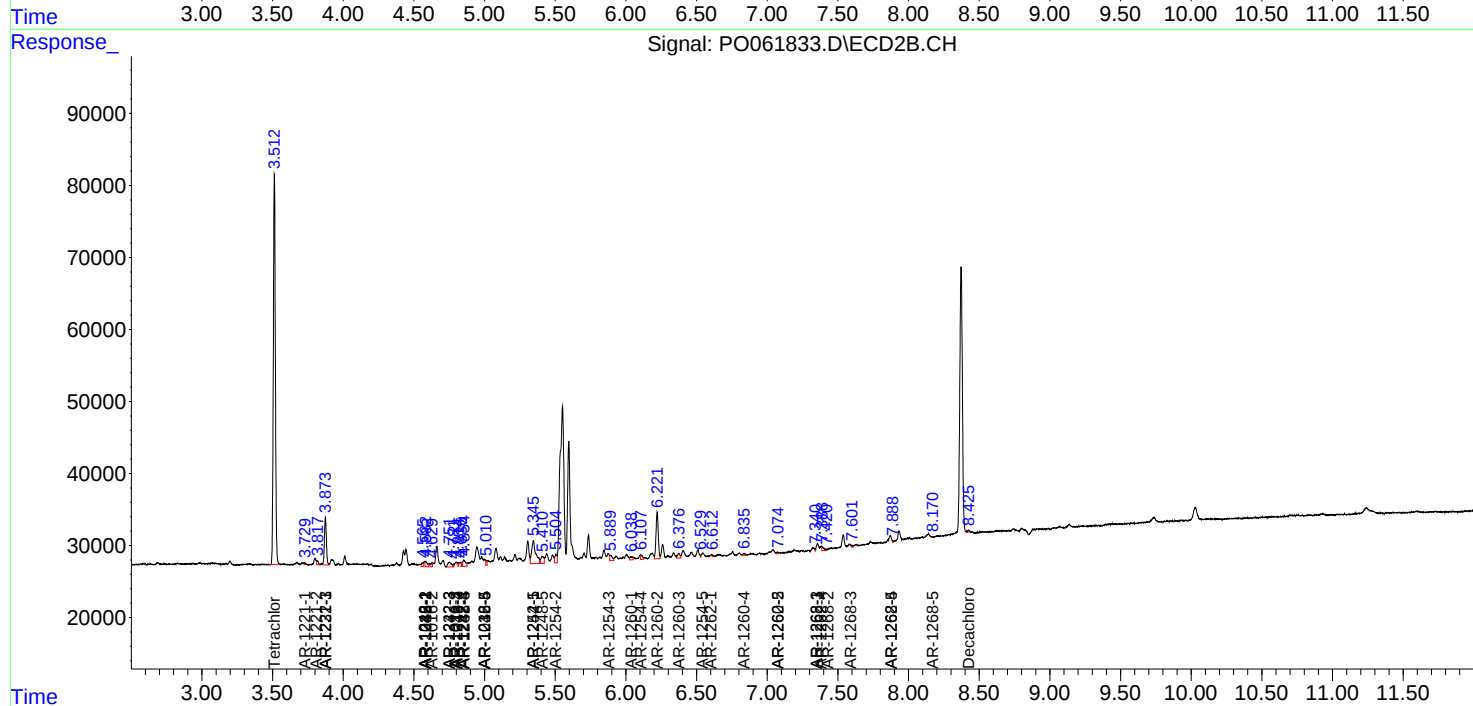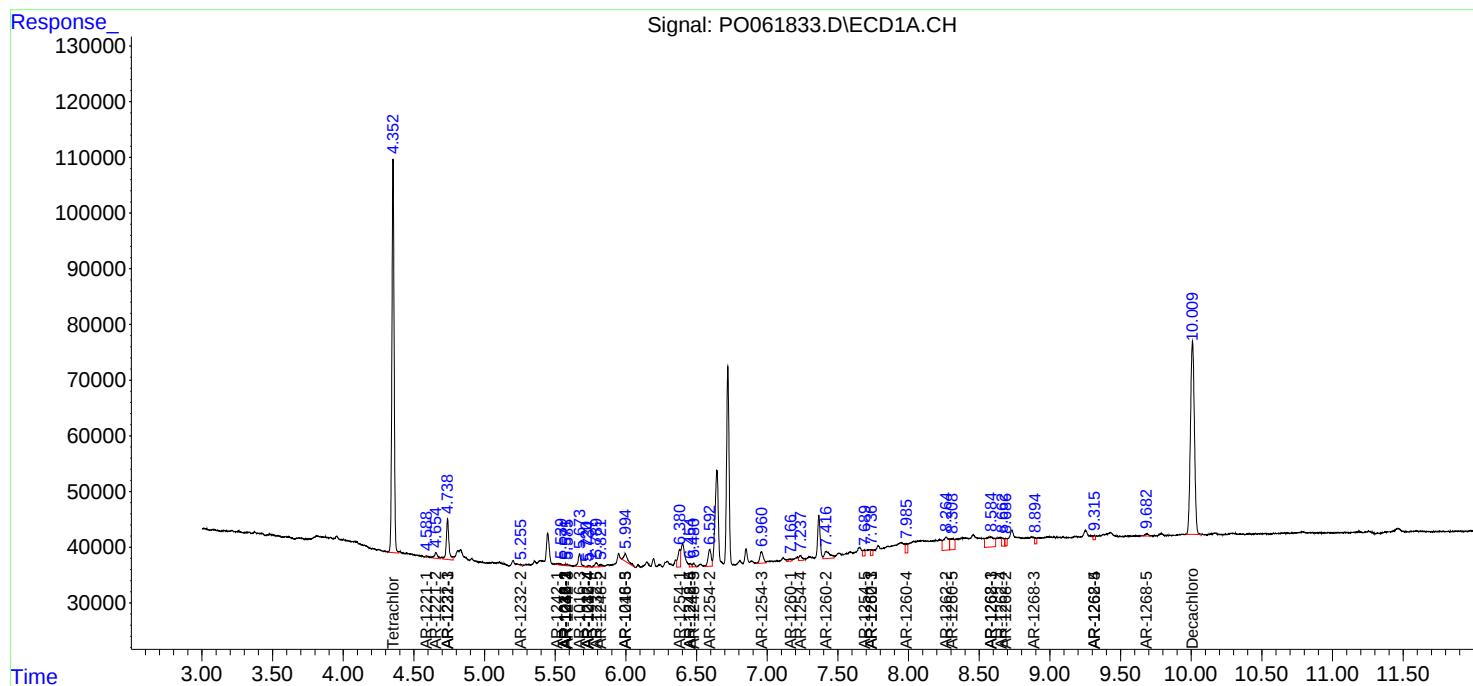


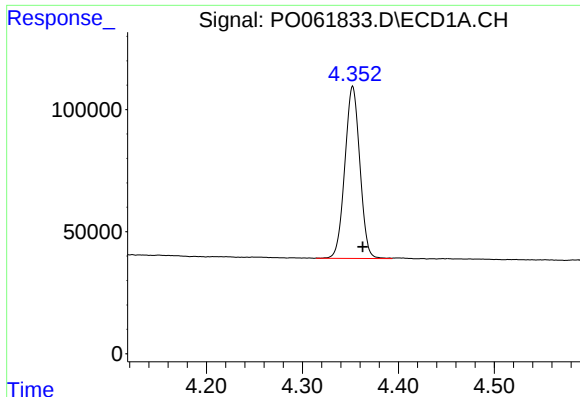

#1 Tetrachloro-m-xylene


R.T.: 4.352 min
Delta R.T.: -0.011 min
Response: 766889
Conc: 18.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

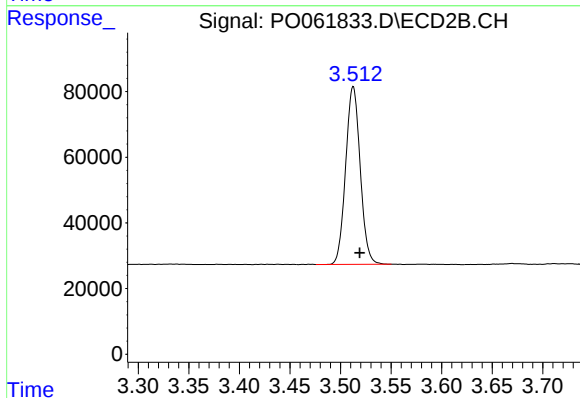


#1 Tetrachloro-m-xylene

R.T.: 3.513 min
Delta R.T.: -0.006 min
Response: 541989
Conc: 16.76 ng/ml

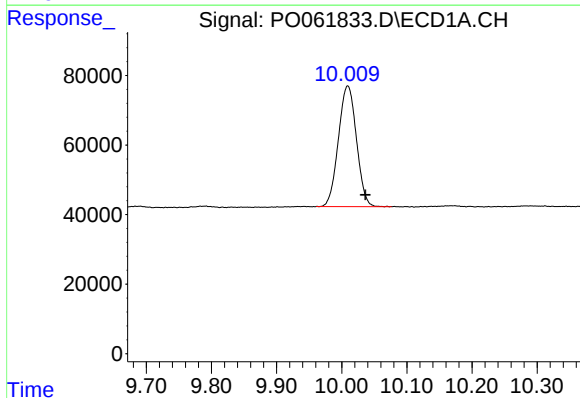


#2 Decachlorobiphenyl

R.T.: 10.009 min
Delta R.T.: -0.027 min
Response: 668522
Conc: 14.35 ng/ml

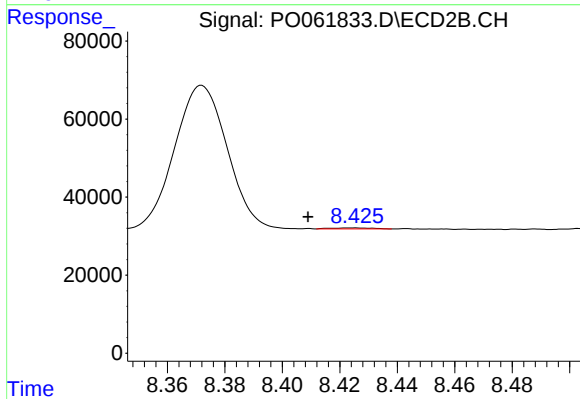

#2 Decachlorobiphenyl


R.T.: 8.425 min
Delta R.T.: 0.016 min
Response: 2436
Conc: 0.08 ng/ml

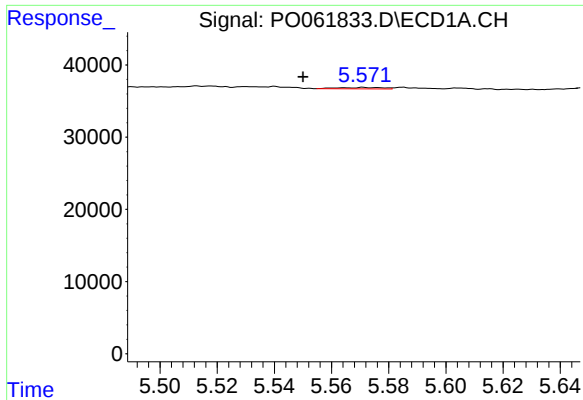

#3 AR-1016-1


R.T.: 5.571 min
Delta R.T.: 0.021 min
Response: 1990
Conc: 1.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

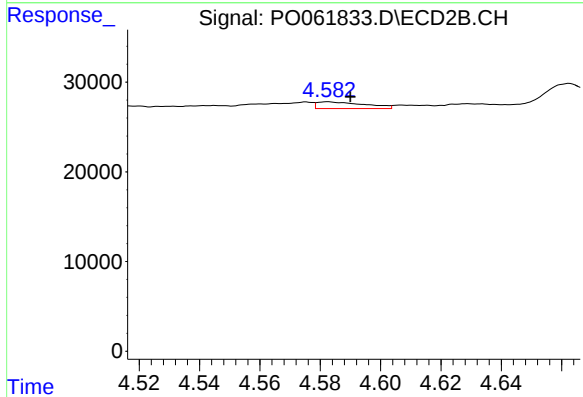


#3 AR-1016-1

R.T.: 4.583 min
Delta R.T.: -0.007 min
Response: 8316
Conc: 6.18 ng/ml

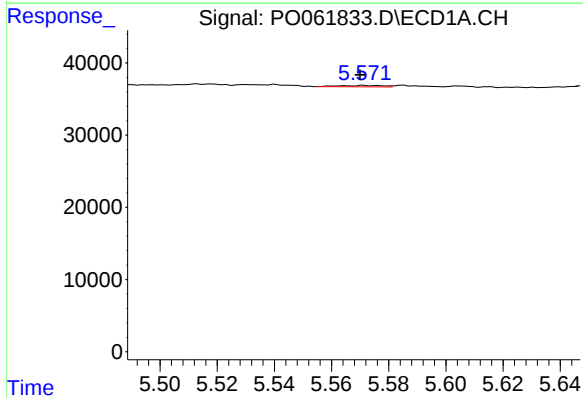


#4 AR-1016-2

R.T.: 5.571 min
Delta R.T.: 0.001 min
Response: 1990
Conc: 0.77 ng/ml

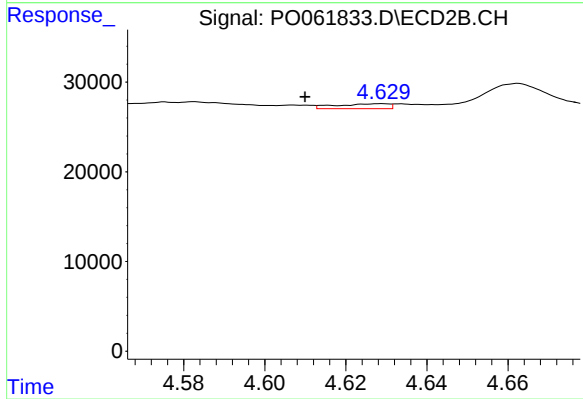

#4 AR-1016-2


R.T.: 4.629 min
Delta R.T.: 0.019 min
Response: 4929
Conc: 2.66 ng/ml

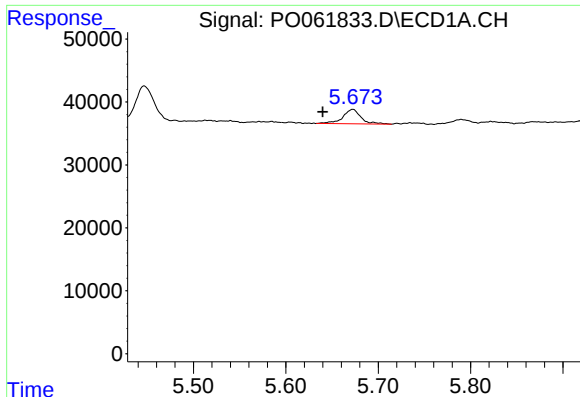

#5 AR-1016-3


R.T.: 5.673 min
Delta R.T.: 0.033 min
Response: 31235
Conc: 19.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

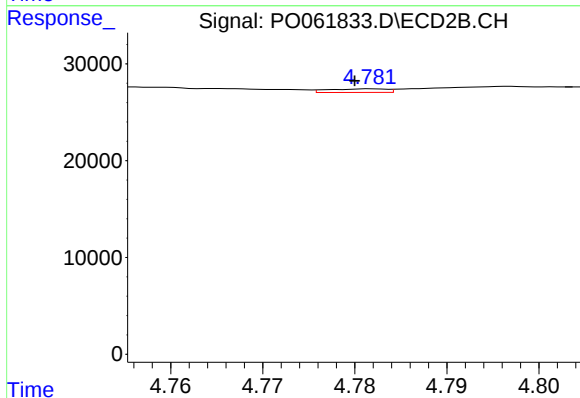


#5 AR-1016-3

R.T.: 4.782 min
Delta R.T.: 0.002 min
Response: 1616
Conc: 1.61 ng/ml

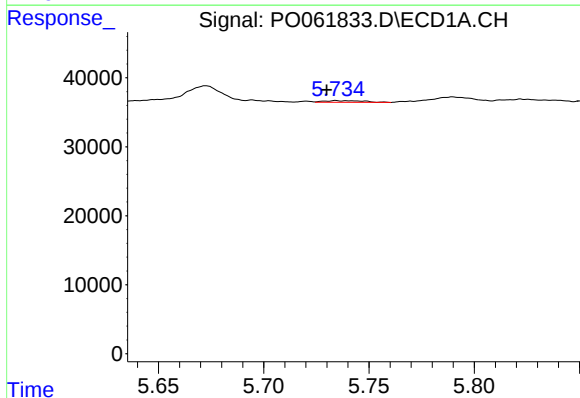


#6 AR-1016-4

R.T.: 5.735 min
Delta R.T.: 0.005 min
Response: 3013
Conc: 2.25 ng/ml

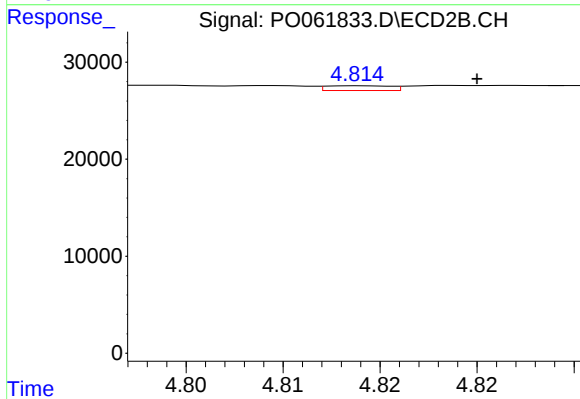

#6 AR-1016-4


R.T.: 4.814 min
Delta R.T.: -0.006 min
Response: 1133
Conc: 1.31 ng/ml

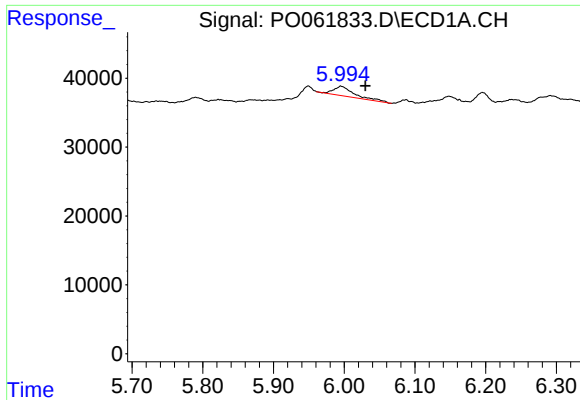

#7 AR-1016-5


R.T.: 5.995 min
Delta R.T.: -0.035 min
Response: 27725
Conc: 20.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

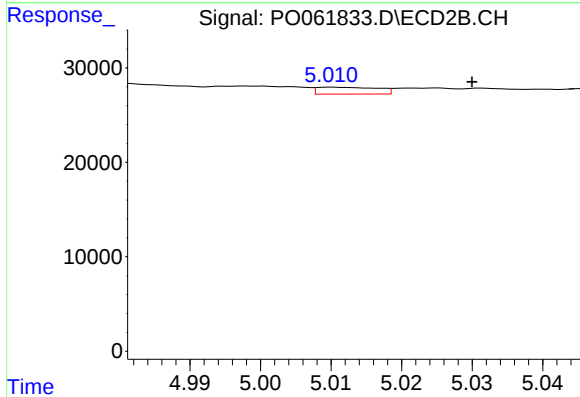


#7 AR-1016-5

R.T.: 5.010 min
Delta R.T.: -0.020 min
Response: 4318
Conc: 3.78 ng/ml

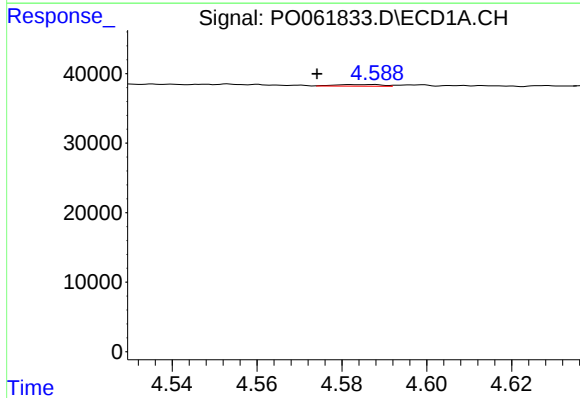


#8 AR-1221-1

R.T.: 4.587 min
Delta R.T.: 0.013 min
Response: 1695
Conc: 3.67 ng/ml

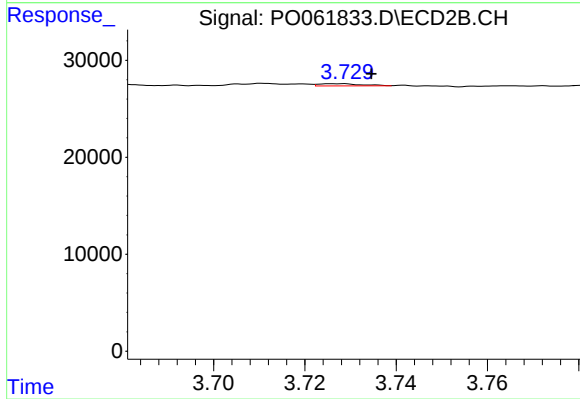

#8 AR-1221-1


R.T.: 3.729 min
Delta R.T.: -0.006 min
Response: 1392
Conc: 3.52 ng/ml

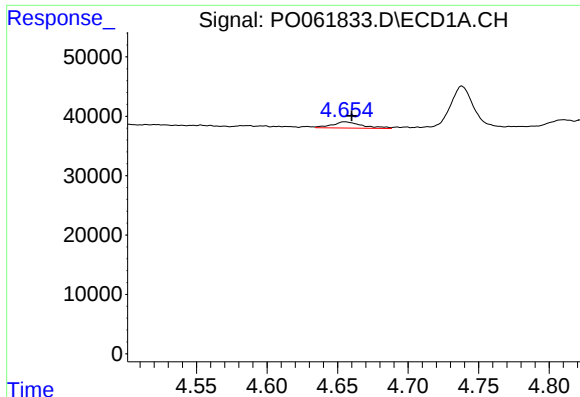

#9 AR-1221-2


R.T.: 4.655 min
Delta R.T.: -0.005 min
Response: 15818
Conc: 44.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

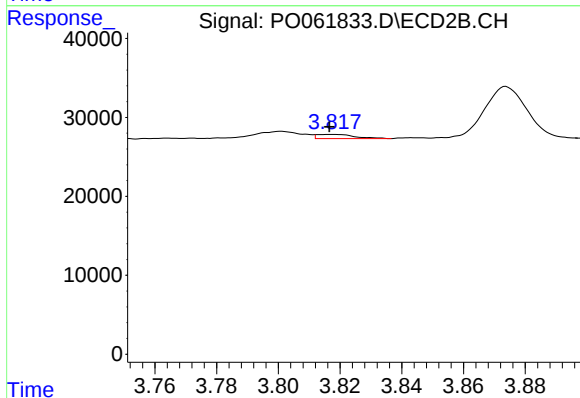


#9 AR-1221-2

R.T.: 3.818 min
Delta R.T.: 0.001 min
Response: 4480
Conc: 14.53 ng/ml

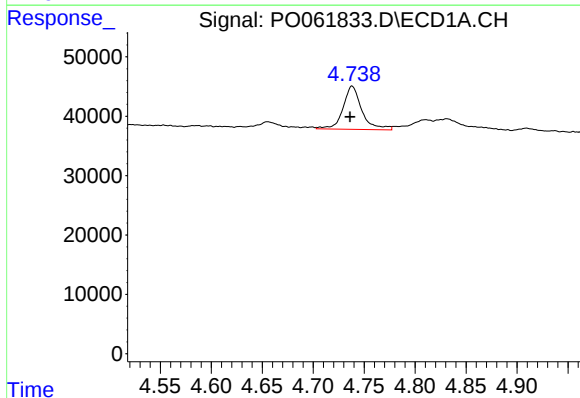


#10 AR-1221-3

R.T.: 4.738 min
Delta R.T.: 0.002 min
Response: 93935
Conc: 82.51 ng/ml

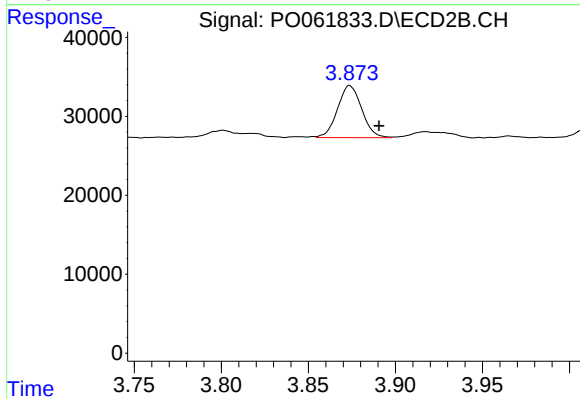

#10 AR-1221-3


R.T.: 3.874 min
Delta R.T.: -0.017 min
Response: 63992
Conc: 70.16 ng/ml

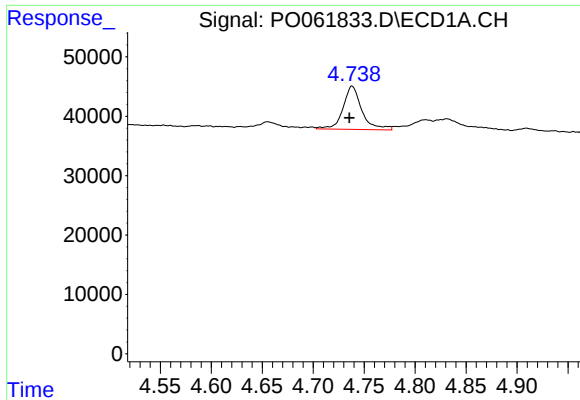

#11 AR-1232-1


R.T.: 4.738 min
Delta R.T.: 0.003 min
Response: 93935
Conc: 67.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

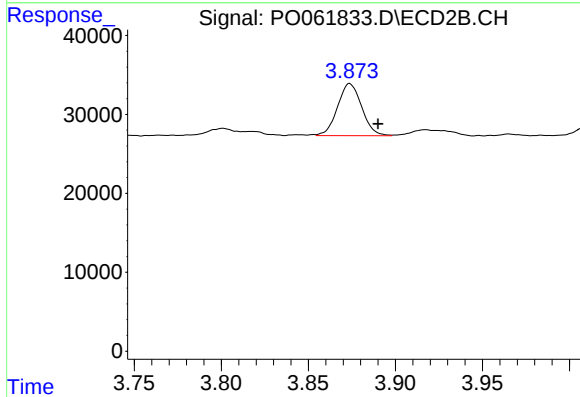


#11 AR-1232-1

R.T.: 3.874 min
Delta R.T.: -0.016 min
Response: 63992
Conc: 56.99 ng/ml

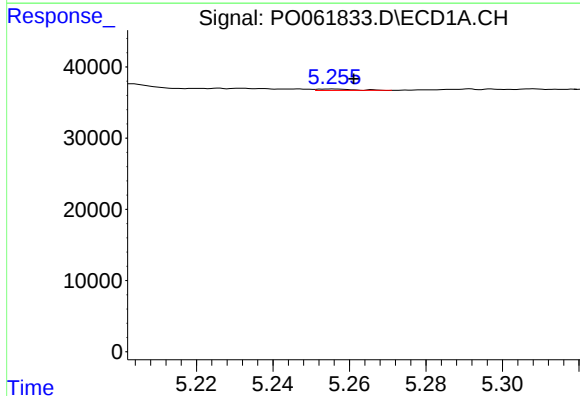


#12 AR-1232-2

R.T.: 5.256 min
Delta R.T.: -0.005 min
Response: 1351
Conc: 1.72 ng/ml

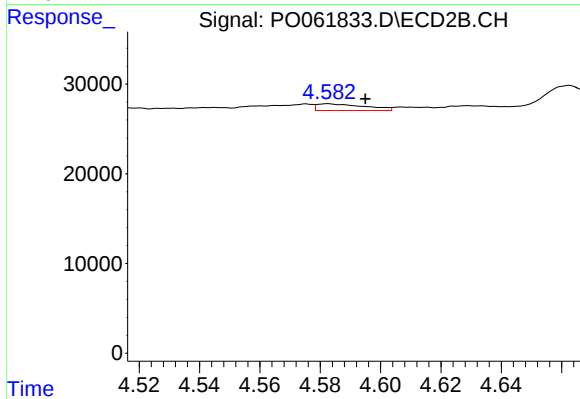

#12 AR-1232-2


R.T.: 4.583 min
Delta R.T.: -0.012 min
Response: 8316
Conc: 6.81 ng/ml

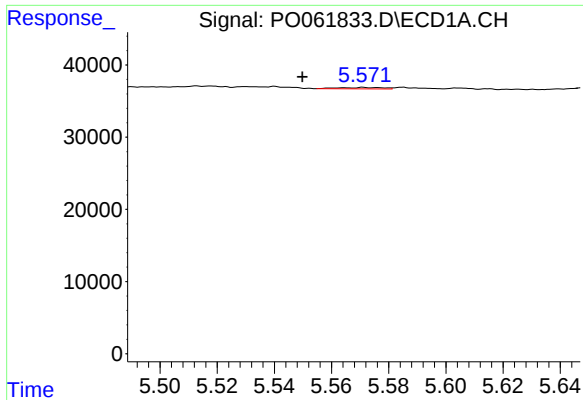

#13 AR-1232-3


R.T.: 5.571 min
Delta R.T.: 0.022 min
Response: 1990
Conc: 1.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

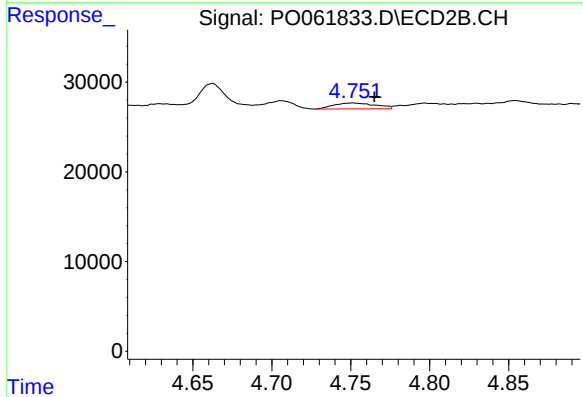


#13 AR-1232-3

R.T.: 4.752 min
Delta R.T.: -0.013 min
Response: 11926
Conc: 18.06 ng/ml

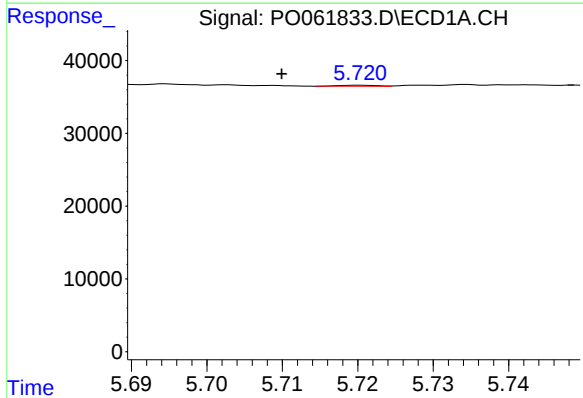


#14 AR-1232-4

R.T.: 5.720 min
Delta R.T.: 0.010 min
Response: 475
Conc: 0.54 ng/ml

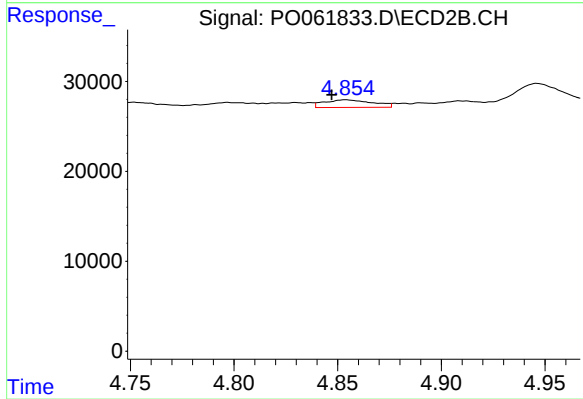

#14 AR-1232-4


R.T.: 4.854 min
Delta R.T.: 0.007 min
Response: 13759
Conc: 21.83 ng/ml

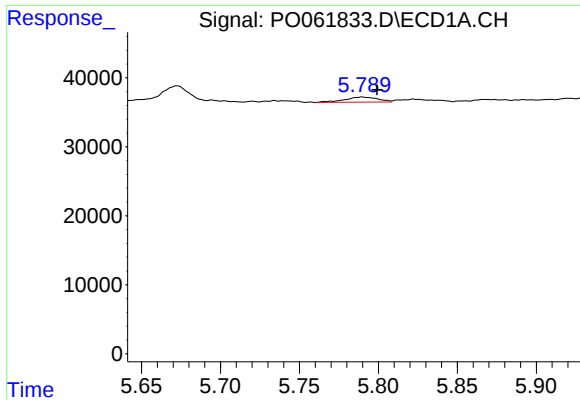

#15 AR-1232-5


R.T.: 5.790 min
Delta R.T.: -0.009 min
Response: 11009
Conc: 15.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

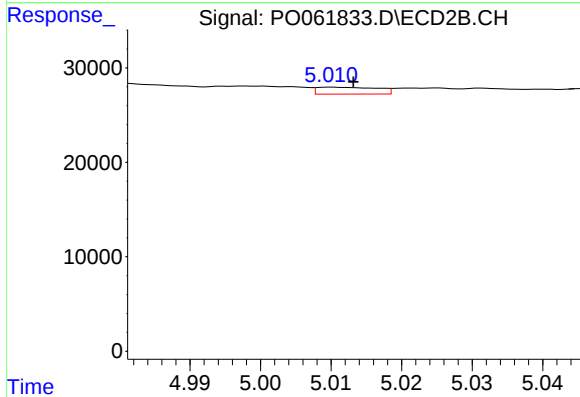


#15 AR-1232-5

R.T.: 5.010 min
Delta R.T.: -0.003 min
Response: 4318
Conc: 6.29 ng/ml

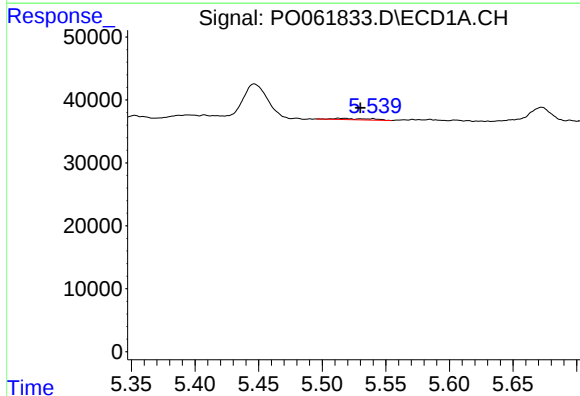


#16 AR-1242-1

R.T.: 5.513 min
Delta R.T.: -0.017 min
Response: 4231
Conc: 2.98 ng/ml

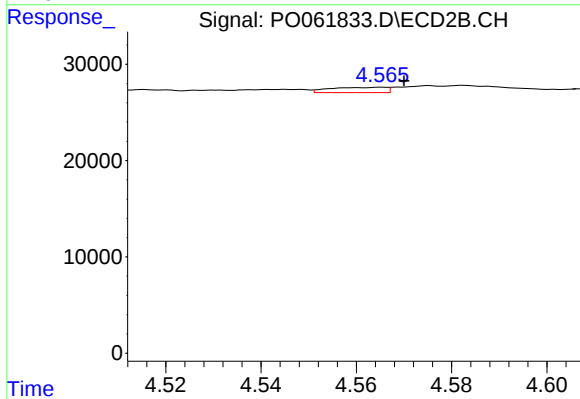

#16 AR-1242-1


R.T.: 4.566 min
Delta R.T.: -0.005 min
Response: 4466
Conc: 4.36 ng/ml

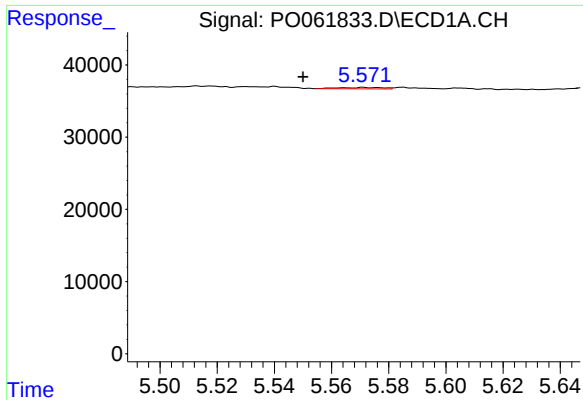

#17 AR-1242-2


R.T.: 5.571 min
Delta R.T.: 0.021 min
Response: 1990
Conc: 0.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

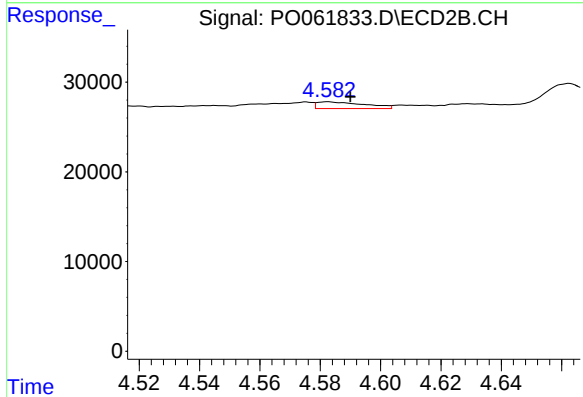


#17 AR-1242-2

R.T.: 4.583 min
Delta R.T.: -0.007 min
Response: 8316
Conc: 5.90 ng/ml

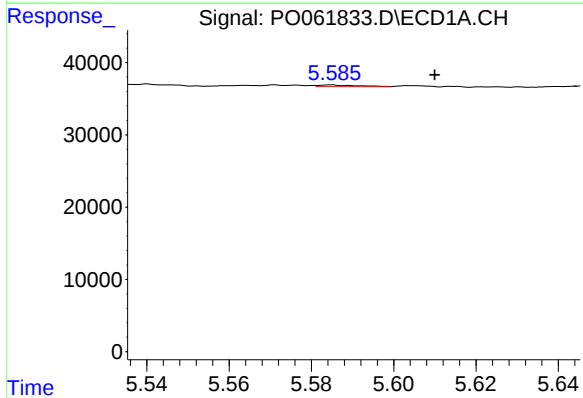


#18 AR-1242-3

R.T.: 5.585 min
Delta R.T.: -0.025 min
Response: 1568
Conc: 1.24 ng/ml

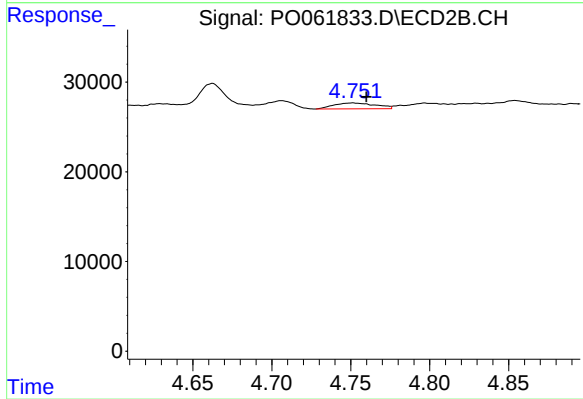

#18 AR-1242-3


R.T.: 4.752 min
Delta R.T.: -0.008 min
Response: 11926
Conc: 15.27 ng/ml

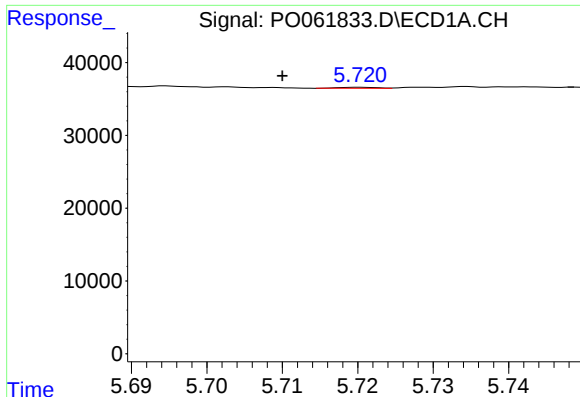

#19 AR-1242-4


R.T.: 5.720 min
Delta R.T.: 0.010 min
Response: 475
Conc: 0.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

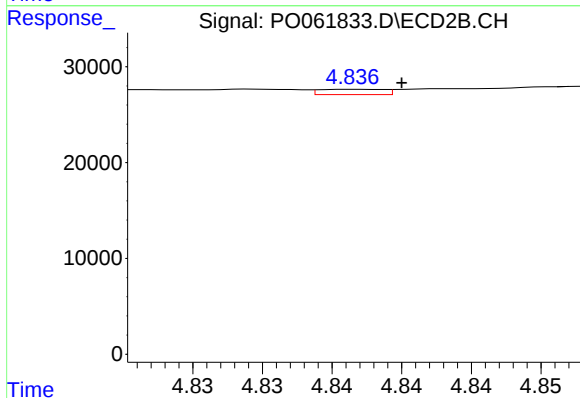


#19 AR-1242-4

R.T.: 4.837 min
Delta R.T.: -0.003 min
Response: 1767
Conc: 2.15 ng/ml

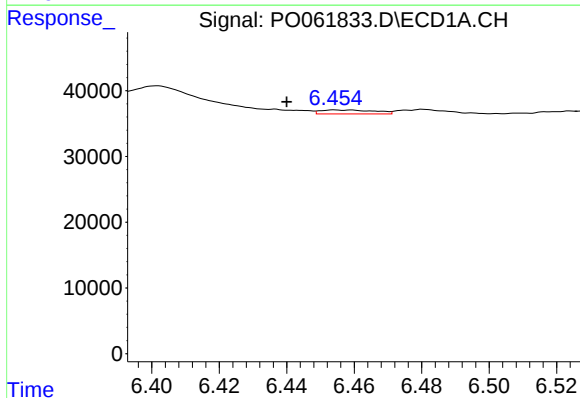


#20 AR-1242-5

R.T.: 6.454 min
Delta R.T.: 0.014 min
Response: 6651
Conc: 4.97 ng/ml

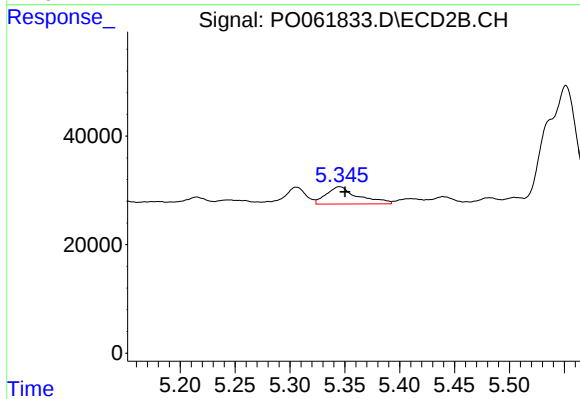

#20 AR-1242-5


R.T.: 5.345 min
Delta R.T.: -0.005 min
Response: 64815
Conc: 60.50 ng/ml

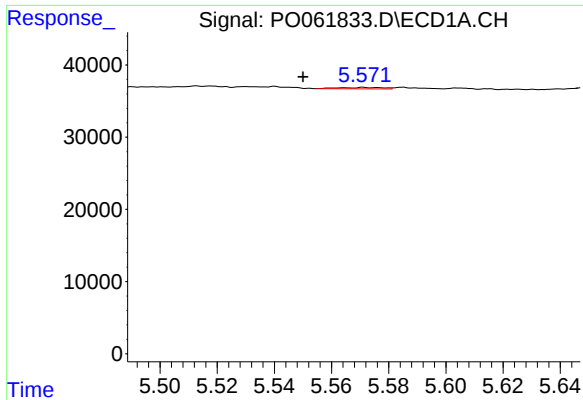

#21 AR-1248-1


R.T.: 5.571 min
Delta R.T.: 0.021 min
Response: 1990
Conc: 1.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

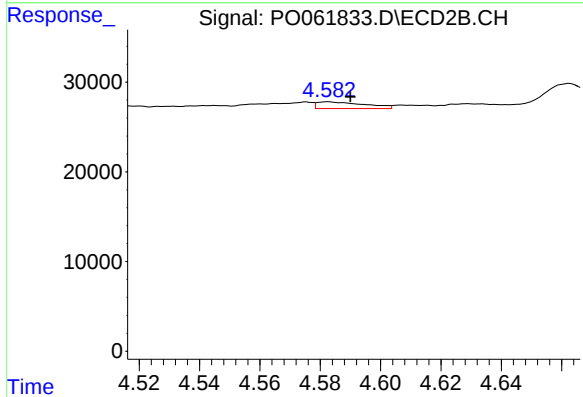


#21 AR-1248-1

R.T.: 4.583 min
Delta R.T.: -0.007 min
Response: 8316
Conc: 9.29 ng/ml

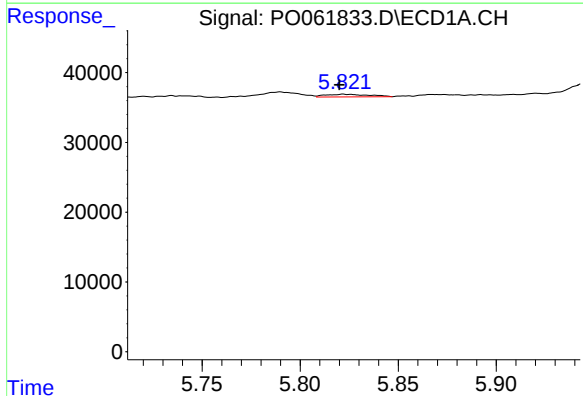


#22 AR-1248-2

R.T.: 5.822 min
Delta R.T.: 0.002 min
Response: 5884
Conc: 3.49 ng/ml

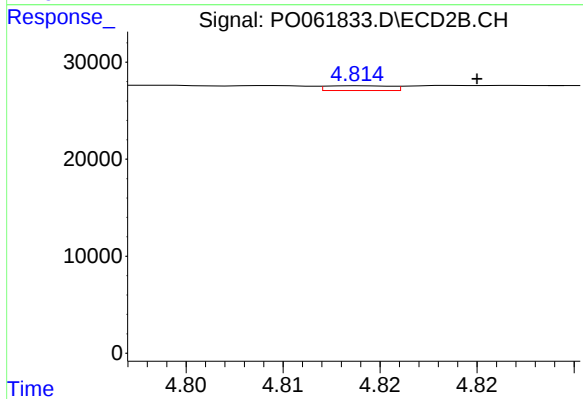

#22 AR-1248-2


R.T.: 4.814 min
Delta R.T.: -0.006 min
Response: 1133
Conc: 0.96 ng/ml

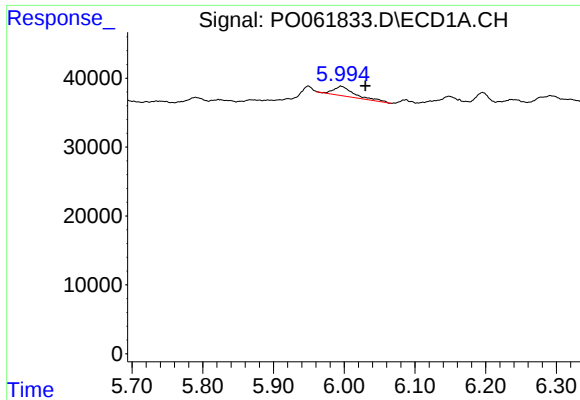

#23 AR-1248-3


R.T.: 5.995 min
Delta R.T.: -0.035 min
Response: 27725
Conc: 14.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

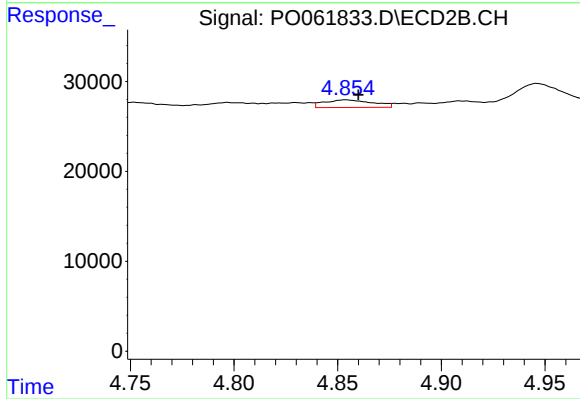


#23 AR-1248-3

R.T.: 4.854 min
Delta R.T.: -0.006 min
Response: 13759
Conc: 11.08 ng/ml

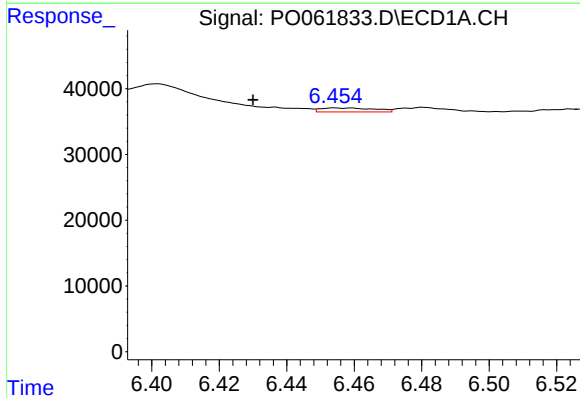


#24 AR-1248-4

R.T.: 6.454 min
Delta R.T.: 0.024 min
Response: 6651
Conc: 2.81 ng/ml

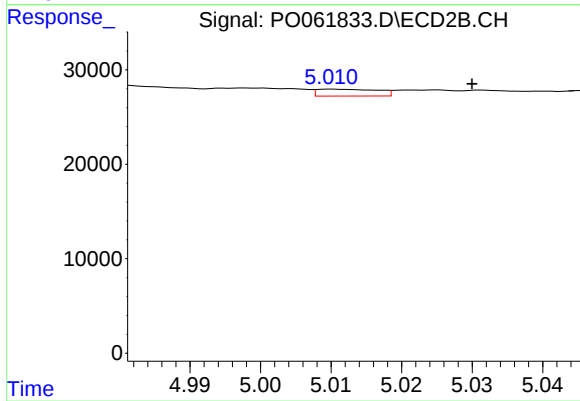

#24 AR-1248-4


R.T.: 5.010 min
Delta R.T.: -0.020 min
Response: 4318
Conc: 2.87 ng/ml

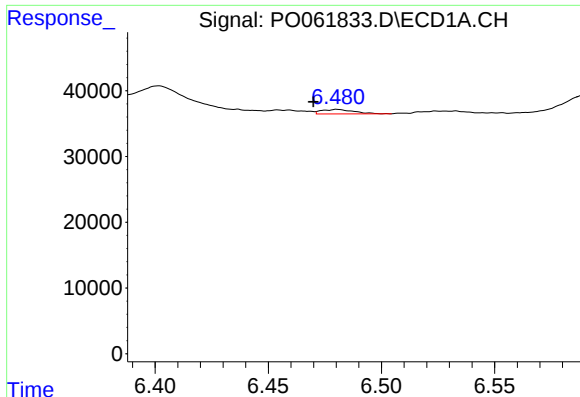

#25 AR-1248-5


R.T.: 6.481 min
Delta R.T.: 0.011 min
Response: 6756
Conc: 2.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

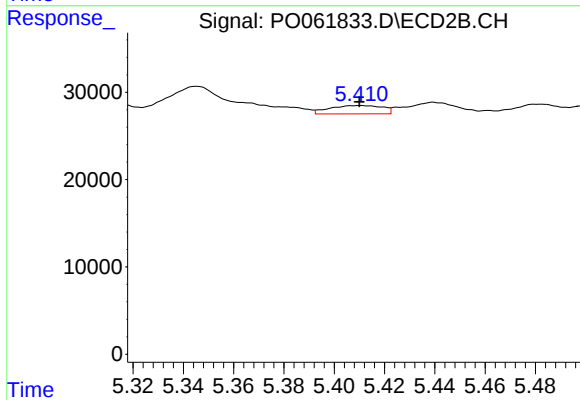


#25 AR-1248-5

R.T.: 5.410 min
Delta R.T.: 0.000 min
Response: 13969
Conc: 9.11 ng/ml

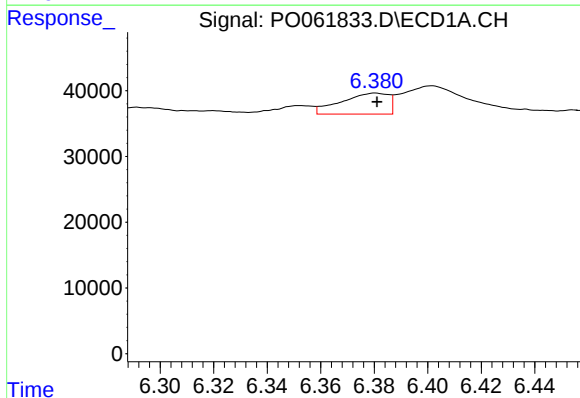


#26 AR-1254-1

R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 39403
Conc: 17.27 ng/ml

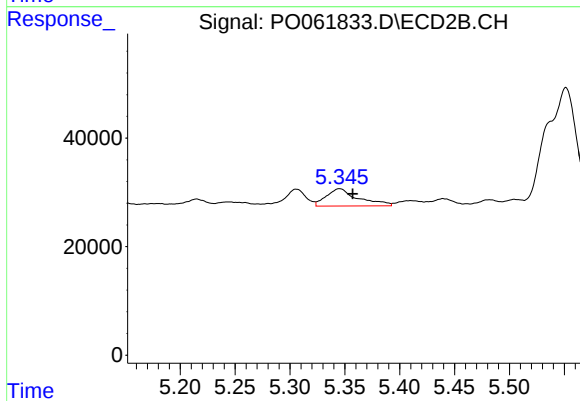

#26 AR-1254-1


R.T.: 5.345 min
Delta R.T.: -0.012 min
Response: 64815
Conc: 29.55 ng/ml

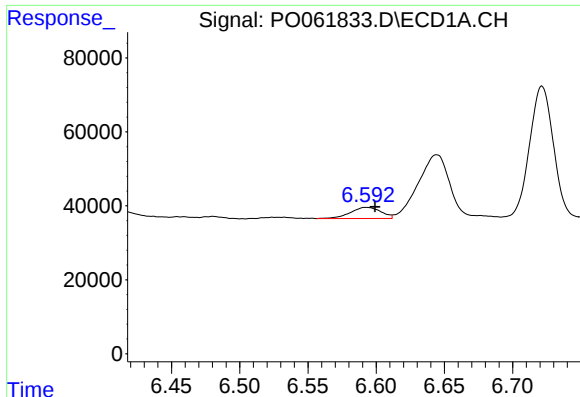

#27 AR-1254-2


R.T.: 6.593 min
Delta R.T.: -0.006 min
Response: 46828
Conc: 12.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

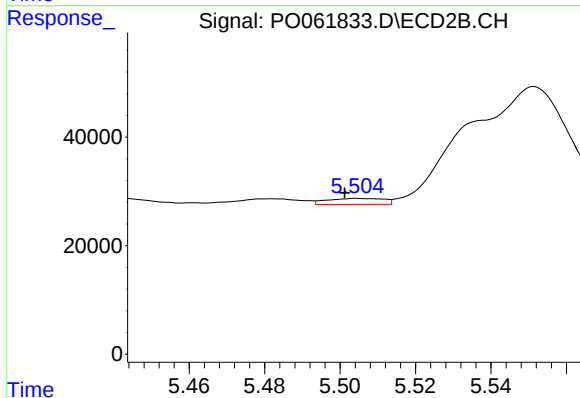


#27 AR-1254-2

R.T.: 5.504 min
Delta R.T.: 0.003 min
Response: 11595
Conc: 5.91 ng/ml

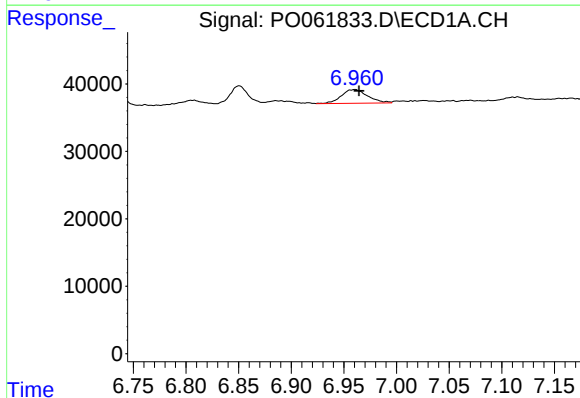


#28 AR-1254-3

R.T.: 6.960 min
Delta R.T.: -0.004 min
Response: 35797
Conc: 9.16 ng/ml

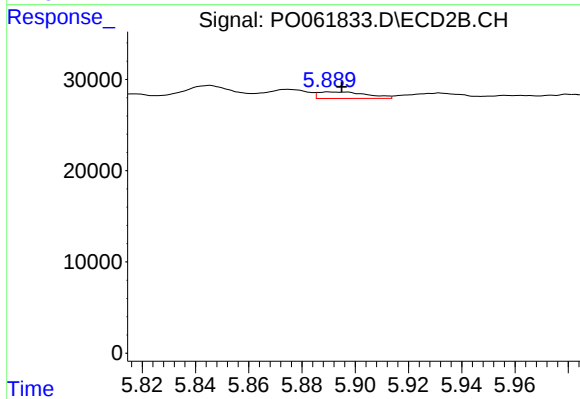

#28 AR-1254-3


R.T.: 5.890 min
Delta R.T.: -0.005 min
Response: 9192
Conc: 2.89 ng/ml

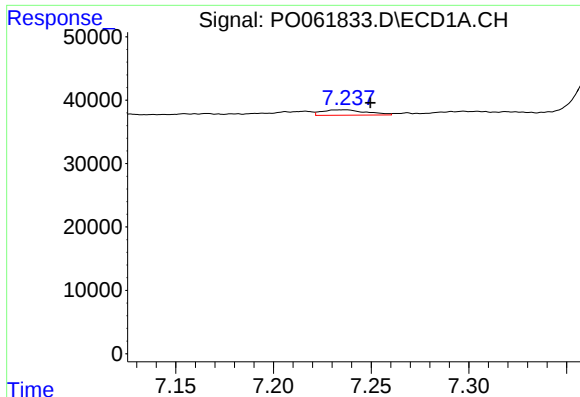

#29 AR-1254-4


R.T.: 7.237 min
Delta R.T.: -0.013 min
Response: 13547
Conc: 4.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

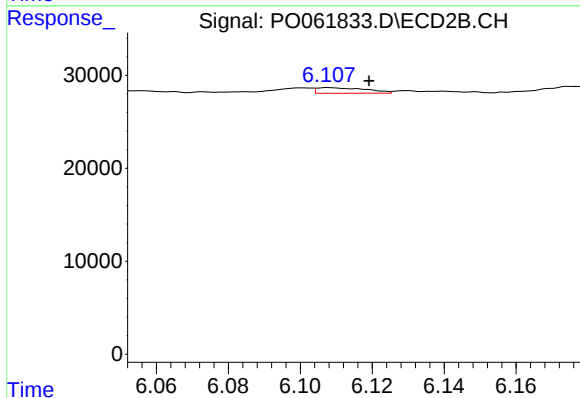


#29 AR-1254-4

R.T.: 6.108 min
Delta R.T.: -0.011 min
Response: 5787
Conc: 2.85 ng/ml

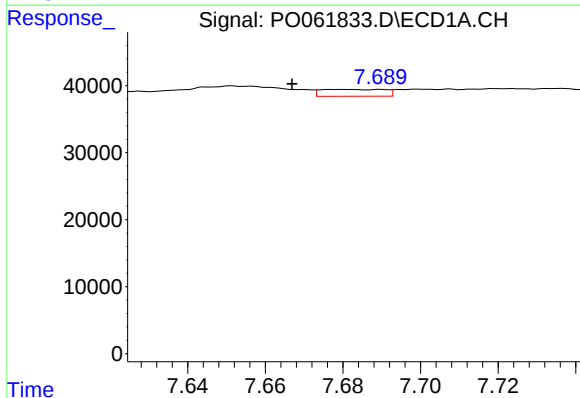


#30 AR-1254-5

R.T.: 7.680 min
Delta R.T.: 0.013 min
Response: 11603
Conc: 3.69 ng/ml

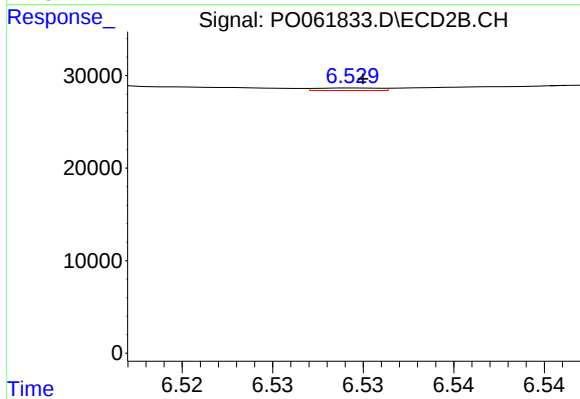

#30 AR-1254-5


R.T.: 6.530 min
Delta R.T.: 0.000 min
Response: 652
Conc: 0.23 ng/ml

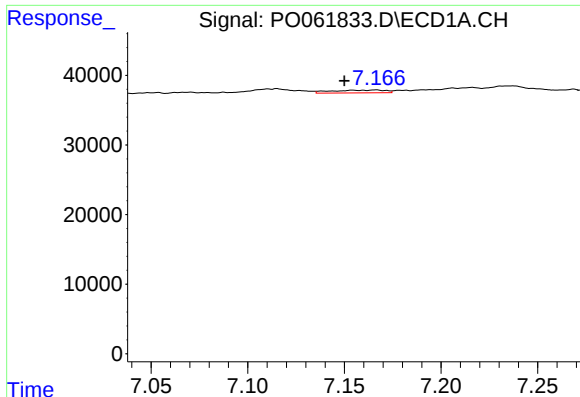

#31 AR-1260-1


R.T.: 7.166 min
Delta R.T.: 0.016 min
Response: 7581
Conc: 2.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

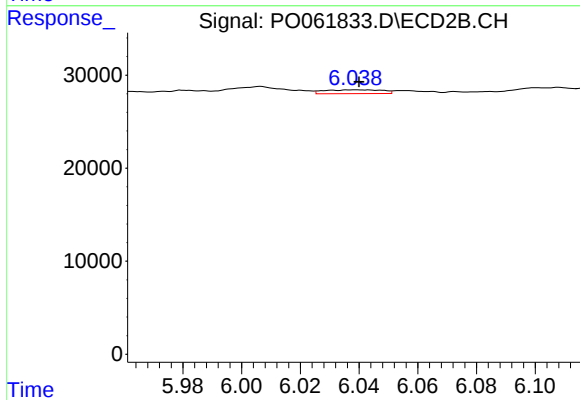


#31 AR-1260-1

R.T.: 6.039 min
Delta R.T.: -0.001 min
Response: 5620
Conc: 2.76 ng/ml

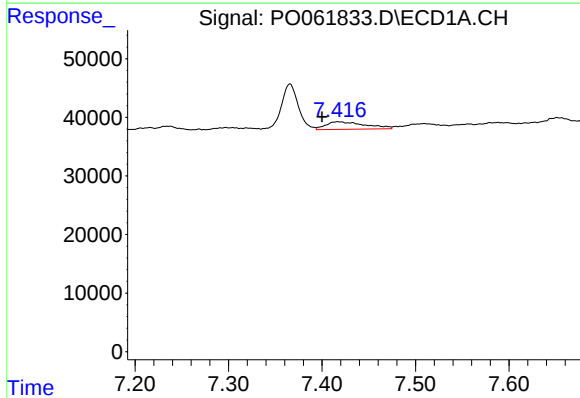


#32 AR-1260-2

R.T.: 7.417 min
Delta R.T.: 0.017 min
Response: 37699
Conc: 11.83 ng/ml

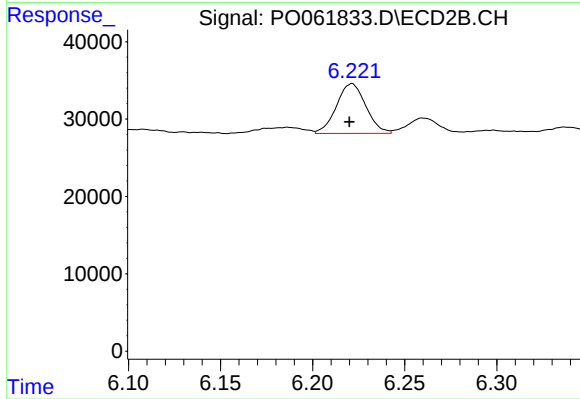

#32 AR-1260-2


R.T.: 6.222 min
Delta R.T.: 0.002 min
Response: 71511
Conc: 29.77 ng/ml

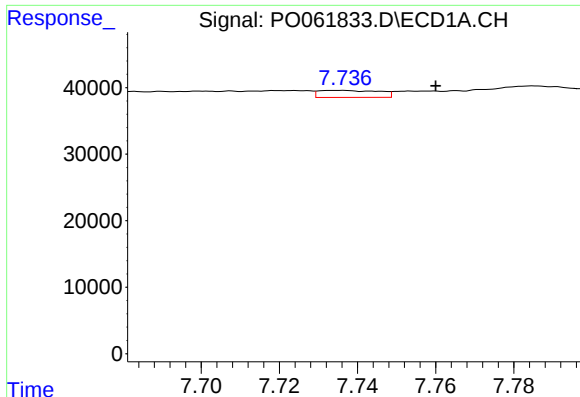

#33 AR-1260-3


R.T.: 7.736 min
Delta R.T.: -0.024 min
Response: 11370
Conc: 4.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

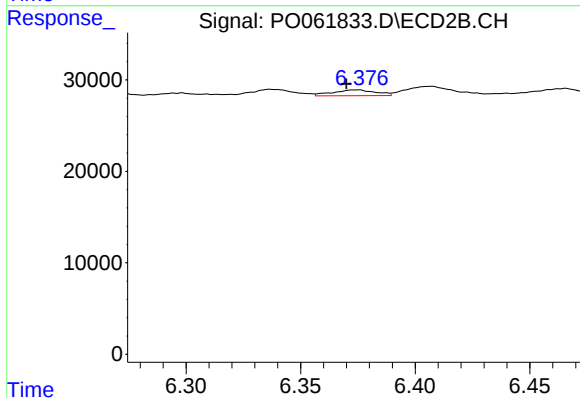


#33 AR-1260-3

R.T.: 6.376 min
Delta R.T.: 0.006 min
Response: 8260
Conc: 3.67 ng/ml

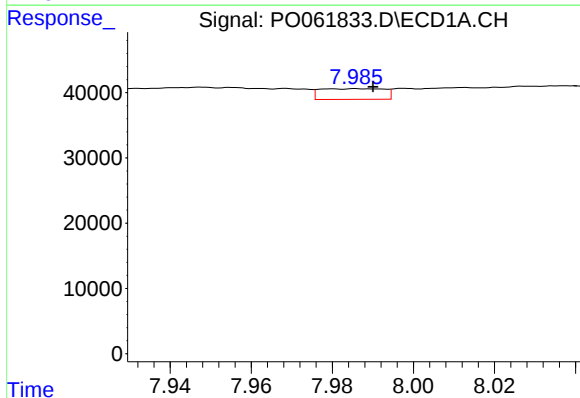


#34 AR-1260-4

R.T.: 7.986 min
Delta R.T.: -0.004 min
Response: 17814
Conc: 6.67 ng/ml

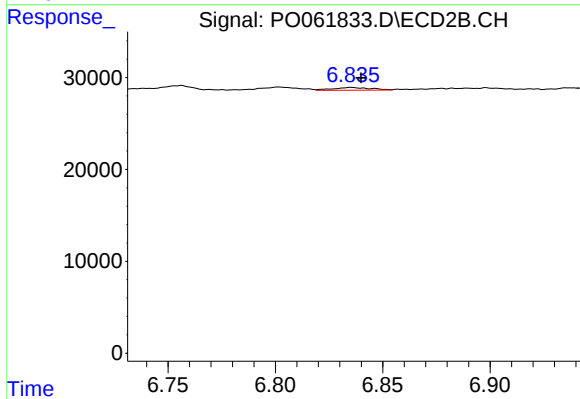

#34 AR-1260-4


R.T.: 6.835 min
Delta R.T.: -0.005 min
Response: 3656
Conc: 1.98 ng/ml

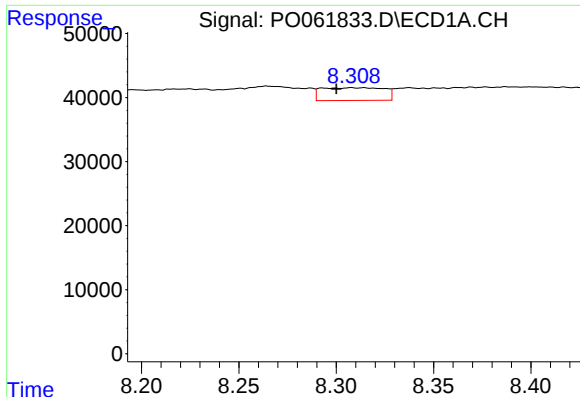

#35 AR-1260-5


R.T.: 8.308 min
Delta R.T.: 0.008 min
Response: 44395
Conc: 8.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

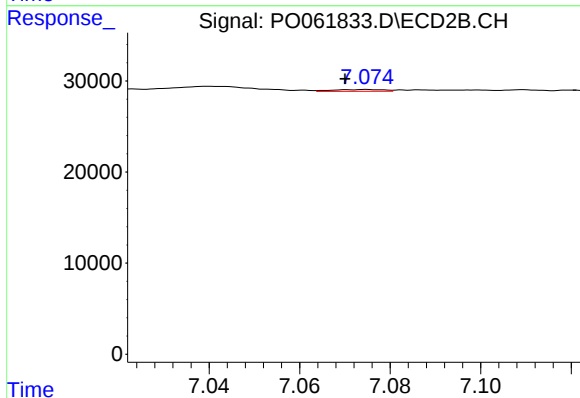


#35 AR-1260-5

R.T.: 7.075 min
Delta R.T.: 0.005 min
Response: 1531
Conc: 0.39 ng/ml

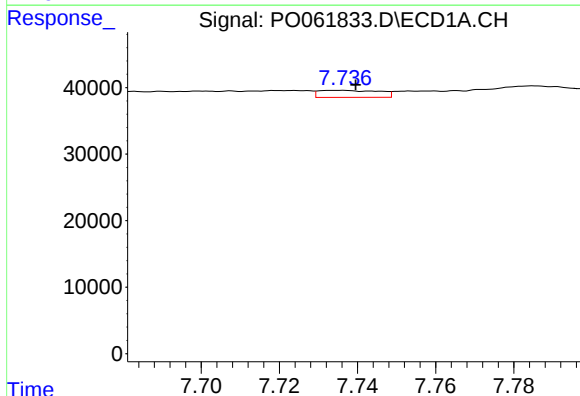


#36 AR-1262-1

R.T.: 7.736 min
Delta R.T.: -0.004 min
Response: 11370
Conc: 2.97 ng/ml

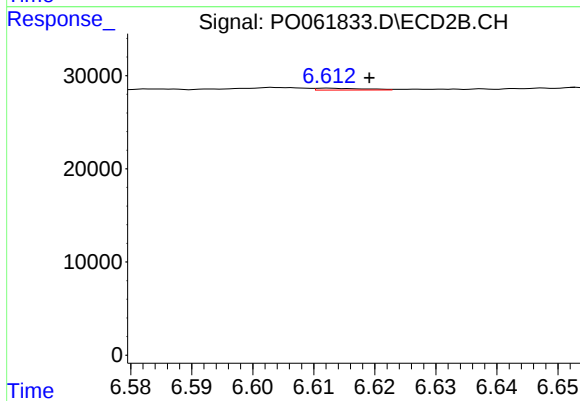

#36 AR-1262-1


R.T.: 6.612 min
Delta R.T.: -0.007 min
Response: 1098
Conc: 0.90 ng/ml

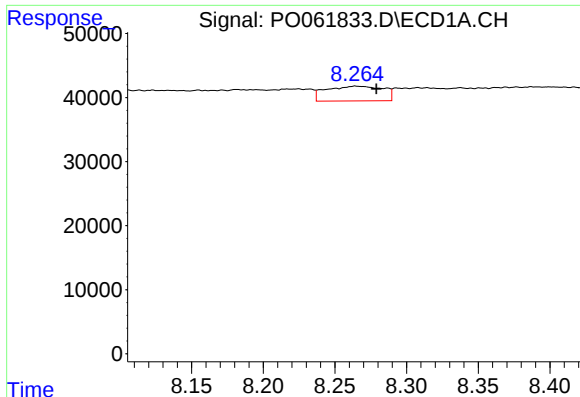

#37 AR-1262-2


R.T.: 8.264 min
Delta R.T.: -0.015 min
Response: 63935
Conc: 10.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

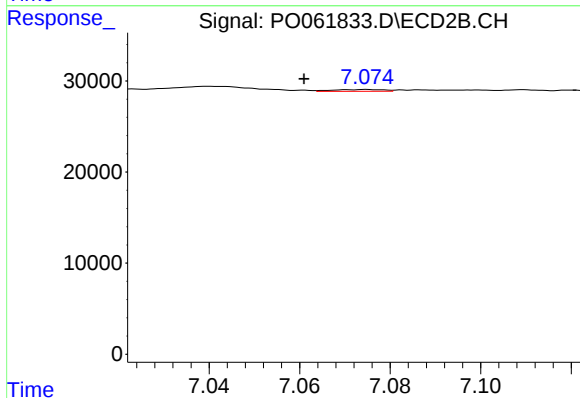


#37 AR-1262-2

R.T.: 7.075 min
Delta R.T.: 0.014 min
Response: 1531
Conc: 0.33 ng/ml

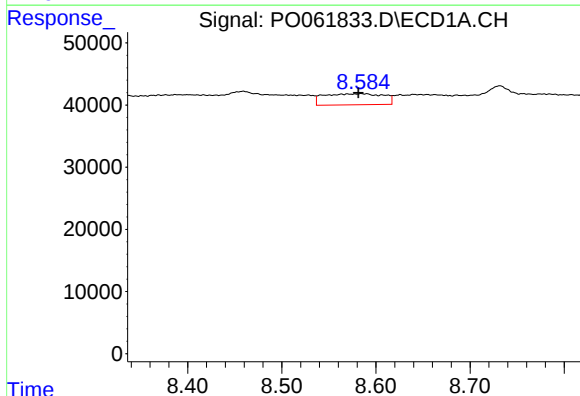


#38 AR-1262-3

R.T.: 8.584 min
Delta R.T.: 0.003 min
Response: 78319
Conc: 18.84 ng/ml

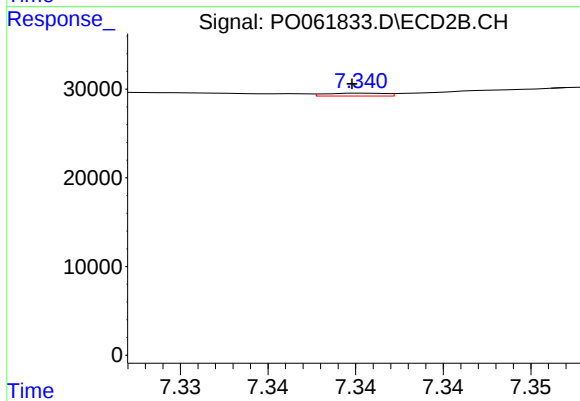

#38 AR-1262-3


R.T.: 7.341 min
Delta R.T.: 0.000 min
Response: 767
Conc: 0.41 ng/ml

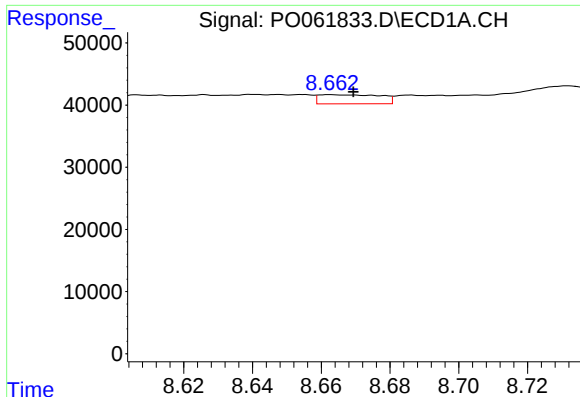

#39 AR-1262-4


R.T.: 8.663 min
Delta R.T.: -0.007 min
Response: 18305
Conc: 5.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

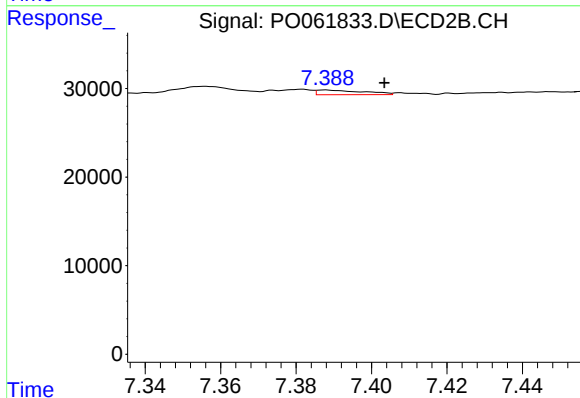


#39 AR-1262-4

R.T.: 7.388 min
Delta R.T.: -0.016 min
Response: 4505
Conc: 1.34 ng/ml

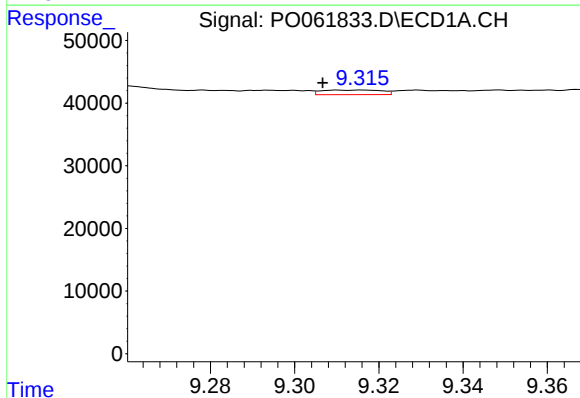


#40 AR-1262-5

R.T.: 9.316 min
Delta R.T.: 0.009 min
Response: 7172
Conc: 3.53 ng/ml

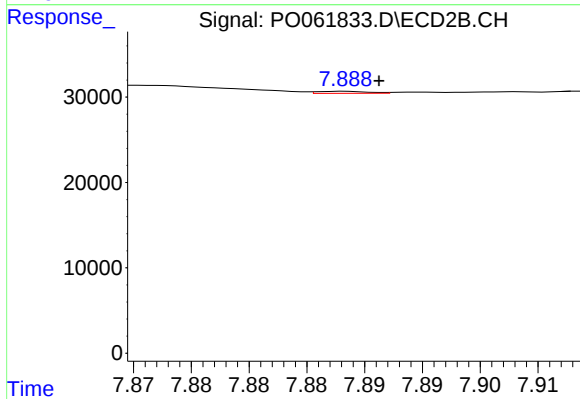

#40 AR-1262-5


R.T.: 7.888 min
Delta R.T.: -0.003 min
Response: 761
Conc: 0.50 ng/ml

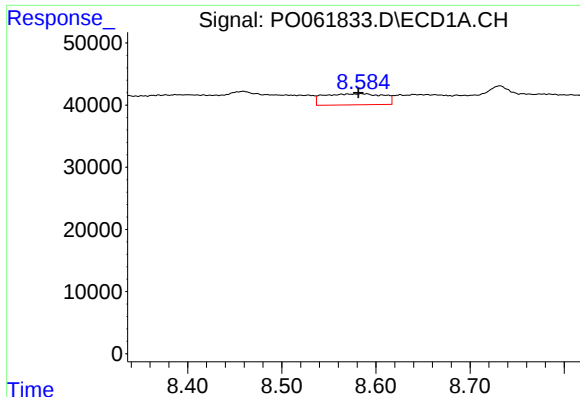

#41 AR-1268-1


R.T.: 8.584 min
Delta R.T.: 0.003 min
Response: 78319
Conc: 11.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

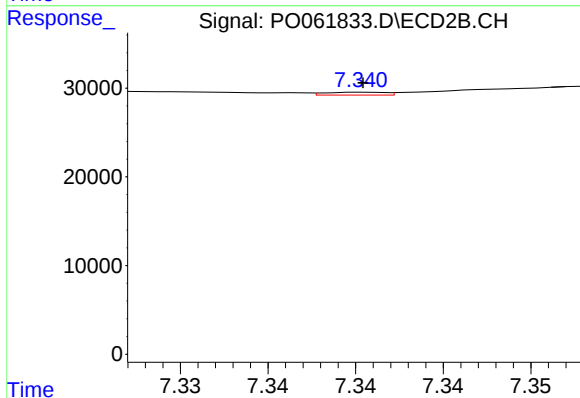


#41 AR-1268-1

R.T.: 7.341 min
Delta R.T.: 0.000 min
Response: 767
Conc: 0.16 ng/ml

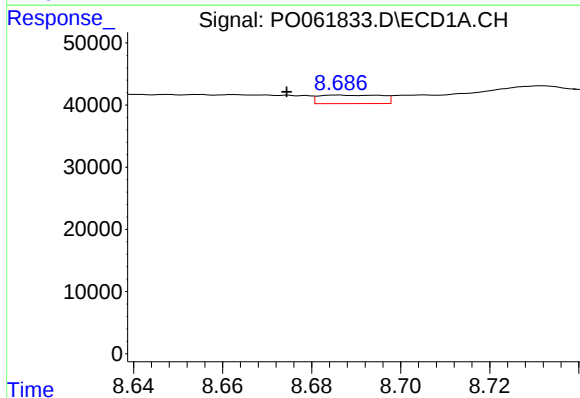


#42 AR-1268-2

R.T.: 8.686 min
Delta R.T.: 0.011 min
Response: 13422
Conc: 2.17 ng/ml

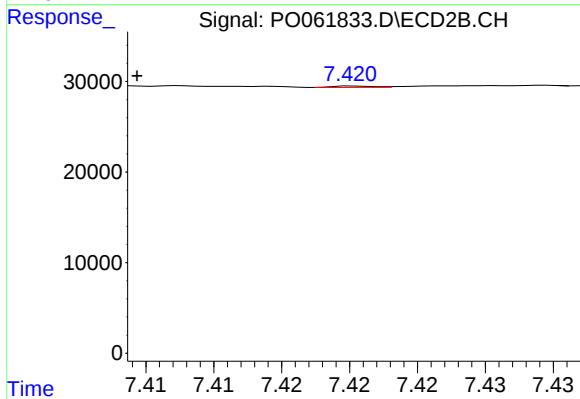

#42 AR-1268-2


R.T.: 7.420 min
Delta R.T.: 0.016 min
Response: 307
Conc: 0.07 ng/ml

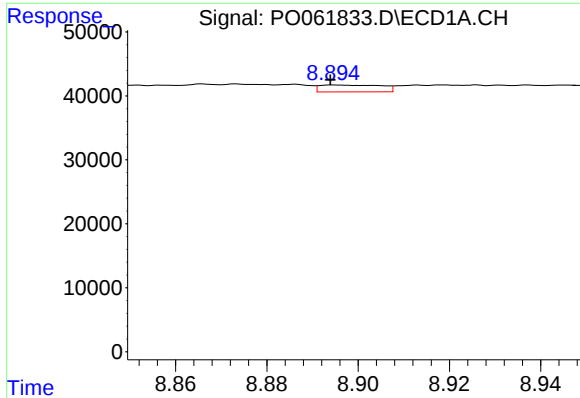

#43 AR-1268-3


R.T.: 8.895 min
Delta R.T.: 0.001 min
Response: 10189
Conc: 1.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

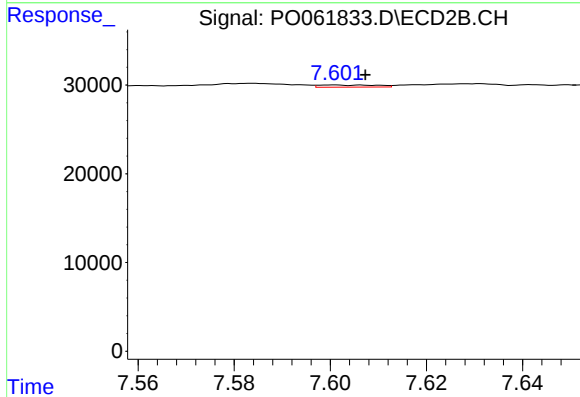


#43 AR-1268-3

R.T.: 7.601 min
Delta R.T.: -0.006 min
Response: 2015
Conc: 0.56 ng/ml

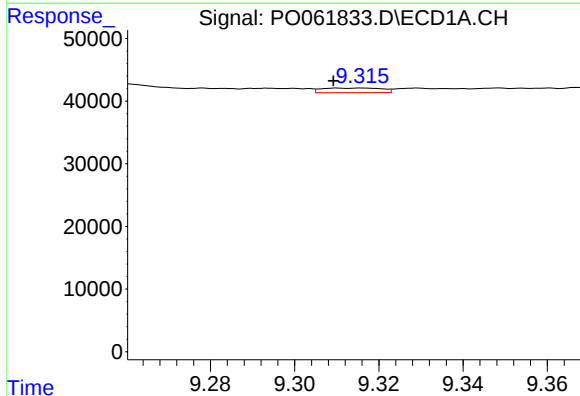


#44 AR-1268-4

R.T.: 9.316 min
Delta R.T.: 0.007 min
Response: 7172
Conc: 3.28 ng/ml

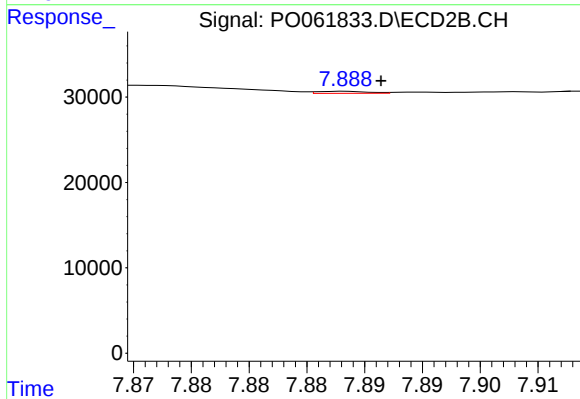

#44 AR-1268-4


R.T.: 7.888 min
Delta R.T.: -0.003 min
Response: 761
Conc: 0.47 ng/ml

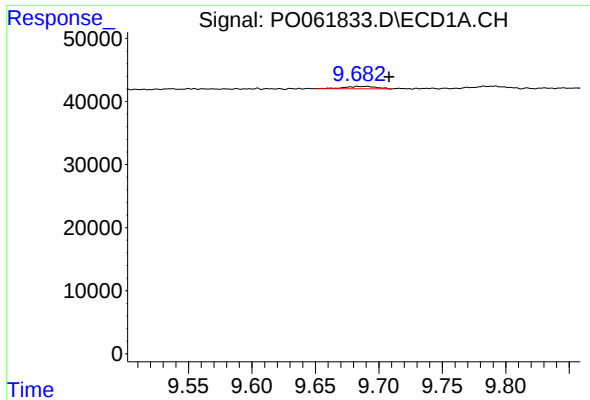

#45 AR-1268-5

R.T.: 9.690 min
Delta R.T.: -0.018 min
Response: 6796
Conc: 0.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-062

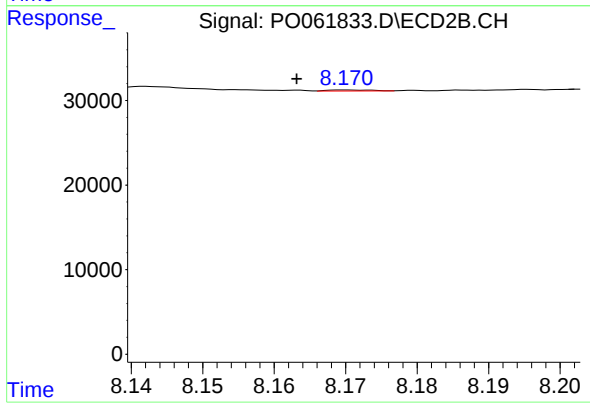

#45 AR-1268-5

R.T.: 8.170 min
Delta R.T.: 0.007 min
Response: 540
Conc: 0.05 ng/ml