

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100919\
 Data File : P0061825.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Oct 2019 13:14
 Operator : HP/AJ
 Sample : K5152-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SU-02-100719

Manual Integrations
 APPROVED

Ankita
 10/10/2019 9:32:09 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 13:31:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.348	3.510	976194	768687	23.801	23.769
2) SA Decachlor...	10.003	8.370	832492	511206	17.876	15.790m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100919\
Data File : PO061825.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Oct 2019 13:14
Operator : HP/AJ
Sample : K5152-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SU-02-100719


Manual Integrations
APPROVED

Ankita
10/10/2019 9:32:09 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 13:31:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

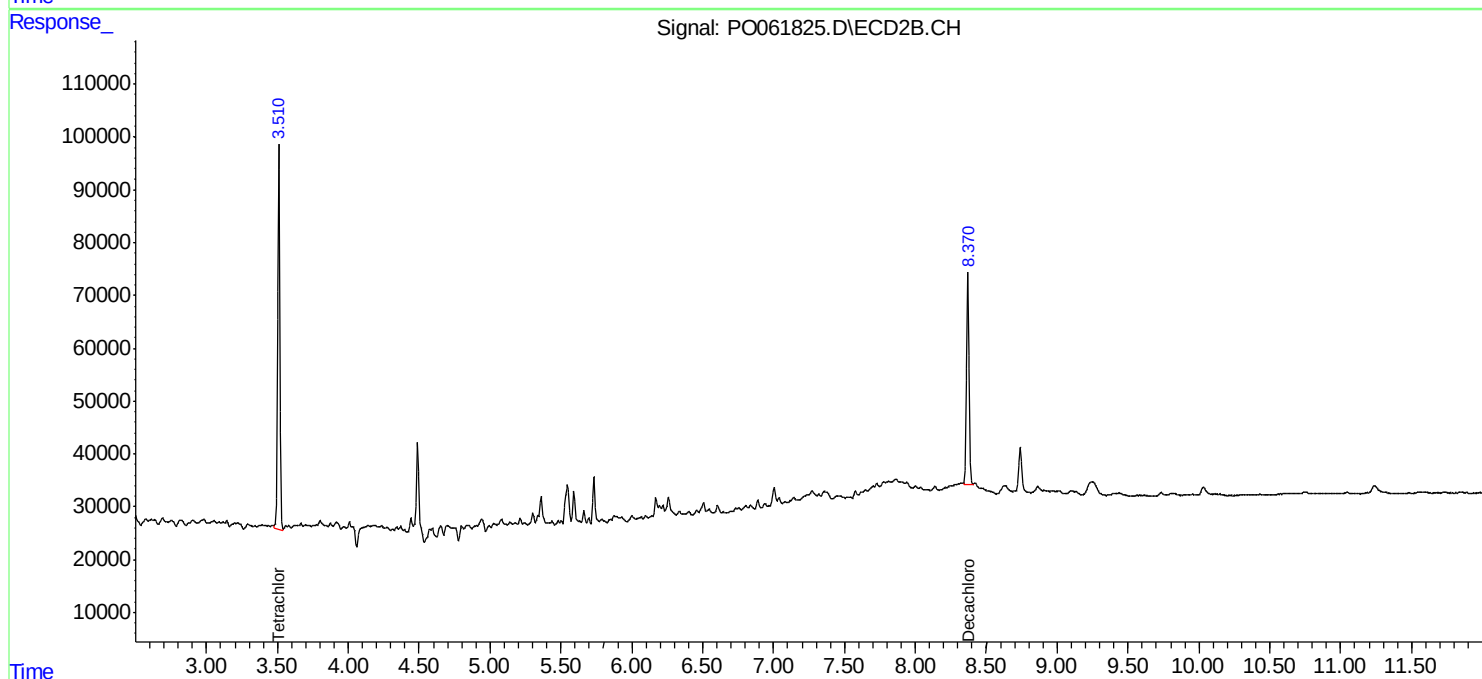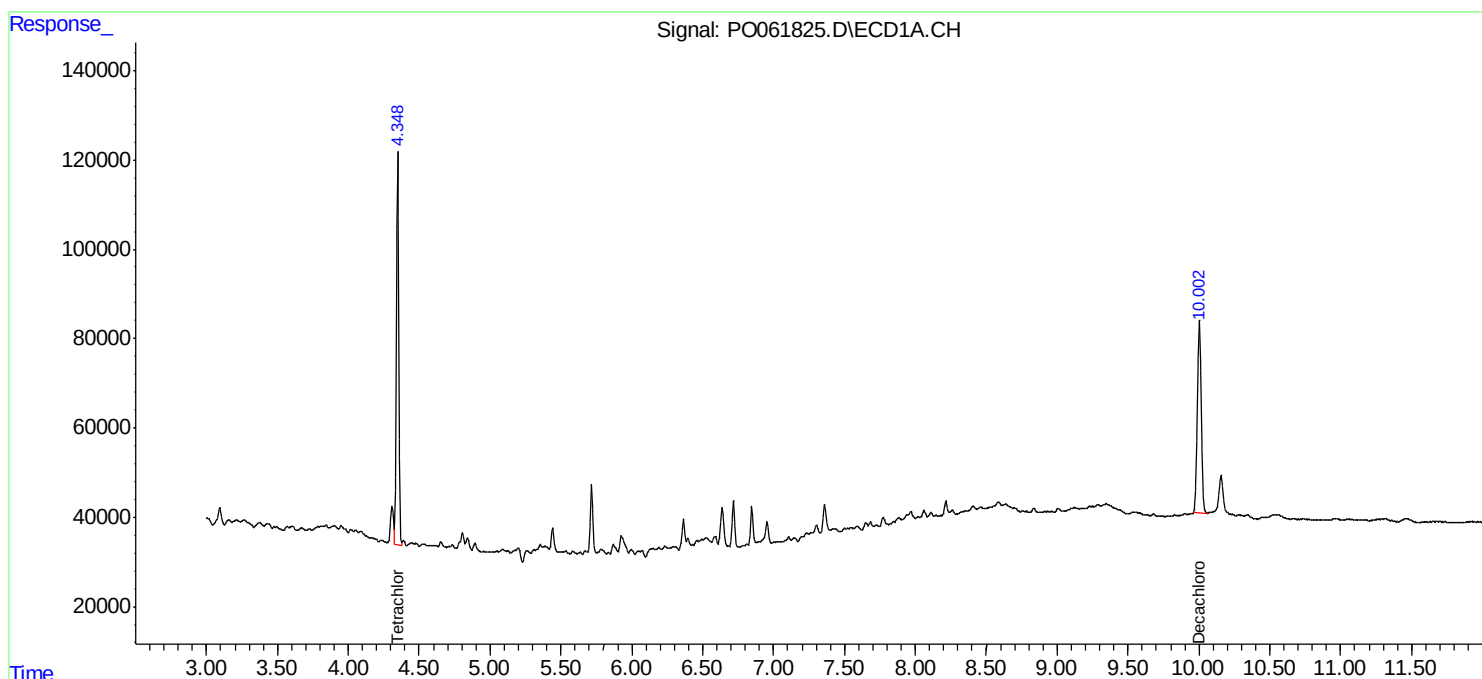

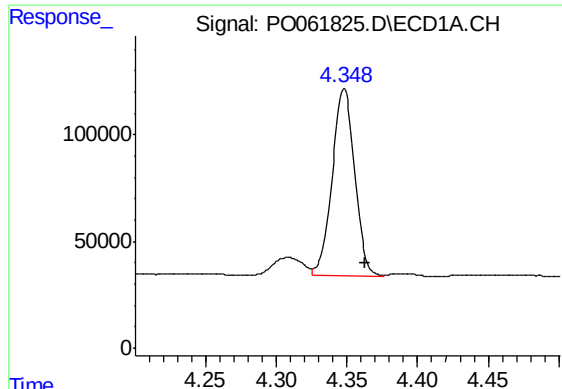


#1 Tetrachloro-m-xylene

R.T.: 4.348 min
Delta R.T.: -0.015 min
Response: 976194
Conc: 23.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU-02-100719


Manual Integrations
APPROVED

Ankita
10/10/2019 9:32:09 AM

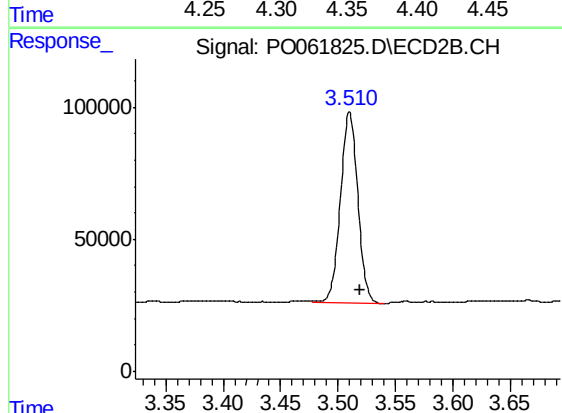


#1 Tetrachloro-m-xylene

R.T.: 3.510 min
Delta R.T.: -0.009 min
Response: 768687
Conc: 23.77 ng/ml

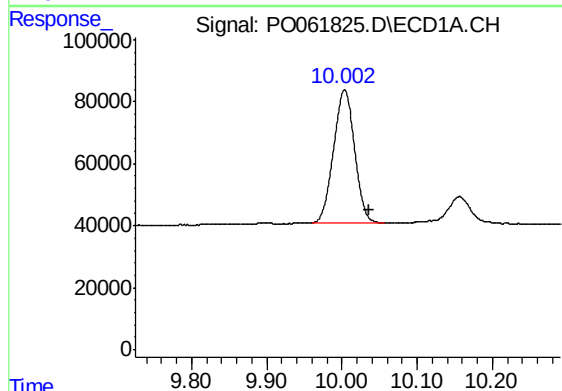

#2 Decachlorobiphenyl

R.T.: 10.003 min
Delta R.T.: -0.033 min
Response: 832492
Conc: 17.88 ng/ml

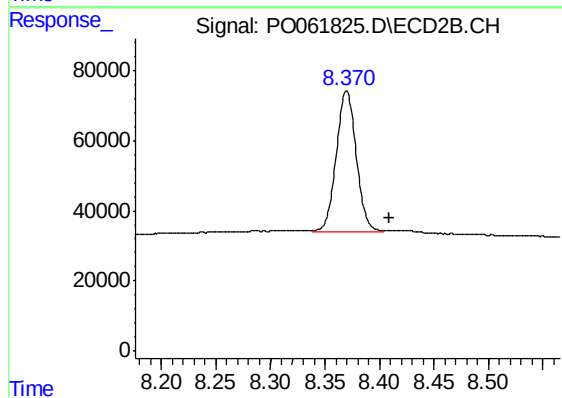

#2 Decachlorobiphenyl

R.T.: 8.370 min
Delta R.T.: -0.039 min
Response: 511206
Conc: 15.79 ng/ml m