

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100919\
 Data File : P0061834.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Oct 2019 17:14
 Operator : HP/AJ
 Sample : K5284-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-EF-01-016-ABCD

Manual Integrations
 APPROVED

Ankita
 10/10/2019 9:32:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 01:13:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 01 15:34:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.353	3.513	844471	597225	20.590	18.467
2)	SA Decachlor...	10.010	8.372	804004	551115	17.264	17.022m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100919\
Data File : PO061834.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Oct 2019 17:14
Operator : HP/AJ
Sample : K5284-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-EF-01-016-ABCD


Manual Integrations
APPROVED

Ankita
10/10/2019 9:32:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 01:13:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 01 15:34:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

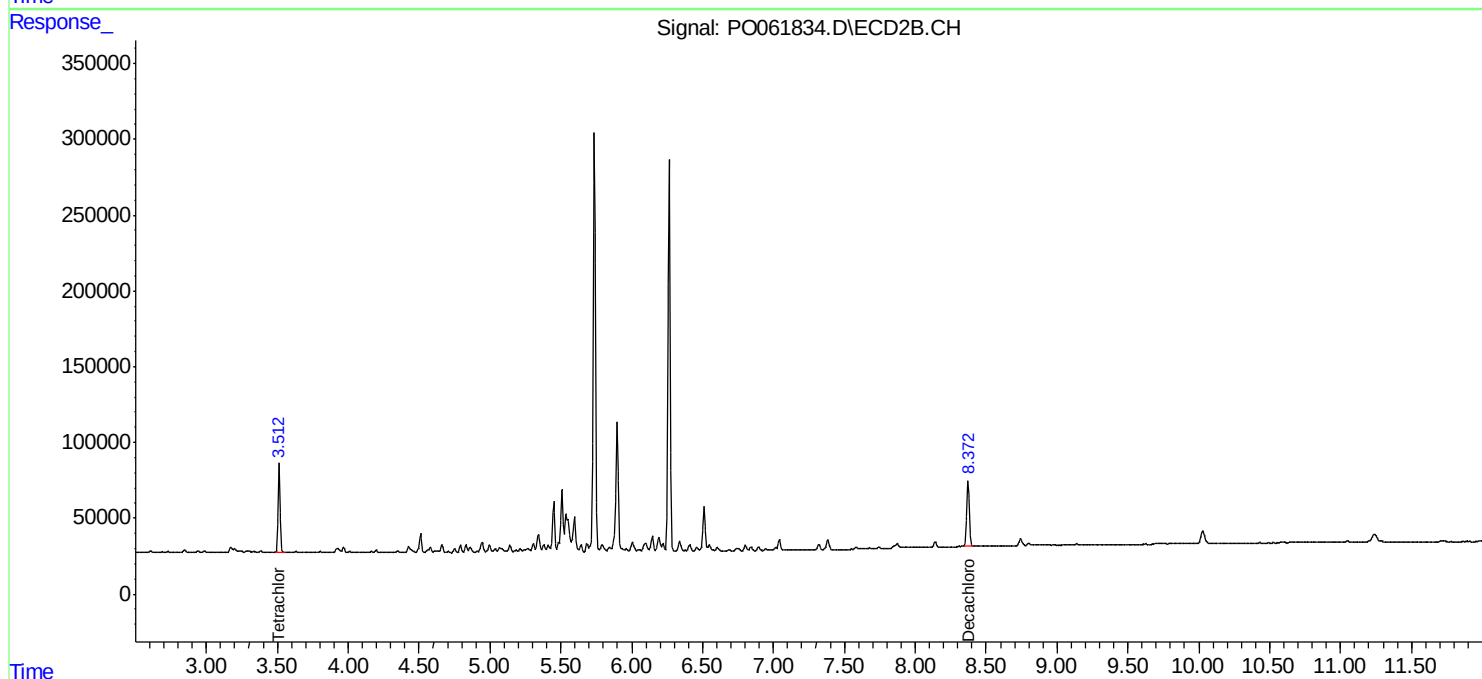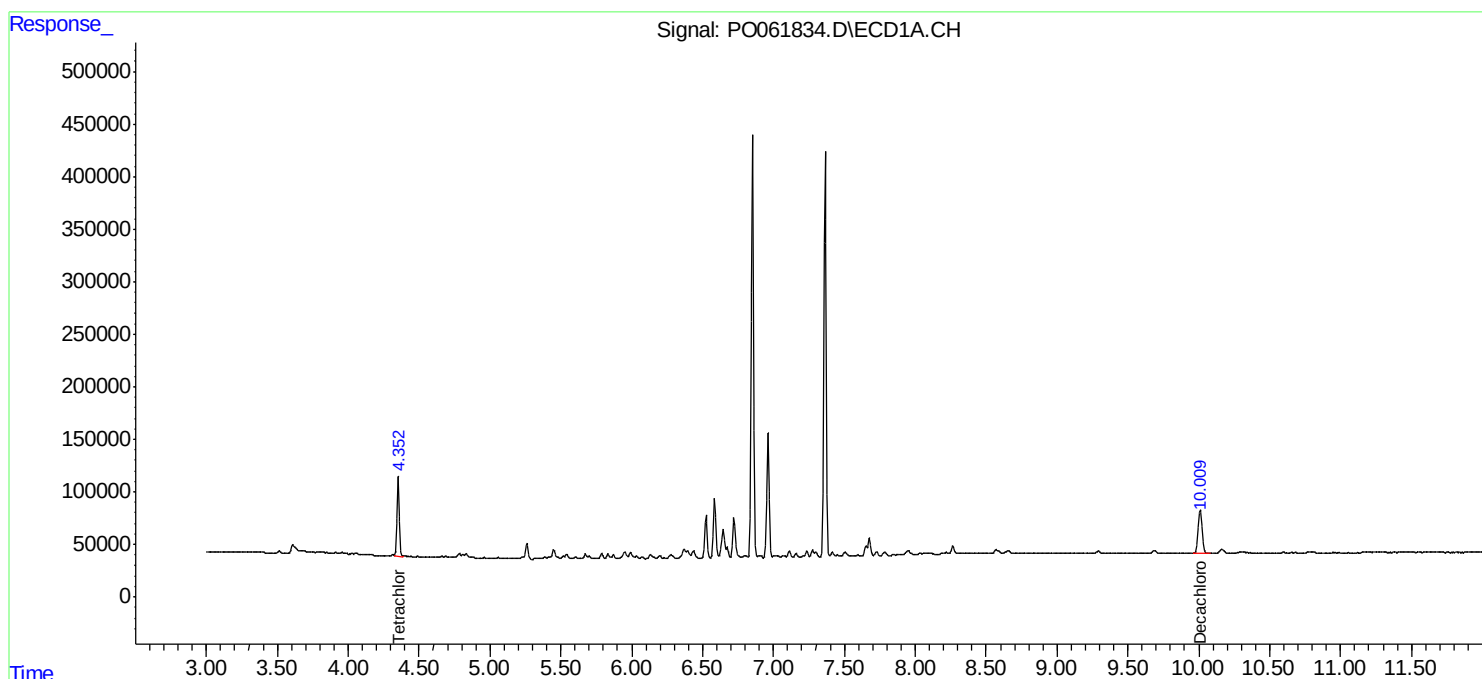

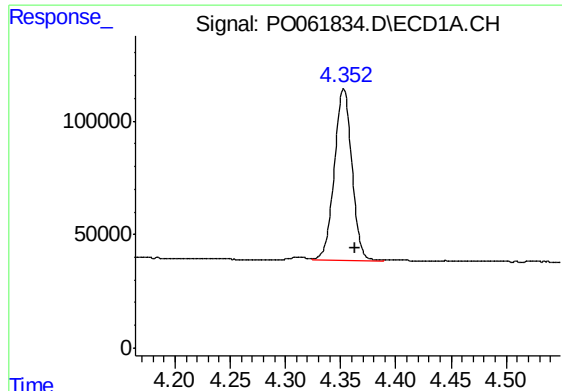


#1 Tetrachloro-m-xylene

R.T.: 4.353 min
Delta R.T.: -0.010 min
Response: 844471
Conc: 20.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-EF-01-016-ABCD


Manual Integrations
APPROVED

Ankita
10/10/2019 9:32:28 AM

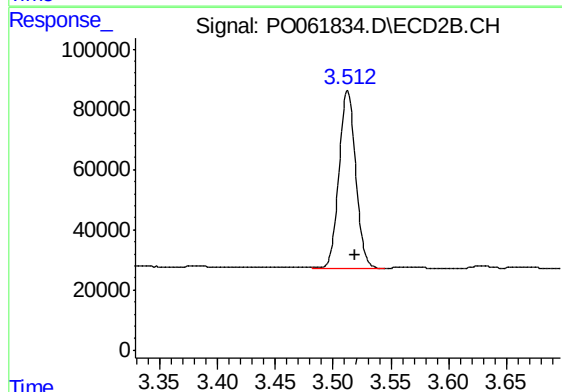


#1 Tetrachloro-m-xylene

R.T.: 3.513 min
Delta R.T.: -0.006 min
Response: 597225
Conc: 18.47 ng/ml

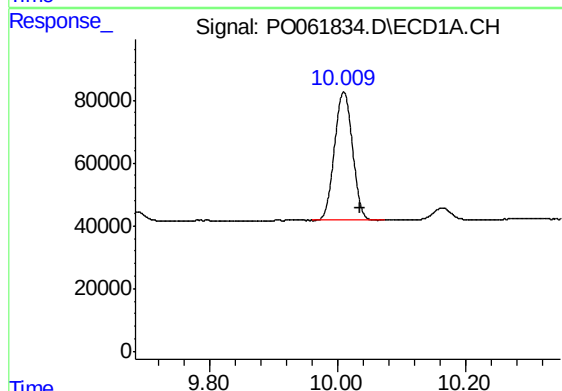

#2 Decachlorobiphenyl

R.T.: 10.010 min
Delta R.T.: -0.026 min
Response: 804004
Conc: 17.26 ng/ml

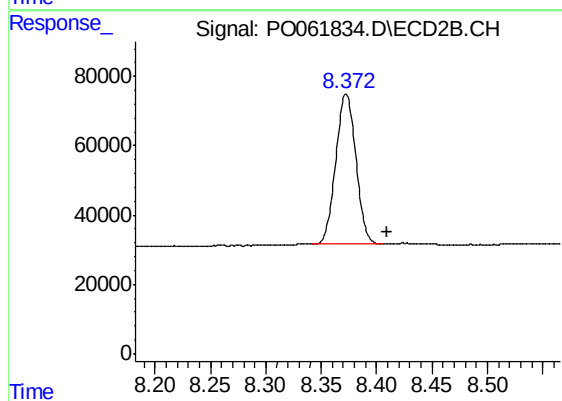

#2 Decachlorobiphenyl

R.T.: 8.372 min
Delta R.T.: -0.037 min
Response: 551115
Conc: 17.02 ng/ml m