

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101419\
 Data File : P0061953.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Oct 2019 14:46
 Operator : HP/AJ
 Sample : K5325-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 10-10-E

Manual Integrations
 APPROVED

Ankita
 10/15/2019 9:02:12 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 15:02:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.325	3.484	1017817	713952	16.457	16.649
2)	SA Decachlor...	9.957	8.340	775925	396785	13.868	13.523
Target Compounds							
26)	L6 AR-1254-1	6.335	5.304	56591	37564	21.230m	15.359 #
27)	L6 AR-1254-2	6.553	5.449	74251	42164	18.161	19.909
28)	L6 AR-1254-3	6.918	5.841	88503	61105	21.152	18.755
29)	L6 AR-1254-4	7.203	6.066	60495	42976	20.076	22.251
30)	L6 AR-1254-5	7.620	6.475	69089	61964	22.046	23.461

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101419\
Data File : PO061953.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Oct 2019 14:46
Operator : HP/AJ
Sample : K5325-05
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
10-10-E


Manual Integrations
APPROVED

Ankita
10/15/2019 9:02:12 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 15:02:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

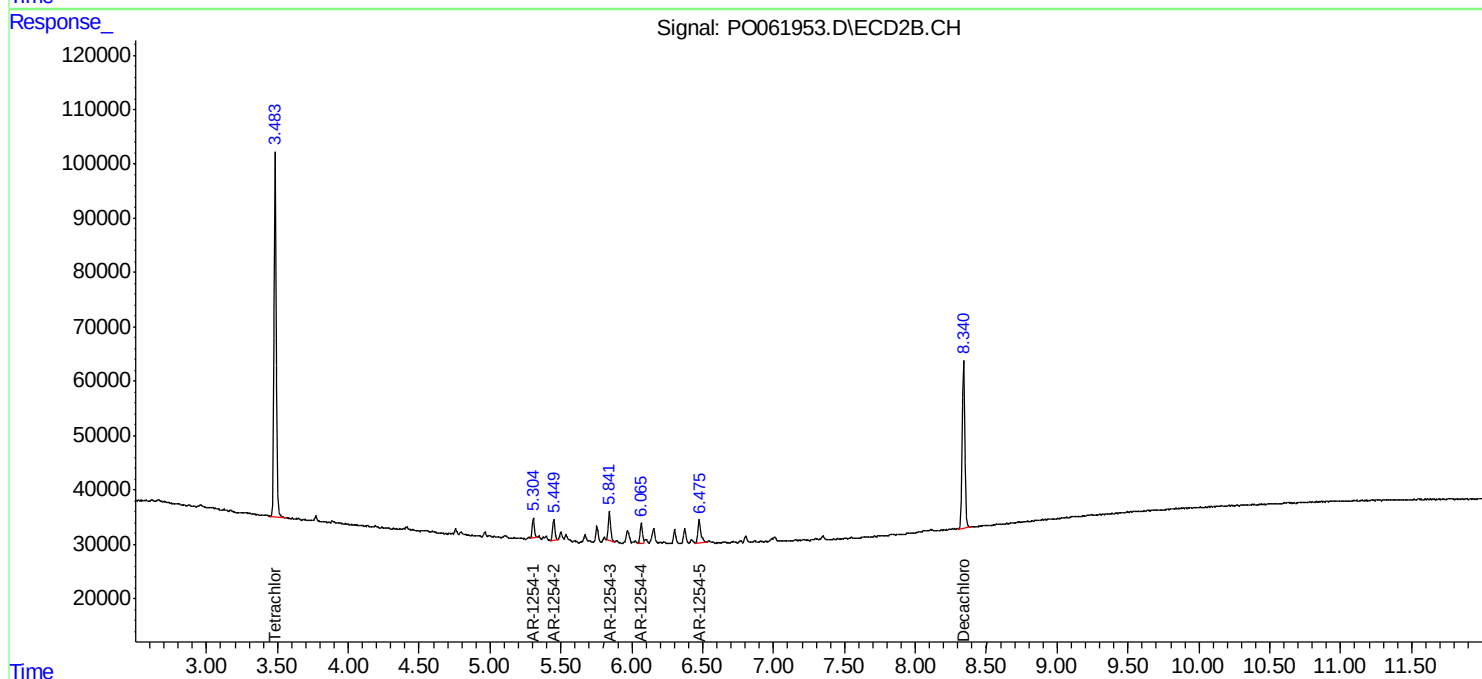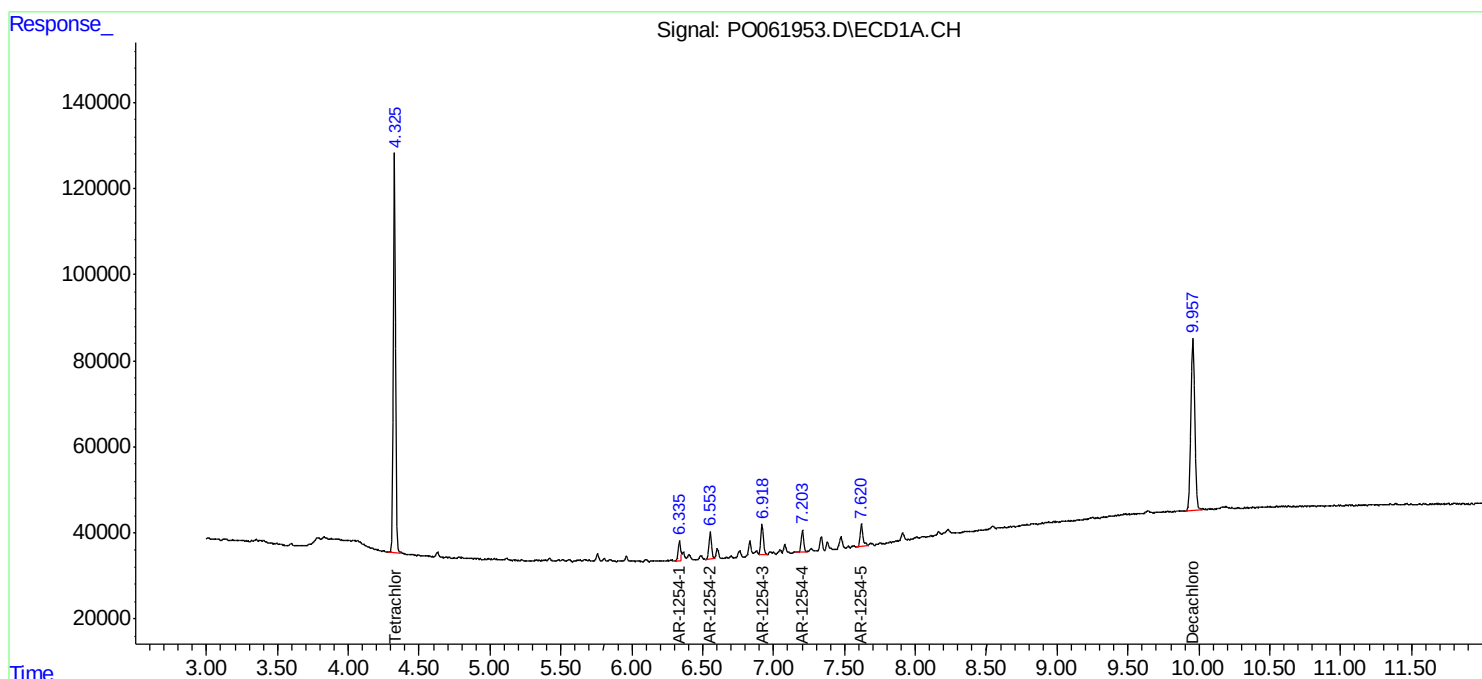

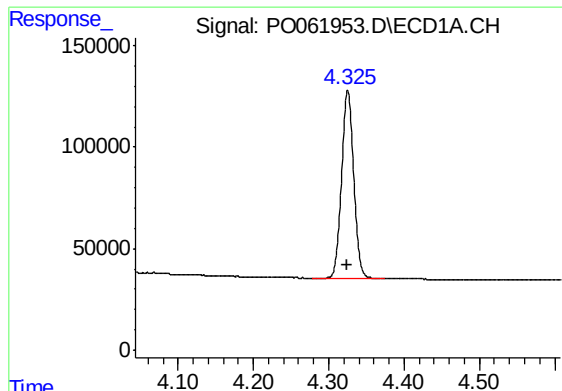


#1 Tetrachloro-m-xylene

R.T.: 4.325 min
Delta R.T.: 0.000 min
Response: 1017817
Conc: 16.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
10-10-E


Manual Integrations
APPROVED

Ankita
10/15/2019 9:02:12 AM

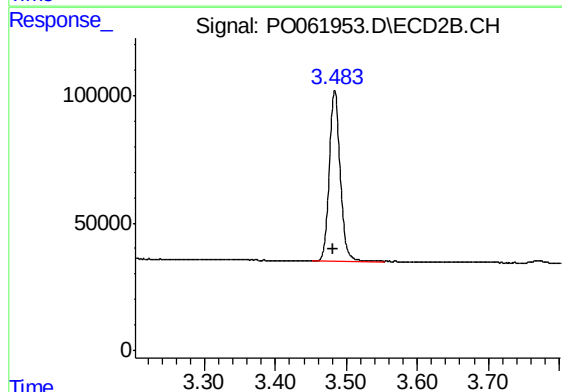


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: 0.002 min
Response: 713952
Conc: 16.65 ng/ml

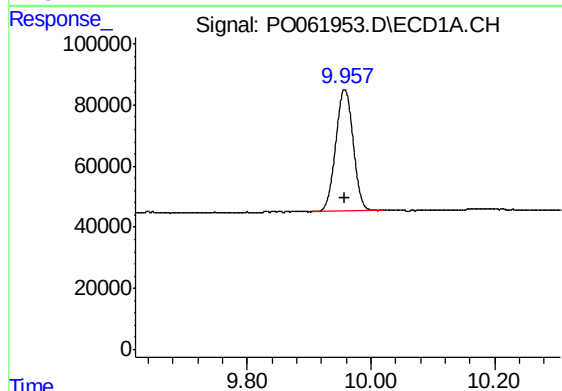


#2 Decachlorobiphenyl

R.T.: 9.957 min
Delta R.T.: 0.000 min
Response: 775925
Conc: 13.87 ng/ml

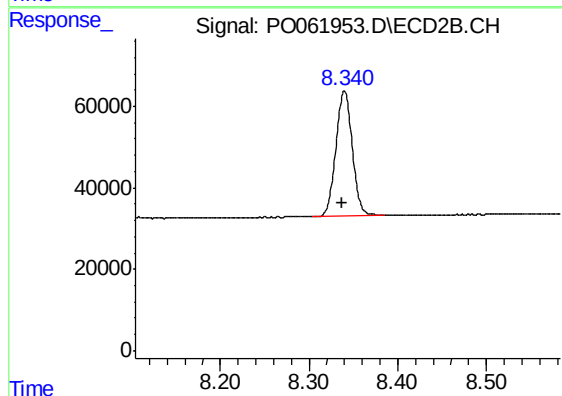

#2 Decachlorobiphenyl

R.T.: 8.340 min
Delta R.T.: 0.002 min
Response: 396785
Conc: 13.52 ng/ml

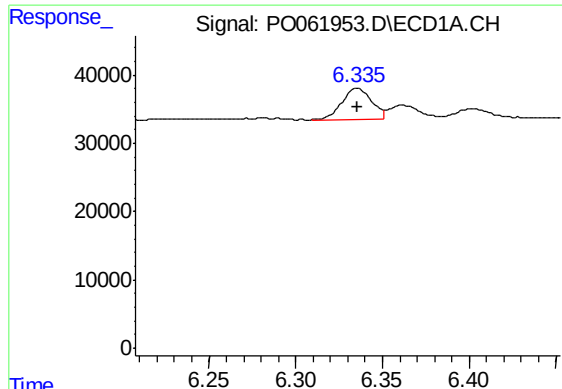


#26 AR-1254-1

R.T.: 6.335 min
Delta R.T.: 0.000 min
Response: 56591
Conc: 21.23 ng/ml m

Instrument :
ECD_O
ClientSampleId :
10-10-E


Manual Integrations
APPROVED

Ankita
10/15/2019 9:02:12 AM

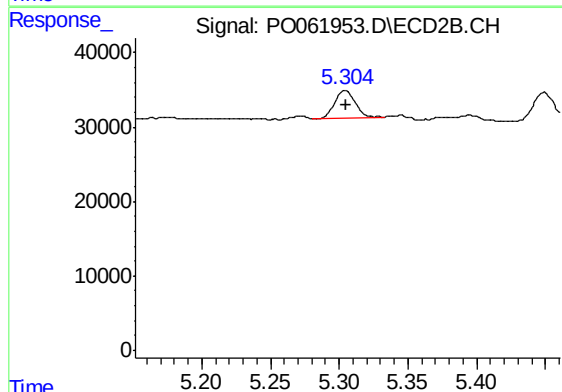


#26 AR-1254-1

R.T.: 5.304 min
Delta R.T.: 0.000 min
Response: 37564
Conc: 15.36 ng/ml

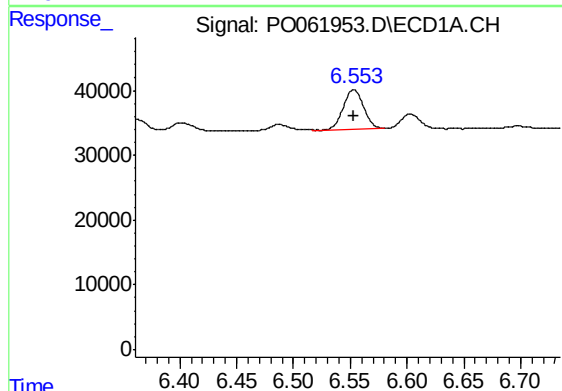


#27 AR-1254-2

R.T.: 6.553 min
Delta R.T.: 0.000 min
Response: 74251
Conc: 18.16 ng/ml

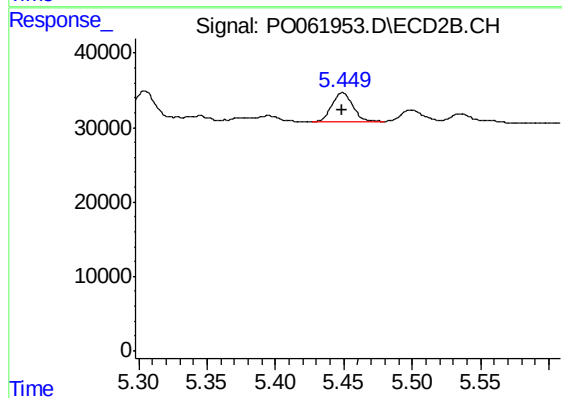

#27 AR-1254-2

R.T.: 5.449 min
Delta R.T.: 0.000 min
Response: 42164
Conc: 19.91 ng/ml

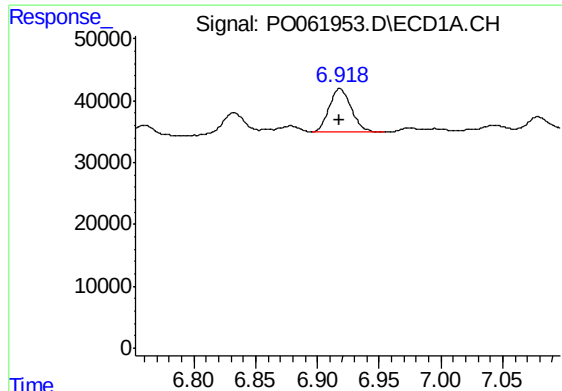


#28 AR-1254-3

R.T.: 6.918 min
Delta R.T.: 0.000 min
Response: 88503
Conc: 21.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
10-10-E


Manual Integrations
APPROVED

Ankita
10/15/2019 9:02:12 AM

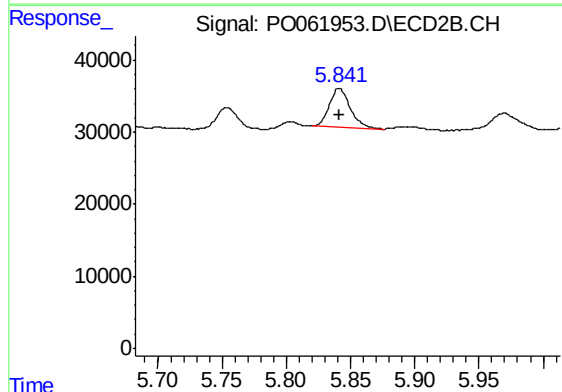


#28 AR-1254-3

R.T.: 5.841 min
Delta R.T.: 0.000 min
Response: 61105
Conc: 18.75 ng/ml

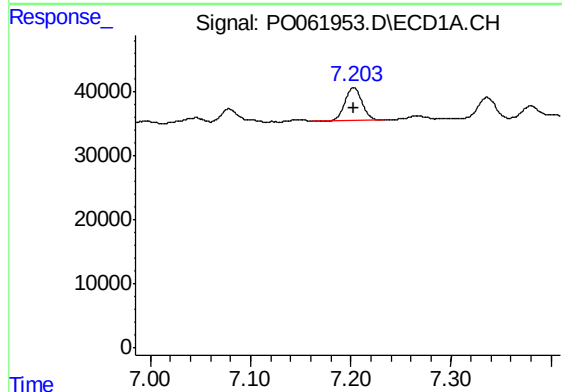


#29 AR-1254-4

R.T.: 7.203 min
Delta R.T.: 0.000 min
Response: 60495
Conc: 20.08 ng/ml

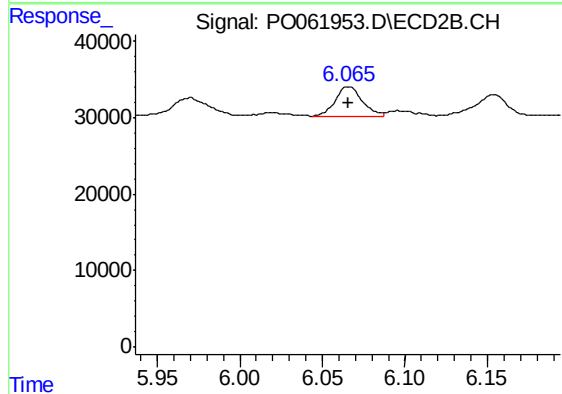

#29 AR-1254-4

R.T.: 6.066 min
Delta R.T.: 0.000 min
Response: 42976
Conc: 22.25 ng/ml

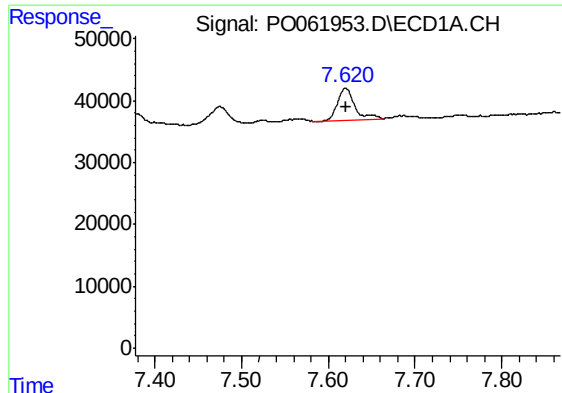


#30 AR-1254-5

R.T.: 7.620 min
Delta R.T.: 0.000 min
Response: 69089
Conc: 22.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
10-10-E

Manual Integrations
APPROVED

Ankita
10/15/2019 9:02:12 AM

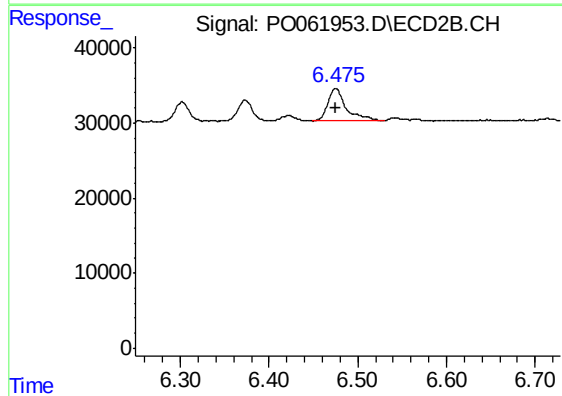

#30 AR-1254-5

R.T.: 6.475 min
Delta R.T.: 0.000 min
Response: 61964
Conc: 23.46 ng/ml