

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101419\
 Data File : P0061954.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Oct 2019 15:03
 Operator : HP/AJ
 Sample : K5325-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 10-10-D

Manual Integrations
 APPROVED

Ankita
 10/15/2019 9:02:14 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 15:31:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.325	3.484	1036990	717809	16.767	16.739
2)	SA Decachlor...	9.955	8.340	776343	398644	13.875	13.586
Target Compounds							
26)	L6 AR-1254-1	6.335	5.304	58672	36031	22.011m	14.732 #
27)	L6 AR-1254-2	6.553	5.449	77250	41806	18.895	19.740
28)	L6 AR-1254-3	6.918	5.842	91412	69786	21.848	21.419
29)	L6 AR-1254-4	7.202	6.066	62497	42053	20.740	21.773
30)	L6 AR-1254-5	7.620	6.475	45979	61337	14.671	23.223 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101419\
Data File : PO061954.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Oct 2019 15:03
Operator : HP/AJ
Sample : K5325-04
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
10-10-D


Manual Integrations
APPROVED

Ankita
10/15/2019 9:02:14 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 15:31:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

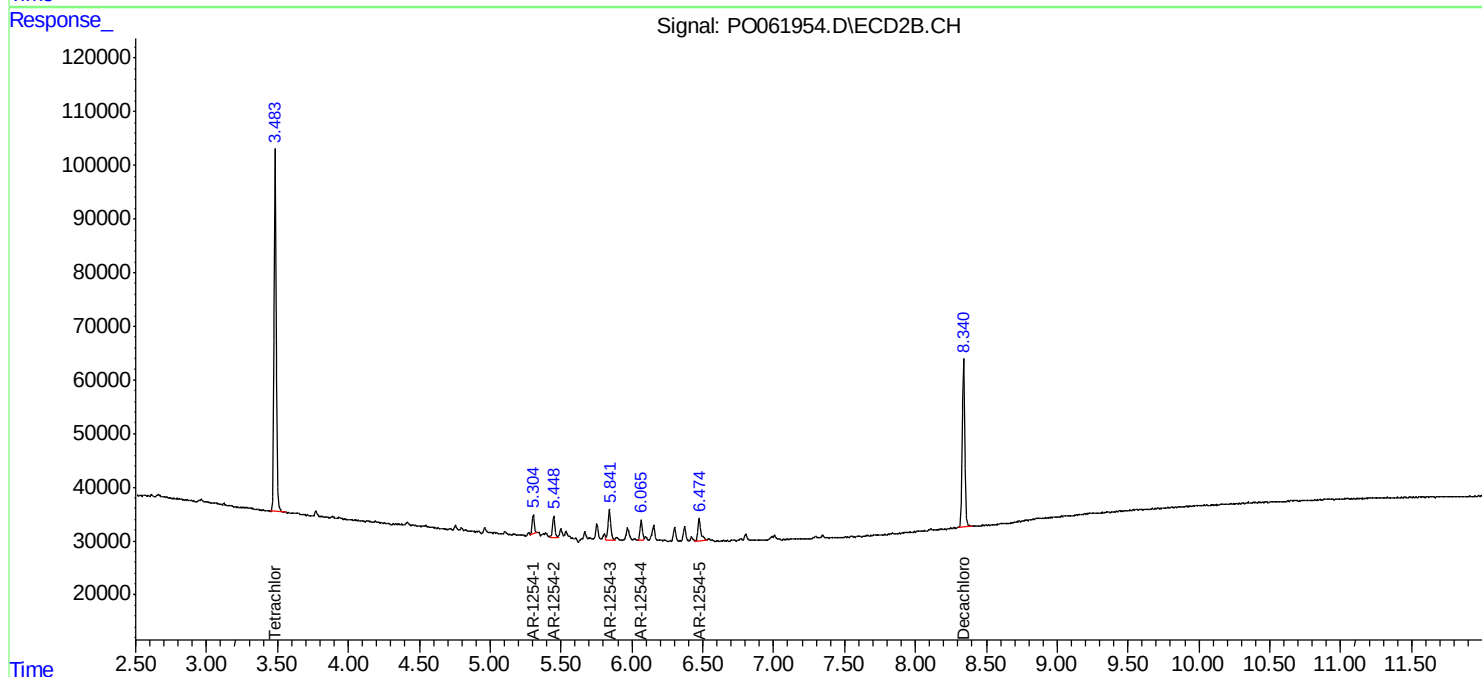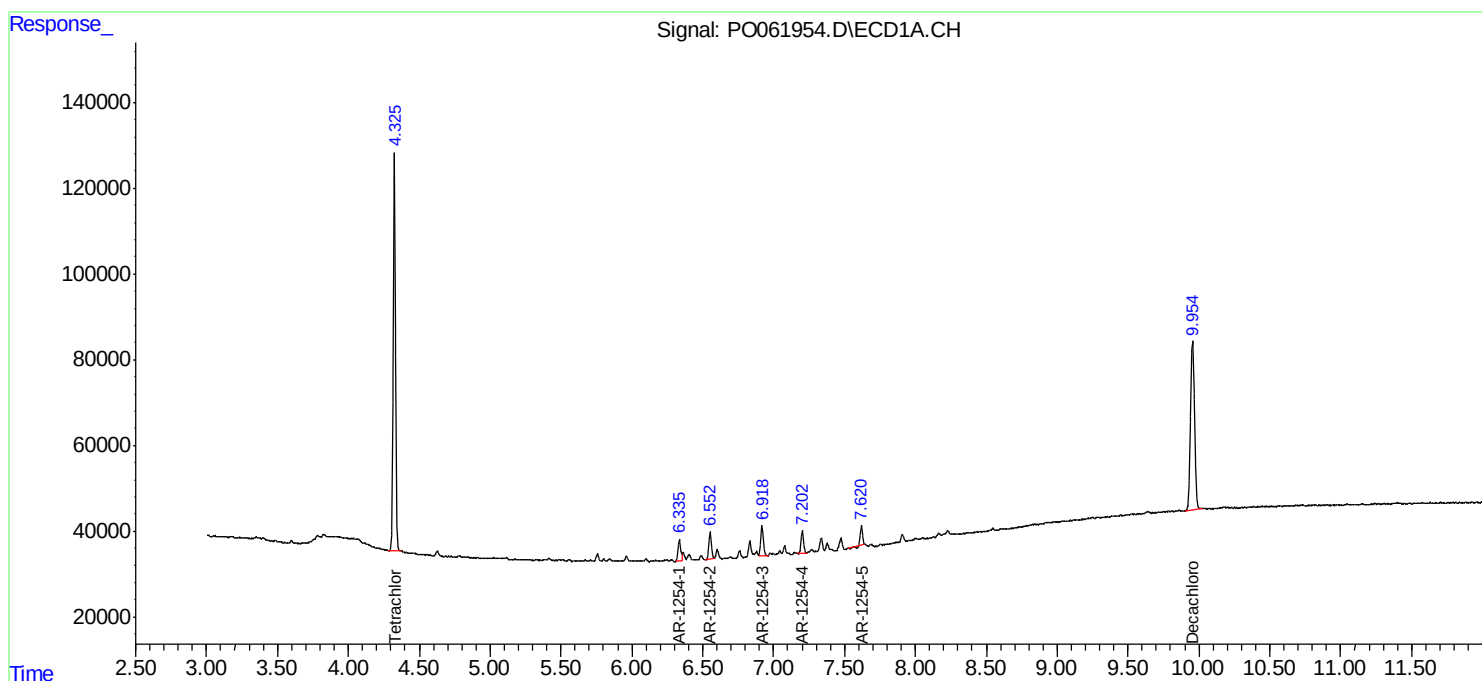

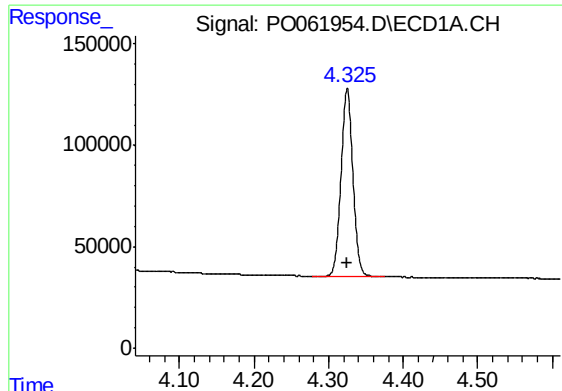


#1 Tetrachloro-m-xylene

R.T.: 4.325 min
Delta R.T.: 0.000 min
Response: 1036990
Conc: 16.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
10-10-D


Manual Integrations
APPROVED

Ankita
10/15/2019 9:02:14 AM

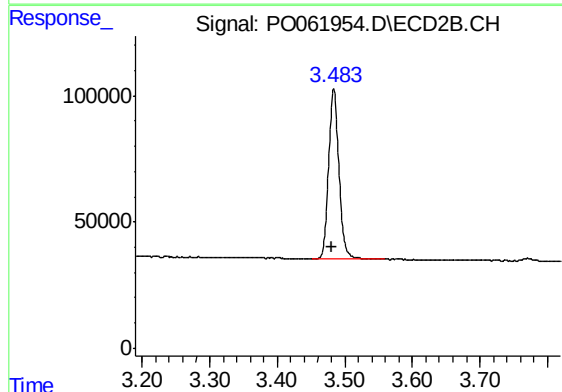


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: 0.002 min
Response: 717809
Conc: 16.74 ng/ml

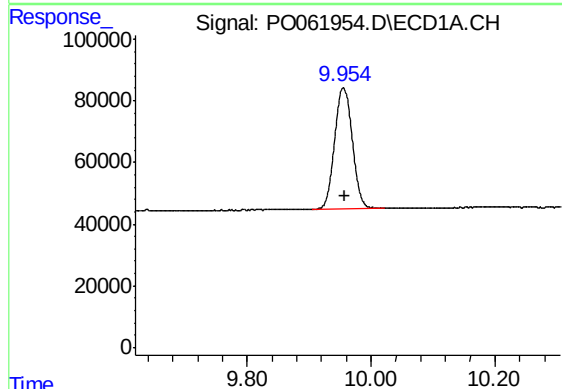


#2 Decachlorobiphenyl

R.T.: 9.955 min
Delta R.T.: -0.002 min
Response: 776343
Conc: 13.88 ng/ml

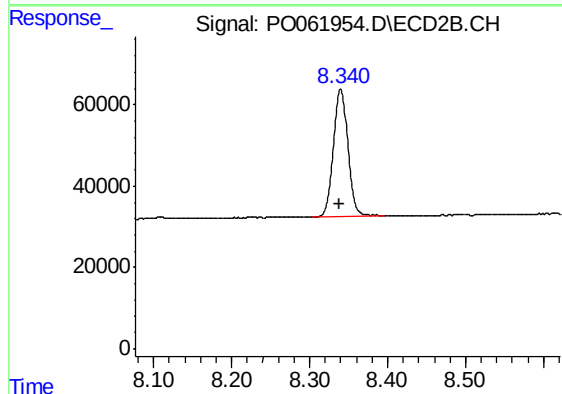

#2 Decachlorobiphenyl

R.T.: 8.340 min
Delta R.T.: 0.002 min
Response: 398644
Conc: 13.59 ng/ml

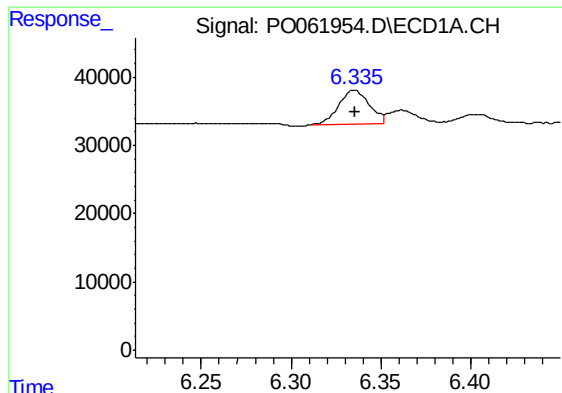


#26 AR-1254-1

R.T.: 6.335 min
Delta R.T.: 0.000 min
Response: 58672
Conc: 22.01 ng/ml m

Instrument :
ECD_O
ClientSampleId :
10-10-D


Manual Integrations
APPROVED

Ankita
10/15/2019 9:02:14 AM

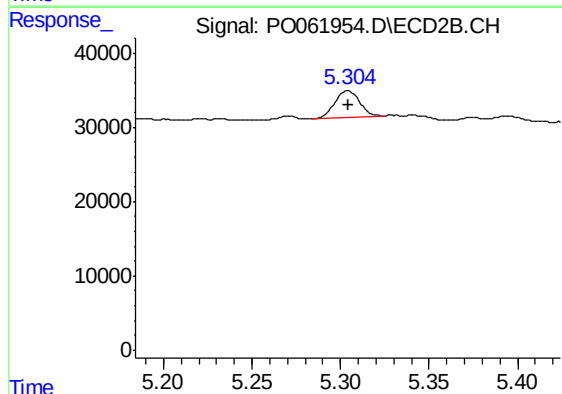


#26 AR-1254-1

R.T.: 5.304 min
Delta R.T.: 0.000 min
Response: 36031
Conc: 14.73 ng/ml

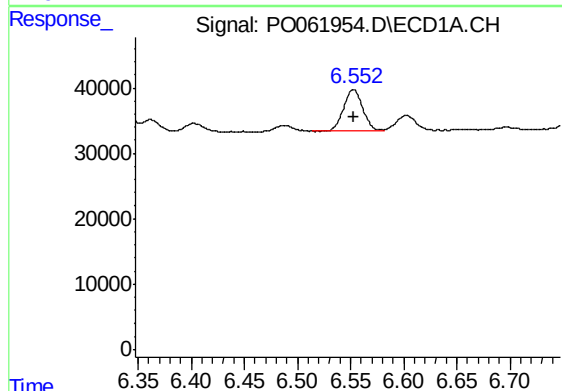


#27 AR-1254-2

R.T.: 6.553 min
Delta R.T.: 0.000 min
Response: 77250
Conc: 18.89 ng/ml

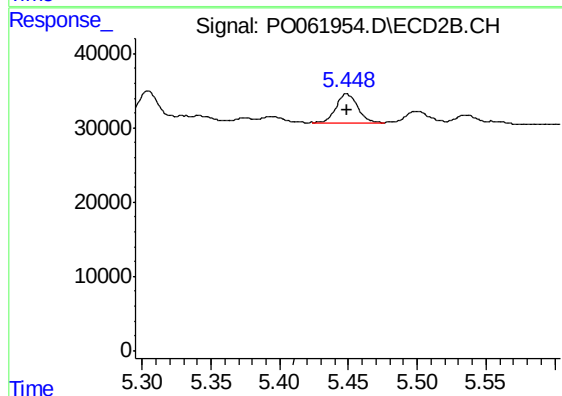

#27 AR-1254-2

R.T.: 5.449 min
Delta R.T.: 0.000 min
Response: 41806
Conc: 19.74 ng/ml

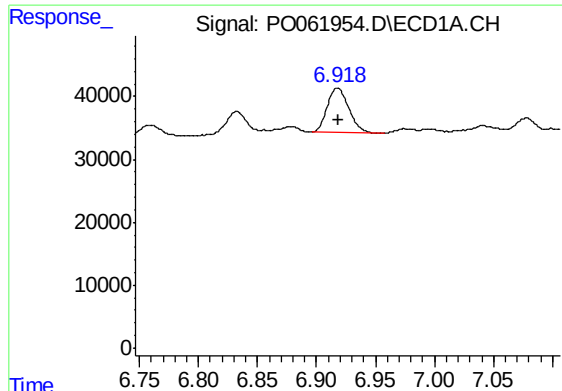


#28 AR-1254-3

R.T.: 6.918 min
Delta R.T.: 0.000 min
Response: 91412
Conc: 21.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
10-10-D


Manual Integrations
APPROVED

Ankita
10/15/2019 9:02:14 AM

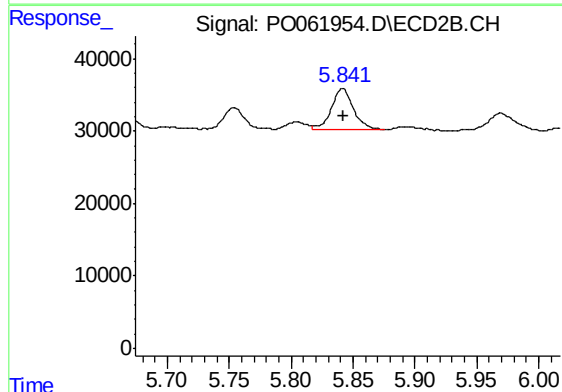


#28 AR-1254-3

R.T.: 5.842 min
Delta R.T.: 0.000 min
Response: 69786
Conc: 21.42 ng/ml

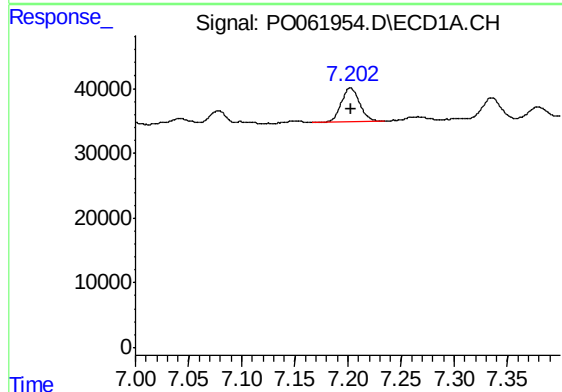


#29 AR-1254-4

R.T.: 7.202 min
Delta R.T.: 0.000 min
Response: 62497
Conc: 20.74 ng/ml

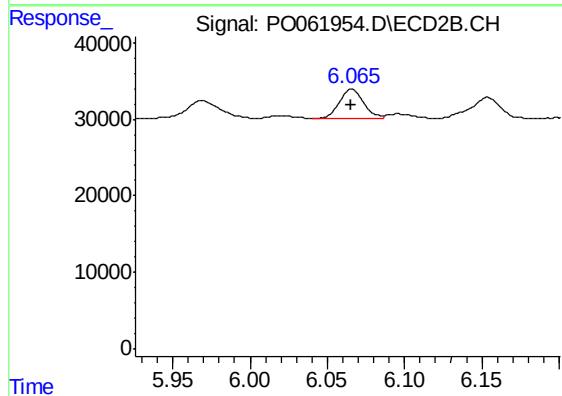

#29 AR-1254-4

R.T.: 6.066 min
Delta R.T.: 0.000 min
Response: 42053
Conc: 21.77 ng/ml

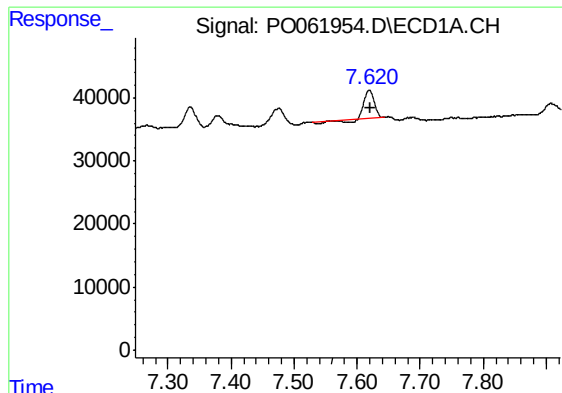


#30 AR-1254-5

R.T.: 7.620 min
Delta R.T.: 0.000 min
Response: 45979
Conc: 14.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
10-10-D

Manual Integrations
APPROVED

Ankita
10/15/2019 9:02:14 AM

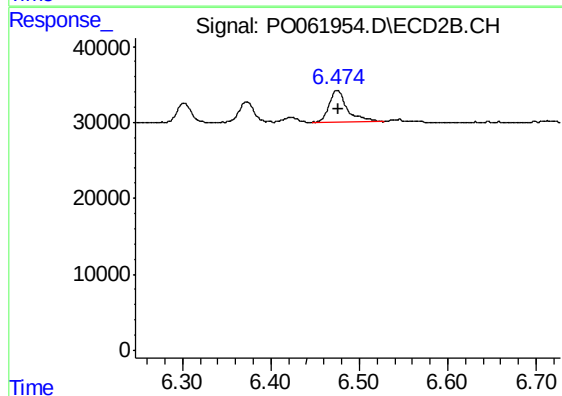

#30 AR-1254-5

R.T.: 6.475 min
Delta R.T.: 0.000 min
Response: 61337
Conc: 23.22 ng/ml