

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101419\
 Data File : P0061967.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Oct 2019 18:47
 Operator : HP/AJ
 Sample : K5325-10
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 10-10-I

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 01:06:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.325	3.483	832599	588525	13.462	13.724
2) SA Decachlor...	9.955	8.341	573138	293562	10.243	10.005

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101419\
Data File : PO061967.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Oct 2019 18:47
Operator : HP/AJ
Sample : K5325-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
10-10-I

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 01:06:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

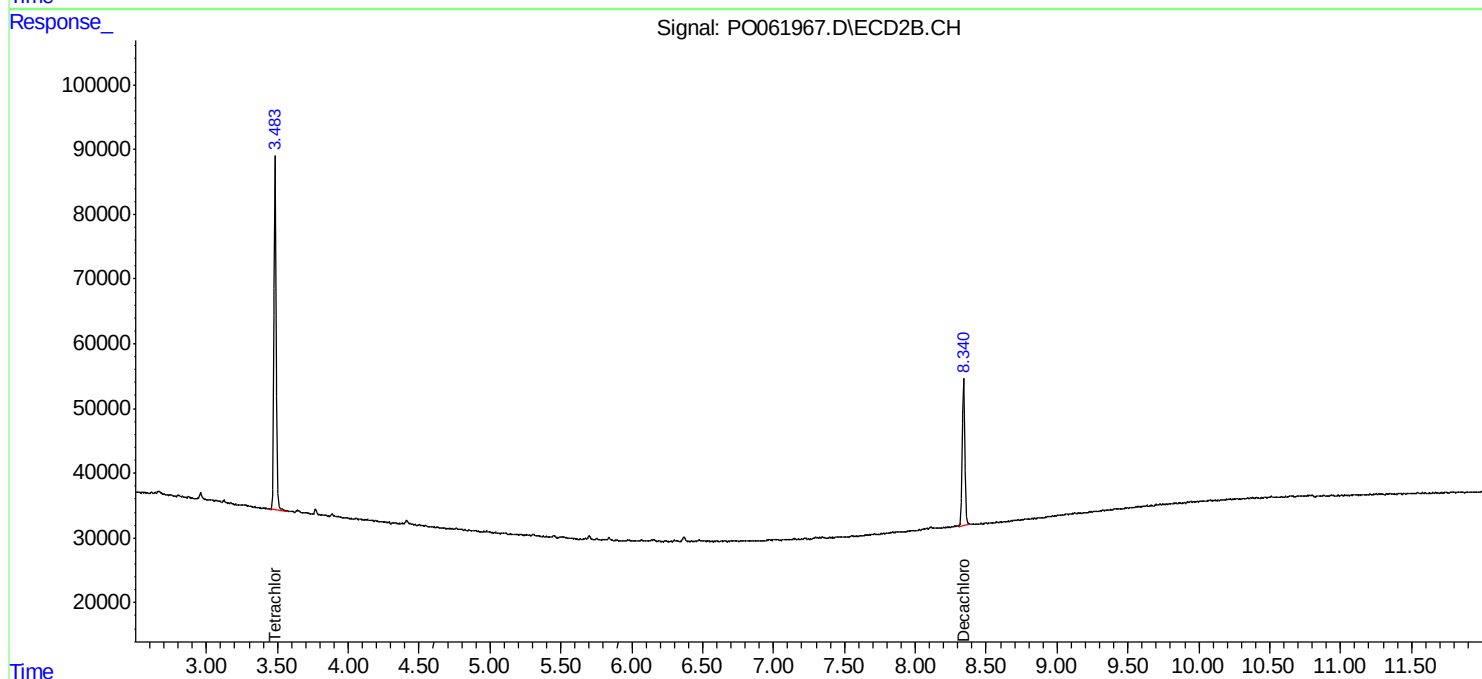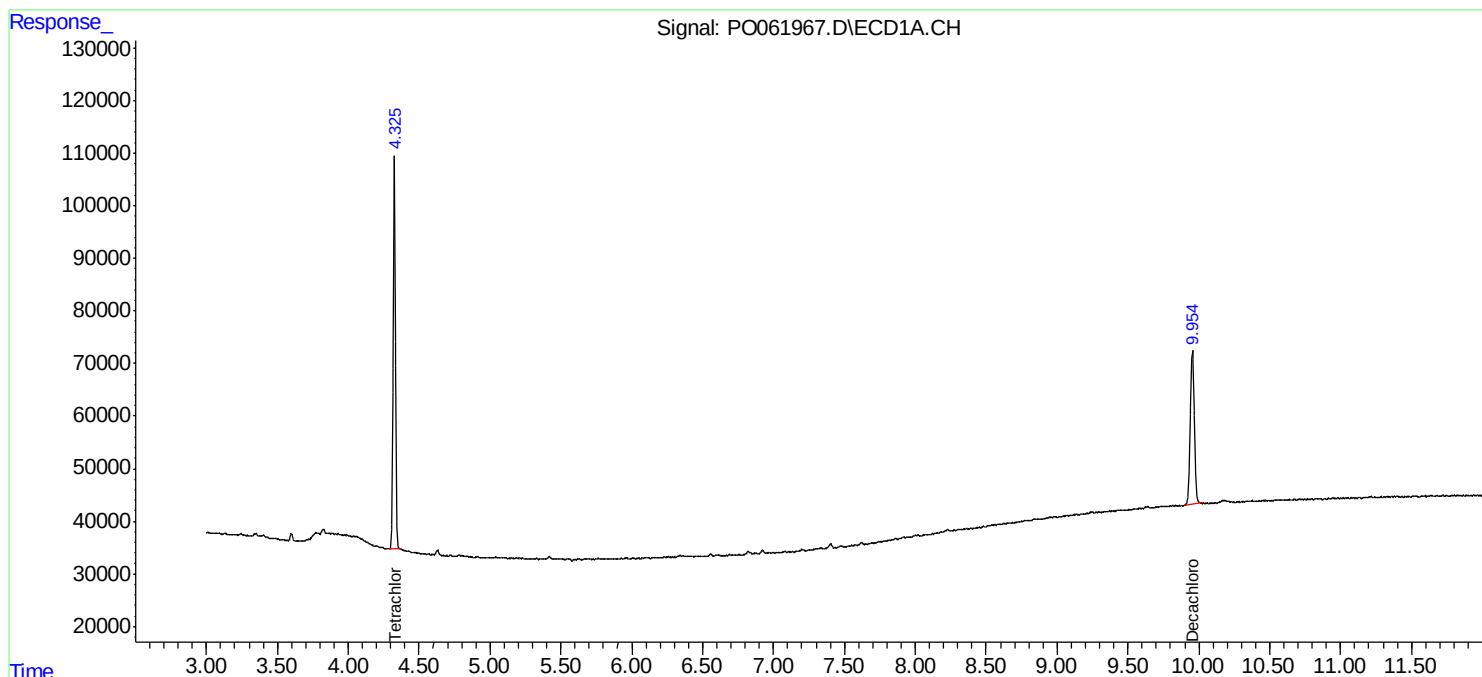


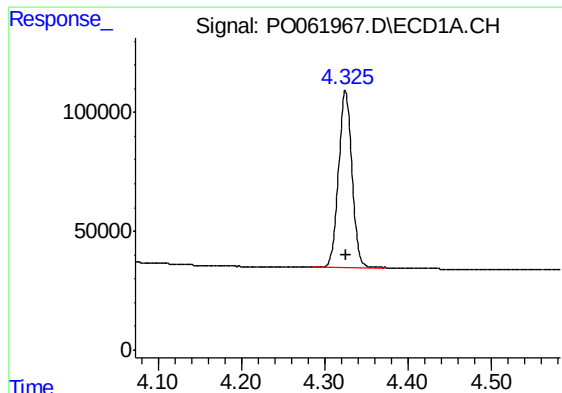

#1 Tetrachloro-m-xylene


R.T.: 4.325 min
Delta R.T.: 0.000 min
Response: 832599
Conc: 13.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
10-10-I

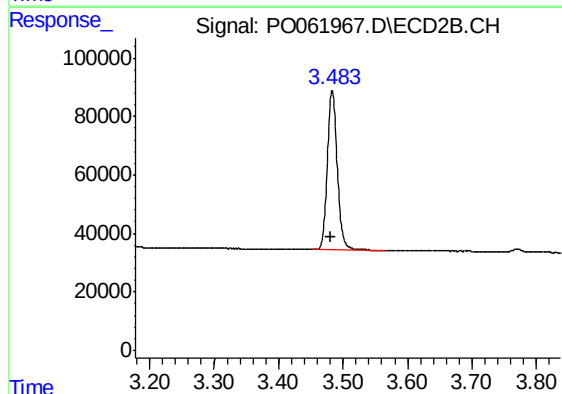


#1 Tetrachloro-m-xylene

R.T.: 3.483 min
Delta R.T.: 0.002 min
Response: 588525
Conc: 13.72 ng/ml

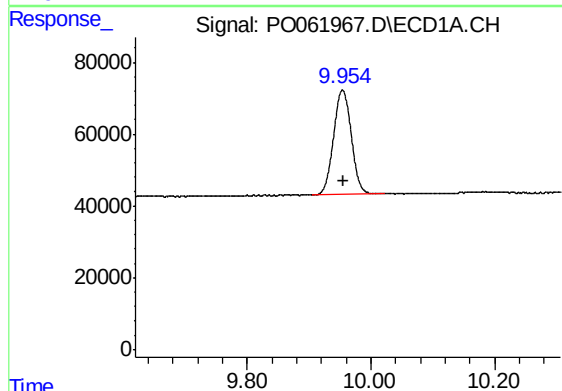

#2 Decachlorobiphenyl

R.T.: 9.955 min
Delta R.T.: -0.002 min
Response: 573138
Conc: 10.24 ng/ml

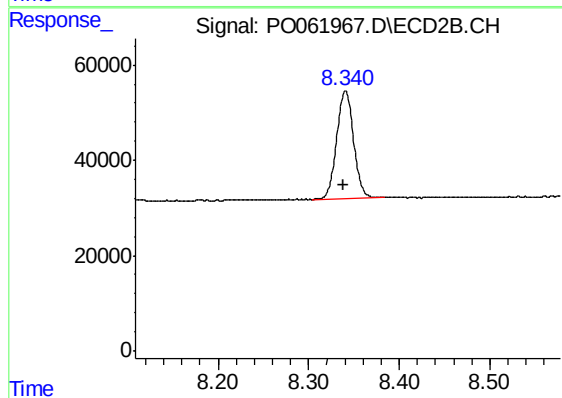

#2 Decachlorobiphenyl

R.T.: 8.341 min
Delta R.T.: 0.003 min
Response: 293562
Conc: 10.01 ng/ml